

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX071020\
 Data File : VX017339.D
 Acq On : 10 Jul 2020 16:41
 Operator : JC/SP
 Sample : L3184-06
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Jul 11 01:03:11 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X062920W.M
 Quant Title : SW846 8260
 QLast Update : Mon Jun 29 17:10:38 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.63	168	256446	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.83	114	428498	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.10	117	467229	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.06	152	245120	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.03	65	163296	51.65	ug/l	0.00
Spiked Amount	50.000		Recovery	=	103.30%	
35) Dibromofluoromethane	5.47	113	139760	51.56	ug/l	0.00
Spiked Amount	50.000		Recovery	=	103.12%	
50) Toluene-d8	8.70	98	535609	53.44	ug/l	0.00
Spiked Amount	50.000		Recovery	=	106.88%	
62) 4-Bromofluorobenzene	11.12	95	230232	58.76	ug/l	0.00
Spiked Amount	50.000		Recovery	=	117.52%	
Target Compounds						
					Qvalue	
5) Bromomethane	1.64	94	304	0.207	ug/l #	38
8) Diethyl Ether	2.17	74	662	0.839	ug/l	70
11) Tert butyl alcohol	3.01	59	1385	2.296	ug/l #	88
13) Acrolein	2.28	56	278	0.771	ug/l #	1
16) Acetone	2.42	43	68196	57.663	ug/l	96
17) Carbon Disulfide	2.55	76	1374	0.217	ug/l #	76
18) Methyl Acetate	2.75	43	2949	0.955	ug/l	94
20) Methylene Chloride	2.84	84	17115	5.615	ug/l	95
25) 2-Butanone	4.65	43	4394	2.230	ug/l	96
29) Tetrahydrofuran	5.12	42	1113	0.855	ug/l #	84
31) Cyclohexane	5.62	56	5672	1.329	ug/l #	1
36) 1,1-Dichloropropene	5.63	75	17952	4.433	ug/l #	49
38) Carbon Tetrachloride	5.63	117	24721	5.542	ug/l #	17
43) Isopropyl Acetate	6.42	43	46500	6.810	ug/l	99
44) Trichloroethene	7.19	130	278	Below Cal		51
48) Methyl methacrylate	7.65	41	4124	1.271	ug/l #	15
49) 1,4-Dioxane	7.76	88	20	0.272	ug/l #	1
51) 4-Methyl-2-Pentanone	8.59	43	52592	12.921	ug/l #	45
54) cis-1,3-Dichloropropene	8.60	75	22090	4.343	ug/l #	61
57) 1,3-Dichloropropane	9.52	76	3415	0.665	ug/l #	42
59) 2-Hexanone	9.41	43	63924	21.505	ug/l #	23
76) 1,2,3-Trichloropropane	11.12	75	115309	23.922	ug/l #	37
81) trans-1,4-Dichloro-2-buten	11.12	75	115309	61.950	ug/l #	13
88) 1,4-Dichlorobenzene	12.01	146	628	Below Cal		84
94) Hexachlorobutadiene	13.76	225	301	0.997	ug/l	89
95) Naphthalene	13.82	128	3779	0.243	ug/l #	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX071020\
Data File : VX017339.D
Acq On : 10 Jul 2020 16:41
Operator : JC/SP
Sample : L3184-06
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Jul 11 01:03:11 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X062920W.M
Quant Title : SW846 8260
QLast Update : Mon Jun 29 17:10:38 2020
Response via : Initial Calibration

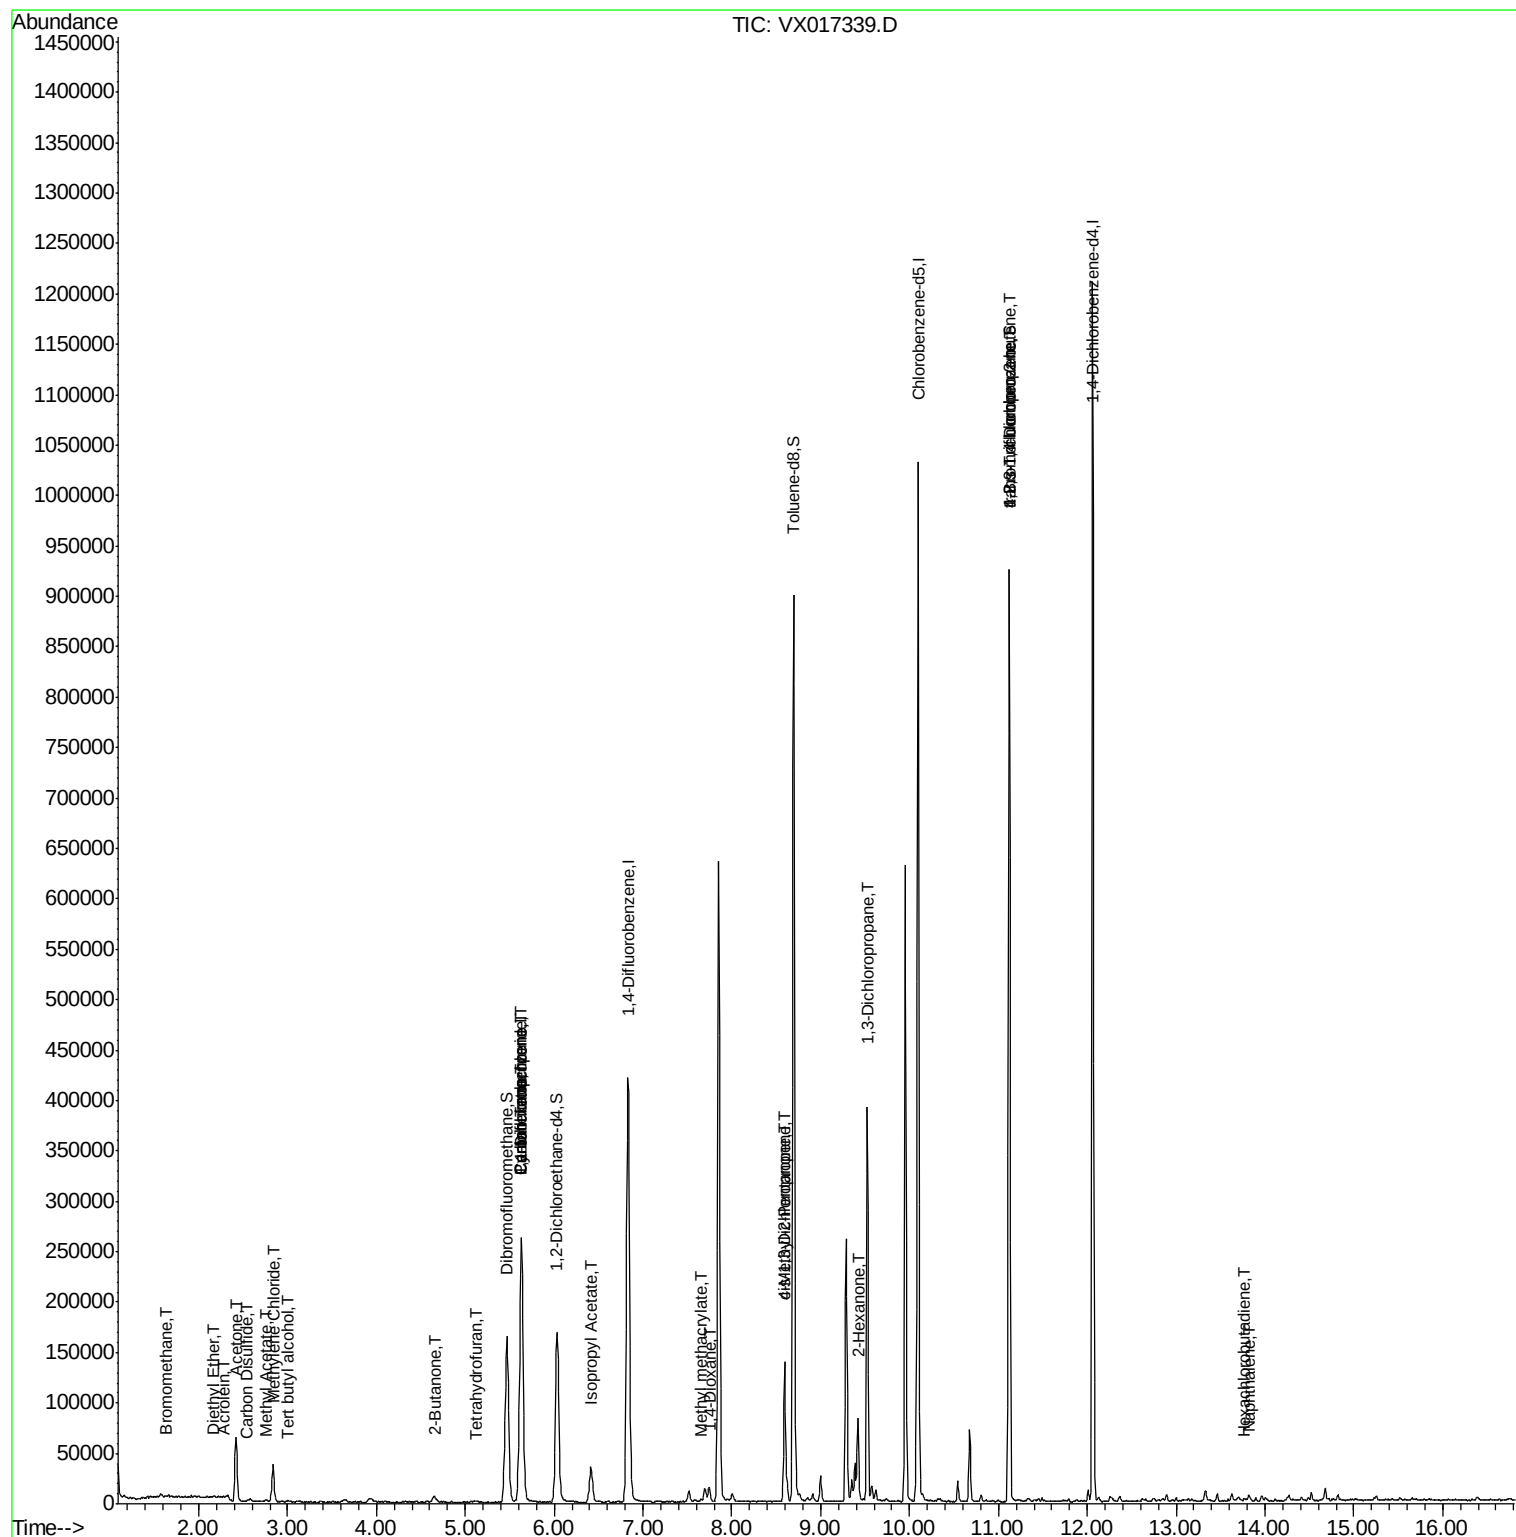

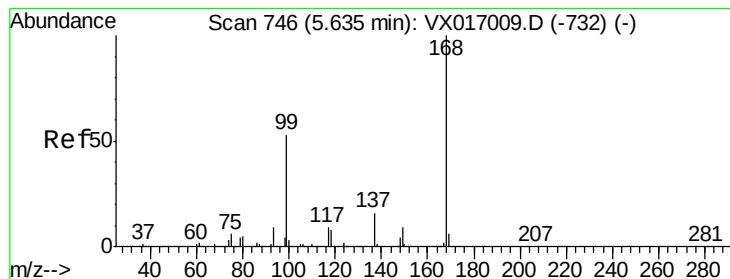

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.63 min Scan# 745

Delta R.T. -0.01 min

Lab File: VX017339.D

Acq: 10 Jul 2020 16:41

Instrument :

MSVOA_X


ClientSampleId :

Tot Ion:168 Resp: 256446

Ion Ratio Lower Upper

168 100

99 54.4 42.6 64.0



Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.63

100000

80000



60000

40000

20000

0

Time-->

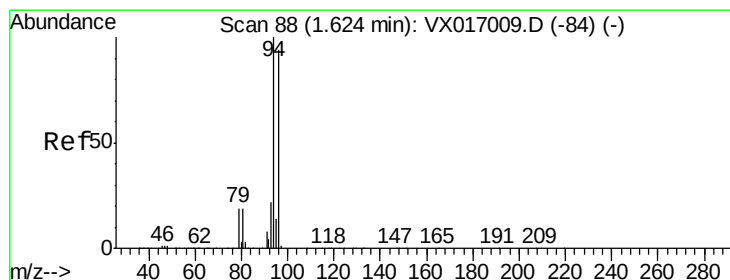

#5

Bromomethane

Concen: 0.207 ug/l

RT: 1.64 min Scan# 91

Delta R.T. 0.02 min

Lab File: VX017339.D


Acq: 10 Jul 2020 16:41

Tgt Ion: 94 Resp: 304

Ion Ratio Lower Upper

94 100

96 34.3 75.0 112.4#



Abundance Ion 93.90 (93.60 to 94.60): VX0

Ion 95.90 (95.60 to 96.60): VX0

1.64

200


150


100

50

0

Time-->



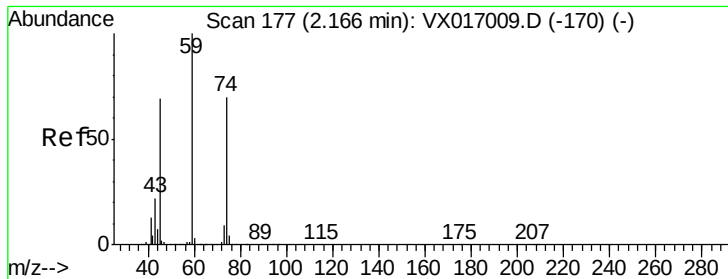

#8

Diethyl Ether

Concen: 0.839 ug/l

RT: 2.17 min Scan# 177

Delta R.T. 0.00 min

Lab File: VX017339.D

Acq: 10 Jul 2020 16:41

Instrument :

MSVOA_X


ClientSampled :

Tot Ion: 74 Resp: 662

Ion Ratio Lower Upper




74 100

45 129.0 49.8 149.3

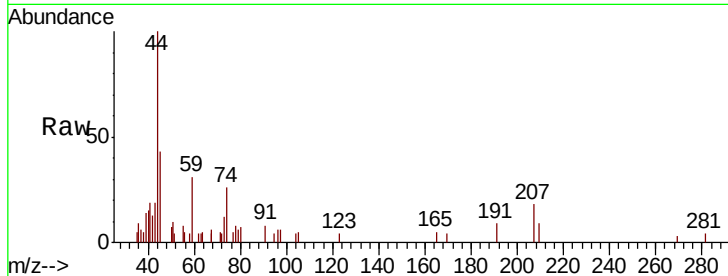

Abundance Ion 74.00 (73.70 to 74.70): VX0

Ion 45.00 (44.70 to 45.70): VX0

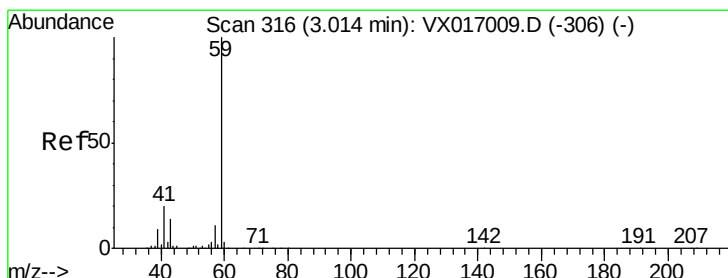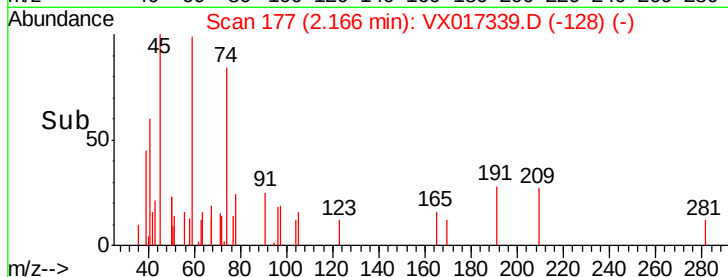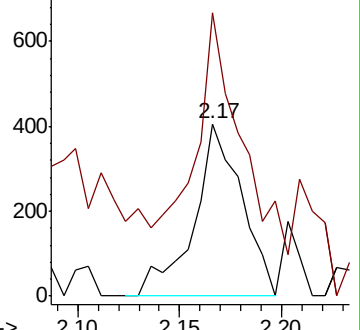

#11

Tert butyl alcohol

Concen: 2.296 ug/l

RT: 3.01 min Scan# 316

Delta R.T. -0.00 min

Lab File: VX017339.D


Acq: 10 Jul 2020 16:41

Tgt Ion: 59 Resp: 1385

Ion Ratio Lower Upper



59 100


57 14.8 8.2 12.2#

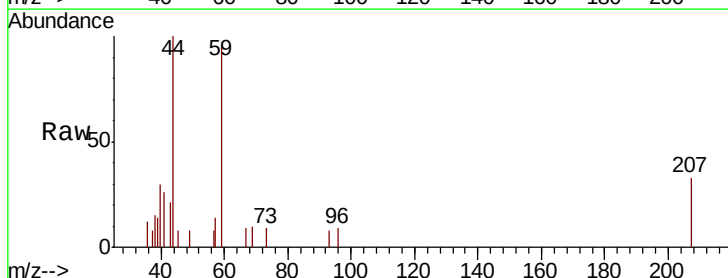

Abundance Ion 59.00 (58.70 to 59.70): VX0

Ion 57.00 (56.70 to 57.70): VX0

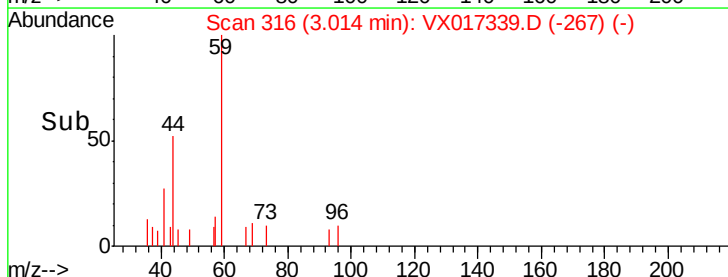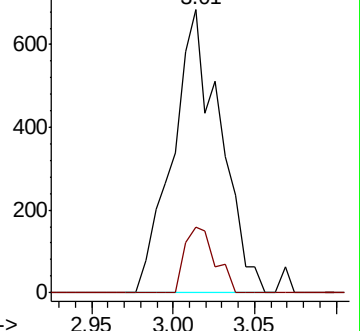

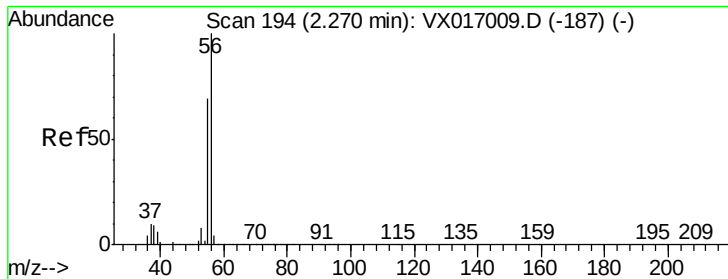

#13

Acrolein

Concen: 0.771 ug/l

RT: 2.28 min Scan# 195

Delta R.T. 0.01 min

Lab File: VX017339.D

Acq: 10 Jul 2020 16:41


Instrument :
MSVOA_X
ClientSampleId :

Tot Ion: 56 Resp: 278




Ion Ratio Lower Upper

56 100

55 195.0 55.7 83.5#

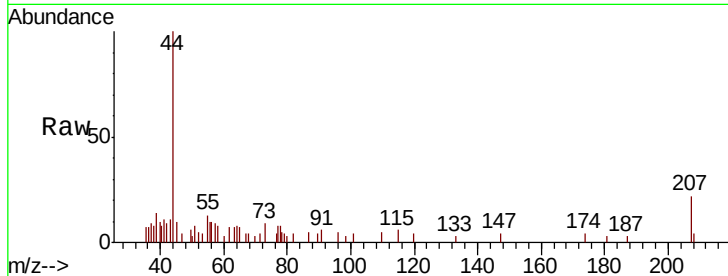

Abundance Ion 56.00 (55.70 to 56.70): VX0
Ion 55.00 (54.70 to 55.70): VX0

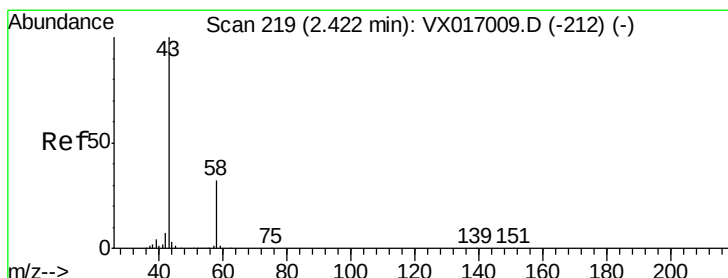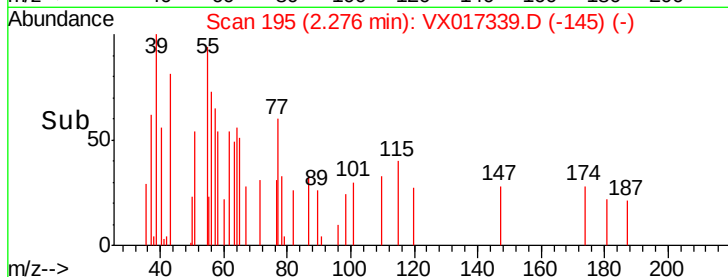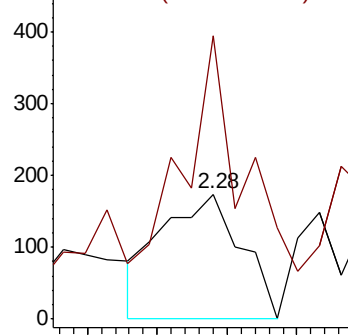

#16

Acetone

Concen: 57.663 ug/l

RT: 2.42 min Scan# 219

Delta R.T. -0.00 min

Lab File: VX017339.D


Acq: 10 Jul 2020 16:41

Tgt Ion: 43 Resp: 68196



Ion Ratio Lower Upper


43 100

58 30.1 25.7 38.5

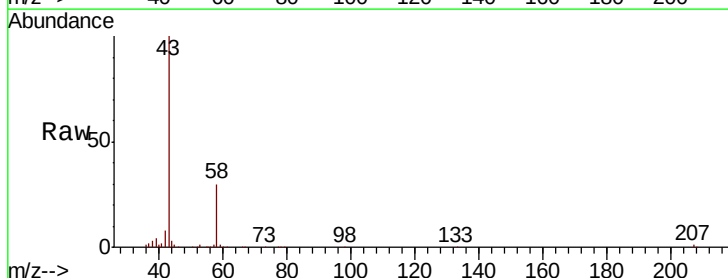

Abundance Ion 43.00 (42.70 to 43.70): VX0
Ion 58.00 (57.70 to 58.70): VX0

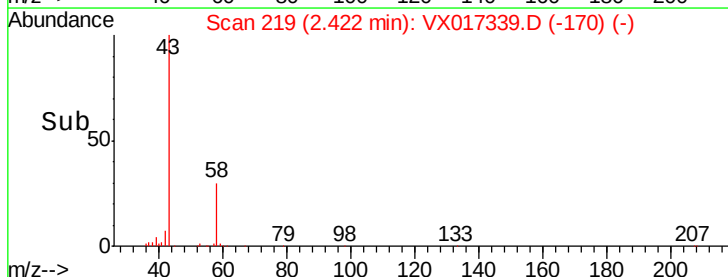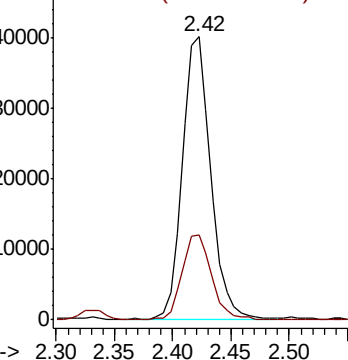

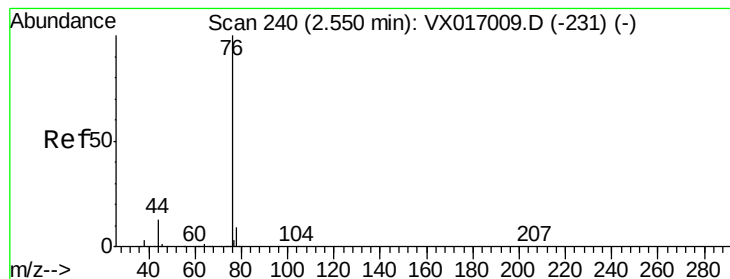

#17

Carbon Disulfide

Concen: 0.217 ug/l

RT: 2.55 min Scan# 240

Delta R.T. 0.00 min

Lab File: VX017339.D

Acq: 10 Jul 2020 16:41

Instrument :

MSVOA_X


ClientSampleId :

Tot Ion: 76 Resp: 1374

Ion Ratio Lower Upper




76 100

78 17.6 7.2 10.8#

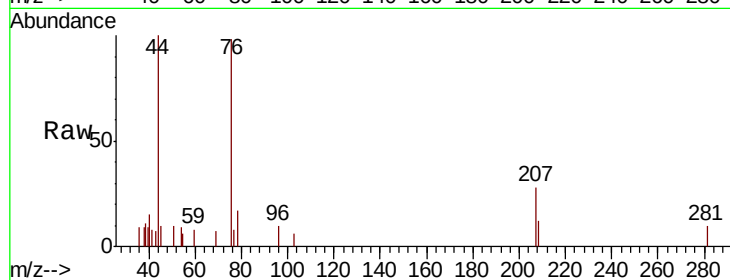

Abundance Ion 75.90 (75.60 to 76.60): VX0

Ion 77.90 (77.60 to 78.60): VX0

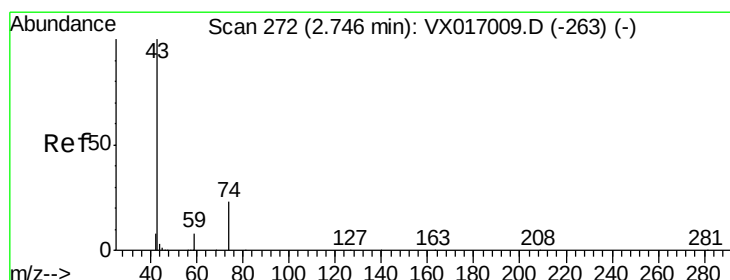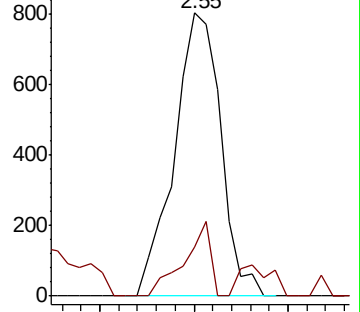

#18

Methyl Acetate

Concen: 0.955 ug/l

RT: 2.75 min Scan# 272

Delta R.T. -0.00 min

Lab File: VX017339.D


Acq: 10 Jul 2020 16:41

Tgt Ion: 43 Resp: 2949

Ion Ratio Lower Upper



43 100


74 27.1 19.3 28.9

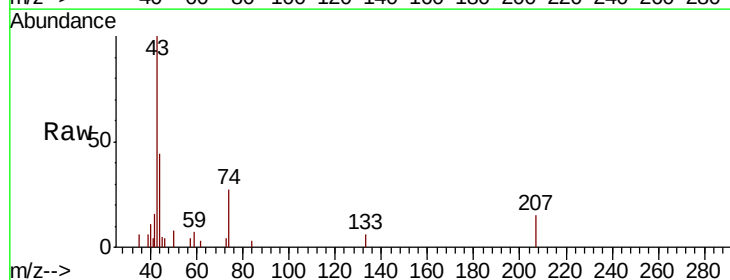

Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 74.00 (73.70 to 74.70): VX0




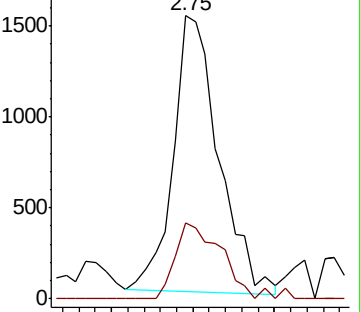


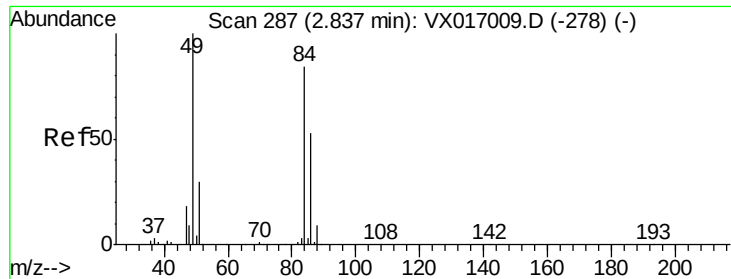

#20
Methvlene Chloride
Concen: 5.615 ug/l
RT: 2.84 min Scan# 287
Delta R.T. 0.00 min
Lab File: VX017339.D
Acq: 10 Jul 2020 16:41




Instrument :
MSVOA_X
ClientSampleId :


Tot Ion:	84	Resp:	17115
Ion	Ratio	Lower	Upper
84	100		
49	115.3	94.7	142.1
51	37.2	28.6	42.8
86	54.8	50.5	75.7

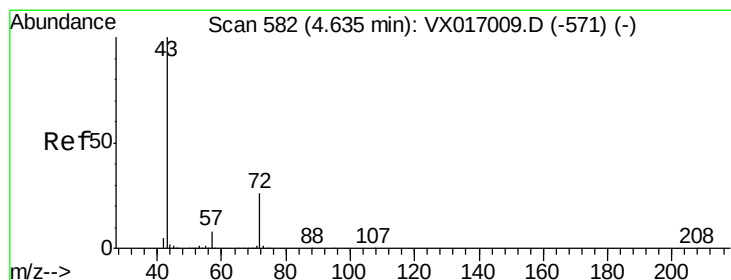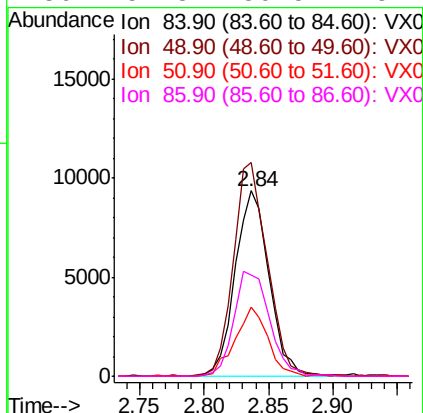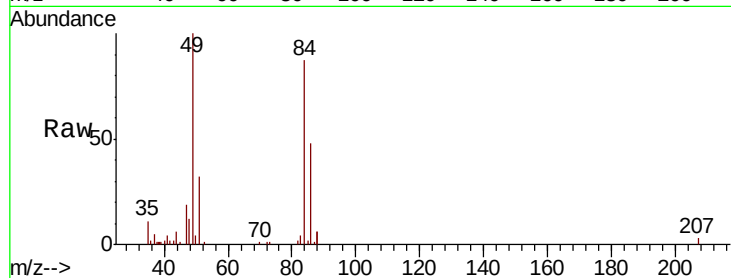

#25
2-Butanone
Concen: 2.230 ug/l
RT: 4.65 min Scan# 584
Delta R.T. 0.01 min
Lab File: VX017339.D
Acq: 10 Jul 2020 16:41

Tgt Ion:	43	Resp:	4394
Ion	Ratio	Lower	Upper
43	100		
72	23.7	20.8	31.2

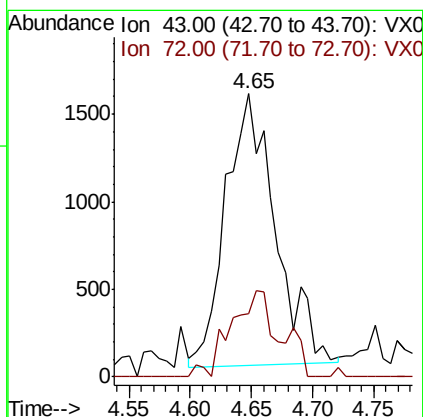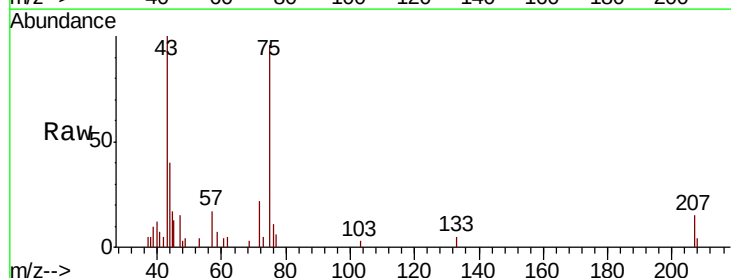



#29

Tetrahydrofuran

Concen: 0.855 ug/l

RT: 5.12 min Scan# 661

Delta R.T. 0.03 min

Lab File: VX017339.D


Acq: 10 Jul 2020 16:41

Instrument :




MSVOA_X

ClientSampled :

Tot Ion:	42	Resp:	1113
Ion	Ratio	Lower	Upper
42	100		
72	27.8	35.3	52.9#
71	37.1	33.1	49.7

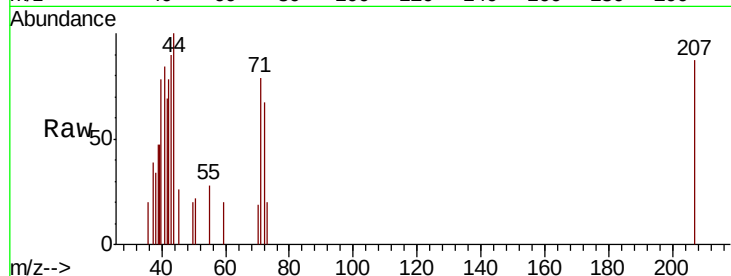

Abundance Ion 42.00 (41.70 to 42.70): VX0
Ion 72.00 (71.70 to 72.70): VX0
Ion 71.00 (70.70 to 71.70): VX0

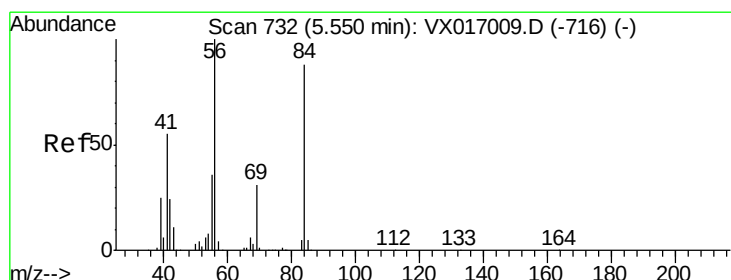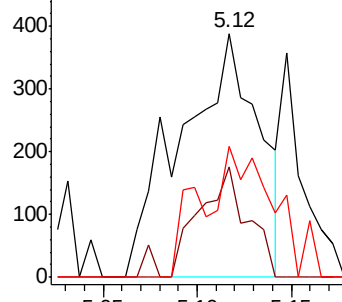

#31

Cyclohexane

Concen: 1.329 ug/l


RT: 5.62 min Scan# 744

Delta R.T. 0.07 min



Lab File: VX017339.D


Acq: 10 Jul 2020 16:41

Tgt Ion:	56	Resp:	5672
Ion	Ratio	Lower	Upper
56	100		
69	154.6	25.0	37.4#
84	141.7	69.1	103.7#

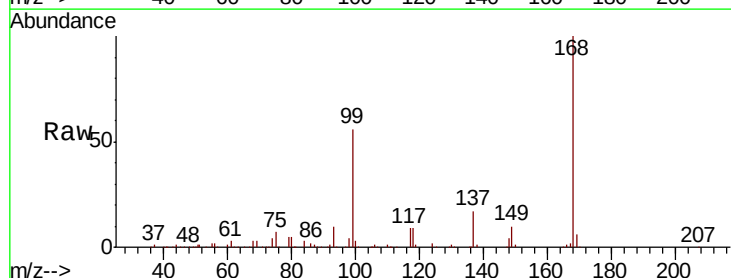

Abundance Ion 56.00 (55.70 to 56.70): VX0
Ion 69.00 (68.70 to 69.70): VX0
Ion 84.00 (83.70 to 84.70): VX0




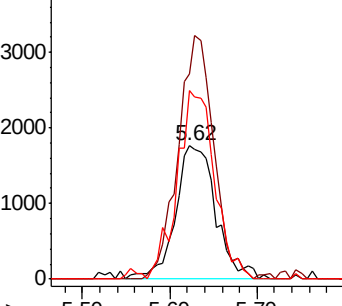


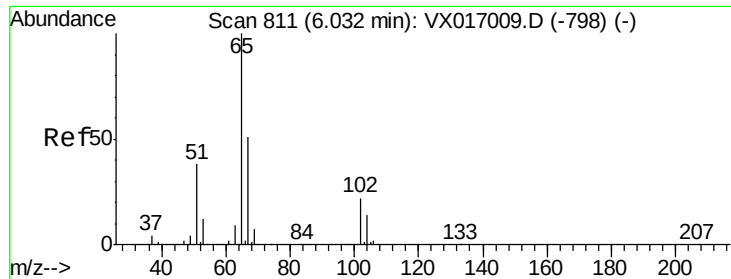

#33
 1,2-Dichloroethane-d4
 Concen: 51.652 ug/l
 RT: 6.03 min Scan# 811
 Delta R.T. -0.00 min
 Lab File: VX017339.D
 Acq: 10 Jul 2020 16:41




Instrument :
 MSVOA_X
 ClientSampleId :


Tot Ion: 65 Resp: 163296
 Ion Ratio Lower Upper
 65 100
 67 51.5 0.0 103.8

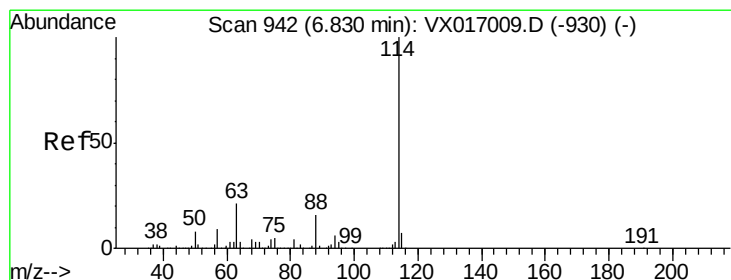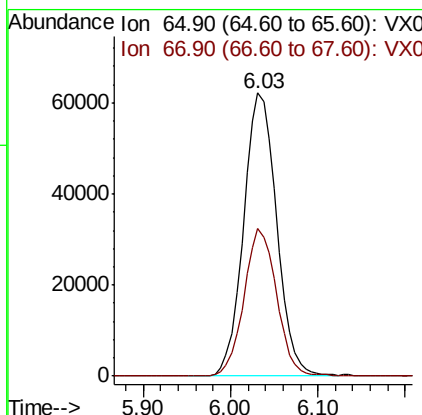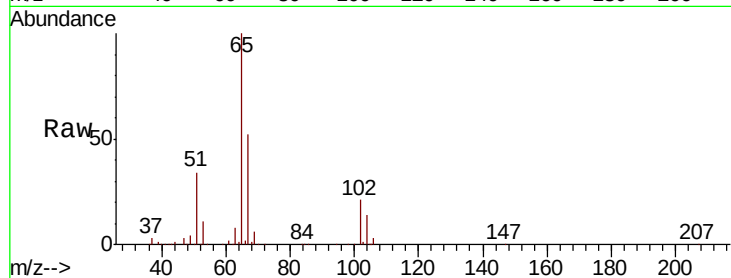

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 6.83 min Scan# 942
 Delta R.T. -0.00 min
 Lab File: VX017339.D
 Acq: 10 Jul 2020 16:41

Tgt Ion: 114 Resp: 428498
 Ion Ratio Lower Upper
 114 100
 63 19.4 0.0 41.4
 88 15.1 0.0 32.4

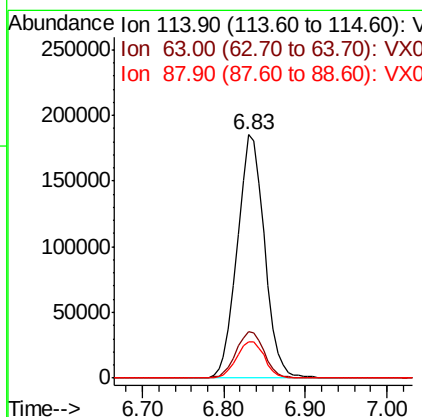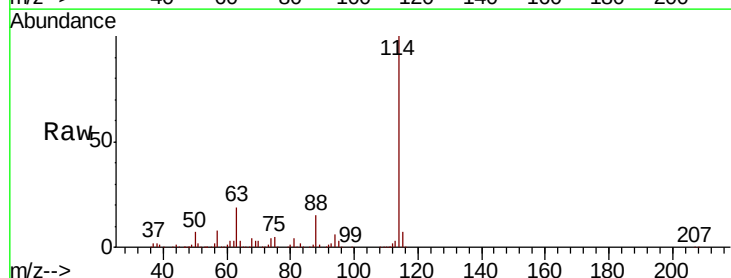



#35

Dibromofluoromethane

Concen: 51.562 ug/l

RT: 5.47 min Scan# 719

Delta R.T. 0.01 min

Lab File: VX017339.D

Acq: 10 Jul 2020 16:41

Instrument :

MSVOA_X

ClientSampleId :


Tot Ion:113 Resp: 139760

Ion Ratio Lower Upper

113 100

111 103.1 81.9 122.9




192 21.8 16.7 25.1



Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

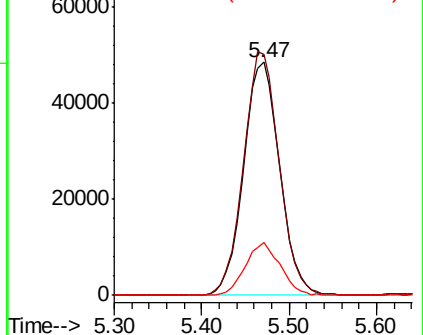

#36

1,1-Dichloropropene

Concen: 4.433 ug/l

RT: 5.63 min Scan# 745

Delta R.T. -0.14 min

Lab File: VX017339.D

Acq: 10 Jul 2020 16:41


Tgt Ion: 75 Resp: 17952

Ion Ratio Lower Upper

75 100

110 8.7 18.1 54.1#



77 0.1 24.6 37.0#




Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 109.90 (109.60 to 110.60): V

Ion 76.90 (76.60 to 77.60): VX0

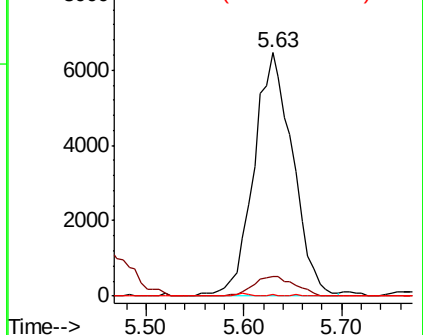

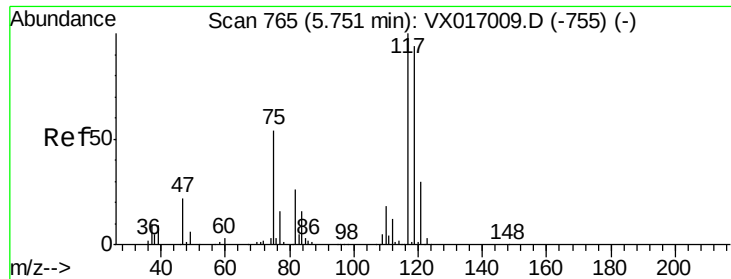

#38

Carbon Tetrachloride

Concen: 5.542 ug/l

RT: 5.63 min Scan# 745

Delta R.T. -0.12 min

Lab File: VX017339.D

Acq: 10 Jul 2020 16:41

Instrument :

MSVOA_X

ClientSampleId :


Tot Ion:117 Resp: 24721

Ion Ratio Lower Upper

117 100

119 6.1 75.4 113.0#




121 0.0 23.8 35.6#

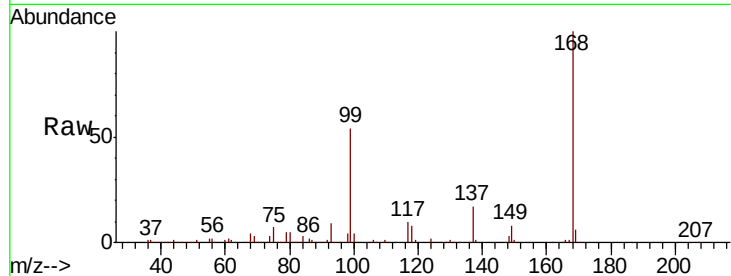

Abundance Ion 116.80 (116.50 to 117.50): V

Ion 118.80 (118.50 to 119.50): V

Ion 120.80 (120.50 to 121.50): V

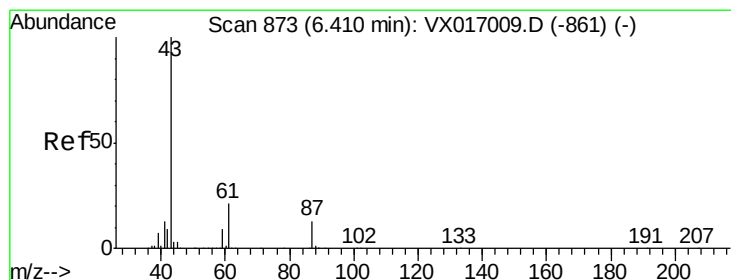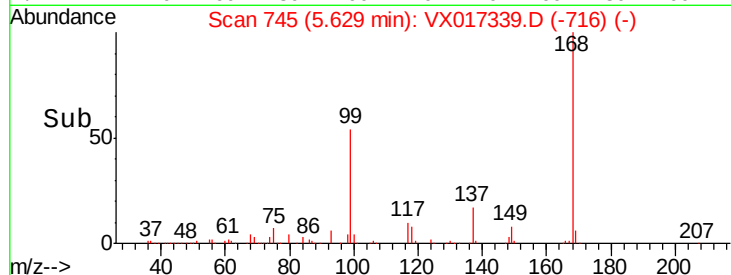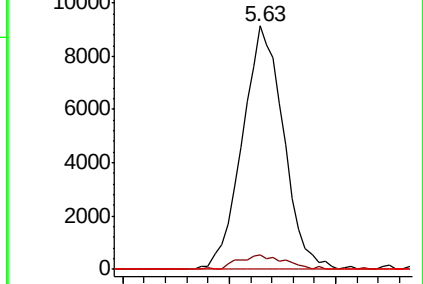

#43

Isopropyl Acetate

Concen: 6.810 ug/l

RT: 6.42 min Scan# 874

Delta R.T. 0.01 min

Lab File: VX017339.D

Acq: 10 Jul 2020 16:41


Tgt Ion: 43 Resp: 46500

Ion Ratio Lower Upper

43 100

61 20.7 16.2 24.2



87 14.0 10.7 16.1

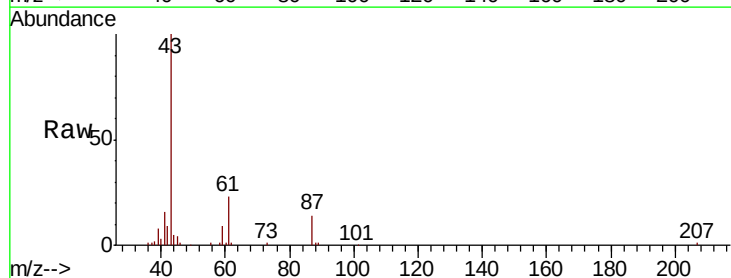


Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 61.00 (60.70 to 61.70): VX0

Ion 87.00 (86.70 to 87.70): VX0

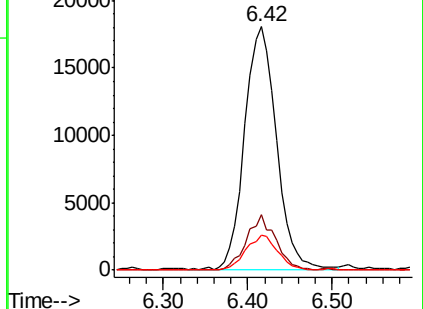


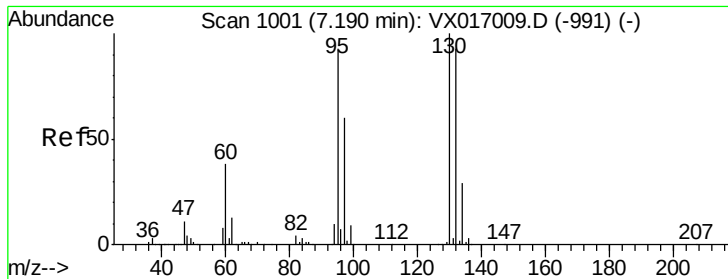




#44
 Trichloroethene
 Concen: Below Cal
 RT: 7.19 min Scan# 1001
 Delta R.T. 0.00 min
 Lab File: VX017339.D
 Acq: 10 Jul 2020 16:41

Instrument :
 MSVOA_X
 ClientSampled :

Tot Ion:130 Resp: 278
 Ion Ratio Lower Upper
 130 100
 95 45.9 0.0 185.0

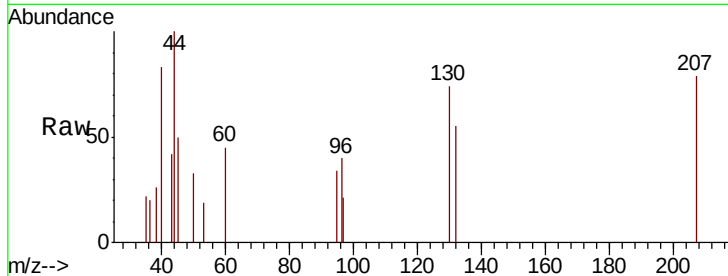


Abundance Ion 129.80 (129.50 to 130.50): V
 Ion 94.90 (94.60 to 95.60): VX0

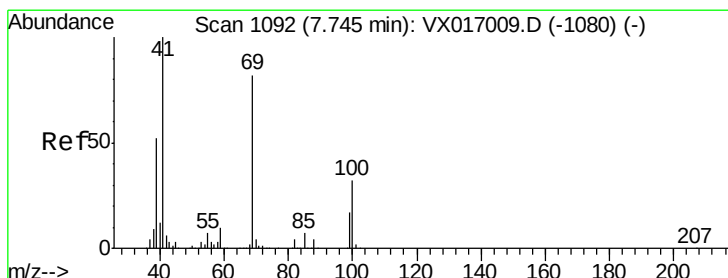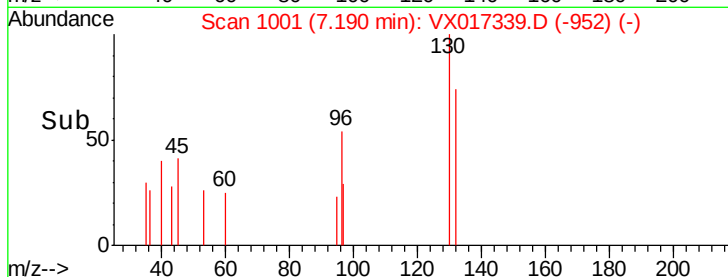
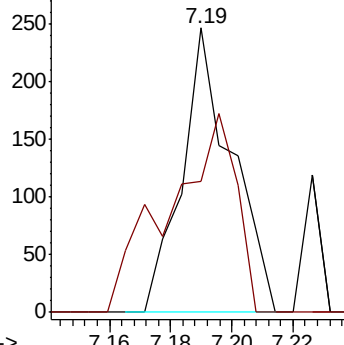



#48
 Methyl methacrylate
 Concen: 1.271 ug/l
 RT: 7.65 min Scan# 1077
 Delta R.T. -0.09 min
 Lab File: VX017339.D
 Acq: 10 Jul 2020 16:41

Tgt Ion: 41 Resp: 4124
 Ion Ratio Lower Upper
 41 100
 69 0.0 65.8 98.8#
 39 0.0 42.5 63.7#

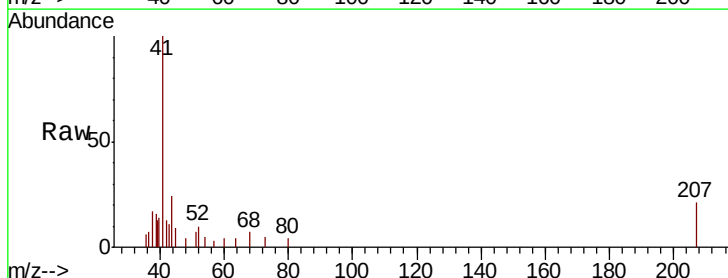

Abundance Ion 41.00 (40.70 to 41.70): VX0
 Ion 69.00 (68.70 to 69.70): VX0
 Ion 39.00 (38.70 to 39.70): VX0



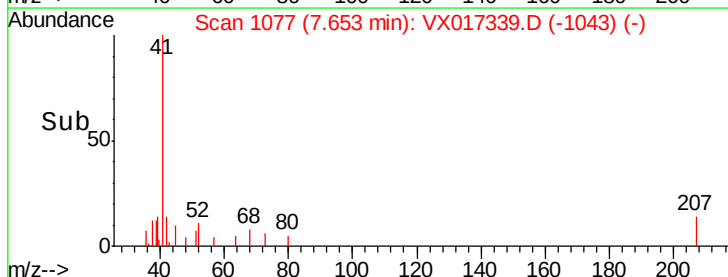
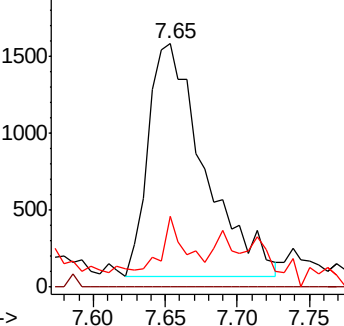




#49
1,4-Dioxane
Concen: 0.272 ug/l
RT: 7.76 min Scan# 1095
Delta R.T. 0.05 min
Lab File: VX017339.D
Acq: 10 Jul 2020 16:41




Instrument :
MSVOA_X
ClientSampleId :


Tot Ion: 88 Resp: 20
Ion Ratio Lower Upper
88 100
43 0.0 25.8 38.8#
58 2920.0 54.8 82.2#

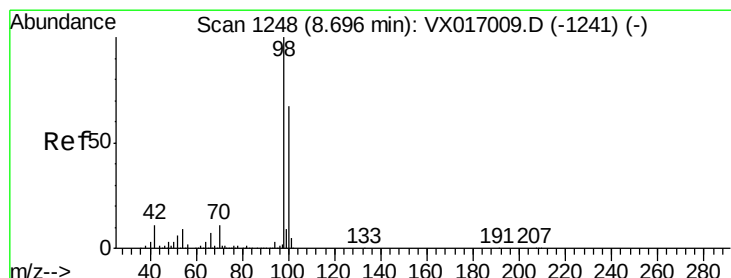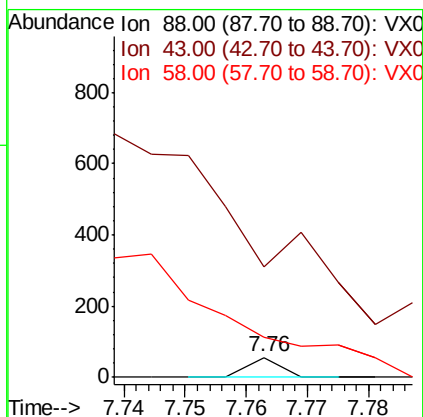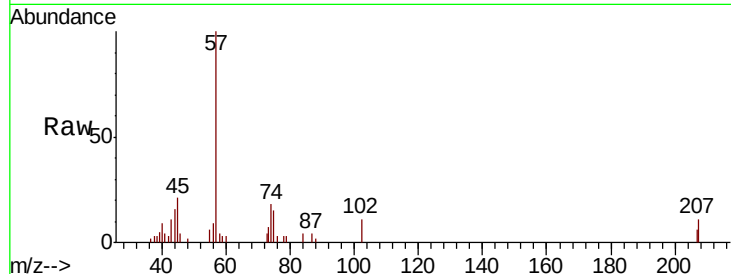

#50
Toluene-d8
Concen: 53.438 ug/l
RT: 8.70 min Scan# 1248
Delta R.T. -0.00 min
Lab File: VX017339.D
Acq: 10 Jul 2020 16:41

Tgt Ion: 98 Resp: 535609
Ion Ratio Lower Upper
98 100
100 66.4 53.8 80.6



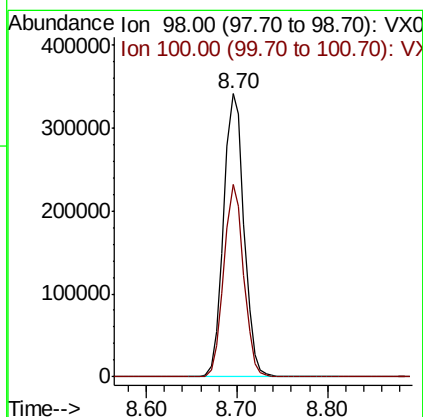
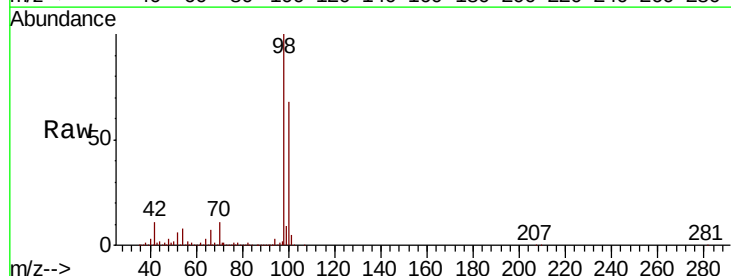




#51
 4-Methyl-2-Pentanone
 Concen: 12.921 ug/l
 RT: 8.59 min Scan# 1231
 Delta R.T. -0.03 min
 Lab File: VX017339.D
 Acq: 10 Jul 2020 16:41




Instrument :
 MSVOA_X
 ClientSampleId :


Tot Ion: 43 Resp: 52592
 Ion Ratio Lower Upper
 43 100
 58 6.1 31.9 47.9#

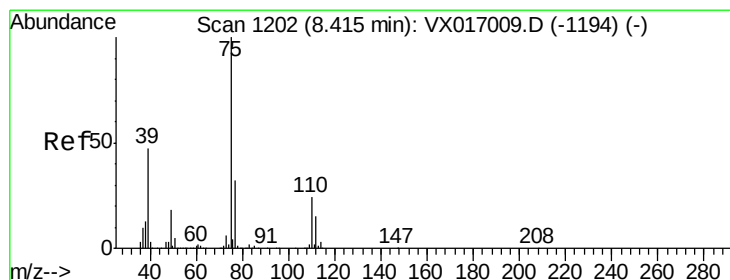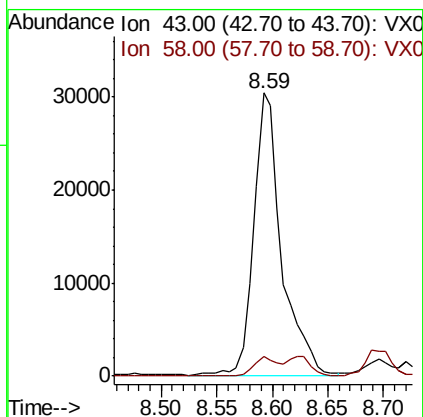

#54
 cis-1,3-Dichloropropene
 Concen: 4.343 ug/l
 RT: 8.60 min Scan# 1232
 Delta R.T. 0.18 min
 Lab File: VX017339.D
 Acq: 10 Jul 2020 16:41

Tgt Ion: 75 Resp: 22090
 Ion Ratio Lower Upper
 75 100
 77 1.0 25.2 37.8#
 39 28.2 37.4 56.2#

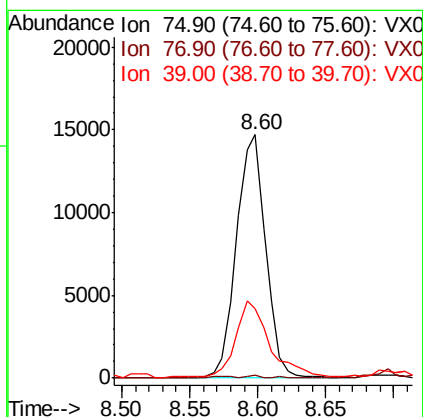



#57

1,3-Dichloropropane

Concen: 0.665 ug/l

RT: 9.52 min Scan# 1384

Delta R.T. 0.17 min

Lab File: VX017339.D

Acq: 10 Jul 2020 16:41

Instrument :

MSVOA_X


ClientSampleId :

Tot Ion: 76 Resp: 3415

Ion Ratio Lower Upper




76 100

78 0.0 25.9 38.9#



Abundance Ion 75.90 (75.60 to 76.60): VX0

Ion 77.90 (77.60 to 78.60): VX0

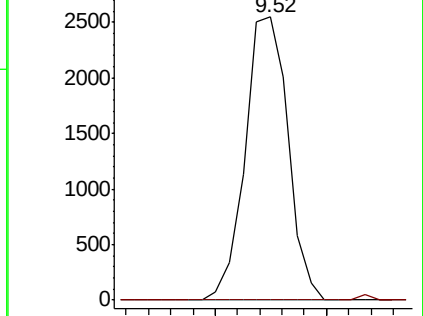

#59

2-Hexanone

Concen: 21.505 ug/l

RT: 9.41 min Scan# 1366

Delta R.T. -0.05 min

Lab File: VX017339.D


Acq: 10 Jul 2020 16:41

Tgt Ion: 43 Resp: 63924

Ion Ratio Lower Upper



43 100


58 0.0 27.9 83.6#



Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0




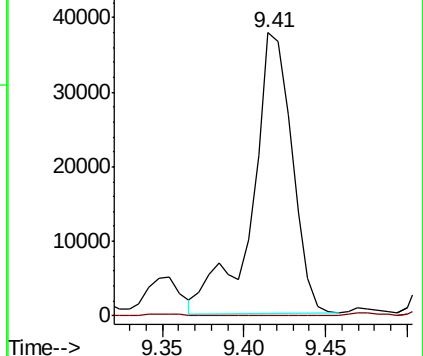




#62
4-Bromofluorobenzene
Concen: 58.761 ug/l
RT: 11.12 min Scan# 1646
Delta R.T. -0.00 min
Lab File: VX017339.D
Acq: 10 Jul 2020 16:41




Instrument :
MSVOA_X
ClientSampleId :


Tot Ion	Ratio	Lower	Upper
95	100		
174	85.8	0.0	164.0
176	84.0	0.0	157.6

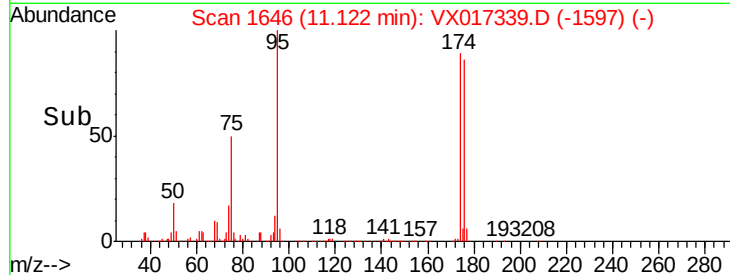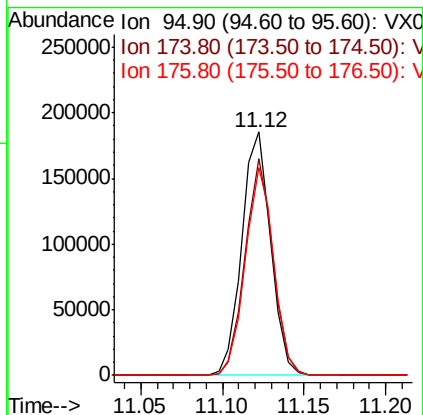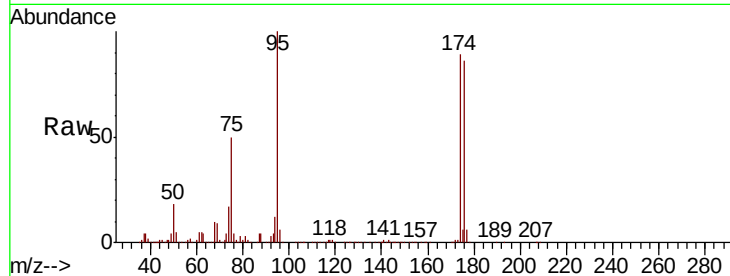

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.10 min Scan# 1478
Delta R.T. -0.00 min
Lab File: VX017339.D
Acq: 10 Jul 2020 16:41

Tgt Ion	Ratio	Lower	Upper
117	100		
82	53.3	42.6	63.8
119	32.8	25.4	38.2

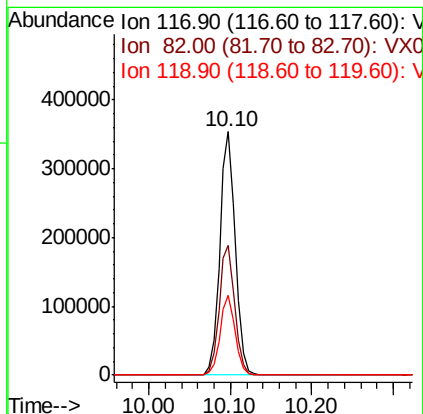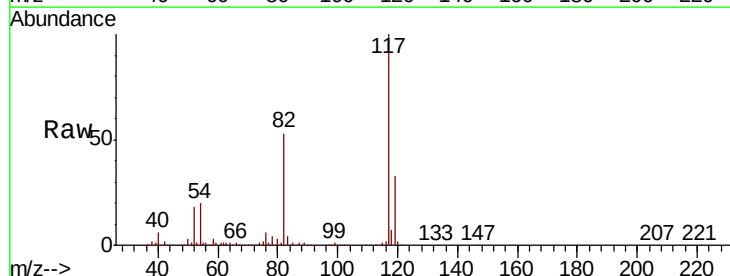



#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.06 min Scan# 1800

Delta R.T. -0.00 min

Lab File: VX017339.D

Acq: 10 Jul 2020 16:41

Instrument :

MSVOA_X

ClientSampleId :


Tot Ion:152 Resp: 245120

Ion Ratio Lower Upper

152 100

115 57.9 40.9 122.7




150 154.6 0.0 351.6

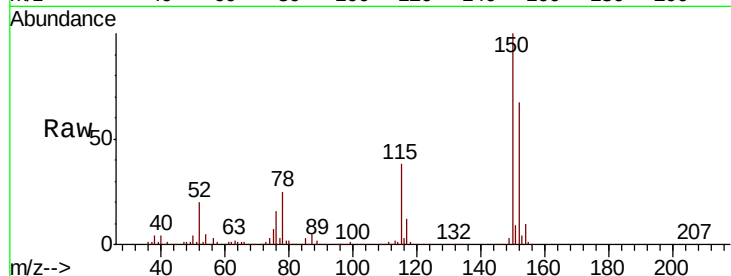

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

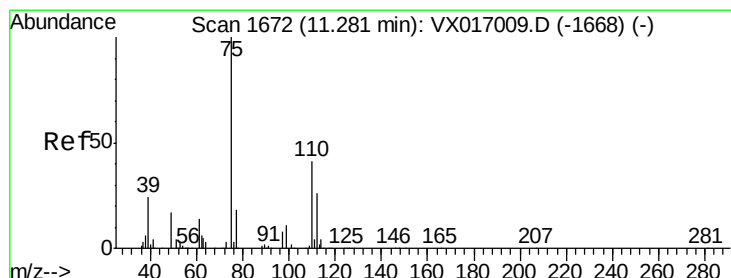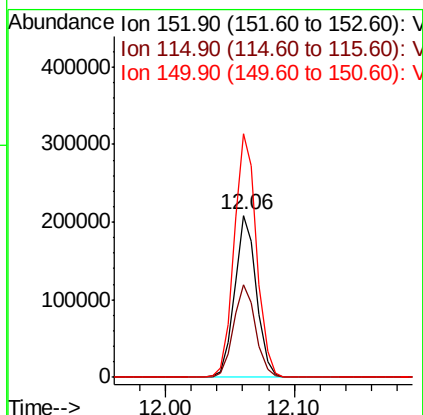

#76

1,2,3-Trichloropropane

Concen: 23.922 ug/l

RT: 11.12 min Scan# 1646

Delta R.T. -0.16 min

Lab File: VX017339.D


Acq: 10 Jul 2020 16:41

Tgt Ion: 75 Resp: 115309

Ion Ratio Lower Upper



75 100


77 1.2 20.2 60.6#

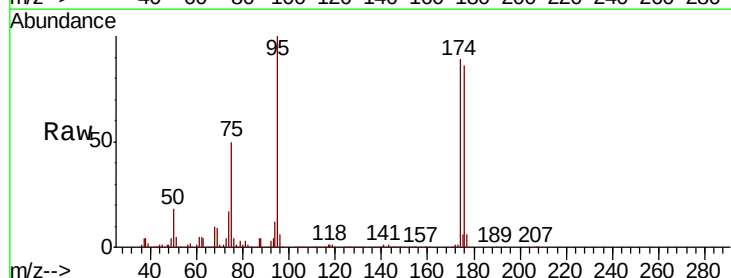

Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 77.00 (76.70 to 77.70): VX0



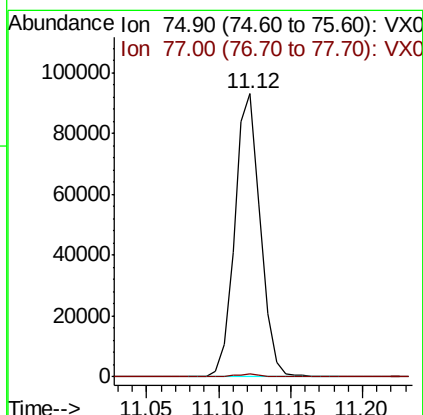





#81
trans-1,4-Dichloro-2-butene
Concen: 61.950 ug/l
RT: 11.12 min Scan# 1646
Delta R.T. 0.07 min
Lab File: VX017339.D
Acq: 10 Jul 2020 16:41




Instrument :
MSVOA_X
ClientSampleId :


Tot Ion: 75 Resp: 115309
Ion Ratio Lower Upper
75 100
53 0.2 72.4 108.6#
89 0.0 37.0 55.4#

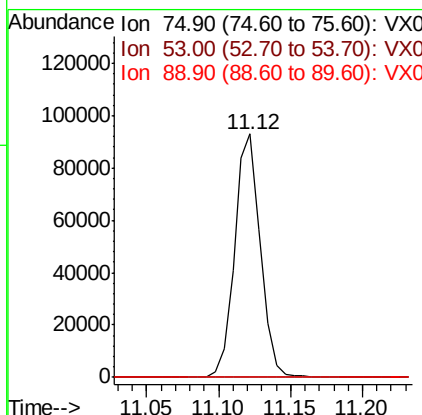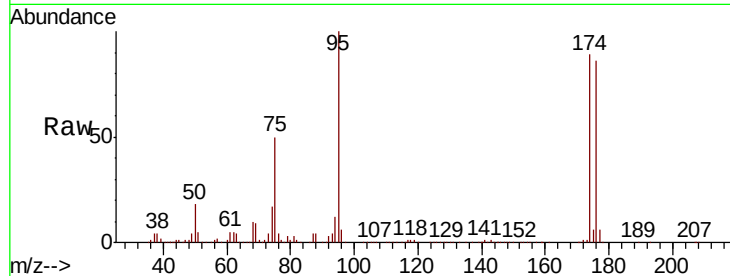

#94
Hexachlorobutadiene
Concen: 0.997 ug/l
RT: 13.76 min Scan# 2079
Delta R.T. -0.01 min
Lab File: VX017339.D
Acq: 10 Jul 2020 16:41

Tgt Ion: 225 Resp: 301
Ion Ratio Lower Upper
225 100
223 71.1 32.5 97.5
227 55.1 33.1 99.2

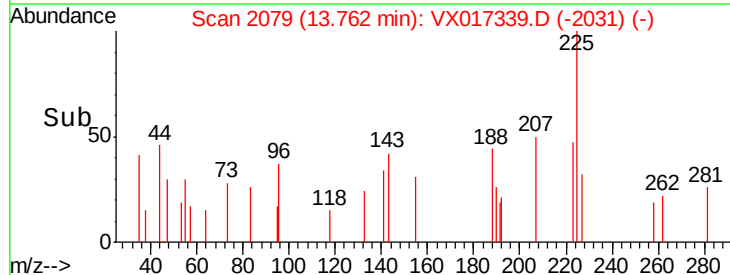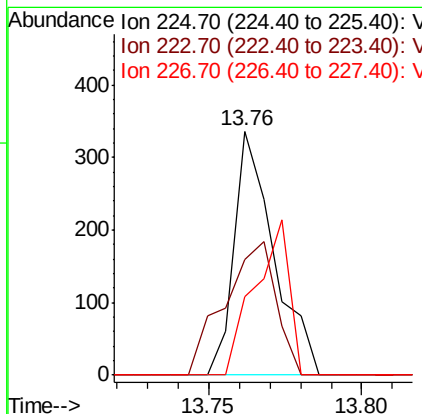

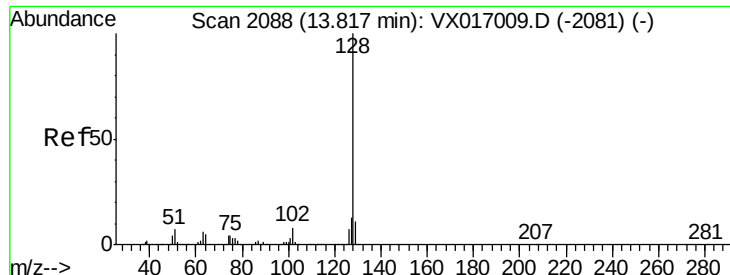

#95

Naphthalene

Concen: 0.243 ug/l

RT: 13.82 min Scan# 2088

Delta R.T. -0.00 min

Lab File: VX017339.D

Acq: 10 Jul 2020 16:41

Instrument :

MSVOA_X

ClientSampleId :


Tot Ion:128 Resp: 3779

Ion Ratio Lower Upper

128 100

127 12.6 10.2 15.4

129 15.2 8.7 13.1#



Abundance Ion 128.00 (127.70 to 128.70): V

Ion 127.00 (126.70 to 127.70): V

Ion 129.00 (128.70 to 129.70): V

