


Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX071020\
 Data File : VX017323.D
 Acq On : 10 Jul 2020 09:05
 Operator : JC/SP
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X062920W.M
 Title : SW846 8260
 Last Update : Mon Jun 29 17:10:38 2020

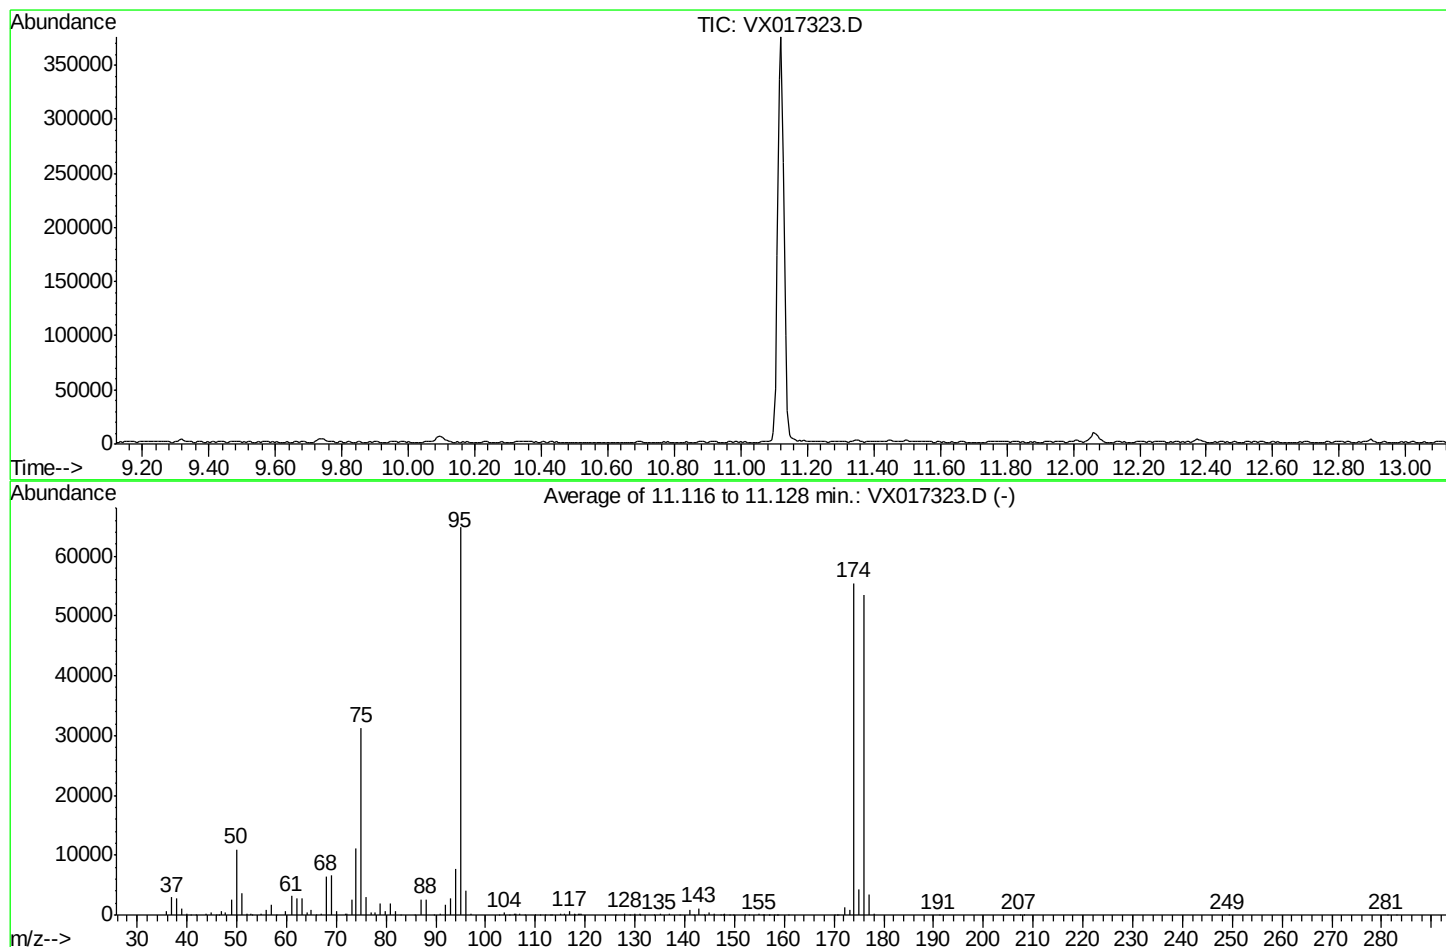

AutoFind: Scans 1645, 1646, 1647; Background Corrected with Scan 1638

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.0	11007	PASS
75	95	30	60	48.3	31290	PASS
95	95	100	100	100.0	64824	PASS
96	95	5	9	6.2	3998	PASS
173	174	0.00	2	1.5	818	PASS
174	95	50	100	85.7	55541	PASS
175	174	5	9	7.7	4285	PASS
176	174	95	101	96.3	53512	PASS
177	176	5	9	6.4	3424	PASS