

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071023\
 Data File : VX036475.D
 Acq On : 10 Jul 2023 11:42
 Operator : JC/MD
 Sample : VX0710MBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0710MBL01

Quant Time: Jul 11 01:25:47 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062323W.M
 Quant Title : SW846 8260
 QLast Update : Fri Jun 23 15:03:28 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.550	168	191670	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	325700	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	303404	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	140615	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	125429	45.653	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery =	91.300%		
35) Dibromofluoromethane	5.385	113	104420	48.622	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	97.240%		
50) Toluene-d8	8.647	98	398174	49.640	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery =	99.280%		
62) 4-Bromofluorobenzene	11.079	95	143656	50.846	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	101.700%		
Target Compounds					Qvalue	
5) Bromomethane	1.611	94	1317	0.523	ug/l #	58
11) Tert butyl alcohol	2.946	59	4393	8.784	ug/l #	81
13) Acrolein	2.239	56	455	0.662	ug/l	88
15) Acrylonitrile	3.068	53	946	0.746	ug/l	90
16) Acetone	2.392	43	1536	1.308	ug/l #	86
17) Carbon Disulfide	2.514	76	2495	0.466	ug/l #	93
20) Methylene Chloride	2.788	84	753	0.298	ug/l	93
21) trans-1,2-Dichloroethene	3.099	96	519	0.223	ug/l #	81
23) Vinyl Acetate	3.727	43	1961	0.381	ug/l #	73
25) 2-Butanone	4.580	43	1268	0.751	ug/l #	51
29) Tetrahydrofuran	5.013	42	773	0.720	ug/l #	54
31) Cyclohexane	5.550	56	4322	1.228	ug/l #	7
36) 1,1-Dichloropropene	5.544	75	16055	5.015	ug/l #	50
38) Carbon Tetrachloride	5.544	117	19970	6.830	ug/l #	15
51) 4-Methyl-2-Pentanone	8.574	43	1507	0.449	ug/l	95
58) 2-Chloroethyl Vinyl ether	8.244	63	663	0.335	ug/l	90
59) 2-Hexanone	9.439	43	1382	0.564	ug/l	92
76) 1,2,3-Trichloropropane	11.079	75	74515	24.844	ug/l #	38
81) trans-1,4-Dichloro-2-b...	11.079	75	74515	80.984	ug/l #	5
82) 4-Chlorotoluene	11.457	91	1795	0.209	ug/l	100
86) p-Isopropyltoluene	12.006	119	2019	0.221	ug/l #	73
87) 1,3-Dichlorobenzene	11.969	146	1185	0.247	ug/l	96
88) 1,4-Dichlorobenzene	11.969	146	1185	0.243	ug/l	97
89) n-Butylbenzene	12.329	91	2339	0.287	ug/l	94
91) 1,2-Dichlorobenzene	12.335	146	1243	0.264	ug/l	95
93) 1,2,4-Trichlorobenzene	13.591	180	1808	0.622	ug/l	97
94) Hexachlorobutadiene	13.725	225	974	0.819	ug/l	94
95) Naphthalene	13.774	128	5713	0.595	ug/l	98
96) 1,2,3-Trichlorobenzene	13.963	180	2166	0.764	ug/l	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071023\
Data File : VX036475.D
Acq On : 10 Jul 2023 11:42
Operator : JC/MD
Sample : VX0710MBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0710MBL01

Quant Time: Jul 11 01:25:47 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062323W.M
Quant Title : SW846 8260
QLast Update : Fri Jun 23 15:03:28 2023
Response via : Initial Calibration




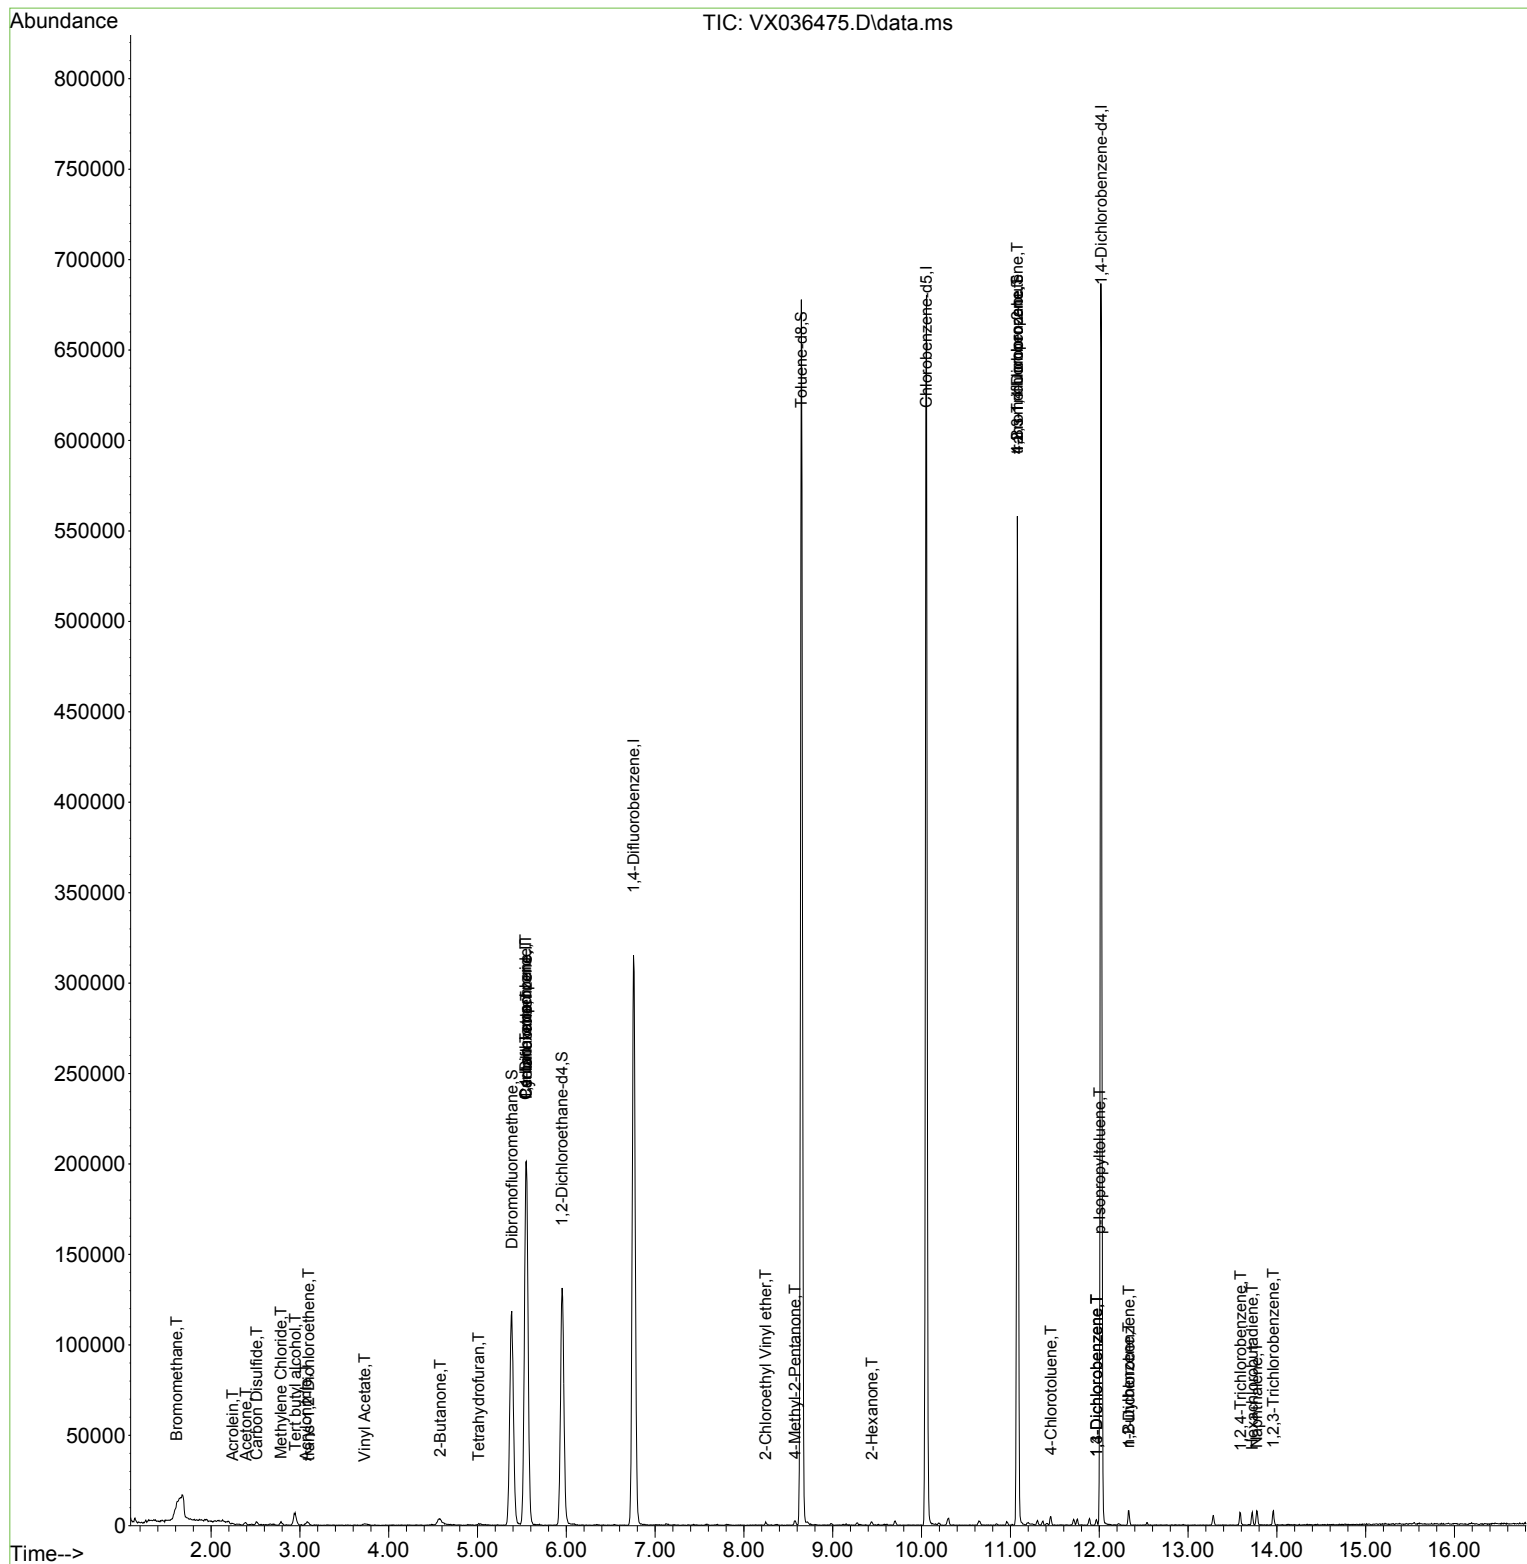




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. 0.001 min
Lab File: VX036475.D
Acq: 10 Jul 2023 11:42




Instrument :
MSVOA_X
ClientSampleId :
VX0710MBL01


Tgt Ion:168 Resp: 191670
Ion Ratio Lower Upper
168 100
99 60.2 56.6 85.0

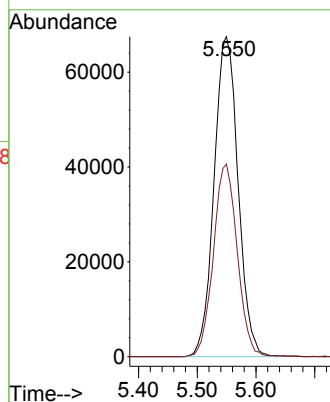

#5
Bromomethane
Concen: 0.523 ug/l
RT: 1.611 min Scan# 86
Delta R.T. -0.006 min
Lab File: VX036475.D
Acq: 10 Jul 2023 11:42

Tgt Ion: 94 Resp: 1317
Ion Ratio Lower Upper
94 100
96 52.5 74.6 111.8#





#11

Tert butyl alcohol

Concen: 8.784 ug/l

RT: 2.946 min Scan# 305

Delta R.T. -0.067 min

Lab File: VX036475.D

Acq: 10 Jul 2023 11:42

Instrument :

MSVOA_X

ClientSampleId :





VX0710MBL01

Tgt Ion: 59 Resp: 4393

Ion Ratio Lower Upper

59 100

57 0.7 6.0 9.0#

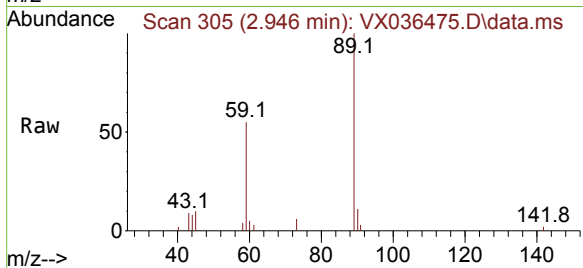

#13

Acrolein

Concen: 0.662 ug/l

RT: 2.239 min Scan# 189

Delta R.T. 0.000 min

Lab File: VX036475.D




Acq: 10 Jul 2023 11:42


Tgt Ion: 56 Resp: 455

Ion Ratio Lower Upper

56 100


55 81.3 57.1 85.7

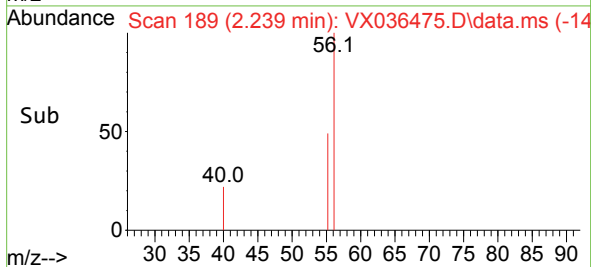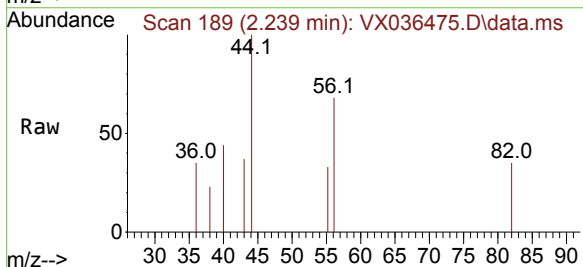





#15
Acrylonitrile
Concen: 0.746 ug/l
RT: 3.068 min Scan# 31
Delta R.T. -0.006 min
Lab File: VX036475.D
Acq: 10 Jul 2023 11:42

Instrument :
MSVOA_X
ClientSampleId :
VX0710MBL01







Tgt Ion:	53	Resp:	946
Ion	Ratio	Lower	Upper
53	100		
52	72.9	66.0	99.0
51	32.6	29.8	44.6

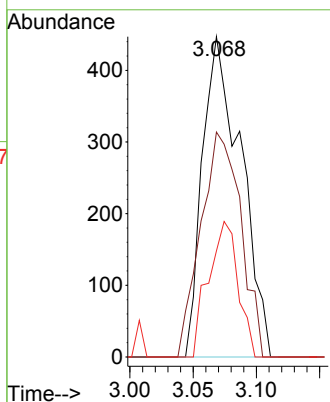

#16
Acetone
Concen: 1.308 ug/l
RT: 2.392 min Scan# 214
Delta R.T. -0.012 min
Lab File: VX036475.D
Acq: 10 Jul 2023 11:42

Tgt Ion:	43	Resp:	1536
Ion	Ratio	Lower	Upper
43	100		
58	20.3	21.9	32.9#



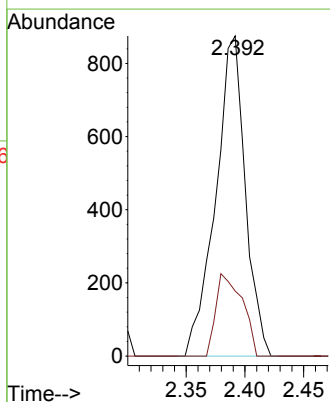





#17
Carbon Disulfide
Concen: 0.466 ug/l
RT: 2.514 min Scan# 21
Delta R.T. 0.001 min
Lab File: VX036475.D
Acq: 10 Jul 2023 11:42




Instrument :
MSVOA_X
ClientSampleId :
VX0710MBL01


Tgt Ion: 76 Resp: 2495
Ion Ratio Lower Upper
76 100
78 6.4 7.0 10.6#

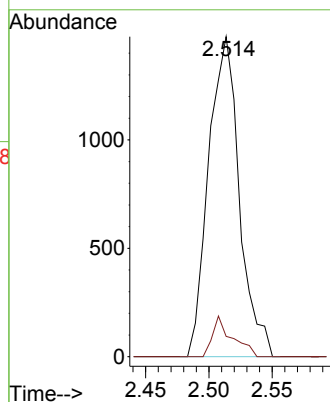

#20
Methylene Chloride
Concen: 0.298 ug/l
RT: 2.788 min Scan# 279
Delta R.T. -0.000 min
Lab File: VX036475.D
Acq: 10 Jul 2023 11:42

Tgt Ion: 84 Resp: 753
Ion Ratio Lower Upper
84 100
49 121.8 103.6 155.4
51 50.0 33.8 50.6
86 64.6 49.4 74.0




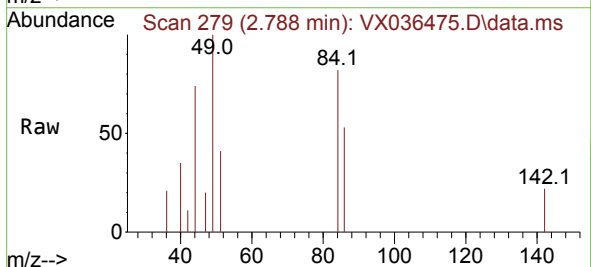




#21
trans-1,2-Dichloroethene
Concen: 0.223 ug/l
RT: 3.099 min Scan# 31
Delta R.T. 0.006 min
Lab File: VX036475.D
Acq: 10 Jul 2023 11:42




Instrument :
MSVOA_X
ClientSampleId :
VX0710MBL01


Tgt Ion: 96 Resp: 519
Ion Ratio Lower Upper
96 100
61 127.8 119.2 178.8
98 42.1 48.7 73.1#

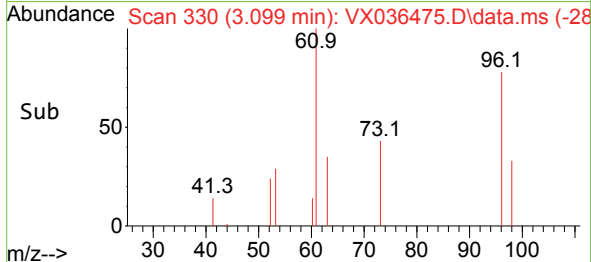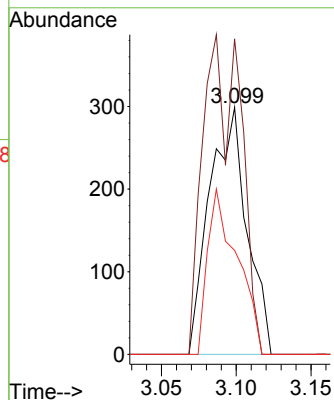

#23
Vinyl Acetate
Concen: 0.381 ug/l
RT: 3.727 min Scan# 433
Delta R.T. 0.006 min
Lab File: VX036475.D
Acq: 10 Jul 2023 11:42

Tgt Ion: 43 Resp: 1961
Ion Ratio Lower Upper
43 100
86 0.0 7.8 11.8#

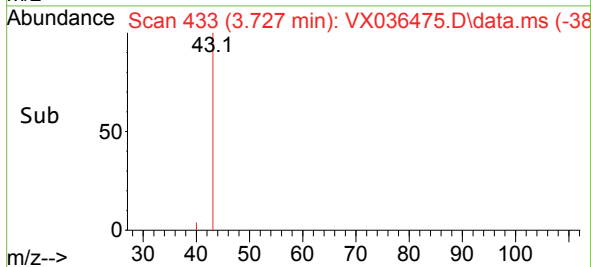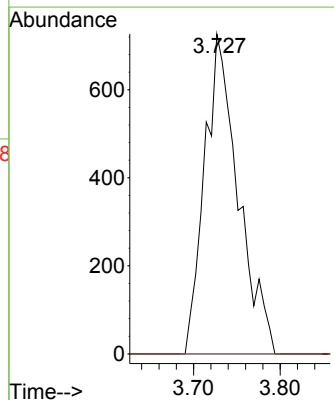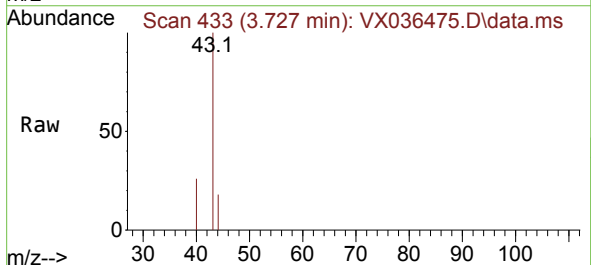

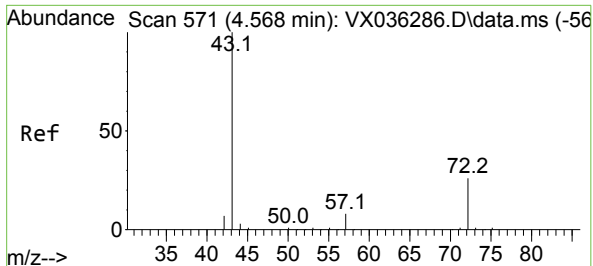

#25

2-Butanone

Concen: 0.751 ug/l

RT: 4.580 min Scan# 571

Delta R.T. 0.012 min

Lab File: VX036475.D

Acq: 10 Jul 2023 11:42

Instrument :

MSVOA_X

ClientSampleId :





VX0710MBL01

Tgt Ion: 43 Resp: 1268

Ion Ratio Lower Upper

43 100

72 0.0 19.4 29.2#

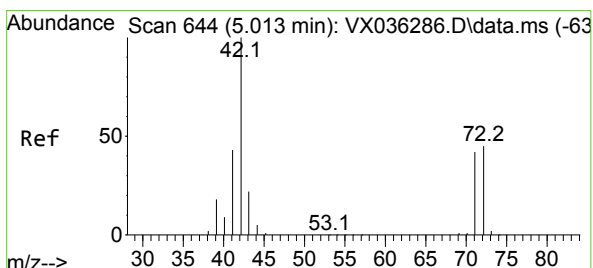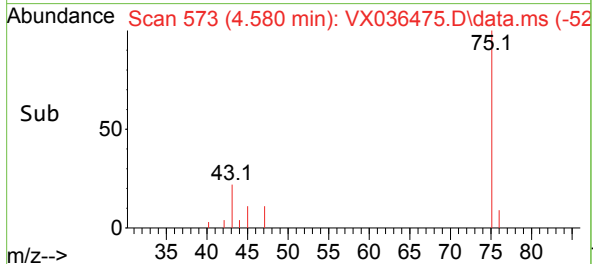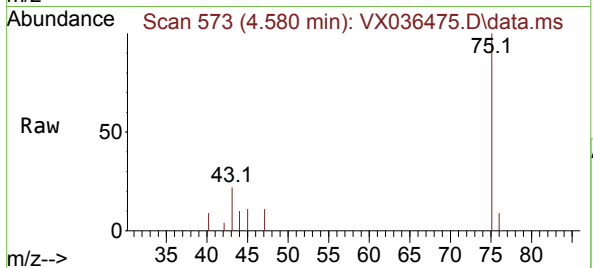

#29

Tetrahydrofuran

Concen: 0.720 ug/l

RT: 5.013 min Scan# 644

Delta R.T. -0.006 min

Lab File: VX036475.D

Acq: 10 Jul 2023 11:42




Tgt Ion: 42 Resp: 773


Ion Ratio Lower Upper

42 100

72 15.0 34.2 51.4#


71 10.2 32.2 48.2#

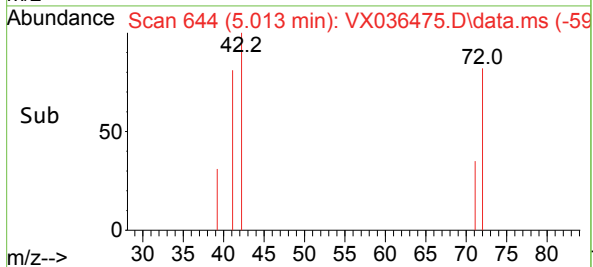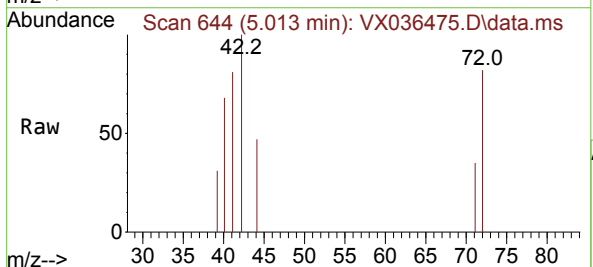






#31
Cyclohexane
Concen: 1.228 ug/l
RT: 5.550 min Scan# 71
Delta R.T. 0.080 min
Lab File: VX036475.D
Acq: 10 Jul 2023 11:42

Instrument :
MSVOA_X
ClientSampleId :
VX0710MBL01







Tgt Ion: 56 Resp: 4322
Ion Ratio Lower Upper
56 100
69 155.8 23.4 35.2#
84 120.4 65.9 98.9#

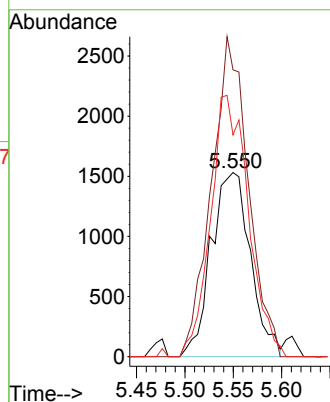

#33
1,2-Dichloroethane-d4
Concen: 45.653 ug/l
RT: 5.952 min Scan# 798
Delta R.T. -0.006 min
Lab File: VX036475.D
Acq: 10 Jul 2023 11:42

Tgt Ion: 65 Resp: 125429
Ion Ratio Lower Upper
65 100
67 51.9 0.0 100.2









#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.757 min Scan# 91
Delta R.T. -0.006 min
Lab File: VX036475.D
Acq: 10 Jul 2023 11:42




Instrument :
MSVOA_X
ClientSampleId :
VX0710MBL01


Tgt Ion:114 Resp: 325700
Ion Ratio Lower Upper
114 100
63 20.0 0.0 45.0
88 15.4 0.0 36.6



#35
Dibromofluoromethane
Concen: 48.622 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.000 min
Lab File: VX036475.D
Acq: 10 Jul 2023 11:42

Tgt Ion:113 Resp: 104420
Ion Ratio Lower Upper
113 100
111 101.5 82.9 124.3
192 18.3 13.3 19.9









#36
1,1-Dichloropropene
Concen: 5.015 ug/l
RT: 5.544 min Scan# 71
Delta R.T. -0.152 min
Lab File: VX036475.D
Acq: 10 Jul 2023 11:42




Instrument :
MSVOA_X
ClientSampleId :
VX0710MBL01


Tgt Ion: 75 Resp: 16055
Ion Ratio Lower Upper
75 100
110 8.8 17.0 50.9#
77 0.0 24.7 37.1#

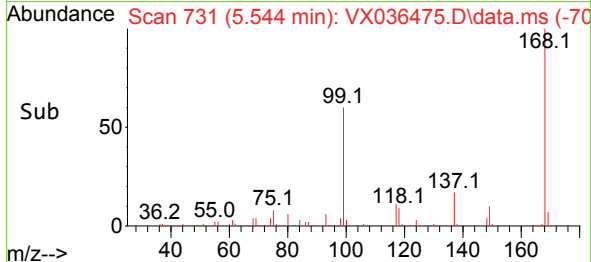

#38
Carbon Tetrachloride
Concen: 6.830 ug/l
RT: 5.544 min Scan# 731
Delta R.T. -0.134 min
Lab File: VX036475.D
Acq: 10 Jul 2023 11:42

Tgt Ion: 117 Resp: 19970
Ion Ratio Lower Upper
117 100
119 4.7 78.2 117.2#
121 0.0 24.4 36.6#


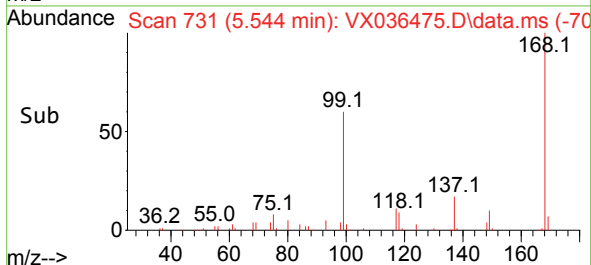
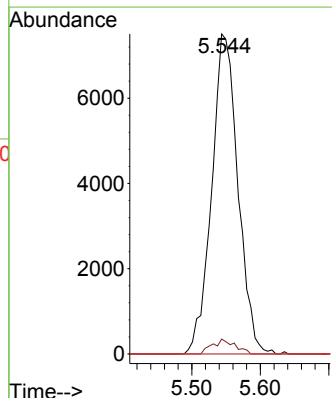
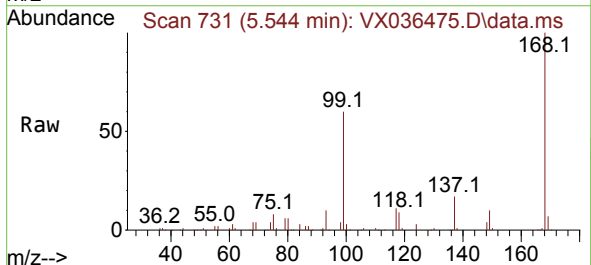




#50
Toluene-d8
Concen: 49.640 ug/l
RT: 8.647 min Scan# 1240
Delta R.T. 0.001 min
Lab File: VX036475.D
Acq: 10 Jul 2023 11:42




Instrument :
MSVOA_X
ClientSampleId :
VX0710MBL01


Tgt Ion: 98 Resp: 398174
Ion Ratio Lower Upper
98 100
100 63.5 53.1 79.7

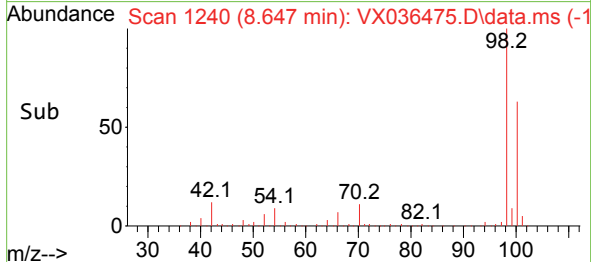

#51
4-Methyl-2-Pentanone
Concen: 0.449 ug/l
RT: 8.574 min Scan# 1228
Delta R.T. 0.001 min
Lab File: VX036475.D
Acq: 10 Jul 2023 11:42

Tgt Ion: 43 Resp: 1507
Ion Ratio Lower Upper
43 100
58 40.7 30.4 45.6


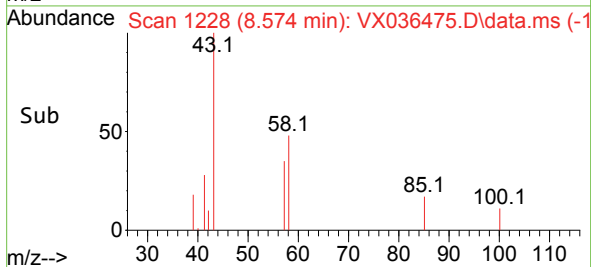

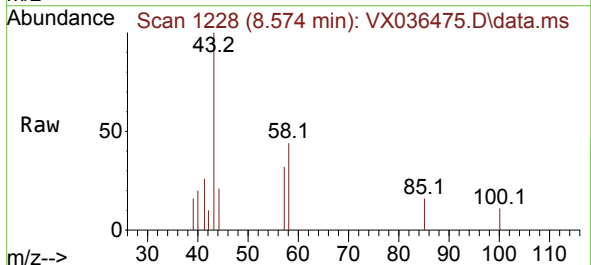




#58
2-Chloroethyl Vinyl ether
Concen: 0.335 ug/l
RT: 8.244 min Scan# 1174
Delta R.T. 0.000 min
Lab File: VX036475.D
Acq: 10 Jul 2023 11:42




Instrument :
MSVOA_X
ClientSampleId :
VX0710MBL01


Tgt Ion: 63 Resp: 663
Ion Ratio Lower Upper
63 100
106 22.6 22.5 33.7



#59
2-Hexanone
Concen: 0.564 ug/l
RT: 9.439 min Scan# 1370
Delta R.T. 0.006 min
Lab File: VX036475.D
Acq: 10 Jul 2023 11:42

Tgt Ion: 43 Resp: 1382
Ion Ratio Lower Upper
43 100
58 47.0 26.2 78.5


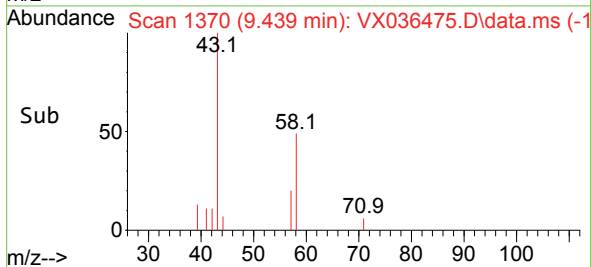

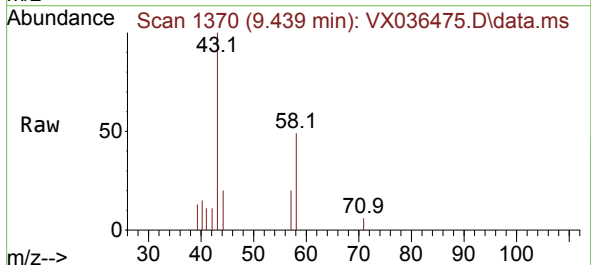




#62
4-Bromofluorobenzene
Concen: 50.846 ug/l
RT: 11.079 min Scan# 1
Delta R.T. 0.000 min
Lab File: VX036475.D
Acq: 10 Jul 2023 11:42




Instrument :
MSVOA_X
ClientSampleId :
VX0710MBL01


Tgt Ion: 95 Resp: 143656
Ion Ratio Lower Upper
95 100
174 77.1 0.0 135.6
176 74.5 0.0 131.0

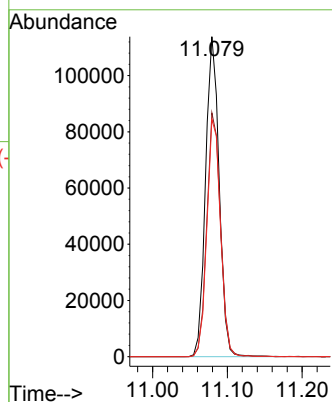

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX036475.D
Acq: 10 Jul 2023 11:42

Tgt Ion: 117 Resp: 303404
Ion Ratio Lower Upper
117 100
82 54.5 46.2 69.4
119 32.5 25.5 38.3





#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.024 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX036475.D

Acq: 10 Jul 2023 11:42

Instrument :

MSVOA_X

ClientSampleId :

VX0710MBL01





Tgt Ion:152 Resp: 140615

Ion Ratio Lower Upper

152 100

115 60.3 43.3 129.9

150 158.3 0.0 345.0

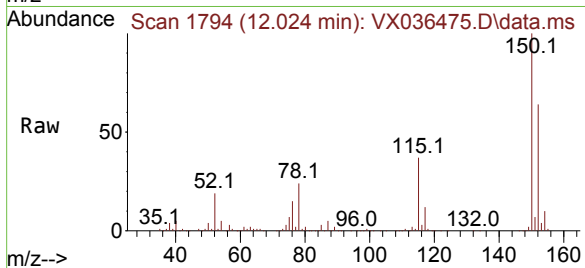

#76

1,2,3-Trichloropropane

Concen: 24.844 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. -0.159 min

Lab File: VX036475.D




Acq: 10 Jul 2023 11:42


Tgt Ion: 75 Resp: 74515

Ion Ratio Lower Upper

75 100

77 1.0 19.1 57.5#




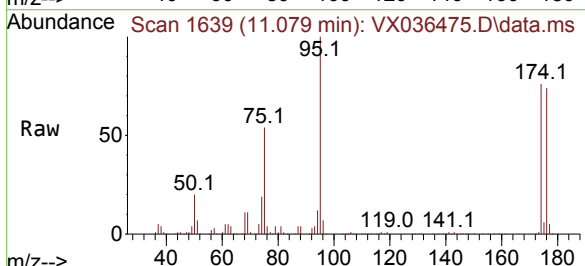




#81
trans-1,4-Dichloro-2-butene
Concen: 80.984 ug/l
RT: 11.079 min Scan# 1
Delta R.T. 0.061 min
Lab File: VX036475.D
Acq: 10 Jul 2023 11:42




Instrument :
MSVOA_X
ClientSampleId :
VX0710MBL01


Tgt Ion: 75 Resp: 74515
Ion Ratio Lower Upper
75 100
53 0.0 90.5 135.7#
89 0.0 36.9 55.3#

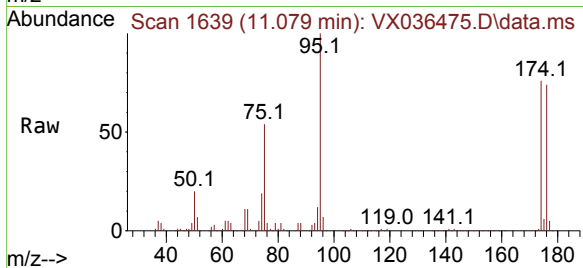

#82
4-Chlorotoluene
Concen: 0.209 ug/l
RT: 11.457 min Scan# 1701
Delta R.T. 0.006 min
Lab File: VX036475.D
Acq: 10 Jul 2023 11:42

Tgt Ion: 91 Resp: 1795
Ion Ratio Lower Upper
91 100
126 28.3 14.2 42.6




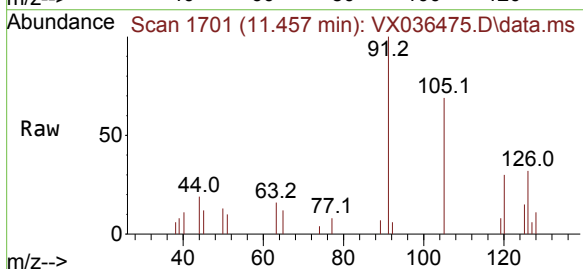




#86
 p-Isopropyltoluene
 Concen: 0.221 ug/l
 RT: 12.006 min Scan# 1791
 Delta R.T. -0.000 min
 Lab File: VX036475.D
 Acq: 10 Jul 2023 11:42




Instrument :
 MSVOA_X
 ClientSampleId :
 VX0710MBL01


Tgt Ion:	119	Resp:	2019
Ion	Ratio	Lower	Upper
119	100		
134	35.2	12.8	38.3
91	44.4	13.1	39.3#

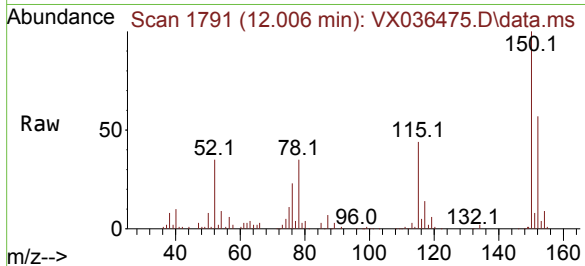

#87
 1,3-Dichlorobenzene
 Concen: 0.247 ug/l
 RT: 11.969 min Scan# 1785
 Delta R.T. 0.000 min
 Lab File: VX036475.D
 Acq: 10 Jul 2023 11:42


Tgt Ion:	146	Resp:	1185
Ion	Ratio	Lower	Upper
146	100		
111	38.2	22.1	66.1
148	63.3	31.8	95.3

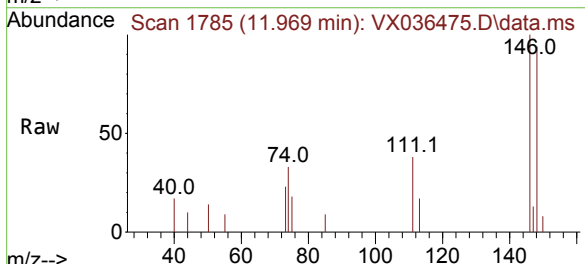






#88
1,4-Dichlorobenzene
Concen: 0.243 ug/l
RT: 11.969 min Scan# 1785
Delta R.T. -0.073 min
Lab File: VX036475.D
Acq: 10 Jul 2023 11:42

Instrument :
MSVOA_X
ClientSampleId :
VX0710MBL01



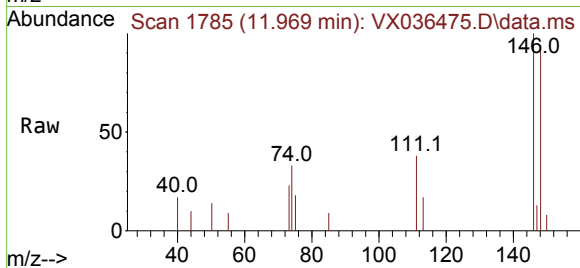



Tgt Ion:146 Resp: 1185
Ion Ratio Lower Upper
146 100
111 38.2 21.3 63.7
148 63.3 31.8 95.4



#89
n-Butylbenzene
Concen: 0.287 ug/l
RT: 12.329 min Scan# 1844
Delta R.T. -0.000 min
Lab File: VX036475.D
Acq: 10 Jul 2023 11:42

Tgt Ion: 91 Resp: 2339
Ion Ratio Lower Upper
91 100
92 50.4 27.4 82.0
134 22.3 12.6 37.8

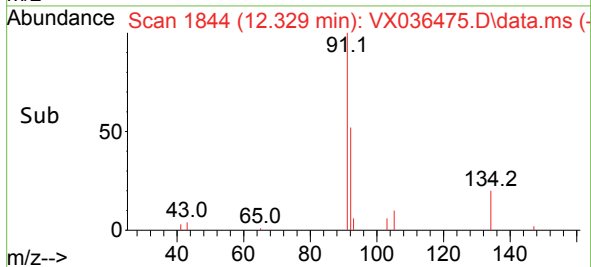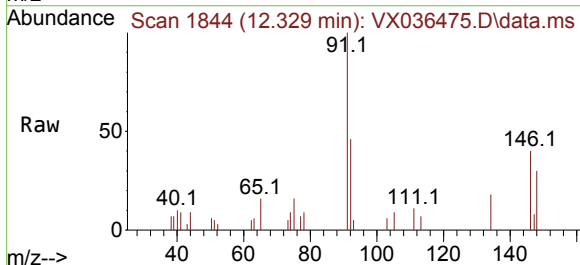



#91

1,2-Dichlorobenzene

Concen: 0.264 ug/l

RT: 12.335 min Scan# 1845

Delta R.T. 0.000 min

Lab File: VX036475.D

Acq: 10 Jul 2023 11:42

Instrument :

MSVOA_X

ClientSampleId :

VX0710MBL01





Tgt Ion:146 Resp: 1243

Ion Ratio Lower Upper

146 100

111 39.4 22.4 67.0

148 61.3 31.6 95.0



#93

1,2,4-Trichlorobenzene

Concen: 0.622 ug/l

RT: 13.591 min Scan# 2051

Delta R.T. 0.006 min

Lab File: VX036475.D

Acq: 10 Jul 2023 11:42




Tgt Ion:180 Resp: 1808


Ion Ratio Lower Upper

180 100

182 97.6 48.3 144.8

145 30.9 18.0 54.0

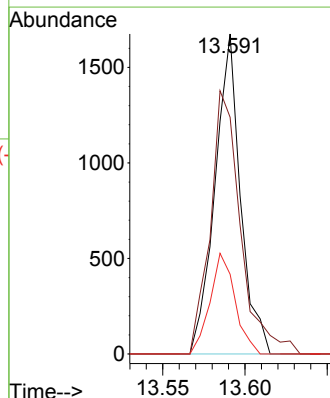



#94

Hexachlorobutadiene

Concen: 0.819 ug/l

RT: 13.725 min Scan# 2073

Delta R.T. 0.000 min

Lab File: VX036475.D

Acq: 10 Jul 2023 11:42

Instrument :





MSVOA_X

ClientSampleId :

VX0710MBL01

Tgt Ion:225 Resp: 974

Ion	Ratio	Lower	Upper
225	100		
223	68.0	31.1	93.2
227	68.8	32.5	97.5

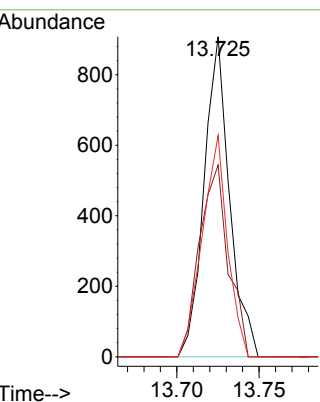

#95

Naphthalene

Concen: 0.595 ug/l

RT: 13.774 min Scan# 2081




Delta R.T. -0.000 min


Lab File: VX036475.D

Acq: 10 Jul 2023 11:42

Tgt Ion:128 Resp: 5713

Ion	Ratio	Lower	Upper
128	100		
127	13.8	10.3	15.5
129	11.3	8.8	13.2

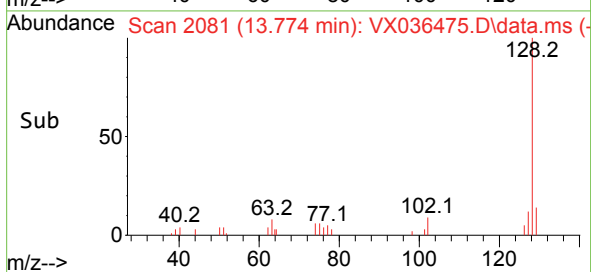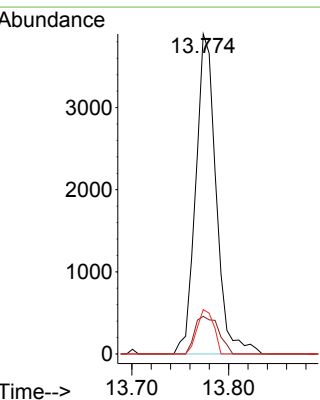



#96

1,2,3-Trichlorobenzene

Concen: 0.764 ug/l

RT: 13.963 min Scan# 2112

Delta R.T. -0.000 min

Lab File: VX036475.D


Acq: 10 Jul 2023 11:42

Instrument :

MSVOA_X

ClientSampleId :

VX0710MBL01

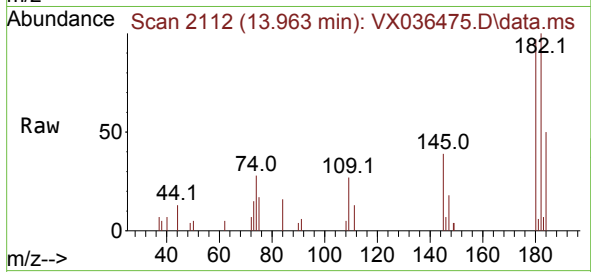

Tgt Ion:180 Resp: 2166

Ion Ratio Lower Upper

180 100

182 90.0 46.9 140.6

145 29.4 17.8 53.5

