

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071024\
 Data File : VX042273.D
 Acq On : 10 Jul 2024 17:30
 Operator : JC/MD
 Sample : P3184-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Jul 11 01:00:58 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061824W.M
 Quant Title : SW846 8260
 QLast Update : Fri Jun 21 23:51:58 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.550	168	162574	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	6.763	114	268872	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	243879	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	119788	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	118443	63.180	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery = 126.360%#			
35) Dibromofluoromethane	5.385	113	112516	58.977	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 117.960%			
50) Toluene-d8	8.647	98	347155	51.797	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery = 103.600%			
62) 4-Bromofluorobenzene	11.079	95	131299	53.145	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery = 106.280%			
Target Compounds						
						Qvalue
6) Chloroethane	1.648	64	94	Below Cal	#	43
11) Tert butyl alcohol	2.989	59	26009	73.103	ug/l	97
15) Acrylonitrile	3.001	53	191	0.206	ug/l #	2
16) Acetone	2.392	43	30272	36.775	ug/l #	87
17) Carbon Disulfide	2.502	76	3560	1.245	ug/l	100
18) Methyl Acetate	2.709	43	3364	1.498	ug/l	96
20) Methylene Chloride	2.788	84	13046	7.238	ug/l	86
25) 2-Butanone	4.599	43	3766	2.941	ug/l	91
29) Tetrahydrofuran	5.050	42	739	0.893	ug/l #	50
32) 1,1,1-Trichloroethane	5.385	97	538	0.235	ug/l #	39
36) 1,1-Dichloropropene	5.550	75	9164	4.523	ug/l #	50
37) Ethyl Acetate	4.739	43	543	0.206	ug/l #	97
38) Carbon Tetrachloride	5.550	117	13525	6.042	ug/l #	15
40) Benzene	6.044	78	6399	0.937	ug/l	95
43) Isopropyl Acetate	6.348	43	74986	18.511	ug/l #	93
48) Methyl methacrylate	7.616	41	3546	1.834	ug/l #	16
51) 4-Methyl-2-Pentanone	8.549	43	44838	16.069	ug/l #	49
52) Toluene	8.720	92	20415	4.692	ug/l	97
53) t-1,3-Dichloropropene	8.958	75	256	1.000	ug/l #	43
54) cis-1,3-Dichloropropene	8.549	75	22503	9.146	ug/l #	50
57) 1,3-Dichloropropane	9.482	76	1996	0.682	ug/l #	42
59) 2-Hexanone	9.482	43	24633	11.526	ug/l #	59
67) Ethyl Benzene	10.195	91	3533	0.444	ug/l	93
68) m/p-Xylenes	10.299	106	4656	1.451	ug/l	97
69) o-Xylene	10.646	106	2522	0.794	ug/l	94
76) 1,2,3-Trichloropropane	11.079	75	59760	27.481	ug/l #	39
81) trans-1,4-Dichloro-2-b...	11.079	75	59760	78.042	ug/l #	5
84) 1,2,4-Trimethylbenzene	11.756	105	2718	0.447	ug/l	90
92) 1,2-Dibromo-3-Chloropr...	12.957	75	400	0.745	ug/l #	9
95) Naphthalene	13.780	128	9639	1.853	ug/l	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071024\
Data File : VX042273.D
Acq On : 10 Jul 2024 17:30
Operator : JC/MD
Sample : P3184-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :


Quant Time: Jul 11 01:00:58 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061824W.M
Quant Title : SW846 8260
QLast Update : Fri Jun 21 23:51:58 2024
Response via : Initial Calibration

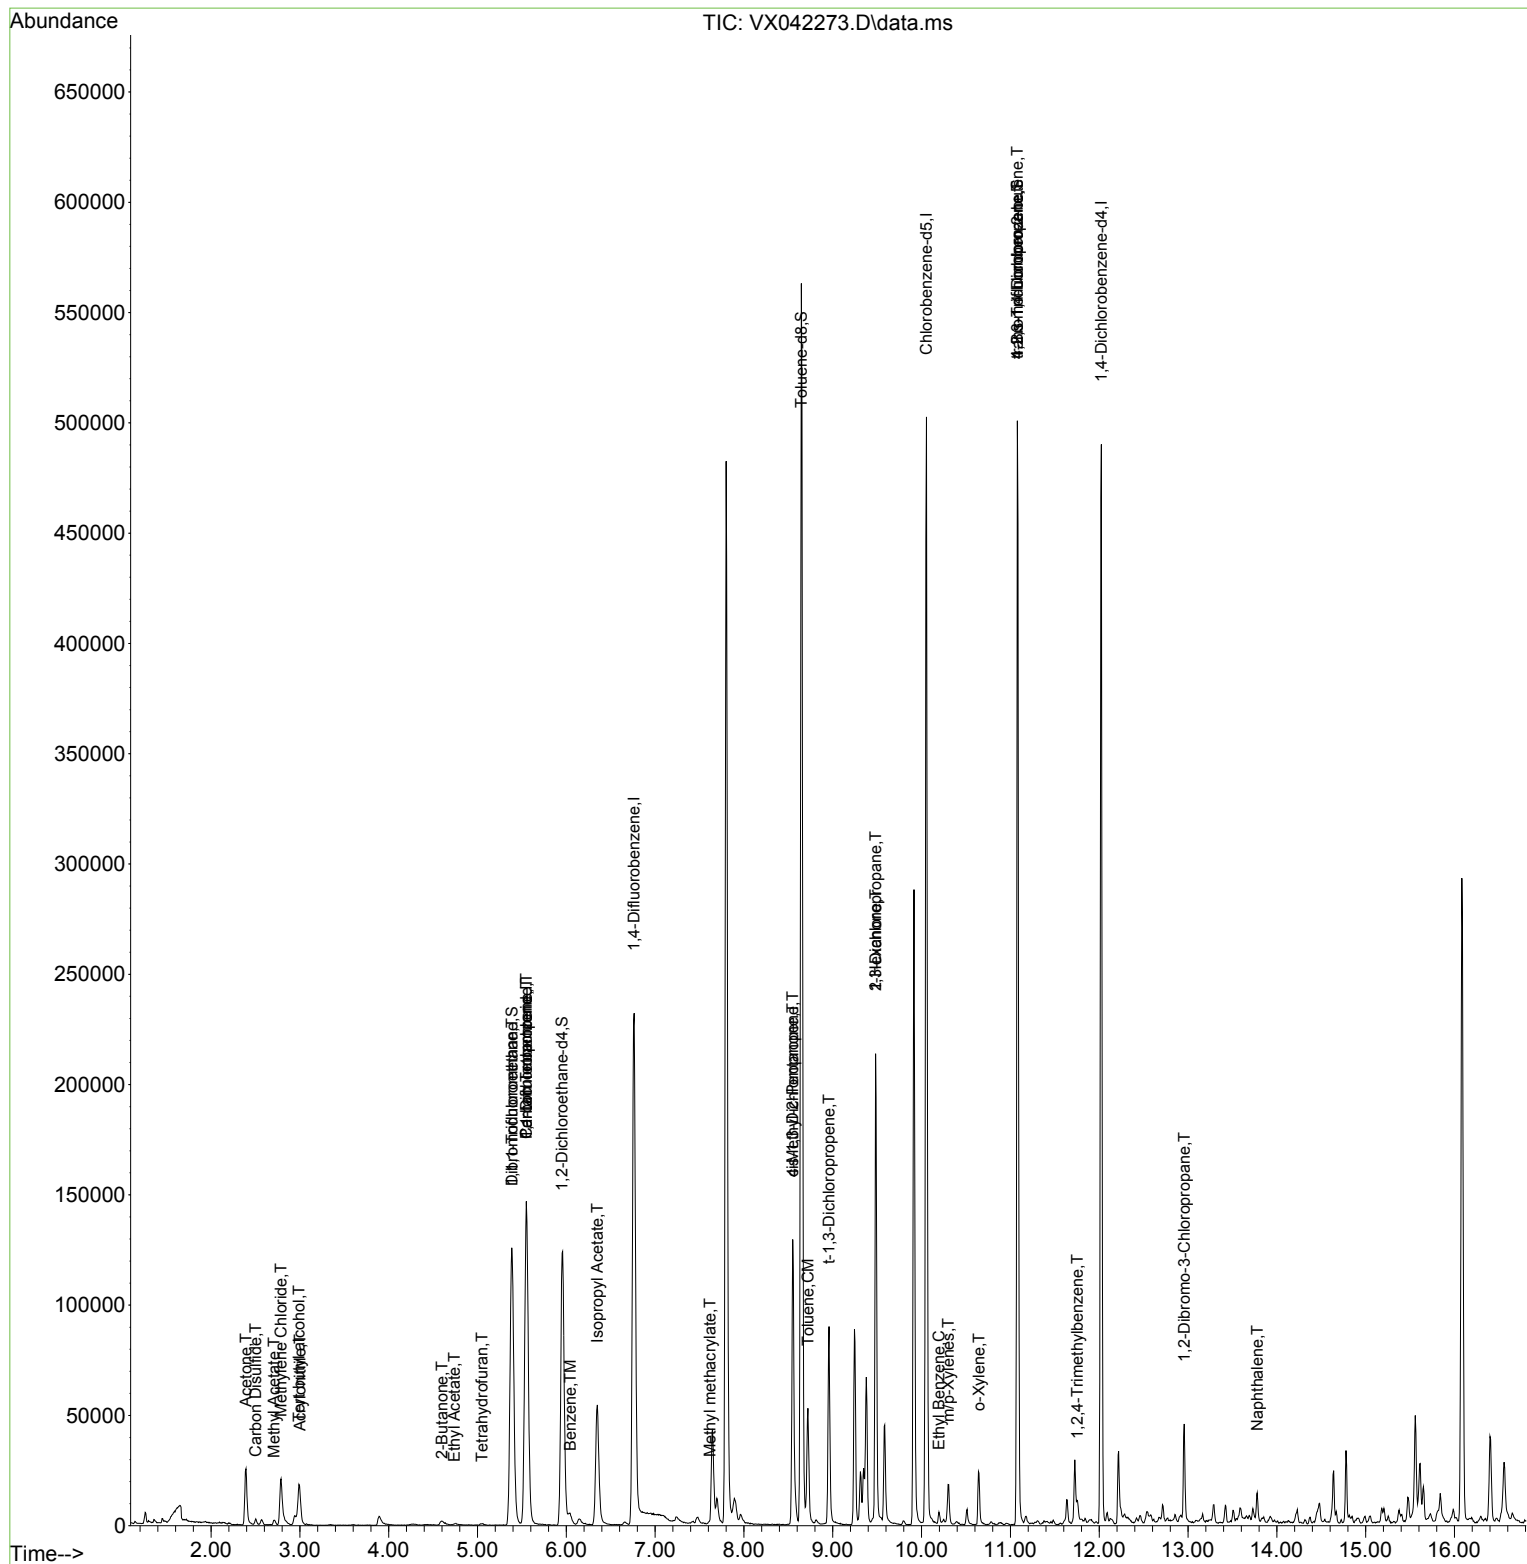






#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX042273.D
Acq: 10 Jul 2024 17:30

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion:168 Resp: 162574
Ion Ratio Lower Upper
168 100
99 46.3 56.6 85.0#



#6
Chloroethane
Concen: Below Cal
RT: 1.648 min Scan# 92
Delta R.T. -0.012 min
Lab File: VX042273.D
Acq: 10 Jul 2024 17:30

Tgt Ion: 64 Resp: 94
Ion Ratio Lower Upper
64 100
66 0.0 25.1 37.7#





#11

Tert butyl alcohol

Concen: 73.103 ug/l

RT: 2.989 min Scan# 312

Delta R.T. -0.018 min

Lab File: VX042273.D

Acq: 10 Jul 2024 17:30

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 59 Resp: 26009

Ion Ratio Lower Upper

59 100

57 8.7 6.0 9.0

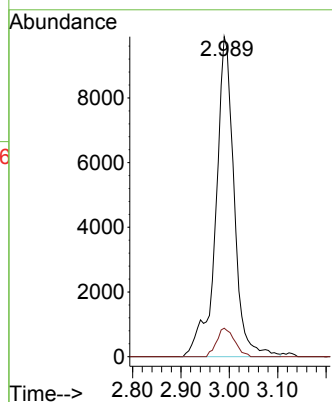

#15

Acrylonitrile

Concen: 0.206 ug/l

RT: 3.001 min Scan# 314

Delta R.T. -0.073 min

Lab File: VX042273.D

Acq: 10 Jul 2024 17:30




Tgt Ion: 53 Resp: 191


Ion Ratio Lower Upper

53 100

52 0.0 66.0 99.0#

51 103.7 29.8 44.6#

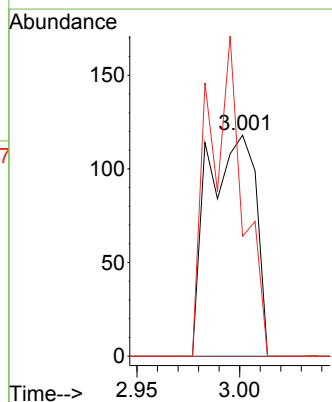



#16

Acetone

Concen: 36.775 ug/l

RT: 2.392 min Scan# 214

Delta R.T. -0.006 min

Lab File: VX042273.D

Acq: 10 Jul 2024 17:30

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 43 Resp: 30272

Ion Ratio Lower Upper

43 100

58 34.2 21.9 32.9#

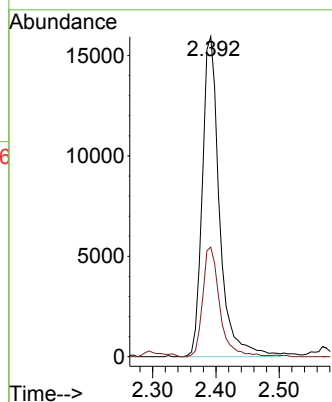

#17

Carbon Disulfide

Concen: 1.245 ug/l

RT: 2.502 min Scan# 232

Delta R.T. 0.000 min

Lab File: VX042273.D




Acq: 10 Jul 2024 17:30


Tgt Ion: 76 Resp: 3560

Ion Ratio Lower Upper

76 100

78 8.6 7.0 10.6









#18
Methyl Acetate
Concen: 1.498 ug/l
RT: 2.709 min Scan# 204
Delta R.T. 0.000 min
Lab File: VX042273.D
Acq: 10 Jul 2024 17:30




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 43 Resp: 3364
Ion Ratio Lower Upper
43 100
74 20.3 17.8 26.8



#20
Methylene Chloride
Concen: 7.238 ug/l
RT: 2.788 min Scan# 279
Delta R.T. 0.006 min
Lab File: VX042273.D
Acq: 10 Jul 2024 17:30


Tgt Ion: 84 Resp: 13046
Ion Ratio Lower Upper
84 100
49 105.4 103.6 155.4
51 35.4 33.8 50.6
86 62.4 49.4 74.0





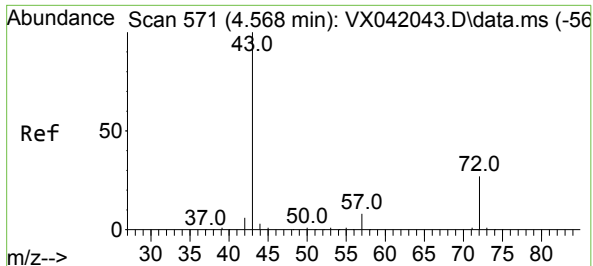


#25
2-Butanone
Concen: 2.941 ug/l
RT: 4.599 min Scan# 51
Delta R.T. 0.024 min
Lab File: VX042273.D
Acq: 10 Jul 2024 17:30

Instrument :
MSVOA_X
ClientSampleId :



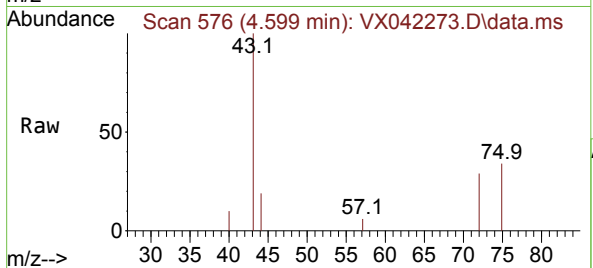



Tgt Ion: 43 Resp: 3766
Ion Ratio Lower Upper
43 100
72 28.6 19.4 29.2

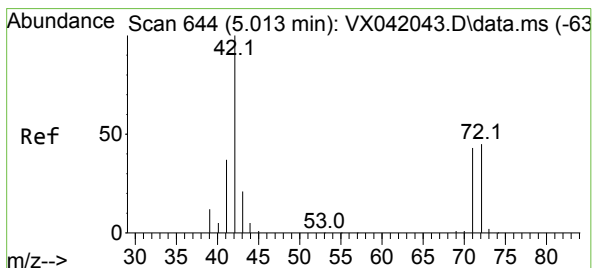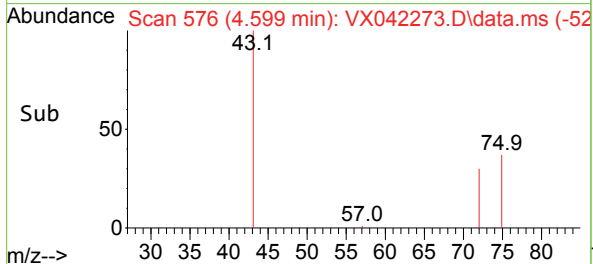

#29
Tetrahydrofuran
Concen: 0.893 ug/l
RT: 5.050 min Scan# 650
Delta R.T. 0.031 min
Lab File: VX042273.D
Acq: 10 Jul 2024 17:30

Tgt Ion: 42 Resp: 739
Ion Ratio Lower Upper
42 100
72 0.0 34.2 51.4#
71 21.0 32.2 48.2#


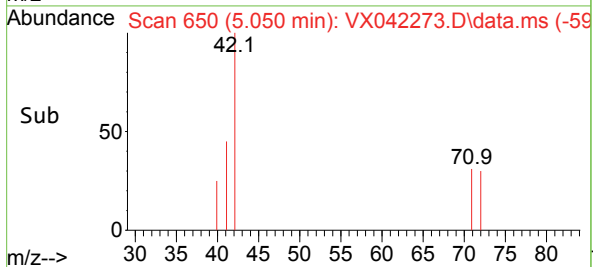

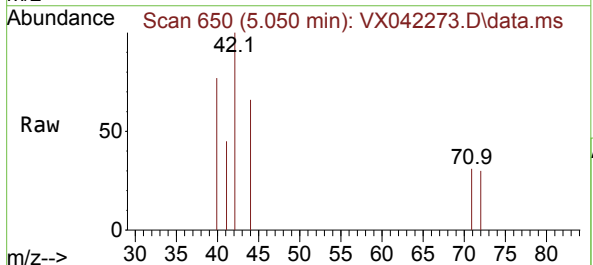




#32
1,1,1-Trichloroethane
Concen: 0.235 ug/l
RT: 5.385 min Scan# 704
Delta R.T. 0.006 min
Lab File: VX042273.D
Acq: 10 Jul 2024 17:30




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 97 Resp: 538
Ion Ratio Lower Upper
97 100
99 0.0 51.1 76.7#
61 24.0 36.4 54.6#



#33
1,2-Dichloroethane-d4
Concen: 63.180 ug/l
RT: 5.952 min Scan# 798
Delta R.T. -0.006 min
Lab File: VX042273.D
Acq: 10 Jul 2024 17:30

Tgt Ion: 65 Resp: 118443
Ion Ratio Lower Upper
65 100
67 53.6 0.0 100.2




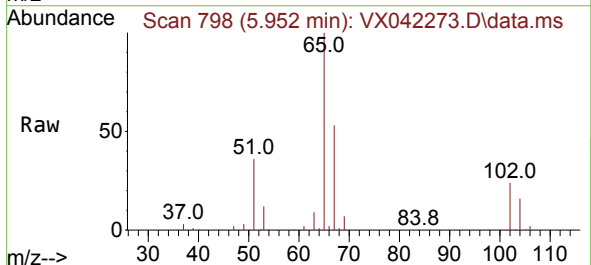


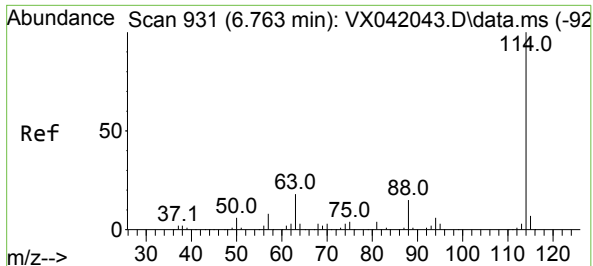

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. 0.000 min
Lab File: VX042273.D
Acq: 10 Jul 2024 17:30




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:114 Resp: 268872
Ion Ratio Lower Upper
114 100
63 17.0 0.0 45.0
88 14.9 0.0 36.6

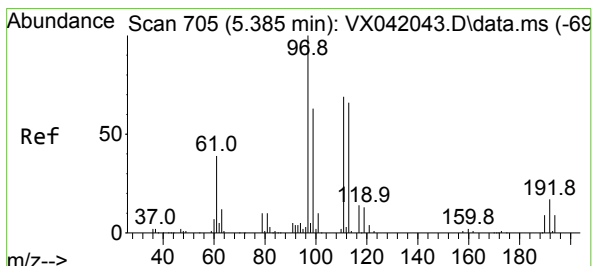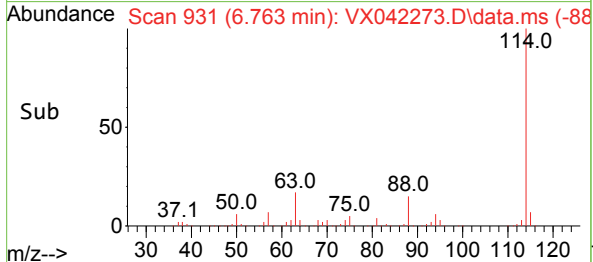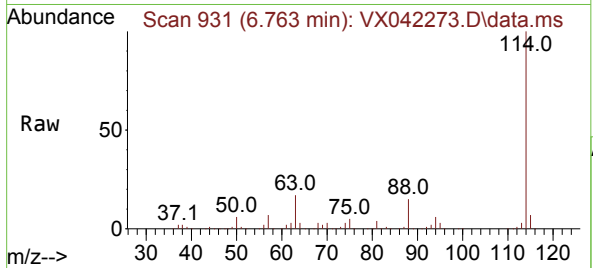

#35
Dibromofluoromethane
Concen: 58.977 ug/l
RT: 5.385 min Scan# 705
Delta R.T. -0.006 min
Lab File: VX042273.D
Acq: 10 Jul 2024 17:30


Tgt Ion:113 Resp: 112516
Ion Ratio Lower Upper
113 100
111 101.2 82.9 124.3
192 25.7 13.3 19.9#

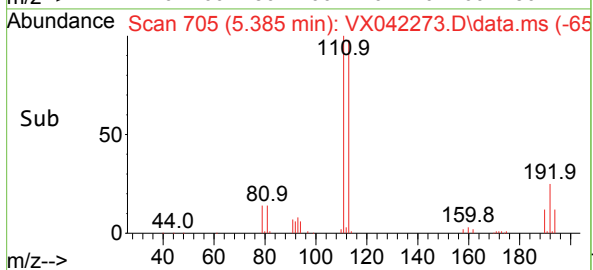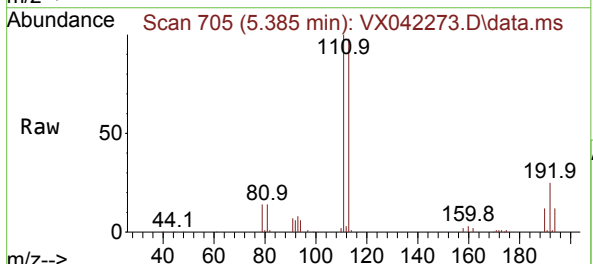






#36
1,1-Dichloropropene
Concen: 4.523 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.140 min
Lab File: VX042273.D
Acq: 10 Jul 2024 17:30

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion: 75 Resp: 9164
Ion Ratio Lower Upper
75 100
110 9.0 17.0 50.9#
77 0.0 24.7 37.1#



#37
Ethyl Acetate
Concen: 0.206 ug/l
RT: 4.739 min Scan# 599
Delta R.T. 0.012 min
Lab File: VX042273.D
Acq: 10 Jul 2024 17:30


Tgt Ion: 43 Resp: 543
Ion Ratio Lower Upper
43 100
61 13.4 10.6 16.0
70 12.9 8.3 12.5#

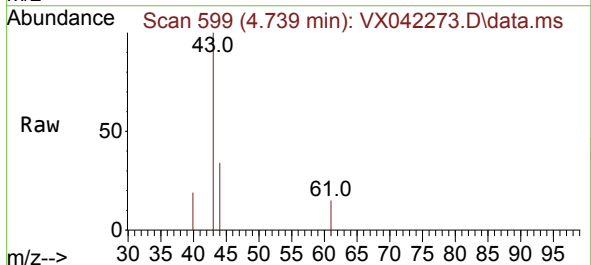






#38
Carbon Tetrachloride
Concen: 6.042 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.128 min
Lab File: VX042273.D
Acq: 10 Jul 2024 17:30

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion:117 Resp: 13525
Ion Ratio Lower Upper
117 100
119 4.4 78.2 117.2#
121 0.0 24.4 36.6#



#40
Benzene
Concen: 0.937 ug/l
RT: 6.044 min Scan# 813
Delta R.T. 0.006 min
Lab File: VX042273.D
Acq: 10 Jul 2024 17:30


Tgt Ion: 78 Resp: 6399
Ion Ratio Lower Upper
78 100
77 21.8 19.3 28.9








#43
Isopropyl Acetate
Concen: 18.511 ug/l
RT: 6.348 min Scan# 80
Delta R.T. 0.000 min
Lab File: VX042273.D
Acq: 10 Jul 2024 17:30


Instrument :
MSVOA_X
ClientSampleId :





Tgt Ion: 43 Resp: 74986
Ion Ratio Lower Upper
43 100
61 22.0 15.2 22.8
87 15.4 9.8 14.6#

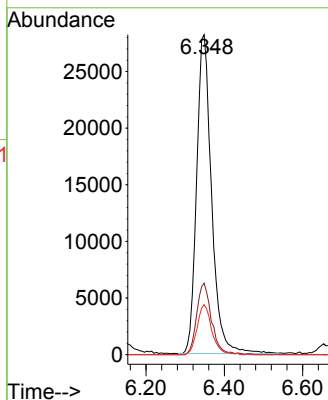


#48
Methyl methacrylate
Concen: 1.834 ug/l
RT: 7.616 min Scan# 1071
Delta R.T. -0.079 min
Lab File: VX042273.D
Acq: 10 Jul 2024 17:30



Tgt Ion: 41 Resp: 3546
Ion Ratio Lower Upper
41 100
69 0.0 59.2 88.8#
39 0.0 47.7 71.5#



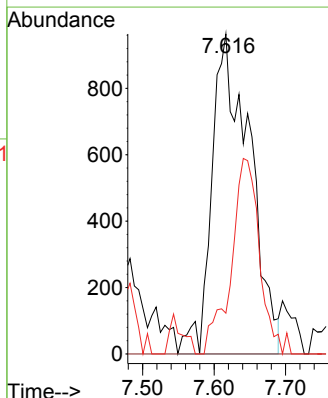





#50
Toluene-d8
Concen: 51.797 ug/l
RT: 8.647 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX042273.D
Acq: 10 Jul 2024 17:30




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 98 Resp: 347155
Ion Ratio Lower Upper
98 100
100 67.0 53.1 79.7



#51
4-Methyl-2-Pentanone
Concen: 16.069 ug/l
RT: 8.549 min Scan# 1224
Delta R.T. -0.030 min
Lab File: VX042273.D
Acq: 10 Jul 2024 17:30

Tgt Ion: 43 Resp: 44838
Ion Ratio Lower Upper
43 100
58 7.0 30.4 45.6#









#52
Toluene
Concen: 4.692 ug/l
RT: 8.720 min Scan# 1252
Delta R.T. 0.000 min
Lab File: VX042273.D
Acq: 10 Jul 2024 17:30




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 92 Resp: 20415
Ion Ratio Lower Upper
92 100
91 171.2 134.2 201.2



#53
t-1,3-Dichloropropene
Concen: 1.000 ug/l
RT: 8.958 min Scan# 1291
Delta R.T. -0.024 min
Lab File: VX042273.D
Acq: 10 Jul 2024 17:30

Tgt Ion: 75 Resp: 256
Ion Ratio Lower Upper
75 100
77 0.0 25.7 38.5#









#54
cis-1,3-Dichloropropene
Concen: 9.146 ug/l
RT: 8.549 min Scan# 1194
Delta R.T. 0.183 min
Lab File: VX042273.D
Acq: 10 Jul 2024 17:30




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion	Ratio	Lower	Upper
75	100		
77	0.0	25.3	37.9#
39	23.9	46.7	70.1#



#57
1,3-Dichloropropane
Concen: 0.682 ug/l
RT: 9.482 min Scan# 1377
Delta R.T. 0.171 min
Lab File: VX042273.D
Acq: 10 Jul 2024 17:30

Tgt Ion	Ratio	Lower	Upper
76	100		
78	0.0	26.1	39.1#









#59
2-Hexanone
Concen: 11.526 ug/l
RT: 9.482 min Scan# 1377
Delta R.T. 0.049 min
Lab File: VX042273.D
Acq: 10 Jul 2024 17:30




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 43 Resp: 24633
Ion Ratio Lower Upper
43 100
58 23.3 26.2 78.5#

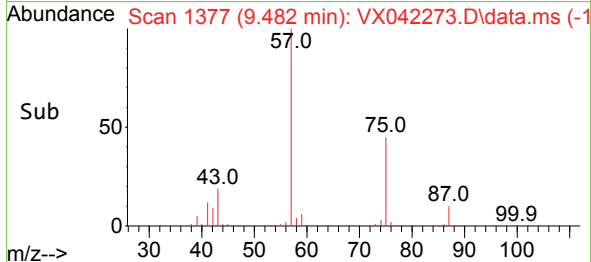

#62
4-Bromofluorobenzene
Concen: 53.145 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX042273.D
Acq: 10 Jul 2024 17:30


Tgt Ion: 95 Resp: 131299
Ion Ratio Lower Upper
95 100
174 99.1 0.0 135.6
176 95.9 0.0 131.0

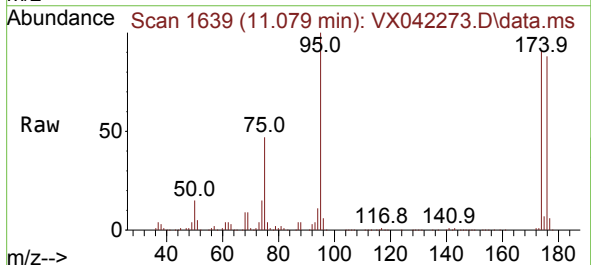






#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX042273.D
Acq: 10 Jul 2024 17:30

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion:117 Resp: 243879
Ion Ratio Lower Upper
117 100
82 49.9 46.2 69.4
119 32.6 25.5 38.3

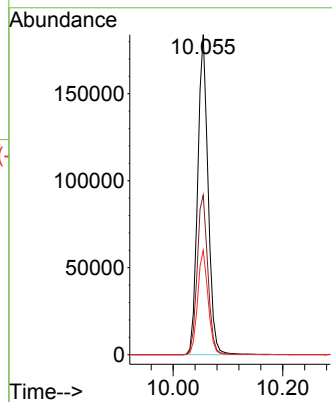

#67
Ethyl Benzene
Concen: 0.444 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. 0.000 min
Lab File: VX042273.D
Acq: 10 Jul 2024 17:30

Tgt Ion: 91 Resp: 3533
Ion Ratio Lower Upper
91 100
106 34.7 24.9 37.3




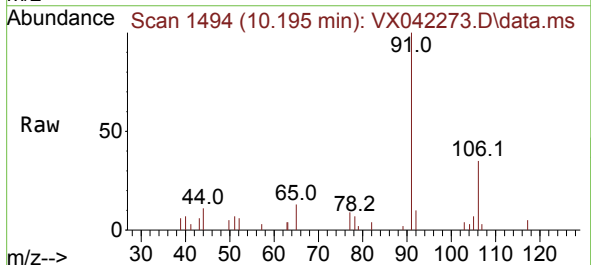




#68
m/p-Xylenes
Concen: 1.451 ug/l
RT: 10.299 min Scan# 1511
Delta R.T. 0.000 min
Lab File: VX042273.D
Acq: 10 Jul 2024 17:30




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:106 Resp: 4656
Ion Ratio Lower Upper
106 100
91 201.8 165.5 248.3

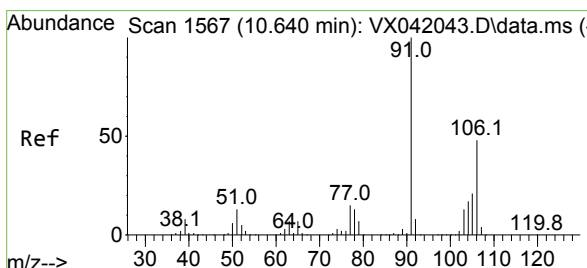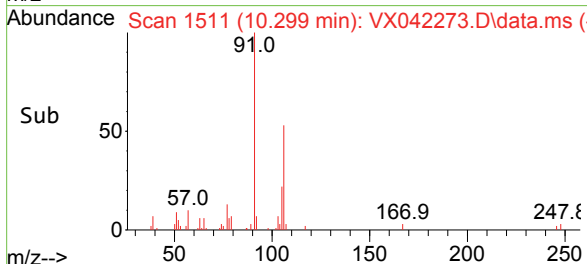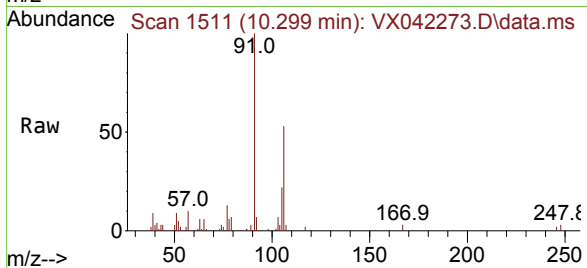

#69
o-Xylene
Concen: 0.794 ug/l
RT: 10.646 min Scan# 1568
Delta R.T. 0.006 min
Lab File: VX042273.D
Acq: 10 Jul 2024 17:30

Tgt Ion:106 Resp: 2522
Ion Ratio Lower Upper
106 100
91 208.6 108.9 326.8

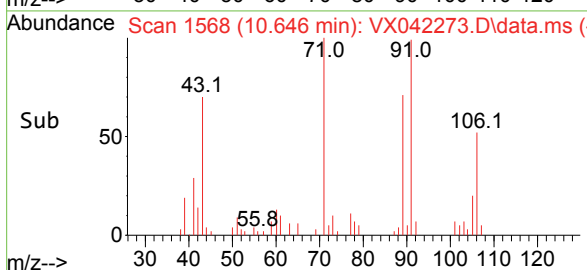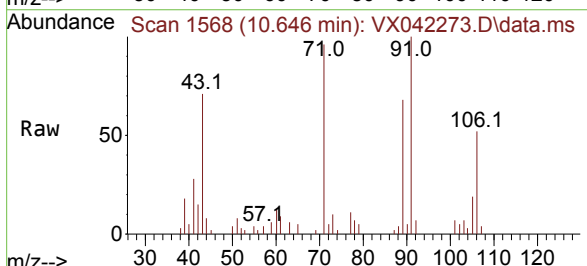



#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.024 min Scan# 11

Delta R.T. 0.000 min

Lab File: VX042273.D

Acq: 10 Jul 2024 17:30

Instrument :

MSVOA_X

ClientSampleId :





Tgt Ion:152 Resp: 119788

Ion Ratio Lower Upper

152 100

115 53.2 43.3 129.9

150 154.3 0.0 345.0

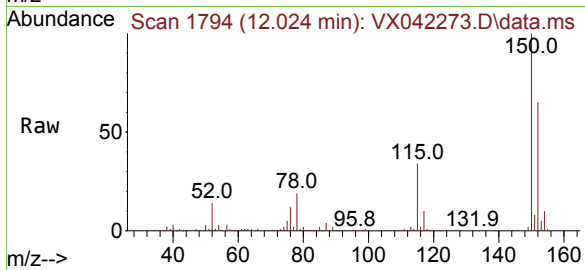

#76

1,2,3-Trichloropropane

Concen: 27.481 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. -0.158 min

Lab File: VX042273.D




Acq: 10 Jul 2024 17:30


Tgt Ion: 75 Resp: 59760

Ion Ratio Lower Upper

75 100

77 1.3 19.1 57.5#




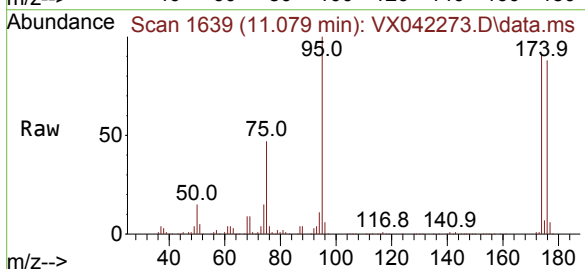




#81
 trans-1,4-Dichloro-2-butene
 Concen: 78.042 ug/l
 RT: 11.079 min Scan# 11
 Delta R.T. 0.061 min
 Lab File: VX042273.D
 Acq: 10 Jul 2024 17:30




Instrument :
 MSVOA_X
 ClientSampleId :


Tgt Ion: 75 Resp: 59760
 Ion Ratio Lower Upper
 75 100
 53 0.0 90.5 135.7#
 89 0.0 36.9 55.3#

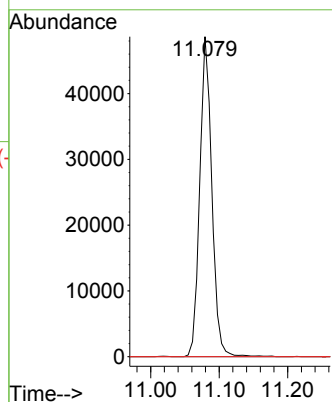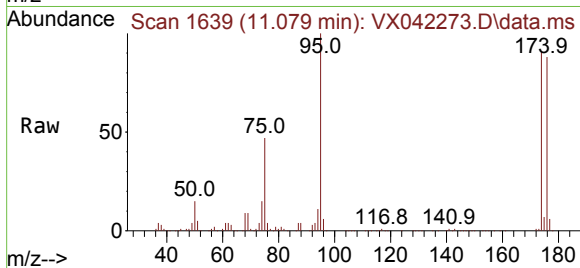

#84
 1,2,4-Trimethylbenzene
 Concen: 0.447 ug/l
 RT: 11.756 min Scan# 1750
 Delta R.T. 0.006 min
 Lab File: VX042273.D
 Acq: 10 Jul 2024 17:30

Tgt Ion: 105 Resp: 2718
 Ion Ratio Lower Upper
 105 100
 120 49.0 21.2 63.6




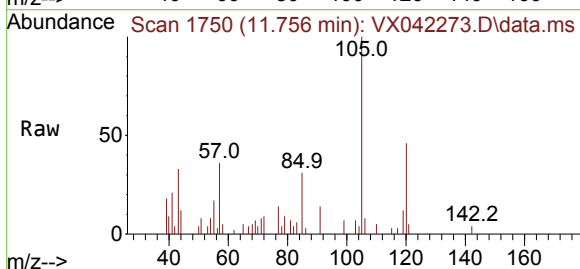


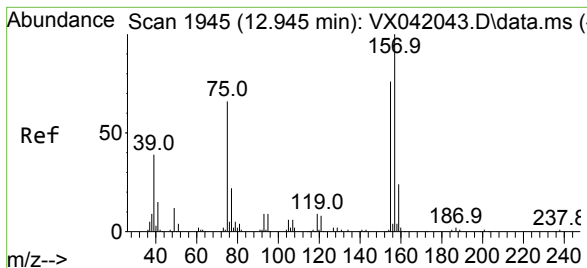

#92
1,2-Dibromo-3-Chloropropane
Concen: 0.745 ug/l
RT: 12.957 min Scan# 1947
Delta R.T. 0.012 min
Lab File: VX042273.D
Acq: 10 Jul 2024 17:30

Instrument :
MSVOA_X
ClientSampleId :

Tgt Ion: 75 Resp: 400
Ion Ratio Lower Upper
75 100
155 0.0 36.1 108.5#
157 0.0 44.9 134.7#

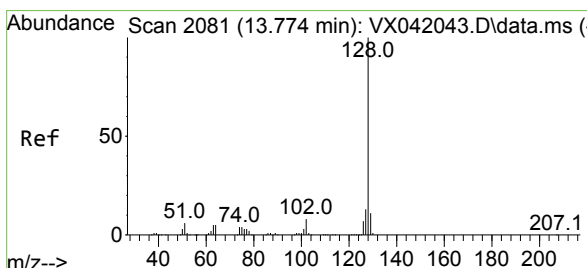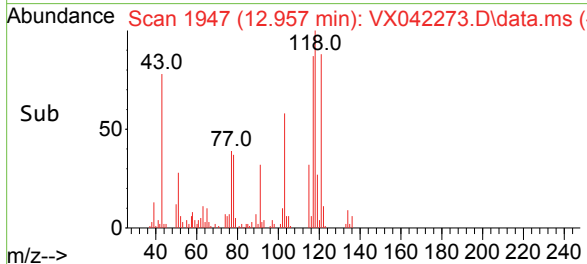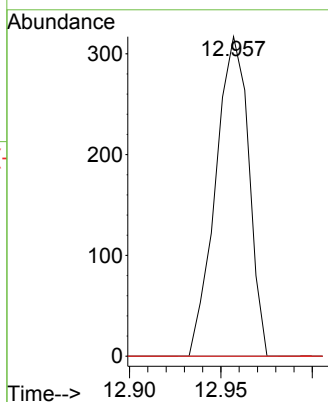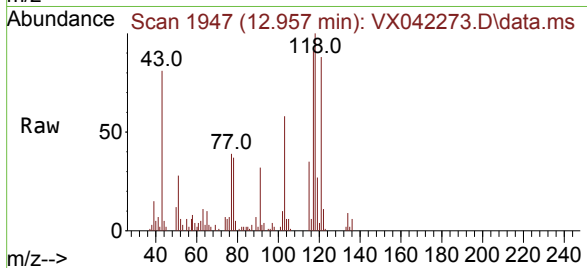

#95
Naphthalene
Concen: 1.853 ug/l
RT: 13.780 min Scan# 2082
Delta R.T. 0.006 min
Lab File: VX042273.D
Acq: 10 Jul 2024 17:30

Tgt Ion: 128 Resp: 9639
Ion Ratio Lower Upper
128 100
127 13.3 10.3 15.5
129 10.2 8.8 13.2

