

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071024\
 Data File : VX042278.D
 Acq On : 10 Jul 2024 19:27
 Operator : JC/MD
 Sample : P3183-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Jul 11 01:03:31 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061824W.M
 Quant Title : SW846 8260
 QLast Update : Fri Jun 21 23:51:58 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.556	168	137910	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	6.763	114	223069	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	196702	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	81755	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	85443	53.728	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	= 107.460%	
35) Dibromofluoromethane	5.385	113	81430	51.447	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 102.900%	
50) Toluene-d8	8.647	98	236118	42.464	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	= 84.920%#	
62) 4-Bromofluorobenzene	11.079	95	82409	40.205	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	= 80.420%#	
Target Compounds						
					Qvalue	
6) Chloroethane	1.642	64	152	Below Cal	#	43
11) Tert butyl alcohol	2.983	59	3285	10.884	ug/l	98
14) Allyl chloride	2.654	41	390	0.207	ug/l	# 24
16) Acetone	2.386	43	74461	106.633	ug/l	91
18) Methyl Acetate	2.709	43	3445	1.808	ug/l	95
20) Methylene Chloride	2.788	84	6670	4.362	ug/l	86
25) 2-Butanone	4.581	43	11783	10.846	ug/l	91
31) Cyclohexane	5.544	56	1755	0.944	ug/l	# 1
36) 1,1-Dichloropropene	5.550	75	7933	4.720	ug/l	# 51
37) Ethyl Acetate	4.581	43	11783	5.382	ug/l	# 69
38) Carbon Tetrachloride	5.556	117	11580	6.236	ug/l	# 14
40) Benzene	6.038	78	17928	3.163	ug/l	99
43) Isopropyl Acetate	6.355	43	9819	2.922	ug/l	# 95
48) Methyl methacrylate	7.610	41	1522	0.949	ug/l	# 20
51) 4-Methyl-2-Pentanone	8.549	43	27030	11.676	ug/l	# 37
52) Toluene	8.720	92	2245	0.622	ug/l	94
54) cis-1,3-Dichloropropene	8.549	75	11110	5.442	ug/l	# 49
57) 1,3-Dichloropropane	9.488	76	608	0.250	ug/l	# 42
59) 2-Hexanone	9.482	43	6412	3.616	ug/l	# 62
67) Ethyl Benzene	10.195	91	5992	0.935	ug/l	91
68) m/p-Xylenes	10.305	106	2204	0.852	ug/l	94
69) o-Xylene	10.640	106	1819	0.710	ug/l	99
71) Bromoform	11.067	173	55	0.916	ug/l	# 29
74) N-amyl acetate	10.884	43	2269	1.028	ug/l	# 69
76) 1,2,3-Trichloropropane	11.079	75	37188	25.056	ug/l	# 39
78) n-propylbenzene	11.305	91	1169	0.217	ug/l	98
79) 2-Chlorotoluene	11.305	91	1169	0.336	ug/l	# 42
81) trans-1,4-Dichloro-2-b...	11.079	75	37188	71.157	ug/l	# 5
82) 4-Chlorotoluene	11.305	91	1169	0.304	ug/l	# 46
90) Hexachloroethane	12.701	117	158	0.207	ug/l	# 17
95) Naphthalene	13.786	128	819	0.886	ug/l	# 77


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071024\
Data File : VX042278.D
Acq On : 10 Jul 2024 19:27
Operator : JC/MD
Sample : P3183-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :


Quant Time: Jul 11 01:03:31 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061824W.M
Quant Title : SW846 8260
QLast Update : Fri Jun 21 23:51:58 2024
Response via : Initial Calibration

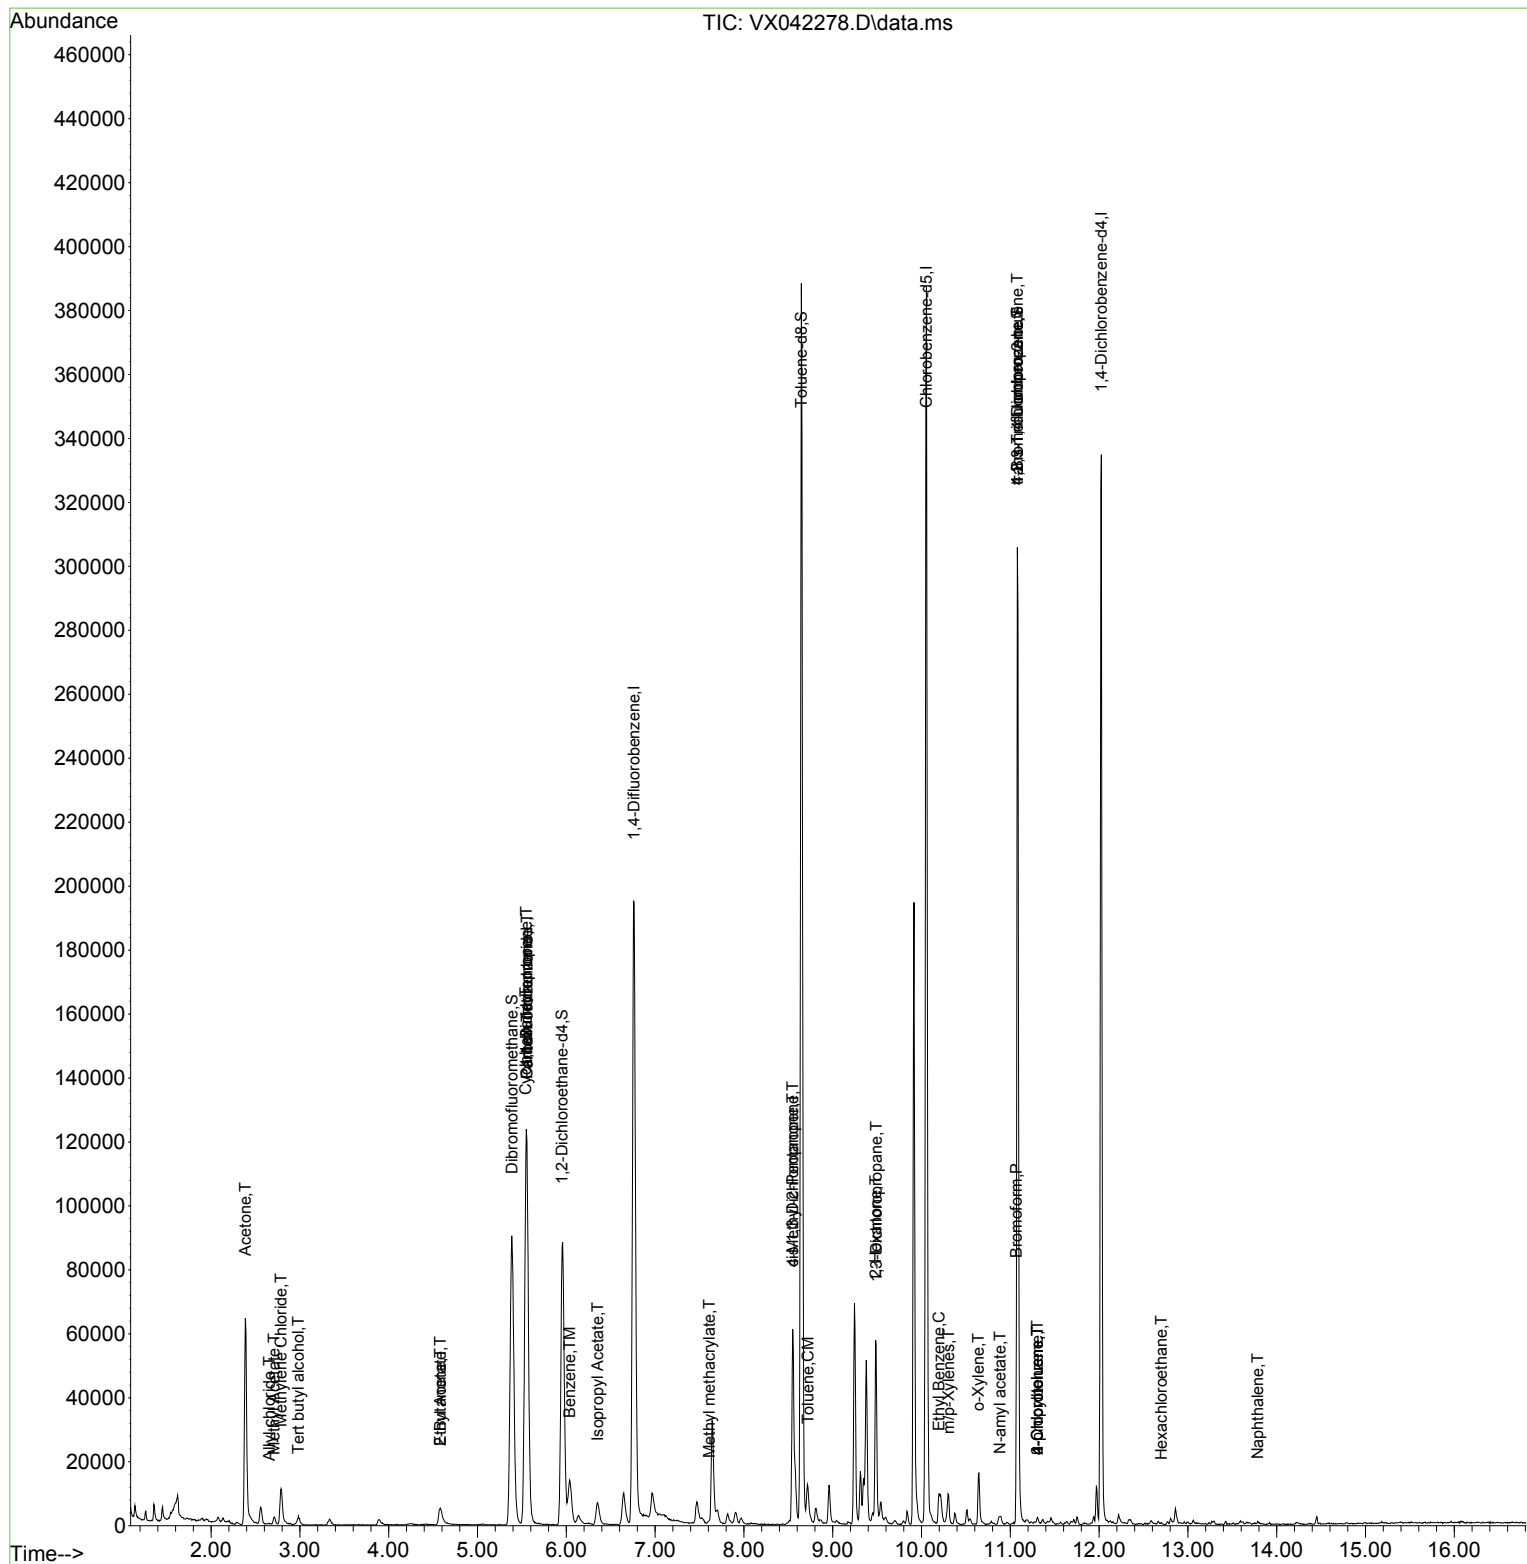






#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. 0.006 min
Lab File: VX042278.D
Acq: 10 Jul 2024 19:27

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion:168 Resp: 137910
Ion Ratio Lower Upper
168 100
99 46.3 56.6 85.0#



#6
Chloroethane
Concen: Below Cal
RT: 1.642 min Scan# 91
Delta R.T. -0.018 min
Lab File: VX042278.D
Acq: 10 Jul 2024 19:27


Tgt Ion: 64 Resp: 152
Ion Ratio Lower Upper
64 100
66 0.0 25.1 37.7#








#11
Tert butyl alcohol
Concen: 10.884 ug/l
RT: 2.983 min Scan# 311
Delta R.T. -0.024 min
Lab File: VX042278.D
Acq: 10 Jul 2024 19:27

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion: 59 Resp: 3285
Ion Ratio Lower Upper
59 100
57 8.2 6.0 9.0



#14
Allyl chloride
Concen: 0.207 ug/l
RT: 2.654 min Scan# 257
Delta R.T. -0.006 min
Lab File: VX042278.D
Acq: 10 Jul 2024 19:27

Tgt Ion: 41 Resp: 390
Ion Ratio Lower Upper
41 100
39 0.0 55.8 83.6#
76 0.0 24.3 36.5#

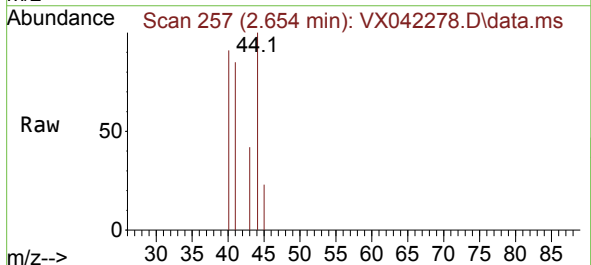



#16

Acetone

Concen: 106.633 ug/l

RT: 2.386 min Scan# 214

Delta R.T. -0.012 min

Lab File: VX042278.D

Acq: 10 Jul 2024 19:27

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 43 Resp: 74461

Ion Ratio Lower Upper

43 100

58 32.2 21.9 32.9

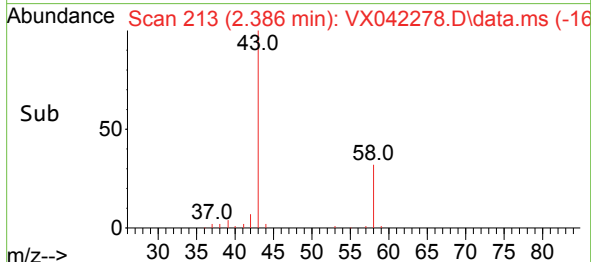

#18

Methyl Acetate

Concen: 1.808 ug/l

RT: 2.709 min Scan# 266

Delta R.T. 0.000 min

Lab File: VX042278.D




Acq: 10 Jul 2024 19:27


Tgt Ion: 43 Resp: 3445

Ion Ratio Lower Upper

43 100


74 19.9 17.8 26.8







#20
Methylene Chloride
Concen: 4.362 ug/l
RT: 2.788 min Scan# 21
Delta R.T. 0.006 min
Lab File: VX042278.D
Acq: 10 Jul 2024 19:27

Instrument :
MSVOA_X
ClientSampleId :



Tgt Ion: 84 Resp: 6670




Ion	Ratio	Lower	Upper
84	100		
49	110.9	103.6	155.4
51	34.1	33.8	50.6
86	70.4	49.4	74.0

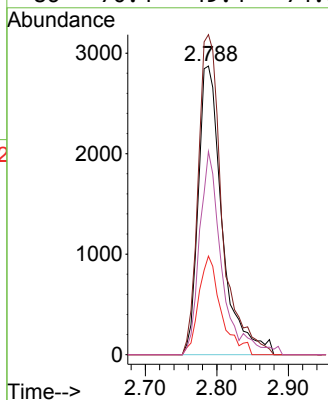


#25
2-Butanone
Concen: 10.846 ug/l
RT: 4.581 min Scan# 573
Delta R.T. 0.006 min
Lab File: VX042278.D
Acq: 10 Jul 2024 19:27

Tgt Ion: 43 Resp: 11783


Ion	Ratio	Lower	Upper
43	100		
72	28.6	19.4	29.2

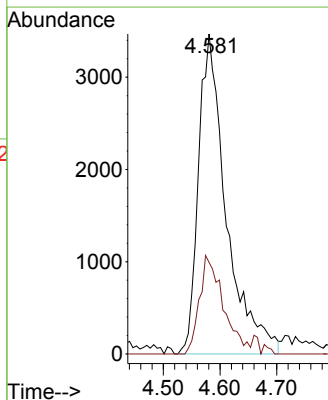



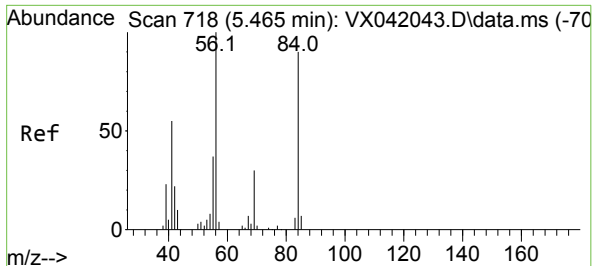


#31
Cyclohexane
Concen: 0.944 ug/l
RT: 5.544 min Scan# 718
Delta R.T. 0.079 min
Lab File: VX042278.D
Acq: 10 Jul 2024 19:27

Instrument :
MSVOA_X
ClientSampleId :



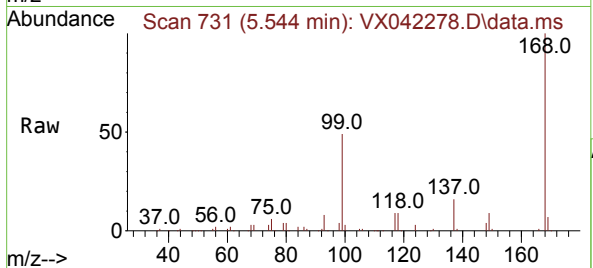



Tgt Ion: 56 Resp: 1755
Ion Ratio Lower Upper
56 100
69 187.5 23.4 35.2#
84 149.0 65.9 98.9#

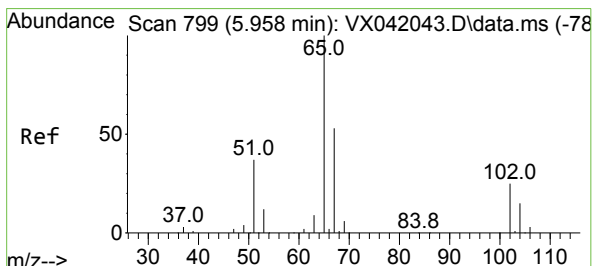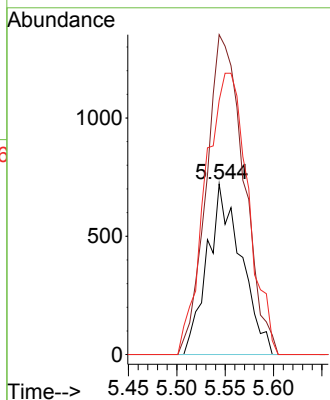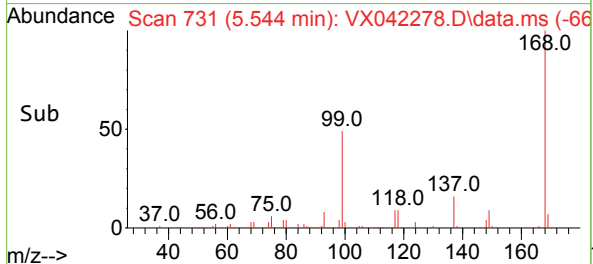

#33
1,2-Dichloroethane-d4
Concen: 53.728 ug/l
RT: 5.952 min Scan# 798
Delta R.T. -0.006 min
Lab File: VX042278.D
Acq: 10 Jul 2024 19:27

Tgt Ion: 65 Resp: 85443
Ion Ratio Lower Upper
65 100
67 53.1 0.0 100.2


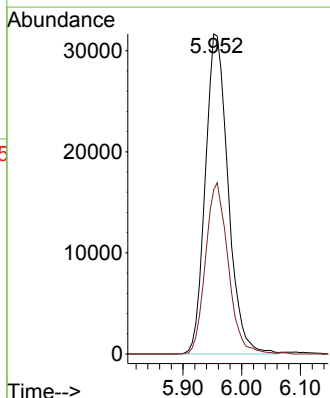
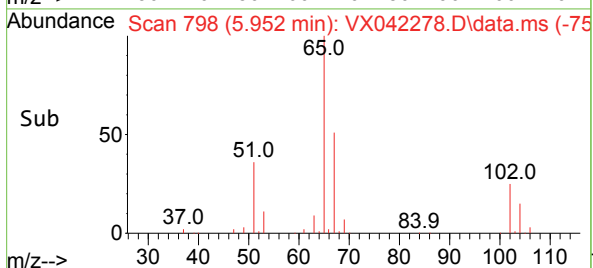
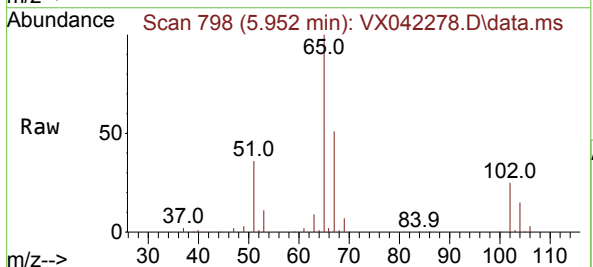




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. 0.000 min
Lab File: VX042278.D
Acq: 10 Jul 2024 19:27




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:114 Resp: 223069
Ion Ratio Lower Upper
114 100
63 17.4 0.0 45.0
88 14.8 0.0 36.6

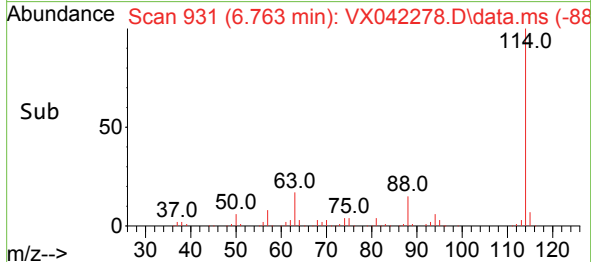

#35
Dibromofluoromethane
Concen: 51.447 ug/l
RT: 5.385 min Scan# 705
Delta R.T. -0.006 min
Lab File: VX042278.D
Acq: 10 Jul 2024 19:27


Tgt Ion:113 Resp: 81430
Ion Ratio Lower Upper
113 100
111 101.9 82.9 124.3
192 26.2 13.3 19.9#

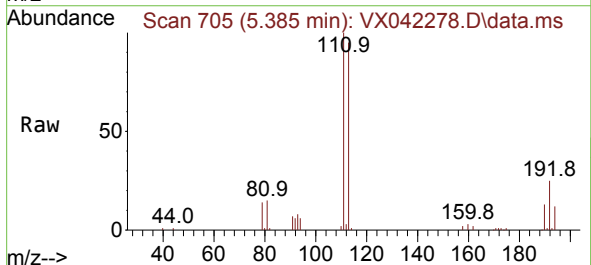






#36
1,1-Dichloropropene
Concen: 4.720 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.140 min
Lab File: VX042278.D
Acq: 10 Jul 2024 19:27

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion: 75 Resp: 7933
Ion Ratio Lower Upper
75 100
110 9.3 17.0 50.9#
77 0.0 24.7 37.1#



#37
Ethyl Acetate
Concen: 5.382 ug/l
RT: 4.581 min Scan# 573
Delta R.T. -0.146 min
Lab File: VX042278.D
Acq: 10 Jul 2024 19:27


Tgt Ion: 43 Resp: 11783
Ion Ratio Lower Upper
43 100
61 0.0 10.6 16.0#
70 0.0 8.3 12.5#

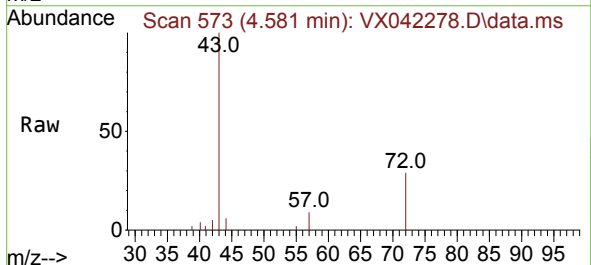






#38
Carbon Tetrachloride
Concen: 6.236 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.122 min
Lab File: VX042278.D
Acq: 10 Jul 2024 19:27

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion:117 Resp: 11580
Ion Ratio Lower Upper
117 100
119 3.4 78.2 117.2#
121 0.0 24.4 36.6#

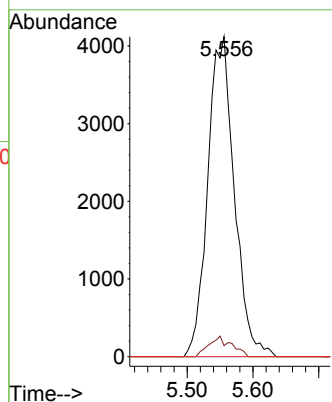

#40
Benzene
Concen: 3.163 ug/l
RT: 6.038 min Scan# 812
Delta R.T. 0.000 min
Lab File: VX042278.D
Acq: 10 Jul 2024 19:27


Tgt Ion: 78 Resp: 17928
Ion Ratio Lower Upper
78 100
77 23.4 19.3 28.9








#43
Isopropyl Acetate
Concen: 2.922 ug/l
RT: 6.355 min Scan# 864
Delta R.T. 0.006 min
Lab File: VX042278.D
Acq: 10 Jul 2024 19:27

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion: 43 Resp: 9819
Ion Ratio Lower Upper
43 100
61 20.5 15.2 22.8
87 15.4 9.8 14.6#

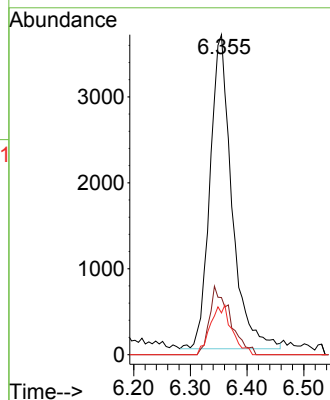

#48
Methyl methacrylate
Concen: 0.949 ug/l
RT: 7.610 min Scan# 1070
Delta R.T. -0.085 min
Lab File: VX042278.D
Acq: 10 Jul 2024 19:27

Tgt Ion: 41 Resp: 1522
Ion Ratio Lower Upper
41 100
69 0.0 59.2 88.8#
39 6.6 47.7 71.5#



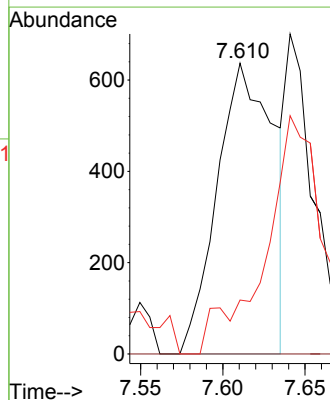





#50
Toluene-d8
Concen: 42.464 ug/l
RT: 8.647 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX042278.D
Acq: 10 Jul 2024 19:27




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 98 Resp: 236118
Ion Ratio Lower Upper
98 100
100 66.5 53.1 79.7

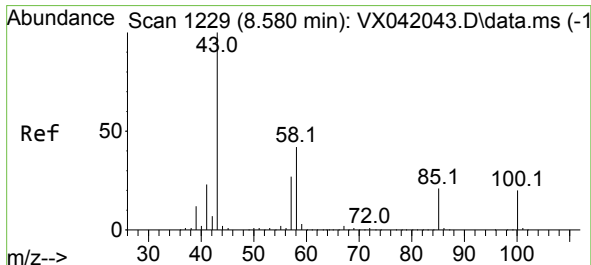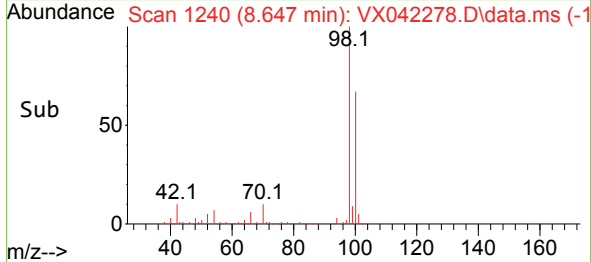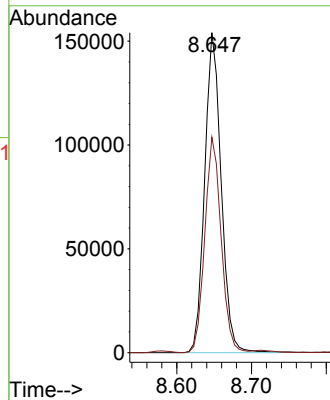

#51
4-Methyl-2-Pentanone
Concen: 11.676 ug/l
RT: 8.549 min Scan# 1224
Delta R.T. -0.030 min
Lab File: VX042278.D
Acq: 10 Jul 2024 19:27

Tgt Ion: 43 Resp: 27030
Ion Ratio Lower Upper
43 100
58 0.0 30.4 45.6#



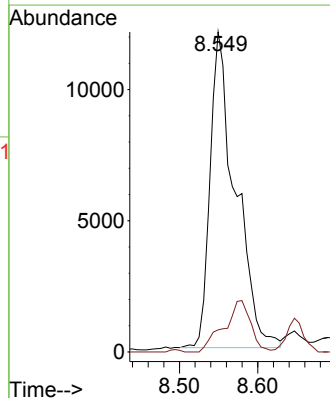
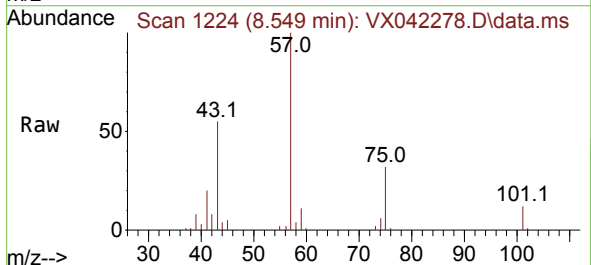




#52
Toluene
Concen: 0.622 ug/l
RT: 8.720 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX042278.D
Acq: 10 Jul 2024 19:27




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 92 Resp: 2245
Ion Ratio Lower Upper
92 100
91 159.2 134.2 201.2

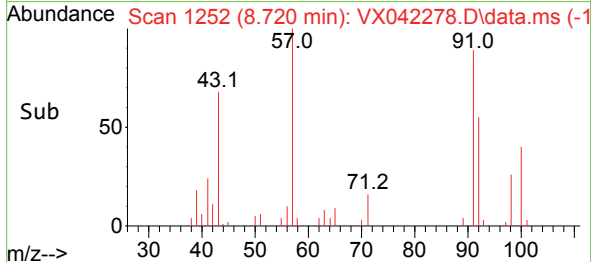

#54
cis-1,3-Dichloropropene
Concen: 5.442 ug/l
RT: 8.549 min Scan# 1224
Delta R.T. 0.183 min
Lab File: VX042278.D
Acq: 10 Jul 2024 19:27

Tgt Ion: 75 Resp: 11110
Ion Ratio Lower Upper
75 100
77 0.0 25.3 37.9#
39 23.2 46.7 70.1#





#57

1,3-Dichloropropane

Concen: 0.250 ug/l

RT: 9.488 min Scan# 1378

Delta R.T. 0.177 min

Lab File: VX042278.D

Acq: 10 Jul 2024 19:27

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 76 Resp: 608

Ion Ratio Lower Upper

76 100

78 0.0 26.1 39.1#

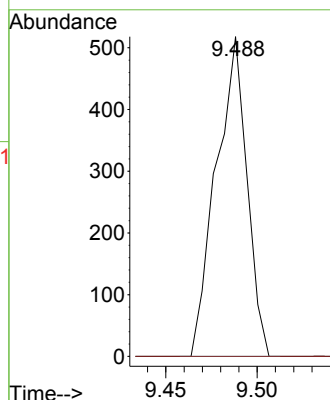

#59

2-Hexanone

Concen: 3.616 ug/l

RT: 9.482 min Scan# 1377

Delta R.T. 0.049 min

Lab File: VX042278.D




Acq: 10 Jul 2024 19:27


Tgt Ion: 43 Resp: 6412

Ion Ratio Lower Upper

43 100


58 25.4 26.2 78.5#

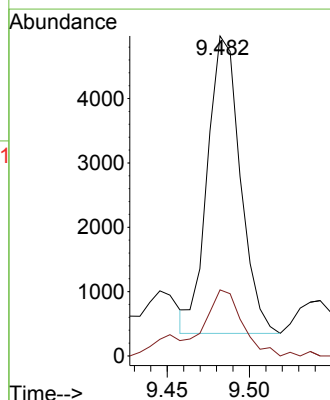






#62
4-Bromofluorobenzene
Concen: 40.205 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX042278.D
Acq: 10 Jul 2024 19:27


Instrument :
MSVOA_X
ClientSampleId :





Tgt Ion: 95 Resp: 82409
Ion Ratio Lower Upper
95 100
174 97.3 0.0 135.6
176 96.6 0.0 131.0

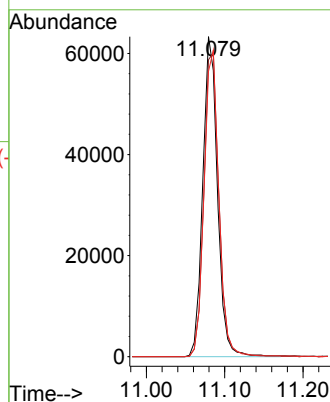


#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX042278.D
Acq: 10 Jul 2024 19:27



Tgt Ion: 117 Resp: 196702
Ion Ratio Lower Upper
117 100
82 48.7 46.2 69.4
119 32.2 25.5 38.3



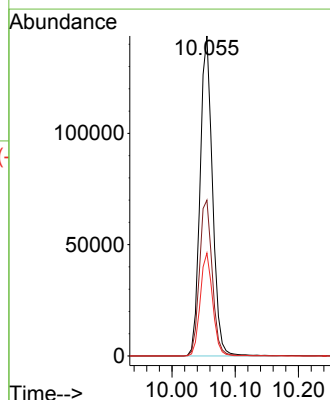





#67
Ethyl Benzene
Concen: 0.935 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. 0.000 min
Lab File: VX042278.D
Acq: 10 Jul 2024 19:27




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 91 Resp: 5992
Ion Ratio Lower Upper
91 100
106 35.9 24.9 37.3



#68
m/p-Xylenes
Concen: 0.852 ug/l
RT: 10.305 min Scan# 1512
Delta R.T. 0.006 min
Lab File: VX042278.D
Acq: 10 Jul 2024 19:27

Tgt Ion: 106 Resp: 2204
Ion Ratio Lower Upper
106 100
91 216.0 165.5 248.3

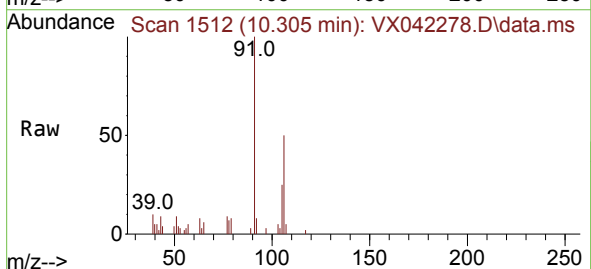



#69

o-Xylene

Concen: 0.710 ug/l

RT: 10.640 min Scan# 11

Delta R.T. 0.000 min

Lab File: VX042278.D

Acq: 10 Jul 2024 19:27

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion:106 Resp: 1819

Ion Ratio Lower Upper

106 100

91 216.8 108.9 326.8



#71

Bromoform

Concen: 0.916 ug/l

RT: 11.067 min Scan# 1637

Delta R.T. 0.268 min

Lab File: VX042278.D

Acq: 10 Jul 2024 19:27




Tgt Ion:173 Resp: 55


Ion Ratio Lower Upper

173 100

175 0.0 24.1 72.4#

254 0.0 0.0 0.0

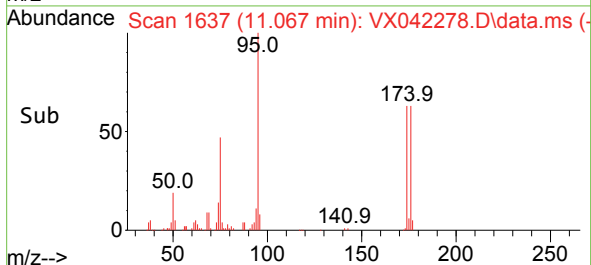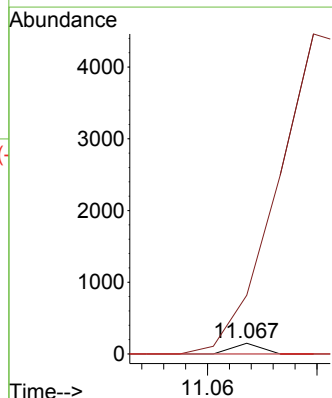



#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.024 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX042278.D

Acq: 10 Jul 2024 19:27

Instrument :

MSVOA_X

ClientSampleId :





Tgt Ion:152 Resp: 81755

Ion Ratio Lower Upper

152 100

115 53.1 43.3 129.9

150 158.3 0.0 345.0

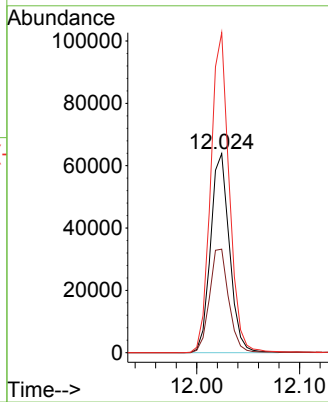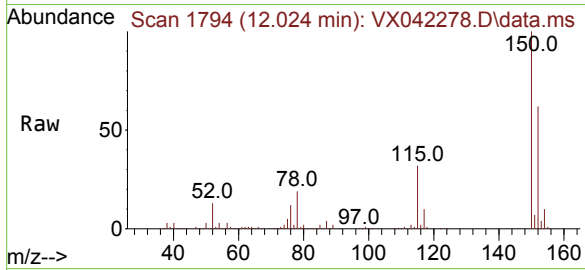

#74

N-ethyl acetate

Concen: 1.028 ug/l

RT: 10.884 min Scan# 1607

Delta R.T. 0.043 min

Lab File: VX042278.D

Acq: 10 Jul 2024 19:27

Tgt Ion: 43 Resp: 2269




Ion Ratio Lower Upper


43 100

70 22.6 32.9 49.3#

55 15.0 19.3 28.9#

61 0.0 18.8 28.2#

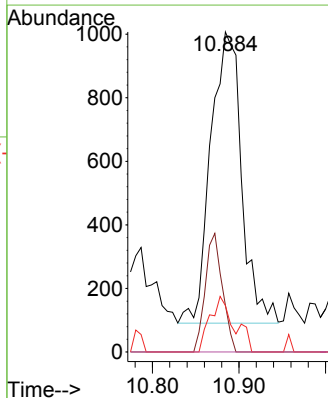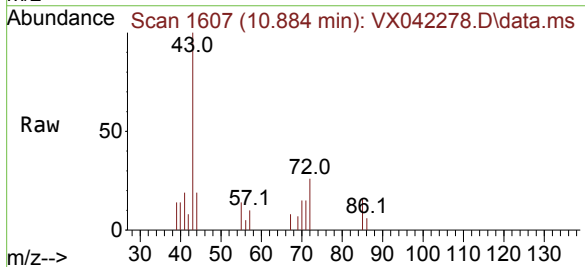



#76

1,2,3-Trichloropropane

Concen: 25.056 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. -0.158 min

Lab File: VX042278.D

Acq: 10 Jul 2024 19:27

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 75 Resp: 37188

Ion Ratio Lower Upper

75 100

77 1.2 19.1 57.5#



#78

n-propylbenzene

Concen: 0.217 ug/l

RT: 11.305 min Scan# 1676

Delta R.T. 0.000 min

Lab File: VX042278.D




Acq: 10 Jul 2024 19:27


Tgt Ion: 91 Resp: 1169

Ion Ratio Lower Upper

91 100


120 24.0 11.5 34.4








#79
2-Chlorotoluene
Concen: 0.336 ug/l
RT: 11.305 min Scan# 1686
Delta R.T. -0.061 min
Lab File: VX042278.D
Acq: 10 Jul 2024 19:27

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion: 91 Resp: 1169
Ion Ratio Lower Upper
91 100
126 0.0 16.3 48.8#

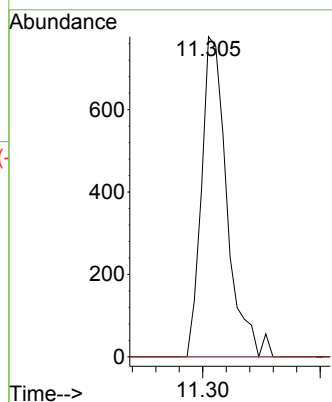

#81
trans-1,4-Dichloro-2-butene
Concen: 71.157 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.061 min
Lab File: VX042278.D
Acq: 10 Jul 2024 19:27

Tgt Ion: 75 Resp: 37188
Ion Ratio Lower Upper
75 100
53 0.0 90.5 135.7#
89 0.0 36.9 55.3#


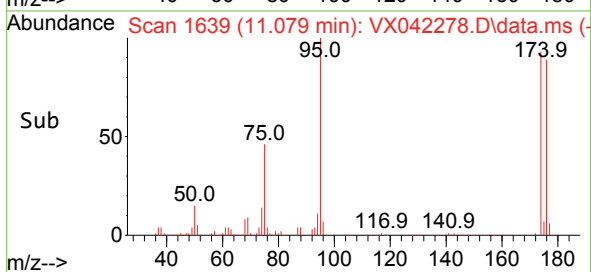
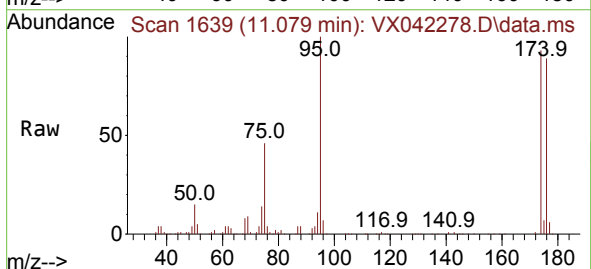
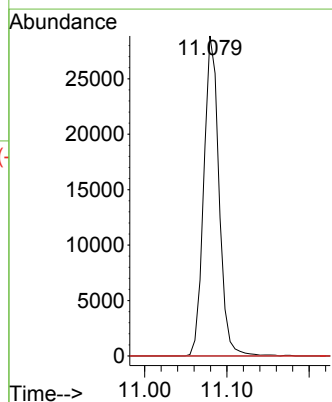




#82
4-Chlorotoluene
Concen: 0.304 ug/l
RT: 11.305 min Scan# 1169
Delta R.T. -0.152 min
Lab File: VX042278.D
Acq: 10 Jul 2024 19:27




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 91 Resp: 1169
Ion Ratio Lower Upper
91 100
126 0.0 14.2 42.6#



#90
Hexachloroethane
Concen: 0.207 ug/l
RT: 12.701 min Scan# 1905
Delta R.T. 0.165 min
Lab File: VX042278.D
Acq: 10 Jul 2024 19:27


Tgt Ion: 117 Resp: 158
Ion Ratio Lower Upper
117 100
201 0.0 32.9 98.6#

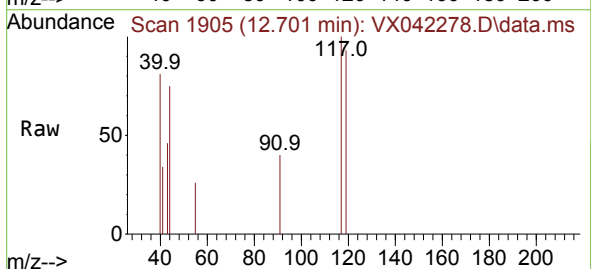



#95
 Naphthalene
 Concen: 0.886 ug/l
 RT: 13.786 min Scan# 2083
 Delta R.T. 0.012 min
 Lab File: VX042278.D
 Acq: 10 Jul 2024 19:27

Instrument :
 MSVOA_X
 ClientSampleId :

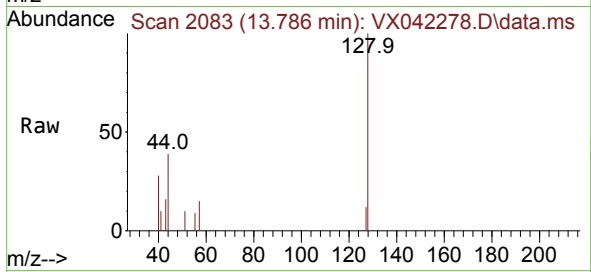

Tgt Ion:	128	Resp:	819
Ion	Ratio	Lower	Upper
128	100		
127	5.5	10.3	15.5#
129	0.0	8.8	13.2#

