

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071122\
 Data File : VX030006.D
 Acq On : 11 Jul 2022 18:41
 Operator : JC/MD
 Sample : N3648-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 CMR-TP2-0708

Quant Time: Jul 12 02:05:12 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062822W.M
 Quant Title : SW846 8260
 QLast Update : Wed Jun 29 05:54:51 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.562	168	189981	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.769	114	327417	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	286224	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	128912	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	103257	42.937	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	85.880%
35) Dibromofluoromethane	5.391	113	96972	47.392	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	94.780%
50) Toluene-d8	8.652	98	371094	48.343	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	96.680%
62) 4-Bromofluorobenzene	11.085	95	125348	46.195	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	92.400%


Target Compounds						Qvalue
6) Chloroethane	1.715	64	191	1.156	ug/l #	41
8) Diethyl Ether	2.129	74	251	0.205	ug/l #	30
11) Tert butyl alcohol	2.952	59	1521	2.418	ug/l #	83
13) Acrolein	2.239	56	777	Below Cal	#	79
16) Acetone	2.379	43	33736	28.674	ug/l	98
17) Carbon Disulfide	2.513	76	2071	0.426	ug/l #	94
18) Methyl Acetate	2.715	43	2914	0.803	ug/l	98
20) Methylene Chloride	2.788	84	23295	9.375	ug/l	86
25) 2-Butanone	4.562	43	10684	5.232	ug/l	100
36) 1,1-Dichloropropene	5.549	75	13772	5.061	ug/l #	48
37) Ethyl Acetate	4.720	43	37200	9.994	ug/l	98
38) Carbon Tetrachloride	5.555	117	17808	7.552	ug/l #	17
40) Benzene	6.043	78	16195	1.840	ug/l	93
43) Isopropyl Acetate	6.348	43	144950	25.861	ug/l	99
44) Trichloroethene	7.128	130	873	0.368	ug/l	67
48) Methyl methacrylate	7.805	41	119255	44.876	ug/l #	41
49) 1,4-Dioxane	7.659	88	29	0.461	ug/l #	1
51) 4-Methyl-2-Pentanone	8.555	43	102286	27.676	ug/l #	50
52) Toluene	8.726	92	9662	1.820	ug/l	97
53) t-1,3-Dichloropropene	8.957	75	937	0.323	ug/l #	42
54) cis-1,3-Dichloropropene	8.555	75	51308	15.631	ug/l #	58
57) 1,3-Dichloropropane	9.488	76	6570	1.765	ug/l #	43
59) 2-Hexanone	9.488	43	84990	29.632	ug/l #	51
68) m/p-Xylenes	10.305	106	2518	0.657	ug/l	95
69) o-Xylene	10.646	106	1297	0.334	ug/l	74
70) Styrene	10.658	104	10377	1.617	ug/l	90
74) N-amyl acetate	10.768	43	942	0.204	ug/l #	44
76) 1,2,3-Trichloropropane	11.085	75	59276	19.208	ug/l #	38
81) trans-1,4-Dichloro-2-b...	11.085	75	59276	61.001	ug/l #	12
84) 1,2,4-Trimethylbenzene	11.756	105	2253	0.290	ug/l	80
90) Hexachloroethane	12.615	117	434	0.345	ug/l #	16
95) Naphthalene	13.780	128	72976	7.009	ug/l	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071122\
Data File : VX030006.D
Acq On : 11 Jul 2022 18:41
Operator : JC/MD
Sample : N3648-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
CMR-TP2-0708

Quant Time: Jul 12 02:05:12 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062822W.M
Quant Title : SW846 8260
QLast Update : Wed Jun 29 05:54:51 2022
Response via : Initial Calibration




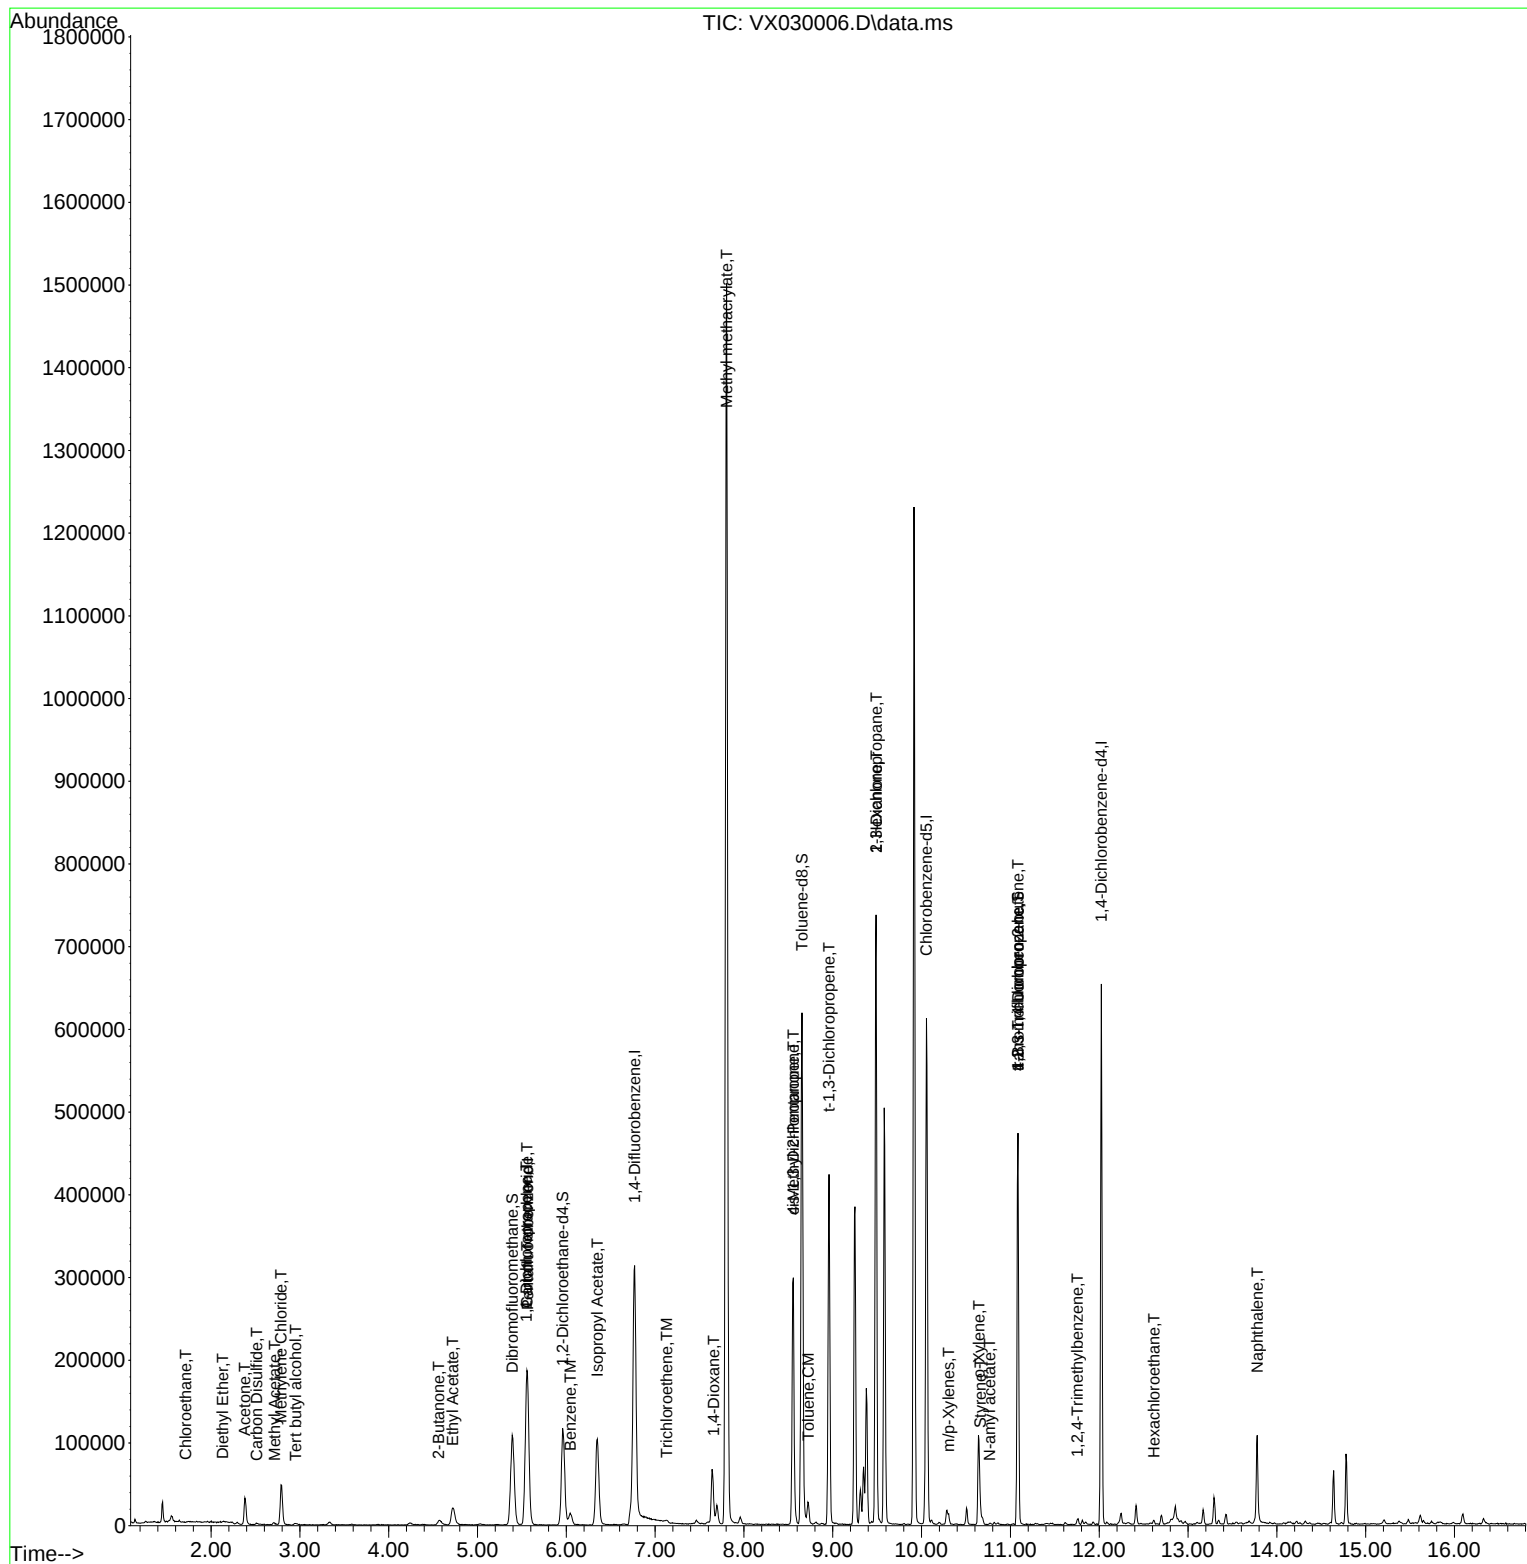




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.562 min Scan# 71
Delta R.T. 0.006 min
Lab File: VX030006.D
Acq: 11 Jul 2022 18:41




Instrument :
MSVOA_X
ClientSampleId :
CMR-TP2-0708


Tgt Ion:168 Resp: 189981
Ion Ratio Lower Upper
168 100
99 51.3 44.0 66.0



#6
Chloroethane
Concen: 1.156 ug/l
RT: 1.715 min Scan# 103
Delta R.T. 0.030 min
Lab File: VX030006.D
Acq: 11 Jul 2022 18:41

Tgt Ion: 64 Resp: 191
Ion Ratio Lower Upper
64 100
66 0.0 27.2 40.8#


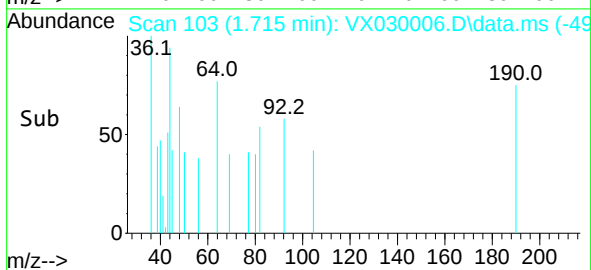

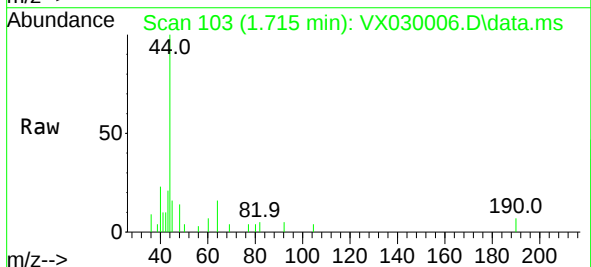


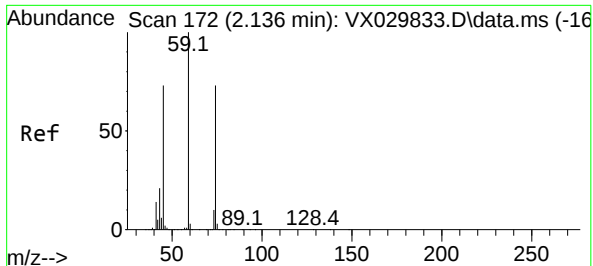

#8
Diethyl Ether
Concen: 0.205 ug/l
RT: 2.129 min Scan# 11
Delta R.T. -0.006 min
Lab File: VX030006.D
Acq: 11 Jul 2022 18:41




Instrument :
MSVOA_X
ClientSampleId :
CMR-TP2-0708


Tgt Ion: 74 Resp: 251
Ion Ratio Lower Upper
74 100
45 174.1 51.5 154.7#

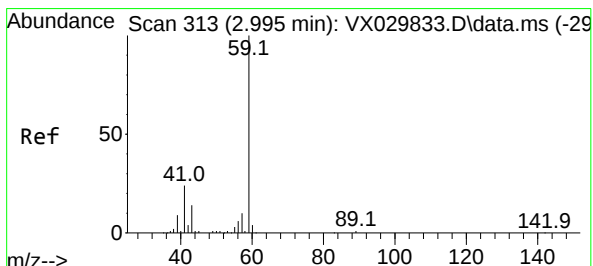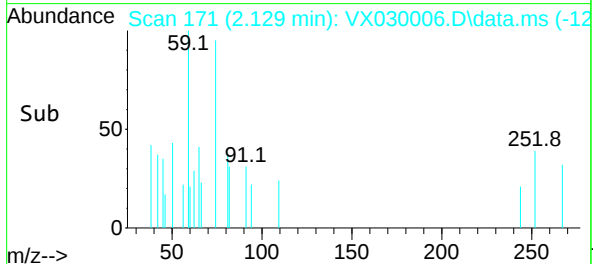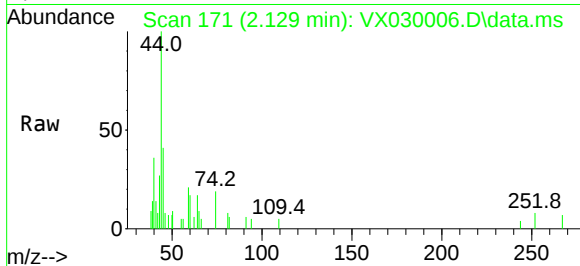

#11
Tert butyl alcohol
Concen: 2.418 ug/l
RT: 2.952 min Scan# 306
Delta R.T. -0.043 min
Lab File: VX030006.D
Acq: 11 Jul 2022 18:41

Tgt Ion: 59 Resp: 1521
Ion Ratio Lower Upper
59 100
57 3.0 7.4 11.2#


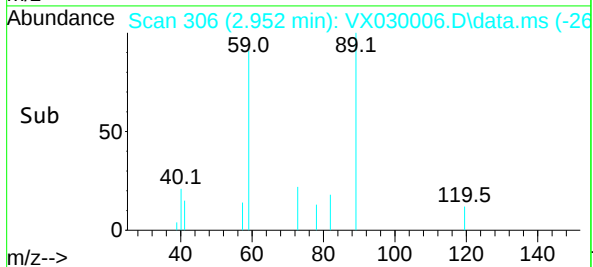

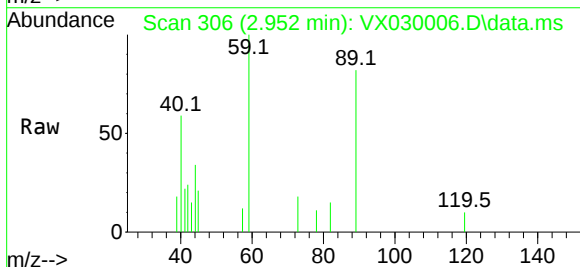




#13
Acrolein
Concen: Below Cal
RT: 2.239 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX030006.D
Acq: 11 Jul 2022 18:41




Instrument :
MSVOA_X
ClientSampleId :
CMR-TP2-0708


Tgt Ion: 56 Resp: 777
Ion Ratio Lower Upper
56 100
55 53.7 56.6 84.8#

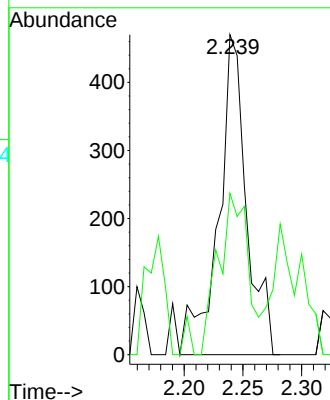

#16
Acetone
Concen: 28.674 ug/l
RT: 2.379 min Scan# 212
Delta R.T. -0.013 min
Lab File: VX030006.D
Acq: 11 Jul 2022 18:41

Tgt Ion: 43 Resp: 33736
Ion Ratio Lower Upper
43 100
58 33.2 27.7 41.5



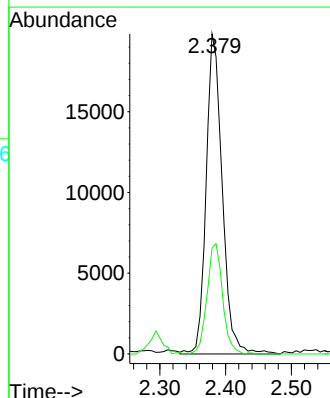



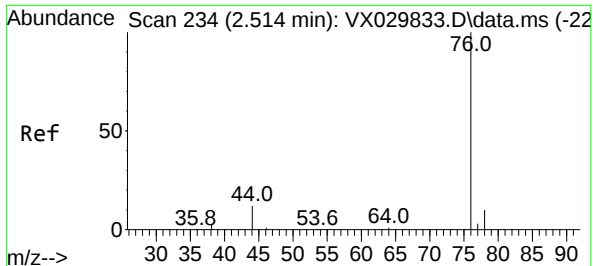

#17
Carbon Disulfide
Concen: 0.426 ug/l
RT: 2.513 min Scan# 21
Delta R.T. -0.000 min
Lab File: VX030006.D
Acq: 11 Jul 2022 18:41




Instrument :
MSVOA_X
ClientSampleId :
CMR-TP2-0708


Tgt Ion: 76 Resp: 2071
Ion Ratio Lower Upper
76 100
78 7.5 7.8 11.6#

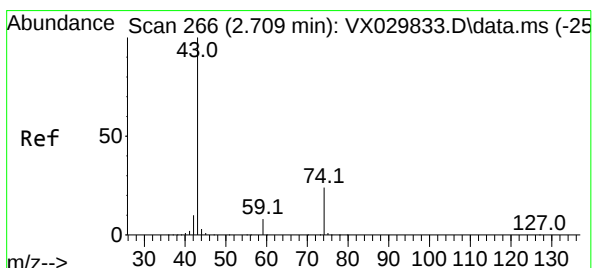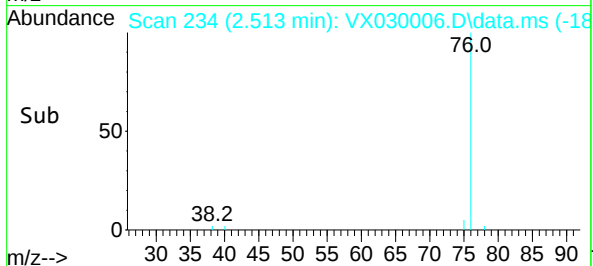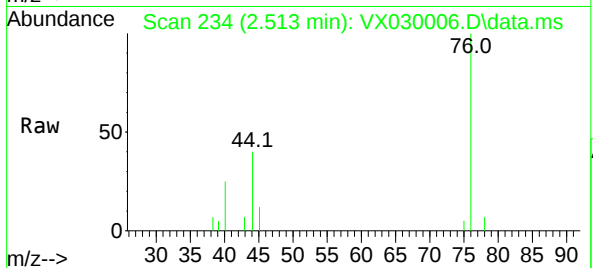

#18
Methyl Acetate
Concen: 0.803 ug/l
RT: 2.715 min Scan# 267
Delta R.T. 0.006 min
Lab File: VX030006.D
Acq: 11 Jul 2022 18:41


Tgt Ion: 43 Resp: 2914
Ion Ratio Lower Upper
43 100
74 25.2 19.4 29.2

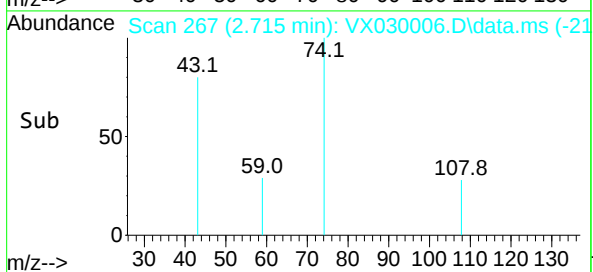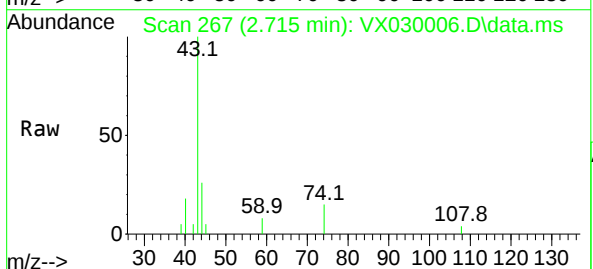





#20
Methylene Chloride
Concen: 9.375 ug/l
RT: 2.788 min Scan# 21
Delta R.T. -0.000 min
Lab File: VX030006.D
Acq: 11 Jul 2022 18:41

Instrument :
MSVOA_X
ClientSampleId :
CMR-TP2-0708







Tgt Ion: 84	Resp: 23295
Ion Ratio	Lower Upper
84 100	
49 96.7	93.8 140.6
51 30.5	29.4 44.0
86 57.2	51.0 76.4



#25
2-Butanone
Concen: 5.232 ug/l
RT: 4.562 min Scan# 570
Delta R.T. -0.006 min
Lab File: VX030006.D
Acq: 11 Jul 2022 18:41

Tgt Ion: 43	Resp: 10684
Ion Ratio	Lower Upper
43 100	
72 26.9	21.7 32.5

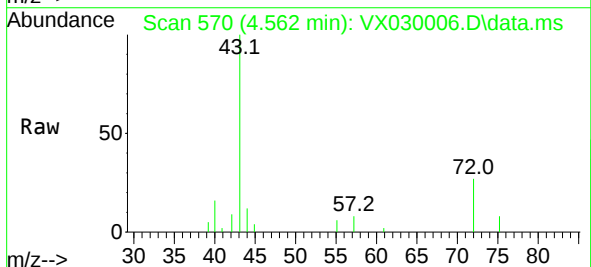

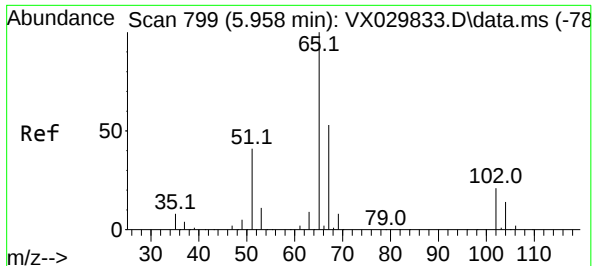

#33

1,2-Dichloroethane-d4

Concen: 42.937 ug/l

RT: 5.958 min Scan# 799

Delta R.T. -0.000 min

Lab File: VX030006.D

Acq: 11 Jul 2022 18:41

Instrument :

MSVOA_X

ClientSampleId :





CMR-TP2-0708

Tgt Ion: 65 Resp: 103257

Ion Ratio Lower Upper

65 100

67 56.4 0.0 109.6

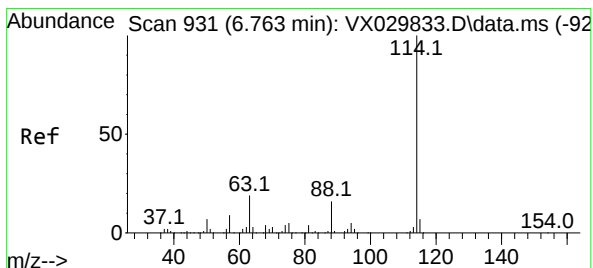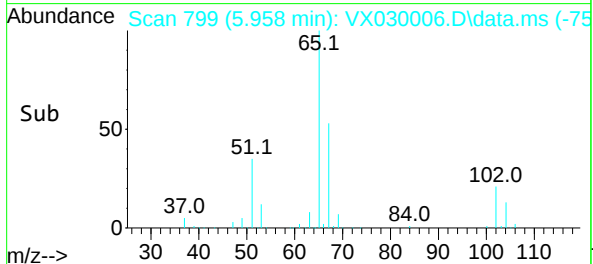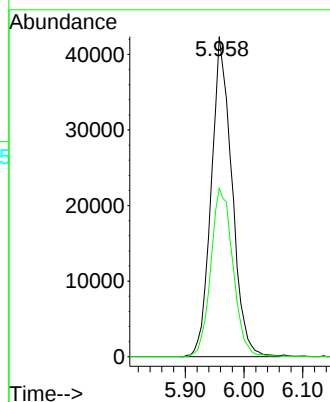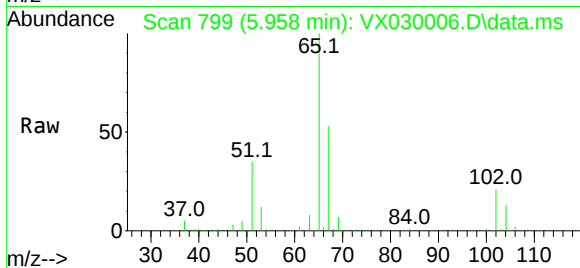

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.769 min Scan# 932

Delta R.T. 0.006 min

Lab File: VX030006.D

Acq: 11 Jul 2022 18:41




Tgt Ion: 114 Resp: 327417


Ion Ratio Lower Upper

114 100

63 18.5 0.0 38.4

88 14.5 0.0 31.8


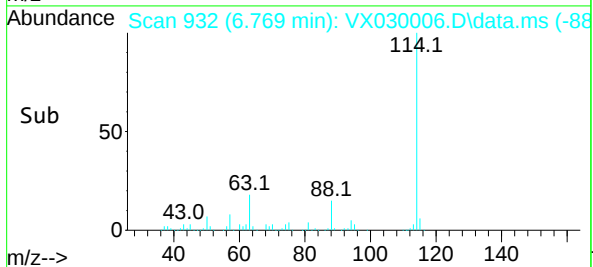
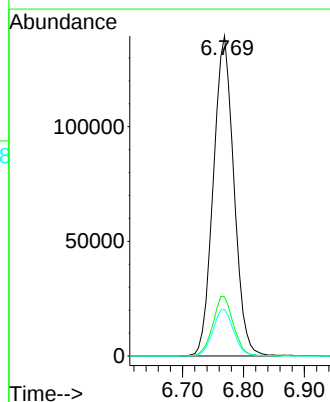
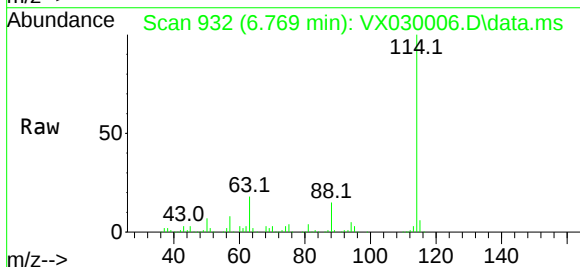


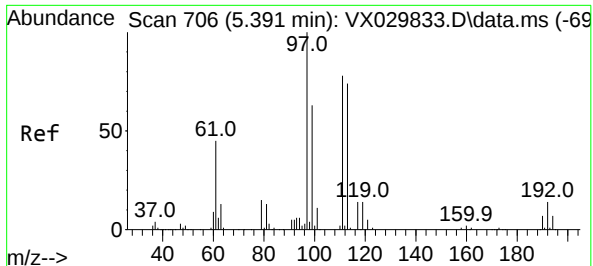

#35
Dibromofluoromethane
Concen: 47.392 ug/l
RT: 5.391 min Scan# 706
Delta R.T. -0.000 min
Lab File: VX030006.D
Acq: 11 Jul 2022 18:41




Instrument :
MSVOA_X
ClientSampleId :
CMR-TP2-0708


Tgt Ion:113 Resp: 96972
Ion Ratio Lower Upper
113 100
111 101.3 83.2 124.8
192 19.3 14.8 22.2

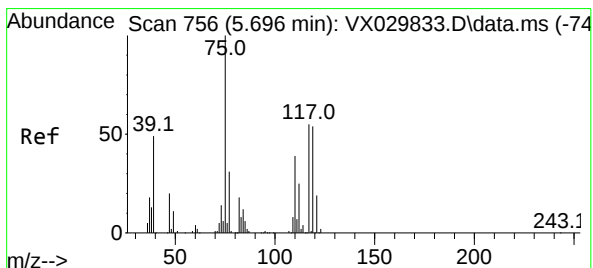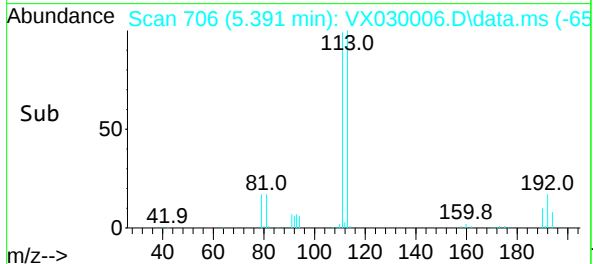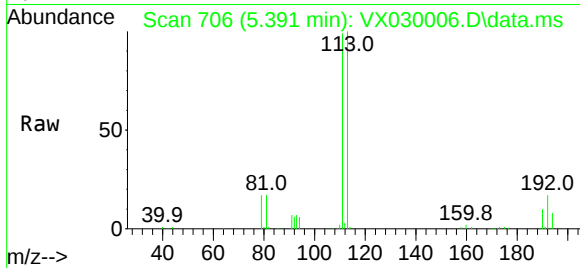

#36
1,1-Dichloropropene
Concen: 5.061 ug/l
RT: 5.549 min Scan# 732
Delta R.T. -0.147 min
Lab File: VX030006.D
Acq: 11 Jul 2022 18:41

Tgt Ion: 75 Resp: 13772
Ion Ratio Lower Upper
75 100
110 8.8 19.3 57.9#
77 0.0 24.4 36.6#

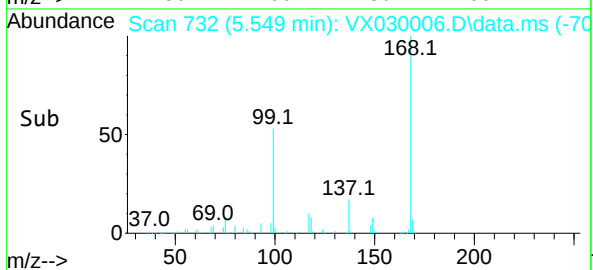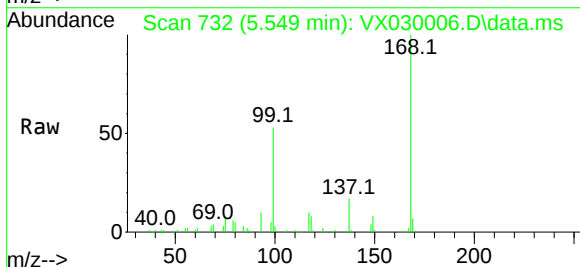



#37

Ethyl Acetate

Concen: 9.994 ug/l

RT: 4.720 min Scan# 596

Delta R.T. -0.000 min

Lab File: VX030006.D

Acq: 11 Jul 2022 18:41





Instrument :

MSVOA_X

ClientSampleId :

CMR-TP2-0708

Tgt Ion:	43	Resp:	37200
Ion	Ratio	Lower	Upper
43	100		
61	16.4	11.7	17.5
70	11.7	9.3	13.9



#38

Carbon Tetrachloride

Concen: 7.552 ug/l




RT: 5.555 min Scan# 733


Delta R.T. -0.128 min

Lab File: VX030006.D

Acq: 11 Jul 2022 18:41

Tgt Ion:	117	Resp:	17808
Ion	Ratio	Lower	Upper
117	100		
119	4.4	74.1	111.1#
121	0.0	25.8	38.8#


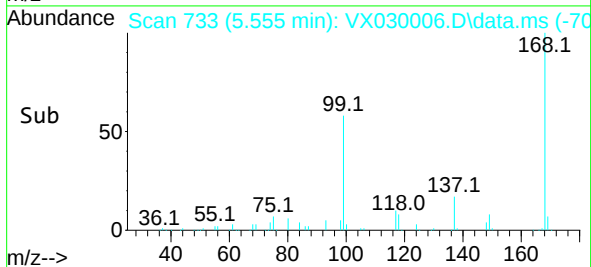

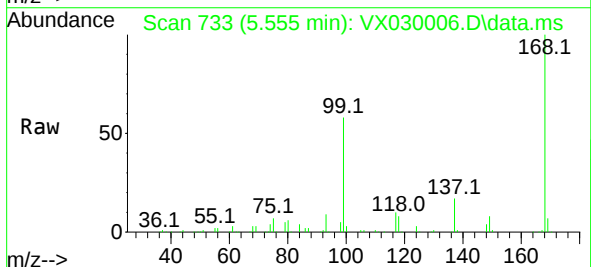


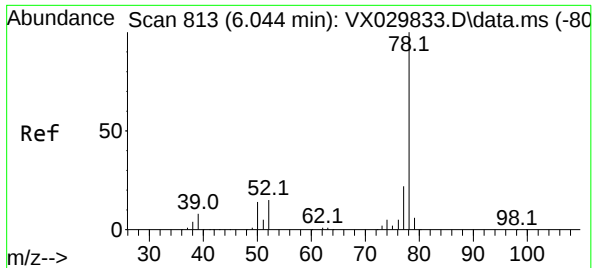

#40
Benzene
Concen: 1.840 ug/l
RT: 6.043 min Scan# 813
Delta R.T. -0.000 min
Lab File: VX030006.D
Acq: 11 Jul 2022 18:41




Instrument :
MSVOA_X
ClientSampleId :
CMR-TP2-0708


Tgt Ion: 78 Resp: 16195
Ion Ratio Lower Upper
78 100
77 19.0 18.0 27.0

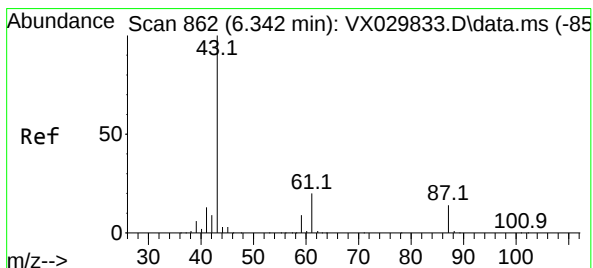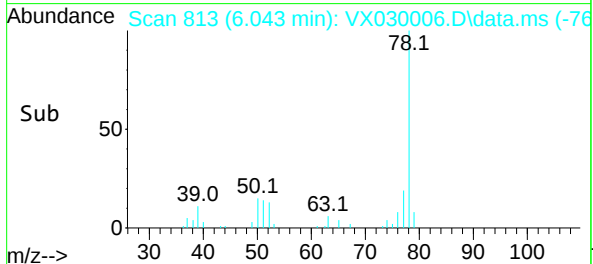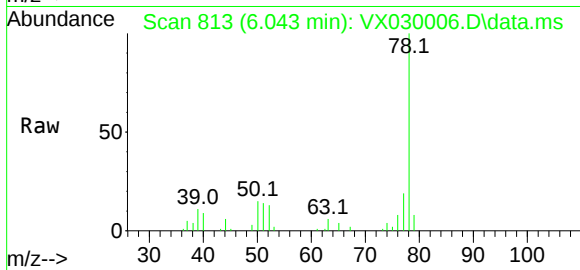

#43
Isopropyl Acetate
Concen: 25.861 ug/l
RT: 6.348 min Scan# 863
Delta R.T. 0.006 min
Lab File: VX030006.D
Acq: 11 Jul 2022 18:41

Tgt Ion: 43 Resp: 144950
Ion Ratio Lower Upper
43 100
61 21.1 16.5 24.7
87 13.3 11.1 16.7


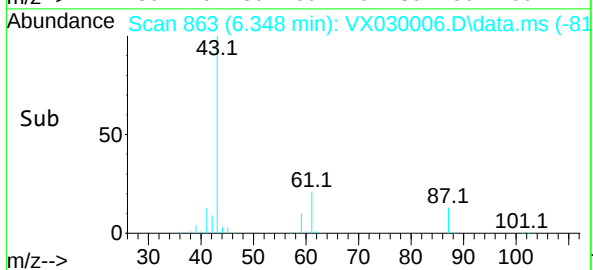

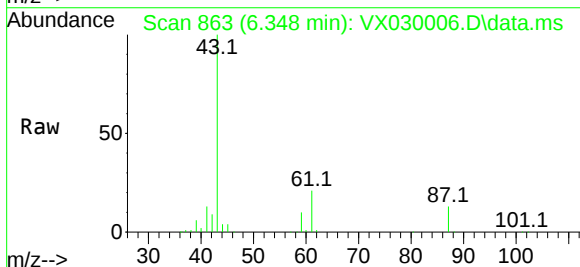


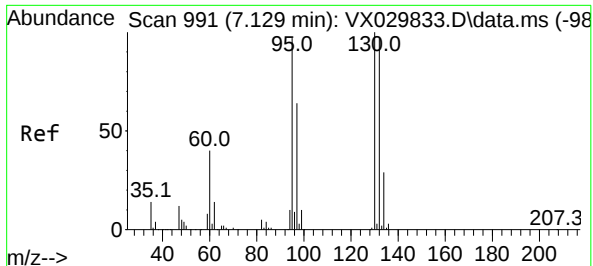

#44
Trichloroethene
Concen: 0.368 ug/l
RT: 7.128 min Scan# 991
Delta R.T. -0.000 min
Lab File: VX030006.D
Acq: 11 Jul 2022 18:41




Instrument :
MSVOA_X
ClientSampleId :
CMR-TP2-0708


Tgt Ion:130 Resp: 873
Ion Ratio Lower Upper
130 100
95 65.2 0.0 194.8

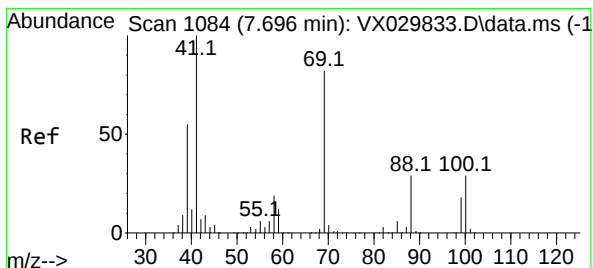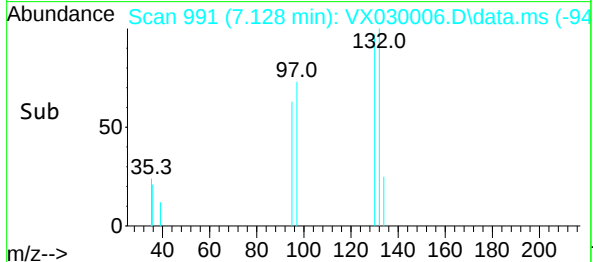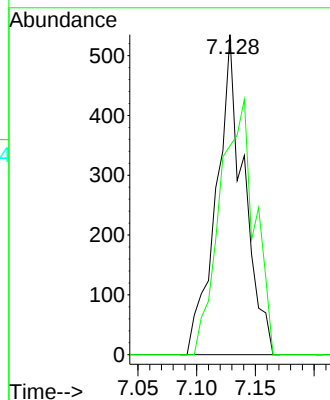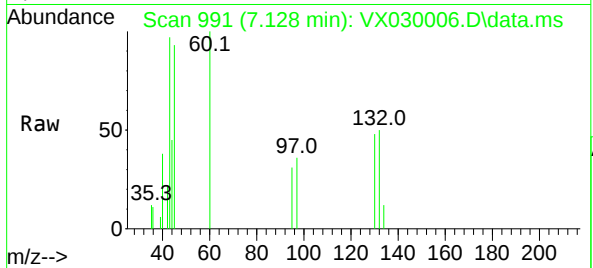

#48
Methyl methacrylate
Concen: 44.876 ug/l
RT: 7.805 min Scan# 1102
Delta R.T. 0.109 min
Lab File: VX030006.D
Acq: 11 Jul 2022 18:41

Tgt Ion: 41 Resp: 119255
Ion Ratio Lower Upper
41 100
69 0.1 68.8 103.2#
39 51.7 44.6 66.8

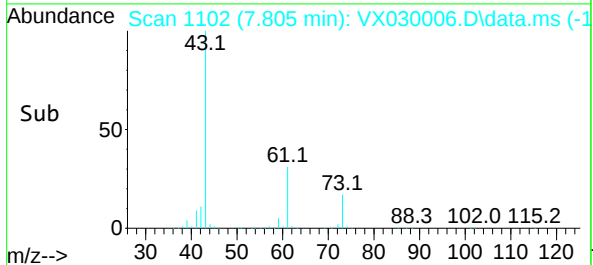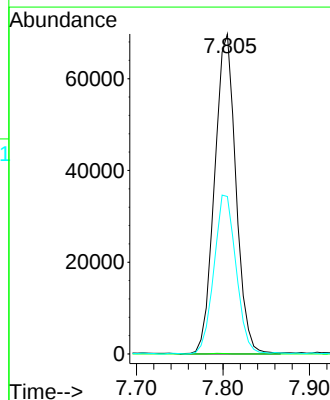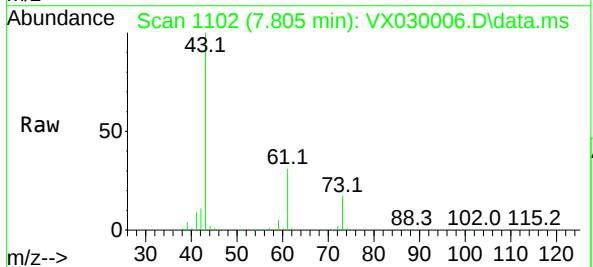



#49

1,4-Dioxane

Concen: 0.461 ug/l

RT: 7.659 min Scan# 1078

Delta R.T. -0.025 min

Lab File: VX030006.D


Acq: 11 Jul 2022 18:41

Instrument :

MSVOA_X

ClientSampleId :

CMR-TP2-0708






Tgt Ion: 88 Resp: 29

Ion Ratio Lower Upper

88 100

43 0.0 23.8 35.8#

58 10741.4 53.8 80.6#



#50

Toluene-d8

Concen: 48.343 ug/l

RT: 8.652 min Scan# 1241

Delta R.T. -0.000 min

Lab File: VX030006.D




Acq: 11 Jul 2022 18:41


Tgt Ion: 98 Resp: 371094

Ion Ratio Lower Upper

98 100

100 66.2 52.3 78.5


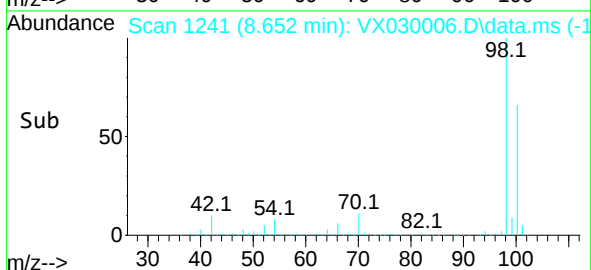






#51
4-Methyl-2-Pentanone
Concen: 27.676 ug/l
RT: 8.555 min Scan# 11
Delta R.T. -0.025 min
Lab File: VX030006.D
Acq: 11 Jul 2022 18:41




Instrument :
MSVOA_X
ClientSampleId :
CMR-TP2-0708


Tgt Ion: 43 Resp: 102286
Ion Ratio Lower Upper
43 100
58 8.8 31.4 47.2#



#52
Toluene
Concen: 1.820 ug/l
RT: 8.726 min Scan# 1253
Delta R.T. 0.006 min
Lab File: VX030006.D
Acq: 11 Jul 2022 18:41

Tgt Ion: 92 Resp: 9662
Ion Ratio Lower Upper
92 100
91 169.6 139.2 208.8

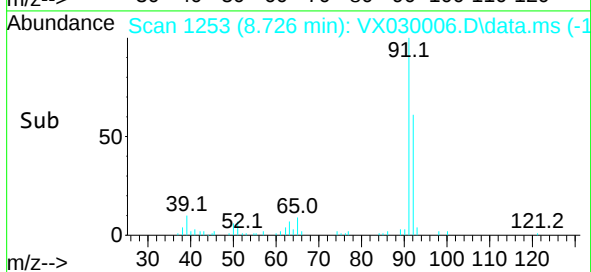

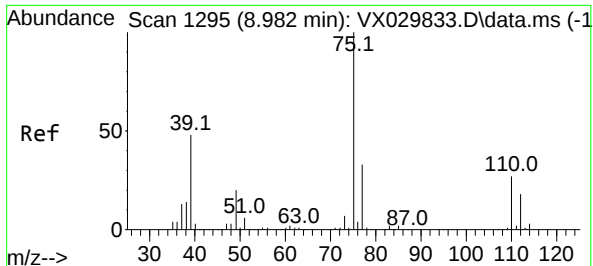

#53

t-1,3-Dichloropropene

Concen: 0.323 ug/l

RT: 8.957 min Scan# 11

Delta R.T. -0.025 min

Lab File: VX030006.D

Acq: 11 Jul 2022 18:41

Instrument :

MSVOA_X

ClientSampleId :





CMR-TP2-0708

Tgt Ion: 75 Resp: 937

Ion Ratio Lower Upper

75 100

77 0.0 26.3 39.5#

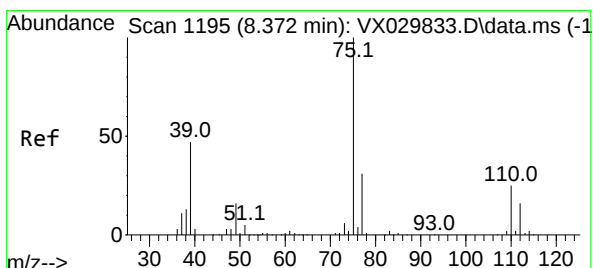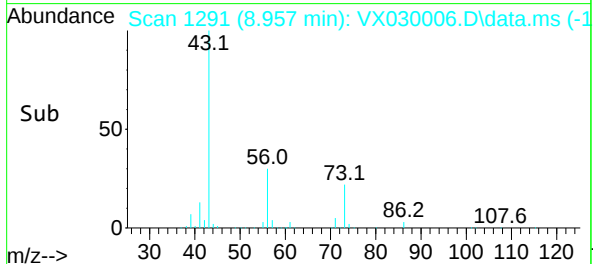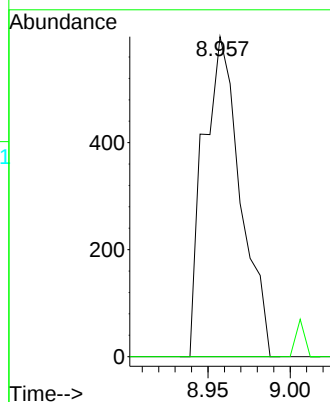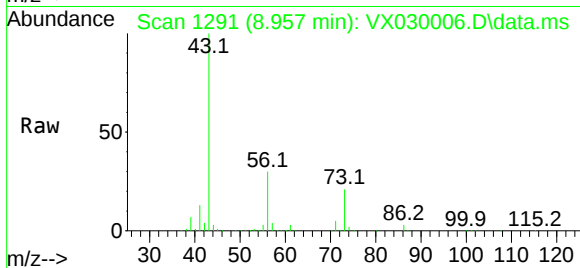

#54

cis-1,3-Dichloropropene

Concen: 15.631 ug/l

RT: 8.555 min Scan# 1225

Delta R.T. 0.183 min

Lab File: VX030006.D

Acq: 11 Jul 2022 18:41




Tgt Ion: 75 Resp: 51308


Ion Ratio Lower Upper

75 100

77 0.3 25.0 37.4#

39 25.0 37.5 56.3#

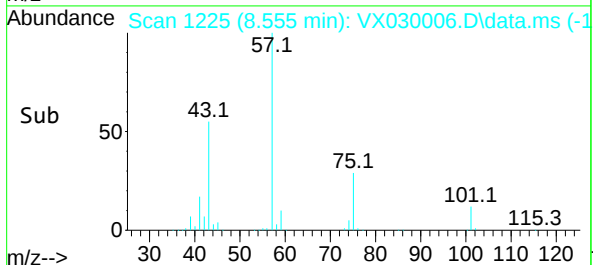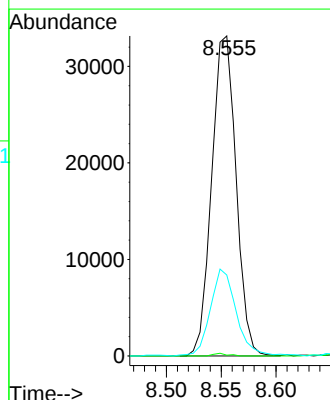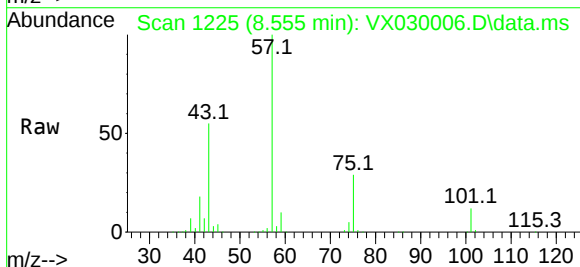



#57

1,3-Dichloropropane

Concen: 1.765 ug/l

RT: 9.488 min Scan# 1378

Delta R.T. 0.176 min

Lab File: VX030006.D

Acq: 11 Jul 2022 18:41

Instrument :

MSVOA_X

ClientSampleId :





CMR-TP2-0708

Tgt Ion: 76 Resp: 6570

Ion Ratio Lower Upper

76 100

78 0.4 25.9 38.9#

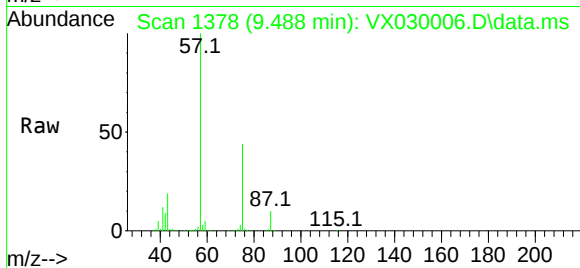

#59

2-Hexanone

Concen: 29.632 ug/l

RT: 9.488 min Scan# 1378

Delta R.T. 0.055 min

Lab File: VX030006.D




Acq: 11 Jul 2022 18:41


Tgt Ion: 43 Resp: 84990

Ion Ratio Lower Upper

43 100

58 19.4 27.6 82.8#




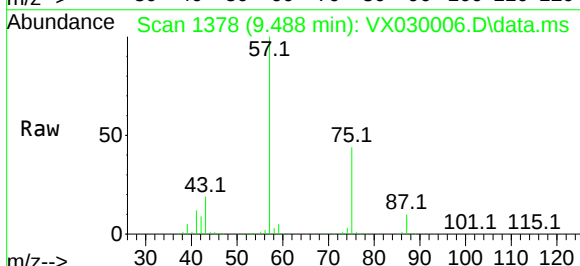




#62
4-Bromofluorobenzene
Concen: 46.195 ug/l
RT: 11.085 min Scan# 1639
Delta R.T. 0.006 min
Lab File: VX030006.D
Acq: 11 Jul 2022 18:41




Instrument :
MSVOA_X
ClientSampleId :
CMR-TP2-0708


Tgt Ion: 95 Resp: 125348
Ion Ratio Lower Upper
95 100
174 81.4 0.0 149.0
176 77.8 0.0 146.0

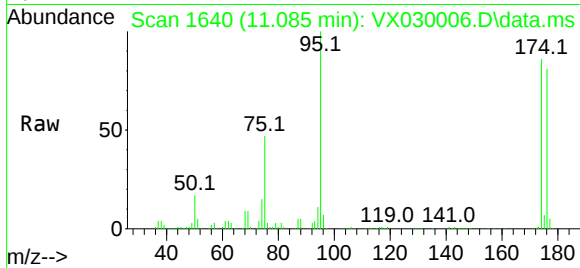

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX030006.D
Acq: 11 Jul 2022 18:41

Tgt Ion: 117 Resp: 286224
Ion Ratio Lower Upper
117 100
82 53.9 42.7 64.1
119 31.7 25.4 38.2


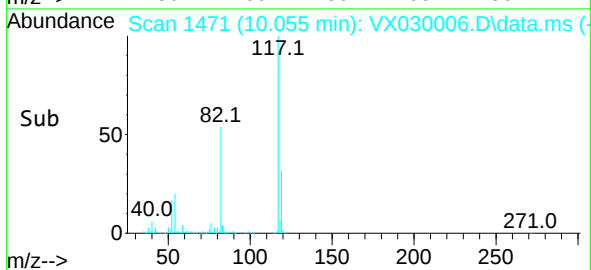

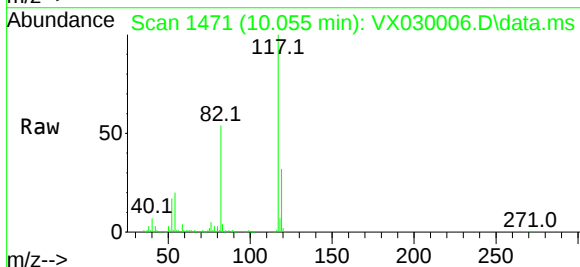




#68
m/p-Xylenes
Concen: 0.657 ug/l
RT: 10.305 min Scan# 1512
Delta R.T. -0.000 min
Lab File: VX030006.D
Acq: 11 Jul 2022 18:41




Instrument :
MSVOA_X
ClientSampleId :
CMR-TP2-0708


Tgt Ion:106 Resp: 2518
Ion Ratio Lower Upper
106 100
91 205.5 158.2 237.4

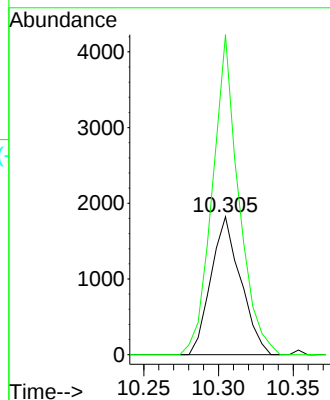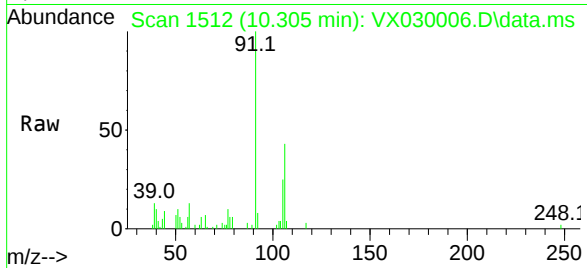

#69
o-Xylene
Concen: 0.334 ug/l
RT: 10.646 min Scan# 1568
Delta R.T. -0.000 min
Lab File: VX030006.D
Acq: 11 Jul 2022 18:41

Tgt Ion:106 Resp: 1297
Ion Ratio Lower Upper
106 100
91 167.2 103.8 311.6

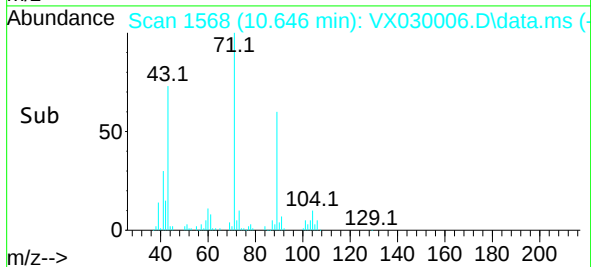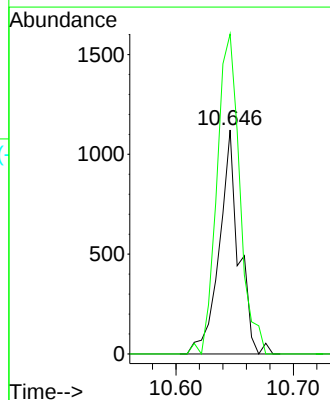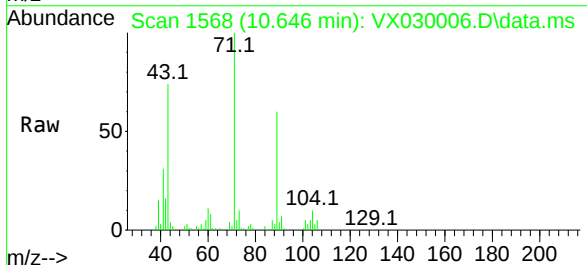



#70

Styrene

Concen: 1.617 ug/l

RT: 10.658 min Scan# 11

Delta R.T. -0.000 min

Lab File: VX030006.D

Acq: 11 Jul 2022 18:41

Instrument :

MSVOA_X

ClientSampleId :

CMR-TP2-0708





Tgt Ion:104 Resp: 10377

Ion Ratio Lower Upper

104 100

78 40.9 37.8 56.8

103 48.1 44.5 66.7

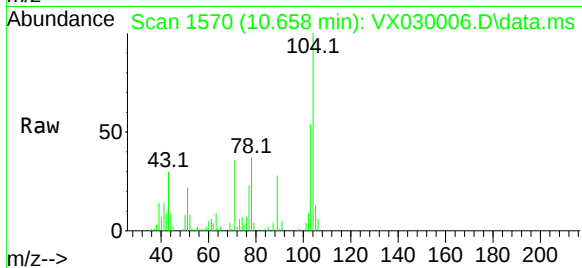

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.024 min Scan# 1794

Delta R.T. -0.000 min

Lab File: VX030006.D

Acq: 11 Jul 2022 18:41




Tgt Ion:152 Resp: 128912


Ion Ratio Lower Upper

152 100

115 59.0 40.5 121.5

150 157.7 0.0 347.0


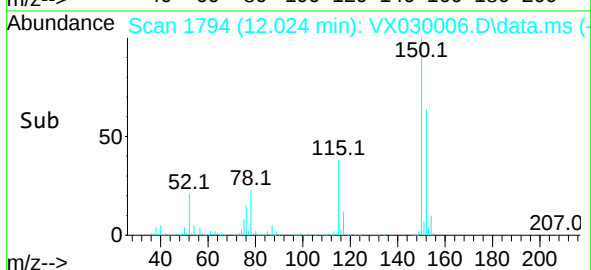

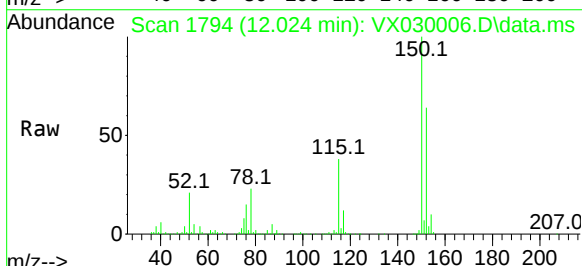




#74
N-amy1 acetate
Concen: 0.204 ug/l
RT: 10.768 min Scan# 11
Delta R.T. -0.080 min
Lab File: VX030006.D
Acq: 11 Jul 2022 18:41




Instrument :
MSVOA_X
ClientSampleId :
CMR-TP2-0708


Tgt Ion: 43	Resp: 942
Ion Ratio	Lower Upper
43	100
70	0.0 32.3 48.5#
55	0.0 18.4 27.6#
61	0.0 19.2 28.8#

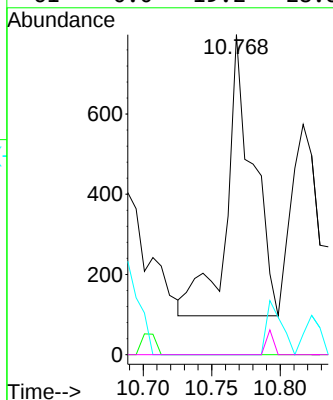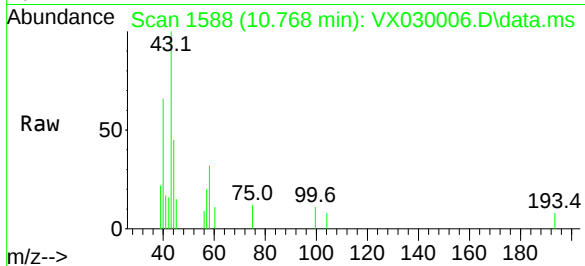

#76
1,2,3-Trichloropropane
Concen: 19.208 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. -0.159 min
Lab File: VX030006.D
Acq: 11 Jul 2022 18:41

Tgt Ion: 75	Resp: 59276
Ion Ratio	Lower Upper
75	100
77	1.4 19.8 59.3#


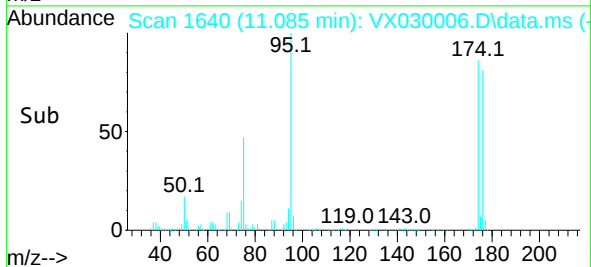
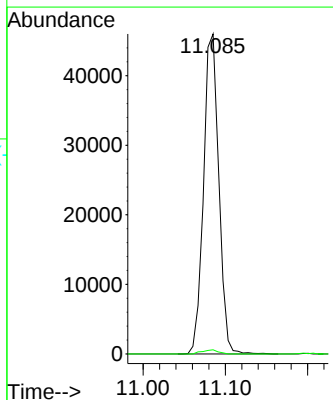
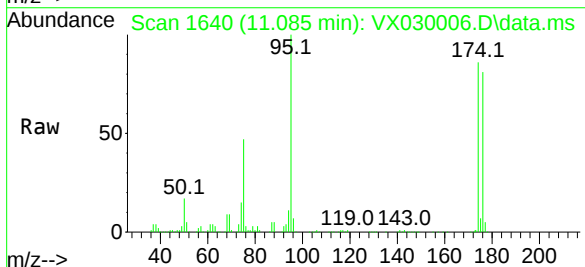




#81
 trans-1,4-Dichloro-2-butene
 Concen: 61.001 ug/l
 RT: 11.085 min Scan# 1
 Delta R.T. 0.067 min
 Lab File: VX030006.D
 Acq: 11 Jul 2022 18:41




Instrument :
 MSVOA_X
 ClientSampleId :
 CMR-TP2-0708


Tgt Ion: 75 Resp: 59276
 Ion Ratio Lower Upper
 75 100
 53 0.0 74.2 111.4#
 89 0.0 34.8 52.2#

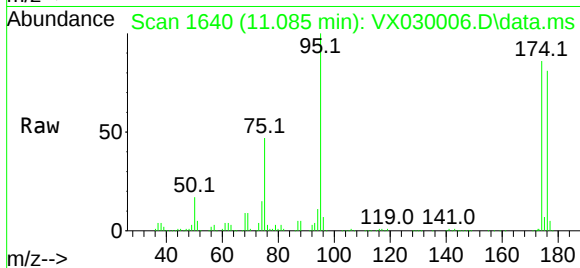

#84
 1,2,4-Trimethylbenzene
 Concen: 0.290 ug/l
 RT: 11.756 min Scan# 1750
 Delta R.T. -0.000 min
 Lab File: VX030006.D
 Acq: 11 Jul 2022 18:41

Tgt Ion: 105 Resp: 2253
 Ion Ratio Lower Upper
 105 100
 120 32.5 22.9 68.8


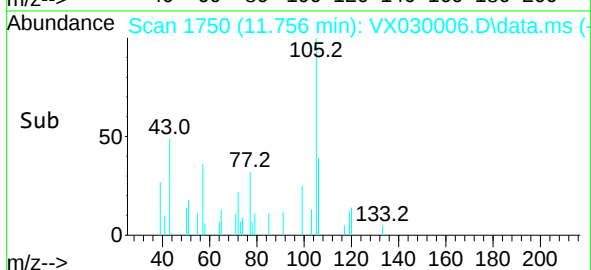

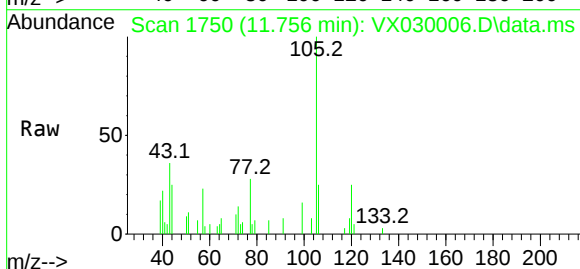




#90
Hexachloroethane
Concen: 0.345 ug/l
RT: 12.615 min Scan# 1879
Delta R.T. 0.073 min
Lab File: VX030006.D
Acq: 11 Jul 2022 18:41

Instrument :
MSVOA_X
ClientSampleId :
CMR-TP2-0708

Tgt Ion:117 Resp: 434
Ion Ratio Lower Upper
117 100
201 0.0 34.2 102.5#

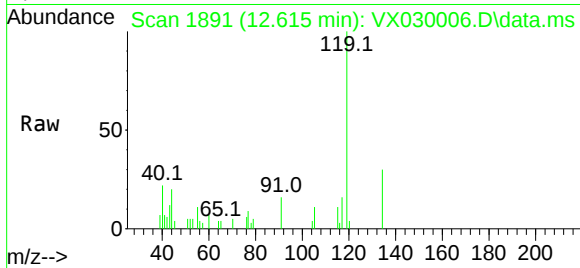

#95
Naphthalene
Concen: 7.009 ug/l
RT: 13.780 min Scan# 2082
Delta R.T. -0.000 min
Lab File: VX030006.D
Acq: 11 Jul 2022 18:41

Tgt Ion:128 Resp: 72976
Ion Ratio Lower Upper
128 100
127 13.1 10.2 15.2
129 11.1 8.6 13.0

