


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071122\
Data File : VX029985.D
Acq On : 11 Jul 2022 09:20
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X062822W.M
Title : SW846 8260
Last Update : Wed Jun 29 05:54:51 2022

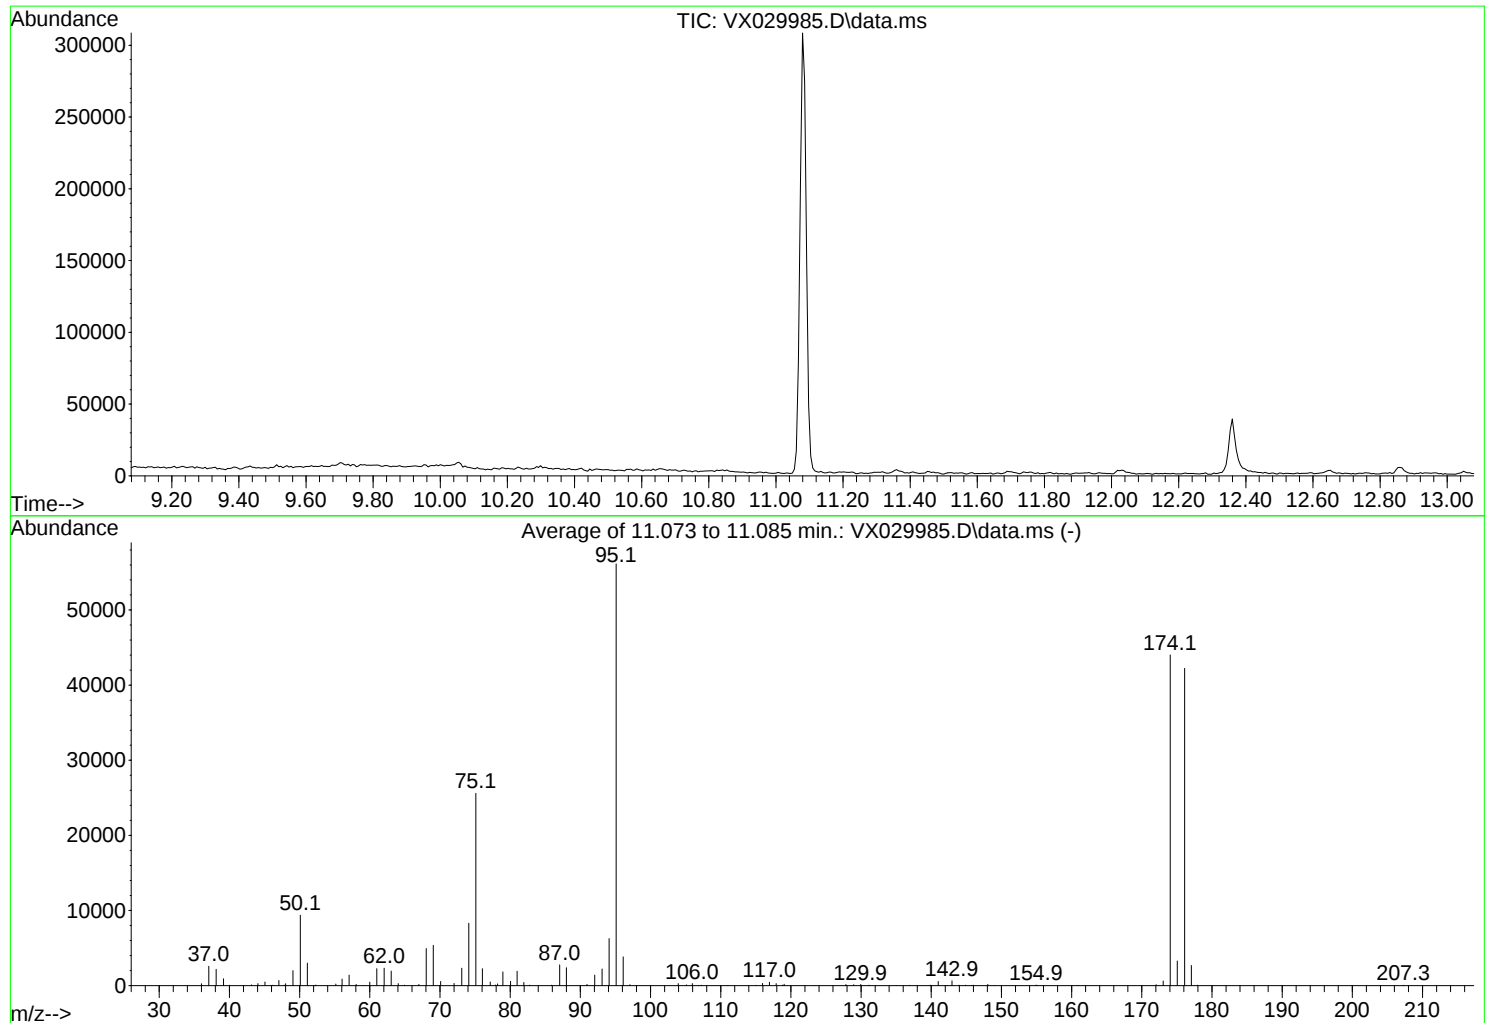

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1631

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.7	9376	PASS
75	95	30	60	45.6	25603	PASS
95	95	100	100	100.0	56144	PASS
96	95	5	9	6.8	3835	PASS
173	174	0.00	2	1.4	624	PASS
174	95	50	100	78.4	44029	PASS
175	174	5	9	7.4	3279	PASS
176	174	95	101	95.9	42229	PASS
177	176	5	9	6.4	2687	PASS