


Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX071218\
 Data File : VX003342.D
 Acq On : 12 Jul 2018 10:13
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\624X071218W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Thu Jul 12 13:28:20 2018

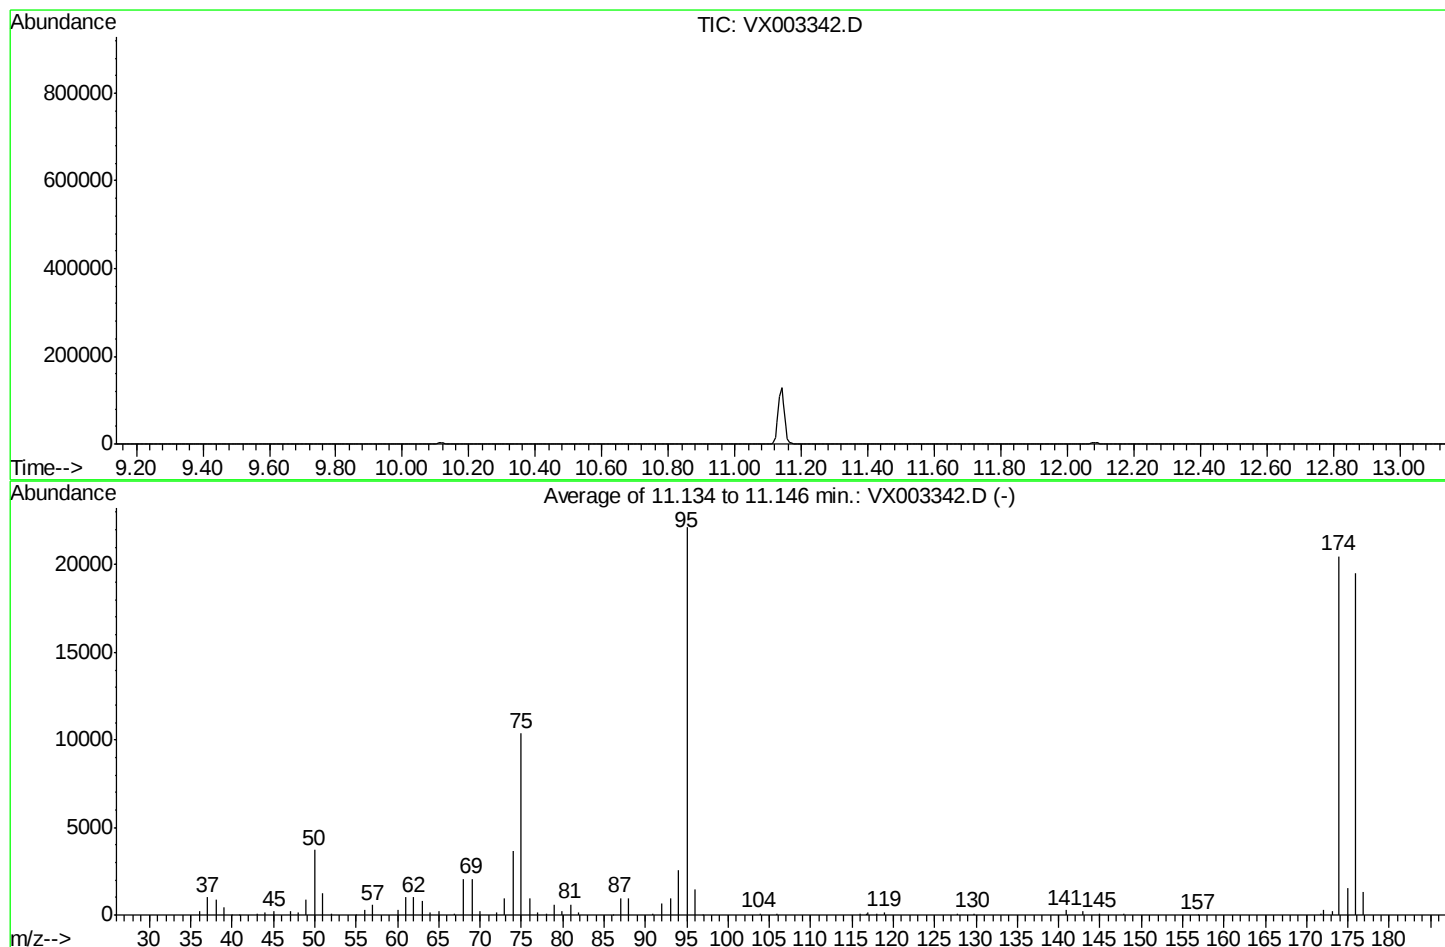

AutoFind: Scans 1730, 1731, 1732; Background Corrected with Scan 1725

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.8	3726	PASS
75	95	30	60	46.8	10366	PASS
95	95	100	100	100.0	22138	PASS
96	95	5	9	6.8	1497	PASS
173	174	0.00	2	1.0	210	PASS
174	95	50	100	92.5	20472	PASS
175	174	5	9	7.5	1536	PASS
176	174	95	101	95.3	19503	PASS
177	176	5	9	6.9	1343	PASS