

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX071219\
 Data File : VX010865.D
 Acq On : 13 Jul 2019 02:55
 Operator : JC/SP
 Sample : K3791-12
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 FL-0603

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X061919W.M
 Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.276	16	20	27	rBV	51837	71739	6.05%	1.110%
2	1.611	65	75	80	rBV10	6667	16547	1.40%	0.256%
3	2.605	232	238	246	rBV	11776	22121	1.87%	0.342%
4	5.501	696	713	727	rBV	138899	402841	33.98%	6.231%
5	5.665	727	740	755	rVB	240525	679800	57.34%	10.515%
6	6.061	793	805	819	rBV	139844	366693	30.93%	5.672%
7	6.860	923	936	948	rBV	361881	849226	71.63%	13.135%
8	8.713	1232	1240	1250	rBV	774974	1185504	100.00%	18.337%
9	10.109	1463	1469	1476	rBV	747035	1027630	86.68%	15.895%
10	11.134	1629	1637	1647	rBV	653863	836306	70.54%	12.936%
11	11.804	1741	1747	1753	rBV	16300	20297	1.71%	0.314%
12	12.073	1786	1791	1798	rBV	766706	972537	82.04%	15.043%
13	14.694	2214	2221	2225	rBV	10204	13909	1.17%	0.215%


Sum of corrected areas: 6465150

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX071219\
Data File : VX010865.D
Acq On : 13 Jul 2019 02:55
Operator : JC/SP
Sample : K3791-12
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FL-0603

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X061919W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

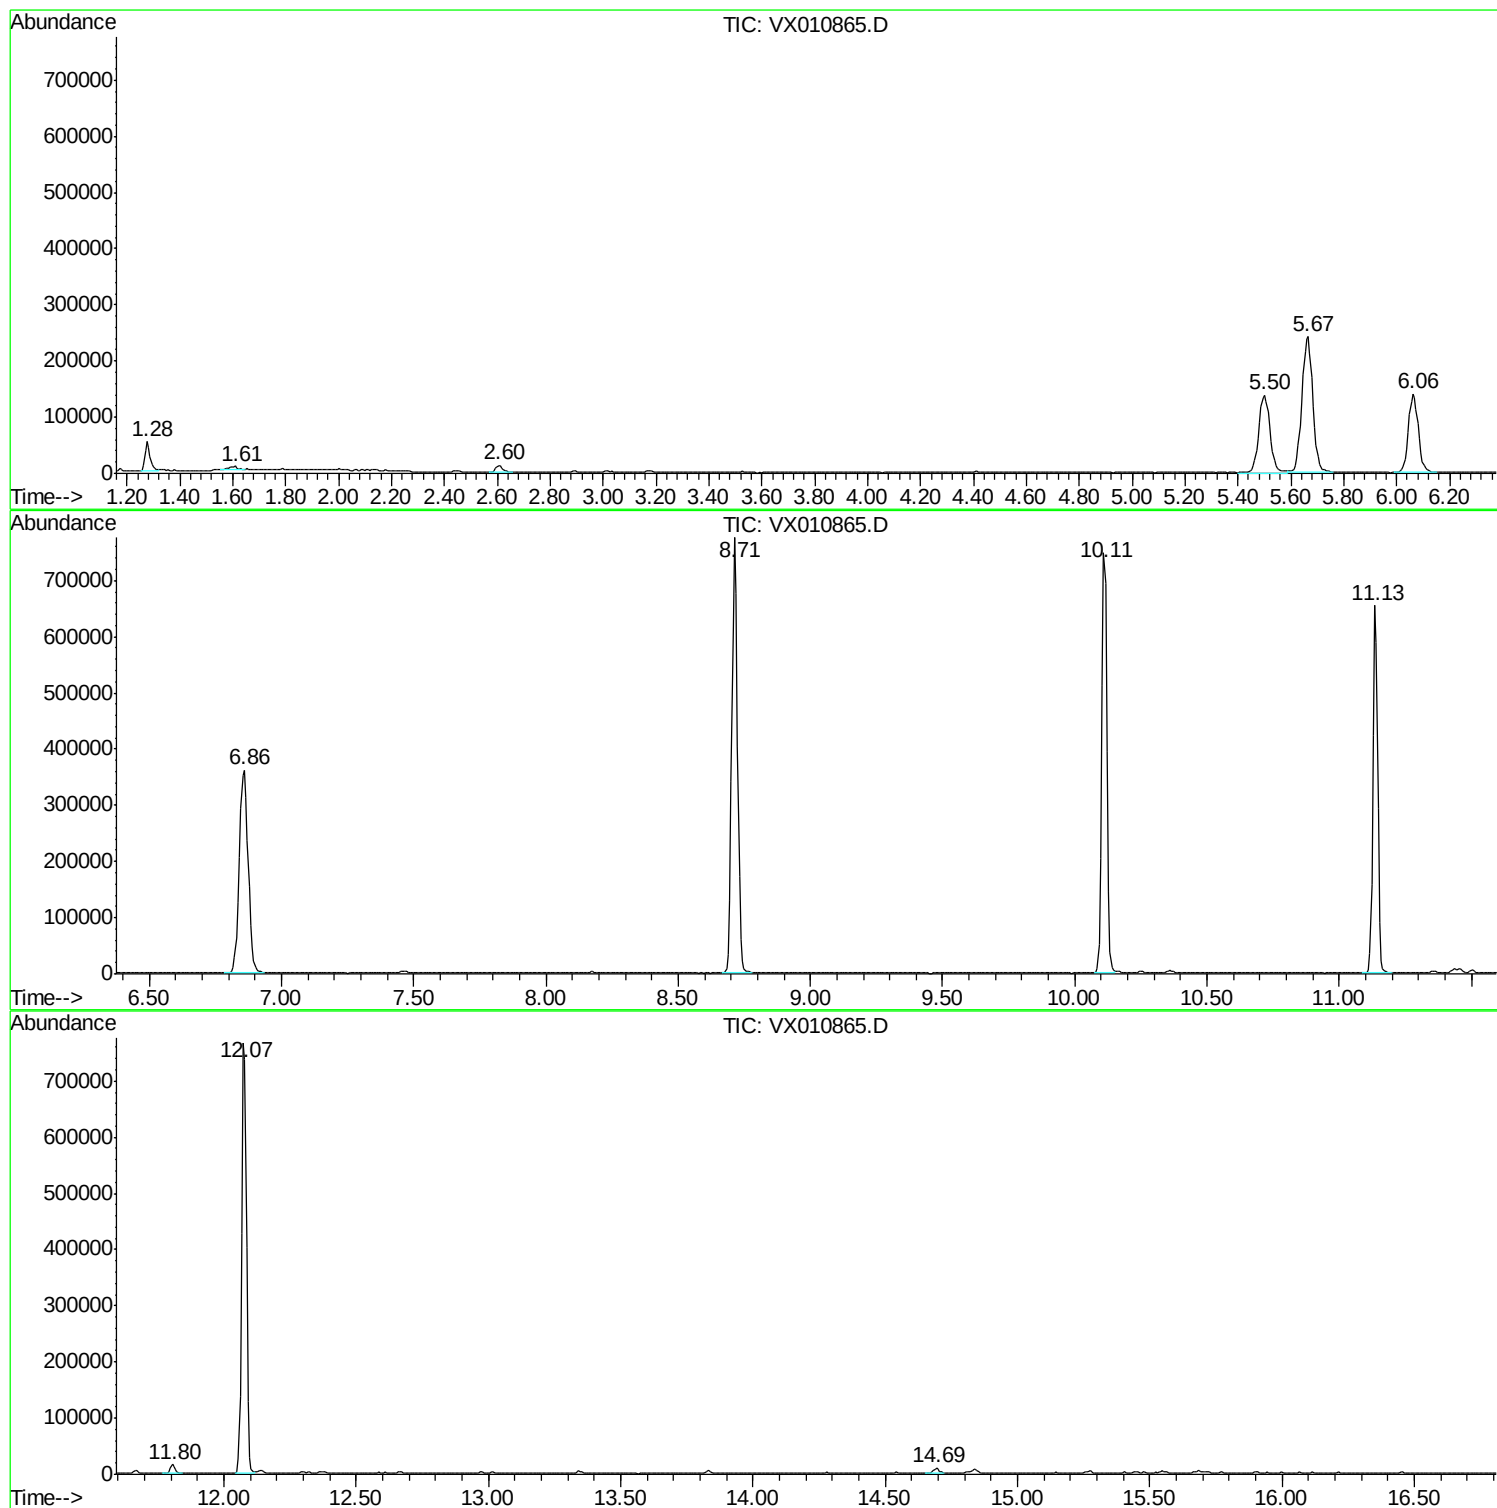

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX071219\
Data File : VX010865.D
Acq On : 13 Jul 2019 02:55
Operator : JC/SP
Sample : K3791-12
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 45 Sample Multiplier: 1










Instrument :
MSVOA_X
ClientSampleId :
FL-0603

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X061919W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Sulfur dioxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.28	5.28 ug/l	71739	Pentafluorobenzene	5.67
Hit# of	5	Tentative ID	MW MolForm	CAS# Qual
1	Sulfur dioxide	64 02S	007446-09-5	83
2	Aminomethanesulfonic acid	111 CH5NO3S	013881-91-9	74
3	L-Alanine, 3-sulfo-	169 C3H7NO5S	000498-40-8	9
4	Ethene, 1,1-difluoro-	64 C2H2F2	000075-38-7	4
5	Ethyl Chloride	64 C2H5Cl	000075-00-3	3

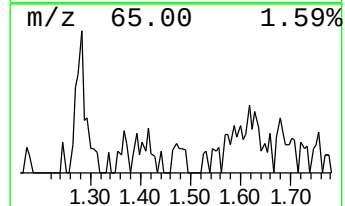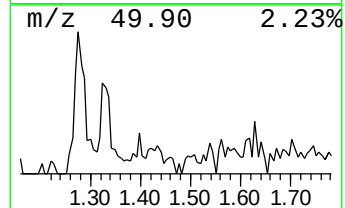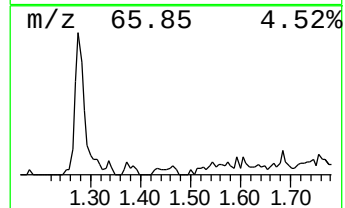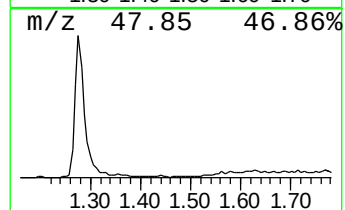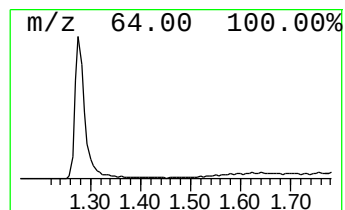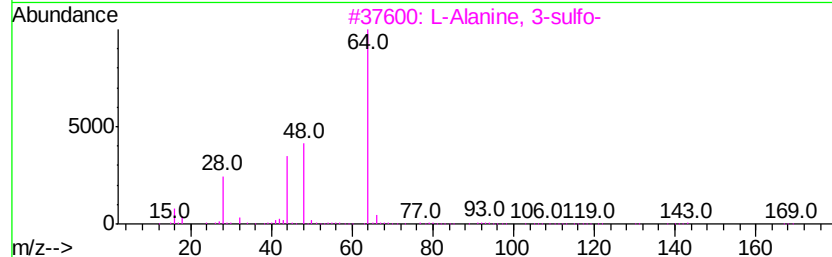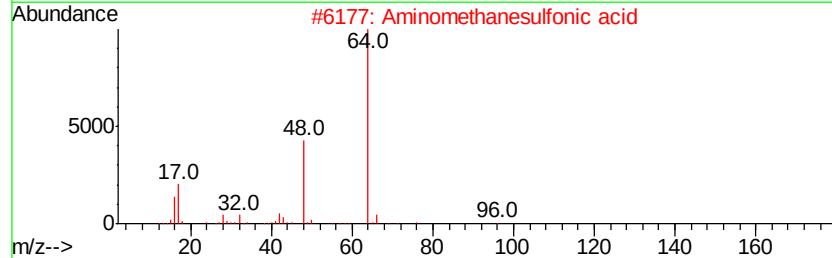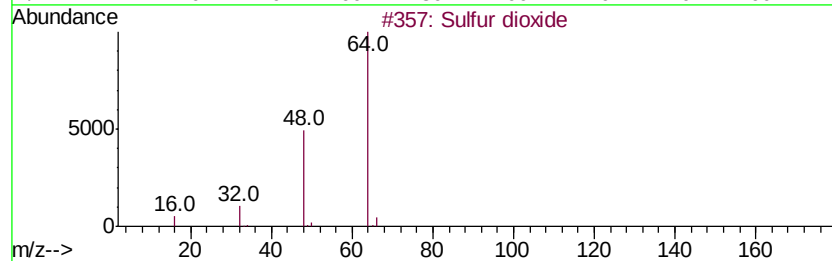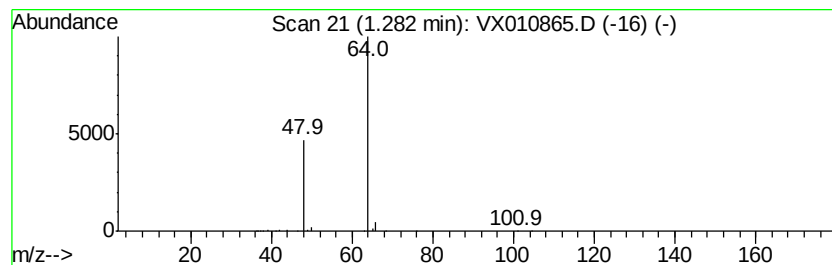

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX071219\
Data File : VX010865.D
Acq On : 13 Jul 2019 02:55
Operator : JC/SP
Sample : K3791-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FL-0603

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X061919W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Sulfur dioxide	1.28	5.3	ug/l	71739	1	5.67	679800	50.0