

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX071219\
 Data File : VX010867.D
 Acq On : 13 Jul 2019 03:42
 Operator : JC/SP
 Sample : K3791-02
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 FL-0600

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X061919W.M

Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.276	16	20	29	rBV	61851	84906	7.28%	1.324%
2	1.605	66	74	78	rBV3	6580	16746	1.44%	0.261%
3	2.605	234	238	246	rVB	9843	17567	1.51%	0.274%
4	5.501	699	713	724	rBV	136517	392022	33.60%	6.115%
5	5.659	728	739	757	rVB	233793	670904	57.50%	10.465%
6	6.062	794	805	819	rBV	139132	364028	31.20%	5.678%
7	6.860	925	936	949	rBV	351390	839928	71.99%	13.102%
8	7.458	1025	1034	1041	rBV6	4734	12735	1.09%	0.199%
9	8.713	1233	1240	1250	rBV	759242	1166750	100.00%	18.200%
10	10.110	1463	1469	1476	rBV	761375	1017073	87.17%	15.865%
11	11.134	1631	1637	1650	rBV	658580	831621	71.28%	12.972%
12	11.804	1743	1747	1752	rBV	9949	13042	1.12%	0.203%
13	12.073	1786	1791	1799	rBV	749364	983451	84.29%	15.341%


Sum of corrected areas: 6410773

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX071219\
Data File : VX010867.D
Acq On : 13 Jul 2019 03:42
Operator : JC/SP
Sample : K3791-02
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FL-0600

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X061919W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

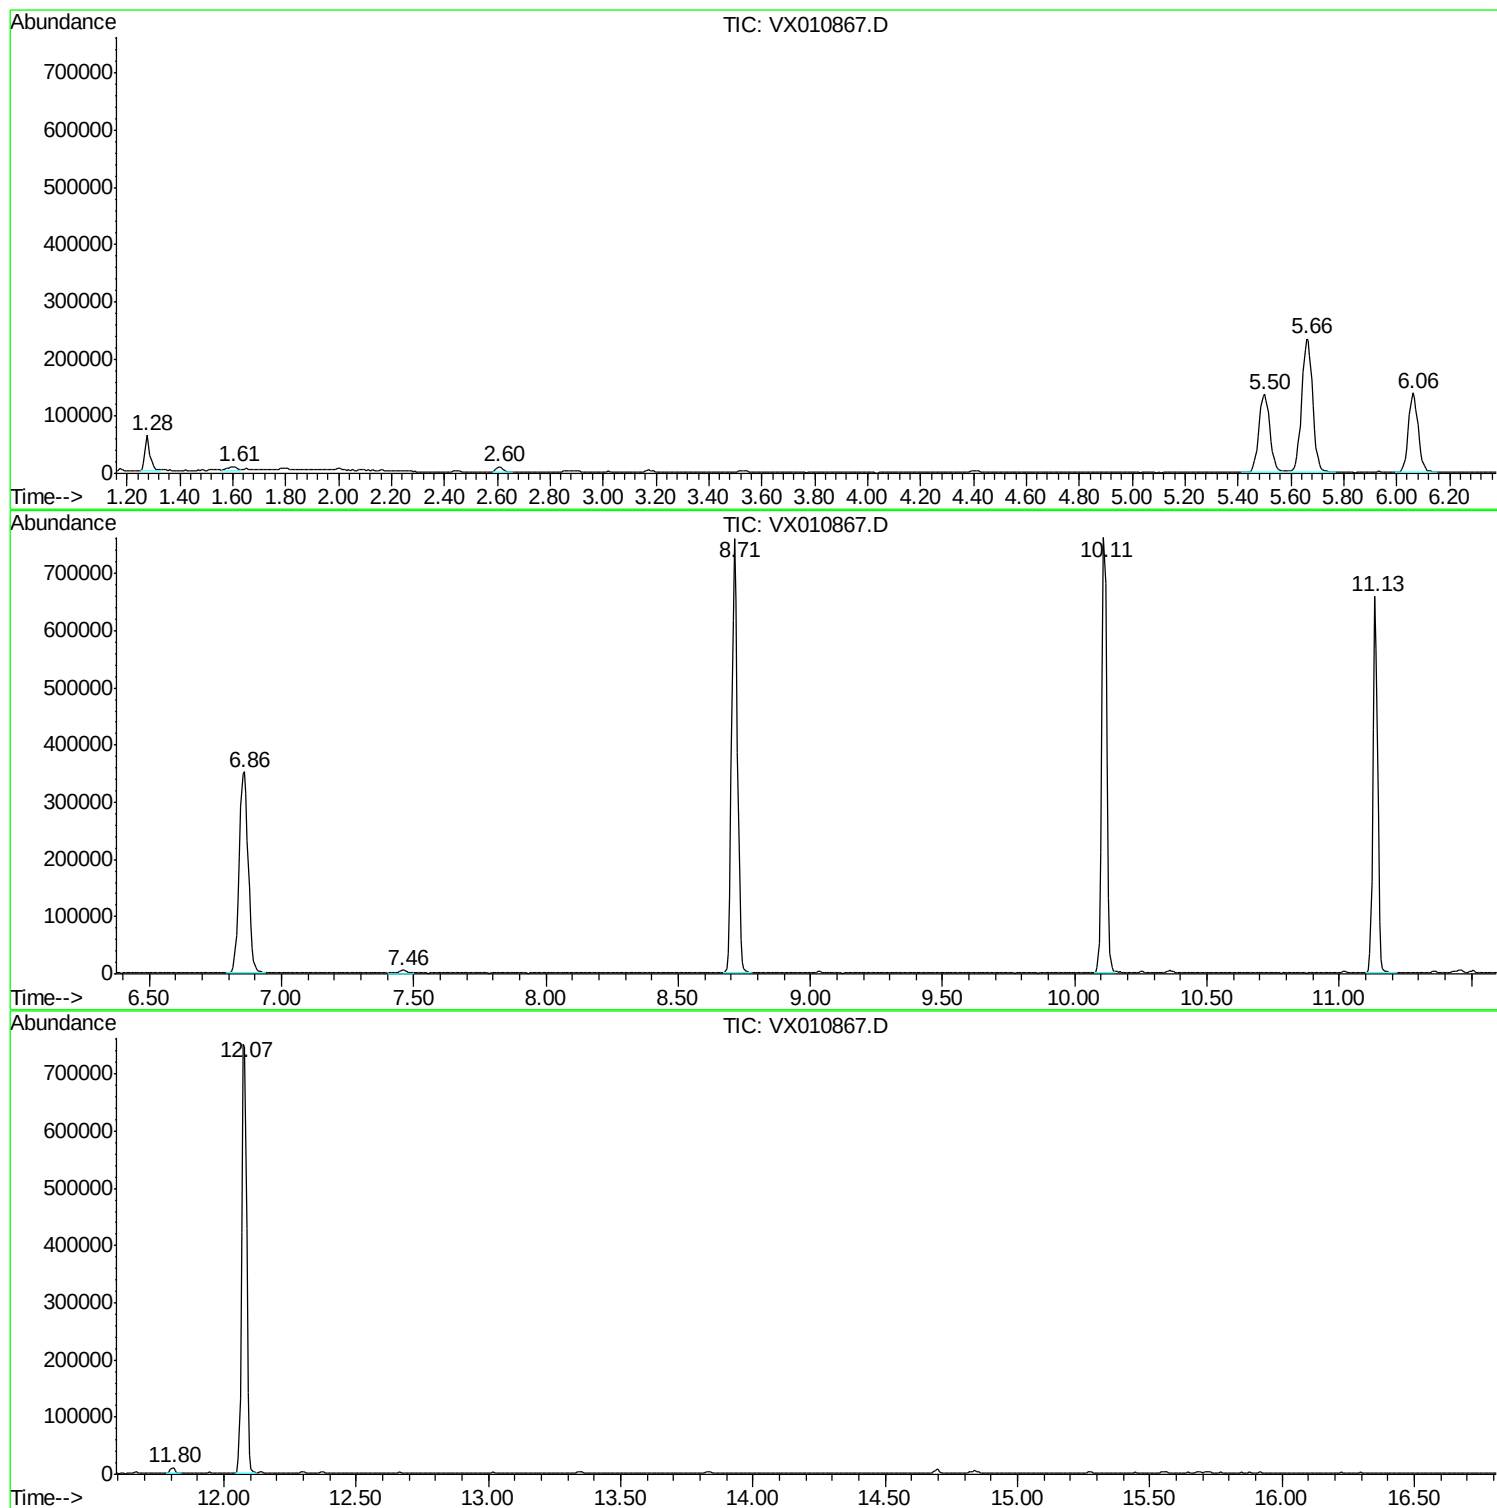

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX071219\
Data File : VX010867.D
Acq On : 13 Jul 2019 03:42
Operator : JC/SP
Sample : K3791-02
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FL-0600










Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X061919W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Sulfur dioxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.28	6.33 ug/l	84906	Pentafluorobenzene	5.67

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Sulfur dioxide	64	O2S	007446-09-5	90
2		Aminomethanesulfonic acid	111	CH5NO3S	013881-91-9	64
3		L-Alanine, 3-sulfo-	169	C3H7NO5S	000498-40-8	9
4		Ethyl Chloride	64	C2H5Cl	000075-00-3	3
5		Ethene, 1,1-difluoro-	64	C2H2F2	000075-38-7	3

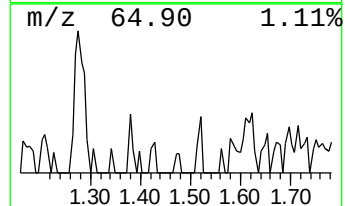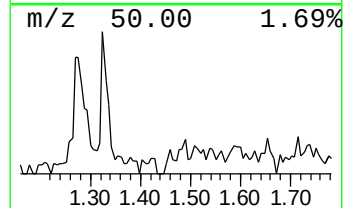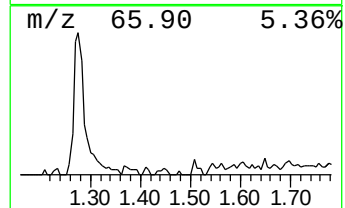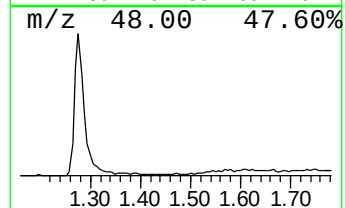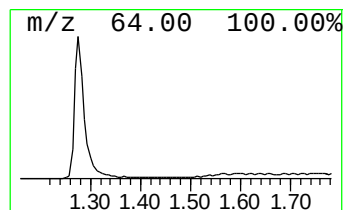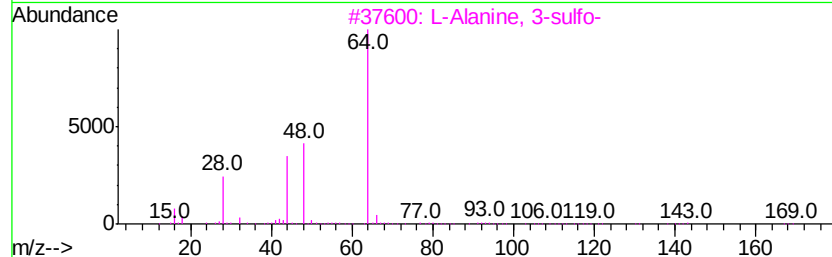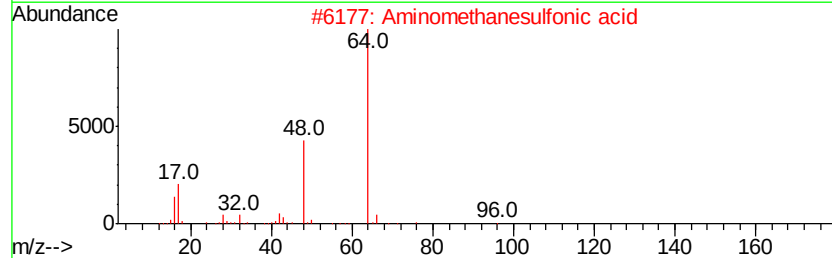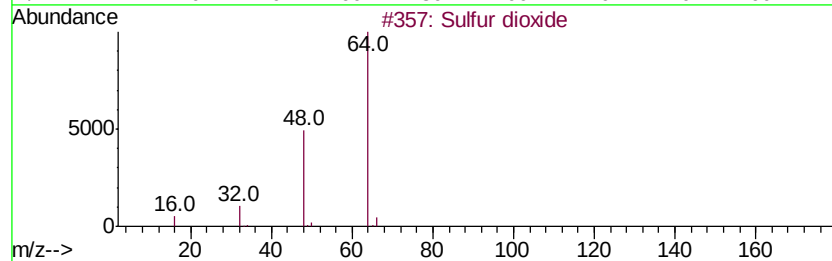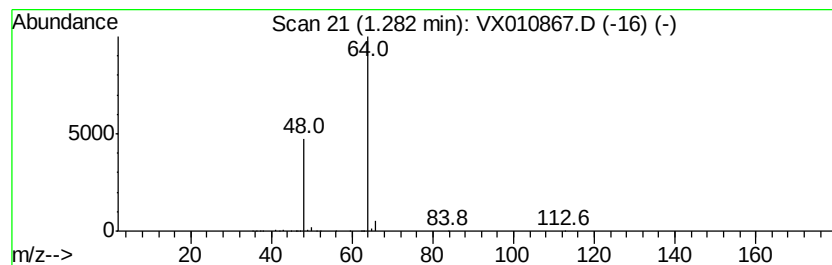

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX071219\
Data File : VX010867.D
Acq On : 13 Jul 2019 03:42
Operator : JC/SP
Sample : K3791-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FL-0600

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X061919W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Sulfur dioxide	1.28	6.3	ug/l	84906	1	5.67	670904	50.0