


Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX071219\
 Data File : VX010850.D
 Acq On : 12 Jul 2019 21:06
 Operator : JC/SP
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X061919W.M
 Title : SW846 8260
 Last Update : Thu Jun 20 03:31:56 2019

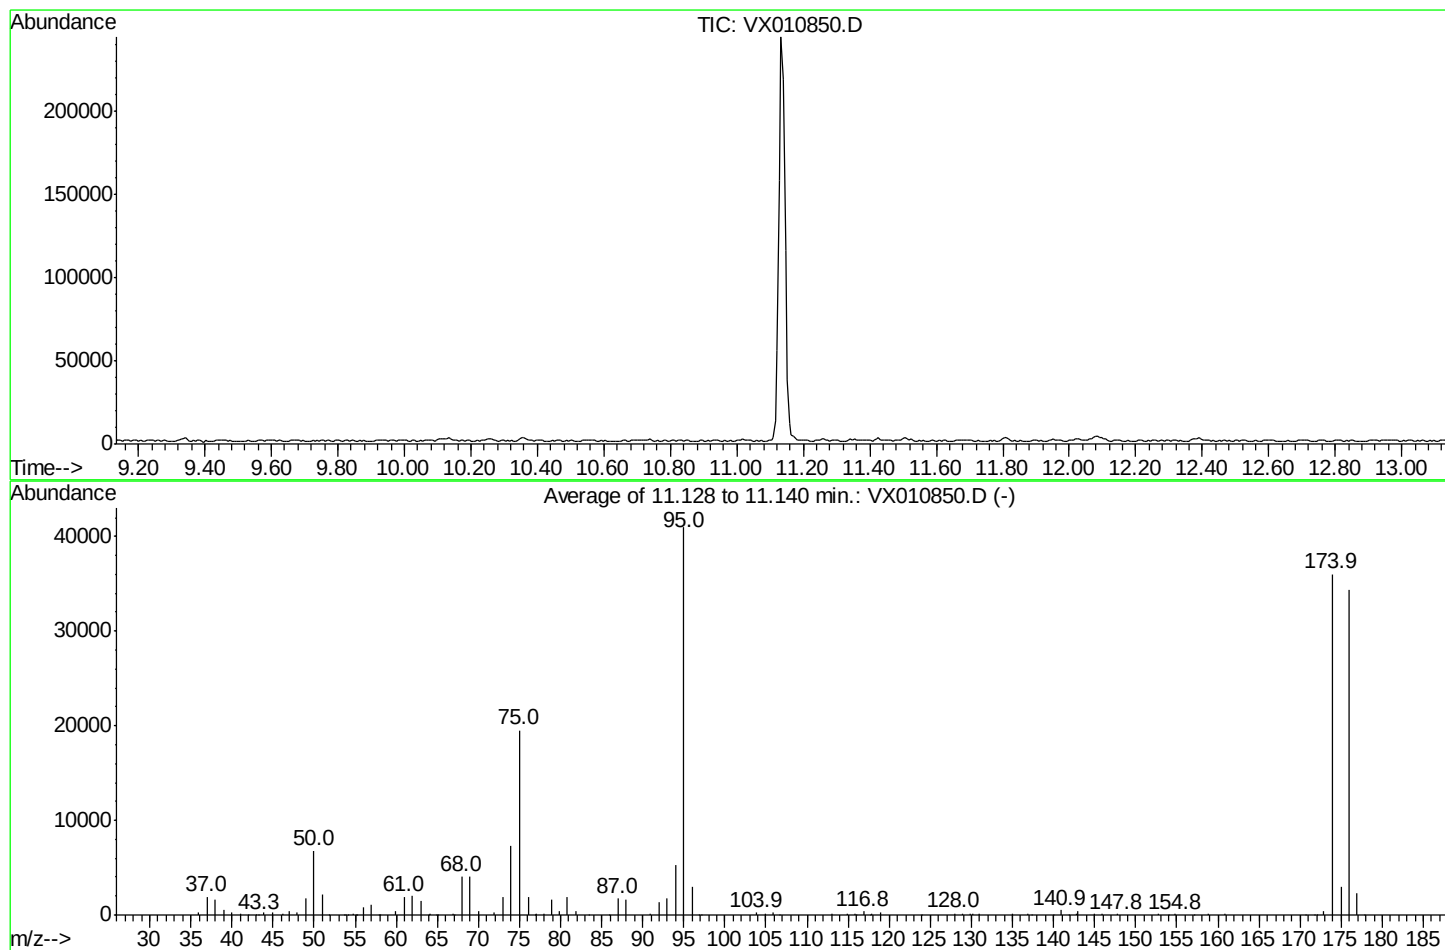

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1630

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.6	6811	PASS
75	95	30	60	47.6	19500	PASS
95	95	100	100	100.0	40970	PASS
96	95	5	9	7.2	2931	PASS
173	174	0.00	2	1.0	345	PASS
174	95	50	100	87.8	35986	PASS
175	174	5	9	8.1	2929	PASS
176	174	95	101	95.5	34384	PASS
177	176	5	9	6.7	2309	PASS