

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071221\
 Data File : VX023248.D
 Acq On : 12 Jul 2021 17:45
 Operator : JC/MD
 Sample : M3007-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 STORAGE-BLANK-SAMPLE-MANA

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X070221W.M

Title : SW846 8260

Signal : TIC: VX023248.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.252	24	27	34	rBV	132475	118156	10.18%	1.891%
2	2.550	234	240	247	rBV	13268	23121	1.99%	0.370%
3	2.953	298	306	315	rVB2	5188	12473	1.08%	0.200%
4	5.397	695	707	721	rBV	138474	398458	34.34%	6.377%
5	5.562	723	734	751	rVB	245030	690573	59.52%	11.052%
6	5.964	789	800	815	rBV	152189	402729	34.71%	6.445%
7	6.769	920	932	945	rBV	375074	876579	75.55%	14.028%
8	8.653	1234	1241	1250	rBV	752271	1160228	100.00%	18.568%
9	10.055	1465	1471	1489	rVB	706970	980713	84.53%	15.695%
10	11.085	1634	1640	1649	rBV	597293	743482	64.08%	11.898%
11	12.024	1789	1794	1802	rBV	686538	842132	72.58%	13.477%




Sum of corrected areas: 6248644

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071221\
Data File : VX023248.D
Acq On : 12 Jul 2021 17:45
Operator : JC/MD
Sample : M3007-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SAMPLE-MANA

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X070221W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

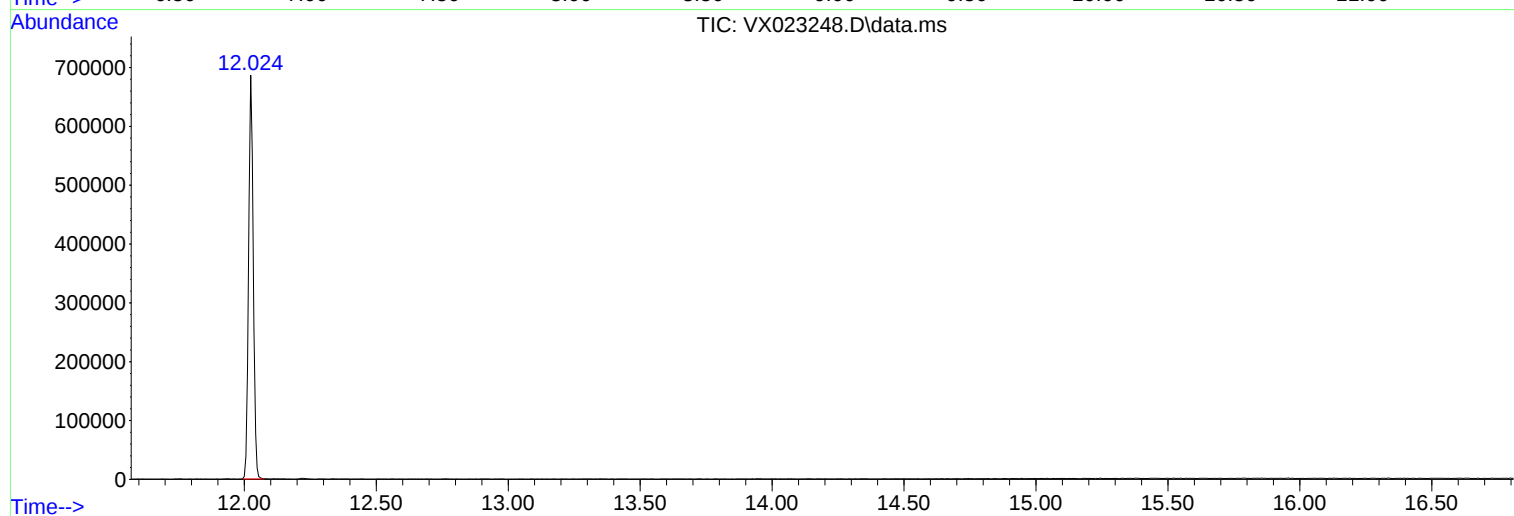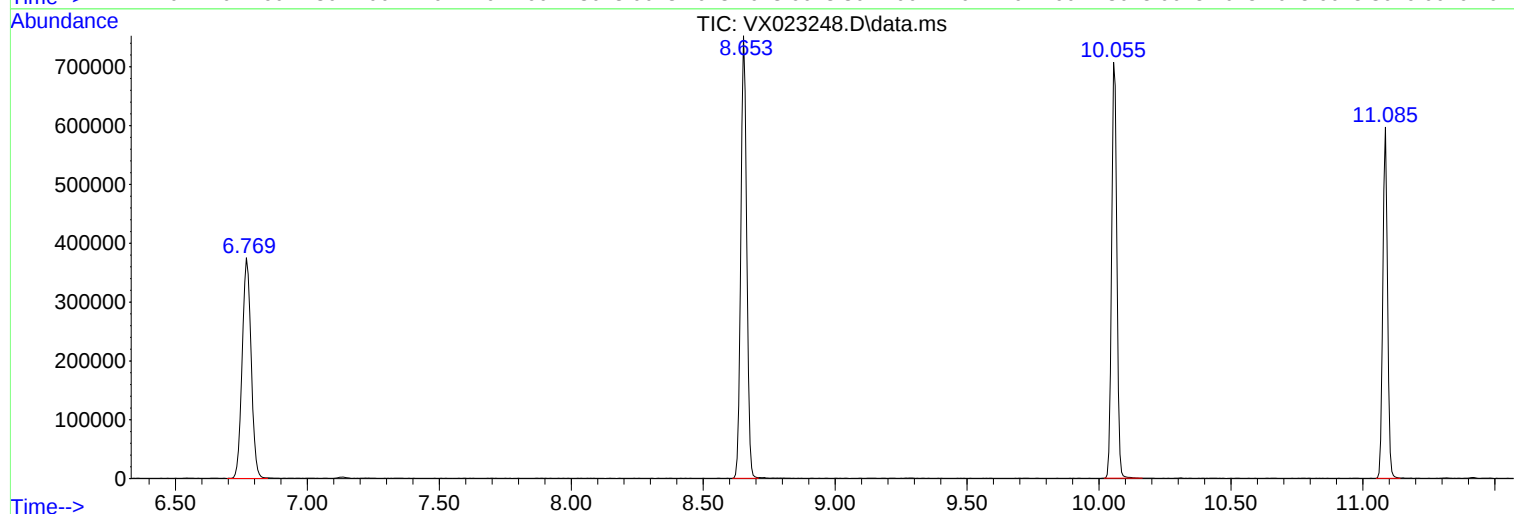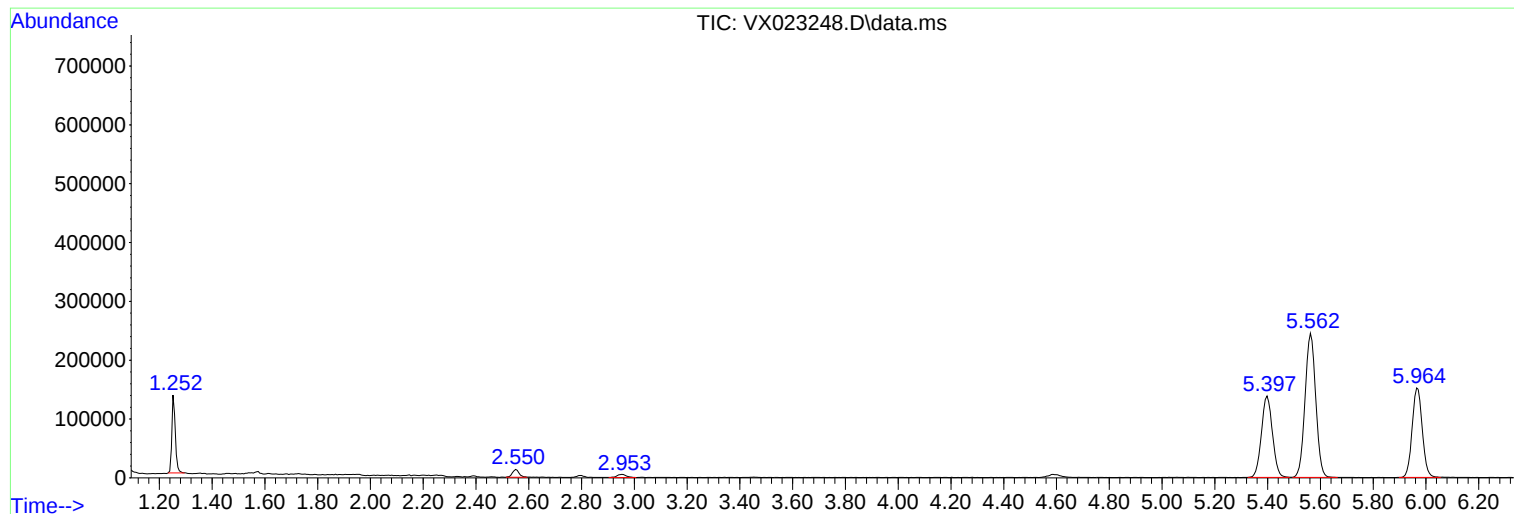

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071221\
Data File : VX023248.D
Acq On : 12 Jul 2021 17:45
Operator : JC/MD
Sample : M3007-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SAMPLE-MANA

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X070221W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071221\
Data File : VX023248.D
Acq On : 12 Jul 2021 17:45
Operator : JC/MD
Sample : M3007-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SAMPLE-MANA

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X070221W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
