
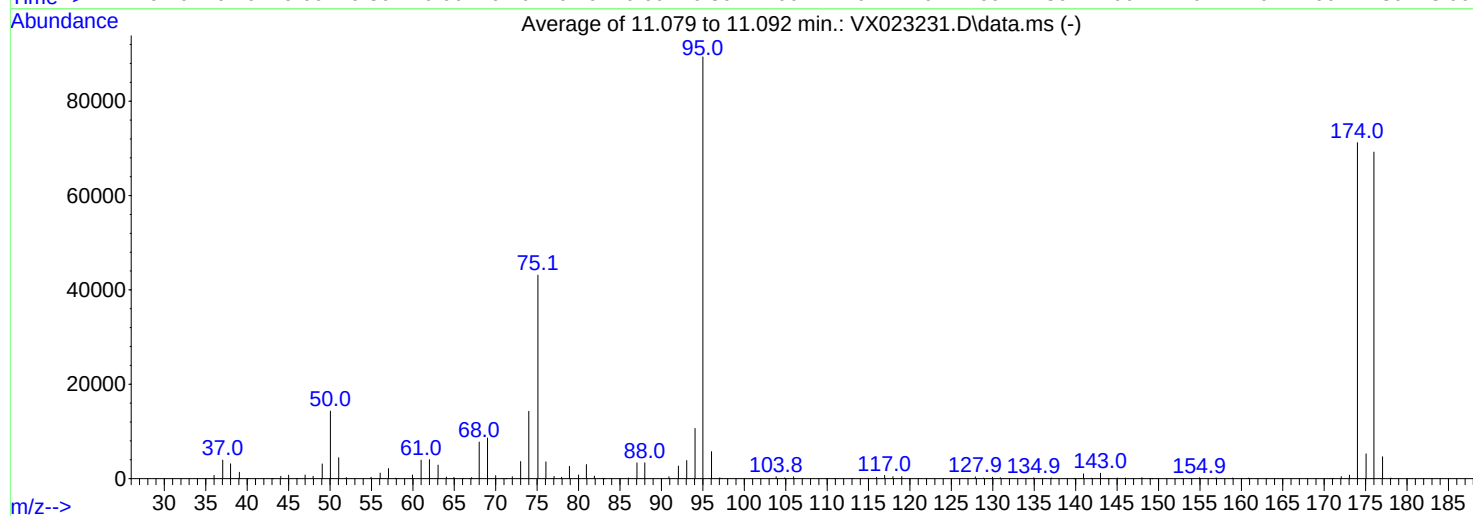


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071221\
Data File : VX023231.D
Acq On : 12 Jul 2021 08:43
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X070221W.M
Title : SW846 8260
Last Update : Fri Jul 02 14:29:42 2021

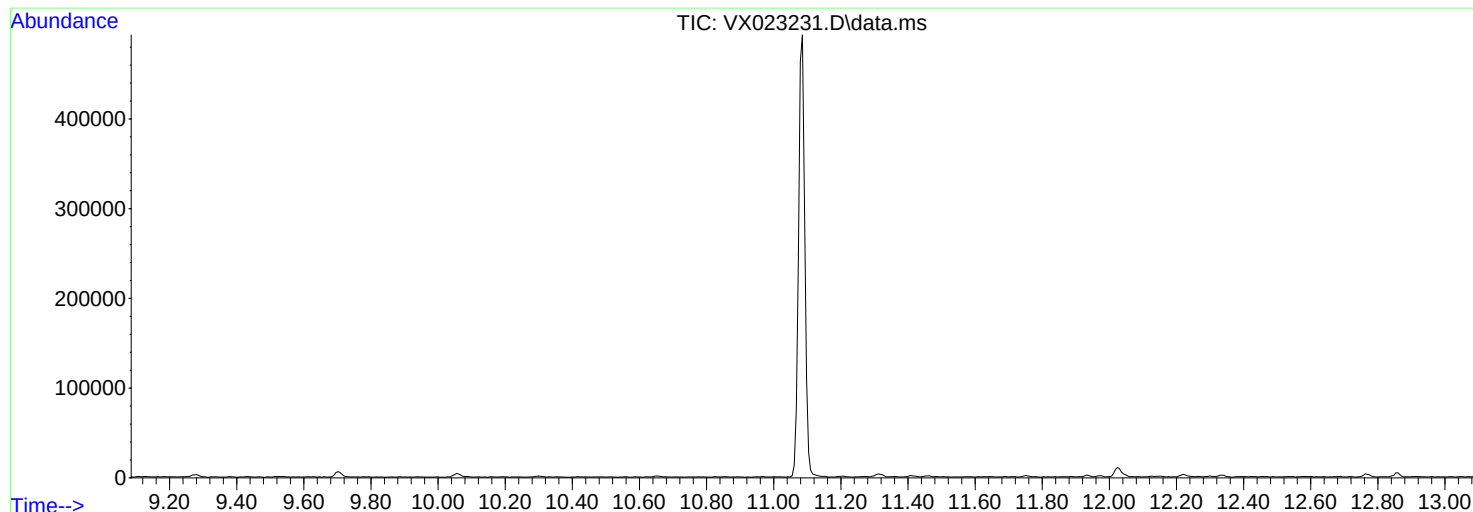

AutoFind: Scans 1639, 1640, 1641; Background Corrected with Scan 1632

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.0	14320	PASS
75	95	30	60	48.3	43149	PASS
95	95	100	100	100.0	89395	PASS
96	95	5	9	6.4	5735	PASS
173	174	0.00	2	1.1	759	PASS
174	95	50	100	79.7	71219	PASS
175	174	5	9	7.4	5248	PASS
176	174	95	101	97.2	69213	PASS
177	176	5	9	6.7	4657	PASS