

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071223\
 Data File : VX036511.D
 Acq On : 12 Jul 2023 12:38
 Operator : JC/MD
 Sample : VX0712MBL01
 Misc : 5.0g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK633

Quant Time: Jul 12 13:04:12 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML071223WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Jul 12 11:52:12 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.757	114	272709	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	248277	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	120307	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	105939	54.461	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery = 108.920%			
7) Chloroethane-d5	1.660	69	101288	47.392	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery = 94.780%			
11) 1,1-Dichloroethene-d2	2.306	65	44551	53.676	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 107.360%			
21) 2-Butanone-d5	4.452	46	152298	112.103	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery = 112.100%			
24) Chloroform-d	5.056	84	178317	50.479	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 100.960%			
26) 1,2-Dichloroethane-d4	5.952	65	130457	54.071	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 108.140%			
32) Benzene-d6	5.970	84	383348	54.539	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 109.080%			
36) 1,2-Dichloropropane-d6	7.306	67	124841	56.031	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery = 112.060%			
41) Toluene-d8	8.647	98	365193	54.425	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 108.860%			
43) trans-1,3-Dichloroprop...	8.952	79	55901	52.697	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 105.400%			
47) 2-Hexanone-d5	9.384	63	113475	115.794	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery = 115.790%			
56) 1,1,2,2-Tetrachloroeth...	11.189	84	164618	56.158	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery = 112.320%			
66) 1,2-Dichlorobenzene-d4	12.317	152	126553	55.374	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 110.740%			
Target Compounds					Qvalue	
25) Chloroform	5.093	83	9123	2.578	ug/L	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071223\
Data File : VX036511.D
Acq On : 12 Jul 2023 12:38
Operator : JC/MD
Sample : VX0712MBL01
Misc : 5.0g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK633

Quant Time: Jul 12 13:04:12 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML071223WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jul 12 11:52:12 2023
Response via : Initial Calibration

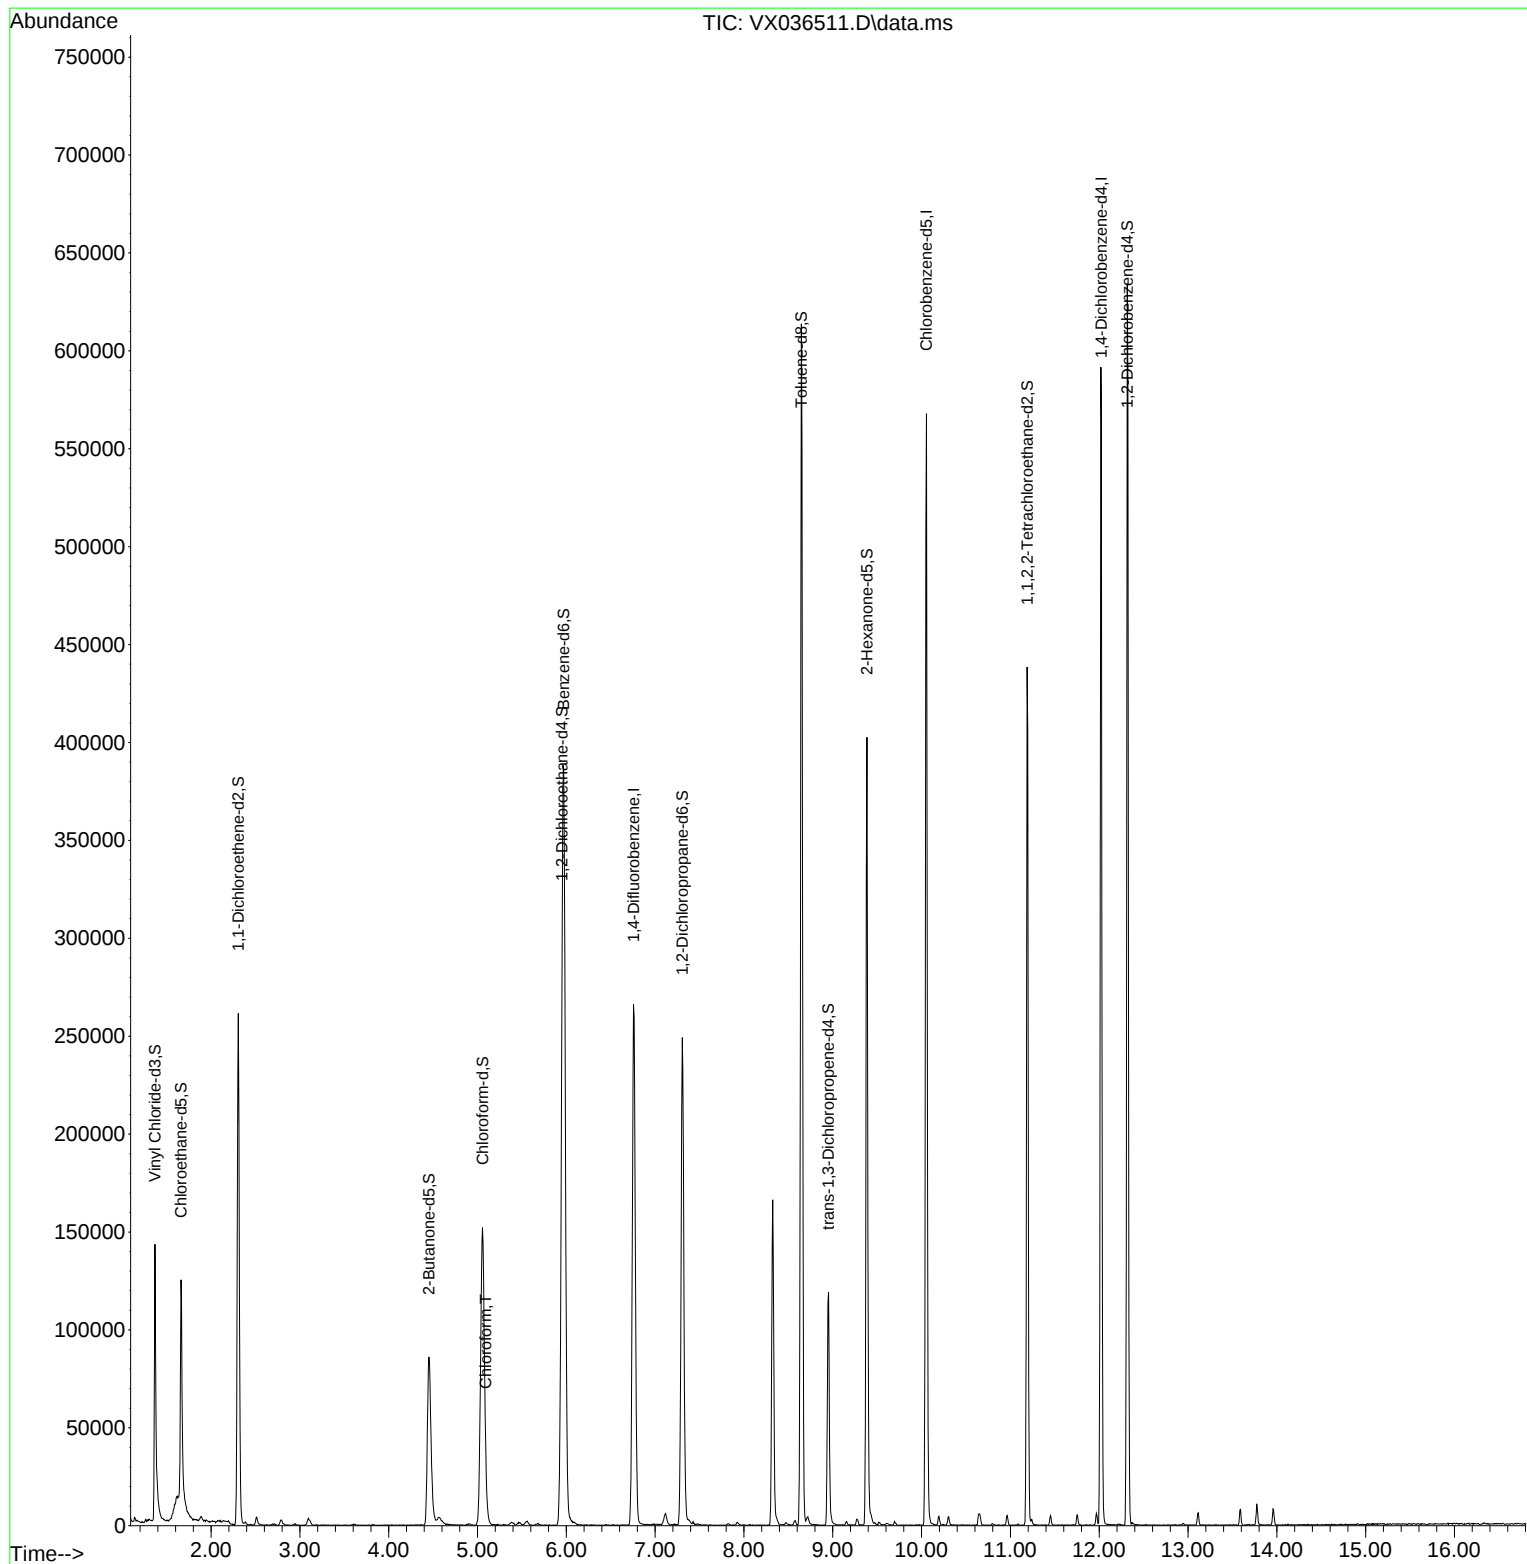

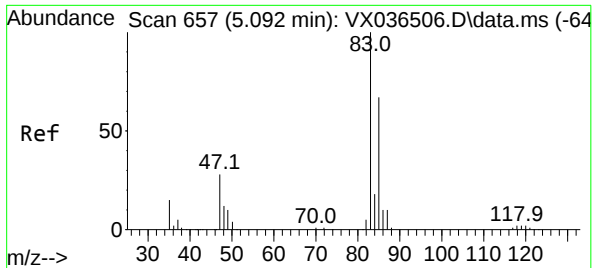

#25
 Chloroform
 Concen: 2.578 ug/L
 RT: 5.093 min Scan# 61
 Delta R.T. 0.000 min
 Lab File: VX036511.D
 Acq: 12 Jul 2023 12:38

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK633

Tgt Ion: 83 Resp: 9123
 Ion Ratio Lower Upper
 83 100
 85 75.2 46.8 87.0

