

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071223\
 Data File : VX036511.D
 Acq On : 12 Jul 2023 12:38
 Operator : JC/MD
 Sample : VX0712MBL01
 Misc : 5.0g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK633

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML071223WMA.M
 Title : VOC Analysis

Signal : TIC: VX036505.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.136	6	8	11	rBV2	1993	1899	0.16%	0.021%
2	1.368	42	46	59	rBV	140866	176962	15.15%	1.983%
3	1.660	91	94	116	rVB	122707	203547	17.43%	2.281%
4	2.306	193	200	209	rBV	261313	408950	35.02%	4.583%
5	2.514	226	234	238	rBV	4197	7089	0.61%	0.079%
6	2.630	251	253	256	rVB	370	404	0.03%	0.005%
7	2.690	261	263	265	rBV2	556	550	0.05%	0.006%
8	2.788	273	279	282	rBV4	2775	5067	0.43%	0.057%
9	2.861	289	291	294	rBV2	269	294	0.03%	0.003%
10	2.916	297	300	301	rBV	315	326	0.03%	0.004%
11	2.940	302	304	310	rVV2	782	1114	0.10%	0.012%
12	3.093	324	329	340	rVV5	3463	8139	0.70%	0.091%
13	3.605	407	413	414	rBV2	589	885	0.08%	0.010%
14	3.824	446	449	454	rBV2	425	654	0.06%	0.007%
15	4.172	504	506	509	rVB	295	264	0.02%	0.003%
16	4.251	517	519	522	rVB2	301	247	0.02%	0.003%
17	4.452	543	552	565	rBV2	85819	247667	21.21%	2.776%
18	4.824	610	613	616	rBV2	238	286	0.02%	0.003%
19	4.885	620	623	624	rBV2	542	629	0.05%	0.007%
20	5.056	638	651	669	rBV	151980	479035	41.02%	5.369%
21	5.221	676	678	679	rBV	502	342	0.03%	0.004%
22	5.294	689	690	692	rVB	438	298	0.03%	0.003%
23	5.318	692	694	697	rBV3	218	263	0.02%	0.003%
24	5.379	699	704	708	rBV6	1336	2913	0.25%	0.033%
25	5.458	712	717	718	rBV	1404	1512	0.13%	0.017%
26	5.562	726	734	740	rVB3	1946	4694	0.40%	0.053%
27	5.684	744	754	755	rBV4	944	1905	0.16%	0.021%
28	5.964	788	800	817	rBV2	387926	1167691	100.00%	13.087%
29	6.159	831	832	836	rVB2	361	352	0.03%	0.004%
30	6.226	841	843	847	rVV	343	294	0.03%	0.003%
31	6.318	857	858	863	rVB2	219	233	0.02%	0.003%
32	6.452	876	880	881	rBV3	331	427	0.04%	0.005%
33	6.525	890	892	893	rBV	375	305	0.03%	0.003%
34	6.757	921	930	950	rBV	265904	636601	54.52%	7.135%
35	7.117	982	989	998	rVB5	5959	14316	1.23%	0.160%
36	7.190	998	1001	1002	rBV2	397	427	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071223\
 Data File : VX036511.D
 Acq On : 12 Jul 2023 12:38
 Operator : JC/MD
 Sample : VX0712MBL01
 Misc : 5.0g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK633

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML071223WMA.M
 Title : VOC Analysis

37	7.214	1003	1005	1006	rVB2	612	350	0.03%	0.004%
38	7.232	1006	1008	1009	rBV2	384	268	0.02%	0.003%
39	7.306	1012	1020	1038	rVV	248812	536410	45.94%	6.012%
40	7.427	1038	1040	1043	rVB4	1432	1288	0.11%	0.014%
41	7.623	1070	1072	1077	rBV2	330	462	0.04%	0.005%
42	7.824	1101	1105	1109	rVV2	688	1122	0.10%	0.013%
43	7.891	1114	1116	1117	rBV2	264	233	0.02%	0.003%
44	7.927	1117	1122	1126	rBV3	1466	2440	0.21%	0.027%
45	8.068	1142	1145	1148	rBV	516	479	0.04%	0.005%
46	8.324	1180	1187	1204	rBV	166135	276702	23.70%	3.101%
47	8.470	1208	1211	1219	rVB3	1201	2165	0.19%	0.024%
48	8.574	1222	1228	1233	rBV2	2299	3757	0.32%	0.042%
49	8.647	1233	1240	1248	rBV	613458	949490	81.31%	10.642%
50	8.952	1283	1290	1305	rVV	119115	185849	15.92%	2.083%
51	9.067	1307	1309	1314	rBV3	262	518	0.04%	0.006%
52	9.153	1319	1323	1328	rVB4	1932	2643	0.23%	0.030%
53	9.275	1339	1343	1347	rVB5	3085	4939	0.42%	0.055%
54	9.311	1347	1349	1350	rBV	298	262	0.02%	0.003%
55	9.384	1355	1361	1374	rBV	402212	552818	47.34%	6.196%
56	9.519	1381	1383	1393	rVB5	1371	1985	0.17%	0.022%
57	9.695	1408	1412	1418	rVB3	1991	2615	0.22%	0.029%
58	10.055	1465	1471	1481	rBV	567430	767829	65.76%	8.606%
59	10.195	1490	1494	1499	rVB	4387	5696	0.49%	0.064%
60	10.244	1499	1502	1508	rVB2	384	478	0.04%	0.005%
61	10.305	1508	1512	1516	rBV2	4243	5911	0.51%	0.066%
62	10.500	1541	1544	1546	rBV2	220	278	0.02%	0.003%
63	10.598	1554	1560	1561	rBV2	255	367	0.03%	0.004%
64	10.652	1564	1569	1575	rVB3	5757	11327	0.97%	0.127%
65	10.799	1589	1593	1597	rVV3	790	1182	0.10%	0.013%
66	10.872	1601	1605	1610	rBV2	247	382	0.03%	0.004%
67	10.963	1615	1620	1626	rBV	4989	6651	0.57%	0.075%
68	11.085	1637	1640	1643	rBV2	639	652	0.06%	0.007%
69	11.189	1652	1657	1664	rBV	438001	569209	48.75%	6.380%
70	11.390	1689	1690	1694	rVB	282	252	0.02%	0.003%
71	11.451	1696	1700	1705	rVB2	4909	6355	0.54%	0.071%
72	11.616	1726	1727	1730	rBV	272	277	0.02%	0.003%
73	11.713	1740	1743	1745	rVV2	325	316	0.03%	0.004%
74	11.750	1745	1749	1755	rVV	5288	6625	0.57%	0.074%
75	11.847	1762	1765	1766	rBV	276	244	0.02%	0.003%
76	11.969	1779	1785	1788	rBV	5944	7592	0.65%	0.085%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071223\
 Data File : VX036511.D
 Acq On : 12 Jul 2023 12:38
 Operator : JC/MD
 Sample : VX0712MBL01
 Misc : 5.0g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK633

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML071223WMA.M
 Title : VOC Analysis

77	12.018	1788	1793	1803	rVB	590983	754333	64.60%	8.455%
78	12.317	1837	1842	1849	rBV	633936	821843	70.38%	9.211%
79	12.762	1912	1915	1917	rBV	271	319	0.03%	0.004%
80	12.859	1929	1931	1933	rVB	406	341	0.03%	0.004%
81	12.945	1939	1945	1949	rBV3	914	1586	0.14%	0.018%
82	13.115	1968	1973	1979	rBV2	6259	8261	0.71%	0.093%
83	13.195	1983	1986	1987	rBV	301	303	0.03%	0.003%
84	13.475	2030	2032	2036	rVB2	371	354	0.03%	0.004%
85	13.591	2046	2051	2056	rVB	8097	10502	0.90%	0.118%
86	13.664	2062	2063	2065	rBV	271	271	0.02%	0.003%
87	13.774	2077	2081	2086	rBV	10768	12897	1.10%	0.145%
88	13.957	2107	2111	2117	rBV	8250	11228	0.96%	0.126%
89	14.127	2137	2139	2144	rVB	530	599	0.05%	0.007%
90	14.164	2144	2145	2148	rBV	349	288	0.02%	0.003%
91	14.243	2155	2158	2159	rBV2	254	240	0.02%	0.003%
92	14.347	2172	2175	2176	rBV2	447	402	0.03%	0.005%
93	14.457	2191	2193	2195	rVB	405	318	0.03%	0.004%
94	14.646	2222	2224	2226	rBV2	454	361	0.03%	0.004%
95	15.024	2284	2286	2287	rVB2	496	280	0.02%	0.003%
96	15.042	2287	2289	2294	rBV3	397	614	0.05%	0.007%
97	15.164	2307	2309	2310	rBV2	495	325	0.03%	0.004%
98	15.542	2368	2371	2372	rBV	633	602	0.05%	0.007%
99	15.719	2396	2400	2401	rBV3	451	591	0.05%	0.007%
100	15.926	2432	2434	2435	rVB2	696	366	0.03%	0.004%




Sum of corrected areas: 8922223

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071223\
Data File : VX036511.D
Acq On : 12 Jul 2023 12:38
Operator : JC/MD
Sample : VX0712MBL01
Misc : 5.0g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK633

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML071223WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

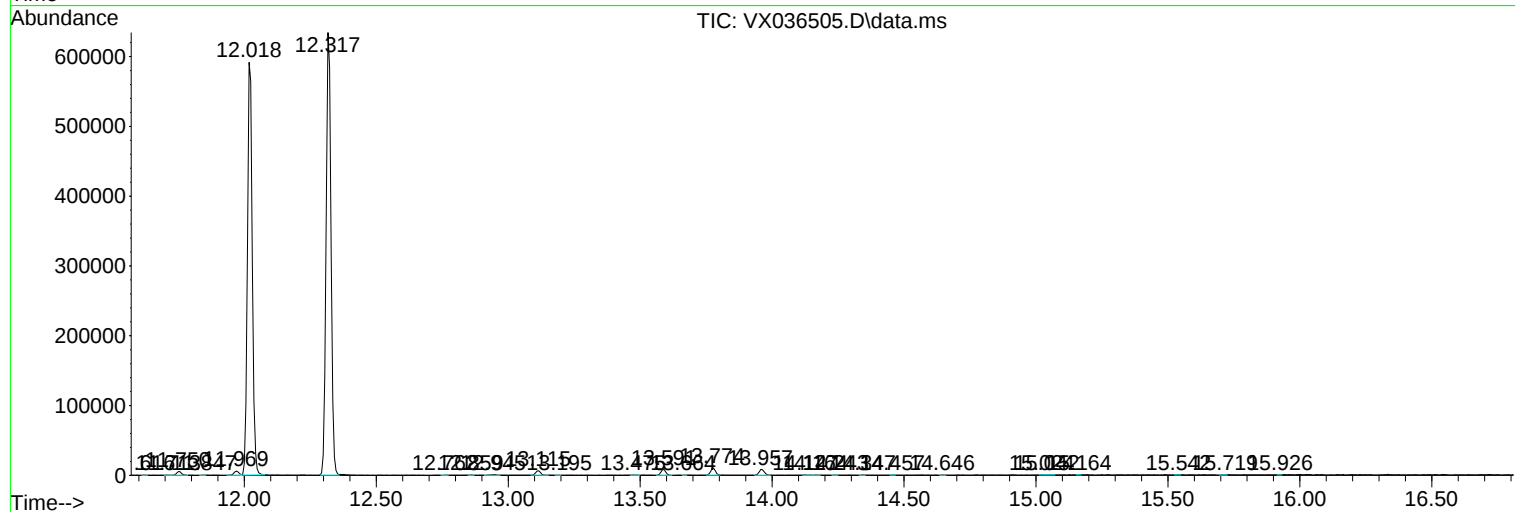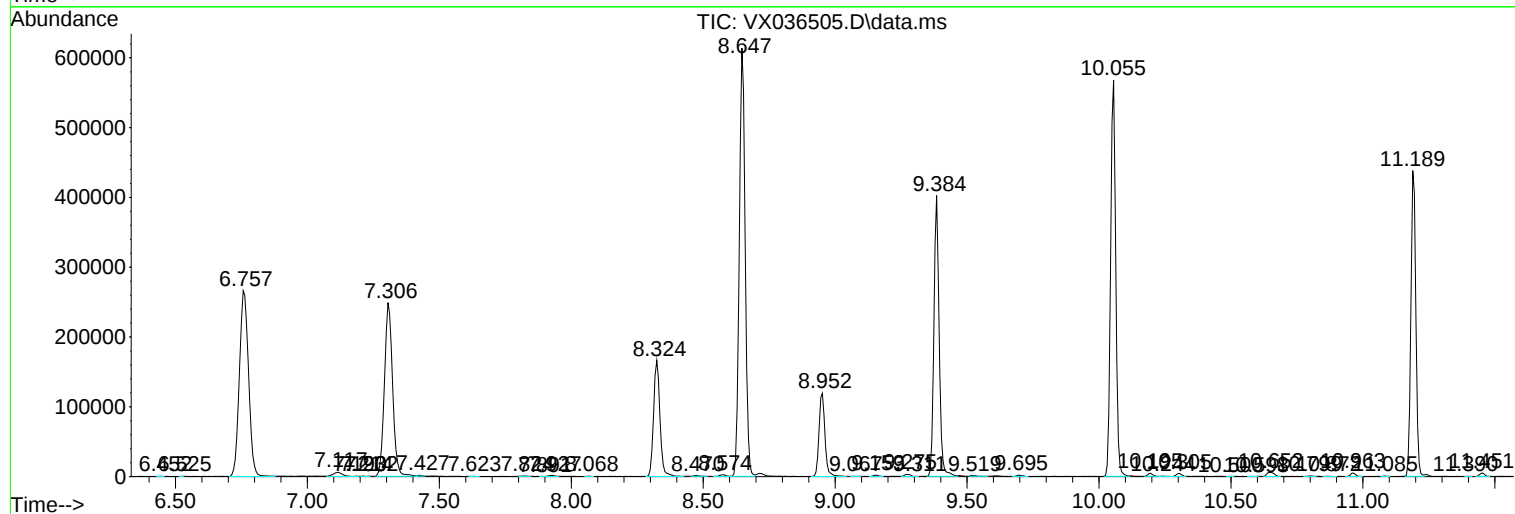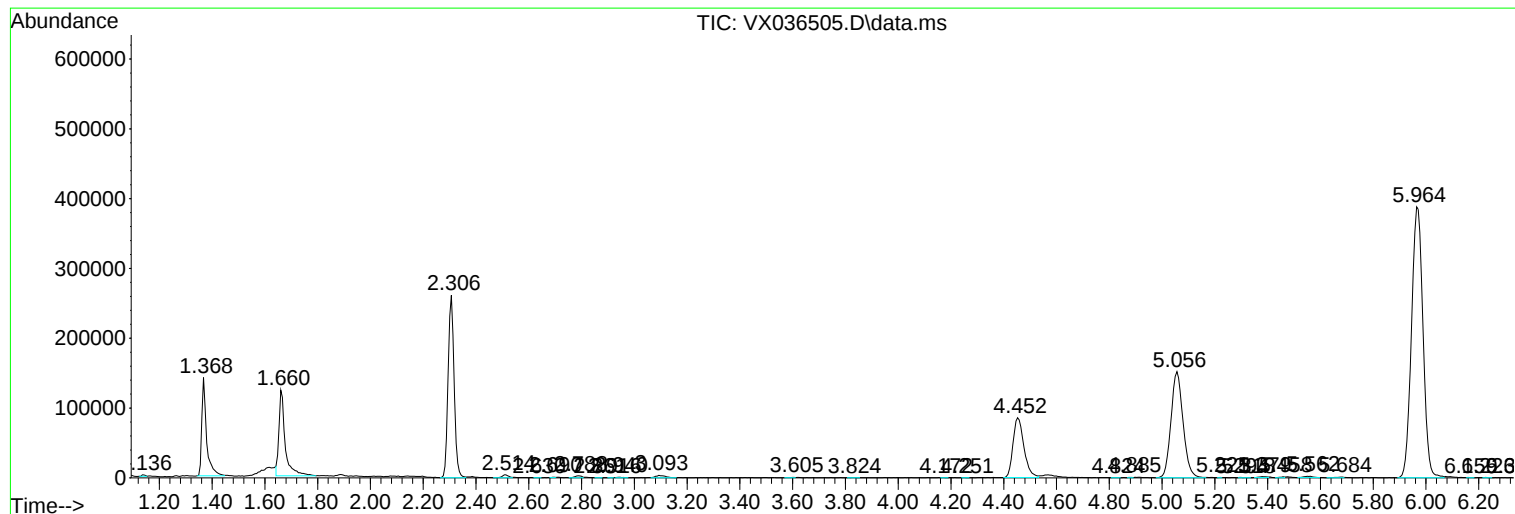

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071223\
Data File : VX036511.D
Acq On : 12 Jul 2023 12:38
Operator : JC/MD
Sample : VX0712MBL01
Misc : 5.0g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK633

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML071223WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071223\
Data File : VX036511.D
Acq On : 12 Jul 2023 12:38
Operator : JC/MD
Sample : VX0712MBL01
Misc : 5.0g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK633

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML071223WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc