

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071223\
 Data File : VX036512.D
 Acq On : 12 Jul 2023 13:01
 Operator : JC/MD
 Sample : VX0712WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK634

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML071223WMA.M
 Title : VOC Analysis

Signal : TIC: VX036506.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.142	7	9	11	rVB	2330	1635	0.14%	0.019%
2	1.264	26	29	31	rBV3	2093	2431	0.21%	0.028%
3	1.368	42	46	60	rBV	121953	155792	13.67%	1.805%
4	1.666	91	95	117	rVB	109783	187245	16.43%	2.169%
5	2.306	194	200	211	rBV	231169	355642	31.21%	4.119%
6	2.514	229	234	239	rBV2	2702	4974	0.44%	0.058%
7	2.611	247	250	253	rVB2	313	419	0.04%	0.005%
8	2.709	263	266	268	rVB2	539	633	0.06%	0.007%
9	2.794	273	280	290	rBV4	2761	5975	0.52%	0.069%
10	2.934	299	303	306	rBV	361	551	0.05%	0.006%
11	3.044	320	321	324	rBV2	222	252	0.02%	0.003%
12	3.093	324	329	330	rBV3	1848	2483	0.22%	0.029%
13	3.251	352	355	358	rBV	227	268	0.02%	0.003%
14	3.331	365	368	371	rVB	217	299	0.03%	0.003%
15	3.428	381	384	389	rBV2	150	342	0.03%	0.004%
16	3.526	398	400	403	rBV	323	290	0.03%	0.003%
17	3.611	410	414	417	rBV2	570	961	0.08%	0.011%
18	3.831	447	450	451	rBV	368	271	0.02%	0.003%
19	4.227	511	515	518	rBV2	250	350	0.03%	0.004%
20	4.343	532	534	537	rBV2	217	275	0.02%	0.003%
21	4.458	542	553	566	rBV	87468	256842	22.54%	2.975%
22	4.885	622	623	624	rBV	345	244	0.02%	0.003%
23	5.056	639	651	669	rBV	147927	467919	41.06%	5.420%
24	5.391	700	706	712	rVB5	1460	3523	0.31%	0.041%
25	5.477	712	720	725	rBV5	1020	2785	0.24%	0.032%
26	5.544	727	731	733	rBV3	1425	2150	0.19%	0.025%
27	5.678	746	753	754	rBV2	1072	1084	0.10%	0.013%
28	5.970	787	801	818	rBV2	382343	1139523	100.00%	13.199%
29	6.287	851	853	856	rVB	314	266	0.02%	0.003%
30	6.464	877	882	886	rVB2	327	534	0.05%	0.006%
31	6.525	890	892	894	rBV2	214	263	0.02%	0.003%
32	6.763	921	931	942	rBV	264030	623082	54.68%	7.217%
33	7.049	975	978	981	rBV4	383	587	0.05%	0.007%
34	7.116	981	989	996	rVV5	5705	12731	1.12%	0.147%
35	7.312	1012	1021	1031	rBV	239630	524067	45.99%	6.070%
36	7.830	1100	1106	1110	rVB2	774	1357	0.12%	0.016%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071223\
 Data File : VX036512.D
 Acq On : 12 Jul 2023 13:01
 Operator : JC/MD
 Sample : VX0712WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK634

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML071223WMA.M
 Title : VOC Analysis

37	7.927	1118	1122	1128	rVV3	1556	2986	0.26%	0.035%
38	8.000	1132	1134	1139	rBV2	204	420	0.04%	0.005%
39	8.202	1163	1167	1171	rVB2	198	341	0.03%	0.004%
40	8.324	1181	1187	1200	rBV	165189	272121	23.88%	3.152%
41	8.476	1210	1212	1215	rVB2	979	916	0.08%	0.011%
42	8.574	1225	1228	1233	rBV3	2303	3361	0.29%	0.039%
43	8.647	1233	1240	1249	rVV	562060	897274	78.74%	10.393%
44	8.714	1249	1251	1262	rVB3	4359	7265	0.64%	0.084%
45	8.830	1267	1270	1271	rBV2	508	487	0.04%	0.006%
46	8.878	1276	1278	1281	rVB2	279	268	0.02%	0.003%
47	8.952	1284	1290	1302	rBV	123276	183078	16.07%	2.121%
48	9.055	1305	1307	1310	rVB	336	301	0.03%	0.003%
49	9.153	1320	1323	1328	rVB	1504	1746	0.15%	0.020%
50	9.275	1339	1343	1347	rVB4	3216	4821	0.42%	0.056%
51	9.384	1355	1361	1378	rBV	407747	567329	49.79%	6.571%
52	9.579	1389	1393	1395	rBV3	391	588	0.05%	0.007%
53	9.701	1409	1413	1418	rVB3	1702	2145	0.19%	0.025%
54	10.055	1465	1471	1485	rBV	581790	774305	67.95%	8.969%
55	10.195	1490	1494	1502	rVB	4290	5712	0.50%	0.066%
56	10.305	1508	1512	1517	rVB2	4308	5954	0.52%	0.069%
57	10.463	1536	1538	1544	rVB2	226	259	0.02%	0.003%
58	10.640	1563	1567	1569	rBV2	4414	6083	0.53%	0.070%
59	10.787	1589	1591	1592	rBV	420	325	0.03%	0.004%
60	10.963	1616	1620	1628	rVV	4535	5813	0.51%	0.067%
61	11.091	1637	1641	1646	rVB4	1010	1439	0.13%	0.017%
62	11.189	1652	1657	1665	rBV	435707	570571	50.07%	6.609%
63	11.305	1674	1676	1678	rBV	605	442	0.04%	0.005%
64	11.451	1696	1700	1706	rVB2	5728	6736	0.59%	0.078%
65	11.561	1715	1718	1720	rBV2	276	288	0.03%	0.003%
66	11.634	1727	1730	1731	rBV	391	245	0.02%	0.003%
67	11.707	1740	1742	1745	rVB	553	444	0.04%	0.005%
68	11.756	1745	1750	1754	rBV	5175	6434	0.56%	0.075%
69	11.902	1770	1774	1776	rBV2	334	384	0.03%	0.004%
70	11.933	1776	1779	1780	rVV	283	256	0.02%	0.003%
71	11.969	1780	1785	1788	rVV	5843	7069	0.62%	0.082%
72	12.024	1788	1794	1804	rVB	562623	721507	63.32%	8.357%
73	12.219	1824	1826	1828	rBV	683	483	0.04%	0.006%
74	12.317	1837	1842	1851	rBV	605012	773435	67.87%	8.959%
75	12.433	1858	1861	1862	rVB2	368	241	0.02%	0.003%
76	12.939	1942	1944	1948	rVB	512	549	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071223\
 Data File : VX036512.D
 Acq On : 12 Jul 2023 13:01
 Operator : JC/MD
 Sample : VX0712WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK634

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML071223WMA.M
 Title : VOC Analysis

77	13.109	1968	1972	1979	rBV	8012	9156	0.80%	0.106%
78	13.207	1986	1988	1990	rBV	231	242	0.02%	0.003%
79	13.298	1999	2003	2004	rVB2	289	290	0.03%	0.003%
80	13.378	2014	2016	2019	rBV2	259	318	0.03%	0.004%
81	13.426	2022	2024	2027	rVB2	310	292	0.03%	0.003%
82	13.585	2046	2050	2056	rVB4	6995	9161	0.80%	0.106%
83	13.688	2063	2067	2074	rBV2	438	827	0.07%	0.010%
84	13.780	2078	2082	2086	rVV3	5237	7200	0.63%	0.083%
85	13.914	2102	2104	2106	rVB	366	254	0.02%	0.003%
86	13.963	2108	2112	2117	rVB3	5568	7660	0.67%	0.089%
87	14.012	2118	2120	2123	rVB2	329	253	0.02%	0.003%
88	14.036	2123	2124	2126	rBV	371	256	0.02%	0.003%
89	14.066	2126	2129	2132	rVB2	322	346	0.03%	0.004%
90	14.158	2142	2144	2149	rVB2	439	524	0.05%	0.006%
91	14.207	2149	2152	2156	rBV3	360	699	0.06%	0.008%
92	14.304	2165	2168	2172	rBV2	257	411	0.04%	0.005%
93	14.341	2172	2174	2177	rVV3	312	297	0.03%	0.003%
94	14.810	2249	2251	2252	rBV2	452	290	0.03%	0.003%
95	15.139	2303	2305	2306	rBV2	435	345	0.03%	0.004%
96	15.962	2438	2440	2441	rBV2	560	302	0.03%	0.003%
97	16.023	2448	2450	2452	rBV2	438	427	0.04%	0.005%
98	16.084	2458	2460	2461	rBV	461	248	0.02%	0.003%
99	16.182	2473	2476	2478	rBV3	689	545	0.05%	0.006%
100	16.511	2528	2530	2531	rBV2	539	393	0.03%	0.005%




Sum of corrected areas: 8633202

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071223\
Data File : VX036512.D
Acq On : 12 Jul 2023 13:01
Operator : JC/MD
Sample : VX0712WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK634

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML071223WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

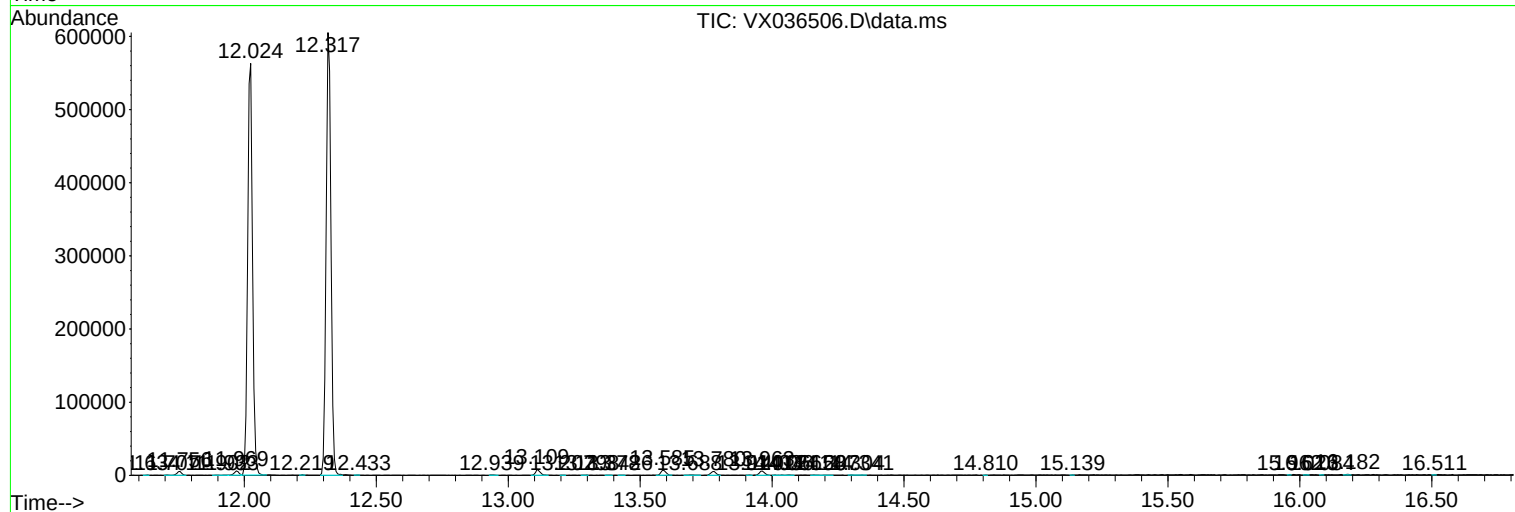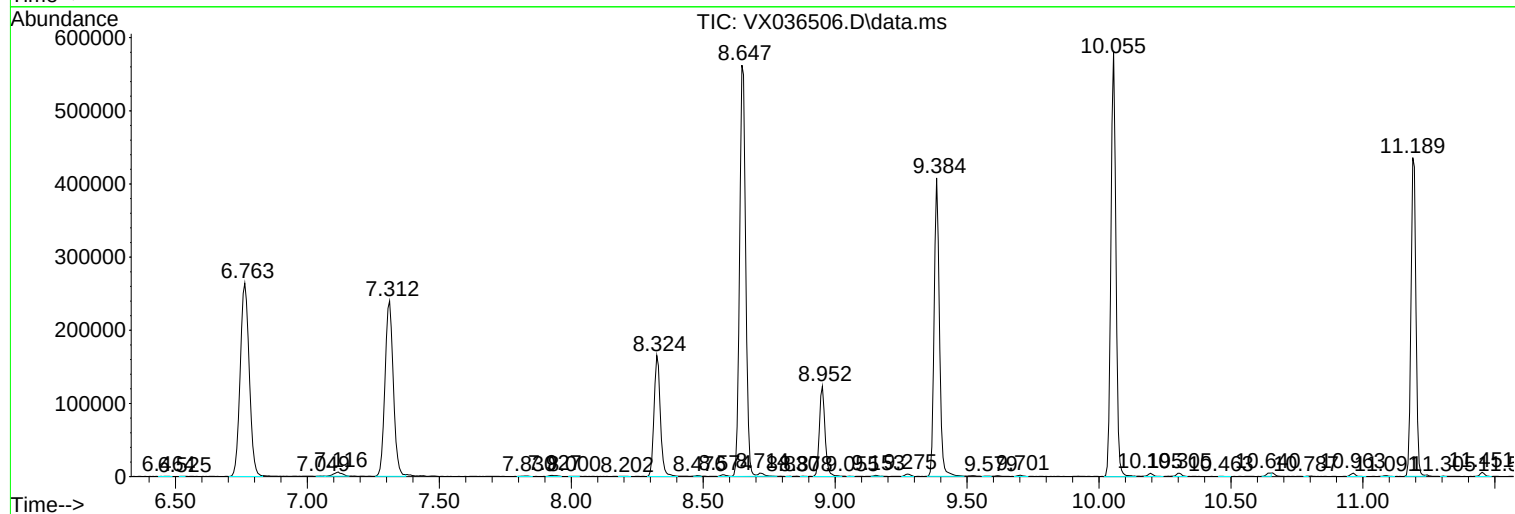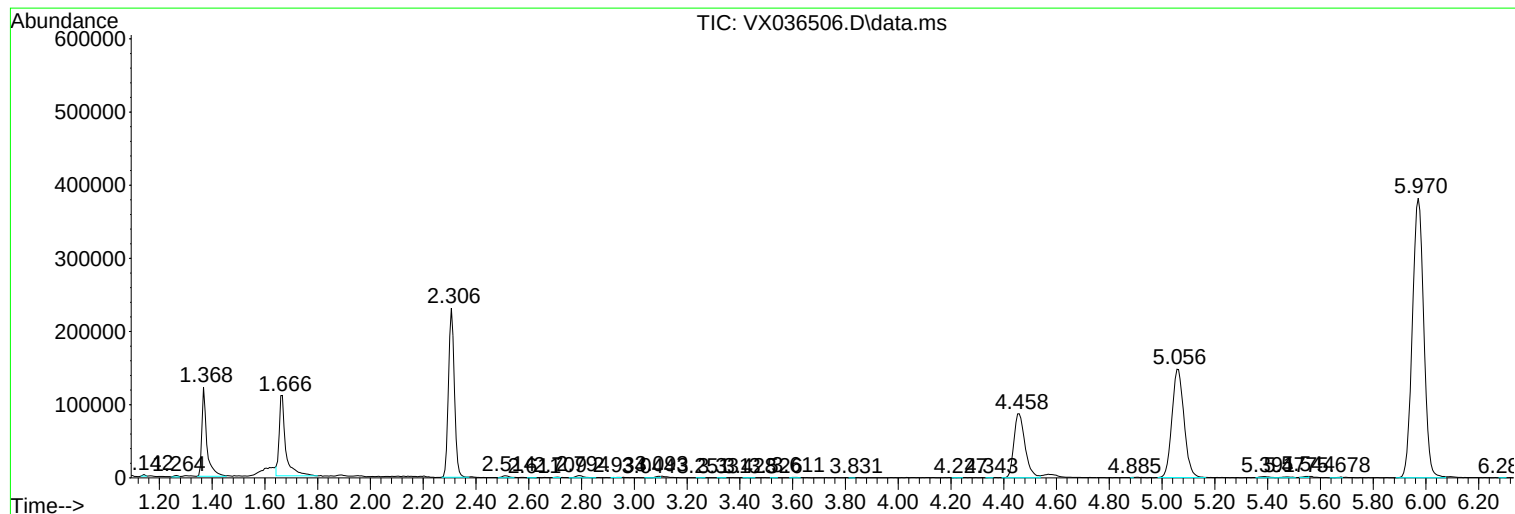

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071223\
Data File : VX036512.D
Acq On : 12 Jul 2023 13:01
Operator : JC/MD
Sample : VX0712WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK634

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML071223WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071223\
Data File : VX036512.D
Acq On : 12 Jul 2023 13:01
Operator : JC/MD
Sample : VX0712WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK634

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML071223WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------