
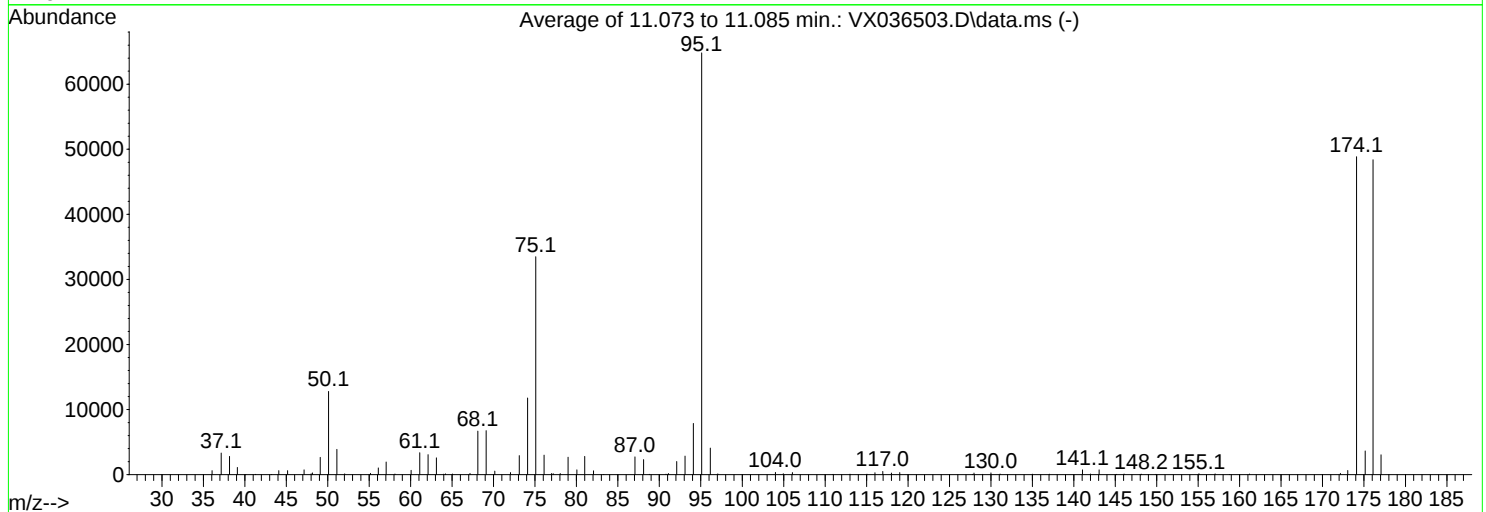


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071223\
Data File : VX036503.D
Acq On : 12 Jul 2023 09:16
Operator : JC/MD
Sample : BFB641
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB631

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM071223WMA.M
Title : VOC Analysis
Last Update : Thu Jul 13 05:47:06 2023

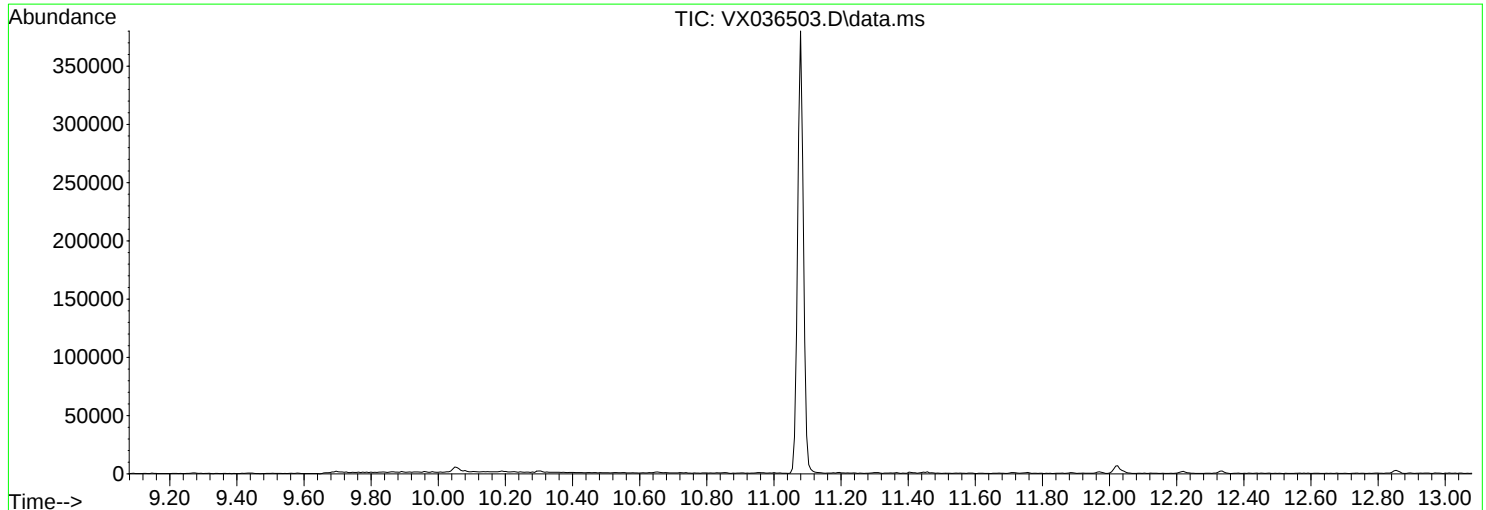

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.7	12789	PASS
75	95	30	80	51.7	33496	PASS
95	95	100	100	100.0	64816	PASS
96	95	5	9	6.3	4075	PASS
173	174	0.00	2	1.3	631	PASS
174	95	50	120	75.4	48864	PASS
175	174	5	9	7.5	3643	PASS
176	174	95	101	99.0	48392	PASS
177	176	5	9	6.3	3043	PASS

m/z	Abundance
36.00	222.0
40.00	129.0
44.10	93.0

Instrument :
MSVOA_X
ClientSampleId :
BFB631

m/z	Abundance
36.10	980.0
37.20	3338.0
38.10	2875.0
39.10	1339.0
40.10	198.0
41.30	82.0
43.20	57.0
44.10	907.0
45.10	689.0
47.10	661.0
48.00	398.0
49.10	2513.0
50.10	13088.0
51.10	3745.0
52.00	128.0
55.10	211.0
56.20	1271.0
57.10	2173.0
58.10	116.0
60.00	611.0
61.10	3699.0
62.10	3258.0
63.10	2450.0
64.00	173.0
65.10	157.0
67.20	237.0
68.10	7050.0
69.10	7201.0
70.20	501.0
72.10	312.0
73.10	2900.0
74.10	11550.0
75.10	34168.0
76.10	3409.0
77.00	349.0
79.00	2607.0
80.10	726.0
81.00	2947.0
82.10	534.0
83.30	81.0
87.00	2754.0
88.10	2141.0
91.10	266.0
92.10	1953.0
93.10	2625.0
94.10	7852.0
95.10	61368.0
96.10	3742.0
97.10	123.0
104.00	304.0
104.90	106.0
106.10	349.0
115.00	66.0
116.00	153.0
116.90	414.0
118.00	286.0
118.90	191.0
127.80	172.0
129.10	86.0
130.00	215.0
131.10	81.0
137.20	72.0
141.00	531.0
142.00	103.0
143.00	567.0
146.00	136.0
148.00	143.0
149.90	88.0
155.10	147.0
157.10	150.0
161.20	115.0
172.20	169.0
173.00	523.0
174.10	39288.0
175.10	3000.0
176.10	39328.0
177.00	2864.0
178.00	53.0

Instrument :
MSVOA_X
ClientSampleId :
BFB631

m/z	Abundance
36.10	932.0
37.10	4076.0
38.10	3368.0
39.10	1387.0
40.00	114.0
41.30	52.0
44.10	608.0
45.20	740.0
47.10	966.0
48.20	560.0
49.10	3108.0
50.10	16045.0
51.10	4712.0
52.10	123.0
55.20	250.0
56.10	1100.0
57.10	2163.0
58.10	113.0
60.00	839.0
61.10	4002.0
62.10	3368.0
63.10	3342.0
64.20	385.0
65.00	91.0
67.10	164.0
68.10	8108.0
69.10	8090.0
70.10	687.0
72.00	422.0
73.10	3450.0
74.10	14352.0
75.10	39672.0
76.10	3500.0
77.20	411.0
78.00	294.0
79.00	3214.0
80.00	956.0
81.00	3309.0
82.00	853.0
87.10	3249.0
88.10	2553.0
88.80	135.0
90.80	206.0
92.10	2310.0
93.10	3335.0
94.10	9338.0
95.10	79224.0
96.20	4938.0
97.00	221.0
104.00	429.0
105.00	292.0
106.00	285.0
111.00	89.0
113.00	184.0
115.10	96.0
116.00	493.0
117.00	626.0
118.00	317.0
119.00	502.0
128.00	508.0
128.90	99.0
130.00	426.0
131.10	90.0
135.00	147.0
137.00	97.0
141.00	914.0
142.00	76.0
143.00	899.0
145.20	84.0
146.10	145.0
148.20	140.0
149.00	75.0
149.90	53.0
155.10	183.0
157.00	155.0
158.80	54.0
161.10	120.0
172.10	185.0
173.10	659.0
174.10	59272.0
175.10	4619.0
176.10	58696.0
177.10	3683.0

Instrument :
MSVOA_X
ClientSampleId :
BFB631

m/z	Abundance
36.20	591.0
37.10	2542.0
38.20	2188.0
39.10	570.0
40.10	121.0
44.10	622.0
45.10	399.0
47.20	619.0
48.10	262.0
49.10	2374.0
50.10	9233.0
51.10	3189.0
52.10	152.0
55.20	132.0
56.00	747.0
57.00	1482.0
58.10	81.0
60.10	563.0
61.10	2391.0
62.10	2601.0
63.10	1955.0
64.00	88.0
65.00	58.0
67.10	165.0
68.10	4943.0
69.10	5032.0
70.10	450.0
72.10	232.0
73.10	2446.0
74.10	9450.0
75.10	26648.0
76.10	2106.0
77.00	174.0
78.10	217.0
79.00	2201.0
80.00	564.0
81.00	2148.0
82.00	395.0
87.10	2156.0
88.10	2254.0
91.10	253.0
92.10	1798.0
93.10	2641.0
94.10	6394.0
95.10	53856.0
96.10	3546.0
104.00	339.0
105.00	69.0
106.00	301.0
110.90	73.0
113.00	56.0
115.10	86.0
116.00	255.0
117.00	480.0
118.10	163.0
119.10	313.0
127.90	218.0
130.00	165.0
131.10	134.0
135.00	114.0
137.00	80.0
141.10	784.0
142.00	147.0
143.10	758.0
145.10	63.0
148.10	104.0
155.10	149.0
157.10	86.0
161.30	73.0
172.20	256.0
173.10	710.0
174.10	48032.0
175.20	3311.0
176.10	47152.0
177.10	2582.0

Instrument :
MSVOA_X
ClientSampleId :
BFB631