

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071224\
 Data File : VX042309.D
 Acq On : 12 Jul 2024 17:45
 Operator : JC/MD
 Sample : PB162021ZHE#06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 PB162021ZHE#06

Quant Time: Jul 15 04:46:38 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061824W.M
 Quant Title : SW846 8260
 QLast Update : Fri Jun 21 23:51:58 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.550	168	122486	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	6.763	114	205704	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	187293	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	81939	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	79126	56.022	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	112.040%
35) Dibromofluoromethane	5.385	113	74969	51.364	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	102.720%
50) Toluene-d8	8.647	98	220600	43.022	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	86.040%#
62) 4-Bromofluorobenzene	11.079	95	78847	41.715	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	83.420%
Target Compounds						
					Qvalue	
16) Acetone	2.386	43	26217	42.272	ug/l	# 84
18) Methyl Acetate	2.703	43	4060	2.400	ug/l	99
20) Methylene Chloride	2.788	84	7435	5.475	ug/l	90
43) Isopropyl Acetate	6.342	43	108278	34.938	ug/l	# 93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071224\
Data File : VX042309.D
Acq On : 12 Jul 2024 17:45
Operator : JC/MD
Sample : PB162021ZHE#06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
PB162021ZHE#06

Quant Time: Jul 15 04:46:38 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061824W.M
Quant Title : SW846 8260
QLast Update : Fri Jun 21 23:51:58 2024
Response via : Initial Calibration




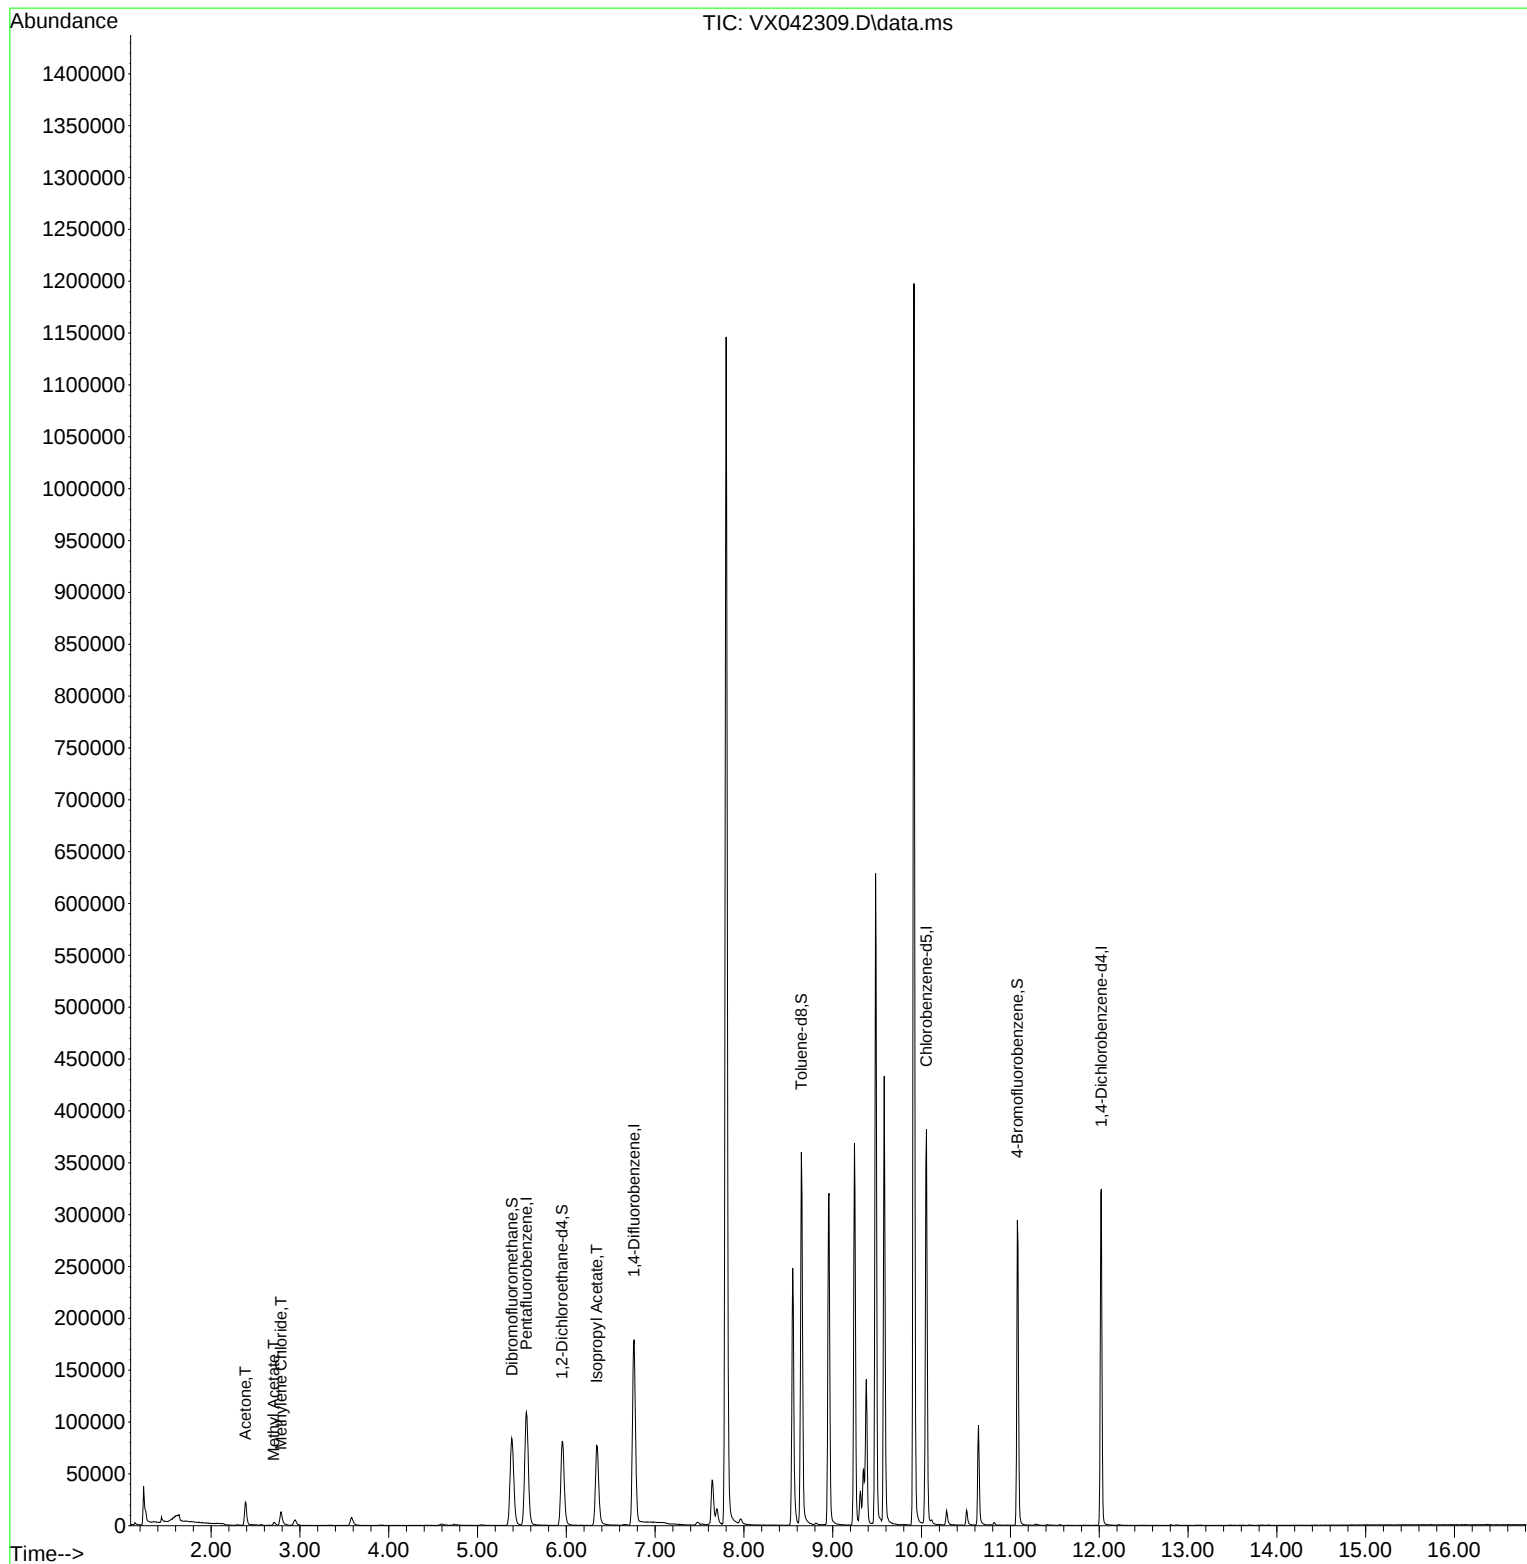


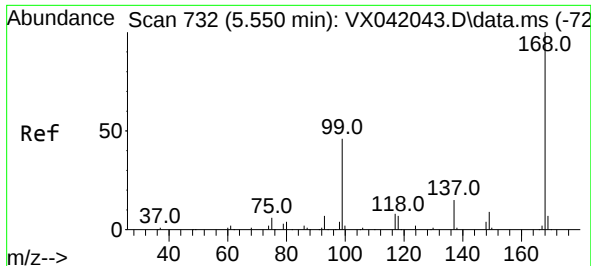

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX042309.D
Acq: 12 Jul 2024 17:45




Instrument :
MSVOA_X
ClientSampleId :
PB162021ZHE#06


Tgt Ion:168 Resp: 122486
Ion Ratio Lower Upper
168 100
99 47.3 56.6 85.0#

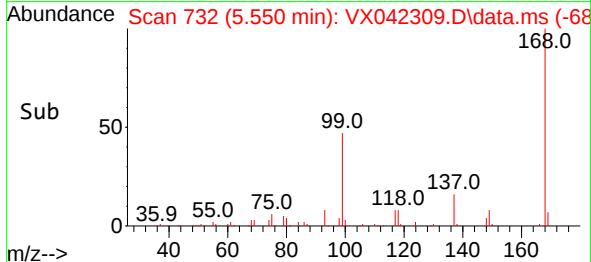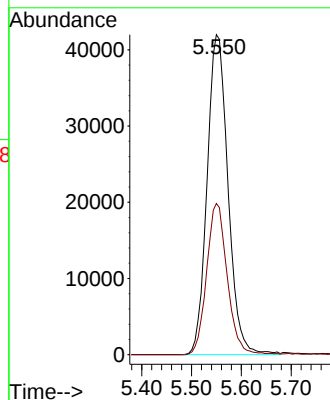

#16
Acetone
Concen: 42.272 ug/l
RT: 2.386 min Scan# 213
Delta R.T. -0.012 min
Lab File: VX042309.D
Acq: 12 Jul 2024 17:45

Tgt Ion: 43 Resp: 26217
Ion Ratio Lower Upper
43 100
58 35.9 21.9 32.9#


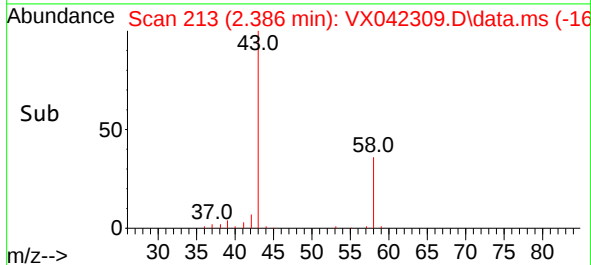
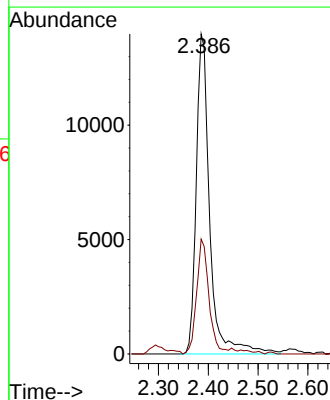
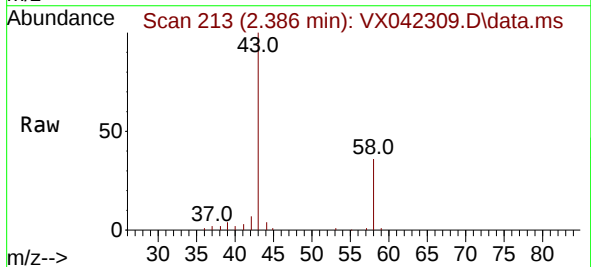


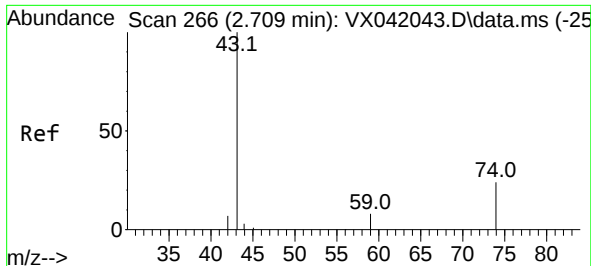

#18
Methyl Acetate
Concen: 2.400 ug/l
RT: 2.703 min Scan# 20
Delta R.T. -0.006 min
Lab File: VX042309.D
Acq: 12 Jul 2024 17:45




Instrument :
MSVOA_X
ClientSampleId :
PB162021ZHE#06


Tgt Ion: 43 Resp: 4060
Ion Ratio Lower Upper
43 100
74 23.0 17.8 26.8

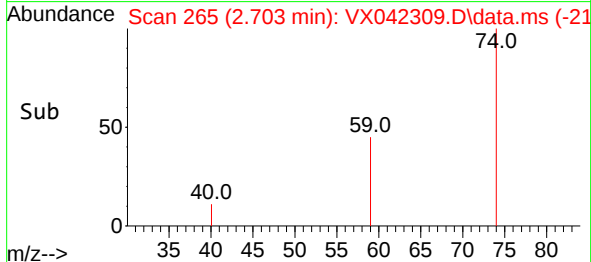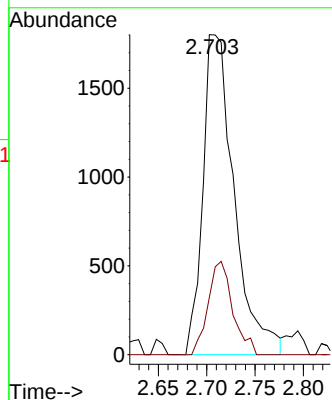

#20
Methylene Chloride
Concen: 5.475 ug/l
RT: 2.788 min Scan# 279
Delta R.T. 0.006 min
Lab File: VX042309.D
Acq: 12 Jul 2024 17:45

Tgt Ion: 84 Resp: 7435
Ion Ratio Lower Upper
84 100
49 112.0 103.6 155.4
51 37.1 33.8 50.6
86 62.6 49.4 74.0

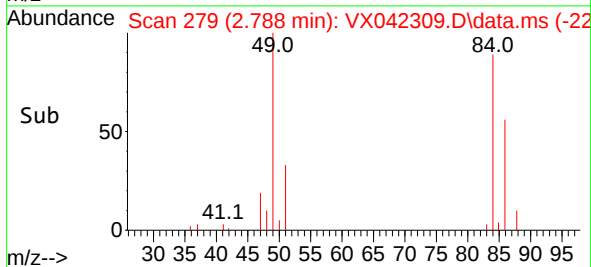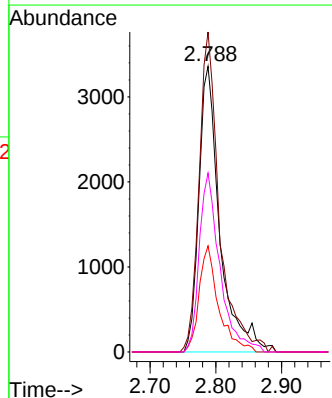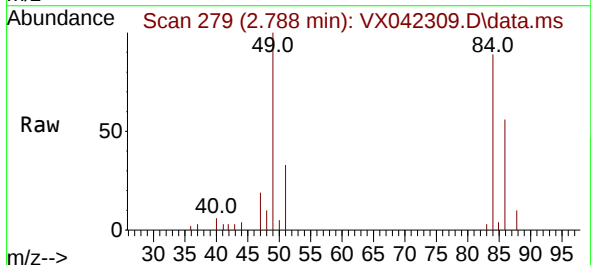

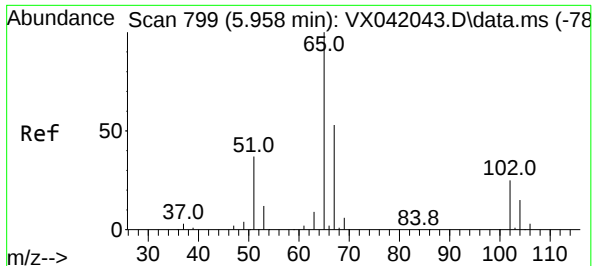

#33

1,2-Dichloroethane-d4

Concen: 56.022 ug/l

RT: 5.952 min Scan# 799

Delta R.T. -0.006 min

Lab File: VX042309.D

Acq: 12 Jul 2024 17:45

Instrument :

MSVOA_X

ClientSampleId :





PB162021ZHE#06

Tgt Ion: 65 Resp: 79126

Ion Ratio Lower Upper

65 100

67 53.3 0.0 100.2

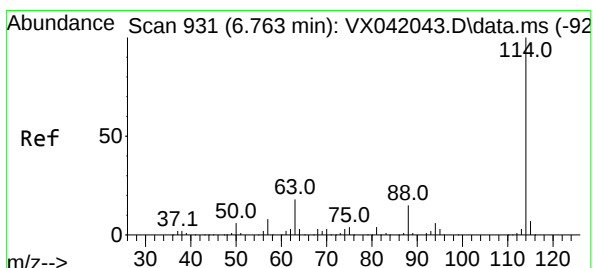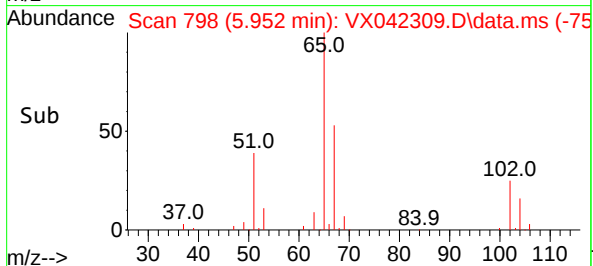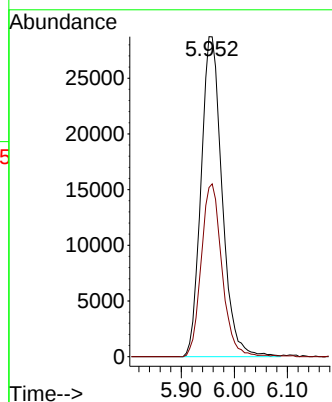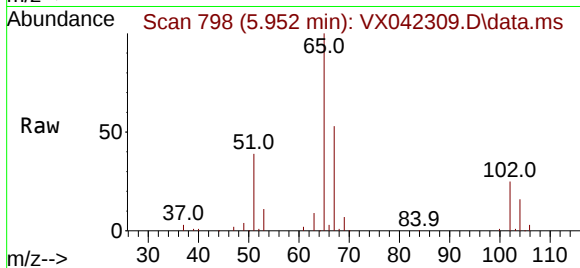

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.763 min Scan# 931

Delta R.T. 0.000 min

Lab File: VX042309.D

Acq: 12 Jul 2024 17:45




Tgt Ion: 114 Resp: 205704


Ion Ratio Lower Upper

114 100

63 17.7 0.0 45.0

88 14.7 0.0 36.6


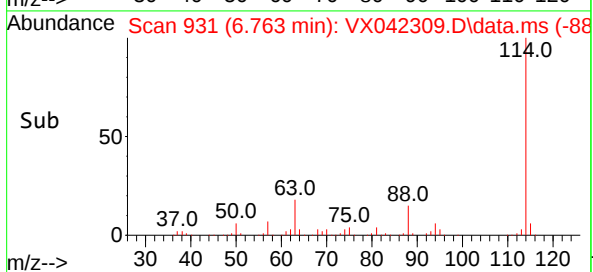
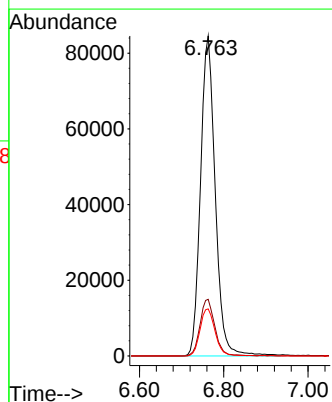
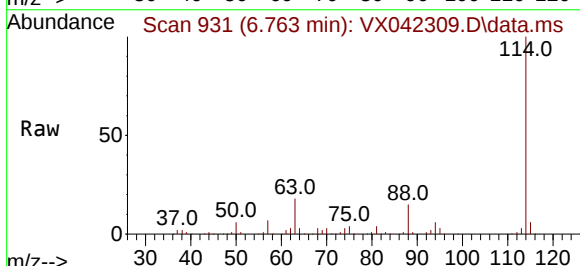


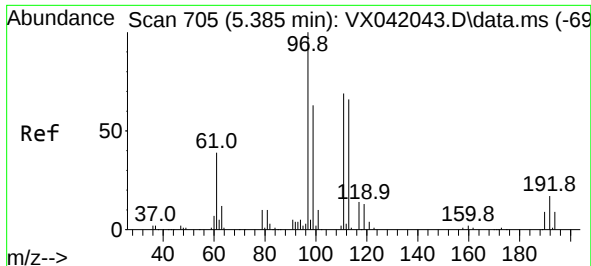

#35
Dibromofluoromethane
Concen: 51.364 ug/l
RT: 5.385 min Scan# 705
Delta R.T. -0.006 min
Lab File: VX042309.D
Acq: 12 Jul 2024 17:45




Instrument :
MSVOA_X
ClientSampleId :
PB162021ZHE#06


Tgt Ion:113 Resp: 74969
Ion Ratio Lower Upper
113 100
111 103.0 82.9 124.3
192 25.5 13.3 19.9#

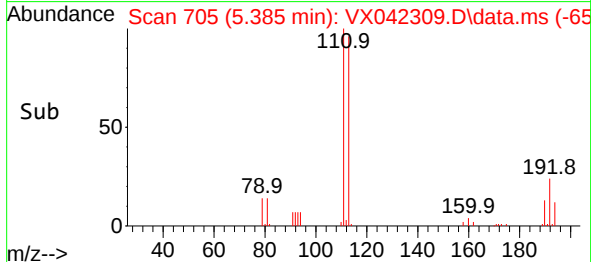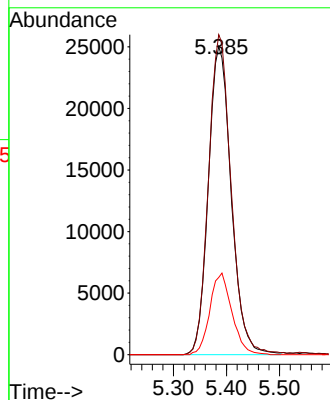

#43
Isopropyl Acetate
Concen: 34.938 ug/l
RT: 6.342 min Scan# 862
Delta R.T. -0.006 min
Lab File: VX042309.D
Acq: 12 Jul 2024 17:45

Tgt Ion: 43 Resp: 108278
Ion Ratio Lower Upper
43 100
61 21.6 15.2 22.8
87 15.3 9.8 14.6#


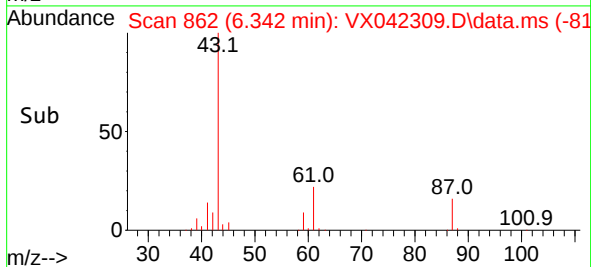
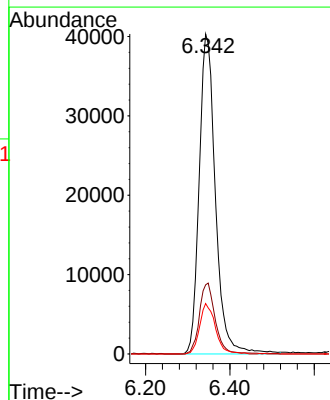
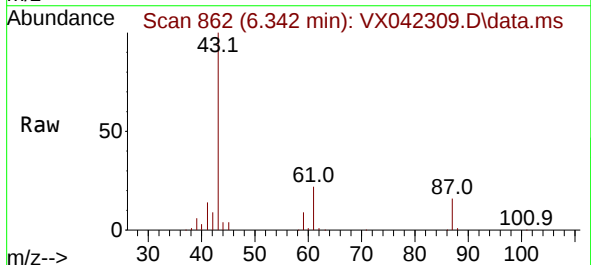




#50
Toluene-d8
Concen: 43.022 ug/l
RT: 8.647 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX042309.D
Acq: 12 Jul 2024 17:45




Instrument :
MSVOA_X
ClientSampleId :
PB162021ZHE#06


Tgt Ion: 98 Resp: 220600
Ion Ratio Lower Upper
98 100
100 65.9 53.1 79.7

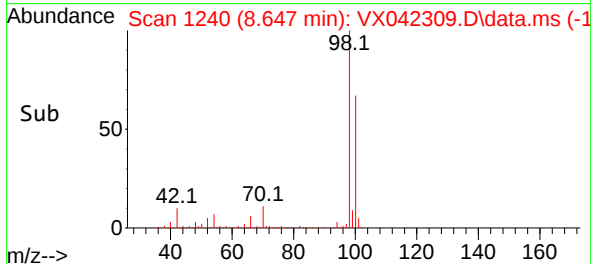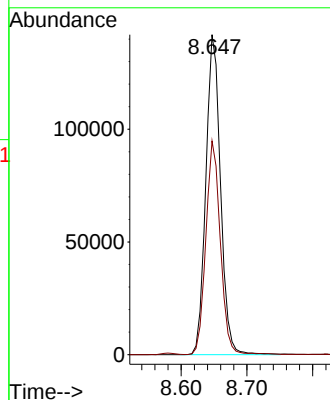

#62
4-Bromofluorobenzene
Concen: 41.715 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX042309.D
Acq: 12 Jul 2024 17:45

Tgt Ion: 95 Resp: 78847
Ion Ratio Lower Upper
95 100
174 101.0 0.0 135.6
176 97.7 0.0 131.0


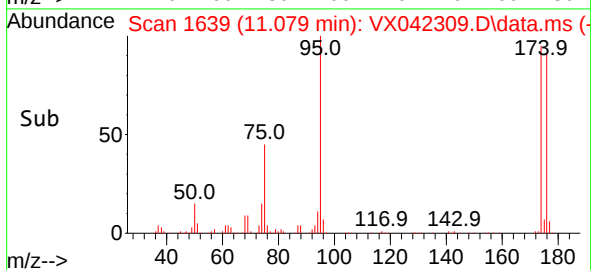
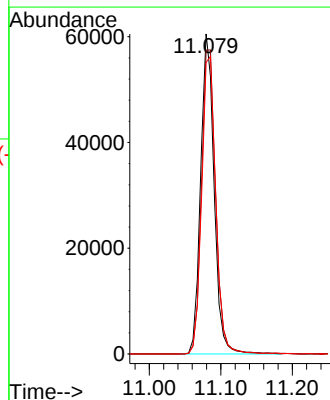
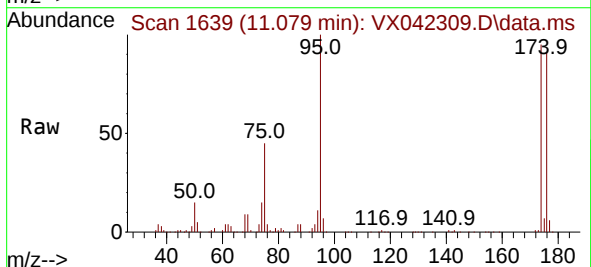




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX042309.D
Acq: 12 Jul 2024 17:45

Instrument :
MSVOA_X
ClientSampleId :
PB162021ZHE#06

Tgt Ion:117 Resp: 187293
Ion Ratio Lower Upper
117 100
82 49.6 46.2 69.4
119 32.3 25.5 38.3

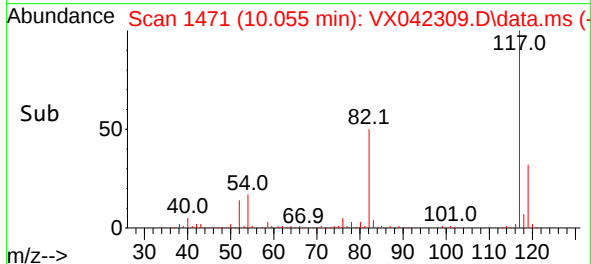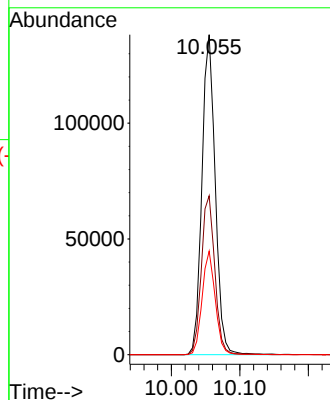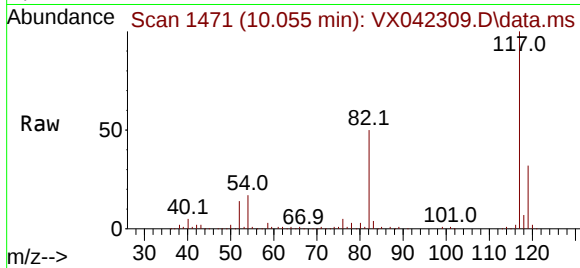

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX042309.D
Acq: 12 Jul 2024 17:45

Tgt Ion:152 Resp: 81939
Ion Ratio Lower Upper
152 100
115 52.2 43.3 129.9
150 155.6 0.0 345.0

