



Dichlorodifluoromethane

Response Ratio

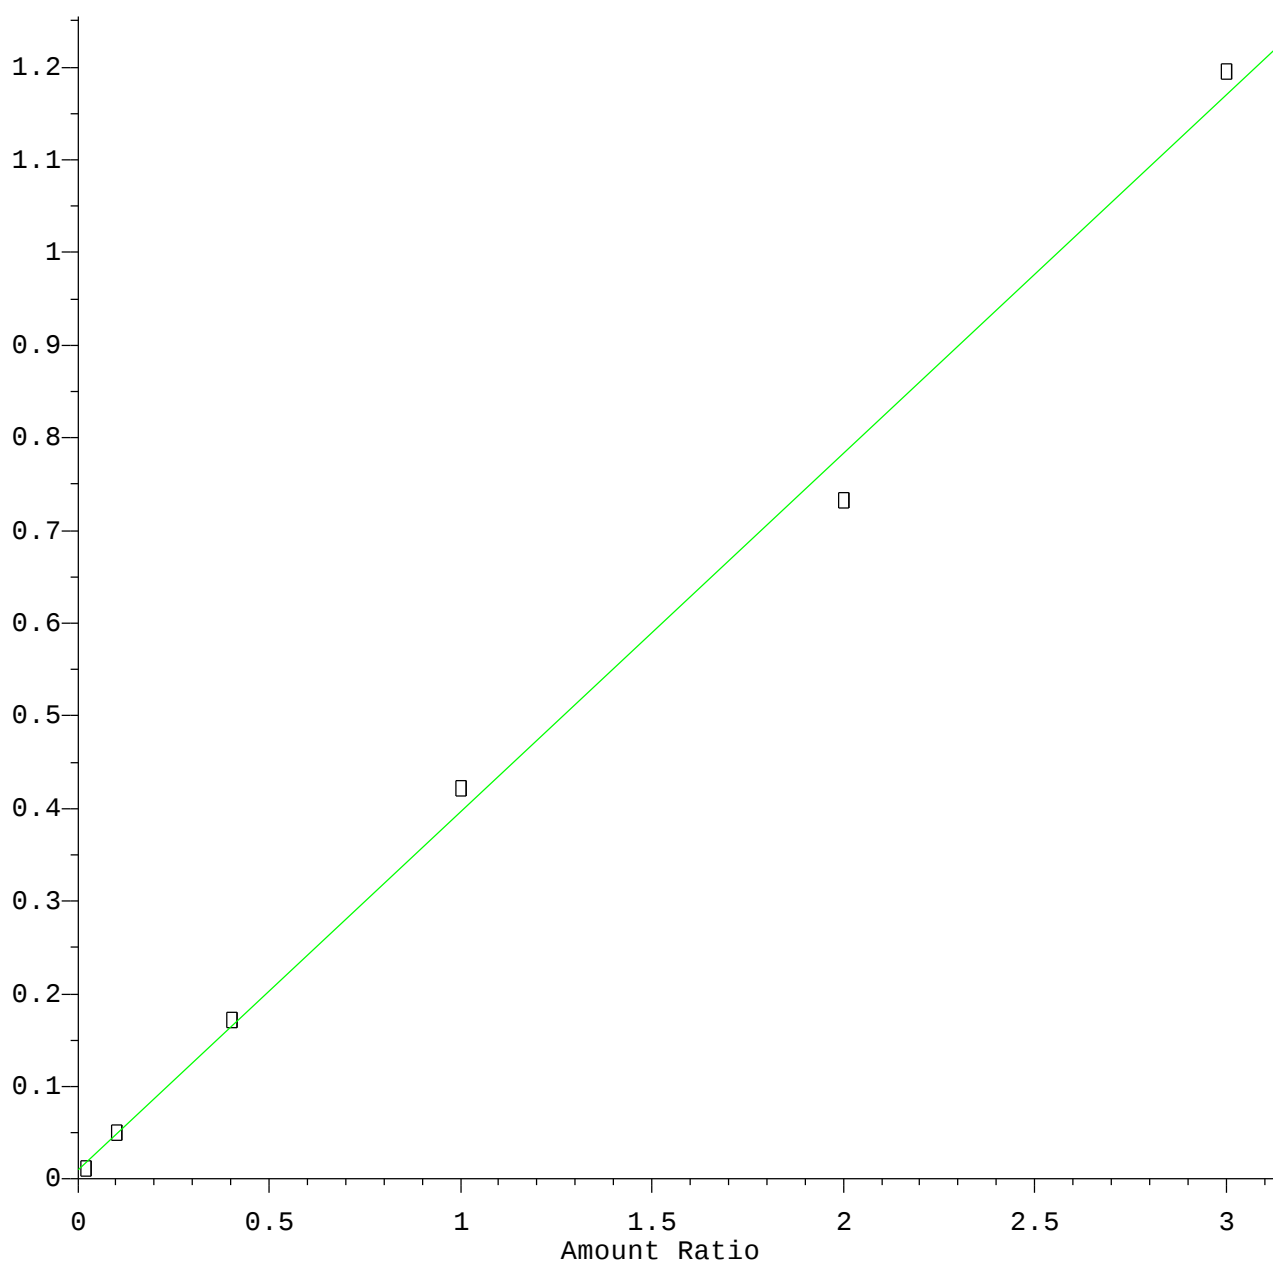


Resp Ratio = $3.87 \times 10^{-1} \times \text{Amt} + 9.94 \times 10^{-3}$
Coef of Det (r^2) = 0.996 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X071318W.M
Calibration Table Last Updated: Fri Jul 13 17:01:02 2018

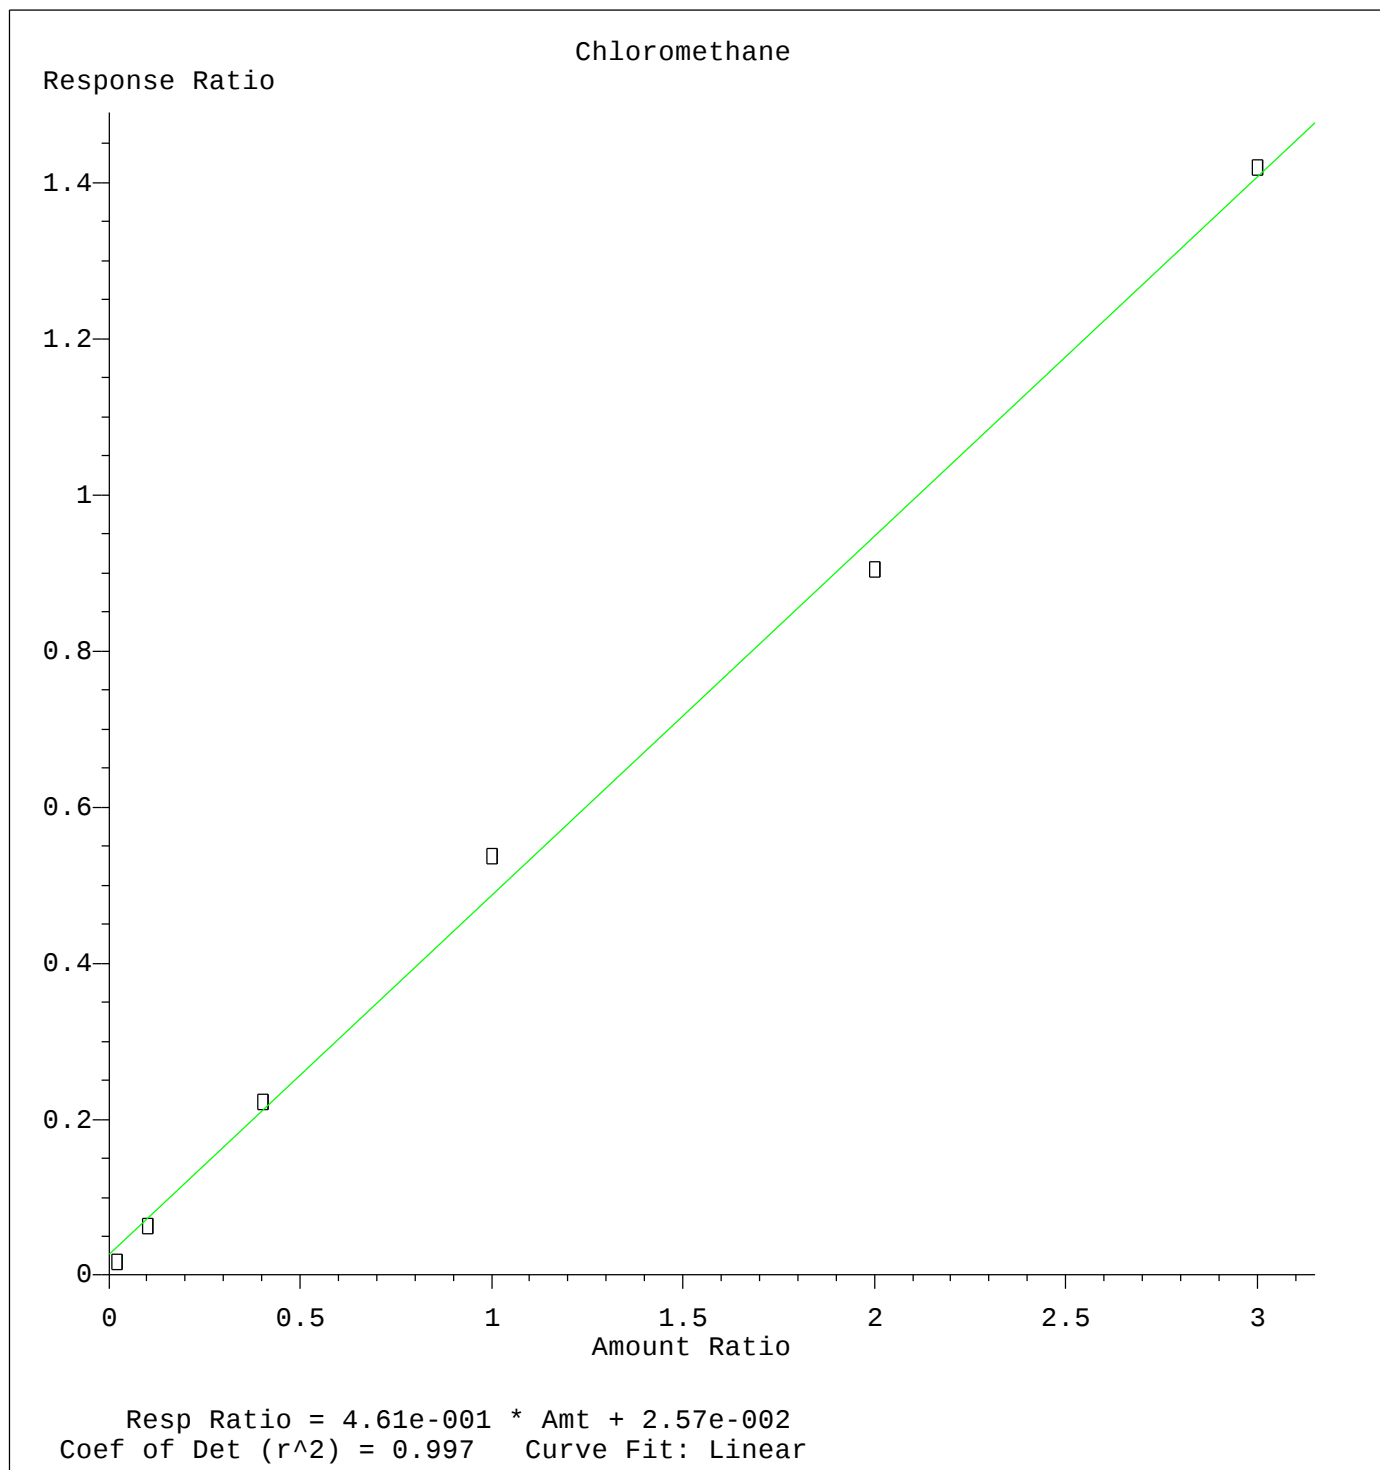


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X071318W.M
Calibration Table Last Updated: Fri Jul 13 17:01:02 2018

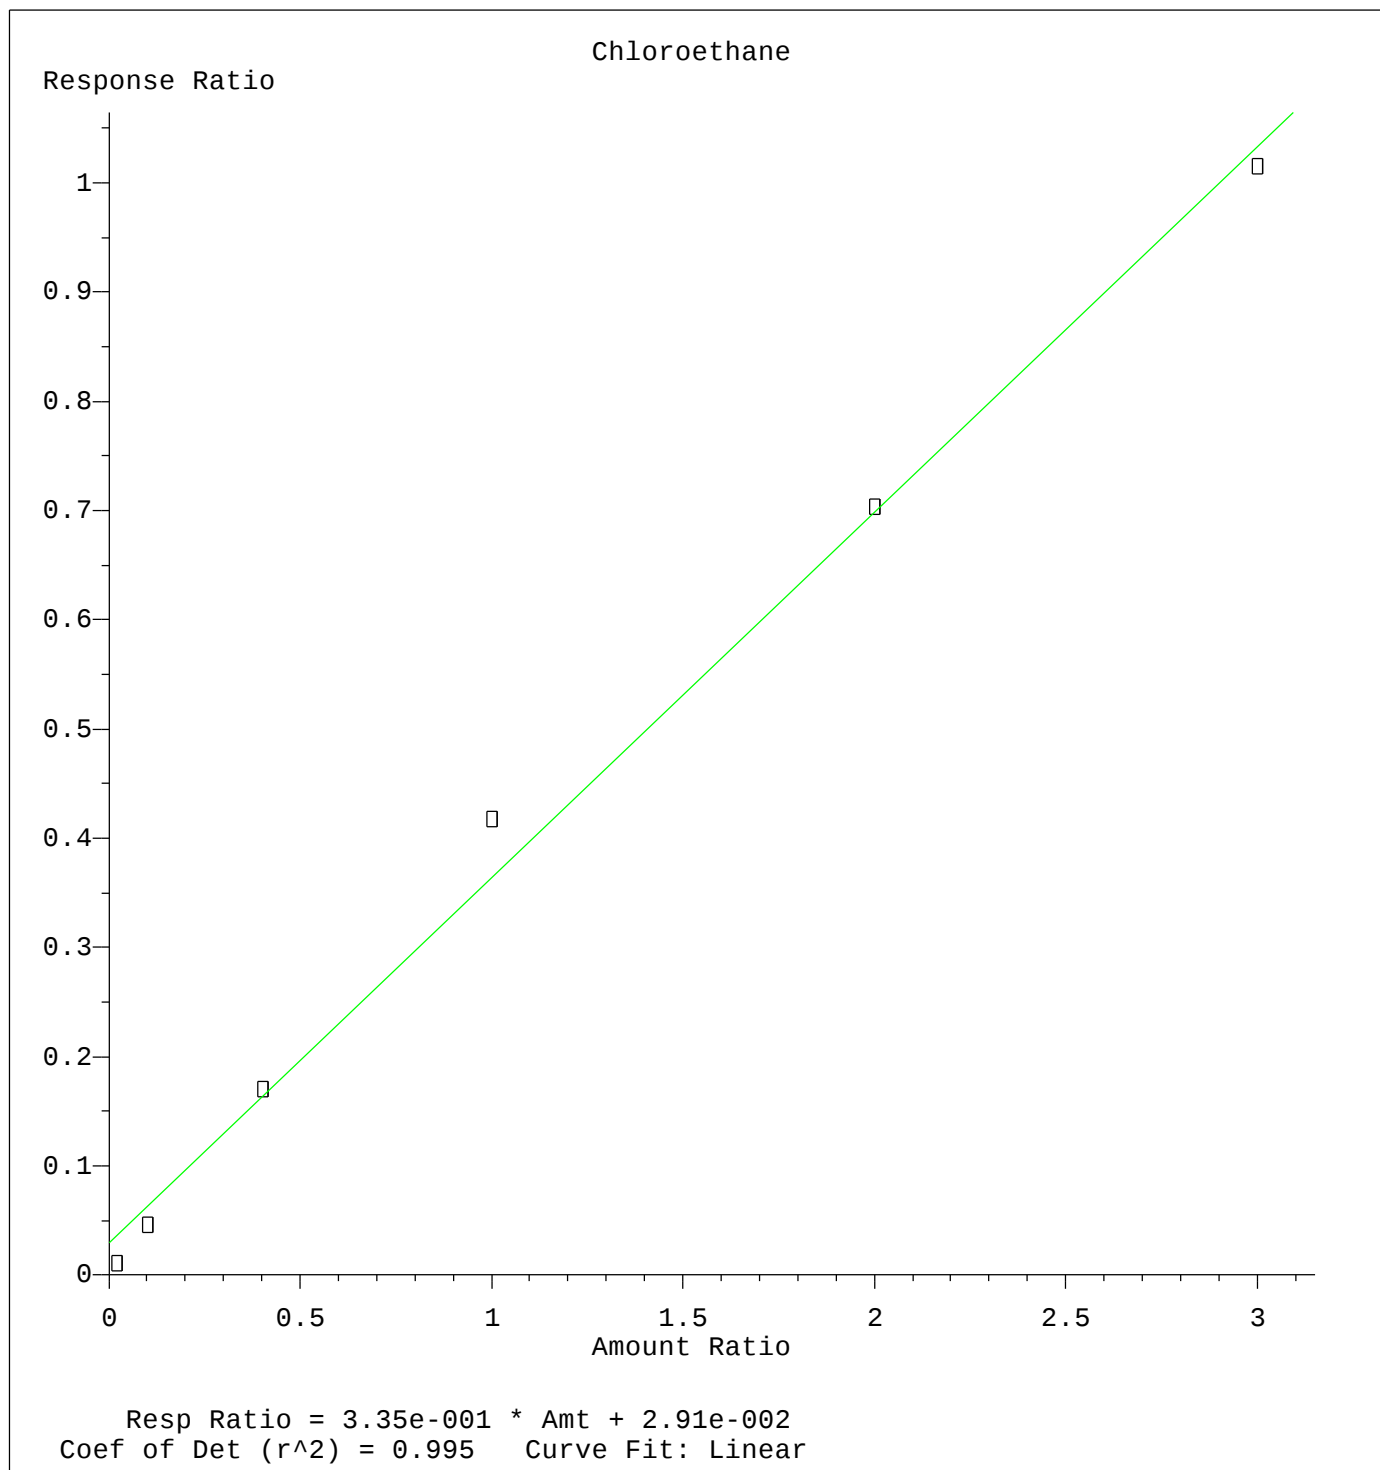

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X071318W.M
Calibration Table Last Updated: Fri Jul 13 17:01:02 2018

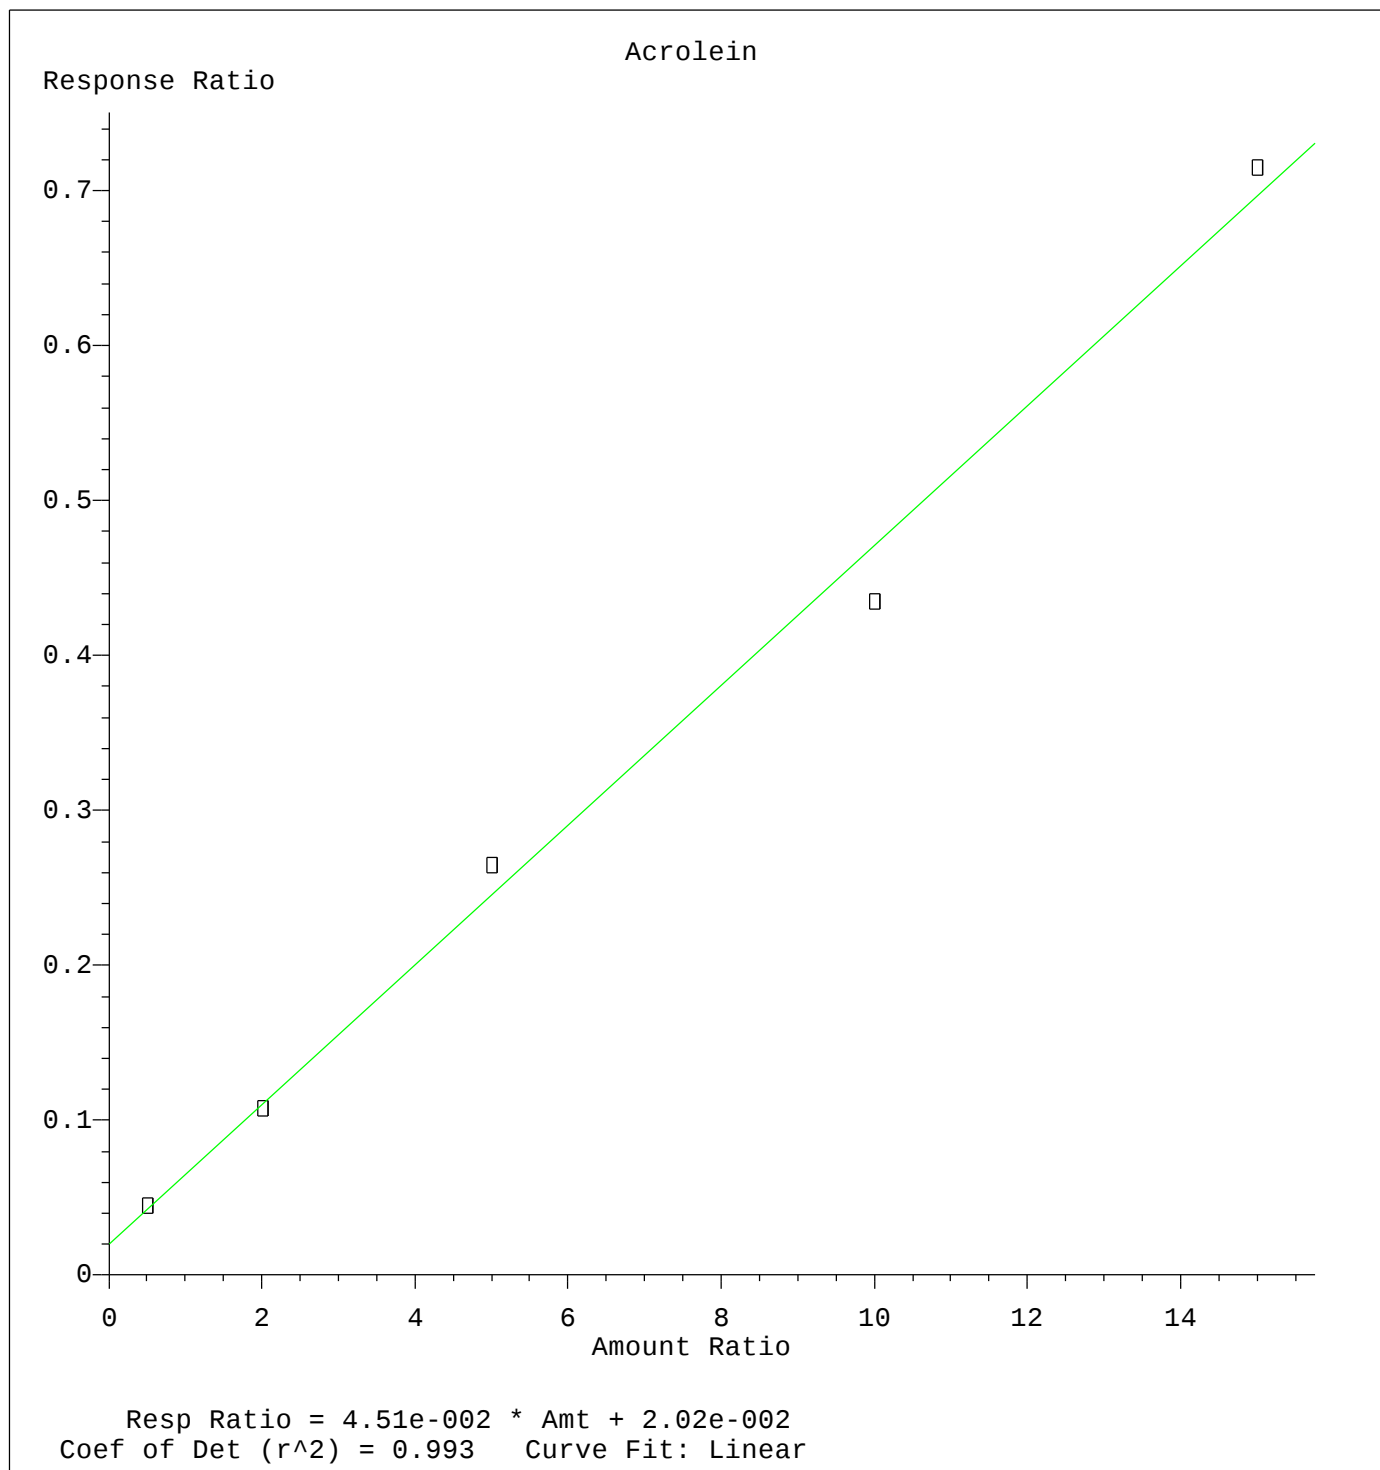


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X071318W.M
Calibration Table Last Updated: Fri Jul 13 17:01:02 2018

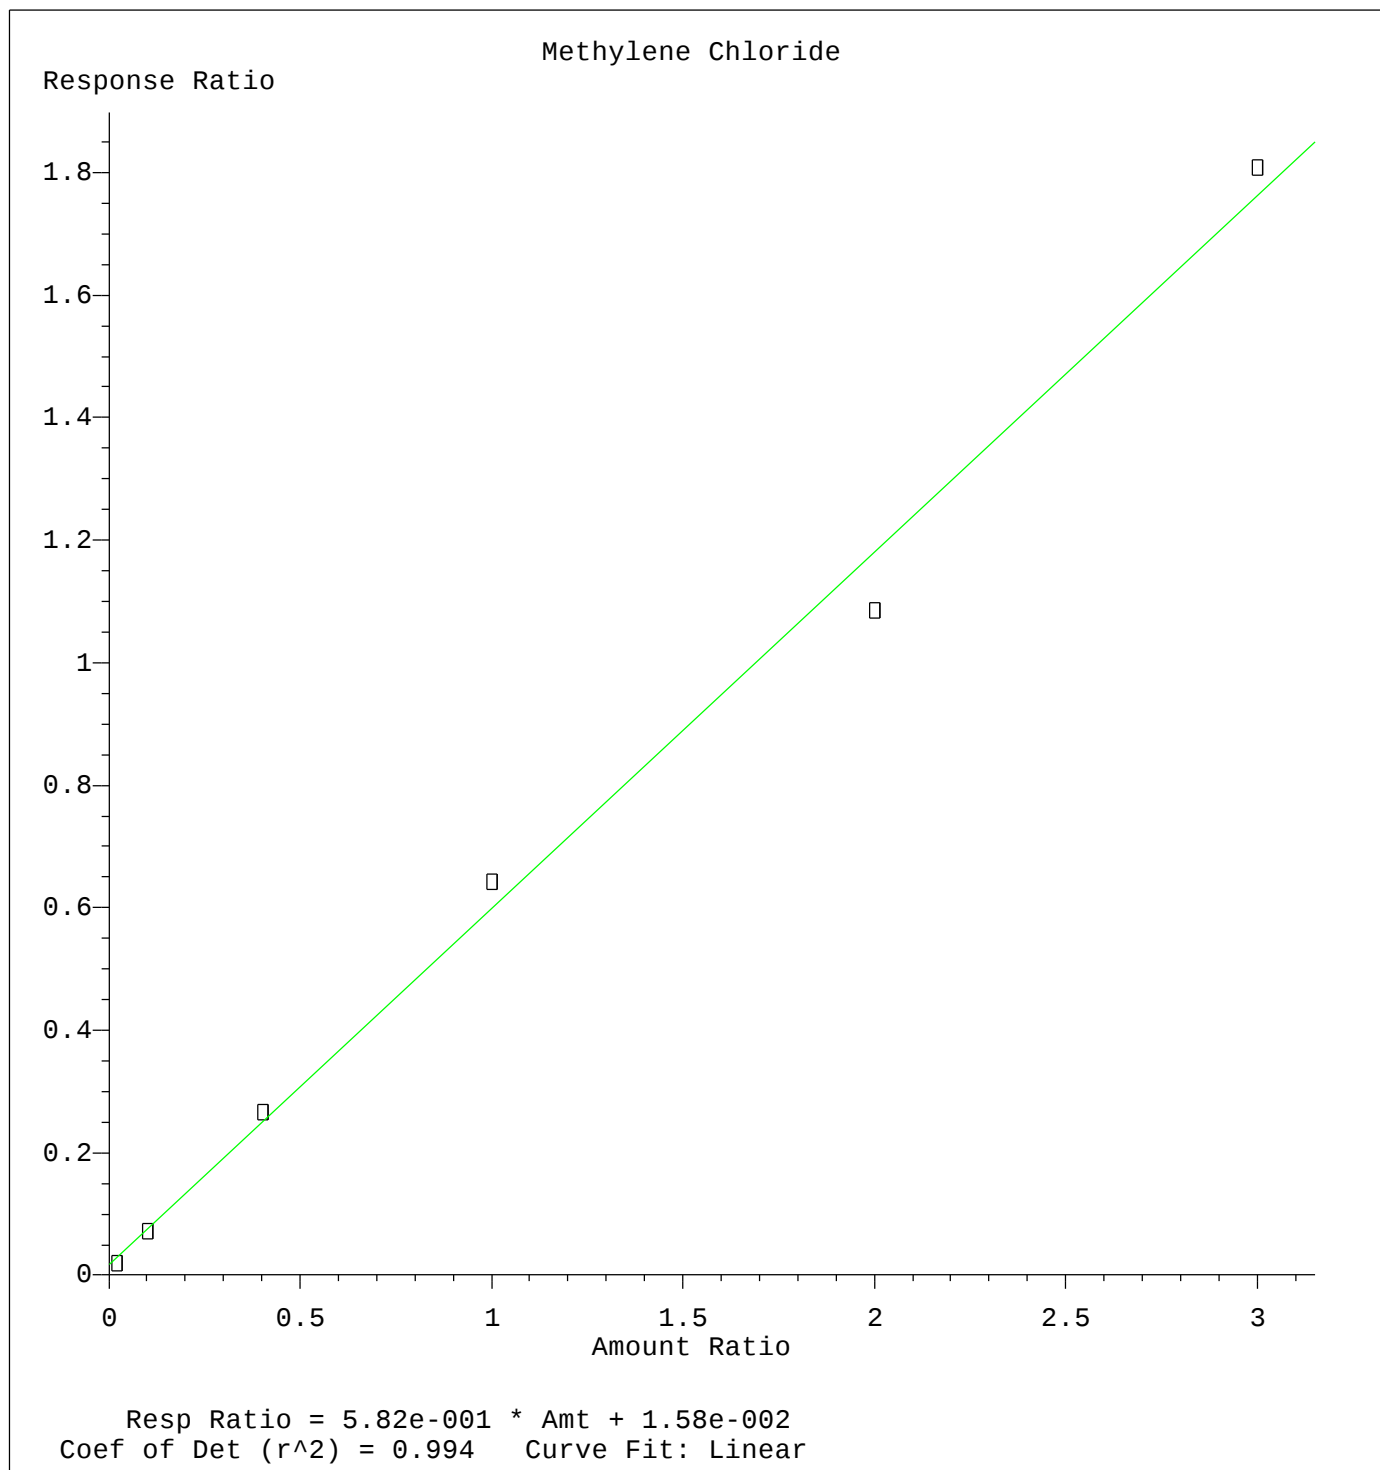

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X071318W.M
Calibration Table Last Updated: Fri Jul 13 17:01:02 2018


1,2-Dichloroethane-d4

Response Ratio

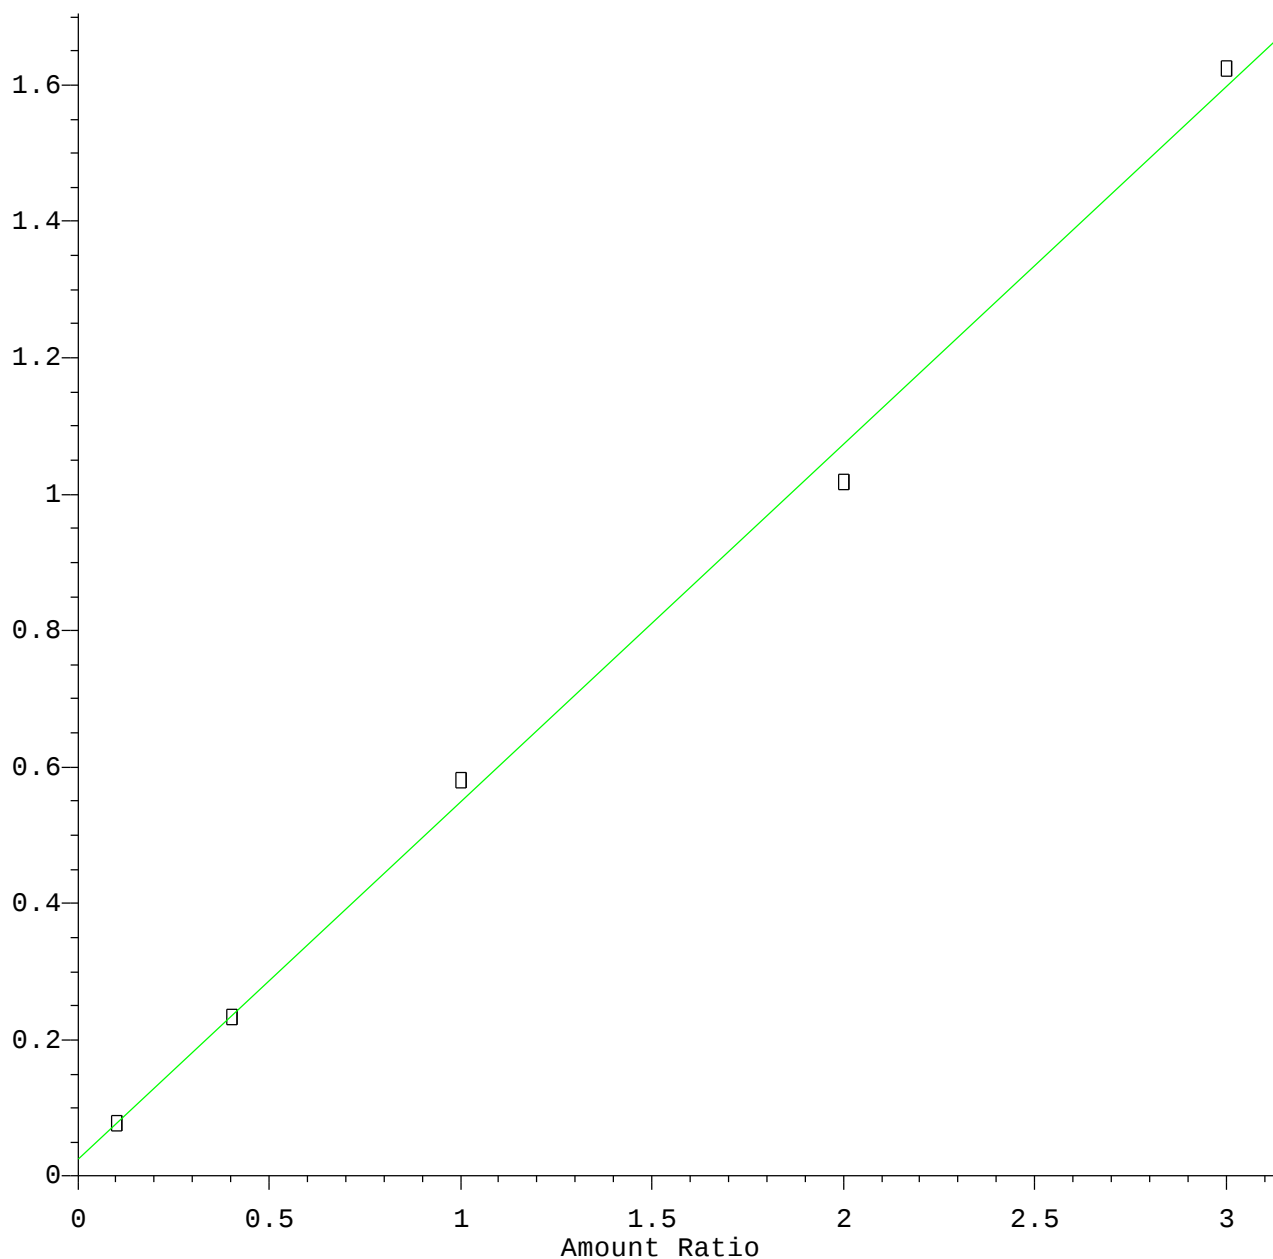

Resp Ratio = $5.24 \times 10^{-1} \times \text{Amt} + 2.50 \times 10^{-2}$
Coef of Det (r^2) = 0.997 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X071318W.M
Calibration Table Last Updated: Fri Jul 13 17:01:02 2018

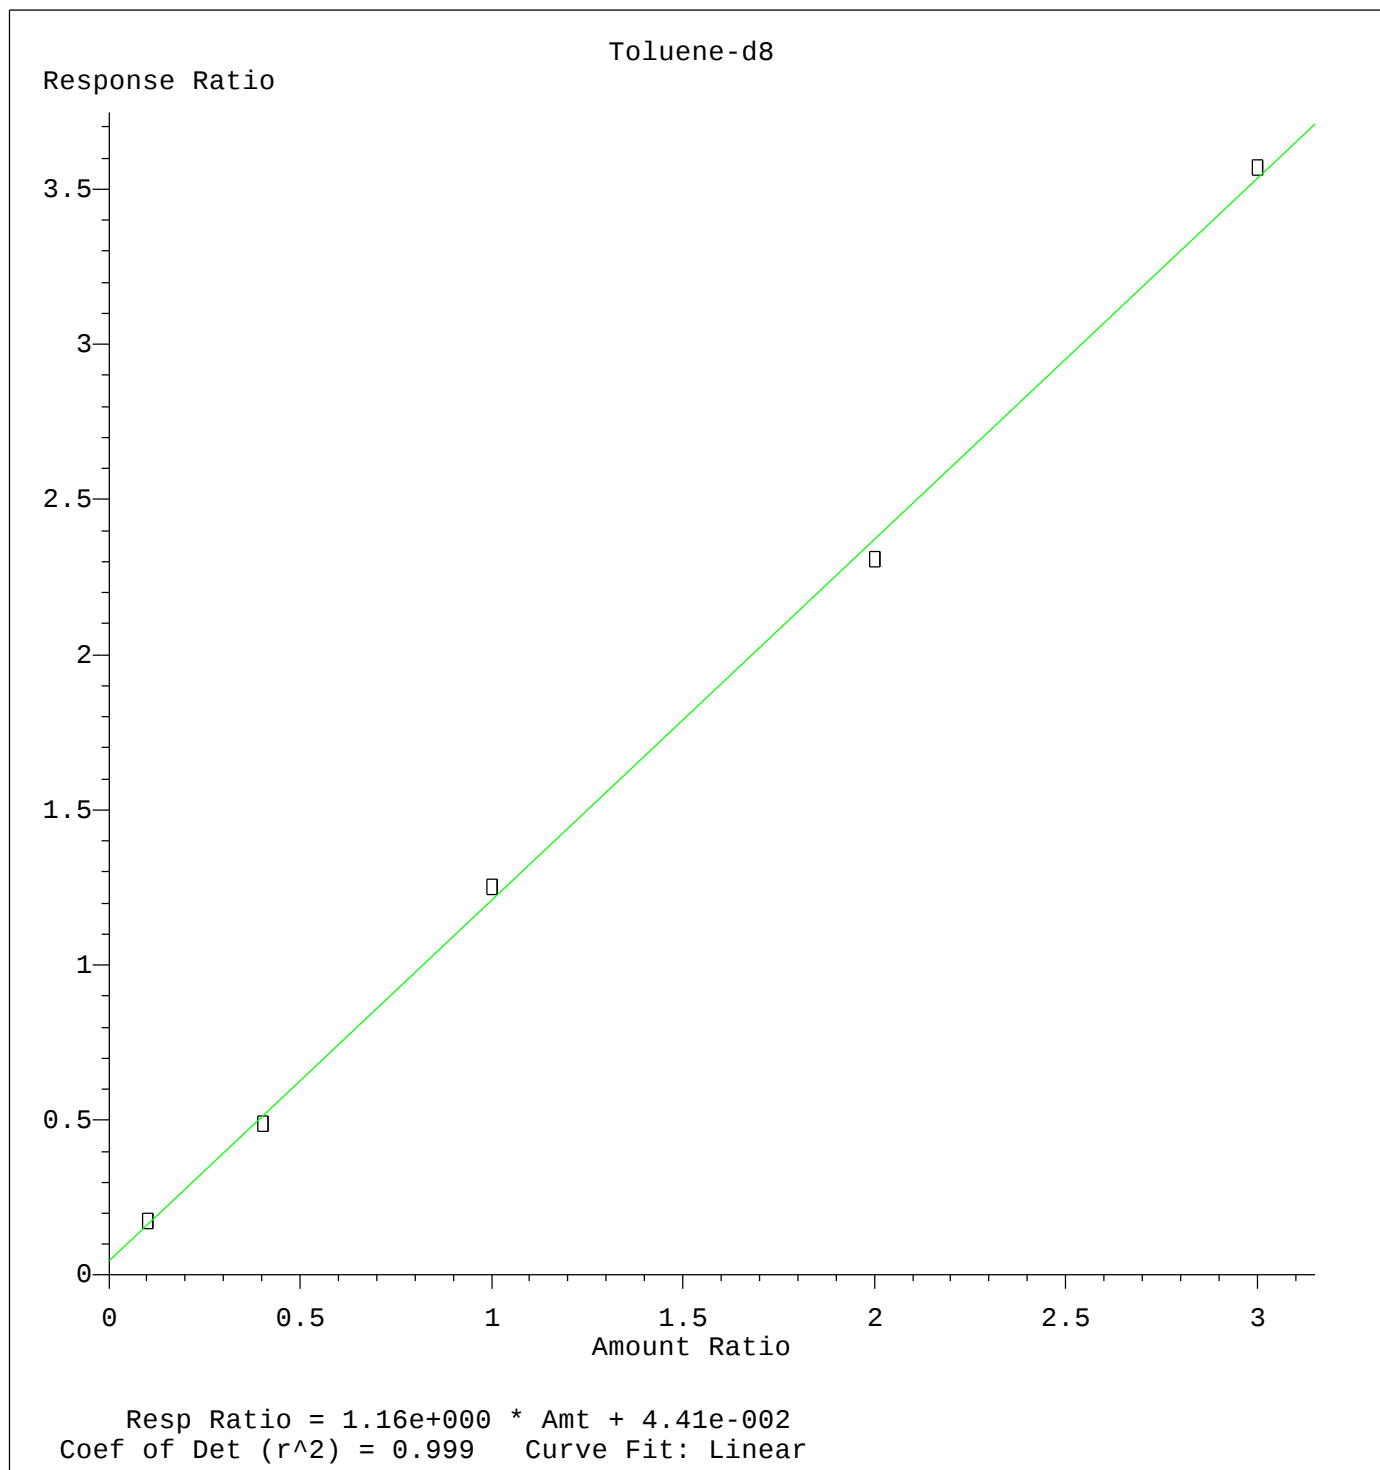

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X071318W.M
Calibration Table Last Updated: Fri Jul 13 17:01:02 2018