


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX071318\
Data File : VX003359.D
Acq On : 13 Jul 2018 10:58
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X071318W.M
Title : SW846 8260
Last Update : Fri Jul 13 17:01:02 2018

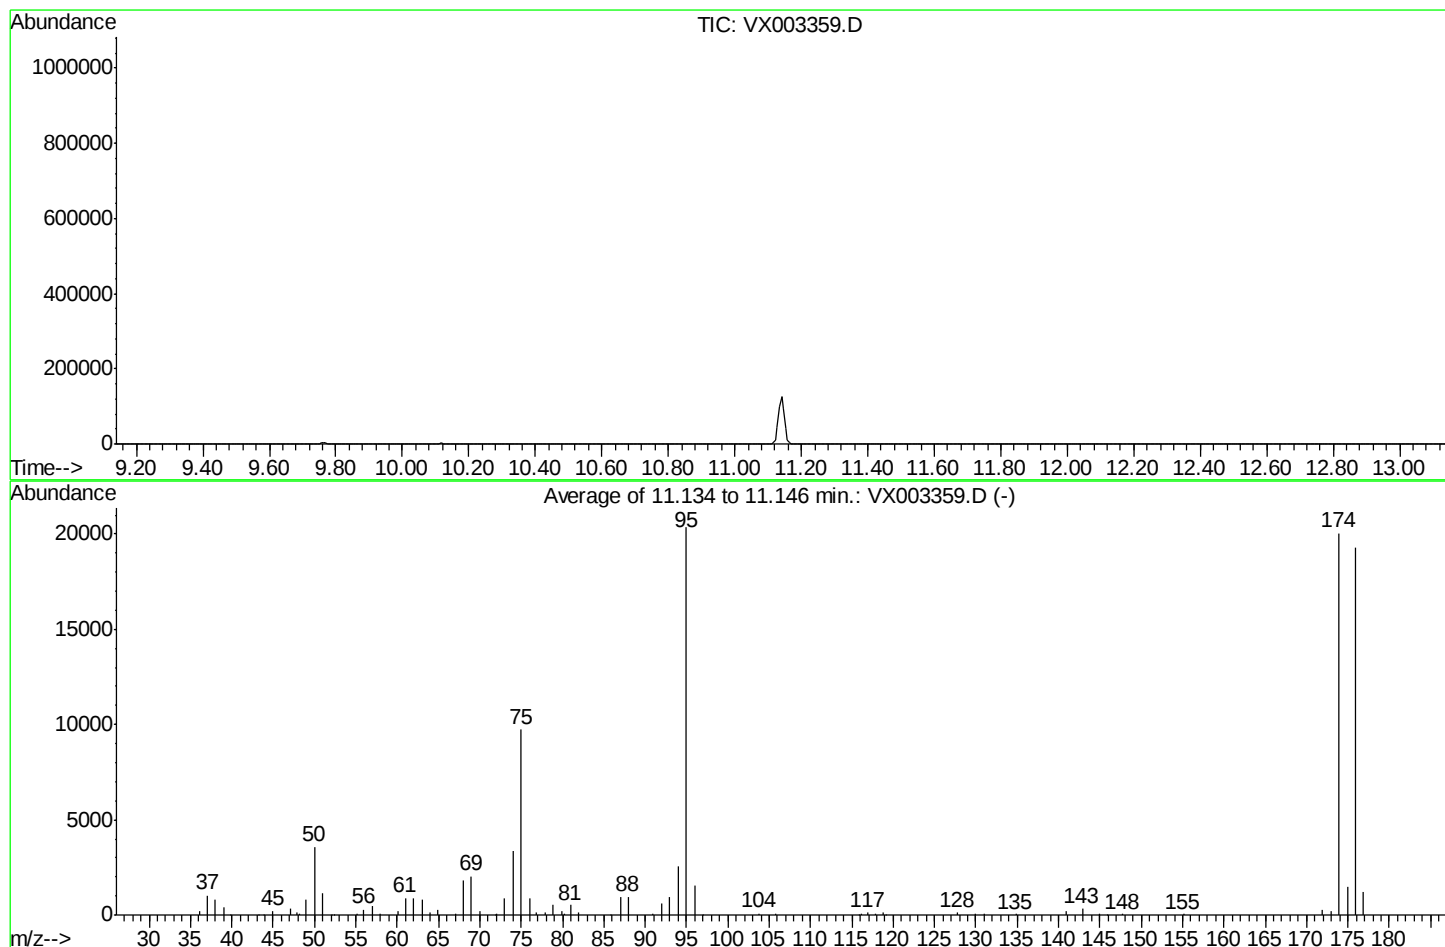

AutoFind: Scans 1730, 1731, 1732; Background Corrected with Scan 1724

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.6	3577	PASS
75	95	30	60	47.8	9739	PASS
95	95	100	100	100.0	20354	PASS
96	95	5	9	7.5	1533	PASS
173	174	0.00	2	1.1	217	PASS
174	95	50	100	98.5	20056	PASS
175	174	5	9	7.4	1488	PASS
176	174	95	101	96.1	19274	PASS
177	176	5	9	6.2	1202	PASS