


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX071318\
Data File : VX003369.D
Acq On : 13 Jul 2018 18:28
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampled :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X071318W.M
Title : SW846 8260
Last Update : Fri Jul 13 17:01:02 2018

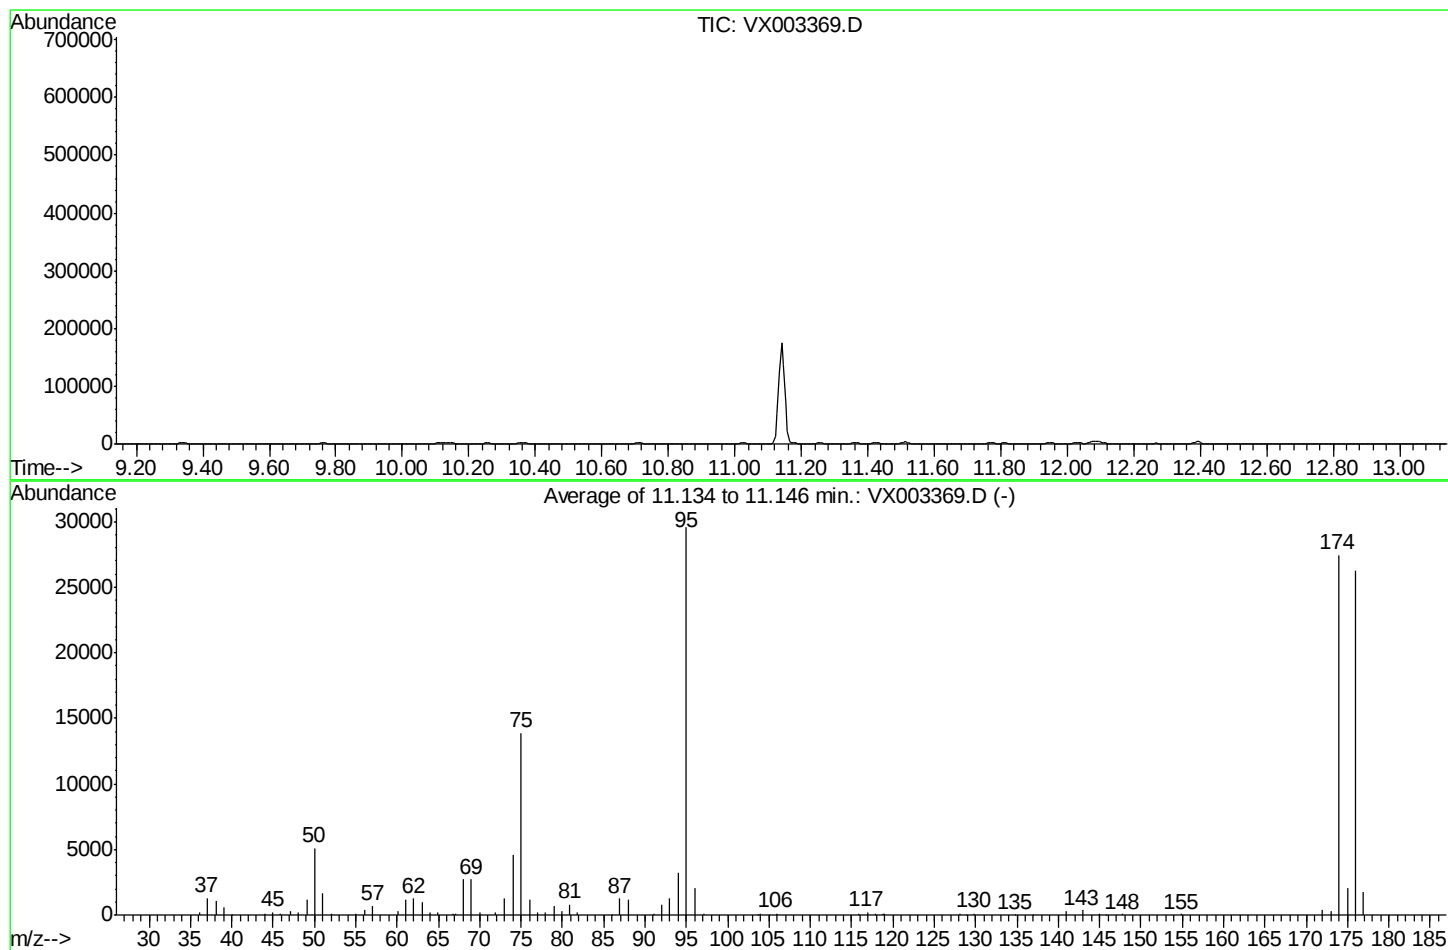

AutoFind: Scans 1730, 1731, 1732; Background Corrected with Scan 1724

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.3	5104	PASS
75	95	30	60	46.9	13865	PASS
95	95	100	100	100.0	29568	PASS
96	95	5	9	6.8	2018	PASS
173	174	0.00	2	1.0	269	PASS
174	95	50	100	92.8	27453	PASS
175	174	5	9	7.5	2050	PASS
176	174	95	101	95.8	26293	PASS
177	176	5	9	6.8	1776	PASS