

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071322\
Data File : VX030042.D
Acq On : 13 Jul 2022 14:08
Operator : JC/MD
Sample : N3695-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SPC-01C-84

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X071222W.M
Title : SW846 8260

Signal : TIC: VX030042.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.495	547	559	572	rBV	226305	616984	25.51%	7.857%
2	5.391	694	706	721	rBV	103289	302828	12.52%	3.856%
3	5.556	721	733	749	rVB	181748	513281	21.22%	6.536%
4	5.958	790	799	813	rBV2	110454	296381	12.25%	3.774%
5	6.769	920	932	944	rBV	283834	687710	28.43%	8.757%
6	7.129	983	991	1003	rBV	46969	102439	4.24%	1.304%
7	8.653	1231	1241	1251	rBV	600267	912695	37.73%	11.622%
8	9.275	1336	1343	1353	rBV	1663878	2418846	100.00%	30.802%
9	10.055	1466	1471	1483	rBV	581374	778903	32.20%	9.919%
10	11.085	1634	1640	1646	rBV	418611	544802	22.52%	6.938%
11	12.024	1789	1794	1804	rVB	562196	677991	28.03%	8.634%




Sum of corrected areas: 7852860

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071322\
Data File : VX030042.D
Acq On : 13 Jul 2022 14:08
Operator : JC/MD
Sample : N3695-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SPC-01C-84

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X071222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

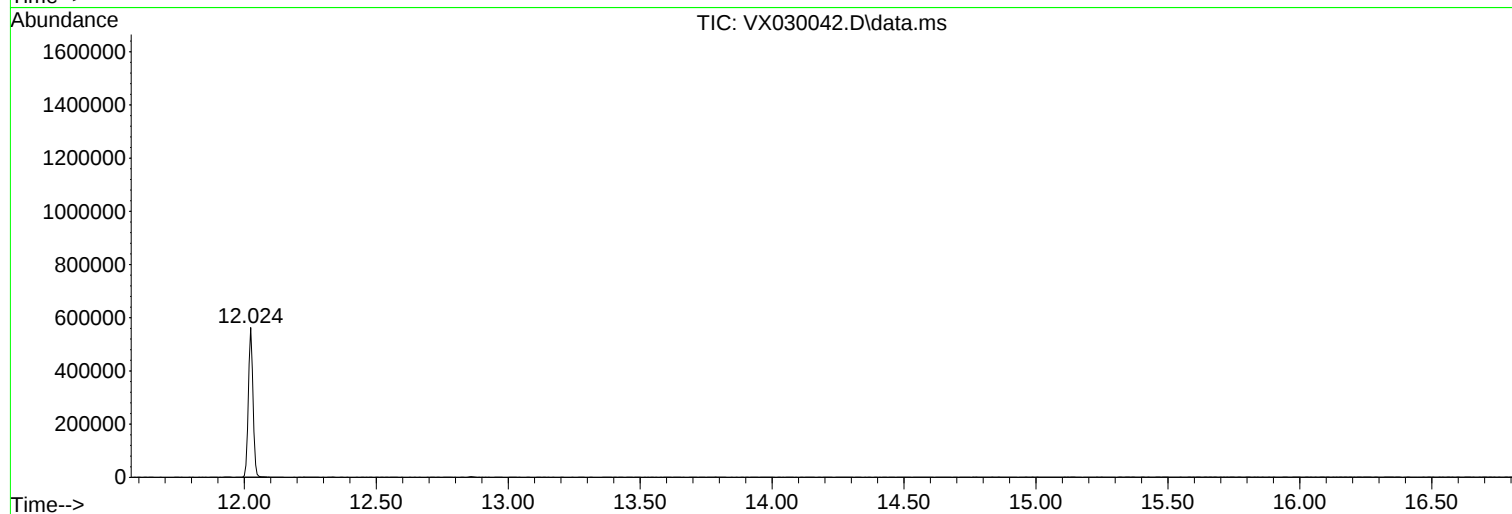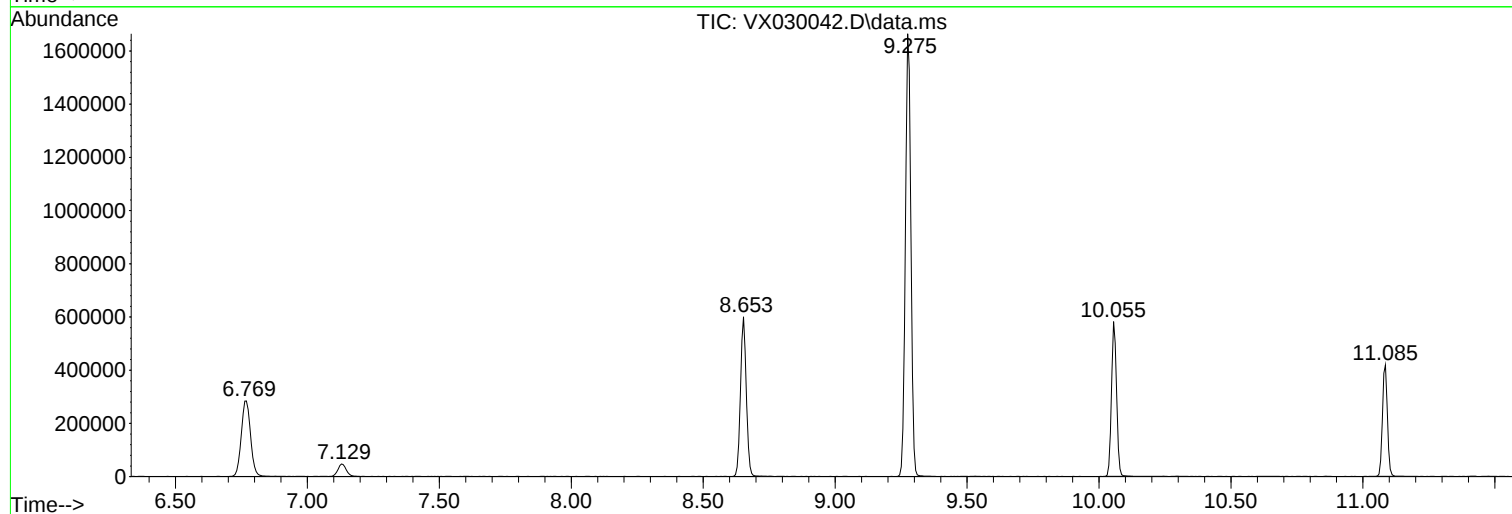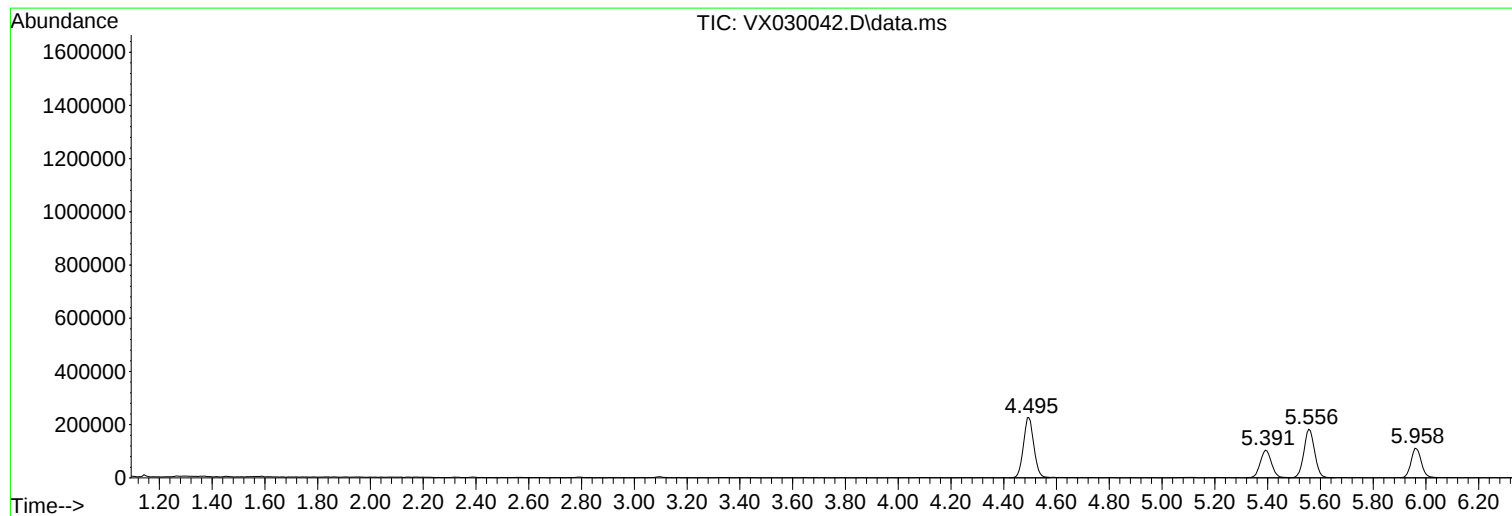

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071322\
Data File : VX030042.D
Acq On : 13 Jul 2022 14:08
Operator : JC/MD
Sample : N3695-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SPC-01C-84

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X071222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071322\
Data File : VX030042.D
Acq On : 13 Jul 2022 14:08
Operator : JC/MD
Sample : N3695-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SPC-01C-84

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X071222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc