

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071323\
 Data File : VX036518.D
 Acq On : 13 Jul 2023 10:48
 Operator : JC/MD
 Sample : VX0713MBL01
 Misc : 5.0g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK635

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML071223WMA.M

Title : VOC Analysis

Signal : TIC: VX036518.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.264	26	29	31	rBV2	1708	1588	0.15%	0.018%
2	1.368	42	46	61	rVB	134263	169382	15.47%	1.967%
3	1.666	91	95	112	rVB	116950	176043	16.08%	2.045%
4	2.306	193	200	211	rBV	254096	389993	35.63%	4.529%
5	2.514	228	234	238	rVB3	757	1635	0.15%	0.019%
6	2.599	247	248	253	rBV2	266	280	0.03%	0.003%
7	2.788	273	279	286	rBV4	2417	4133	0.38%	0.048%
8	2.934	300	303	305	rBV	415	413	0.04%	0.005%
9	3.087	325	328	329	rBV	397	419	0.04%	0.005%
10	3.514	396	398	401	rVB	237	198	0.02%	0.002%
11	3.544	401	403	405	rBV2	184	196	0.02%	0.002%
12	3.611	412	414	416	rBV2	259	239	0.02%	0.003%
13	3.636	416	418	419	rBV	263	215	0.02%	0.002%
14	3.696	426	428	429	rBV	216	201	0.02%	0.002%
15	3.745	434	436	438	rVV2	228	222	0.02%	0.003%
16	4.452	542	552	565	rBV	80204	229101	20.93%	2.661%
17	4.715	593	595	596	rBV	416	330	0.03%	0.004%
18	4.794	605	608	609	rBV	377	366	0.03%	0.004%
19	4.861	615	619	625	rBV2	368	908	0.08%	0.011%
20	5.056	638	651	671	rBV	144935	458357	41.87%	5.323%
21	5.379	698	704	705	rBV2	1413	2142	0.20%	0.025%
22	5.556	725	733	740	rBV3	2592	7167	0.65%	0.083%
23	5.727	760	761	764	rVB	379	233	0.02%	0.003%
24	5.970	788	801	818	rBV2	368828	1094705	100.00%	12.714%
25	6.269	846	850	853	rBV2	348	460	0.04%	0.005%
26	6.312	856	857	859	rBV	304	273	0.02%	0.003%
27	6.672	914	916	920	rBV	182	225	0.02%	0.003%
28	6.757	921	930	948	rVV	302646	717987	65.59%	8.339%
29	6.940	959	960	963	rVB	346	202	0.02%	0.002%
30	7.001	968	970	971	rBV	387	271	0.02%	0.003%
31	7.062	979	980	982	rVB2	449	314	0.03%	0.004%
32	7.104	982	987	996	rBV6	4438	10199	0.93%	0.118%
33	7.196	1000	1002	1004	rBV	568	550	0.05%	0.006%
34	7.306	1011	1020	1035	rBV	226845	496048	45.31%	5.761%
35	7.476	1044	1048	1052	rVB2	627	851	0.08%	0.010%
36	7.617	1069	1071	1073	rBV	317	287	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071323\
 Data File : VX036518.D
 Acq On : 13 Jul 2023 10:48
 Operator : JC/MD
 Sample : VX0713MBL01
 Misc : 5.0g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK635

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML071223WMA.M
 Title : VOC Analysis

37	7.677	1080	1081	1084	rBV	254	237	0.02%	0.003%
38	7.836	1104	1107	1108	rBV	232	230	0.02%	0.003%
39	7.879	1111	1114	1117	rBV2	240	342	0.03%	0.004%
40	7.927	1117	1122	1124	rBV2	1392	1973	0.18%	0.023%
41	8.031	1136	1139	1143	rVB2	246	235	0.02%	0.003%
42	8.092	1147	1149	1152	rBV2	190	205	0.02%	0.002%
43	8.129	1153	1155	1158	rVV	230	236	0.02%	0.003%
44	8.190	1161	1165	1166	rVB2	185	215	0.02%	0.002%
45	8.324	1180	1187	1201	rBV	156463	256344	23.42%	2.977%
46	8.482	1206	1213	1222	rVB4	1159	2752	0.25%	0.032%
47	8.647	1233	1240	1251	rBV	583438	897894	82.02%	10.428%
48	8.824	1266	1269	1272	rVB2	297	337	0.03%	0.004%
49	8.952	1284	1290	1302	rVB	111781	169173	15.45%	1.965%
50	9.043	1302	1305	1307	rVB	402	380	0.03%	0.004%
51	9.067	1307	1309	1314	rBV2	295	452	0.04%	0.005%
52	9.269	1340	1342	1345	rVB2	654	565	0.05%	0.007%
53	9.384	1355	1361	1375	rVV	356092	502349	45.89%	5.834%
54	9.701	1410	1413	1418	rVB2	882	1045	0.10%	0.012%
55	9.890	1442	1444	1446	rVV2	219	195	0.02%	0.002%
56	10.055	1465	1471	1483	rBV	628250	853605	77.98%	9.914%
57	10.305	1508	1512	1515	rBV3	511	580	0.05%	0.007%
58	10.348	1517	1519	1522	rBV2	247	242	0.02%	0.003%
59	10.732	1581	1582	1584	rBV	306	203	0.02%	0.002%
60	10.884	1605	1607	1608	rBV2	242	210	0.02%	0.002%
61	10.957	1617	1619	1624	rVB3	251	408	0.04%	0.005%
62	10.994	1624	1625	1628	rBV	302	234	0.02%	0.003%
63	11.085	1635	1640	1645	rBV	5297	7254	0.66%	0.084%
64	11.189	1652	1657	1664	rBV	402672	522935	47.77%	6.074%
65	11.335	1677	1681	1684	rBV2	165	283	0.03%	0.003%
66	11.457	1698	1701	1703	rVB2	510	601	0.05%	0.007%
67	11.616	1725	1727	1730	rBV2	216	225	0.02%	0.003%
68	11.707	1739	1742	1747	rBV	244	455	0.04%	0.005%
69	11.750	1747	1749	1754	rVB2	561	557	0.05%	0.006%
70	11.975	1782	1786	1788	rBV3	772	937	0.09%	0.011%
71	12.024	1788	1794	1805	rBV	657826	836053	76.37%	9.710%
72	12.177	1818	1819	1822	rVB2	319	278	0.03%	0.003%
73	12.225	1822	1827	1829	rBV	504	729	0.07%	0.008%
74	12.317	1837	1842	1849	rBV	597189	770185	70.36%	8.945%
75	12.445	1859	1863	1865	rVB2	359	476	0.04%	0.006%
76	12.481	1865	1869	1872	rBV2	256	309	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071323\
 Data File : VX036518.D
 Acq On : 13 Jul 2023 10:48
 Operator : JC/MD
 Sample : VX0713MBL01
 Misc : 5.0g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK635

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML071223WMA.M
 Title : VOC Analysis

77	12.524	1875	1876	1878	rBV	229	224	0.02%	0.003%
78	12.610	1887	1890	1892	rBV2	239	298	0.03%	0.003%
79	12.896	1936	1937	1939	rBV	288	229	0.02%	0.003%
80	13.109	1970	1972	1976	rBV3	844	914	0.08%	0.011%
81	13.463	2028	2030	2033	rBV	278	303	0.03%	0.004%
82	13.542	2042	2043	2046	rBV2	209	237	0.02%	0.003%
83	13.591	2046	2051	2055	rVV4	1084	1698	0.16%	0.020%
84	13.646	2057	2060	2062	rBV	227	257	0.02%	0.003%
85	13.756	2076	2078	2079	rBV	351	237	0.02%	0.003%
86	13.774	2079	2081	2086	rVB	833	1066	0.10%	0.012%
87	14.121	2136	2138	2146	rVB3	791	1223	0.11%	0.014%
88	14.262	2158	2161	2162	rBV2	334	287	0.03%	0.003%
89	14.457	2192	2193	2194	rBV	467	247	0.02%	0.003%
90	14.701	2230	2233	2236	rBV2	540	573	0.05%	0.007%
91	14.841	2255	2256	2257	rBV	543	220	0.02%	0.003%
92	15.005	2282	2283	2288	rBV2	407	333	0.03%	0.004%
93	15.231	2318	2320	2321	rBV	554	343	0.03%	0.004%
94	15.268	2324	2326	2330	rVV3	366	427	0.04%	0.005%
95	15.298	2330	2331	2332	rBV	529	204	0.02%	0.002%
96	15.389	2343	2346	2347	rBV2	569	605	0.06%	0.007%
97	15.755	2404	2406	2409	rBV4	662	881	0.08%	0.010%
98	15.828	2417	2418	2420	rVB2	457	291	0.03%	0.003%
99	16.225	2480	2483	2486	rBV3	619	661	0.06%	0.008%
100	16.432	2515	2517	2518	rBV	524	273	0.02%	0.003%

Sum of corrected areas: 8610082




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071323\
Data File : VX036518.D
Acq On : 13 Jul 2023 10:48
Operator : JC/MD
Sample : VX0713MBL01
Misc : 5.0g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK635

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML071223WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

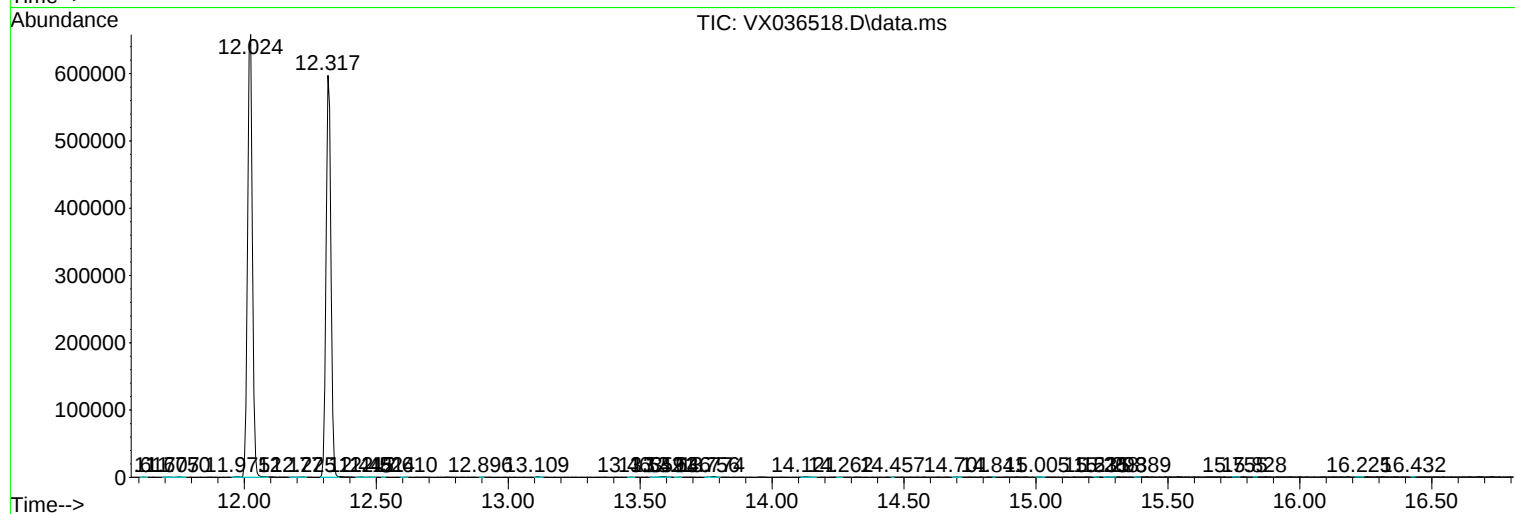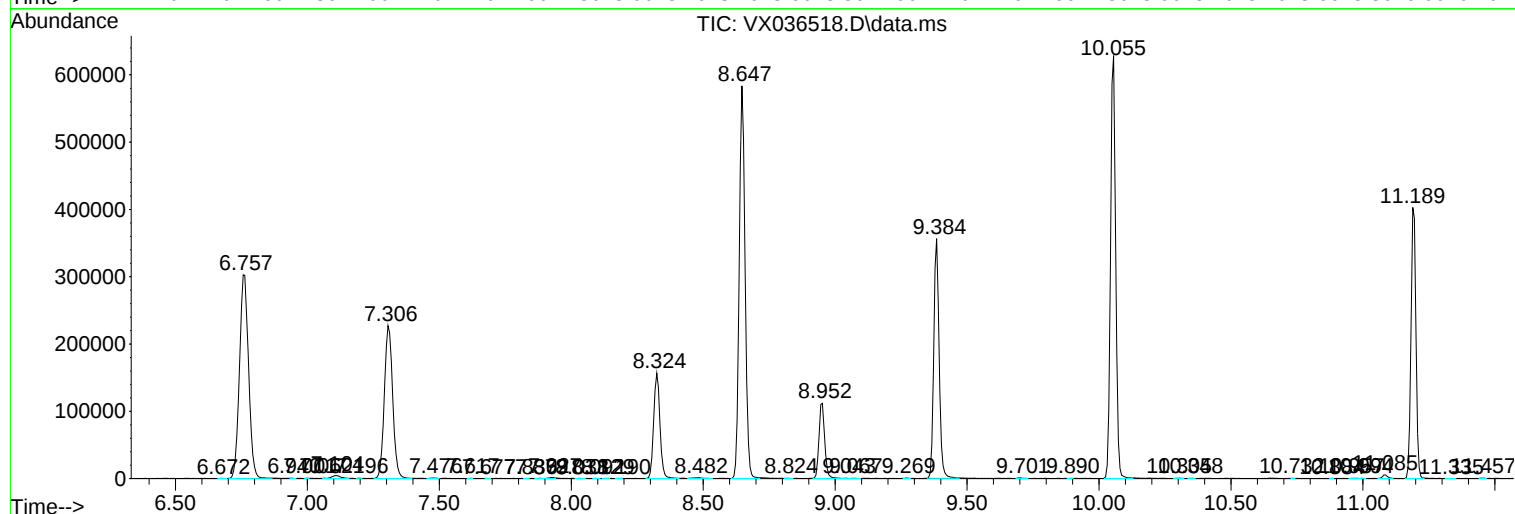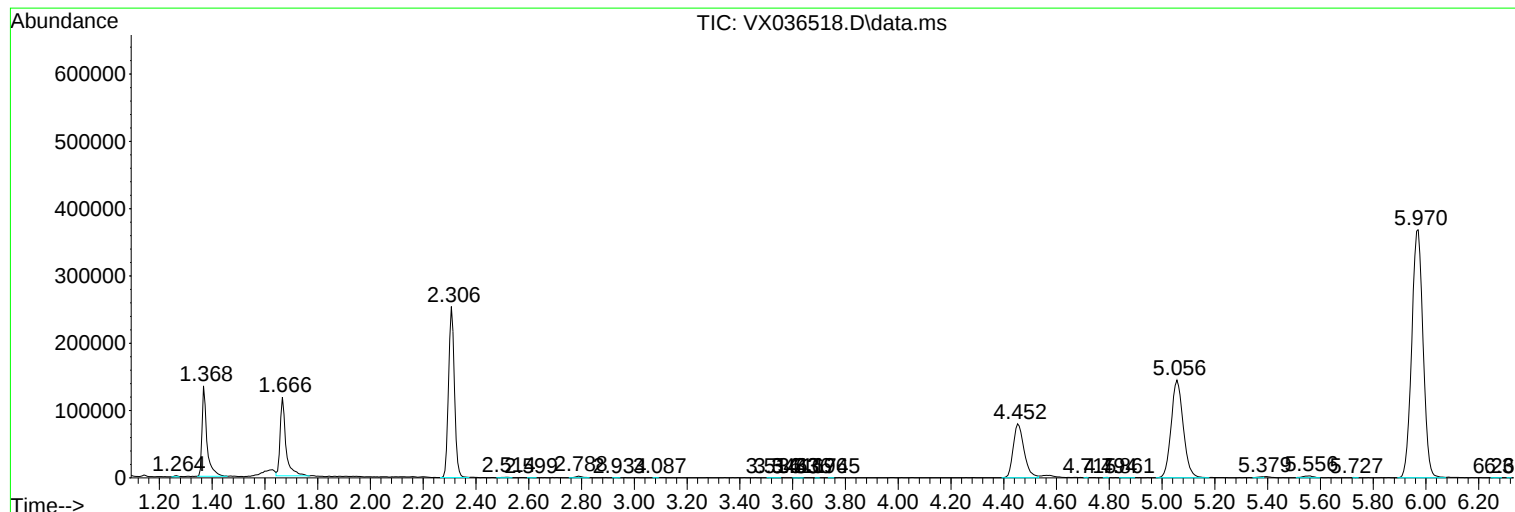

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071323\
Data File : VX036518.D
Acq On : 13 Jul 2023 10:48
Operator : JC/MD
Sample : VX0713MBL01
Misc : 5.0g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK635

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML071223WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071323\
Data File : VX036518.D
Acq On : 13 Jul 2023 10:48
Operator : JC/MD
Sample : VX0713MBL01
Misc : 5.0g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK635

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML071223WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc