
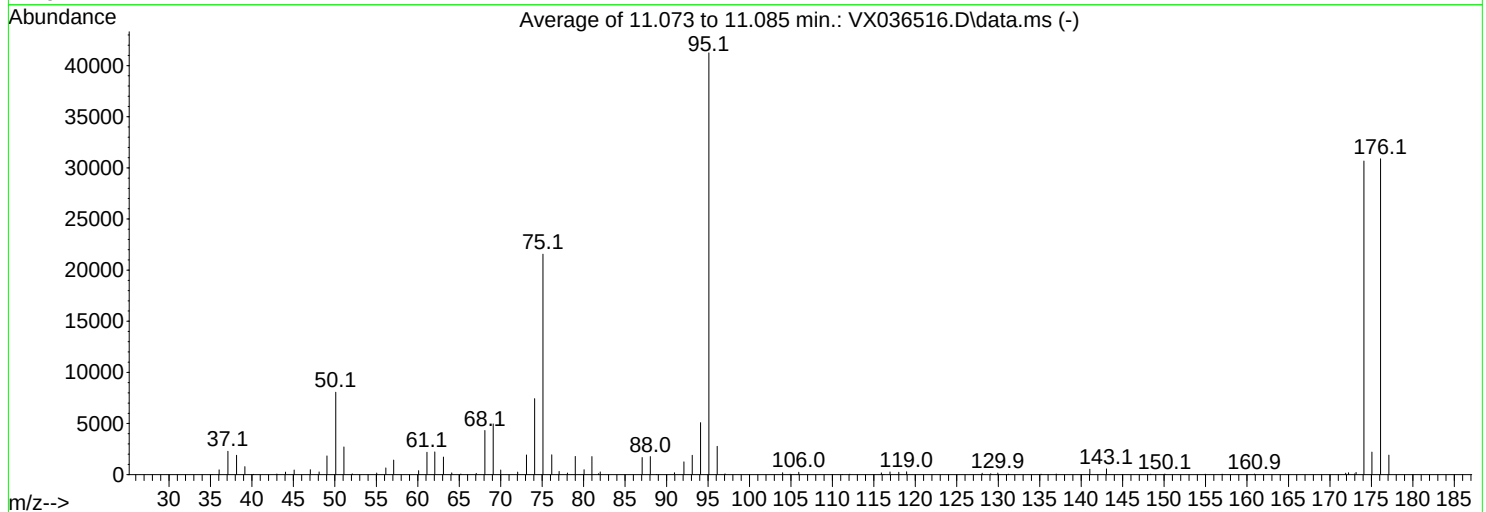


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071323\
Data File : VX036516.D
Acq On : 13 Jul 2023 09:14
Operator : JC/MD
Sample : BFB642
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB642

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM071223WMA.M
Title : VOC Analysis
Last Update : Fri Jul 14 07:34:36 2023

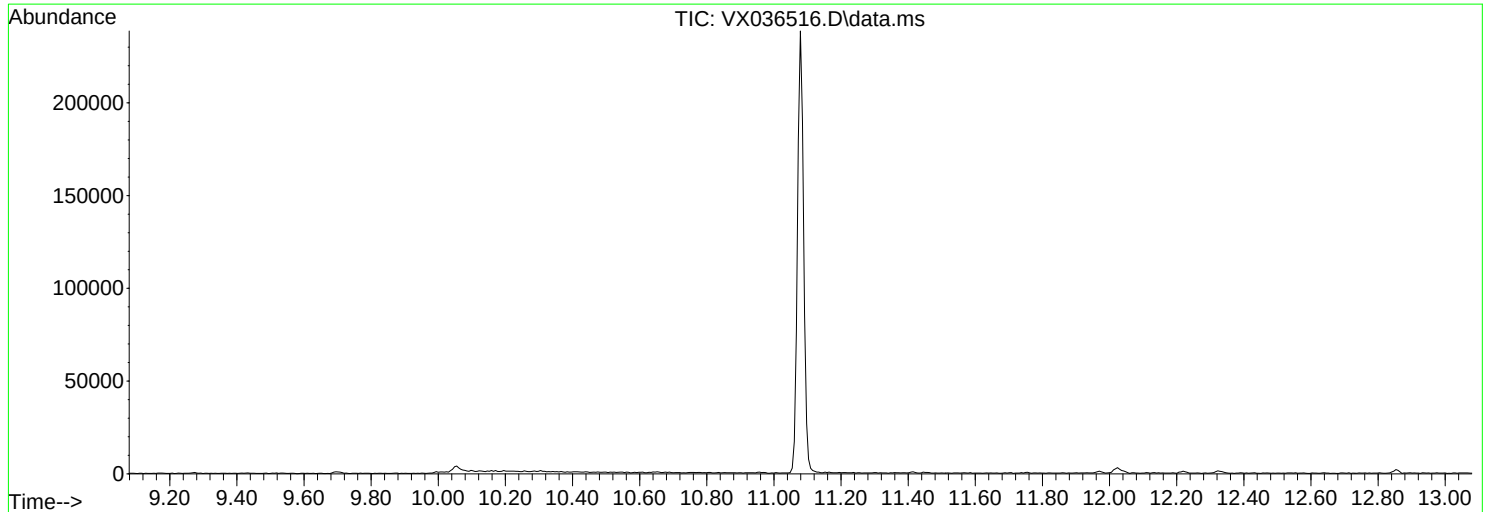

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.5	8061	PASS
75	95	30	80	52.3	21563	PASS
95	95	100	100	100.0	41248	PASS
96	95	5	9	6.7	2769	PASS
173	174	0.00	2	0.7	222	PASS
174	95	50	120	74.4	30669	PASS
175	174	5	9	7.2	2201	PASS
176	174	95	101	100.7	30885	PASS
177	176	5	9	6.2	1912	PASS

m/z	Abundance
36.10	140.0
40.10	151.0
44.10	221.0

Instrument :
MSVOA_X
ClientSampleId :
BFB642

m/z	Abundance
36.10	478.0
37.10	2077.0
38.20	1745.0
39.20	743.0
40.00	178.0
44.00	447.0
45.10	533.0
47.00	565.0
48.20	255.0
49.00	1915.0
50.10	8302.0
51.10	2734.0
52.10	167.0
55.10	217.0
56.20	601.0
57.10	1317.0
60.10	290.0
61.10	2470.0
62.00	2062.0
63.10	1621.0
64.10	206.0
65.20	113.0
67.10	140.0
68.10	3829.0
69.10	4944.0
70.00	465.0
72.00	289.0
73.10	1716.0
74.10	7327.0
75.10	20696.0
76.20	1843.0
77.10	362.0
78.10	78.0
79.00	1738.0
80.10	385.0
81.00	1571.0
81.80	282.0
87.00	1535.0
88.10	1774.0
91.00	144.0
92.10	1123.0
93.20	1603.0
94.10	4463.0
95.10	36456.0
96.10	2620.0
97.10	55.0
104.10	222.0
104.90	64.0
106.00	278.0
112.10	59.0
116.00	208.0
117.00	368.0
118.00	221.0
119.00	313.0
128.00	114.0
129.10	78.0
130.00	118.0
131.20	53.0
135.10	75.0
141.10	458.0
143.00	436.0
148.40	63.0
157.00	57.0
160.90	71.0
172.20	135.0
173.00	237.0
174.10	23856.0
175.10	1835.0
176.10	24480.0
177.10	1463.0

Instrument :
MSVOA_X
ClientSampleId :
BFB642

m/z	Abundance
36.10	709.0
37.10	2965.0
38.10	2504.0
39.10	951.0
40.00	114.0
43.00	104.0
44.00	592.0
45.10	566.0
47.10	564.0
48.10	335.0
49.10	2107.0
50.10	9233.0
51.10	2903.0
52.10	60.0
55.00	94.0
56.10	767.0
57.10	1739.0
60.10	609.0
61.10	2508.0
62.10	2867.0
63.10	2137.0
64.10	254.0
67.00	99.0
68.10	5321.0
69.10	5896.0
70.00	453.0
72.10	227.0
73.10	2346.0
74.10	8802.0
75.10	25456.0
76.10	1980.0
77.00	312.0
78.00	188.0
79.00	1944.0
79.90	485.0
81.00	2197.0
82.00	545.0
87.10	2007.0
88.10	1912.0
90.90	232.0
92.10	1040.0
93.10	2321.0
94.10	6040.0
95.10	50312.0
96.10	3197.0
97.10	107.0
103.90	200.0
104.90	55.0
105.90	278.0
111.20	52.0
112.10	104.0
115.00	51.0
115.90	223.0
116.90	254.0
118.10	281.0
119.00	339.0
128.00	173.0
129.10	135.0
129.90	171.0
131.20	98.0
135.20	62.0
137.00	83.0
141.10	684.0
143.10	542.0
148.40	67.0
150.10	89.0
155.00	78.0
157.00	75.0
160.90	107.0
171.90	203.0
172.30	201.0
173.20	339.0
174.10	35640.0
175.00	2209.0
176.10	35296.0
177.10	2501.0

Instrument :
MSVOA_X
ClientSampleId :
BFB642

m/z	Abundance
35.20	56.0
36.00	625.0
37.10	1807.0
38.10	1428.0
39.10	655.0
40.20	83.0
43.00	107.0
44.10	393.0
45.10	288.0
47.00	319.0
48.00	221.0
49.10	1473.0
50.10	6649.0
51.10	2501.0
55.00	161.0
56.10	618.0
57.10	1201.0
60.00	281.0
61.00	1598.0
62.10	1753.0
63.10	1408.0
64.10	72.0
65.20	58.0
67.00	129.0
68.10	3820.0
69.10	4055.0
70.00	463.0
72.10	238.0
73.10	1707.0
74.10	6158.0
75.10	18536.0
76.10	2024.0
77.10	283.0
78.10	227.0
79.00	1657.0
80.10	601.0
81.00	1564.0
82.00	277.0
87.00	1500.0
88.00	1619.0
88.80	65.0
91.00	188.0
92.10	1576.0
93.00	1760.0
94.10	4767.0
95.10	36976.0
96.10	2491.0
97.00	77.0
104.00	156.0
106.00	127.0
115.80	89.0
116.20	68.0
116.90	186.0
117.90	181.0
118.80	190.0
128.10	118.0
129.10	97.0
129.90	182.0
137.00	99.0
141.00	455.0
143.00	701.0
145.00	63.0
150.10	78.0
154.90	88.0
171.90	210.0
172.30	212.0
173.10	327.0
174.10	32512.0
175.10	2560.0
176.10	32880.0
177.10	1771.0

Instrument :
MSVOA_X
ClientSampleId :
BFB642