

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071421\
 Data File : VX023285.D
 Acq On : 14 Jul 2021 17:33
 Operator : JC/MD
 Sample : M3026-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 ABN-JG-1

Quant Time: Jul 15 04:29:22 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X070221W.M
 Quant Title : SW846 8260
 QLast Update : Fri Jul 02 14:29:42 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.562	168	220940	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.769	114	363190	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	321659	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	135698	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.964	65	154800	52.131	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	104.260%
35) Dibromofluoromethane	5.397	113	66034	28.156	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	56.320%#
50) Toluene-d8	8.653	98	430943	49.258	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	98.520%
62) 4-Bromofluorobenzene	11.085	95	153561	45.466	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	90.940%
Target Compounds						
						Qvalue
16) Acetone	2.386	43	109457	93.171	ug/l	91
20) Methylene Chloride	2.794	84	19826	7.838	ug/l	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071421\
Data File : VX023285.D
Acq On : 14 Jul 2021 17:33
Operator : JC/MD
Sample : M3026-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
ABN-JG-1

Quant Time: Jul 15 04:29:22 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X070221W.M
Quant Title : SW846 8260
QLast Update : Fri Jul 02 14:29:42 2021
Response via : Initial Calibration




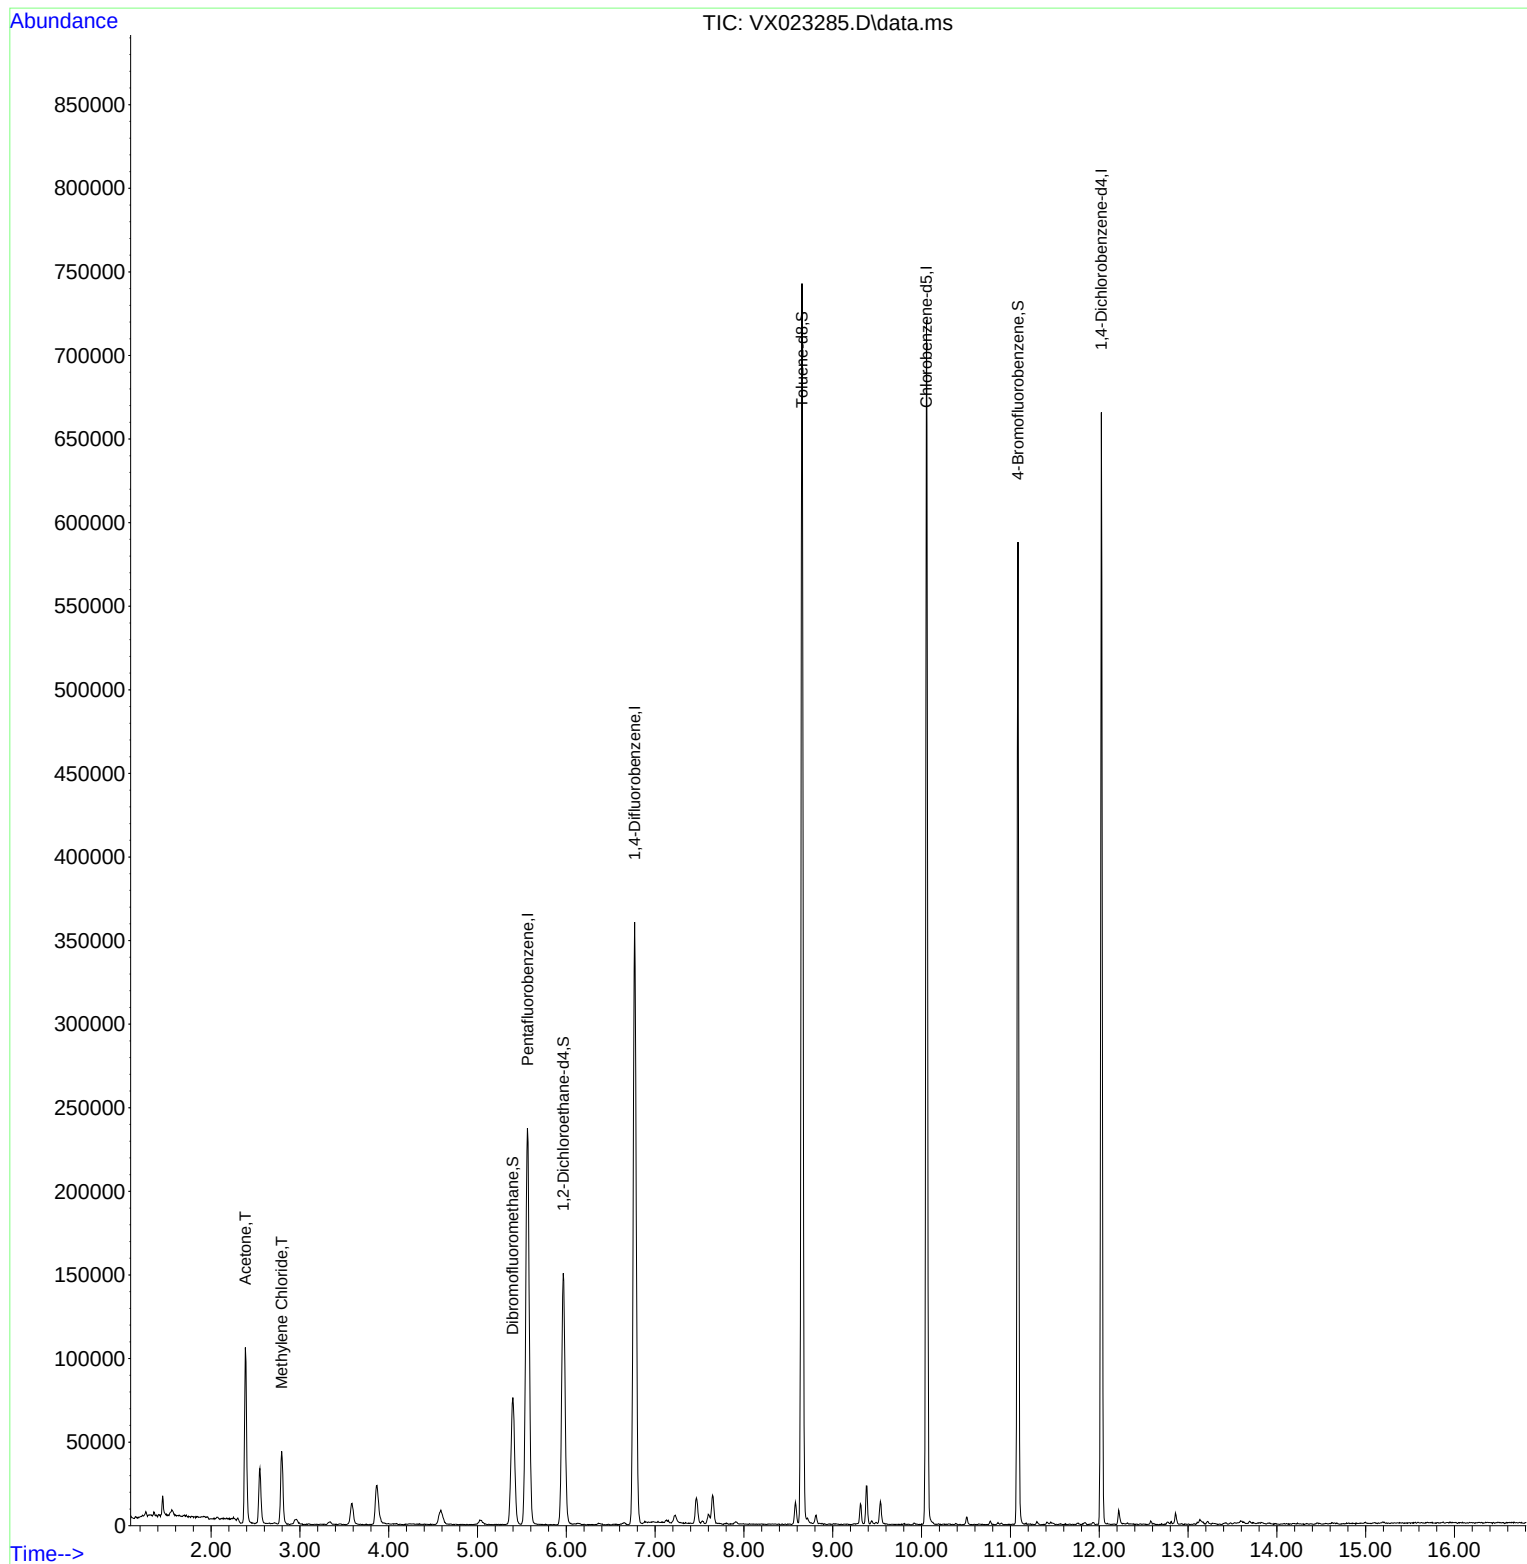


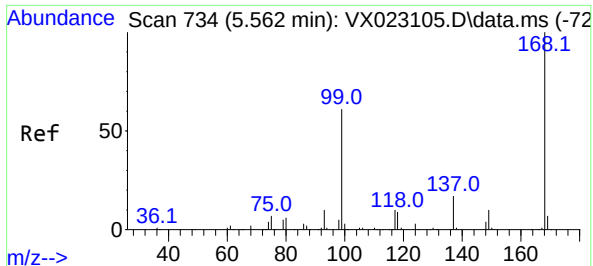

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.562 min Scan# 734
Delta R.T. -0.000 min
Lab File: VX023285.D
Acq: 14 Jul 2021 17:33




Instrument :
MSVOA_X
ClientSampled :
ABN-JG-1


Tgt Ion:168 Resp: 220940
Ion Ratio Lower Upper
168 100
99 60.2 45.8 68.6

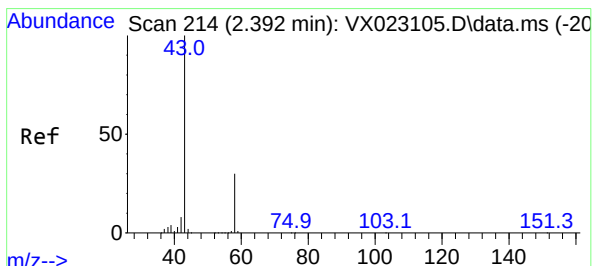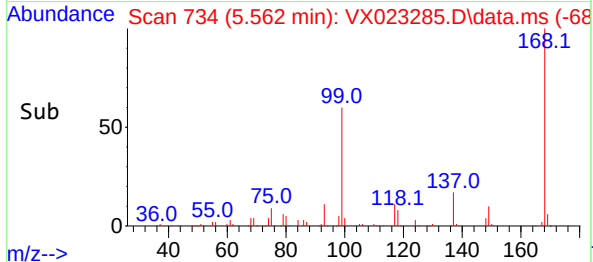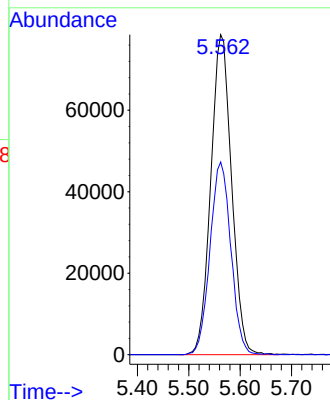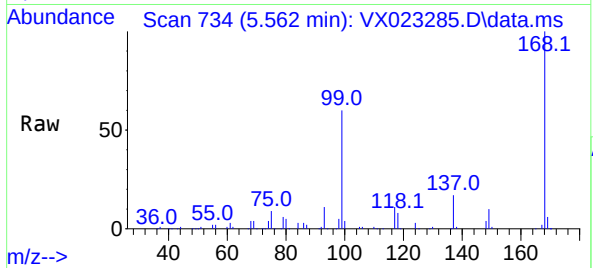

#16
Acetone
Concen: 93.171 ug/l
RT: 2.386 min Scan# 213
Delta R.T. -0.006 min
Lab File: VX023285.D
Acq: 14 Jul 2021 17:33

Tgt Ion: 43 Resp: 109457
Ion Ratio Lower Upper
43 100
58 29.5 27.8 41.8

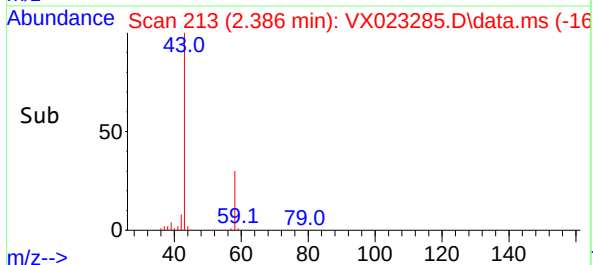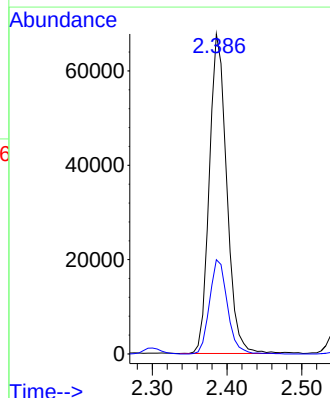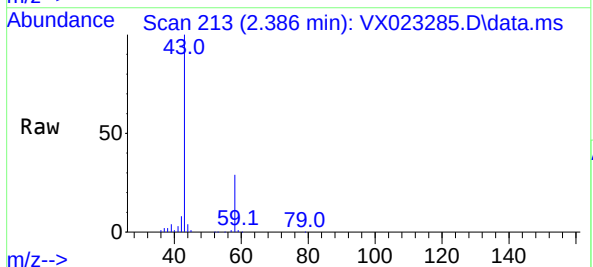




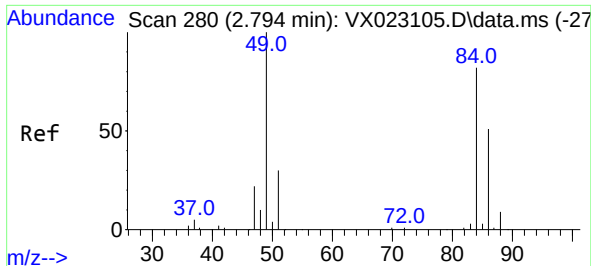


#20
Methylene Chloride
Concen: 7.838 ug/l
RT: 2.794 min Scan# 280
Delta R.T. 0.000 min
Lab File: VX023285.D
Acq: 14 Jul 2021 17:33

Instrument :
MSVOA_X
ClientSampleId :
ABN-JG-1

Tgt Ion: 84 Resp: 19826




Ion	Ratio	Lower	Upper
84	100		
49	126.2	88.6	132.8
51	39.4	27.0	40.6
86	70.4	50.3	75.5

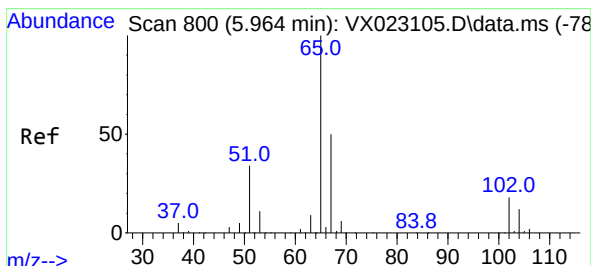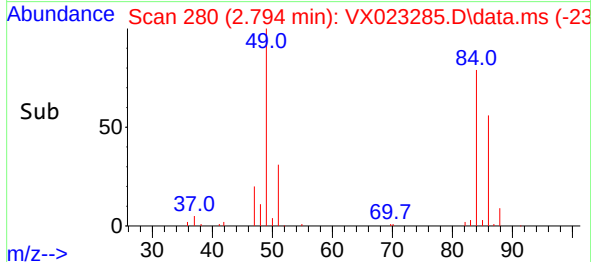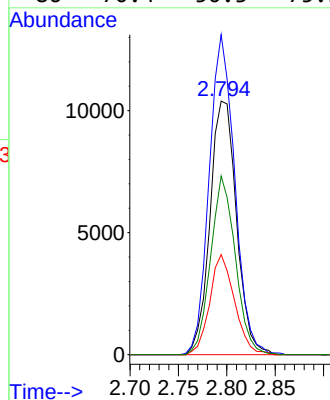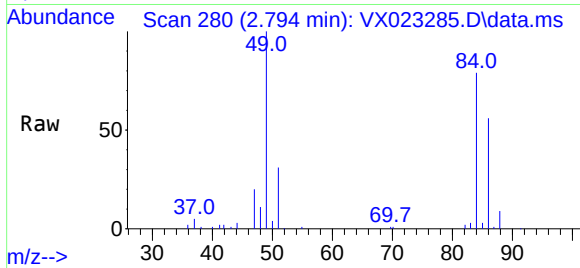


#33
1,2-Dichloroethane-d4
Concen: 52.131 ug/l
RT: 5.964 min Scan# 800
Delta R.T. 0.000 min
Lab File: VX023285.D
Acq: 14 Jul 2021 17:33

Tgt Ion: 65 Resp: 154800

Ion	Ratio	Lower	Upper
65	100		
67	49.7	0.0	105.4


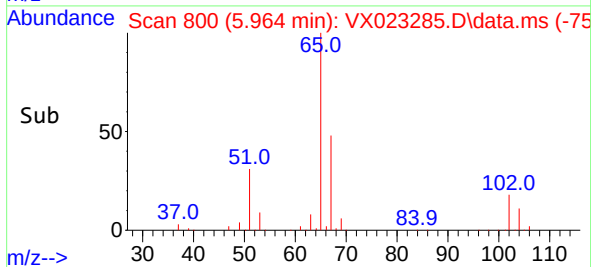
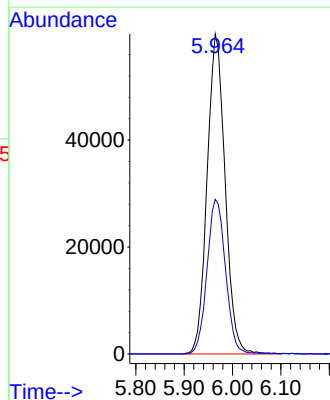
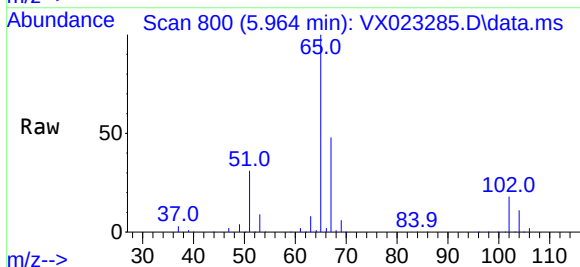


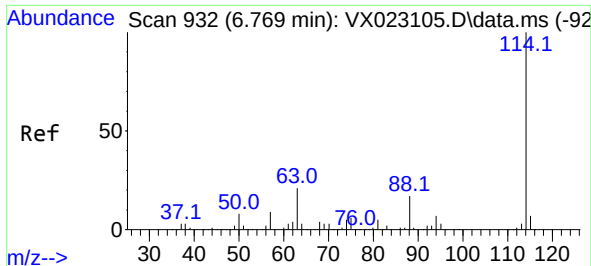

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.769 min Scan# 932
Delta R.T. 0.000 min
Lab File: VX023285.D
Acq: 14 Jul 2021 17:33




Instrument :
MSVOA_X
ClientSampleId :
ABN-JG-1


Tgt Ion:114 Resp: 363190
Ion Ratio Lower Upper
114 100
63 20.5 0.0 40.8
88 16.5 0.0 32.8

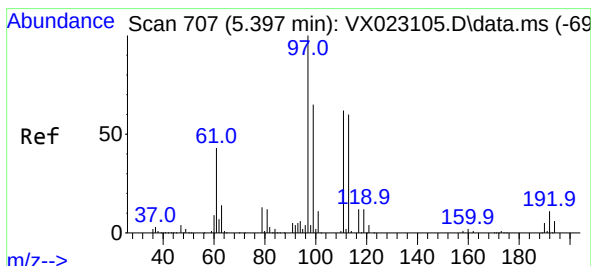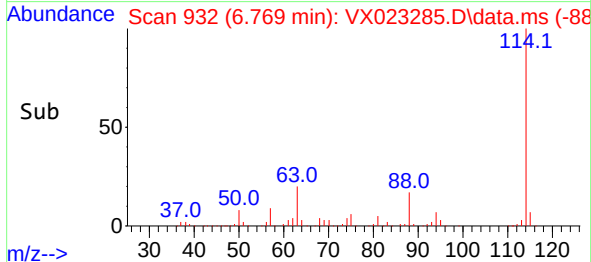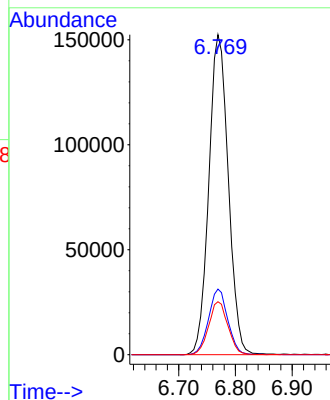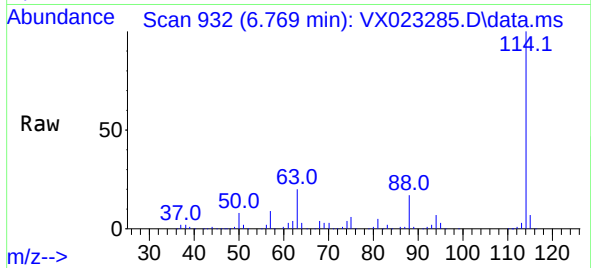

#35
Dibromofluoromethane
Concen: 28.156 ug/l
RT: 5.397 min Scan# 707
Delta R.T. 0.000 min
Lab File: VX023285.D
Acq: 14 Jul 2021 17:33

Tgt Ion:113 Resp: 66034
Ion Ratio Lower Upper
113 100
111 103.4 81.9 122.9
192 19.5 16.7 25.1


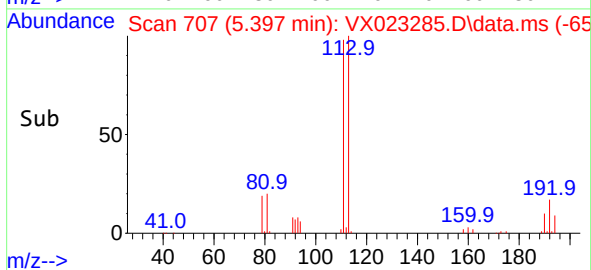
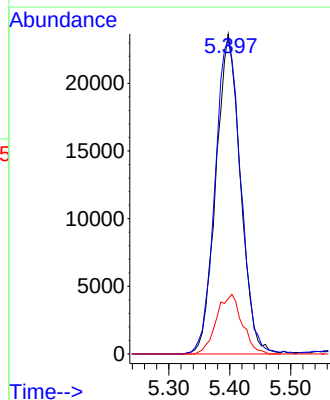
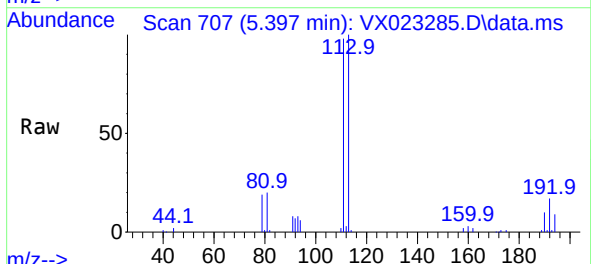


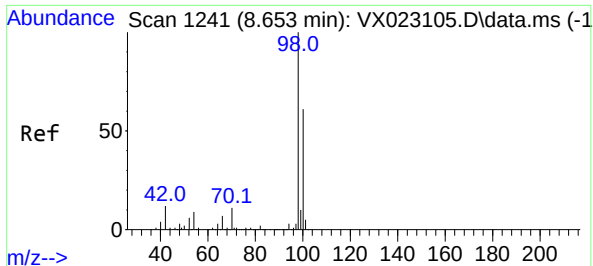

#50
Toluene-d8
Concen: 49.258 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. -0.000 min
Lab File: VX023285.D
Acq: 14 Jul 2021 17:33




Instrument :
MSVOA_X
ClientSampleId :
ABN-JG-1


Tgt Ion: 98 Resp: 430943
Ion Ratio Lower Upper
98 100
100 64.0 51.9 77.9

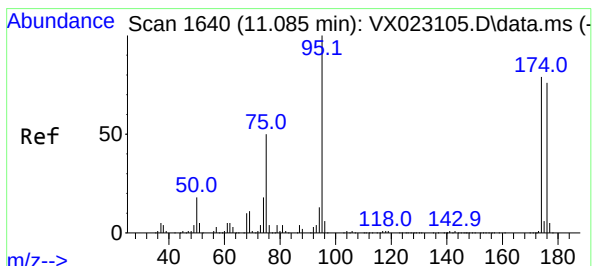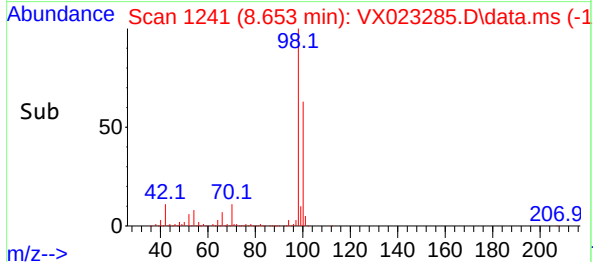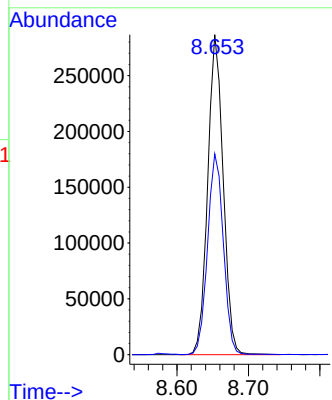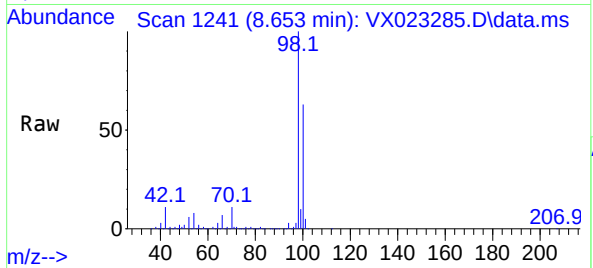

#62
4-Bromofluorobenzene
Concen: 45.466 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.000 min
Lab File: VX023285.D
Acq: 14 Jul 2021 17:33

Tgt Ion: 95 Resp: 153561
Ion Ratio Lower Upper
95 100
174 78.1 0.0 154.6
176 74.4 0.0 155.8


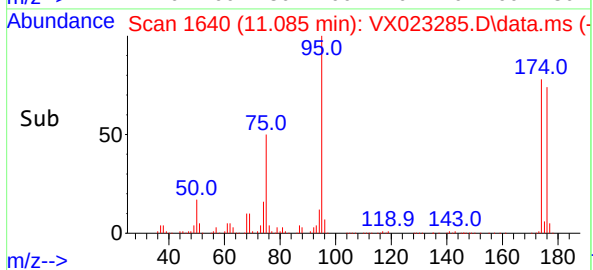
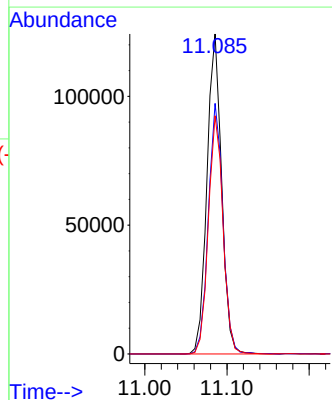
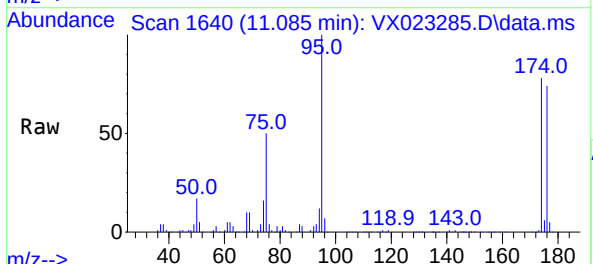


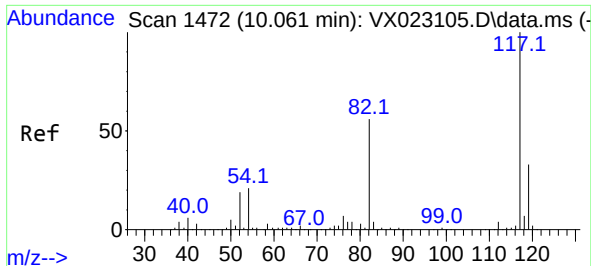

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.006 min
Lab File: VX023285.D
Acq: 14 Jul 2021 17:33

Instrument :
MSVOA_X
ClientSampleId :
ABN-JG-1

Tgt Ion:117 Resp: 321659
Ion Ratio Lower Upper
117 100
82 58.0 47.4 71.2
119 31.4 26.6 39.8

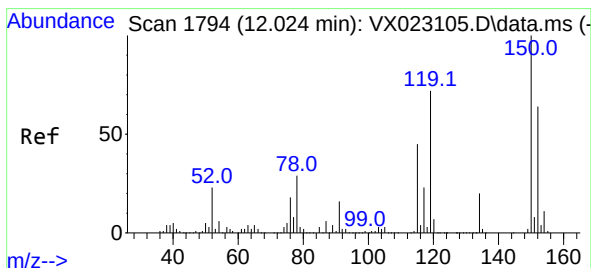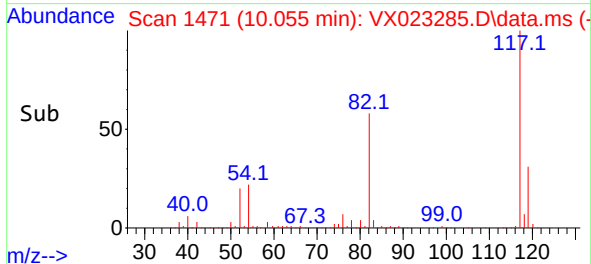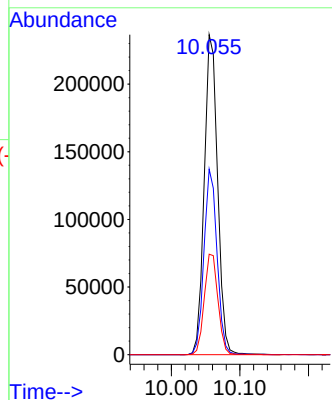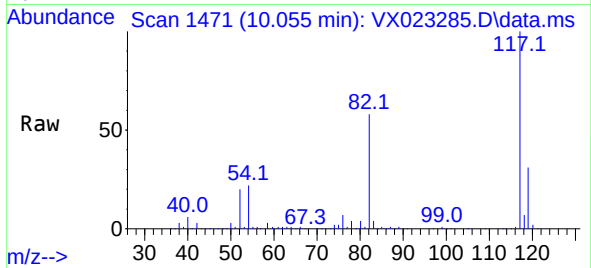

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX023285.D
Acq: 14 Jul 2021 17:33

Tgt Ion:152 Resp: 135698
Ion Ratio Lower Upper
152 100
115 61.0 41.1 123.3
150 156.4 0.0 349.0

