

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071422\
 Data File : VX030064.D
 Acq On : 14 Jul 2022 16:33
 Operator : JC/MD
 Sample : N3705-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TT-149S1-20220712

Quant Time: Jul 15 04:18:30 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X071222W.M
 Quant Title : SW846 8260
 QLast Update : Wed Jul 13 09:05:23 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.556	168	168873	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.769	114	291216	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	248568	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	101047	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.964	65	94800	46.120	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	92.240%
35) Dibromofluoromethane	5.391	113	85966	46.208	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	92.420%
50) Toluene-d8	8.653	98	327603	46.821	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	93.640%
62) 4-Bromofluorobenzene	11.085	95	105235	43.340	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	86.680%
Target Compounds						
					Qvalue	
2) Dichlorodifluoromethane	1.166	85	109	Below Cal	#	42
5) Bromomethane	1.617	94	273	0.329	ug/l	81
9) 1,1,2-Trichlorotrifluo...	2.324	101	425	0.247	ug/l #	82
10) Methyl Iodide	2.459	142	738	2.823	ug/l #	87
11) Tert butyl alcohol	2.977	59	418	0.788	ug/l #	74
12) 1,1-Dichloroethene	2.318	96	406	0.236	ug/l #	75
13) Acrolein	2.239	56	41	0.388	ug/l #	1
16) Acetone	2.392	43	1381	1.426	ug/l	91
17) Carbon Disulfide	2.507	76	1656	Below Cal	#	79
19) Methyl tert-butyl Ether	3.117	73	70783	13.015	ug/l	98
20) Methylene Chloride	2.788	84	258	Below Cal	#	79
22) Diisopropyl ether	3.769	45	4977	0.846	ug/l #	77
23) Vinyl Acetate	3.763	43	2964	0.595	ug/l #	72
24) 1,1-Dichloroethane	3.611	63	2759	0.846	ug/l #	83
27) cis-1,2-Dichloroethene	4.495	96	1436	0.654	ug/l	95
31) Cyclohexane	5.549	56	3397	1.140	ug/l #	20
36) 1,1-Dichloropropene	5.549	75	12798	5.326	ug/l #	45
38) Carbon Tetrachloride	5.556	117	15661	6.989	ug/l #	17
42) 1,2-Dichloroethane	6.098	62	2871	1.225	ug/l	95
44) Trichloroethene	7.128	130	18024	8.155	ug/l	94
49) 1,4-Dioxane	7.695	88	156	2.803	ug/l #	72
60) Dibromochloromethane	9.274	129	5371	2.784	ug/l #	11
64) Tetrachloroethene	9.274	164	5397	2.705	ug/l	94
76) 1,2,3-Trichloropropane	11.085	75	49064	21.118	ug/l #	37
81) trans-1,4-Dichloro-2-b...	11.085	75	49064	60.947	ug/l #	13
87) 1,3-Dichlorobenzene	11.975	146	655	0.201	ug/l	92
93) 1,2,4-Trichlorobenzene	13.591	180	646	0.318	ug/l	90
94) Hexachlorobutadiene	13.731	225	350	0.432	ug/l	87
95) Naphthalene	13.780	128	1691	0.210	ug/l #	87
96) 1,2,3-Trichlorobenzene	13.969	180	664	0.322	ug/l #	76


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071422\
Data File : VX030064.D
Acq On : 14 Jul 2022 16:33
Operator : JC/MD
Sample : N3705-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TT-149S1-20220712

Quant Time: Jul 15 04:18:30 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X071222W.M
Quant Title : SW846 8260
QLast Update : Wed Jul 13 09:05:23 2022
Response via : Initial Calibration




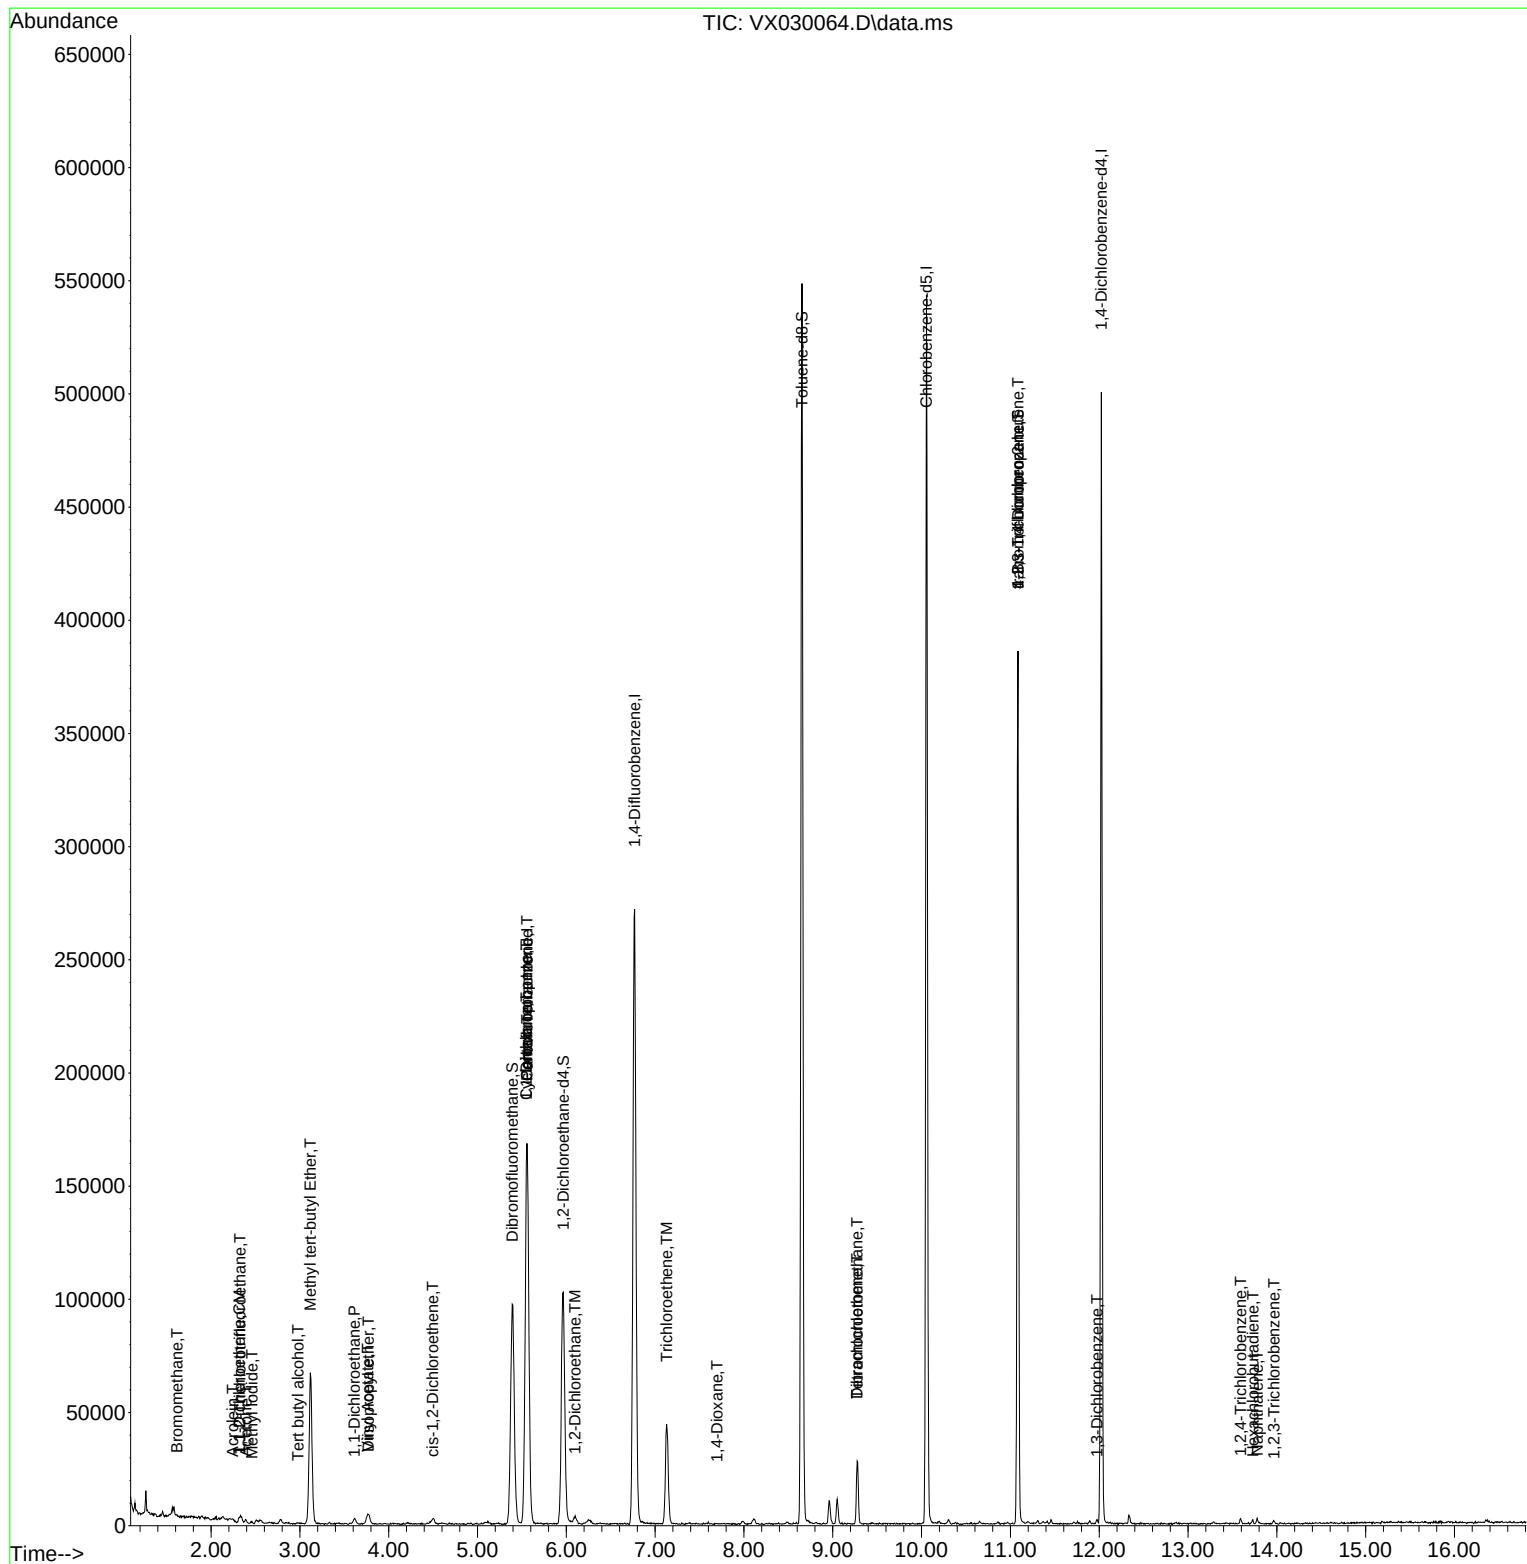




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX030064.D
Acq: 14 Jul 2022 16:33




Instrument :
MSVOA_X
ClientSampleId :
TT-149S1-20220712


Tgt Ion:168 Resp: 168873
Ion Ratio Lower Upper
168 100
99 51.7 44.0 66.0

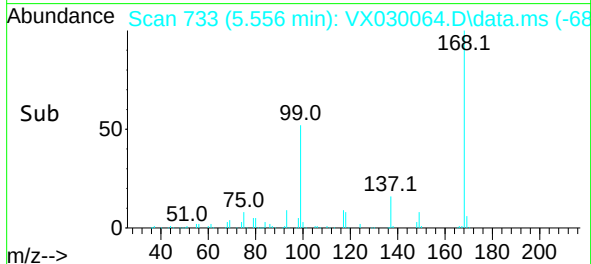

#2
Dichlorodifluoromethane
Concen: Below Cal
RT: 1.166 min Scan# 13
Delta R.T. 0.000 min
Lab File: VX030064.D
Acq: 14 Jul 2022 16:33

Tgt Ion: 85 Resp: 109
Ion Ratio Lower Upper
85 100
87 0.0 16.5 49.5#


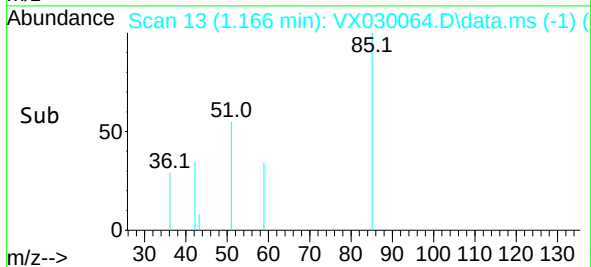

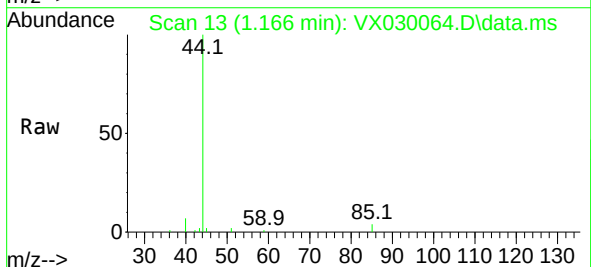


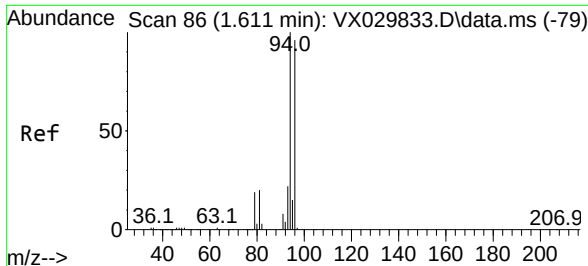

#5
Bromomethane
Concen: 0.329 ug/l
RT: 1.617 min Scan# 81
Delta R.T. 0.006 min
Lab File: VX030064.D
Acq: 14 Jul 2022 16:33




Instrument :
MSVOA_X
ClientSampleId :
TT-149S1-20220712


Tgt Ion: 94 Resp: 273
Ion Ratio Lower Upper
94 100
96 77.7 76.9 115.3

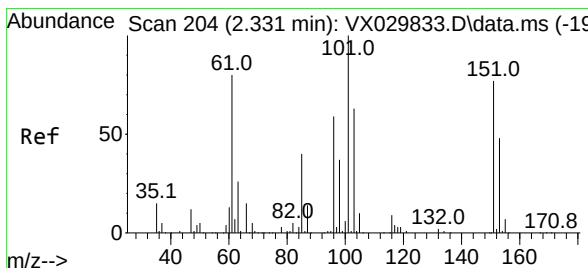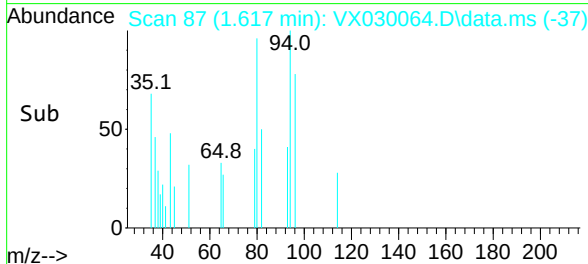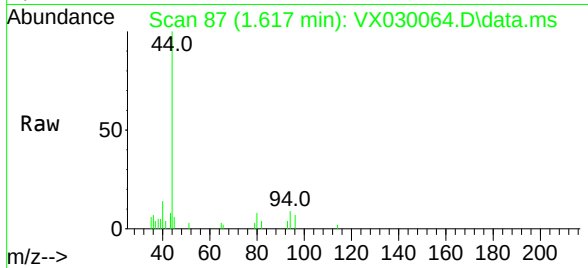

#9
1,1,2-Trichlorotrifluoroethane
Concen: 0.247 ug/l
RT: 2.324 min Scan# 203
Delta R.T. -0.007 min
Lab File: VX030064.D
Acq: 14 Jul 2022 16:33


Tgt Ion: 101 Resp: 425
Ion Ratio Lower Upper
101 100
85 27.5 34.0 51.0#
151 61.9 59.4 89.0

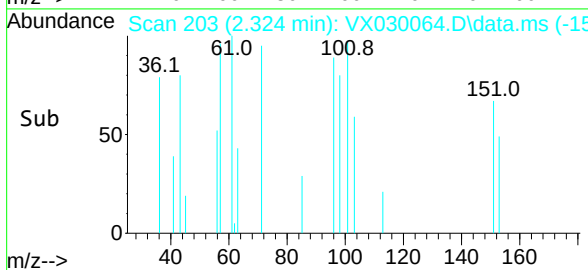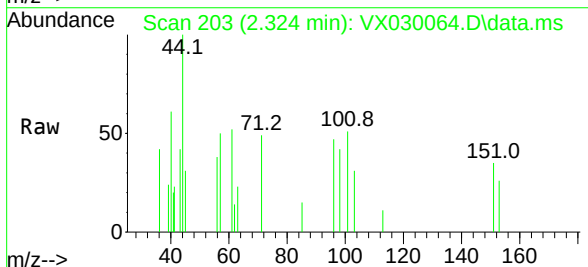



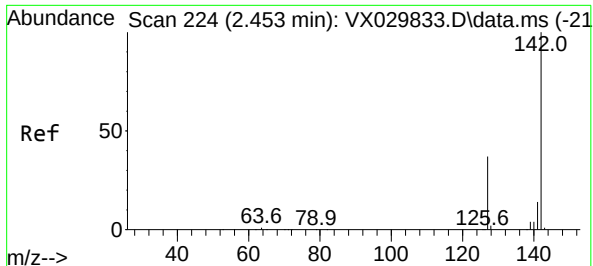


#10
Methyl Iodide
Concen: 2.823 ug/l
RT: 2.459 min Scan# 21
Delta R.T. 0.006 min
Lab File: VX030064.D
Acq: 14 Jul 2022 16:33

Instrument :
MSVOA_X
ClientSampleId :
TT-149S1-20220712



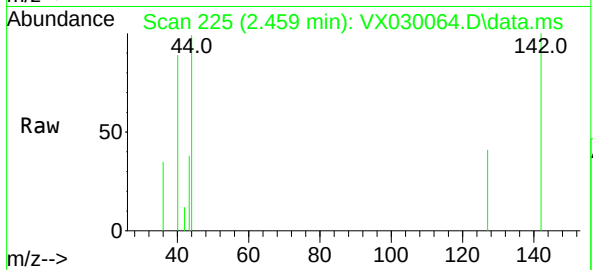



Tgt Ion:142 Resp: 738
Ion Ratio Lower Upper
142 100
127 35.0 30.2 45.2
141 0.0 11.3 16.9#

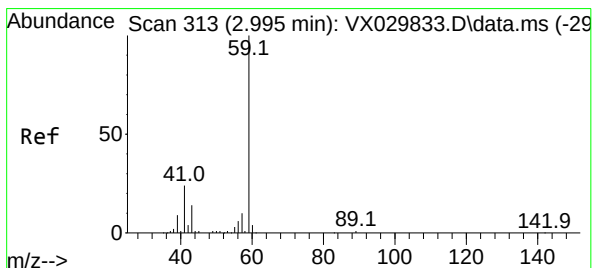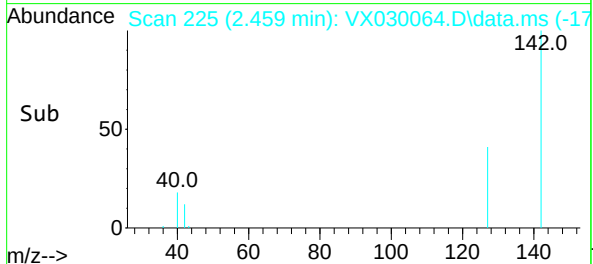

#11
Tert butyl alcohol
Concen: 0.788 ug/l
RT: 2.977 min Scan# 310
Delta R.T. -0.018 min
Lab File: VX030064.D
Acq: 14 Jul 2022 16:33

Tgt Ion: 59 Resp: 418
Ion Ratio Lower Upper
59 100
57 0.0 7.4 11.2#

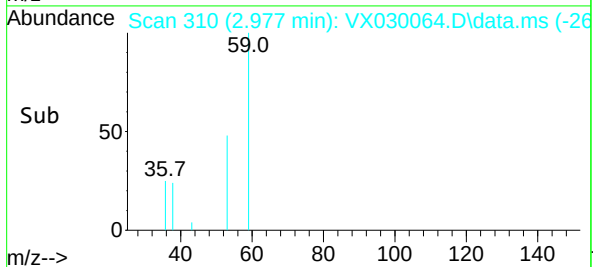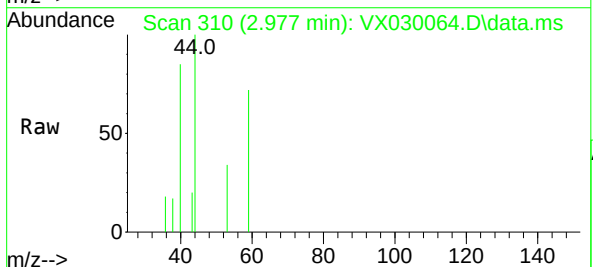



#12

1,1-Dichloroethene

Concen: 0.236 ug/l

RT: 2.318 min Scan# 20

Delta R.T. -0.001 min

Lab File: VX030064.D

Acq: 14 Jul 2022 16:33

Instrument :

MSVOA_X

ClientSampleId :

TT-149S1-20220712





Tgt Ion: 96 Resp: 406

Ion Ratio Lower Upper

96 100

61 117.3 117.4 176.0#

98 86.7 52.2 78.4#

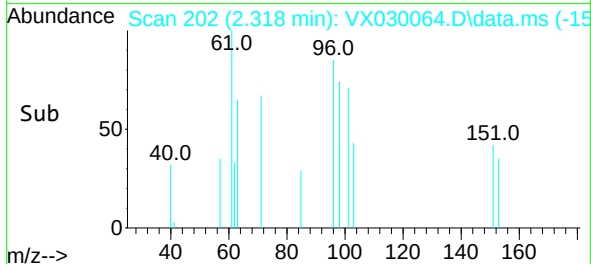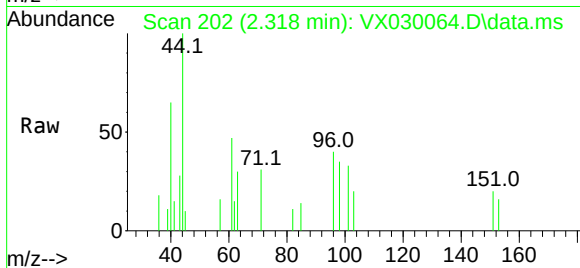

#13

Acrolein

Concen: 0.388 ug/l

RT: 2.239 min Scan# 189

Delta R.T. 0.000 min

Lab File: VX030064.D




Acq: 14 Jul 2022 16:33


Tgt Ion: 56 Resp: 41

Ion Ratio Lower Upper

56 100

55 292.7 56.6 84.8#


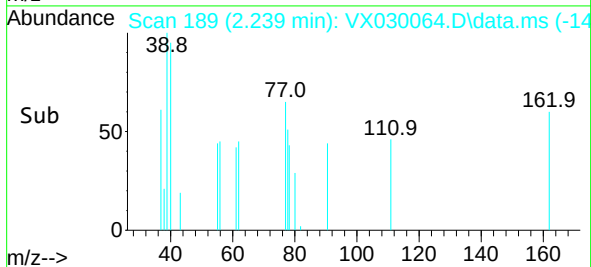

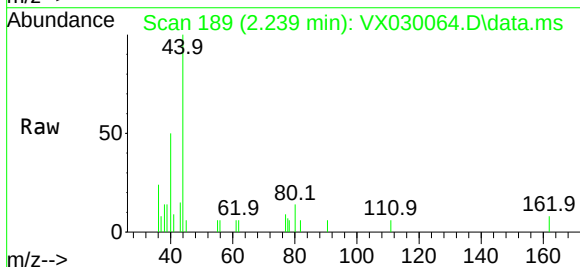




#16
 Acetone
 Concen: 1.426 ug/l
 RT: 2.392 min Scan# 214
 Delta R.T. -0.000 min
 Lab File: VX030064.D
 Acq: 14 Jul 2022 16:33




Instrument :
 MSVOA_X
 ClientSampleId :
 TT-149S1-20220712


Tgt Ion: 43 Resp: 1381
 Ion Ratio Lower Upper
 43 100
 58 29.2 27.7 41.5

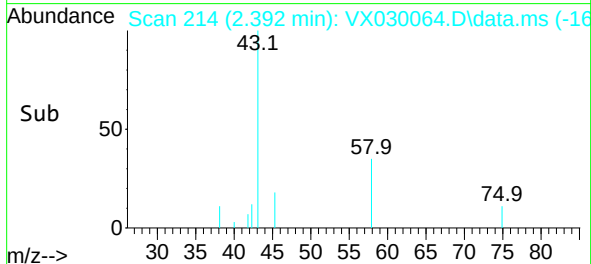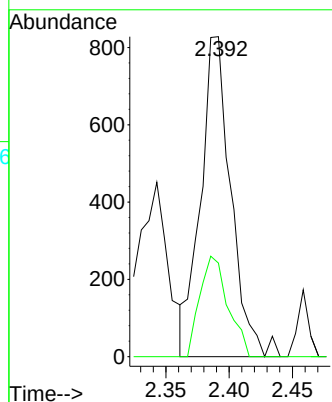

#19
 Methyl tert-butyl Ether
 Concen: 13.015 ug/l
 RT: 3.117 min Scan# 333
 Delta R.T. -0.000 min
 Lab File: VX030064.D
 Acq: 14 Jul 2022 16:33


Tgt Ion: 73 Resp: 70783
 Ion Ratio Lower Upper
 73 100
 57 22.7 19.0 28.6

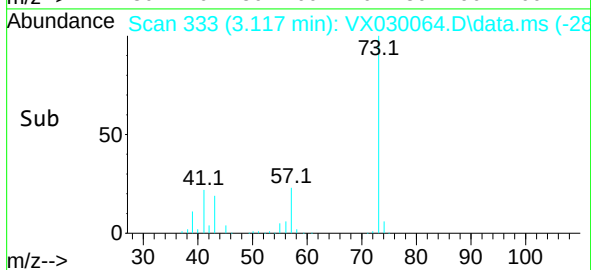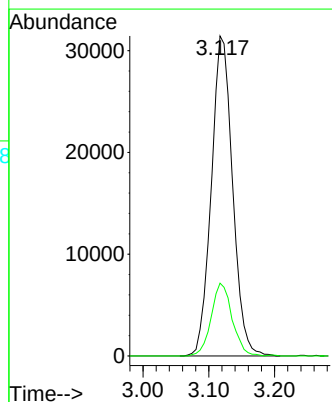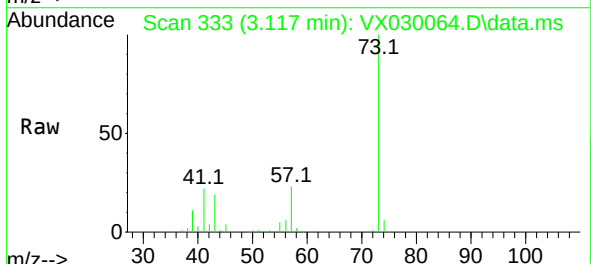





#20
Methylene Chloride
Concen: Below Cal
RT: 2.788 min Scan# 21
Delta R.T. -0.000 min
Lab File: VX030064.D
Acq: 14 Jul 2022 16:33


Instrument :
MSVOA_X
ClientSampleId :
TT-149S1-20220712





Tgt Ion: 84	Resp: 258
Ion Ratio	Lower Upper
84 100	
49 138.0	93.8 140.6
51 28.8	29.4 44.0#
86 86.5	51.0 76.4#

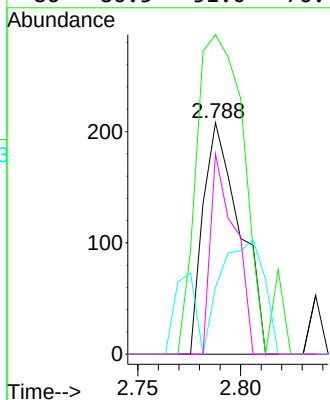


#22
Diisopropyl ether
Concen: 0.846 ug/l
RT: 3.769 min Scan# 440
Delta R.T. 0.006 min
Lab File: VX030064.D
Acq: 14 Jul 2022 16:33

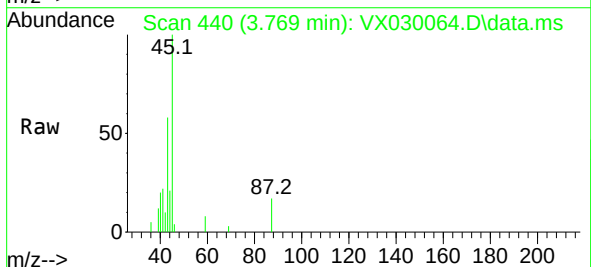

Tgt Ion: 45	Resp: 4977
Ion Ratio	Lower Upper
45 100	
43 57.9	65.4 98.0#
87 17.1	22.3 33.5#
59 8.4	9.0 13.4#



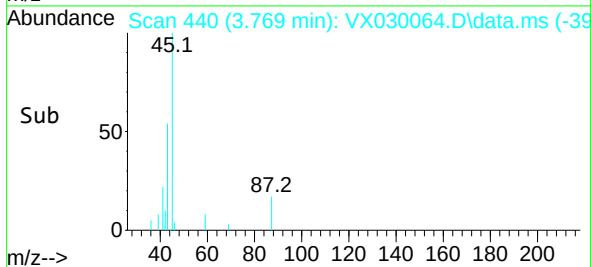
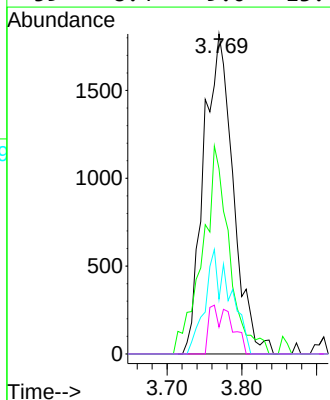


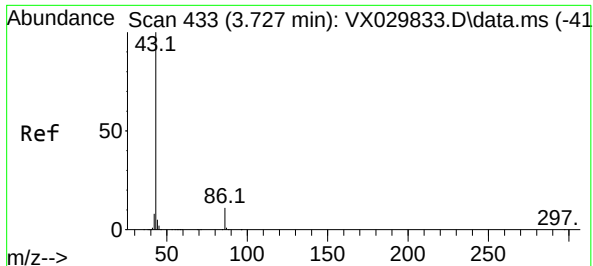

#23
 Vinyl Acetate
 Concen: 0.595 ug/l
 RT: 3.763 min Scan# 41
 Delta R.T. 0.036 min
 Lab File: VX030064.D
 Acq: 14 Jul 2022 16:33




Instrument :
 MSVOA_X
 ClientSampleId :
 TT-149S1-20220712


Tgt Ion: 43 Resp: 2964
 Ion Ratio Lower Upper
 43 100
 86 0.0 8.5 12.7#

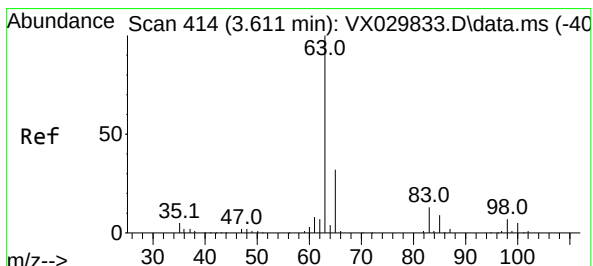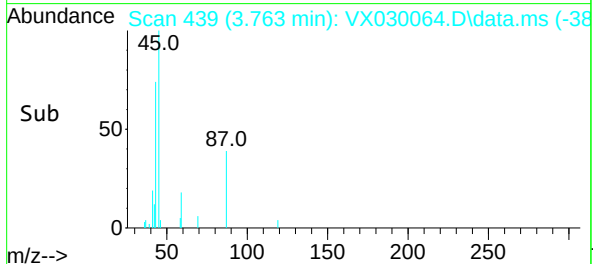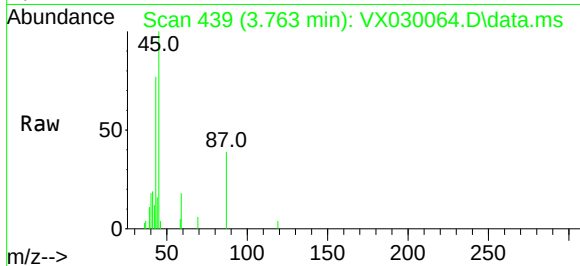

#24
 1,1-Dichloroethane
 Concen: 0.846 ug/l
 RT: 3.611 min Scan# 414
 Delta R.T. -0.000 min
 Lab File: VX030064.D
 Acq: 14 Jul 2022 16:33

Tgt Ion: 63 Resp: 2759
 Ion Ratio Lower Upper
 63 100
 98 0.0 3.5 10.5#
 100 8.7 2.3 6.9#

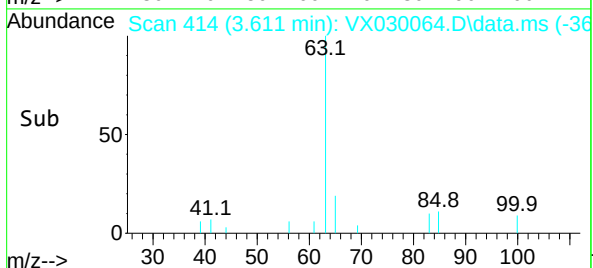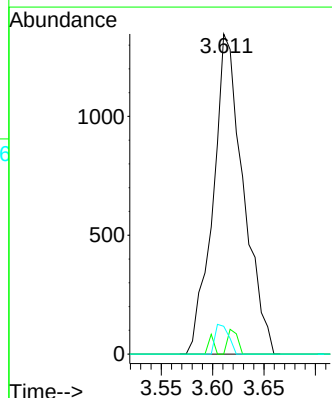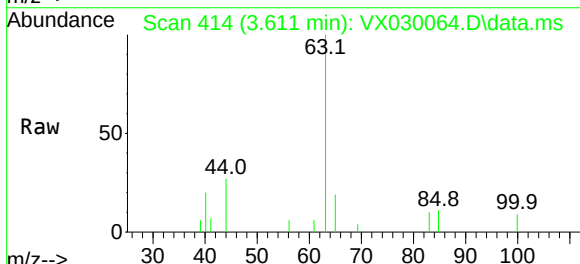



#27

cis-1,2-Dichloroethene

Concen: 0.654 ug/l

RT: 4.495 min Scan# 51

Delta R.T. -0.000 min

Lab File: VX030064.D


Acq: 14 Jul 2022 16:33

Instrument :




MSVOA_X

ClientSampleId :

TT-149S1-20220712

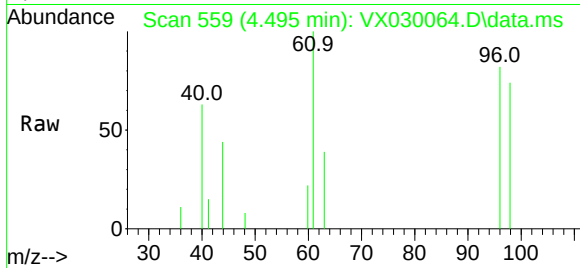

Tgt Ion: 96	Resp: 1436
Ion Ratio	Lower Upper
96	100
61	131.2 0.0 270.0
98	69.7 0.0 127.8

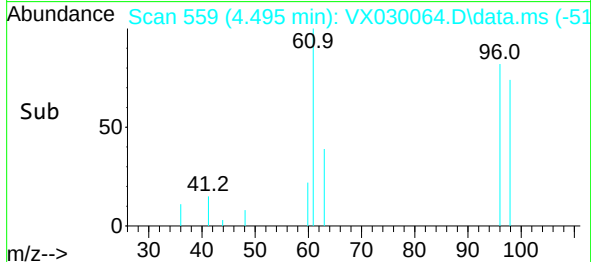

#31

Cyclohexane

Concen: 1.140 ug/l




RT: 5.549 min Scan# 732


Delta R.T. 0.079 min

Lab File: VX030064.D

Acq: 14 Jul 2022 16:33

Tgt Ion: 56	Resp: 3397
Ion Ratio	Lower Upper
56	100
69	151.3 25.4 38.0#
84	113.5 68.9 103.3#


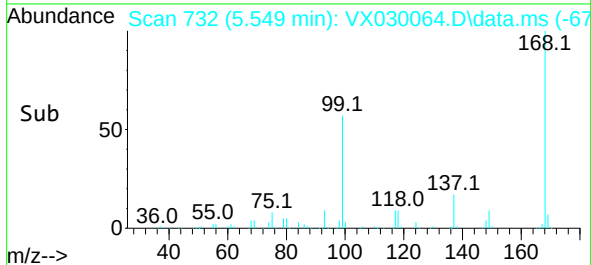

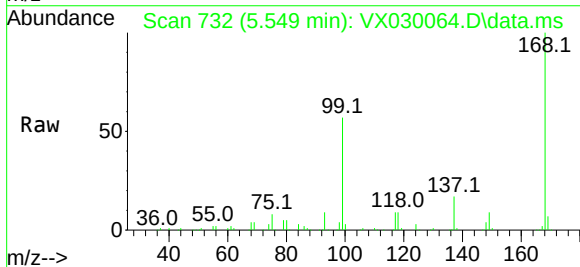


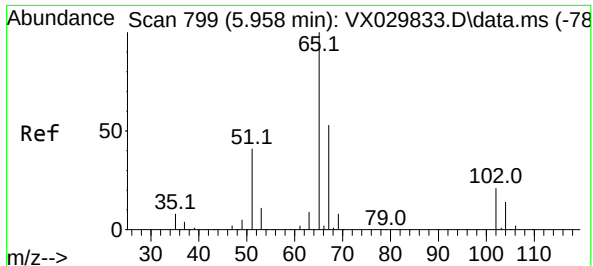

#33
 1,2-Dichloroethane-d4
 Concen: 46.120 ug/l
 RT: 5.964 min Scan# 80
 Delta R.T. 0.006 min
 Lab File: VX030064.D
 Acq: 14 Jul 2022 16:33




Instrument :
 MSVOA_X
 ClientSampleId :
 TT-149S1-20220712


Tgt Ion: 65 Resp: 94800
 Ion Ratio Lower Upper
 65 100
 67 54.5 0.0 109.6

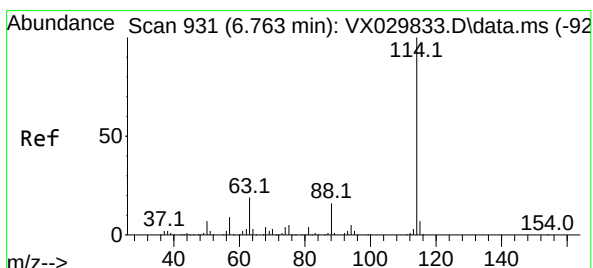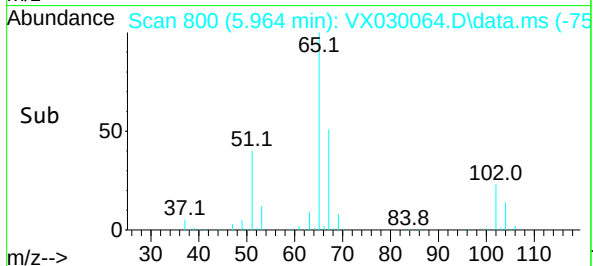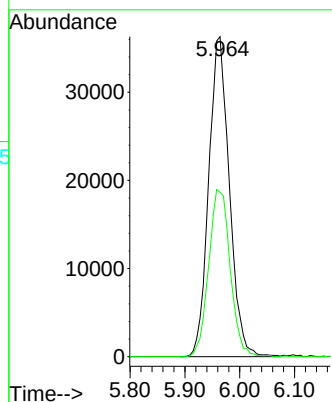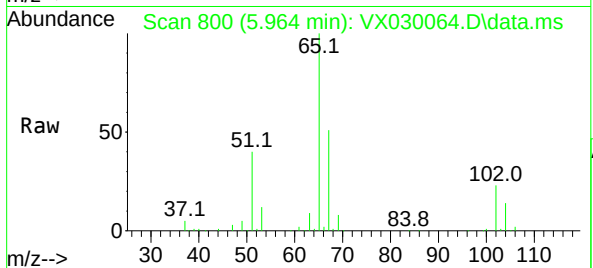

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 6.769 min Scan# 932
 Delta R.T. 0.006 min
 Lab File: VX030064.D
 Acq: 14 Jul 2022 16:33

Tgt Ion: 114 Resp: 291216
 Ion Ratio Lower Upper
 114 100
 63 19.1 0.0 38.4
 88 14.5 0.0 31.8

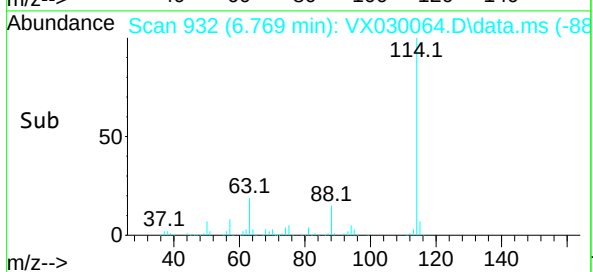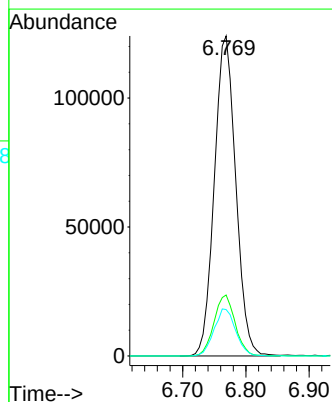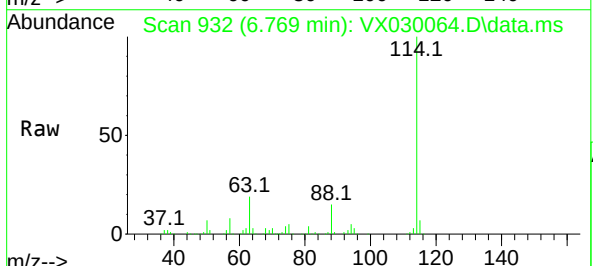

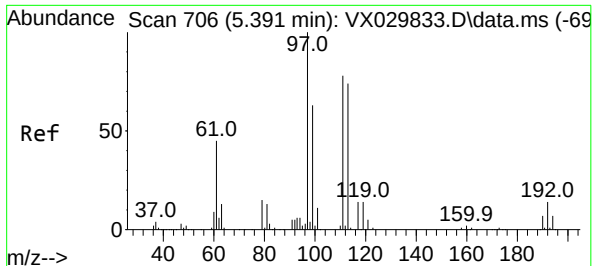

#35

Dibromofluoromethane

Concen: 46.208 ug/l

RT: 5.391 min Scan# 706

Delta R.T. -0.000 min

Lab File: VX030064.D


Acq: 14 Jul 2022 16:33

Instrument :

MSVOA_X

ClientSampleId :

TT-149S1-20220712

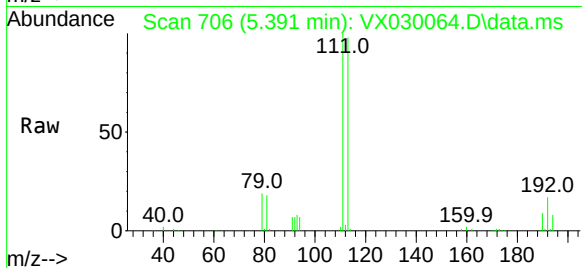




Tgt Ion:113 Resp: 85966

Ion Ratio Lower Upper

113 100

111 103.0 83.2 124.8

192 18.4 14.8 22.2

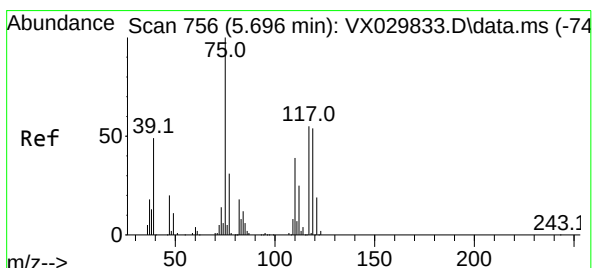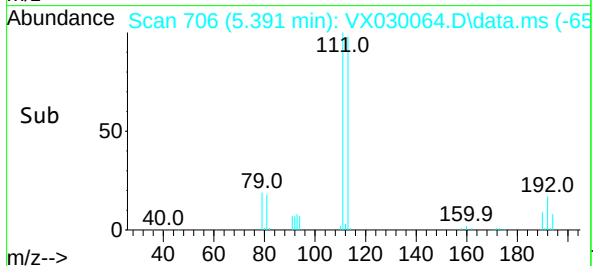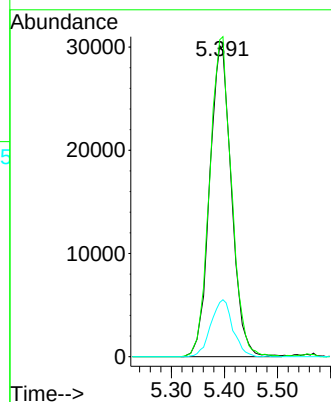

#36

1,1-Dichloropropene

Concen: 5.326 ug/l

RT: 5.549 min Scan# 732

Delta R.T. -0.147 min

Lab File: VX030064.D

Acq: 14 Jul 2022 16:33




Tgt Ion: 75 Resp: 12798


Ion Ratio Lower Upper

75 100

110 5.3 19.3 57.9#

77 0.0 24.4 36.6#


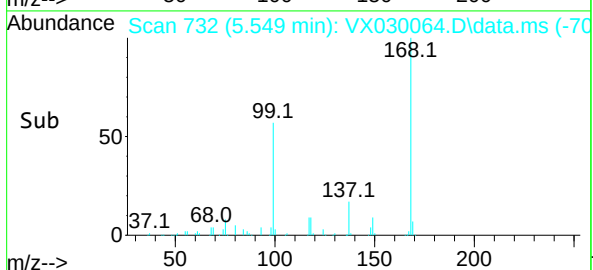
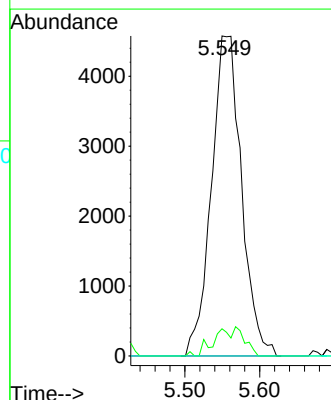
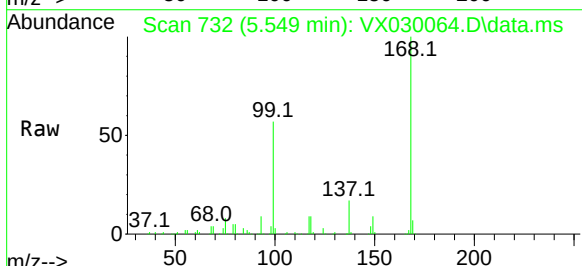




#38
Carbon Tetrachloride
Concen: 6.989 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.128 min
Lab File: VX030064.D
Acq: 14 Jul 2022 16:33




Instrument :
MSVOA_X
ClientSampleId :
TT-149S1-20220712


Tgt Ion:117 Resp: 15661
Ion Ratio Lower Upper
117 100
119 4.1 74.1 111.1#
121 0.0 25.8 38.8#

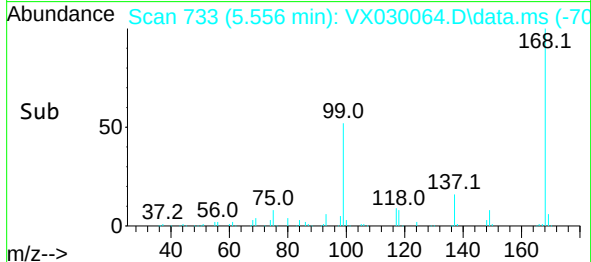

#42
1,2-Dichloroethane
Concen: 1.225 ug/l
RT: 6.098 min Scan# 822
Delta R.T. 0.006 min
Lab File: VX030064.D
Acq: 14 Jul 2022 16:33

Tgt Ion: 62 Resp: 2871
Ion Ratio Lower Upper
62 100
98 8.2 0.0 20.2


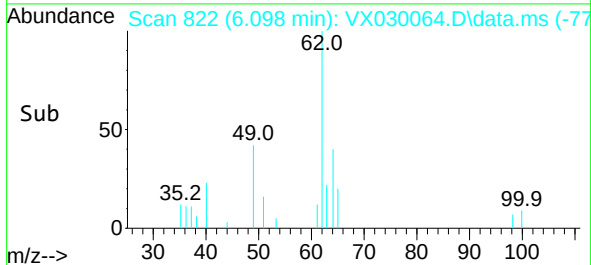

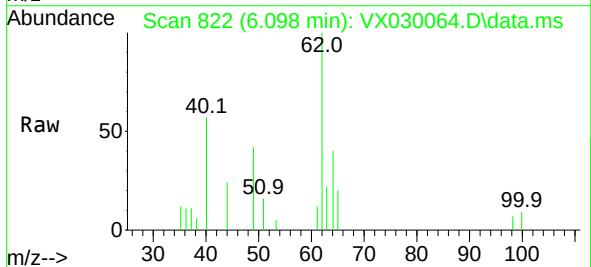




#44
Trichloroethene
Concen: 8.155 ug/l
RT: 7.128 min Scan# 991
Delta R.T. -0.001 min
Lab File: VX030064.D
Acq: 14 Jul 2022 16:33




Instrument :
MSVOA_X
ClientSampleId :
TT-149S1-20220712


Tgt Ion:130 Resp: 18024
Ion Ratio Lower Upper
130 100
95 91.7 0.0 194.8

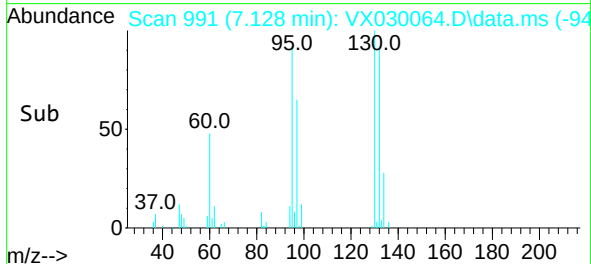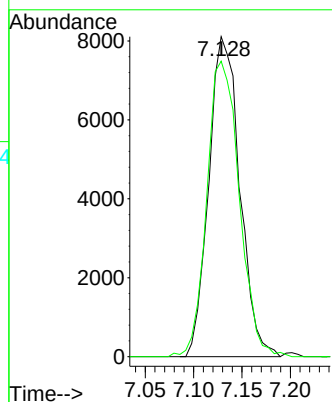

#49
1,4-Dioxane
Concen: 2.803 ug/l
RT: 7.695 min Scan# 1084
Delta R.T. 0.012 min
Lab File: VX030064.D
Acq: 14 Jul 2022 16:33

Tgt Ion: 88 Resp: 156
Ion Ratio Lower Upper
88 100
43 70.5 23.8 35.8#
58 61.5 53.8 80.6


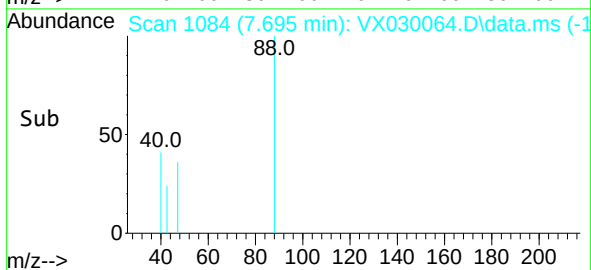

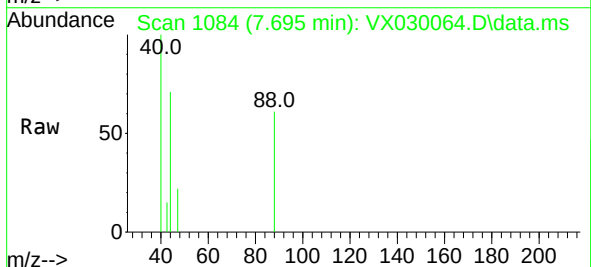




#50
Toluene-d8
Concen: 46.821 ug/l
RT: 8.653 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX030064.D
Acq: 14 Jul 2022 16:33




Instrument :
MSVOA_X
ClientSampleId :
TT-149S1-20220712


Tgt Ion: 98 Resp: 327603
Ion Ratio Lower Upper
98 100
100 66.1 52.3 78.5

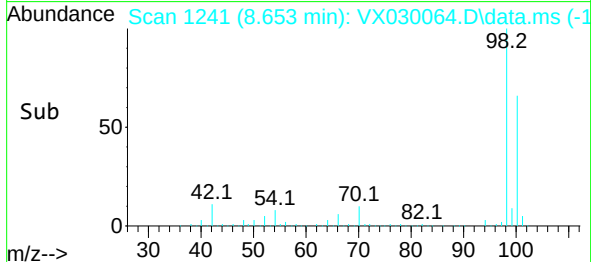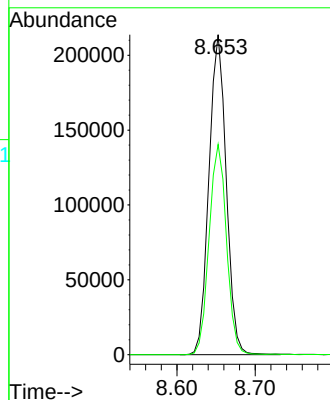

#60
Dibromochloromethane
Concen: 2.784 ug/l
RT: 9.274 min Scan# 1343
Delta R.T. -0.251 min
Lab File: VX030064.D
Acq: 14 Jul 2022 16:33

Tgt Ion: 129 Resp: 5371
Ion Ratio Lower Upper
129 100
127 0.0 38.5 115.5#

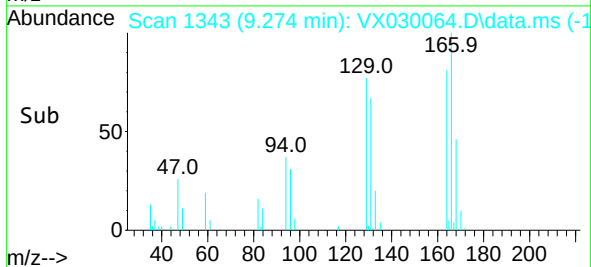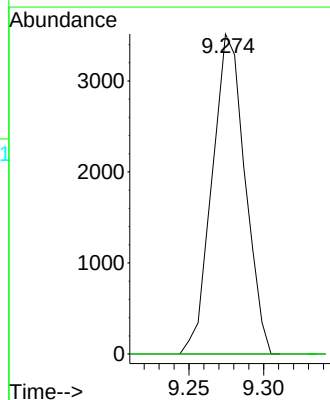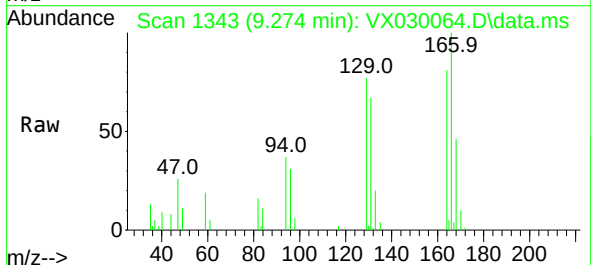



#62

4-Bromofluorobenzene

Concen: 43.340 ug/l

RT: 11.085 min Scan# 1

Delta R.T. 0.006 min

Lab File: VX030064.D

Acq: 14 Jul 2022 16:33

Instrument :

MSVOA_X

ClientSampleId :

TT-149S1-20220712





Tgt Ion: 95 Resp: 105235

Ion Ratio Lower Upper

95 100

174 78.3 0.0 149.0

176 74.2 0.0 146.0

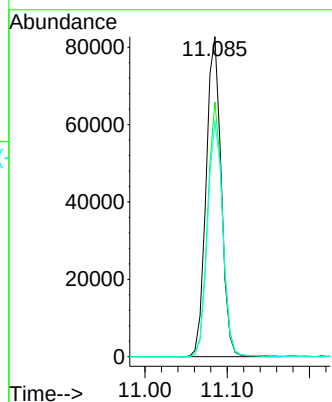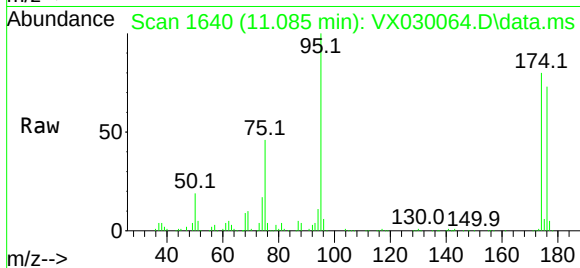

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.055 min Scan# 1471

Delta R.T. -0.000 min

Lab File: VX030064.D

Acq: 14 Jul 2022 16:33




Tgt Ion: 117 Resp: 248568


Ion Ratio Lower Upper

117 100

82 54.3 42.7 64.1

119 31.0 25.4 38.2


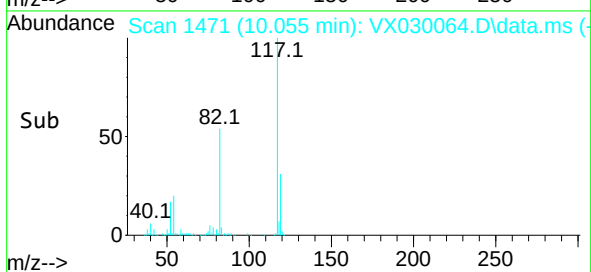
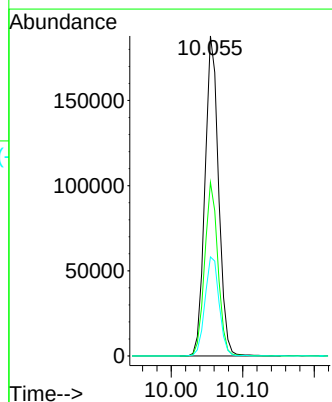
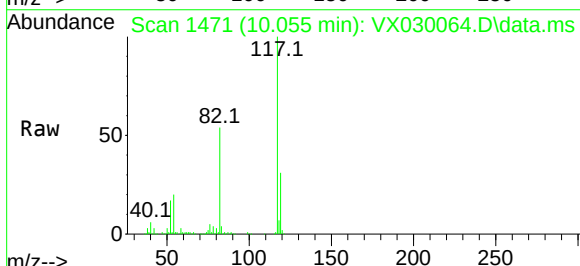




#64
Tetrachloroethene
Concen: 2.705 ug/l
RT: 9.274 min Scan# 11
Delta R.T. -0.001 min
Lab File: VX030064.D
Acq: 14 Jul 2022 16:33




Instrument :
MSVOA_X
ClientSampleId :
TT-149S1-20220712


Tgt Ion:164	Resp:	5397
Ion	Ratio	Lower Upper
164	100	
166	123.4	98.2 147.4
129	95.0	80.8 121.2
131	83.0	75.5 113.3

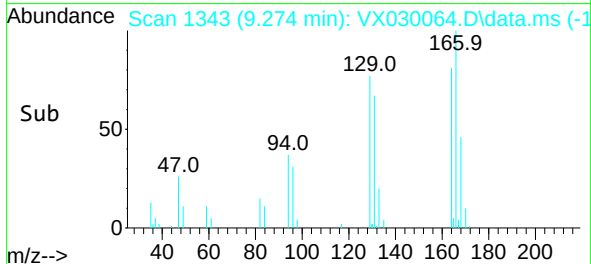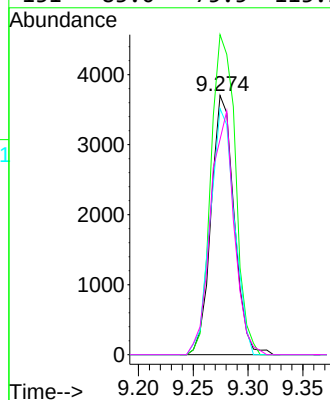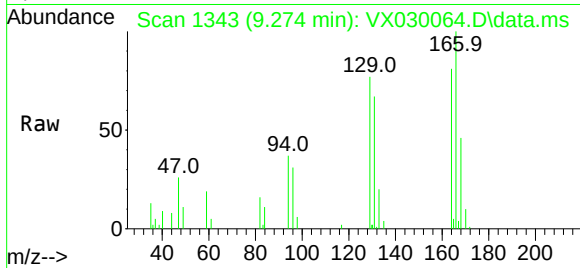

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. -0.000 min
Lab File: VX030064.D
Acq: 14 Jul 2022 16:33

Tgt Ion:152	Resp:	101047
Ion	Ratio	Lower Upper
152	100	
115	60.0	40.5 121.5
150	156.9	0.0 347.0


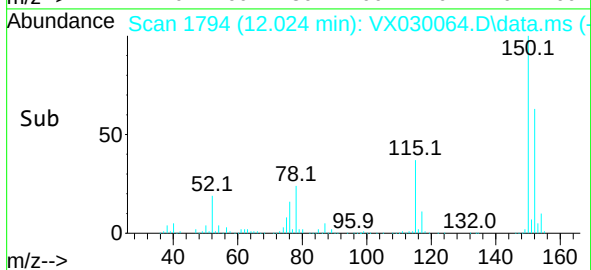
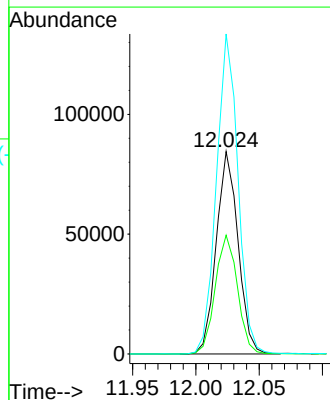
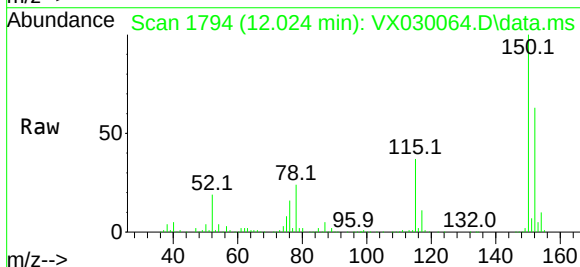




#76
1,2,3-Trichloropropane
Concen: 21.118 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. -0.159 min
Lab File: VX030064.D
Acq: 14 Jul 2022 16:33




Instrument :
MSVOA_X
ClientSampleId :
TT-149S1-20220712


Tgt Ion: 75 Resp: 49064
Ion Ratio Lower Upper
75 100
77 1.0 19.8 59.3#

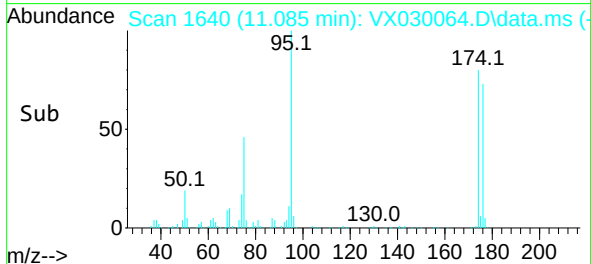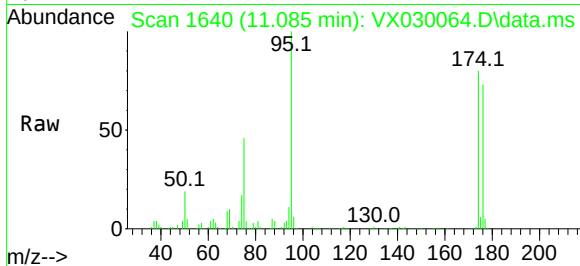

#81
trans-1,4-Dichloro-2-butene
Concen: 60.947 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.067 min
Lab File: VX030064.D
Acq: 14 Jul 2022 16:33

Tgt Ion: 75 Resp: 49064
Ion Ratio Lower Upper
75 100
53 0.0 74.2 111.4#
89 0.1 34.8 52.2#

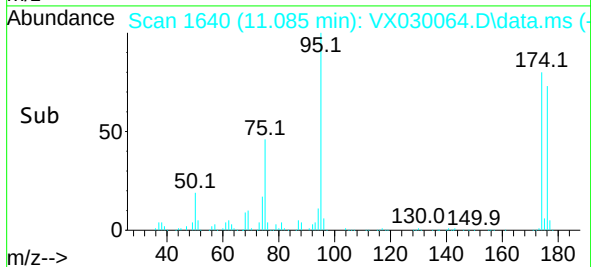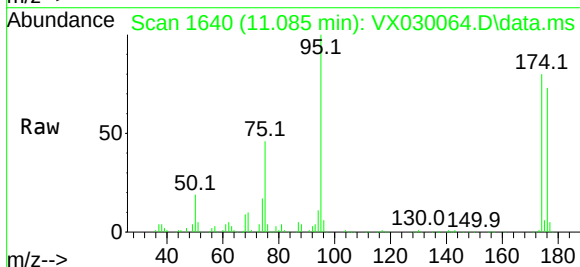

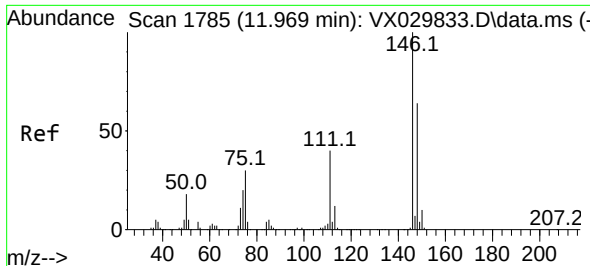

#87

1,3-Dichlorobenzene

Concen: 0.201 ug/l

RT: 11.975 min Scan# 11

Delta R.T. 0.006 min

Lab File: VX030064.D


Acq: 14 Jul 2022 16:33

Instrument :

MSVOA_X

ClientSampleId :

TT-149S1-20220712

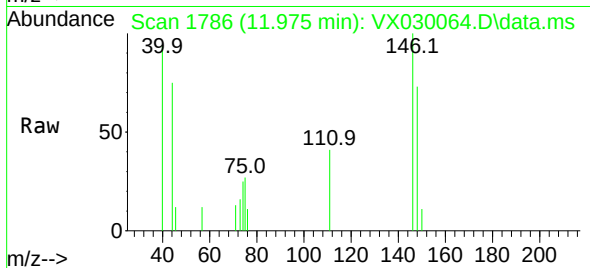




Tgt Ion:146 Resp: 655

Ion Ratio Lower Upper

146 100

111 43.4 20.3 60.8

148 55.7 31.8 95.3

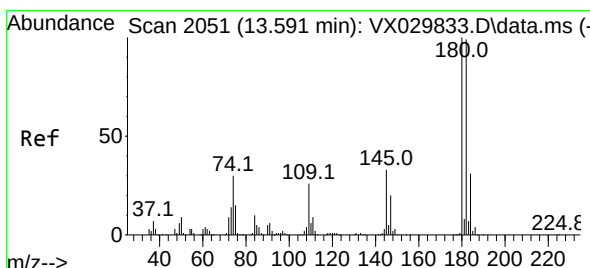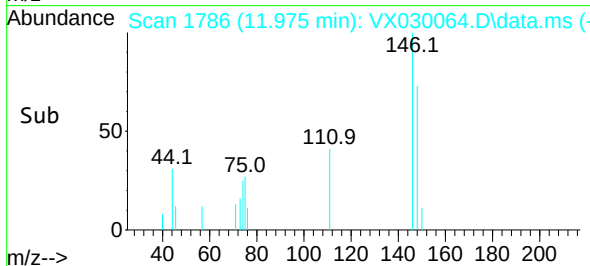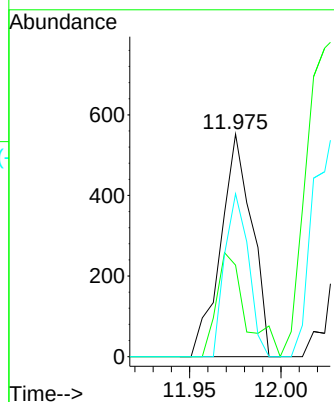

#93

1,2,4-Trichlorobenzene

Concen: 0.318 ug/l

RT: 13.591 min Scan# 2051

Delta R.T. -0.000 min

Lab File: VX030064.D

Acq: 14 Jul 2022 16:33




Tgt Ion:180 Resp: 646


Ion Ratio Lower Upper

180 100

182 87.8 48.2 144.6

145 39.6 15.9 47.6


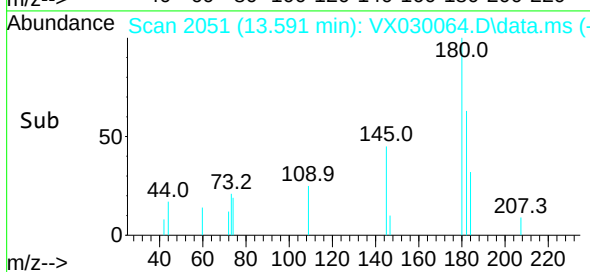
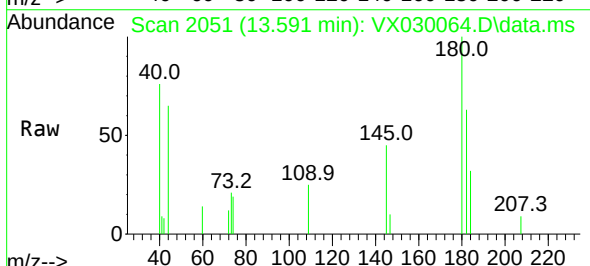
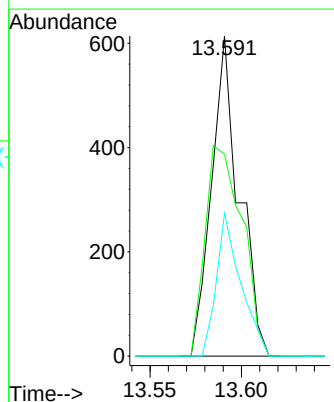




#94
Hexachlorobutadiene
Concen: 0.432 ug/l
RT: 13.731 min Scan# 2073
Delta R.T. 0.006 min
Lab File: VX030064.D
Acq: 14 Jul 2022 16:33




Instrument :
MSVOA_X
ClientSampleId :
TT-149S1-20220712


Tgt Ion:	225	Resp:	350
Ion Ratio	Lower	Upper	
225	100		
223	42.0	30.6	91.6
227	63.1	31.9	95.9

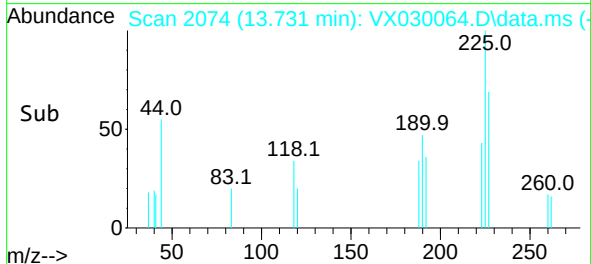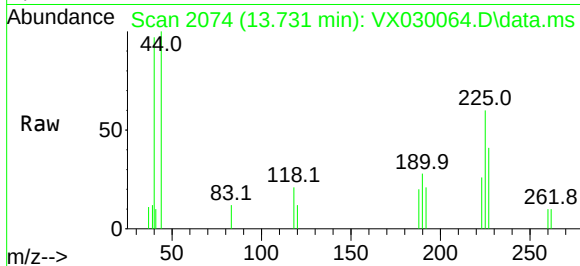

#95
Naphthalene
Concen: 0.210 ug/l
RT: 13.780 min Scan# 2082
Delta R.T. -0.000 min
Lab File: VX030064.D
Acq: 14 Jul 2022 16:33


Tgt Ion:	128	Resp:	1691
Ion Ratio	Lower	Upper	
128	100		
127	3.4	10.2	15.2#
129	10.8	8.6	13.0

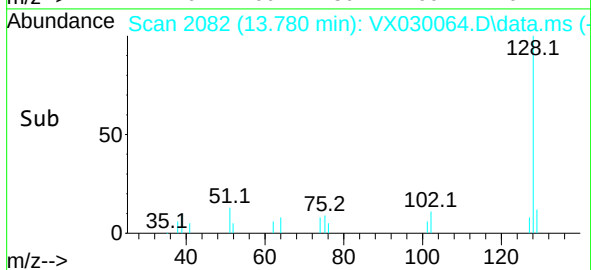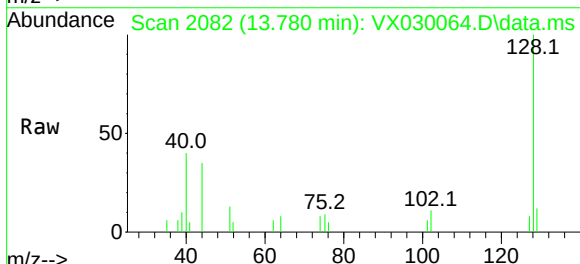



#96
 1,2,3-Trichlorobenzene
 Concen: 0.322 ug/l
 RT: 13.969 min Scan# 2113
 Delta R.T. 0.006 min
 Lab File: VX030064.D
 Acq: 14 Jul 2022 16:33

Instrument :
 MSVOA_X
 ClientSampleId :
 TT-149S1-20220712

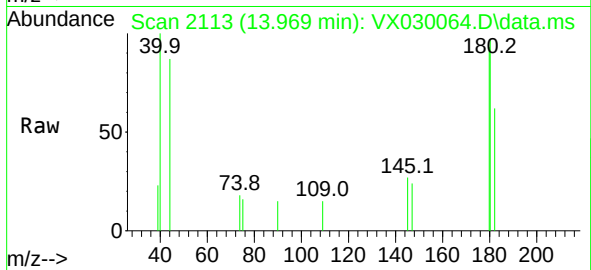

Tgt Ion:180	Resp:	664
Ion	Ratio	Lower Upper
180	100	
182	74.5	47.0 141.0
145	13.7	17.0 50.9#

