

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071422\
 Data File : VX030066.D
 Acq On : 14 Jul 2022 17:20
 Operator : JC/MD
 Sample : N3705-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TB01-20220711

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X071222W.M

Title : SW846 8260

Signal : TIC: VX030066.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.556	231	241	250	rBV	21044	45837	5.30%	1.012%
2	4.592	564	575	585	rBV2	11055	39477	4.57%	0.871%
3	5.391	695	706	719	rBV	97288	283426	32.80%	6.255%
4	5.555	722	733	746	rVV	166563	475519	55.03%	10.495%
5	5.964	785	800	812	rBV	107025	285892	33.08%	6.310%
6	6.769	921	932	943	rBV2	271990	657979	76.14%	14.522%
7	8.652	1234	1241	1255	rBV	557049	864124	100.00%	19.071%
8	9.274	1339	1343	1350	rVB3	10552	16842	1.95%	0.372%
9	10.055	1465	1471	1484	rBV	540467	731659	84.67%	16.148%
10	11.085	1634	1640	1649	rBV	403682	501365	58.02%	11.065%
11	12.024	1789	1794	1802	rVB	517355	628863	72.77%	13.879%




Sum of corrected areas: 4530983

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071422\
Data File : VX030066.D
Acq On : 14 Jul 2022 17:20
Operator : JC/MD
Sample : N3705-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TB01-20220711

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X071222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

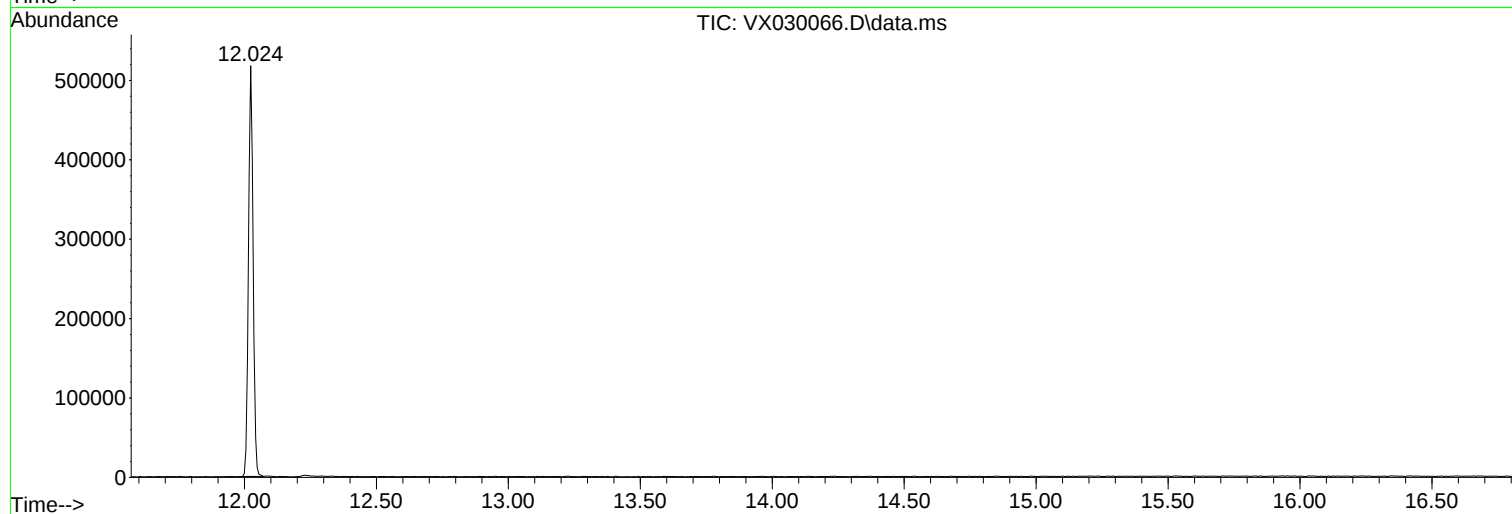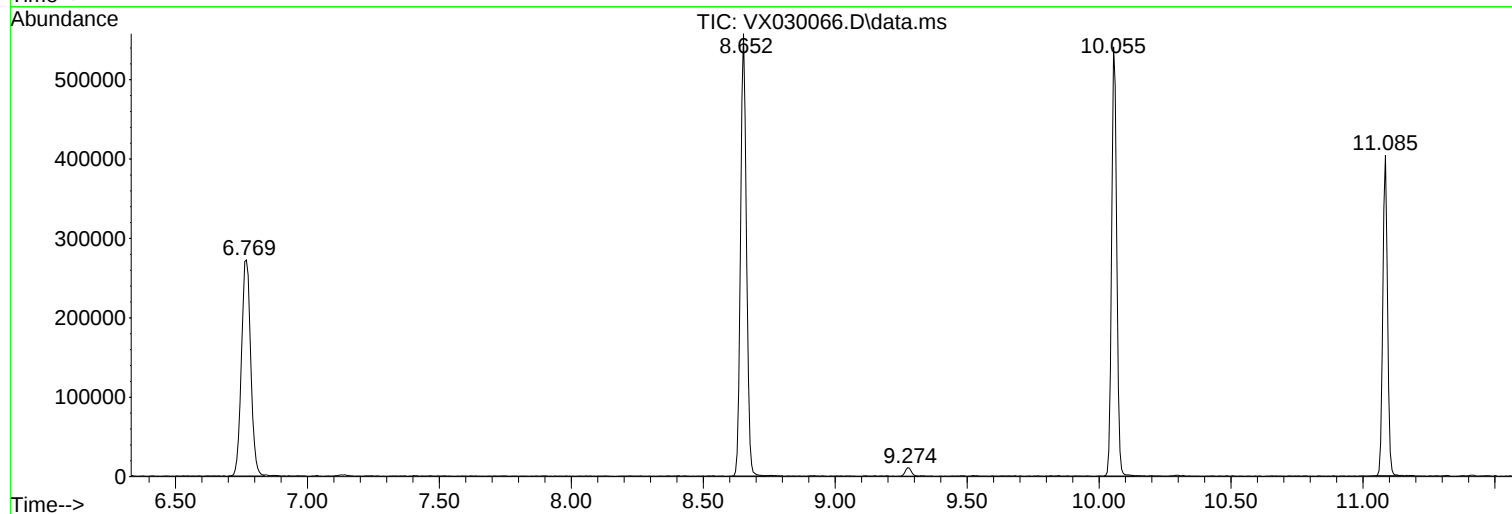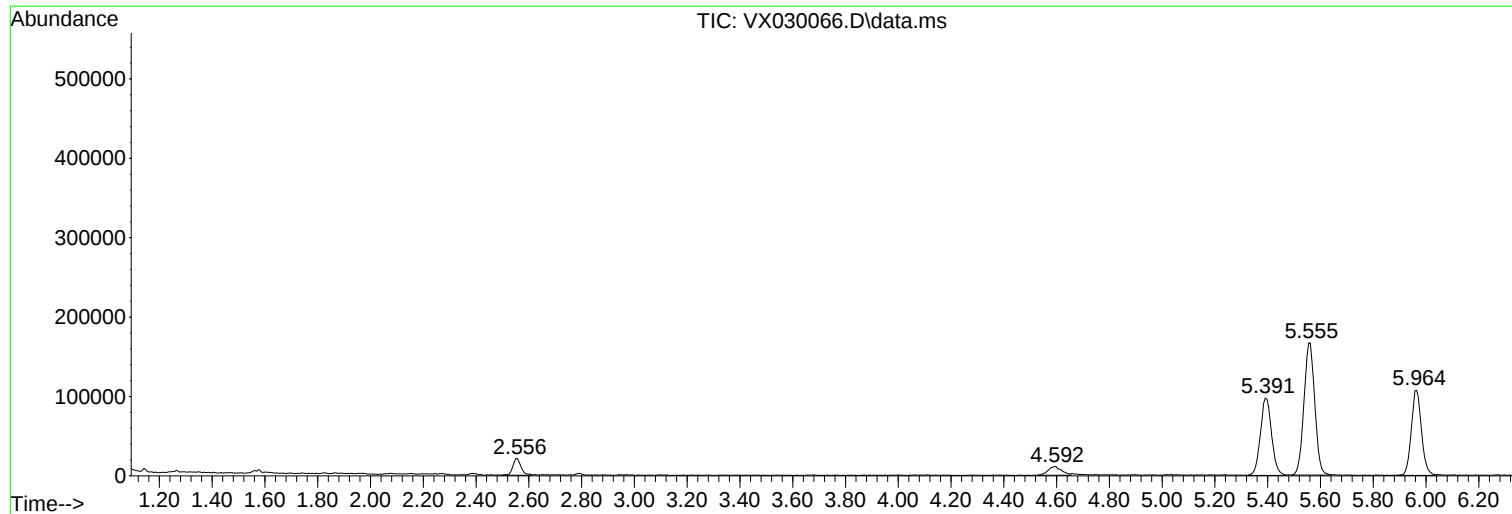

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071422\
Data File : VX030066.D
Acq On : 14 Jul 2022 17:20
Operator : JC/MD
Sample : N3705-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TB01-20220711

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X071222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071422\
Data File : VX030066.D
Acq On : 14 Jul 2022 17:20
Operator : JC/MD
Sample : N3705-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TB01-20220711

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X071222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------