

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071422\
 Data File : VX030070.D
 Acq On : 14 Jul 2022 18:54
 Operator : JC/MD
 Sample : N3718-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 220713004-03-TRIP-BLANK

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X071222W.M

Title : SW846 8260

Signal : TIC: VX030070.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.391	207	214	221	rBV	12654	21651	2.46%	0.477%
2	2.568	236	243	254	rBV2	11526	29540	3.35%	0.651%
3	5.391	695	706	722	rBV2	98672	281617	31.94%	6.210%
4	5.556	722	733	747	rBV	169882	480497	54.49%	10.596%
5	5.964	790	800	813	rBV	106497	286397	32.48%	6.316%
6	6.769	921	932	945	rBV	277423	662154	75.09%	14.602%
7	8.653	1234	1241	1250	rBV	578579	881823	100.00%	19.446%
8	9.274	1338	1343	1350	rBV2	12241	19171	2.17%	0.423%
9	10.055	1465	1471	1480	rBV	552137	744471	84.42%	16.417%
10	11.085	1634	1640	1650	rBV	396027	509161	57.74%	11.228%
11	12.024	1788	1794	1805	rBV	504923	618191	70.10%	13.633%




Sum of corrected areas: 4534673

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071422\
Data File : VX030070.D
Acq On : 14 Jul 2022 18:54
Operator : JC/MD
Sample : N3718-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
220713004-03-TRIP-BLANK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X071222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

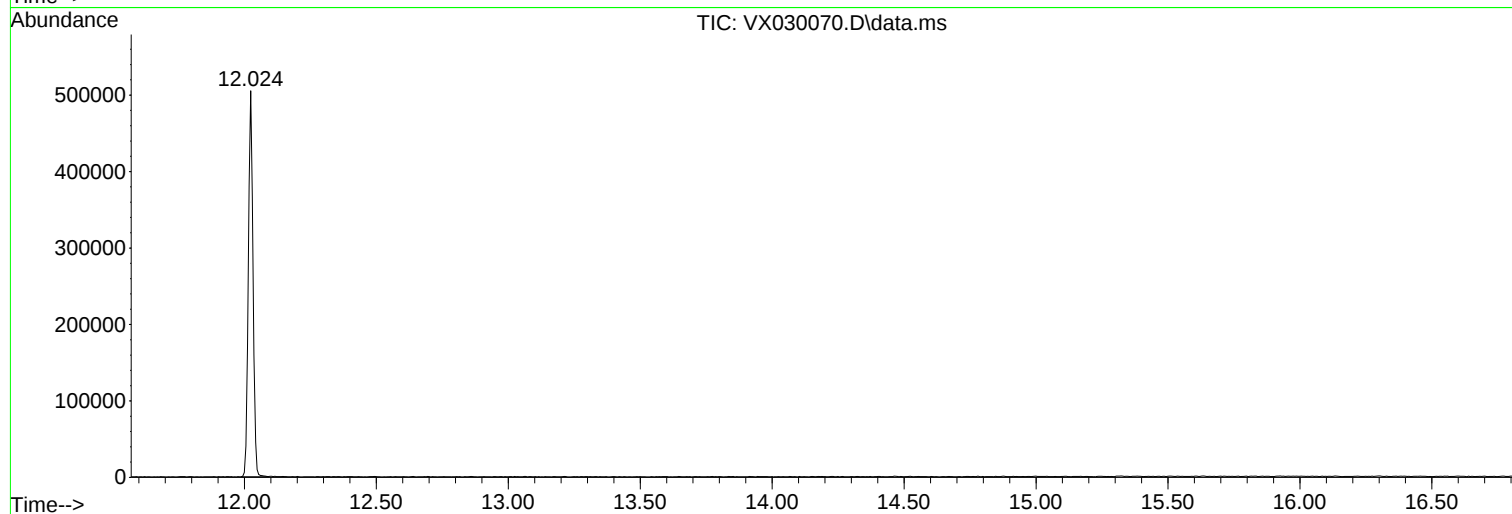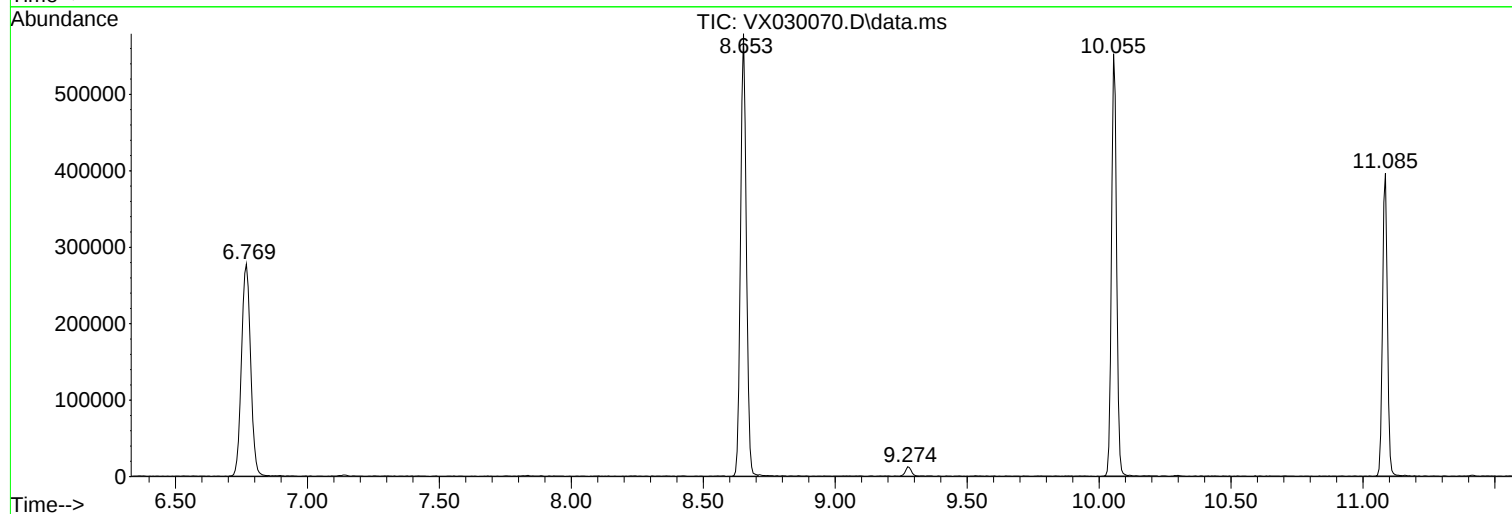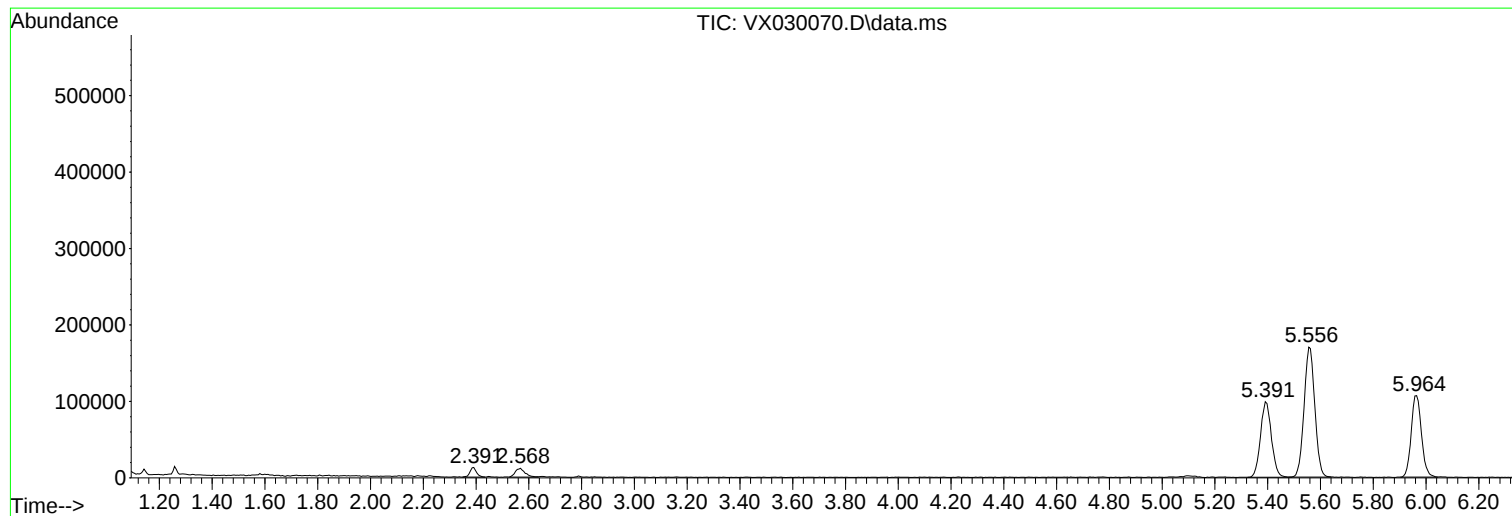

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071422\
Data File : VX030070.D
Acq On : 14 Jul 2022 18:54
Operator : JC/MD
Sample : N3718-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
220713004-03-TRIP-BLANK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X071222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071422\
Data File : VX030070.D
Acq On : 14 Jul 2022 18:54
Operator : JC/MD
Sample : N3718-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
220713004-03-TRIP-BLANK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X071222W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------