


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX071422\  
Data File : VX030051.D  
Acq On : 14 Jul 2022 10:38  
Operator : JC/MD  
Sample : BFB  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\624X070822W.M  
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS  
Last Update : Sat Jul 09 02:10:54 2022

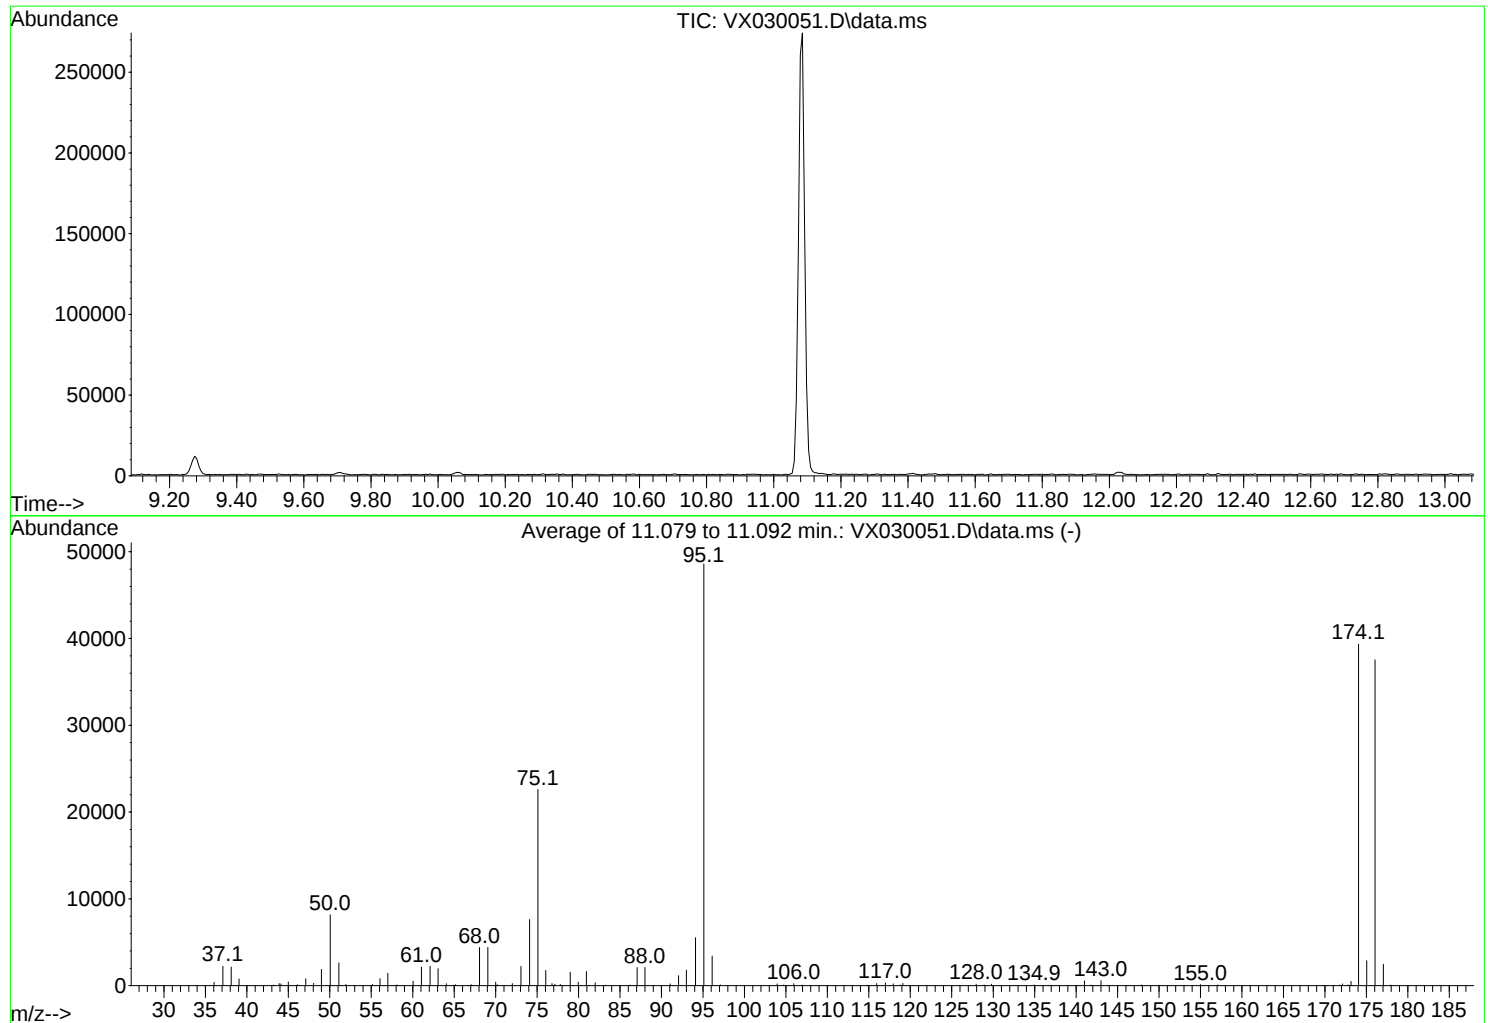

AutoFind: Scans 1639, 1640, 1641; Background Corrected with Scan 1633

| Target | Rel. to | Lower  | Upper  | Rel.  | Raw   | Result    |
|--------|---------|--------|--------|-------|-------|-----------|
| Mass   | Mass    | Limit% | Limit% | Abn%  | Abn   | Pass/Fail |
| 50     | 95      | 15     | 40     | 16.8  | 8165  | PASS      |
| 75     | 95      | 30     | 60     | 46.5  | 22611 | PASS      |
| 95     | 95      | 100    | 100    | 100.0 | 48605 | PASS      |
| 96     | 95      | 5      | 9      | 7.0   | 3405  | PASS      |
| 173    | 174     | 0.00   | 2      | 1.2   | 480   | PASS      |
| 174    | 95      | 50     | 100    | 81.0  | 39365 | PASS      |
| 175    | 174     | 5      | 9      | 7.3   | 2881  | PASS      |
| 176    | 174     | 95     | 101    | 95.4  | 37536 | PASS      |
| 177    | 176     | 5      | 9      | 6.6   | 2470  | PASS      |