

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071423\
 Data File : VX036533.D
 Acq On : 13 Jul 2023 18:18
 Operator : JC/MD
 Sample : VX0714WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Jul 14 04:37:22 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X071423W.M
 Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 QLast Update : Fri Jul 14 04:32:22 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Bromochloromethane	4.898	128	32614	30.000	ug/l	0.00
28) 1,4-Difluorobenzene	6.763	114	170710	30.000	ug/l	0.00
57) Chlorobenzene-d5	10.055	117	153535	30.000	ug/l	0.00
System Monitoring Compounds						
27) 1,2-Dichloroethane-d4	5.958	65	79005	29.187	ug/l	0.00
Spiked Amount	30.000	Range	91 - 110	Recovery	=	97.300%
60) 4-Bromofluorobenzene	11.079	95	69788	28.022	ug/l	0.00
Spiked Amount	30.000	Range	63 - 112	Recovery	=	93.400%
63) Toluene-d8	8.653	98	211166	29.889	ug/l	0.00
Spiked Amount	30.000	Range	91 - 112	Recovery	=	99.633%
Target Compounds						
					Qvalue	
14) Acrylonitrile	3.075	53	468	0.372	ug/l	74
15) Acetone	2.380	58	316	0.888	ug/l #	1
16) Carbon Disulfide	2.514	76	2605	0.563	ug/l	98
18) Methylene Chloride	2.794	84	1128	0.491	ug/l #	79
19) trans-1,2-Dichloroethene	3.087	96	643	0.308	ug/l #	84
23) tert-Butyl Alcohol	2.971	59	248	0.425	ug/l #	1
29) 1,1-Dichloropropene	5.690	75	518	0.201	ug/l #	64
42) Vinyl Acetate	3.739	43	1223	0.250	ug/l #	75
53) Dibromochloromethane	9.275	129	454	0.213	ug/l #	11
55) 2-Chloroethyl vinyl ether	8.251	63	1852	1.037	ug/l	96
56) Bromoform	11.085	173	746	0.502	ug/l #	1
58) 4-Methyl-2-Pentanone	8.580	43	983	0.310	ug/l #	69
59) 2-Hexanone	9.439	43	650	0.269	ug/l #	86
61) Tetrachloroethene	9.275	164	584	0.318	ug/l #	78
67) m/p-Xylenes	10.305	106	1484	0.407	ug/l	99
73) Bromobenzene	11.201	156	515	0.231	ug/l	89
74) n-propylbenzene	11.305	91	2669	0.251	ug/l	99
75) 2-Chlorotoluene	11.366	91	1440	0.223	ug/l	99
76) 1,3,5-Trimethylbenzene	11.451	105	1624	0.209	ug/l	98
77) t-1,4-Dichloro-2-butene	11.079	75	36198	36.125	ug/l #	7
78) 4-Chlorotoluene	11.463	91	2300	0.313	ug/l	96
80) 1,2,4-Trimethylbenzene	11.750	105	2087	0.272	ug/l	92
81) sec-Butylbenzene	11.890	105	2278	0.246	ug/l	97
82) p-Isopropyltoluene	12.012	119	2345	0.304	ug/l	92
83) 1,3-Dichlorobenzene	11.969	146	1726	0.416	ug/l	95
84) 1,4-Dichlorobenzene	12.043	146	1774	0.429	ug/l	97
85) n-Butylbenzene	12.335	91	2711	0.386	ug/l	98
87) 1,2-Dichlorobenzene	12.335	146	1294	0.311	ug/l	94
89) 1,2,4-Trichlorobenzene	13.591	180	1767	0.673	ug/l	95
90) Hexachlorobutadiene	13.719	225	705	0.740	ug/l	96
91) Naphthalene	13.780	128	3740	0.406	ug/l #	92
92) 1,2,3-Trichlorobenzene	13.963	180	1496	0.565	ug/l	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071423\
Data File : VX036533.D
Acq On : 13 Jul 2023 18:18
Operator : JC/MD
Sample : VX0714WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :


Quant Time: Jul 14 04:37:22 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X071423W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
QLast Update : Fri Jul 14 04:32:22 2023
Response via : Initial Calibration

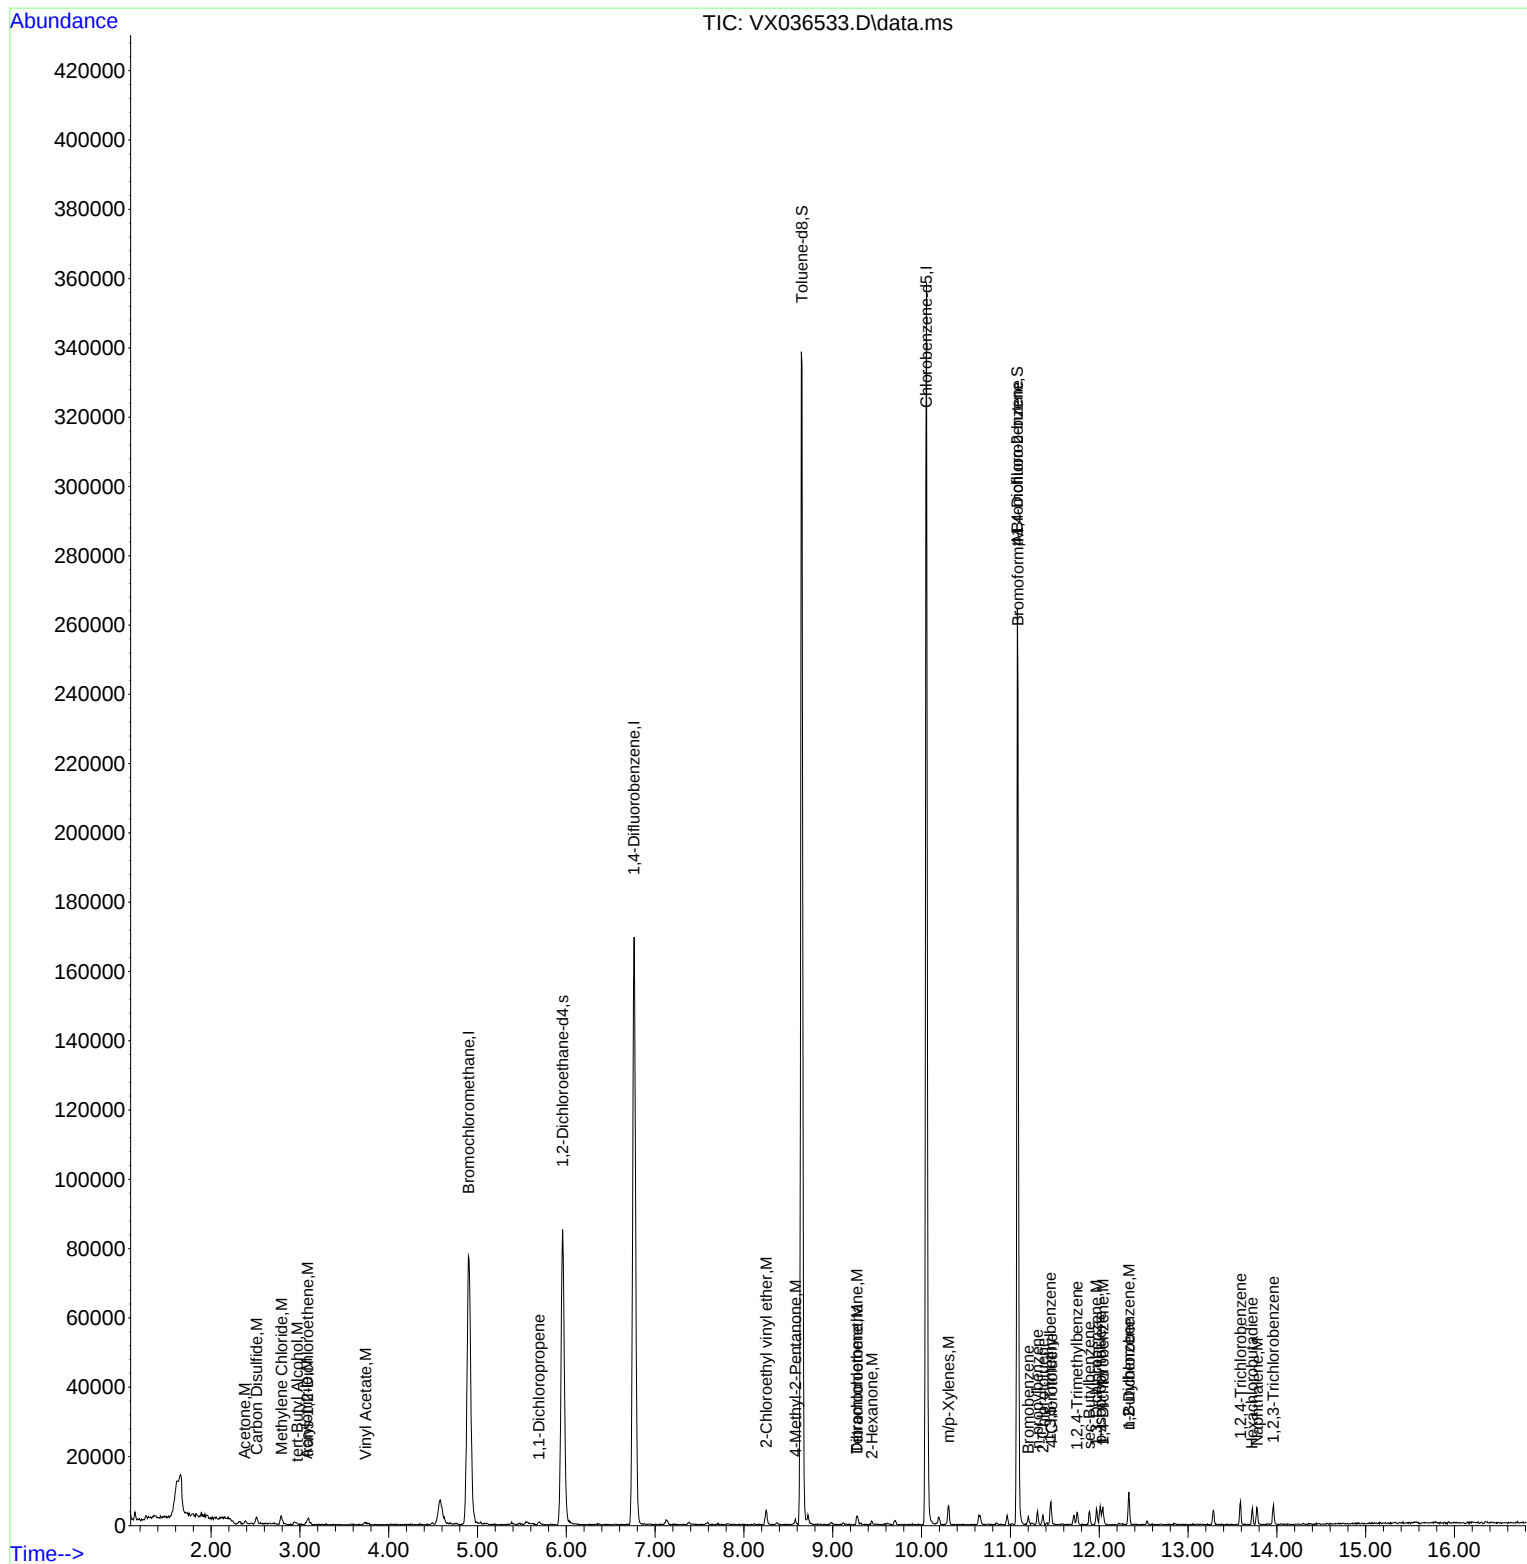



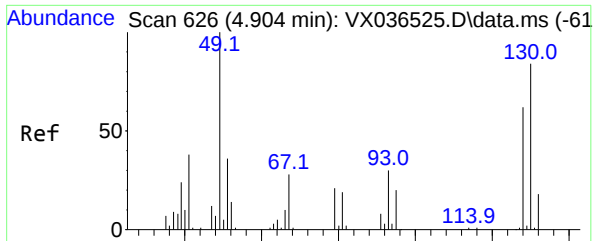


#1
Bromochloromethane
Concen: 30.000 ug/l
RT: 4.898 min Scan# 61
Delta R.T. -0.006 min
Lab File: VX036533.D
Acq: 13 Jul 2023 18:18

Instrument :
MSVOA_X
ClientSampleId :



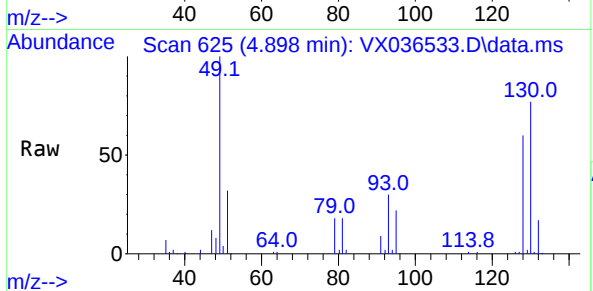



Tgt Ion:128 Resp: 32614
Ion Ratio Lower Upper
128 100
49 160.4 0.0 406.3
130 128.5 0.0 328.0

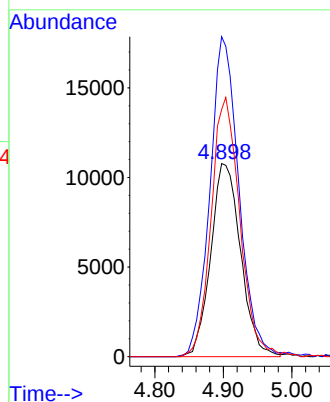

#14
Acrylonitrile
Concen: 0.372 ug/l
RT: 3.075 min Scan# 326
Delta R.T. 0.006 min
Lab File: VX036533.D
Acq: 13 Jul 2023 18:18

Tgt Ion: 53 Resp: 468
Ion Ratio Lower Upper
53 100
52 56.2 40.0 119.9
51 21.4 18.2 54.6

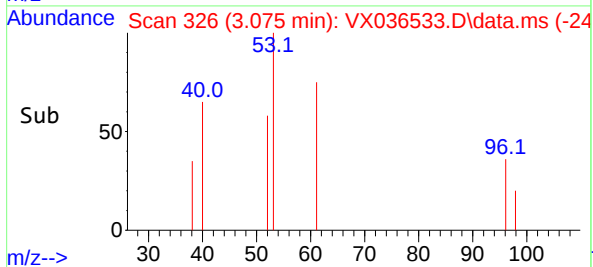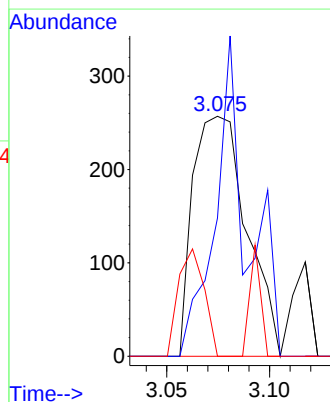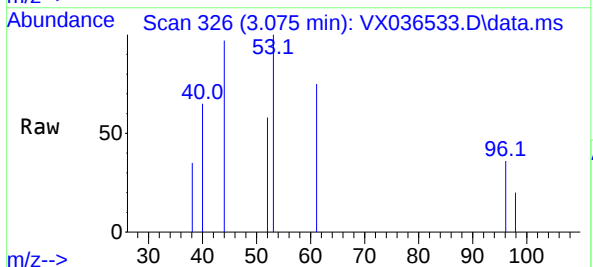



#15

Acetone

Concen: 0.888 ug/l

RT: 2.380 min Scan# 212

Delta R.T. 0.000 min

Lab File: VX036533.D

Acq: 13 Jul 2023 18:18

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 58 Resp: 316

Ion Ratio Lower Upper

58 100

43 90.7 261.0 391.4#

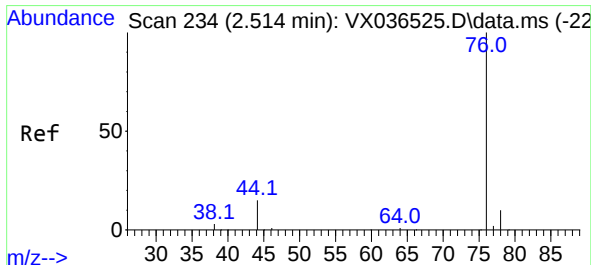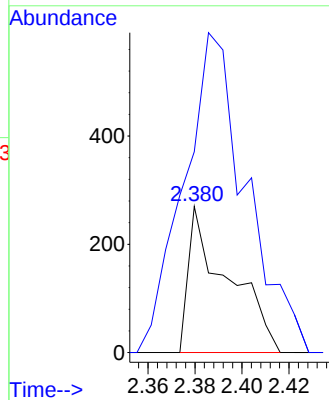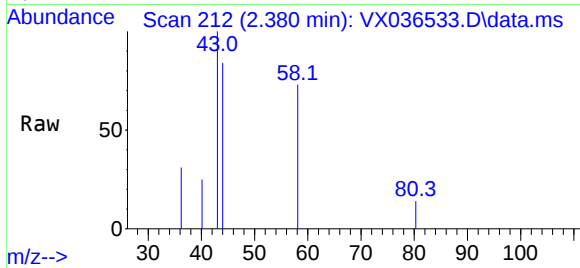

#16

Carbon Disulfide

Concen: 0.563 ug/l

RT: 2.514 min Scan# 234

Delta R.T. 0.000 min

Lab File: VX036533.D




Acq: 13 Jul 2023 18:18


Tgt Ion: 76 Resp: 2605

Ion Ratio Lower Upper

76 100


78 10.8 8.0 12.0

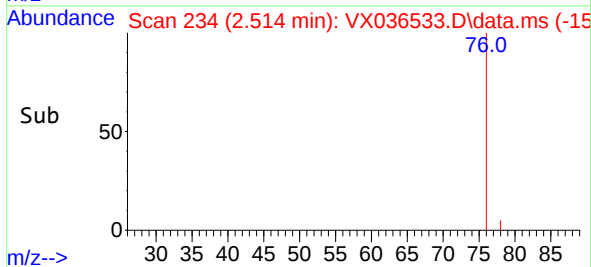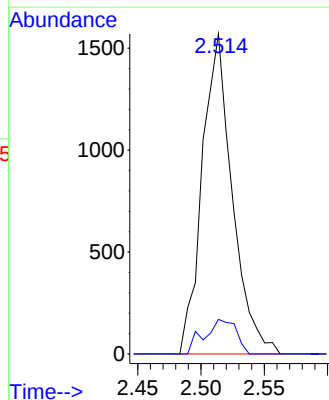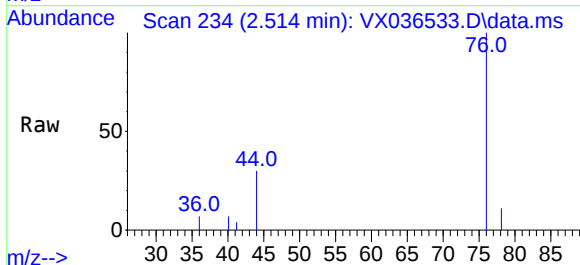






#18
Methylene Chloride
Concen: 0.491 ug/l
RT: 2.794 min Scan# 21
Delta R.T. 0.006 min
Lab File: VX036533.D
Acq: 13 Jul 2023 18:18

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion: 84 Resp: 1128
Ion Ratio Lower Upper
84 100
49 80.6 95.4 143.0#
51 33.8 28.3 42.5
86 66.0 49.0 73.6

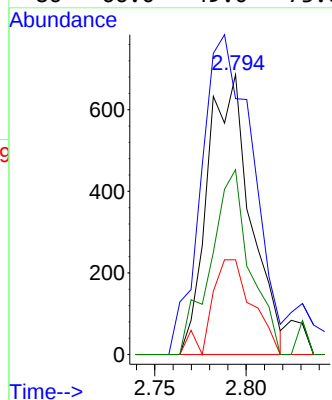

#19
trans-1,2-Dichloroethene
Concen: 0.308 ug/l
RT: 3.087 min Scan# 328
Delta R.T. -0.006 min
Lab File: VX036533.D
Acq: 13 Jul 2023 18:18

Tgt Ion: 96 Resp: 643
Ion Ratio Lower Upper
96 100
61 131.4 108.7 163.1
98 29.4 49.1 73.7#


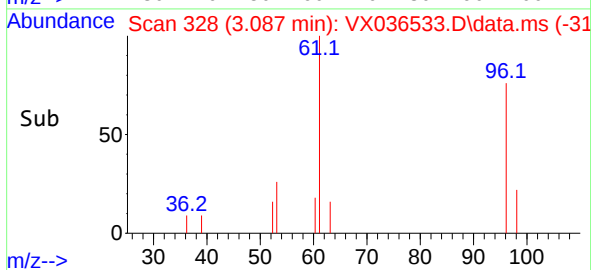
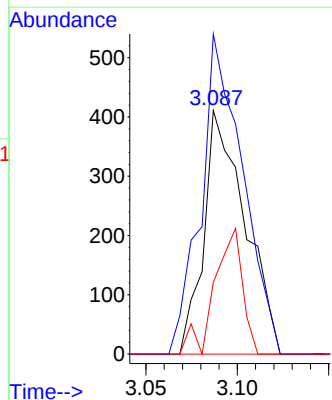





#23
tert-Butyl Alcohol
Concen: 0.425 ug/l
RT: 2.971 min Scan# 309
Delta R.T. 0.006 min
Lab File: VX036533.D
Acq: 13 Jul 2023 18:18




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 59 Resp: 248
Ion Ratio Lower Upper
59 100
52 0.0 142.6 213.8#



#27
1,2-Dichloroethane-d4
Concen: 29.187 ug/l
RT: 5.958 min Scan# 799
Delta R.T. -0.000 min
Lab File: VX036533.D
Acq: 13 Jul 2023 18:18

Tgt Ion: 65 Resp: 79005
Ion Ratio Lower Upper
65 100
67 51.9 42.1 63.1

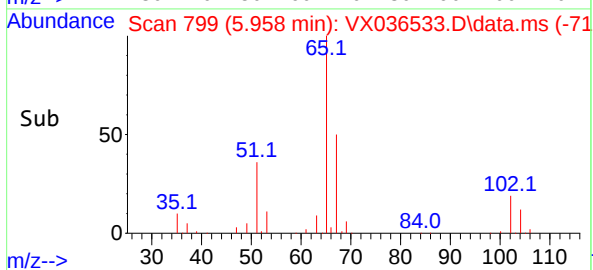



#28

1,4-Difluorobenzene

Concen: 30.000 ug/l

RT: 6.763 min Scan# 91

Delta R.T. -0.000 min

Lab File: VX036533.D

Acq: 13 Jul 2023 18:18

Instrument :

MSVOA_X

ClientSampleId :





Tgt Ion:114 Resp: 170710

Ion Ratio Lower Upper

114 100

63 20.4 16.6 24.8

88 15.9 12.9 19.3

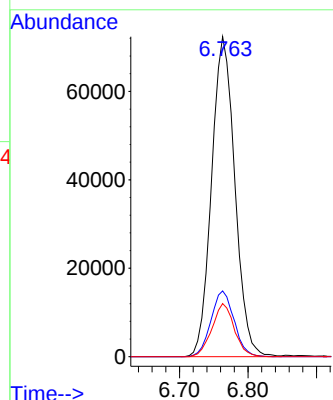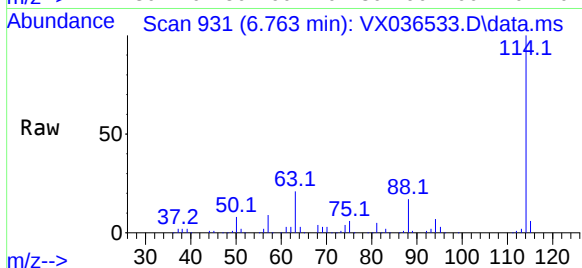

#29

1,1-Dichloropropene

Concen: 0.201 ug/l

RT: 5.690 min Scan# 755

Delta R.T. -0.006 min

Lab File: VX036533.D

Acq: 13 Jul 2023 18:18




Tgt Ion: 75 Resp: 518


Ion Ratio Lower Upper

75 100

110 24.9 0.0 70.4

77 0.0 0.0 62.8


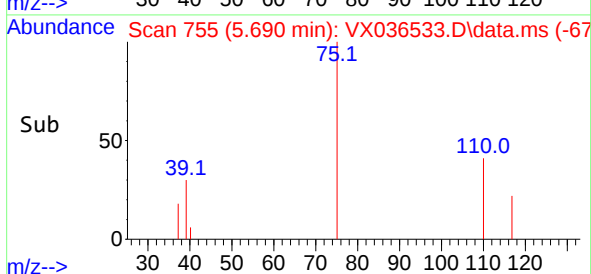
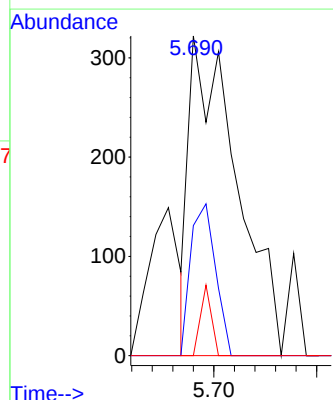
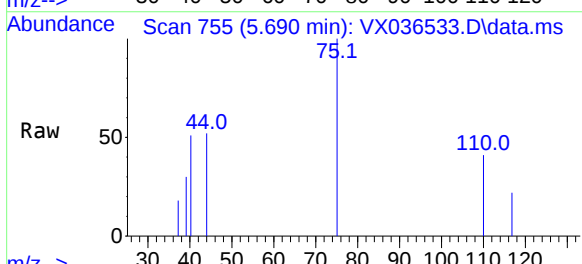




#42
 Vinyl Acetate
 Concen: 0.250 ug/l
 RT: 3.739 min Scan# 41
 Delta R.T. 0.018 min
 Lab File: VX036533.D
 Acq: 13 Jul 2023 18:18




Instrument :
 MSVOA_X
 ClientSampleId :


Tgt Ion: 43 Resp: 1223
 Ion Ratio Lower Upper
 43 100
 86 0.0 7.4 11.0#

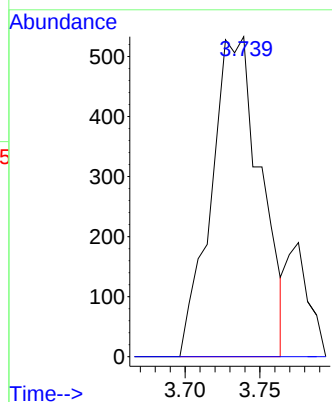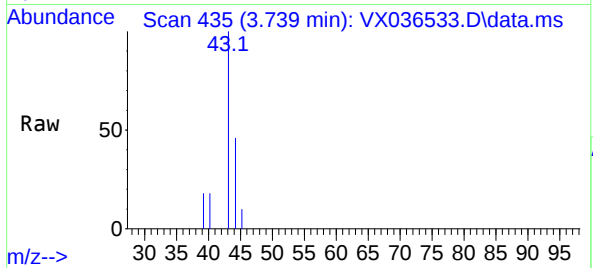

#53
 Dibromochloromethane
 Concen: 0.213 ug/l
 RT: 9.275 min Scan# 1343
 Delta R.T. -0.250 min
 Lab File: VX036533.D
 Acq: 13 Jul 2023 18:18

Tgt Ion: 129 Resp: 454
 Ion Ratio Lower Upper
 129 100
 127 0.0 38.6 115.8#


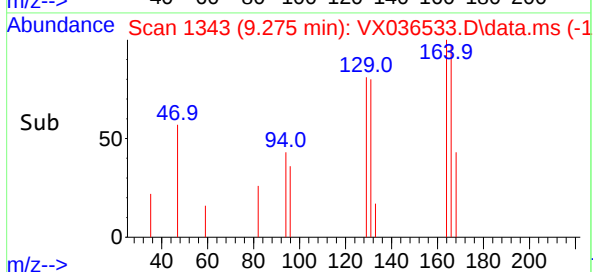
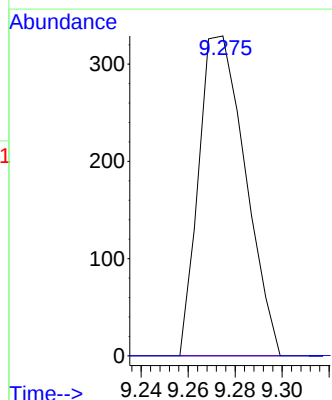





#55
2-Chloroethyl vinyl ether
Concen: 1.037 ug/l
RT: 8.251 min Scan# 1175
Delta R.T. 0.006 min
Lab File: VX036533.D
Acq: 13 Jul 2023 18:18




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 63	Resp:	1852
Ion	Ratio	Lower Upper
63	100	
65	29.4	25.9 38.9
106	25.6	21.8 32.8



#56
Bromoform
Concen: 0.502 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.287 min
Lab File: VX036533.D
Acq: 13 Jul 2023 18:18

Tgt Ion: 173	Resp:	746
Ion	Ratio	Lower Upper
173	100	
175	540.1	38.1 57.1#
254	0.0	6.7 10.1#


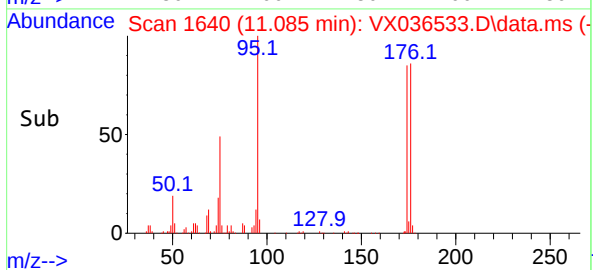






#57
Chlorobenzene-d5
Concen: 30.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX036533.D
Acq: 13 Jul 2023 18:18




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:117 Resp: 153535
Ion Ratio Lower Upper
117 100
82 56.5 44.7 67.1
119 31.9 25.6 38.4

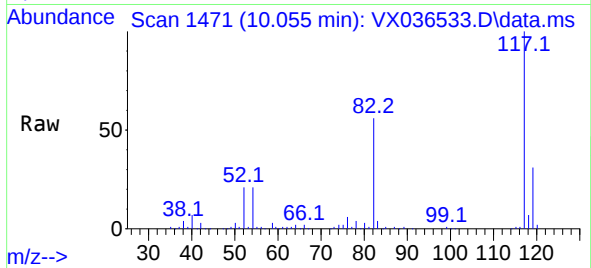

#58
4-Methyl-2-Pentanone
Concen: 0.310 ug/l
RT: 8.580 min Scan# 1229
Delta R.T. 0.006 min
Lab File: VX036533.D
Acq: 13 Jul 2023 18:18

Tgt Ion: 43 Resp: 983
Ion Ratio Lower Upper
43 100
58 22.9 30.9 46.3#
85 0.0 14.4 21.6#

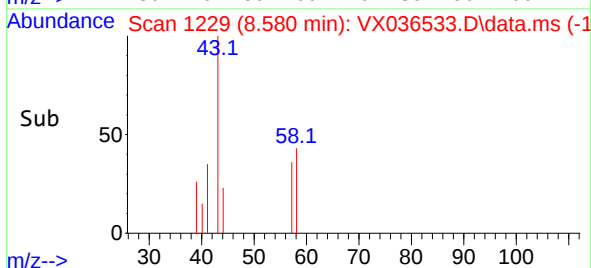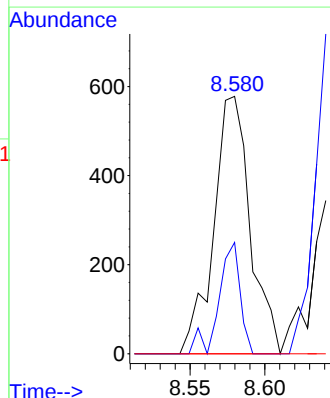



#59

2-Hexanone

Concen: 0.269 ug/l

RT: 9.439 min Scan# 11

Delta R.T. 0.006 min

Lab File: VX036533.D





Acq: 13 Jul 2023 18:18

Instrument :

MSVOA_X

ClientSampleId :

Tgt Ion: 43	Resp: 650
Ion Ratio	Lower Upper
43	100
58	51.7 43.4 65.2
57	0.0 15.1 22.7#

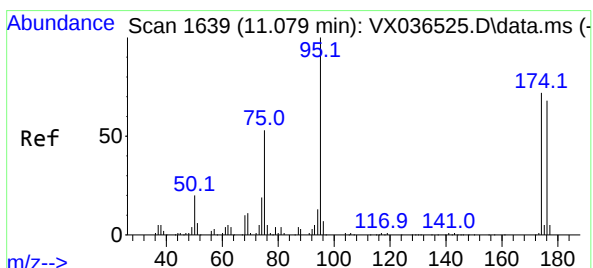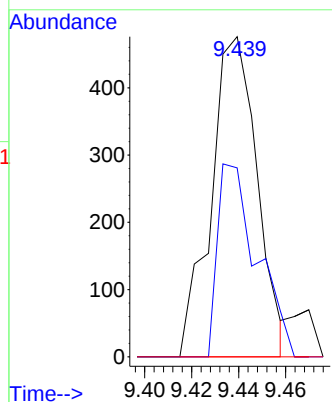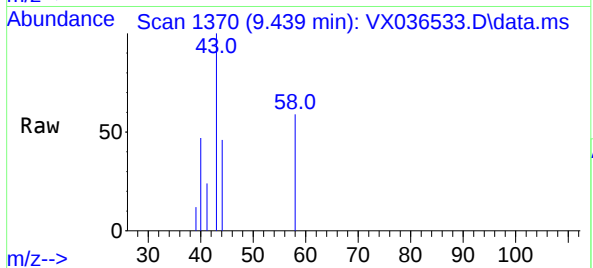

#60

4-Bromofluorobenzene

Concen: 28.022 ug/l




RT: 11.079 min Scan# 1639


Delta R.T. 0.000 min

Lab File: VX036533.D

Acq: 13 Jul 2023 18:18


Tgt Ion: 95	Resp: 69788
Ion Ratio	Lower Upper
95	100
174	77.0 60.5 90.7
176	74.9 58.2 87.4

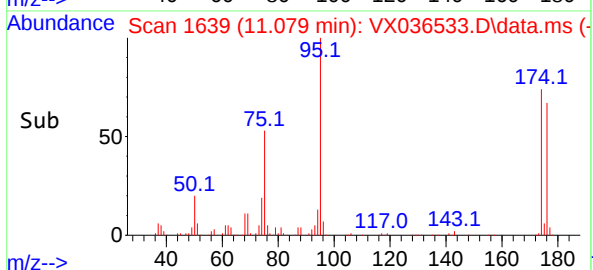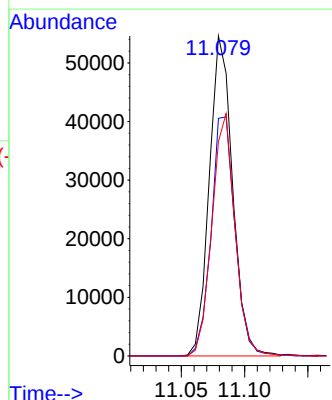






#61
Tetrachloroethene
Concen: 0.318 ug/l
RT: 9.275 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX036533.D
Acq: 13 Jul 2023 18:18

Instrument :
MSVOA_X
ClientSampleId :

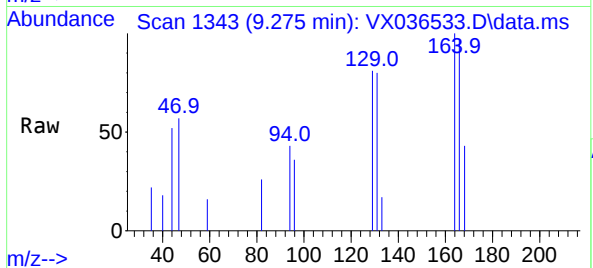

Tgt Ion:164 Resp: 584




Ion	Ratio	Lower	Upper
164	100		
166	96.6	104.5	156.7#
129	81.0	78.0	117.0
131	79.6	77.5	116.3

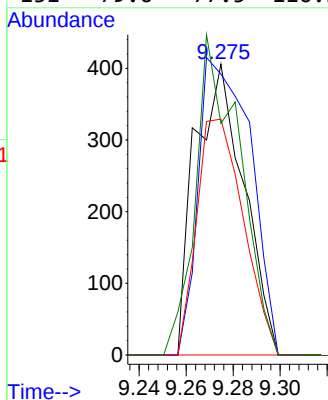


#63
Toluene-d8
Concen: 29.889 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. -0.000 min
Lab File: VX036533.D
Acq: 13 Jul 2023 18:18

Tgt Ion: 98 Resp: 211166


Ion	Ratio	Lower	Upper
98	100		
100	63.0	51.6	77.4

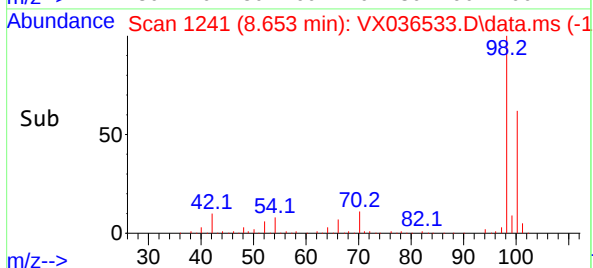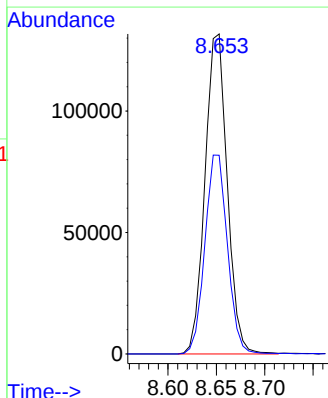






#67
m/p-Xylenes
Concen: 0.407 ug/l
RT: 10.305 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX036533.D
Acq: 13 Jul 2023 18:18


Instrument :
MSVOA_X
ClientSampleId :

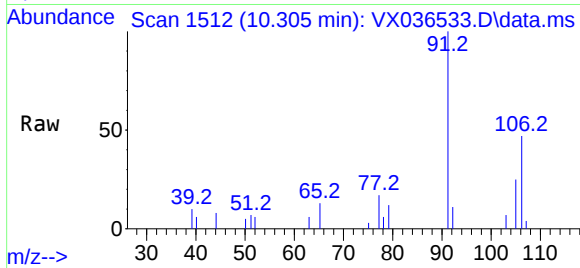



Tgt Ion:106 Resp: 1484
Ion Ratio Lower Upper
106 100
91 202.4 160.5 240.7

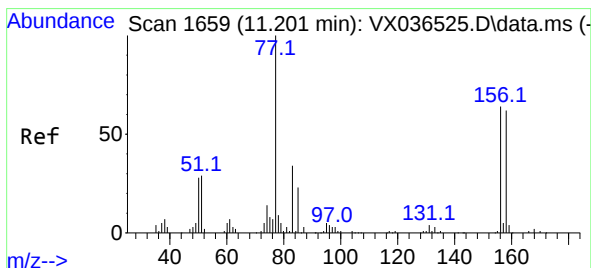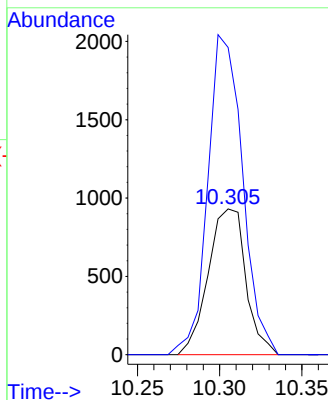


#73
Bromobenzene
Concen: 0.231 ug/l
RT: 11.201 min Scan# 1659
Delta R.T. 0.000 min
Lab File: VX036533.D
Acq: 13 Jul 2023 18:18

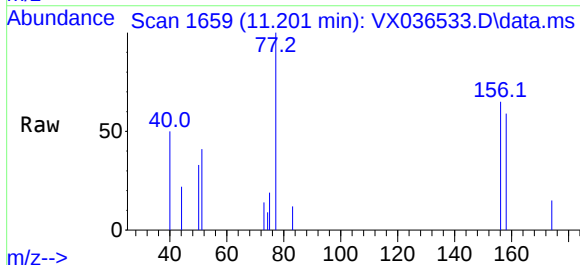

Tgt Ion:156 Resp: 515
Ion Ratio Lower Upper
156 100
77 154.8 0.0 333.0
158 84.3 0.0 196.4



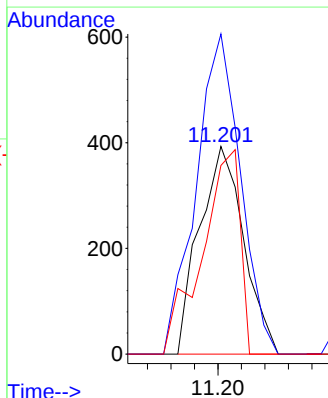
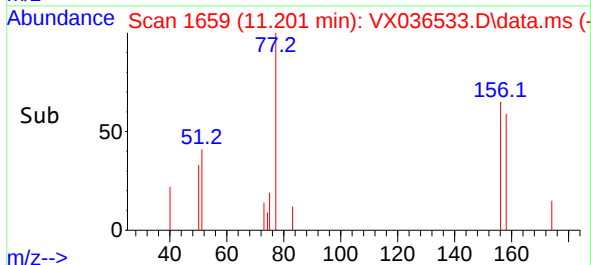




#74
n-propylbenzene
Concen: 0.251 ug/l
RT: 11.305 min Scan# 1676
Delta R.T. -0.000 min
Lab File: VX036533.D
Acq: 13 Jul 2023 18:18




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 91 Resp: 2669
Ion Ratio Lower Upper
91 100
120 22.8 0.0 46.6

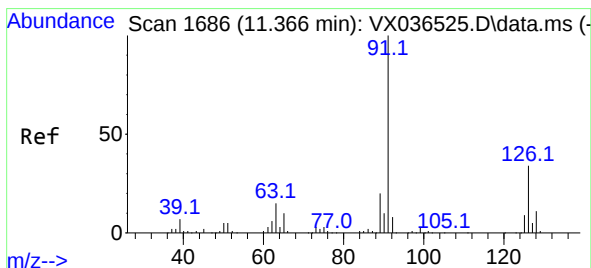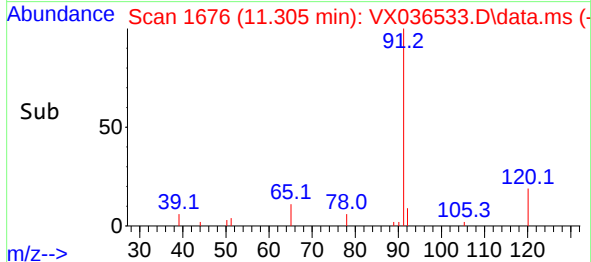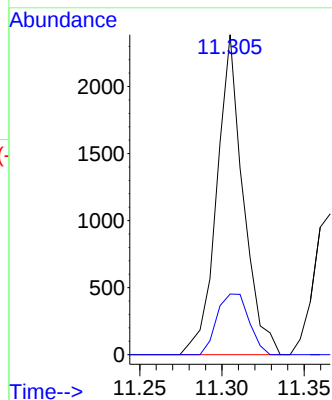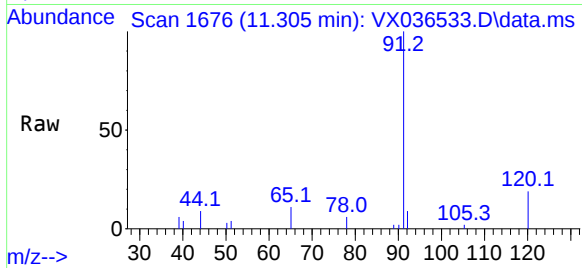

#75
2-Chlorotoluene
Concen: 0.223 ug/l
RT: 11.366 min Scan# 1686
Delta R.T. 0.000 min
Lab File: VX036533.D
Acq: 13 Jul 2023 18:18

Tgt Ion: 91 Resp: 1440
Ion Ratio Lower Upper
91 100
126 32.3 0.0 66.2


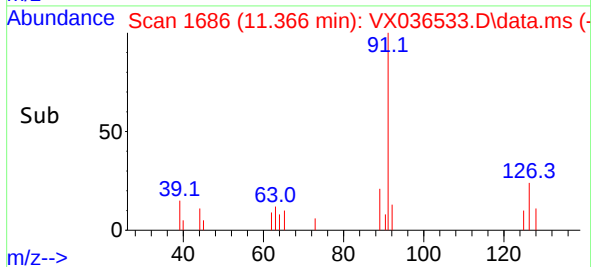
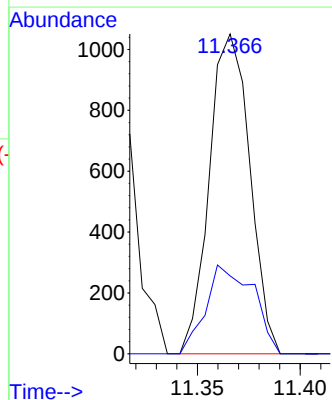
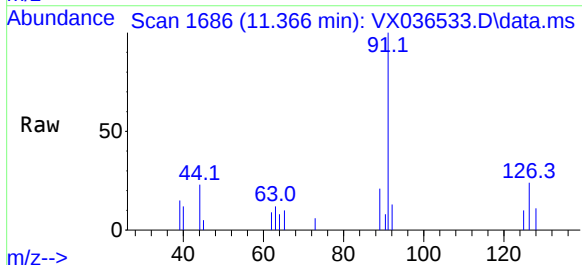




#76
1,3,5-Trimethylbenzene
Concen: 0.209 ug/l
RT: 11.451 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX036533.D
Acq: 13 Jul 2023 18:18




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:105 Resp: 1624
Ion Ratio Lower Upper
105 100
120 49.5 0.0 96.4

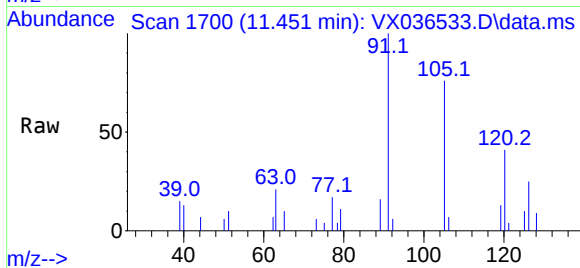

#77
t-1,4-Dichloro-2-butene
Concen: 36.125 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.061 min
Lab File: VX036533.D
Acq: 13 Jul 2023 18:18

Tgt Ion: 75 Resp: 36198
Ion Ratio Lower Upper
75 100
53 0.0 53.9 161.7#
89 0.0 22.1 66.1#


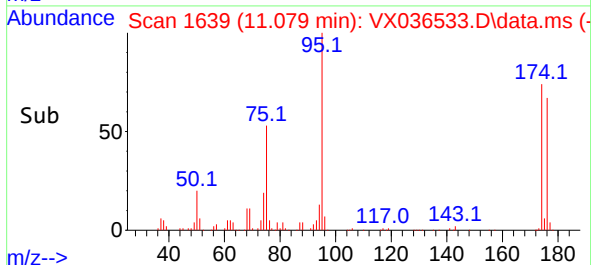
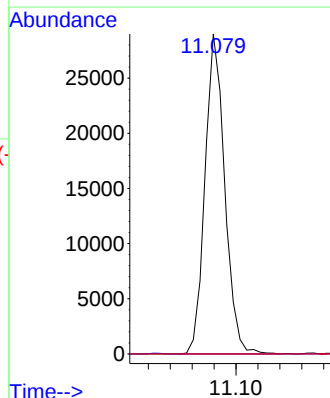
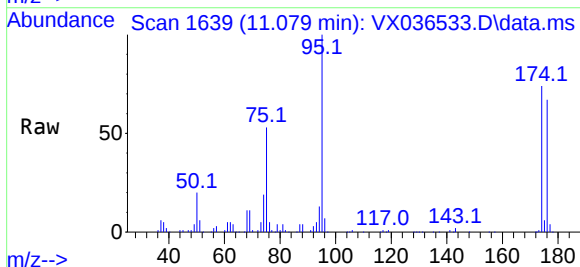




#78
4-Chlorotoluene
Concen: 0.313 ug/l
RT: 11.463 min Scan# 11
Delta R.T. 0.006 min
Lab File: VX036533.D
Acq: 13 Jul 2023 18:18




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 91 Resp: 2300
Ion Ratio Lower Upper
91 100
126 27.5 0.0 59.4

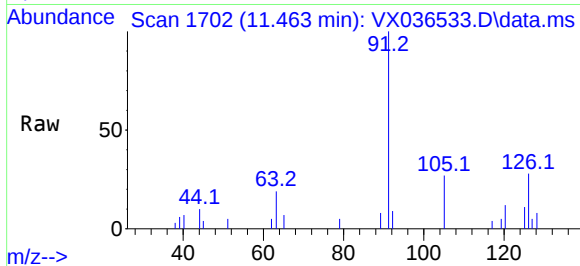

#80
1,2,4-Trimethylbenzene
Concen: 0.272 ug/l
RT: 11.750 min Scan# 1749
Delta R.T. 0.000 min
Lab File: VX036533.D
Acq: 13 Jul 2023 18:18

Tgt Ion: 105 Resp: 2087
Ion Ratio Lower Upper
105 100
120 39.8 0.0 90.2


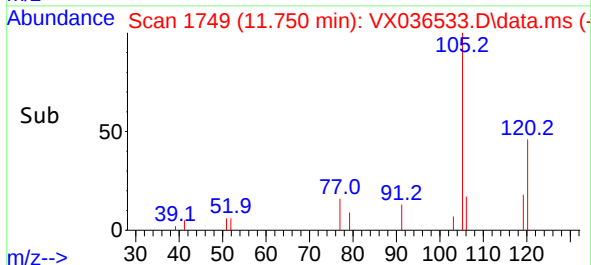

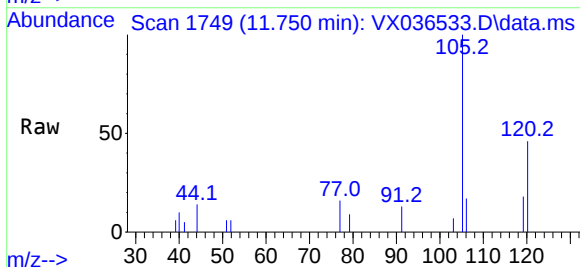




#81
 sec-Butylbenzene
 Concen: 0.246 ug/l
 RT: 11.890 min Scan# 1772
 Delta R.T. 0.000 min
 Lab File: VX036533.D
 Acq: 13 Jul 2023 18:18




Instrument :
 MSVOA_X
 ClientSampleId :


Tgt Ion:105 Resp: 2278
 Ion Ratio Lower Upper
 105 100
 134 19.1 0.0 41.2

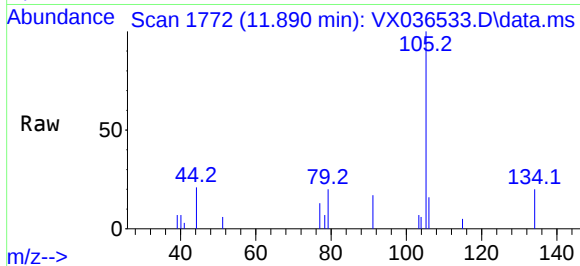

#82
 p-Isopropyltoluene
 Concen: 0.304 ug/l
 RT: 12.012 min Scan# 1792
 Delta R.T. 0.000 min
 Lab File: VX036533.D
 Acq: 13 Jul 2023 18:18

Tgt Ion:119 Resp: 2345
 Ion Ratio Lower Upper
 119 100
 134 22.8 0.0 53.2
 91 29.1 0.0 49.4


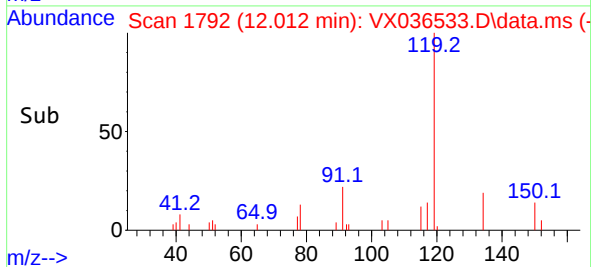

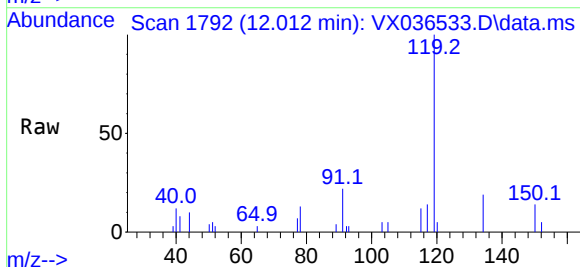




#83
1,3-Dichlorobenzene
Concen: 0.416 ug/l
RT: 11.969 min Scan# 1785
Delta R.T. 0.000 min
Lab File: VX036533.D
Acq: 13 Jul 2023 18:18




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:146 Resp: 1726
Ion Ratio Lower Upper
146 100
111 39.2 20.4 61.2
148 67.7 31.6 94.8

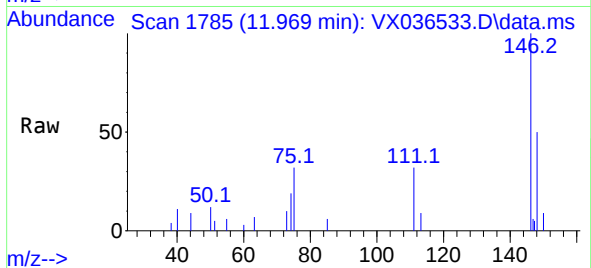

#84
1,4-Dichlorobenzene
Concen: 0.429 ug/l
RT: 12.043 min Scan# 1797
Delta R.T. -0.000 min
Lab File: VX036533.D
Acq: 13 Jul 2023 18:18

Tgt Ion:146 Resp: 1774
Ion Ratio Lower Upper
146 100
111 37.0 20.2 60.6
148 63.4 32.1 96.3


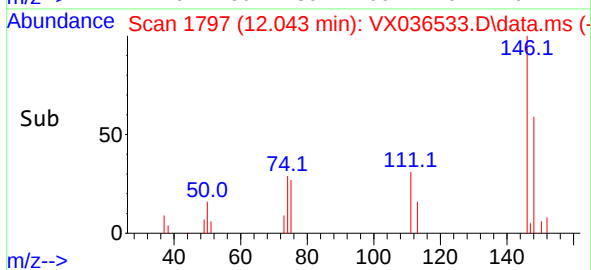






#85
n-Butylbenzene
Concen: 0.386 ug/l
RT: 12.335 min Scan# 1845
Delta R.T. -0.000 min
Lab File: VX036533.D
Acq: 13 Jul 2023 18:18




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 91	Resp: 2711
Ion Ratio	Lower Upper
91 100	
92 51.1	0.0 105.2
134 27.2	0.0 51.4

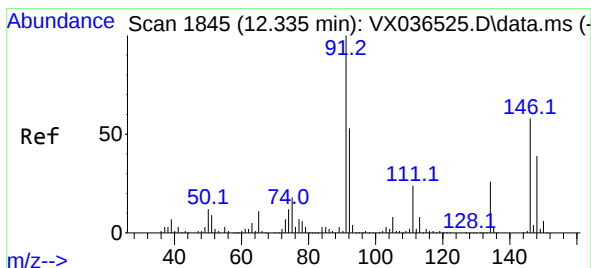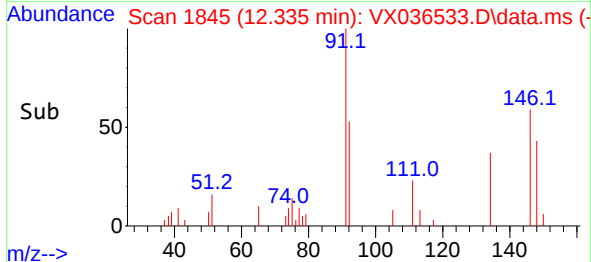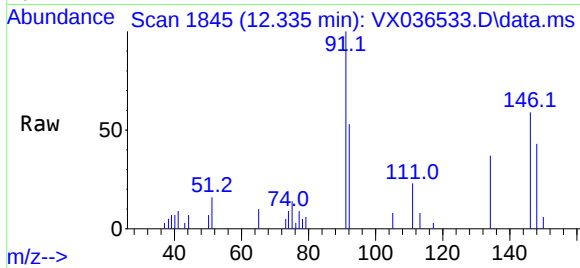

#87
1,2-Dichlorobenzene
Concen: 0.311 ug/l
RT: 12.335 min Scan# 1845
Delta R.T. -0.000 min
Lab File: VX036533.D
Acq: 13 Jul 2023 18:18


Tgt Ion:146	Resp:	1294	
Ion Ratio	Lower	Upper	
146	100		
111	40.8	21.4	64.3
148	59.7	33.2	99.6

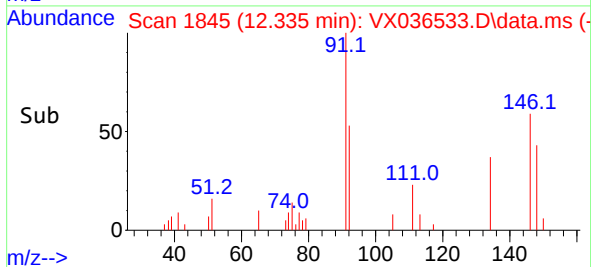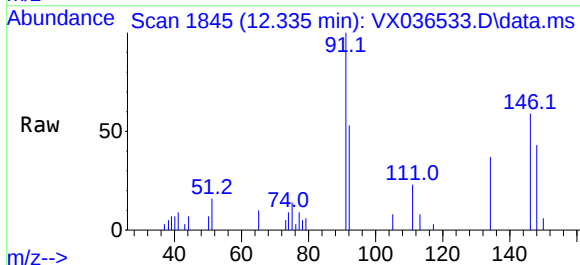






#89
1,2,4-Trichlorobenzene
Concen: 0.673 ug/l
RT: 13.591 min Scan# 2050
Delta R.T. 0.006 min
Lab File: VX036533.D
Acq: 13 Jul 2023 18:18

Instrument :
MSVOA_X
ClientSampleId :



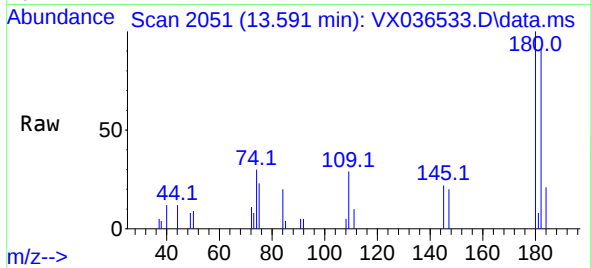



Tgt Ion:180 Resp: 1767
Ion Ratio Lower Upper
180 100
182 90.8 75.6 113.4
145 27.8 25.4 38.2

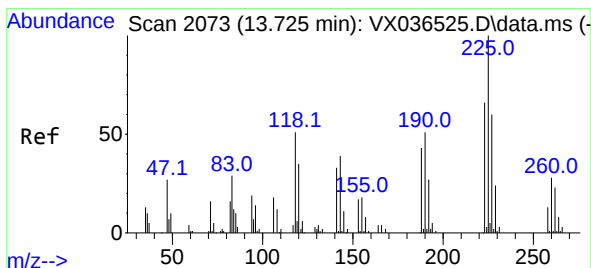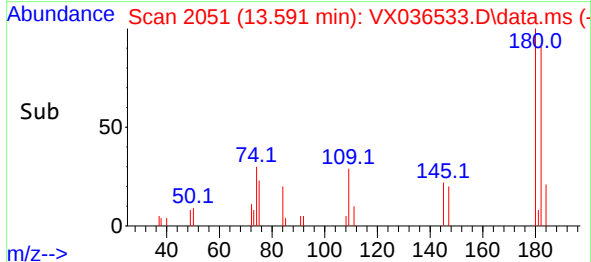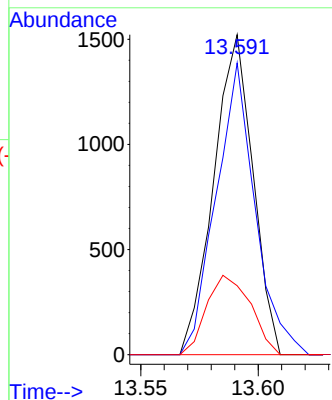

#90
Hexachlorobutadiene
Concen: 0.740 ug/l
RT: 13.719 min Scan# 2072
Delta R.T. -0.006 min
Lab File: VX036533.D
Acq: 13 Jul 2023 18:18


Tgt Ion:225 Resp: 705
Ion Ratio Lower Upper
225 100
223 59.7 0.0 124.2
227 64.5 0.0 120.4

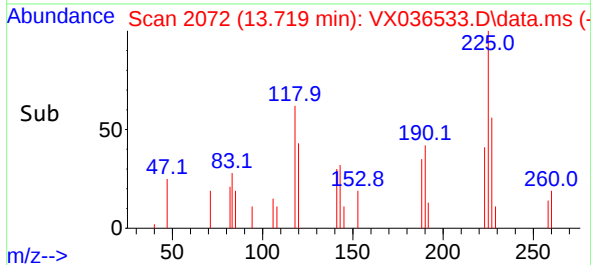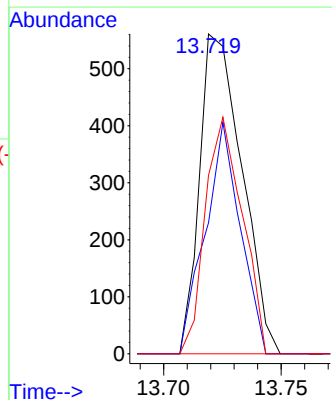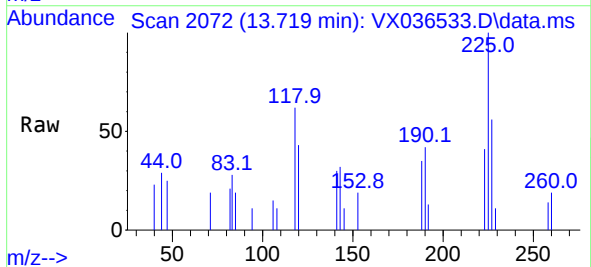






#91
Naphthalene
Concen: 0.406 ug/l
RT: 13.780 min Scan# 2081
Delta R.T. 0.006 min
Lab File: VX036533.D
Acq: 13 Jul 2023 18:18

Instrument :
MSVOA_X
ClientSampleId :

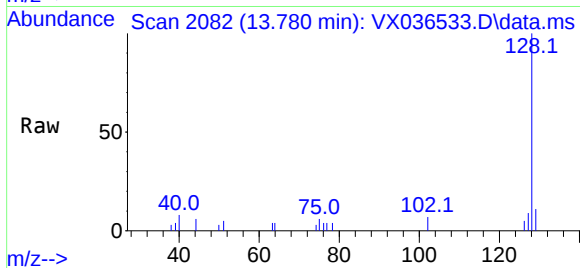

Tgt Ion:128 Resp: 3740
Ion Ratio Lower Upper
128 100
127 10.0 10.3 15.5#
129 7.7 8.7 13.1#

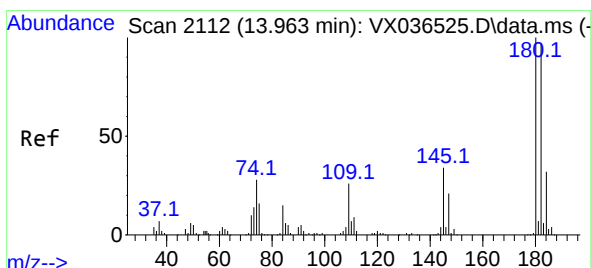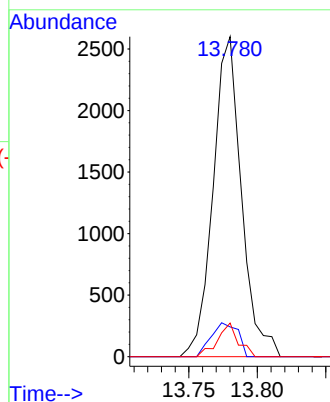

#92
1,2,3-Trichlorobenzene
Concen: 0.565 ug/l
RT: 13.963 min Scan# 2112
Delta R.T. 0.000 min
Lab File: VX036533.D
Acq: 13 Jul 2023 18:18

Tgt Ion:180 Resp: 1496
Ion Ratio Lower Upper
180 100
182 92.0 0.0 190.6
145 32.4 0.0 66.8

