

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071423\
 Data File : VX036545.D
 Acq On : 13 Jul 2023 23:01
 Operator : JC/MD
 Sample : 03593-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 002-35TH-AVE(JUNE)

Quant Time: Jul 14 04:39:51 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X071423W.M
 Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 QLast Update : Fri Jul 14 04:32:22 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Bromochloromethane	4.904	128	31592	30.000	ug/l	0.00
28) 1,4-Difluorobenzene	6.763	114	167079	30.000	ug/l	0.00
57) Chlorobenzene-d5	10.055	117	154467	30.000	ug/l	0.00
System Monitoring Compounds						
27) 1,2-Dichloroethane-d4	5.952	65	77491	29.554	ug/l	0.00
Spiked Amount 30.000	Range 91 - 110		Recovery =	98.500%		
60) 4-Bromofluorobenzene	11.079	95	72621	28.983	ug/l	0.00
Spiked Amount 30.000	Range 63 - 112		Recovery =	96.600%		
63) Toluene-d8	8.647	98	207294	29.164	ug/l	0.00
Spiked Amount 30.000	Range 91 - 112		Recovery =	97.200%		
Target Compounds						
					Qvalue	
12) Methyl Acetate	2.703	43	11048	2.542	ug/l	95
15) Acetone	2.380	58	266986	774.197	ug/l	100
16) Carbon Disulfide	2.514	76	4671	1.041	ug/l #	87
18) Methylene Chloride	2.794	84	1558	0.700	ug/l #	81
30) 2-Butanone	4.556	43	83280	52.497	ug/l	99
58) 4-Methyl-2-Pentanone	8.574	43	15635	4.895	ug/l	98
62) Toluene	8.720	91	1958651	225.994	ug/l	98
67) m/p-Xylenes	10.305	106	1221	0.333	ug/l	92
80) 1,2,4-Trimethylbenzene	11.756	105	6827	0.883	ug/l	46
82) p-Isopropyltoluene	12.012	119	8590	1.108	ug/l	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071423\
Data File : VX036545.D
Acq On : 13 Jul 2023 23:01
Operator : JC/MD
Sample : 03593-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
002-35TH-AVE(JUNE)

Quant Time: Jul 14 04:39:51 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X071423W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
QLast Update : Fri Jul 14 04:32:22 2023
Response via : Initial Calibration




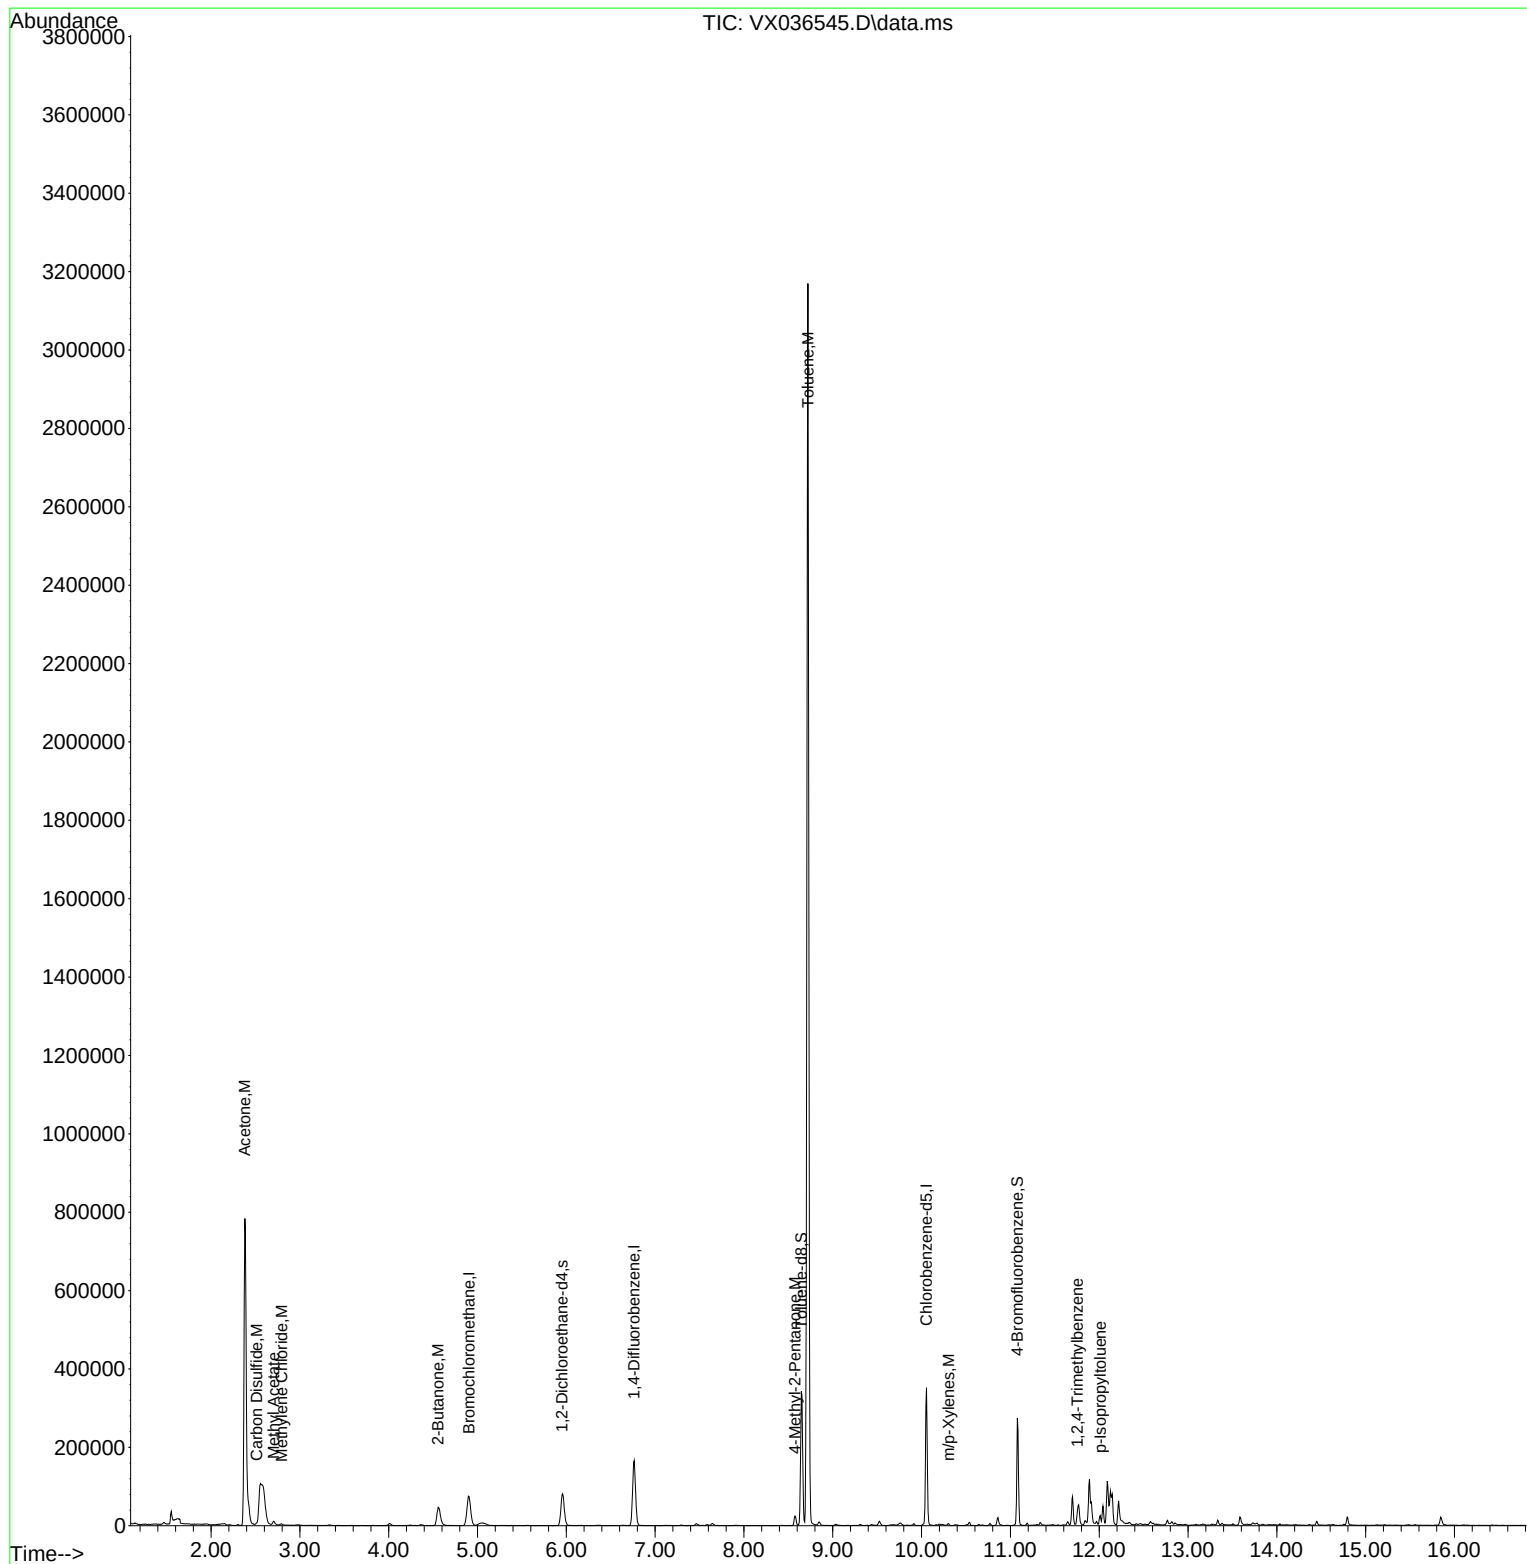




#1
Bromochloromethane
Concen: 30.000 ug/l
RT: 4.904 min Scan# 61
Delta R.T. -0.000 min
Lab File: VX036545.D
Acq: 13 Jul 2023 23:01




Instrument :
MSVOA_X
ClientSampleId :
002-35TH-AVE(JUNE)


Tgt Ion:128 Resp: 31592
Ion Ratio Lower Upper
128 100
49 163.7 0.0 406.3
130 127.9 0.0 328.0

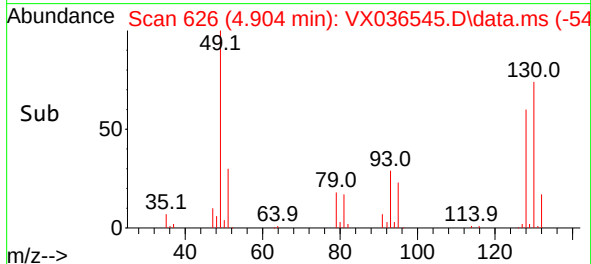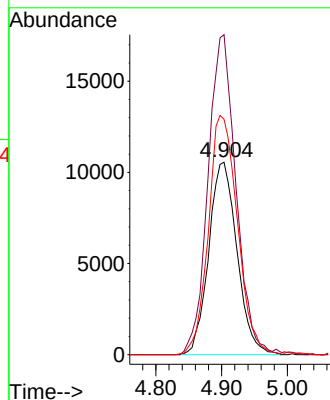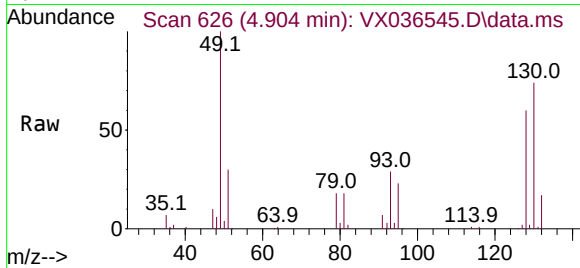

#12
Methyl Acetate
Concen: 2.542 ug/l
RT: 2.703 min Scan# 265
Delta R.T. -0.000 min
Lab File: VX036545.D
Acq: 13 Jul 2023 23:01

Tgt Ion: 43 Resp: 11048
Ion Ratio Lower Upper
43 100
74 23.1 20.3 30.5

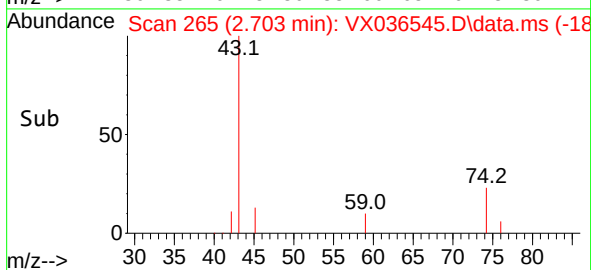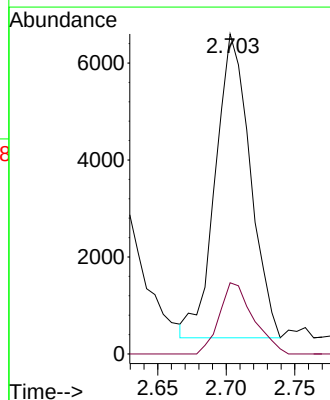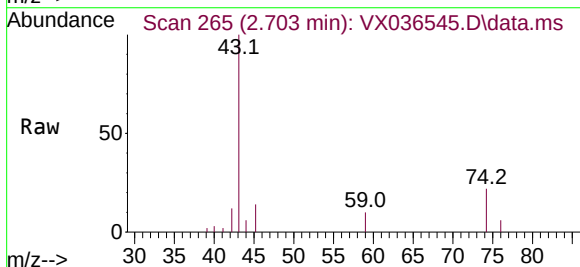

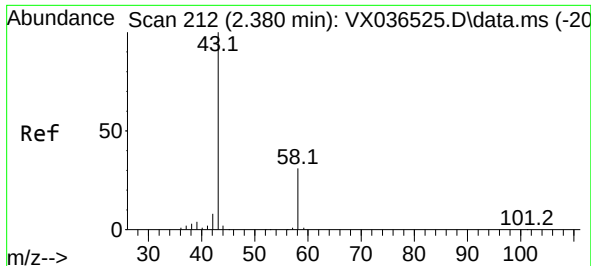

#15

Acetone

Concen: 774.197 ug/l

RT: 2.380 min Scan# 212

Delta R.T. -0.000 min

Lab File: VX036545.D

Acq: 13 Jul 2023 23:01

Instrument :

MSVOA_X

ClientSampleId :





002-35TH-AVE(JUNE)

Tgt Ion: 58 Resp: 266986

Ion Ratio Lower Upper

58 100

43 325.9 261.0 391.4

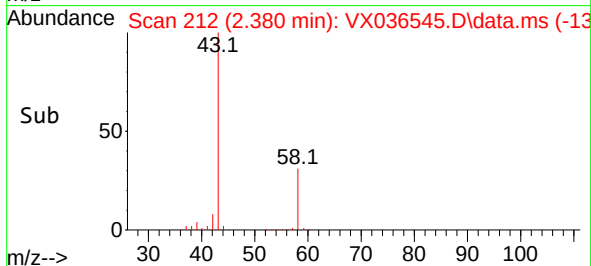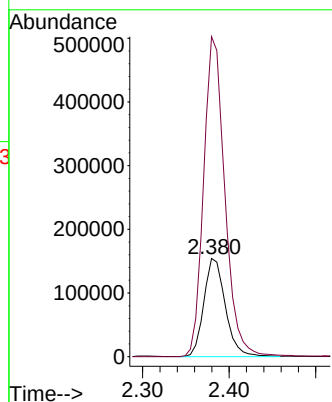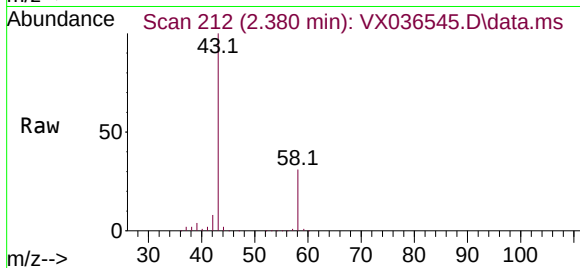

#16

Carbon Disulfide

Concen: 1.041 ug/l

RT: 2.514 min Scan# 234

Delta R.T. -0.000 min

Lab File: VX036545.D




Acq: 13 Jul 2023 23:01


Tgt Ion: 76 Resp: 4671

Ion Ratio Lower Upper

76 100


78 5.0 8.0 12.0#

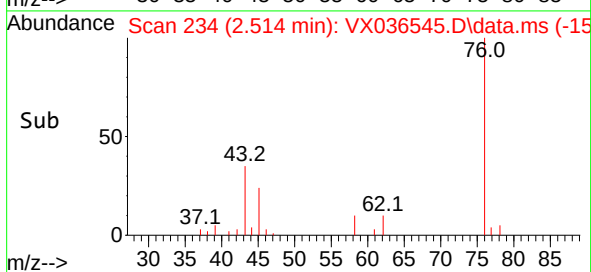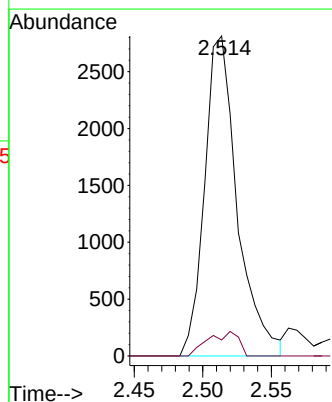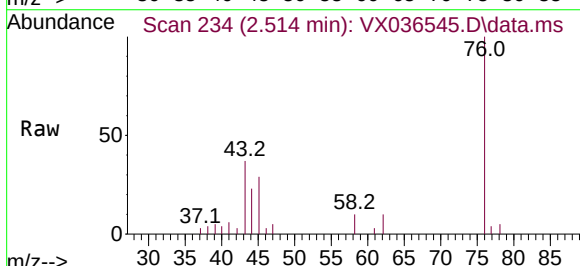



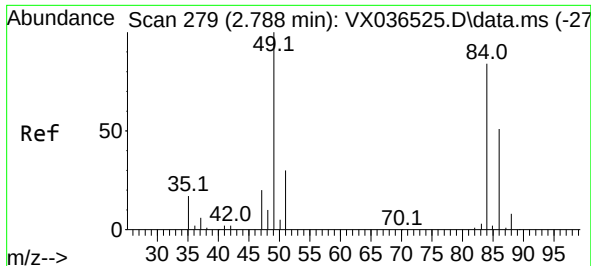


#18
Methylene Chloride
Concen: 0.700 ug/l
RT: 2.794 min Scan# 21
Delta R.T. 0.006 min
Lab File: VX036545.D
Acq: 13 Jul 2023 23:01

Instrument :
MSVOA_X
ClientSampleId :
002-35TH-AVE(JUNE)







Tgt Ion: 84 Resp: 1558
Ion Ratio Lower Upper
84 100
49 98.5 95.4 143.0
51 36.2 28.3 42.5
86 39.6 49.0 73.6#

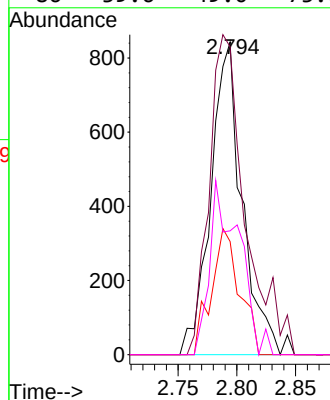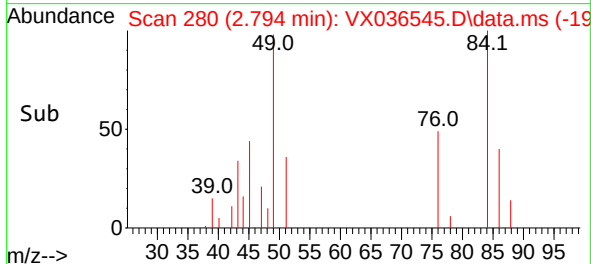

#27
1,2-Dichloroethane-d4
Concen: 29.554 ug/l
RT: 5.952 min Scan# 798
Delta R.T. -0.006 min
Lab File: VX036545.D
Acq: 13 Jul 2023 23:01

Tgt Ion: 65 Resp: 77491
Ion Ratio Lower Upper
65 100
67 51.7 42.1 63.1

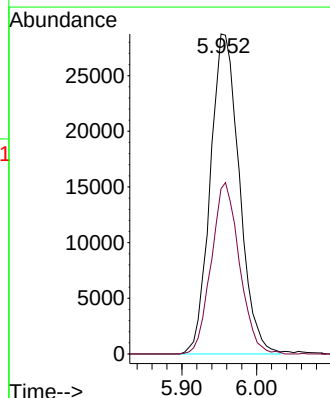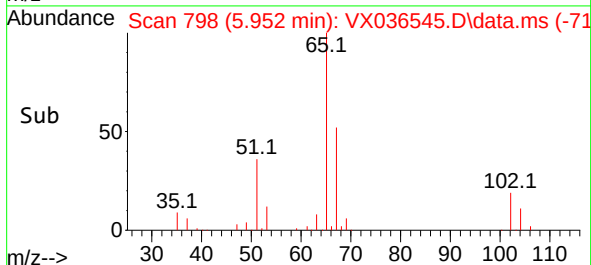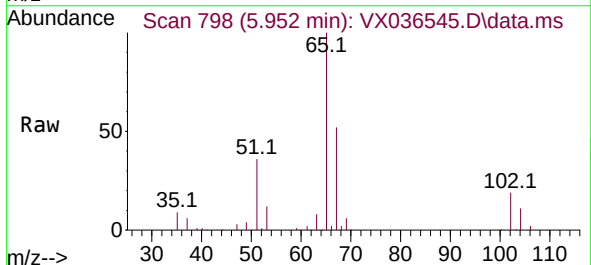

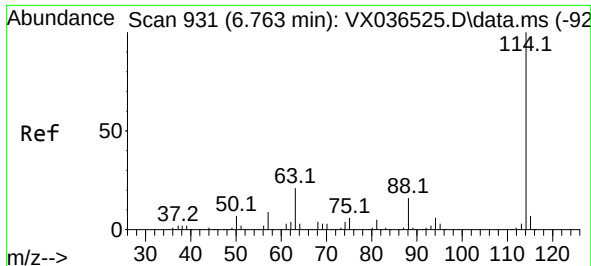

#28

1,4-Difluorobenzene

Concen: 30.000 ug/l

RT: 6.763 min Scan# 91

Delta R.T. -0.000 min

Lab File: VX036545.D

Acq: 13 Jul 2023 23:01

Instrument :

MSVOA_X

ClientSampleId :

002-35TH-AVE(JUNE)





Tgt Ion:114 Resp: 167079

Ion Ratio Lower Upper

114 100

63 20.3 16.6 24.8

88 15.3 12.9 19.3

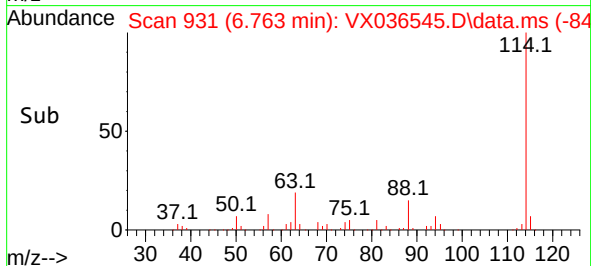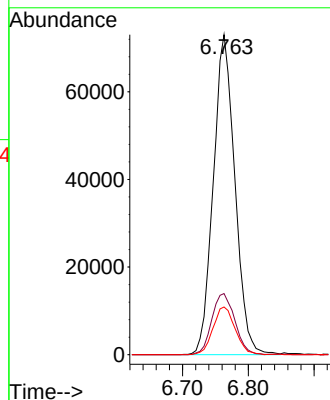

#30

2-Butanone

Concen: 52.497 ug/l

RT: 4.556 min Scan# 569

Delta R.T. -0.006 min

Lab File: VX036545.D

Acq: 13 Jul 2023 23:01




Tgt Ion: 43 Resp: 83280


Ion Ratio Lower Upper

43 100

57 7.6 6.4 9.6

72 27.2 21.6 32.4

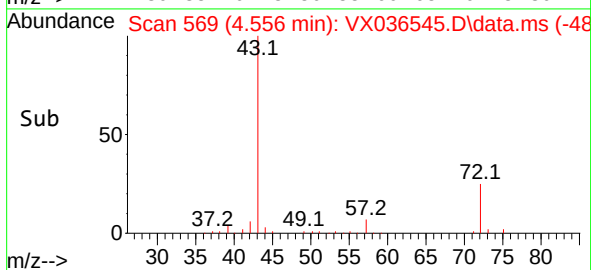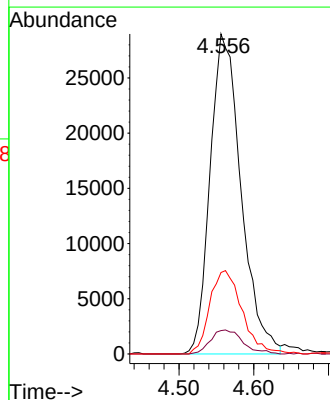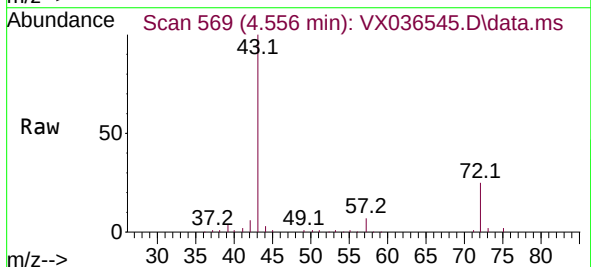

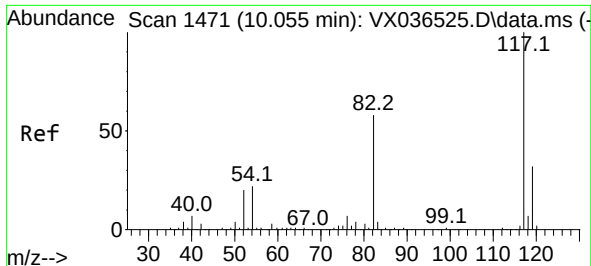

#57

Chlorobenzene-d5

Concen: 30.000 ug/l

RT: 10.055 min Scan# 1471

Delta R.T. -0.000 min

Lab File: VX036545.D

Acq: 13 Jul 2023 23:01

Instrument :

MSVOA_X

ClientSampleId :

002-35TH-AVE(JUNE)





Tgt Ion:117 Resp: 154467

Ion Ratio Lower Upper

117 100

82 55.0 44.7 67.1

119 31.5 25.6 38.4

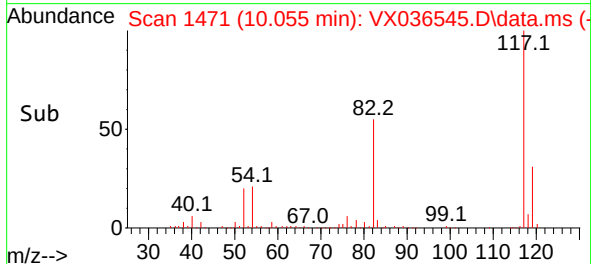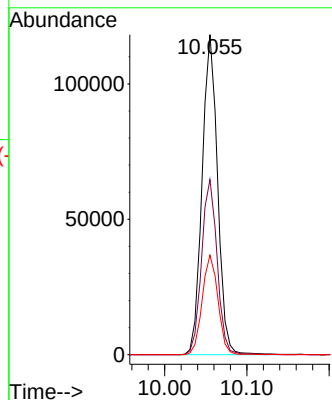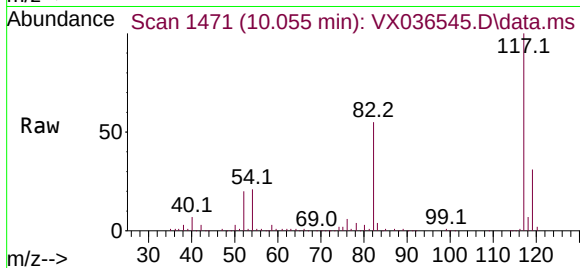

#58

4-Methyl-2-Pentanone

Concen: 4.895 ug/l

RT: 8.574 min Scan# 1228

Delta R.T. -0.000 min

Lab File: VX036545.D

Acq: 13 Jul 2023 23:01




Tgt Ion: 43 Resp: 15635


Ion Ratio Lower Upper

43 100

58 36.6 30.9 46.3

85 18.1 14.4 21.6


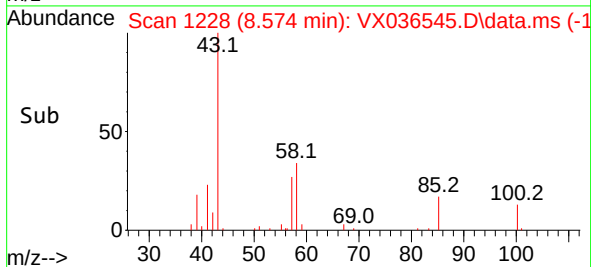
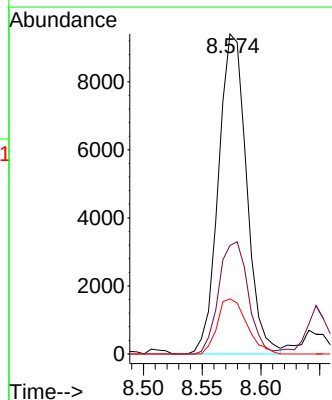
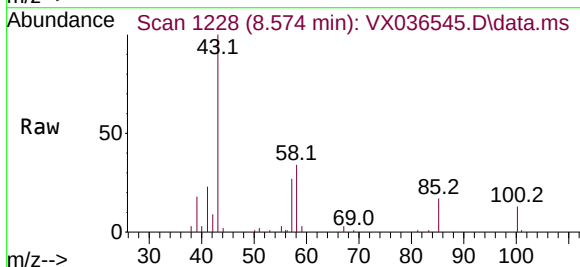


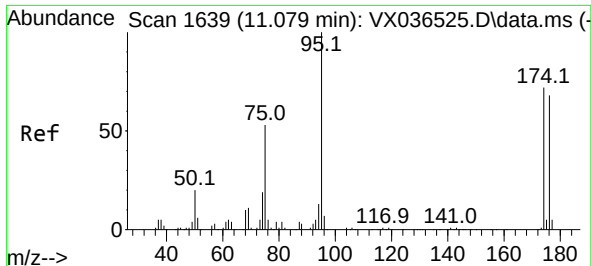

#60
4-Bromofluorobenzene
Concen: 28.983 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.000 min
Lab File: VX036545.D
Acq: 13 Jul 2023 23:01




Instrument :
MSVOA_X
ClientSampleId :
002-35TH-AVE(JUNE)


Tgt Ion: 95 Resp: 72621
Ion Ratio Lower Upper
95 100
174 74.2 60.5 90.7
176 71.9 58.2 87.4

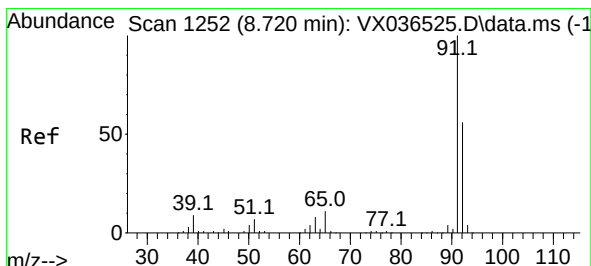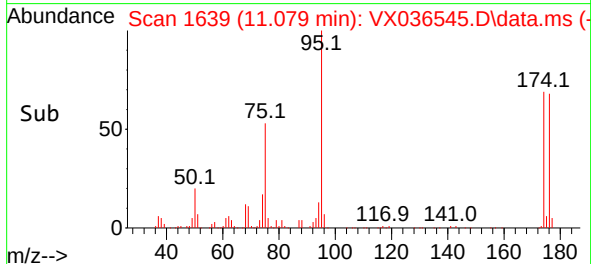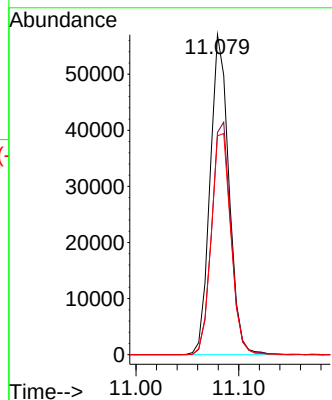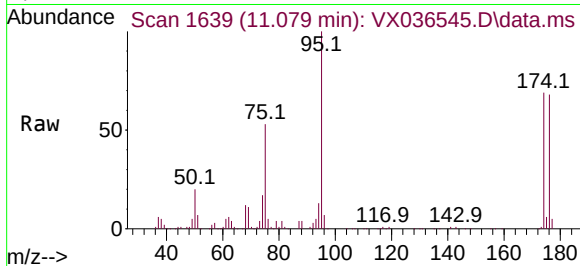

#62
Toluene
Concen: 225.994 ug/l
RT: 8.720 min Scan# 1252
Delta R.T. -0.000 min
Lab File: VX036545.D
Acq: 13 Jul 2023 23:01

Tgt Ion: 91 Resp: 1958651
Ion Ratio Lower Upper
91 100
92 57.5 44.9 67.3


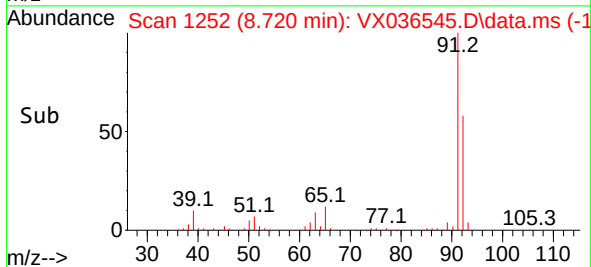
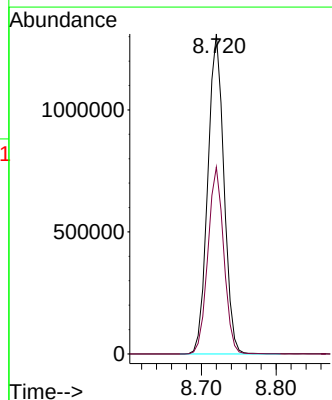
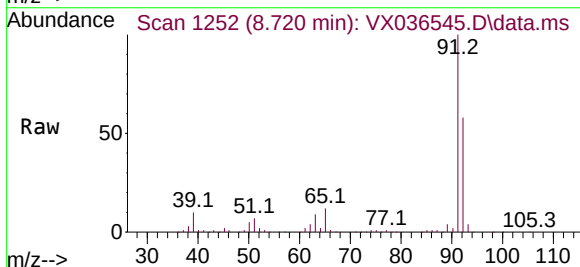




#63
Toluene-d8
Concen: 29.164 ug/l
RT: 8.647 min Scan# 11
Delta R.T. -0.006 min
Lab File: VX036545.D
Acq: 13 Jul 2023 23:01




Instrument :
MSVOA_X
ClientSampleId :
002-35TH-AVE(JUNE)


Tgt Ion: 98 Resp: 207294
Ion Ratio Lower Upper
98 100
100 62.4 51.6 77.4

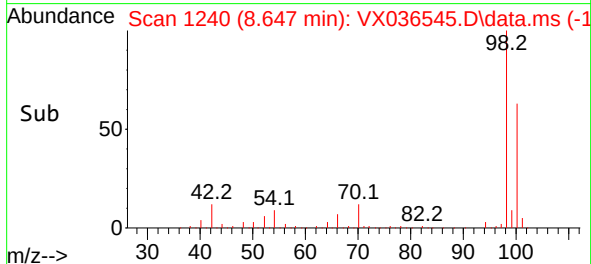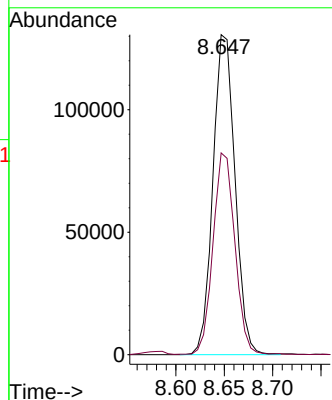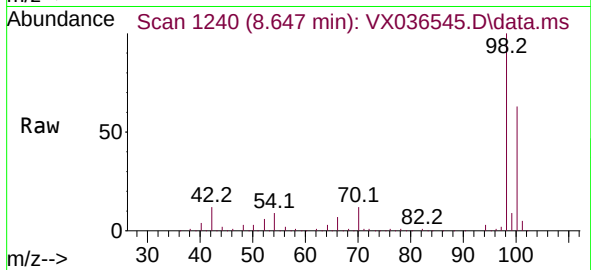

#67
m/p-Xylenes
Concen: 0.333 ug/l
RT: 10.305 min Scan# 1512
Delta R.T. -0.000 min
Lab File: VX036545.D
Acq: 13 Jul 2023 23:01

Tgt Ion:106 Resp: 1221
Ion Ratio Lower Upper
106 100
91 213.2 160.5 240.7

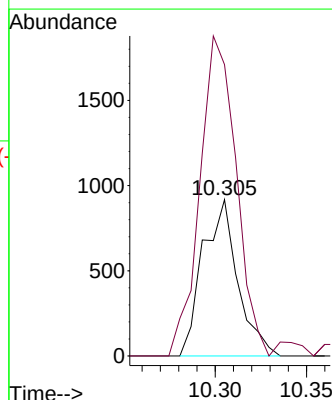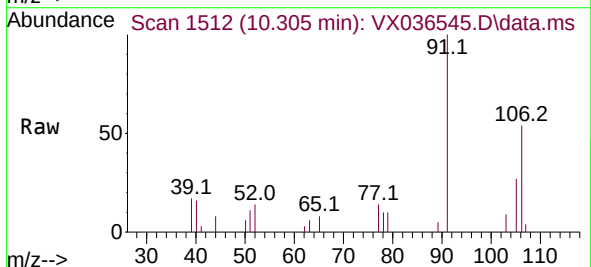



#80

1,2,4-Trimethylbenzene

Concen: 0.883 ug/l

RT: 11.756 min Scan# 11

Delta R.T. 0.006 min

Lab File: VX036545.D

Acq: 13 Jul 2023 23:01

Instrument :

MSVOA_X

ClientSampleId :





002-35TH-AVE(JUNE)

Tgt Ion:105 Resp: 6827

Ion Ratio Lower Upper

105 100

120 9.6 0.0 90.2

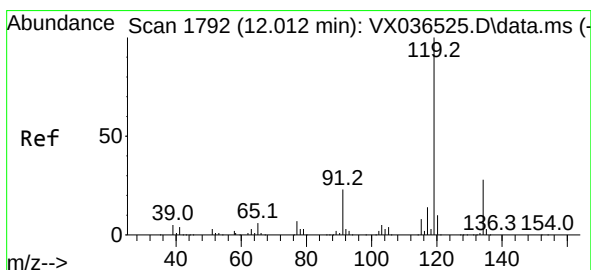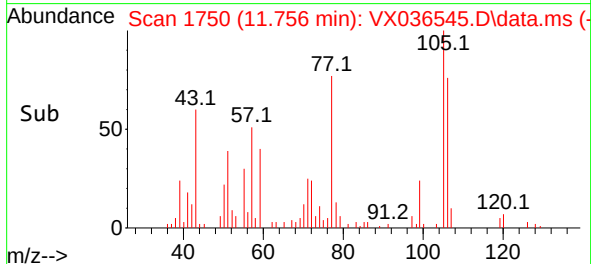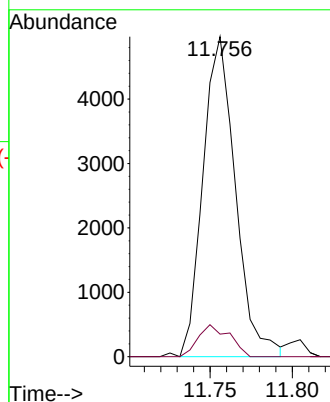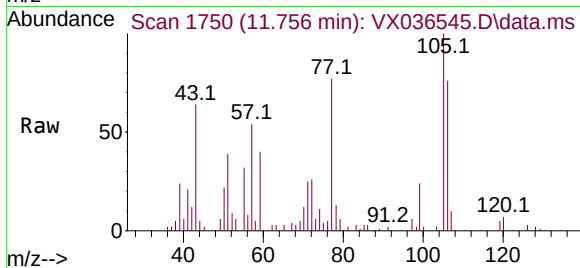

#82

p-Isopropyltoluene

Concen: 1.108 ug/l

RT: 12.012 min Scan# 1792

Delta R.T. -0.000 min

Lab File: VX036545.D

Acq: 13 Jul 2023 23:01

Tgt Ion:119 Resp: 8590

Ion Ratio Lower Upper

119 100

134 25.9 0.0 53.2

91 24.9 0.0 49.4

