
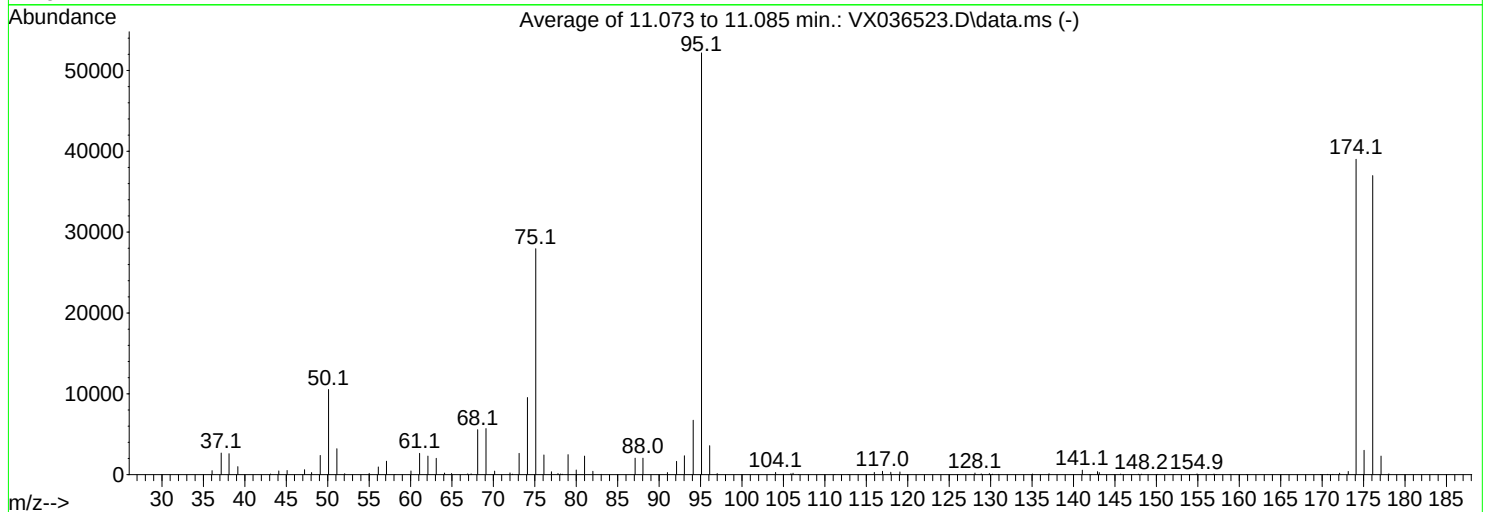


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071423\
Data File : VX036523.D
Acq On : 13 Jul 2023 13:40
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X071423W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Fri Jul 14 04:32:22 2023

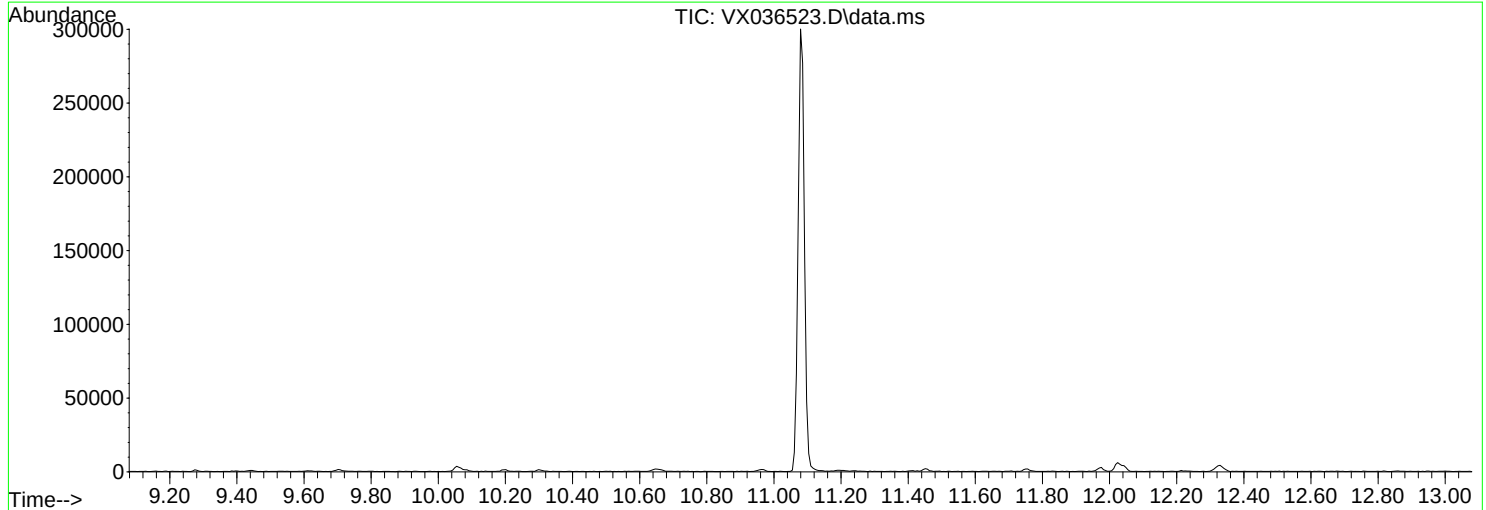

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.2	10522	PASS
75	95	30	60	53.6	27955	PASS
95	95	100	100	100.0	52181	PASS
96	95	5	9	6.9	3585	PASS
173	174	0.00	2	1.0	398	PASS
174	95	50	100	74.8	39011	PASS
175	174	5	9	7.7	3000	PASS
176	174	95	101	94.8	36987	FAIL*
177	176	5	9	6.2	2288	PASS