

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071425\
 Data File : VX046973.D
 Acq On : 14 Jul 2025 15:02
 Operator : JC/MD
 Sample : Q2565-04
 Misc : 1.06g/10mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MOO-25-0196

Quant Time: Jul 15 01:21:24 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X070225W.M
 Quant Title : SW846 8260
 QLast Update : Thu Jul 03 05:51:11 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.556	168	311535	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	535193	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	489066	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	243403	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	216796	52.676	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery = 105.360%			
35) Dibromofluoromethane	5.397	113	168652	46.423	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 92.840%			
50) Toluene-d8	8.647	98	624812	48.746	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery = 97.500%			
62) 4-Bromofluorobenzene	11.079	95	251366	51.600	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery = 103.200%			
Target Compounds						Qvalue
3) Chloromethane	1.307	50	1252	0.385	ug/l #	75
5) Bromomethane	1.611	94	4263	1.872	ug/l	87
10) Methyl Iodide	2.453	142	7920	2.081	ug/l	100
11) Tert butyl alcohol	3.032	59	102	0.378	ug/l #	72
13) Acrolein	2.245	56	25	2.918	ug/l #	63
16) Acetone	2.410	43	7789	6.093	ug/l	93
18) Methyl Acetate	2.721	43	11939	3.543	ug/l #	84
20) Methylene Chloride	2.794	84	5465	1.446	ug/l #	82
31) Cyclohexane	5.556	56	8013	1.362	ug/l #	1
36) 1,1-Dichloropropene	5.556	75	25233	5.148	ug/l #	51
38) Carbon Tetrachloride	5.556	117	32545	6.280	ug/l #	17
39) Methylcyclohexane	7.379	83	1243	0.203	ug/l #	58
43) Isopropyl Acetate	6.367	43	1280	0.200	ug/l #	61
51) 4-Methyl-2-Pentanone	8.586	43	806	0.214	ug/l #	37
52) Toluene	8.720	92	298598	32.502	ug/l	100
53) t-1,3-Dichloropropene	8.714	75	3434	0.694	ug/l #	1
68) m/p-Xylenes	10.305	106	2570	0.377	ug/l	86
76) 1,2,3-Trichloropropane	11.079	75	124948	33.223	ug/l #	36
78) n-propylbenzene	11.305	91	6012	0.291	ug/l	91
79) 2-Chlorotoluene	11.378	91	3901	0.320	ug/l #	41
80) 1,3,5-Trimethylbenzene	11.451	105	11608	0.835	ug/l	96
81) trans-1,4-Dichloro-2-b...	11.079	75	124948	89.153	ug/l #	8
83) tert-Butylbenzene	11.969	119	9436	0.657	ug/l	72
84) 1,2,4-Trimethylbenzene	11.750	105	50409	3.587	ug/l	96
85) sec-Butylbenzene	11.890	105	7059	0.390	ug/l	87
86) p-Isopropyltoluene	11.969	119	9767	0.644	ug/l	91
89) n-Butylbenzene	12.329	91	28725	2.016	ug/l #	49
90) Hexachloroethane	12.530	117	3724	1.386	ug/l #	15
92) 1,2-Dibromo-3-Chloropr...	12.933	75	527	0.640	ug/l #	1
95) Naphthalene	13.774	128	22140	1.601	ug/l #	79
96) 1,2,3-Trichlorobenzene	13.975	180	3564	0.719	ug/l #	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071425\
Data File : VX046973.D
Acq On : 14 Jul 2025 15:02
Operator : JC/MD
Sample : Q2565-04
Misc : 1.06g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MOO-25-0196


Quant Time: Jul 15 01:21:24 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X070225W.M
Quant Title : SW846 8260
QLast Update : Thu Jul 03 05:51:11 2025
Response via : Initial Calibration

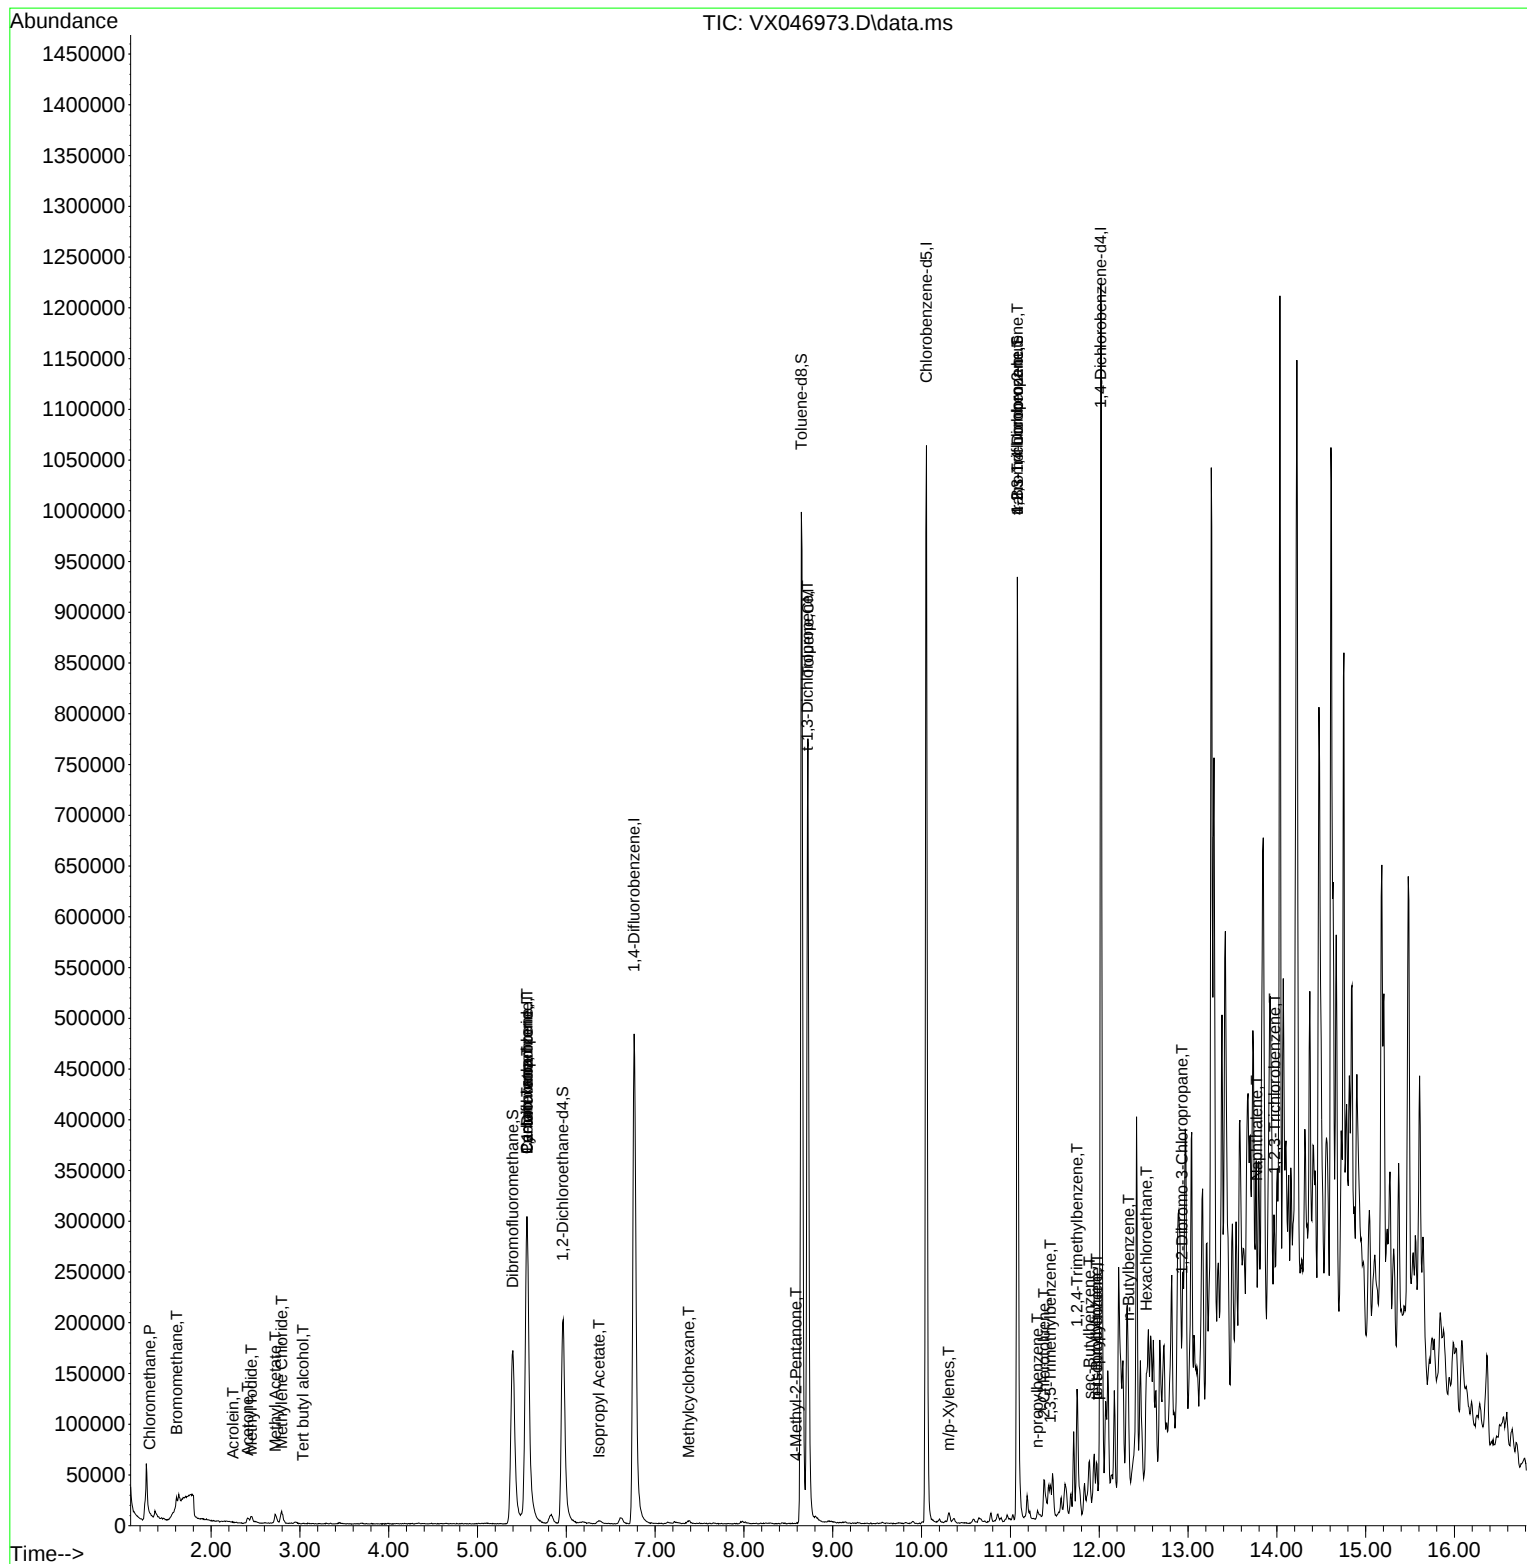






#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.006 min
Lab File: VX046973.D
Acq: 14 Jul 2025 15:02

Instrument :
MSVOA_X
ClientSampleId :
MOO-25-0196







Tgt Ion:168 Resp: 311535
Ion Ratio Lower Upper
168 100
99 58.8 48.8 73.2

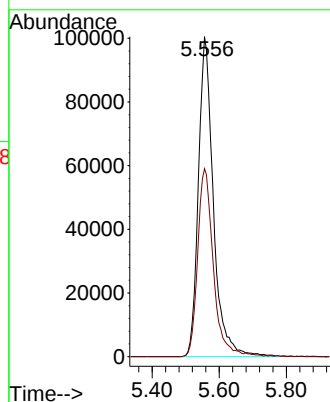

#3
Chloromethane
Concen: 0.385 ug/l
RT: 1.307 min Scan# 36
Delta R.T. -0.000 min
Lab File: VX046973.D
Acq: 14 Jul 2025 15:02

Tgt Ion: 50 Resp: 1252
Ion Ratio Lower Upper
50 100
52 45.1 25.0 37.4#



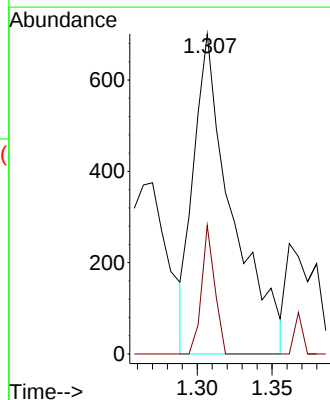
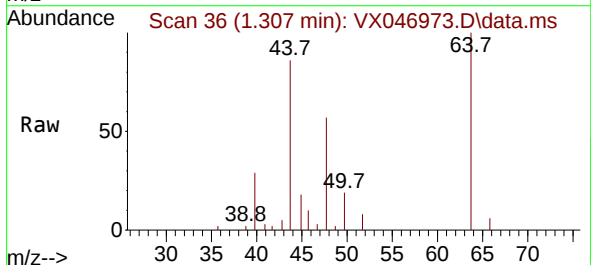


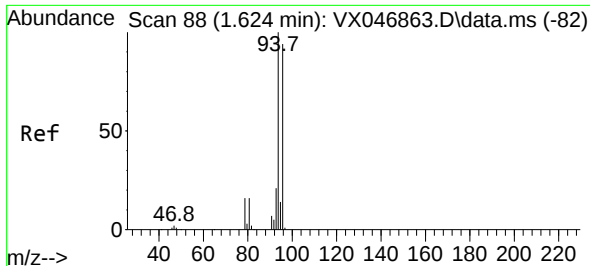

#5
Bromomethane
Concen: 1.872 ug/l
RT: 1.611 min Scan# 80
Delta R.T. -0.012 min
Lab File: VX046973.D
Acq: 14 Jul 2025 15:02




Instrument :
MSVOA_X
ClientSampleId :
MOO-25-0196


Tgt Ion: 94 Resp: 4263
Ion Ratio Lower Upper
94 100
96 81.4 75.5 113.3

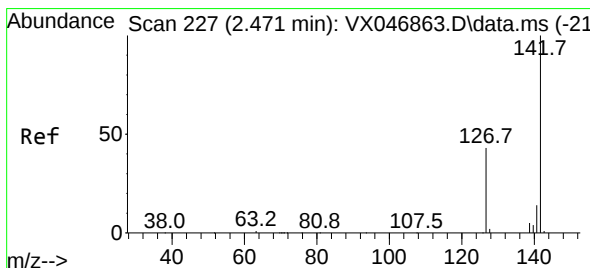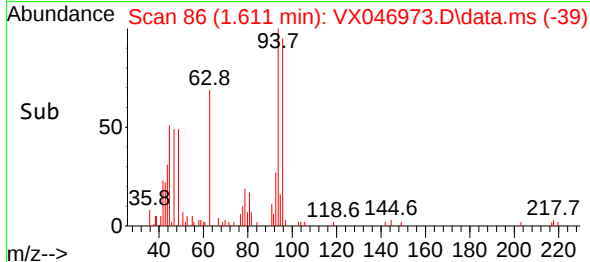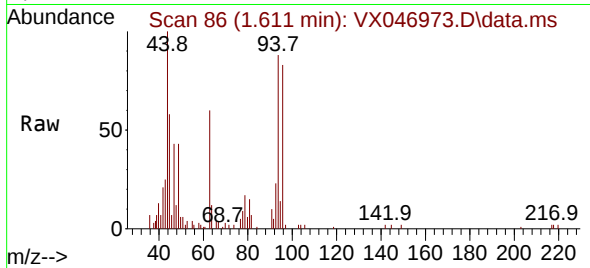

#10
Methyl Iodide
Concen: 2.081 ug/l
RT: 2.453 min Scan# 224
Delta R.T. -0.018 min
Lab File: VX046973.D
Acq: 14 Jul 2025 15:02

Tgt Ion: 142 Resp: 7920
Ion Ratio Lower Upper
142 100
127 43.9 34.9 52.3
141 13.7 11.1 16.7

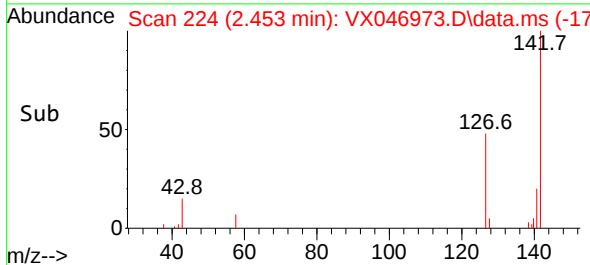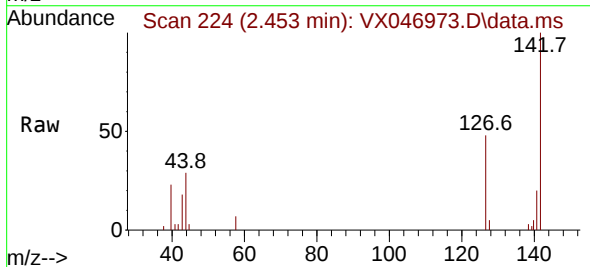

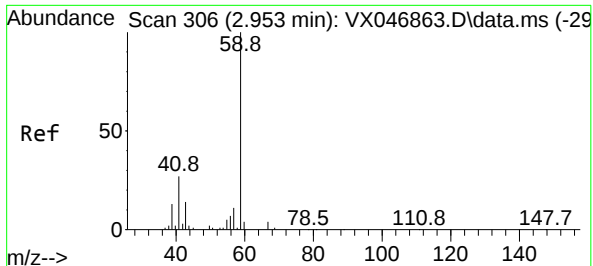

#11

Tert butyl alcohol

Concen: 0.378 ug/l

RT: 3.032 min Scan# 31

Delta R.T. 0.079 min

Lab File: VX046973.D

Acq: 14 Jul 2025 15:02

Instrument :

MSVOA_X

ClientSampleId :





MOO-25-0196

Tgt Ion: 59 Resp: 102

Ion Ratio Lower Upper

59 100

57 0.0 8.5 12.7#

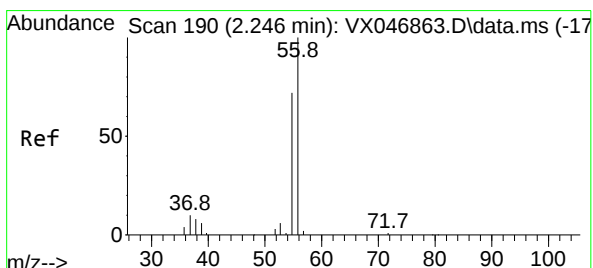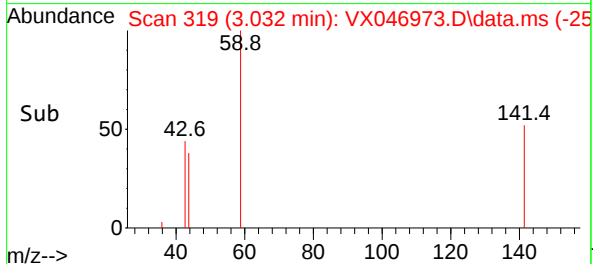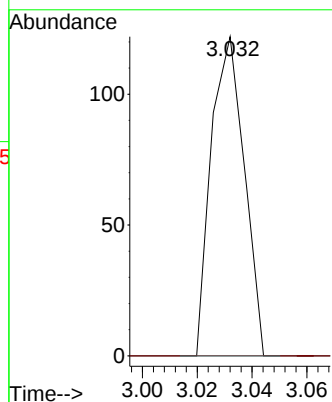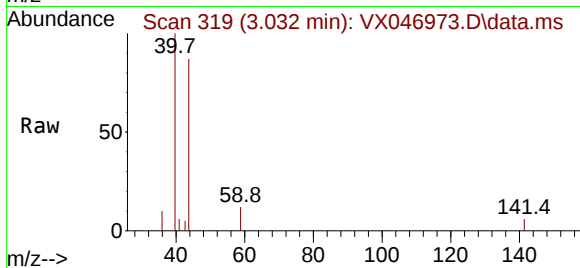

#13

Acrolein

Concen: 2.918 ug/l

RT: 2.245 min Scan# 190

Delta R.T. -0.001 min

Lab File: VX046973.D




Acq: 14 Jul 2025 15:02


Tgt Ion: 56 Resp: 25

Ion Ratio Lower Upper

56 100

55 100.0 55.5 83.3#


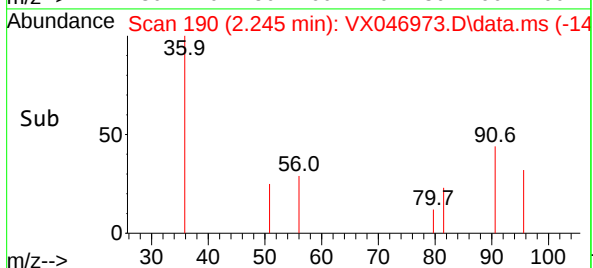

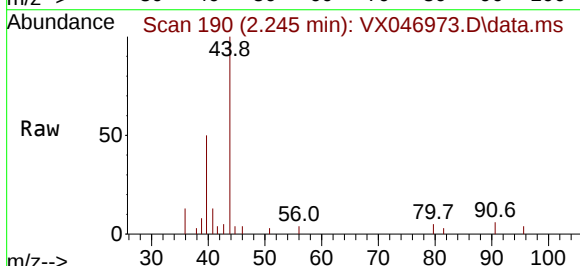




#16
Acetone
Concen: 6.093 ug/l
RT: 2.410 min Scan# 21
Delta R.T. 0.024 min
Lab File: VX046973.D
Acq: 14 Jul 2025 15:02




Instrument :
MSVOA_X
ClientSampleId :
MOO-25-0196


Tgt Ion: 43 Resp: 7789
Ion Ratio Lower Upper
43 100
58 36.1 25.8 38.6

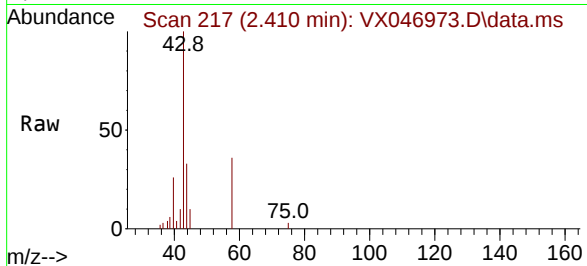

#18
Methyl Acetate
Concen: 3.543 ug/l
RT: 2.721 min Scan# 268
Delta R.T. 0.006 min
Lab File: VX046973.D
Acq: 14 Jul 2025 15:02

Tgt Ion: 43 Resp: 11939
Ion Ratio Lower Upper
43 100
74 15.4 18.3 27.5#




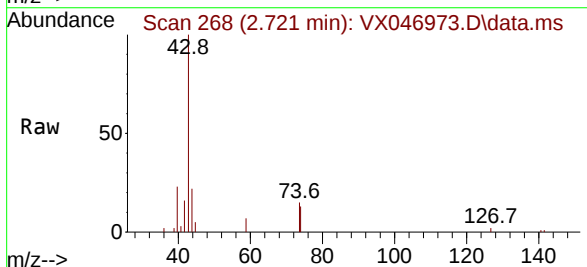




#20
Methylene Chloride
Concen: 1.446 ug/l
RT: 2.794 min Scan# 21
Delta R.T. -0.006 min
Lab File: VX046973.D
Acq: 14 Jul 2025 15:02




Instrument :
MSVOA_X
ClientSampleId :
MOO-25-0196


Tgt Ion:	84	Resp:	5465
Ion	Ratio	Lower	Upper
84	100		
49	156.3	102.8	154.2#
51	44.6	31.1	46.7
86	71.9	50.6	75.8

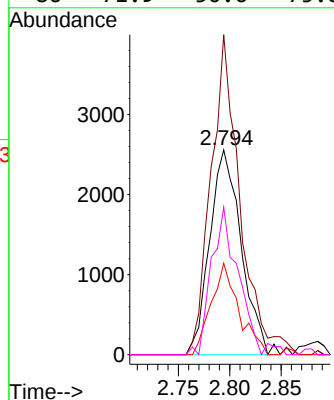

#31
Cyclohexane
Concen: 1.362 ug/l
RT: 5.556 min Scan# 733
Delta R.T. 0.073 min
Lab File: VX046973.D
Acq: 14 Jul 2025 15:02

Tgt Ion:	56	Resp:	8013
Ion	Ratio	Lower	Upper
56	100		
69	172.1	24.0	36.0#
84	144.8	66.5	99.7#


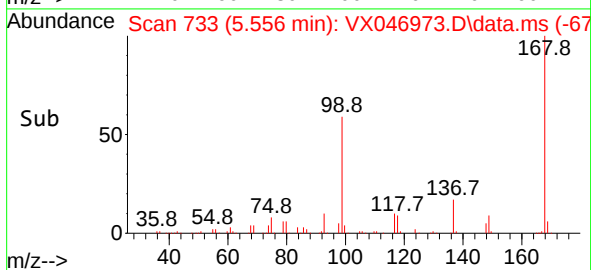
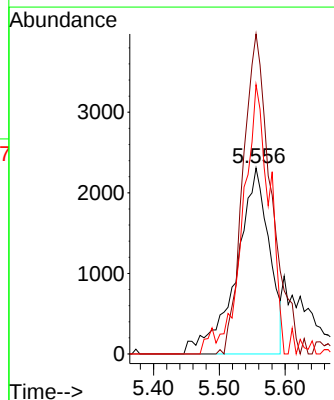





#33
 1,2-Dichloroethane-d4
 Concen: 52.676 ug/l
 RT: 5.958 min Scan# 799
 Delta R.T. -0.000 min
 Lab File: VX046973.D
 Acq: 14 Jul 2025 15:02




Instrument :
 MSVOA_X
 ClientSampleId :
 MOO-25-0196


Tgt Ion: 65 Resp: 216796
 Ion Ratio Lower Upper
 65 100
 67 52.4 0.0 105.2

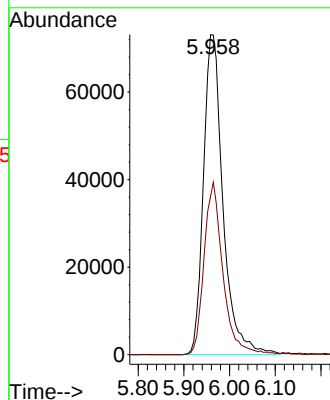

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 6.763 min Scan# 931
 Delta R.T. -0.006 min
 Lab File: VX046973.D
 Acq: 14 Jul 2025 15:02

Tgt Ion: 114 Resp: 535193
 Ion Ratio Lower Upper
 114 100
 63 22.6 0.0 40.4
 88 16.7 0.0 31.0



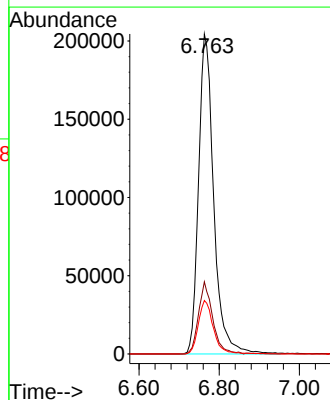





#35
Dibromofluoromethane
Concen: 46.423 ug/l
RT: 5.397 min Scan# 707
Delta R.T. -0.000 min
Lab File: VX046973.D
Acq: 14 Jul 2025 15:02




Instrument :
MSVOA_X
ClientSampleId :
MOO-25-0196


Tgt Ion:113 Resp: 168652
Ion Ratio Lower Upper
113 100
111 102.9 81.2 121.8
192 19.2 15.3 22.9

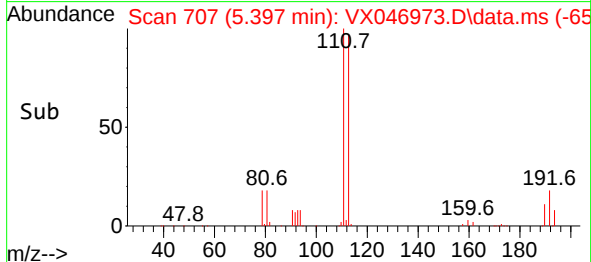

#36
1,1-Dichloropropene
Concen: 5.148 ug/l
RT: 5.556 min Scan# 733
Delta R.T. -0.146 min
Lab File: VX046973.D
Acq: 14 Jul 2025 15:02


Tgt Ion: 75 Resp: 25233
Ion Ratio Lower Upper
75 100
110 9.8 17.3 51.9#
77 0.0 24.2 36.4#

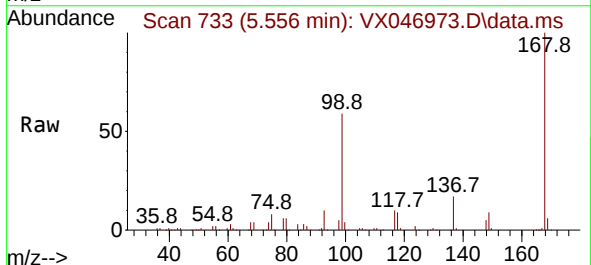



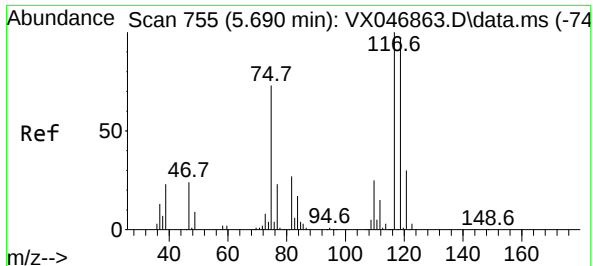


#38
Carbon Tetrachloride
Concen: 6.280 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.134 min
Lab File: VX046973.D
Acq: 14 Jul 2025 15:02

Instrument :
MSVOA_X
ClientSampleId :
MOO-25-0196



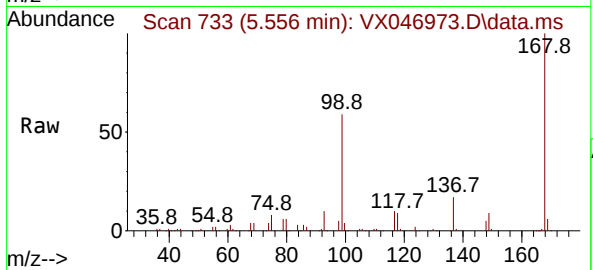



Tgt Ion:117 Resp: 32545
Ion Ratio Lower Upper
117 100
119 6.0 76.6 114.8#
121 0.0 24.1 36.1#

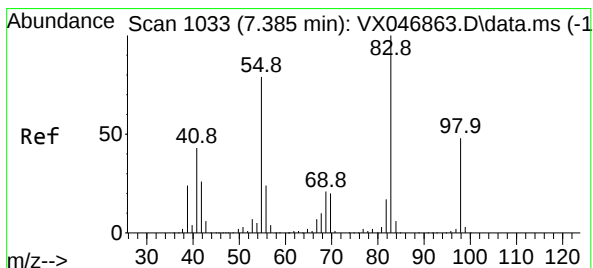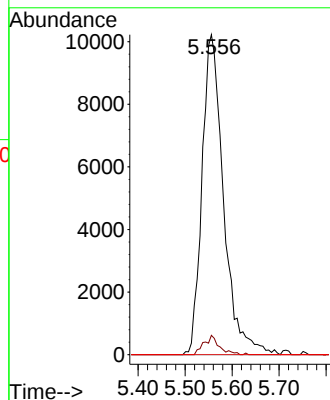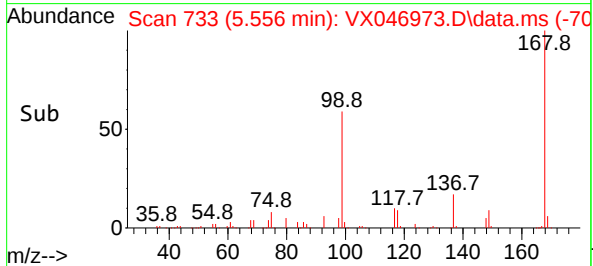

#39
Methylcyclohexane
Concen: 0.203 ug/l
RT: 7.379 min Scan# 1032
Delta R.T. -0.006 min
Lab File: VX046973.D
Acq: 14 Jul 2025 15:02

Tgt Ion: 83 Resp: 1243
Ion Ratio Lower Upper
83 100
55 135.2 63.0 94.4#
98 45.4 38.5 57.7


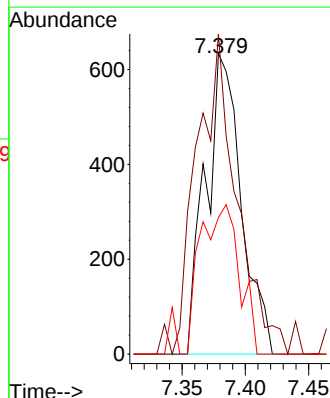
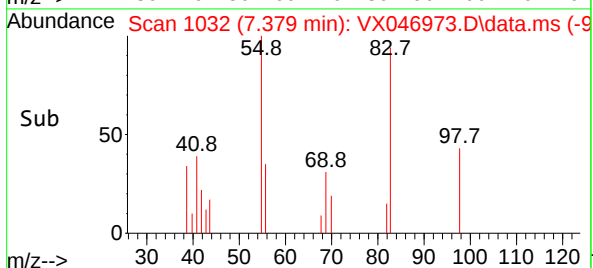
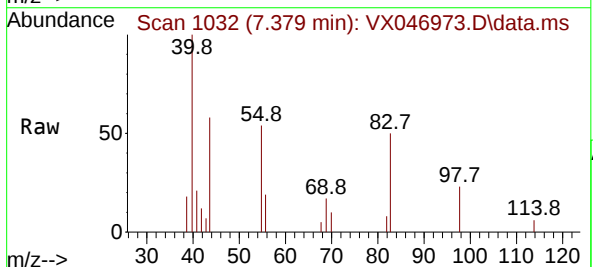




#43
Isopropyl Acetate
Concen: 0.200 ug/l
RT: 6.367 min Scan# 866
Delta R.T. 0.024 min
Lab File: VX046973.D
Acq: 14 Jul 2025 15:02




Instrument :
MSVOA_X
ClientSampleId :
MOO-25-0196


Tgt Ion: 43 Resp: 1280
Ion Ratio Lower Upper
43 100
61 0.0 15.7 23.5#
87 0.0 10.1 15.1#

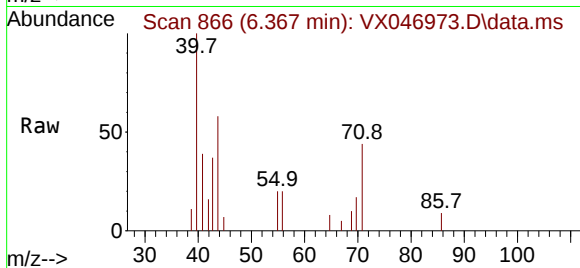

#50
Toluene-d8
Concen: 48.746 ug/l
RT: 8.647 min Scan# 1240
Delta R.T. -0.000 min
Lab File: VX046973.D
Acq: 14 Jul 2025 15:02

Tgt Ion: 98 Resp: 624812
Ion Ratio Lower Upper
98 100
100 66.6 53.0 79.6

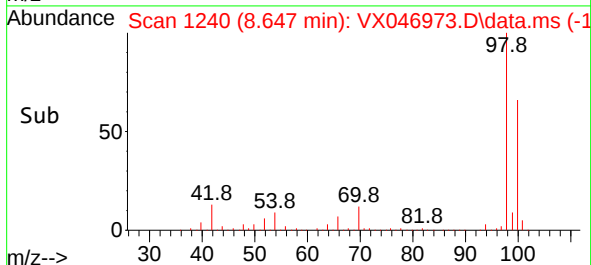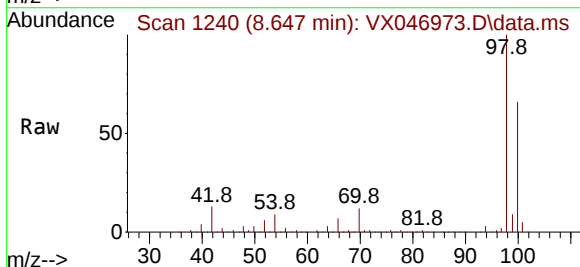

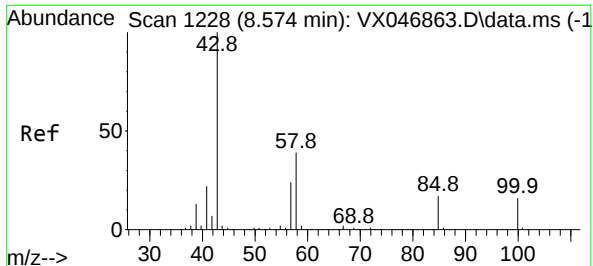

#51

4-Methyl-2-Pentanone

Concen: 0.214 ug/l

RT: 8.586 min Scan# 11

Delta R.T. 0.012 min

Lab File: VX046973.D

Acq: 14 Jul 2025 15:02

Instrument :

MSVOA_X

ClientSampleId :





MOO-25-0196

Tgt Ion: 43 Resp: 806

Ion Ratio Lower Upper

43 100

58 0.0 30.4 45.6#

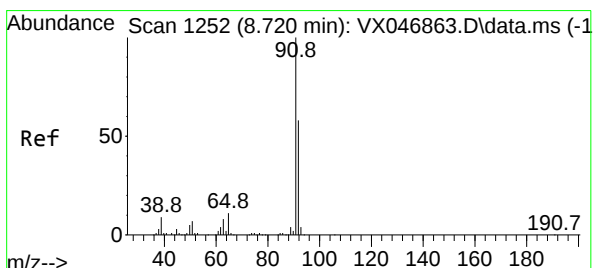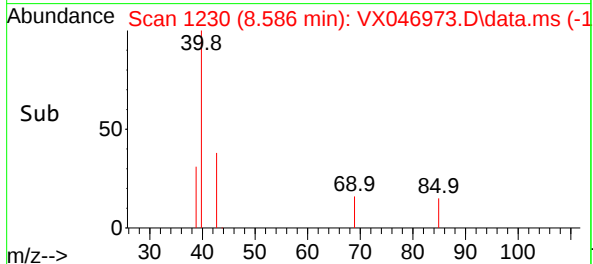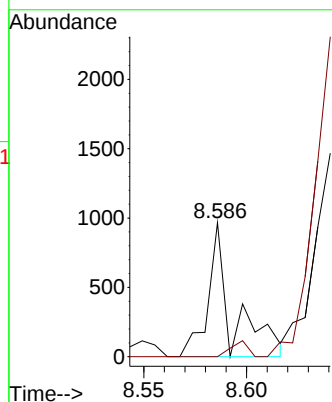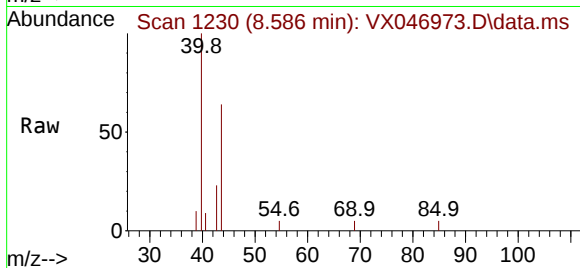

#52

Toluene

Concen: 32.502 ug/l

RT: 8.720 min Scan# 1252

Delta R.T. -0.000 min

Lab File: VX046973.D




Acq: 14 Jul 2025 15:02


Tgt Ion: 92 Resp: 298598

Ion Ratio Lower Upper

92 100

91 172.7 137.9 206.9

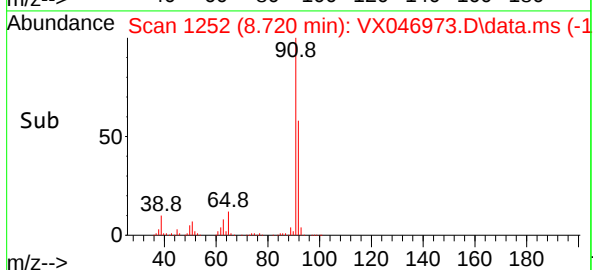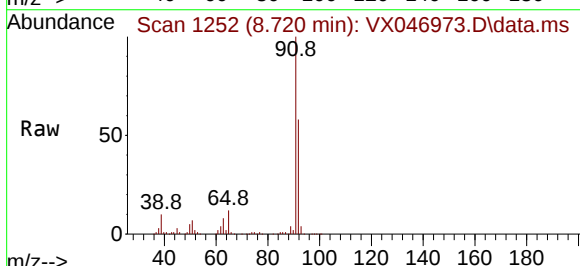

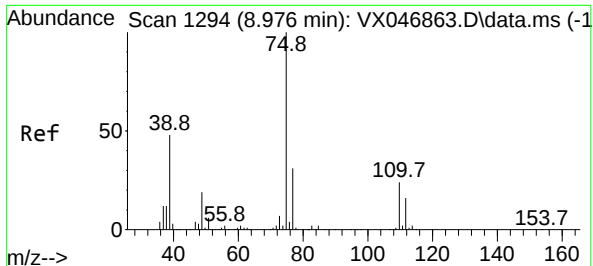

#53

t-1,3-Dichloropropene

Concen: 0.694 ug/l

RT: 8.714 min Scan# 1

Delta R.T. -0.262 min

Lab File: VX046973.D

Acq: 14 Jul 2025 15:02

Instrument :

MSVOA_X

ClientSampleId :





MOO-25-0196

Tgt Ion: 75 Resp: 3434

Ion Ratio Lower Upper

75 100

77 164.3 25.0 37.6#

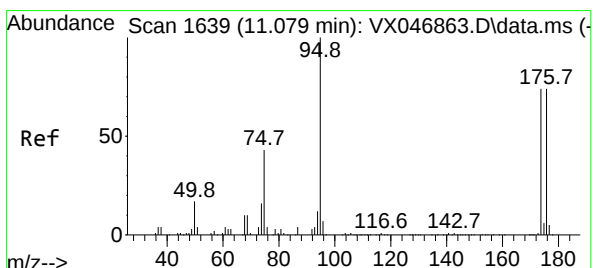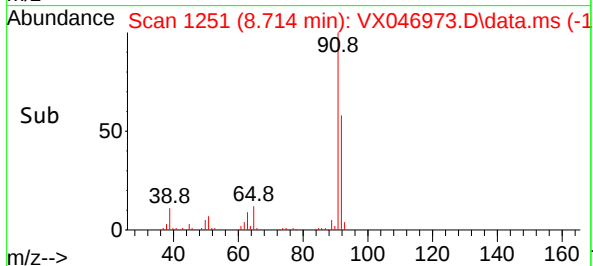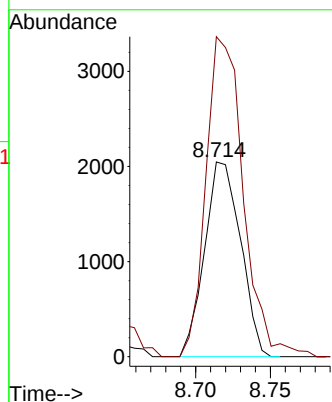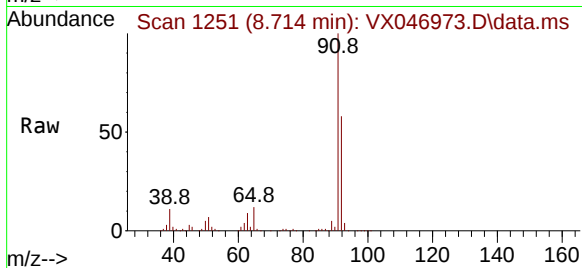

#62

4-Bromofluorobenzene

Concen: 51.600 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. -0.000 min

Lab File: VX046973.D

Acq: 14 Jul 2025 15:02




Tgt Ion: 95 Resp: 251366


Ion Ratio Lower Upper

95 100

174 74.0 0.0 152.0

176 70.8 0.0 145.2


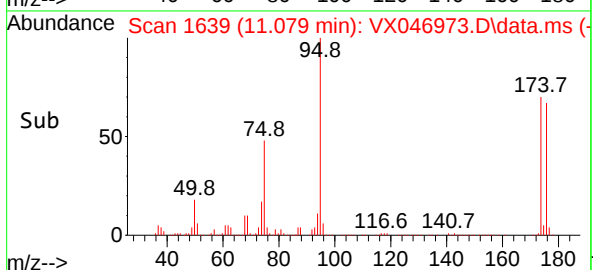

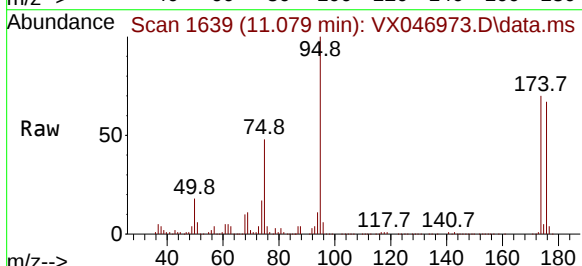




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX046973.D
Acq: 14 Jul 2025 15:02




Instrument :
MSVOA_X
ClientSampleId :
MOO-25-0196


Tgt Ion:117 Resp: 489066
Ion Ratio Lower Upper
117 100
82 55.7 43.3 64.9
119 32.2 26.4 39.6

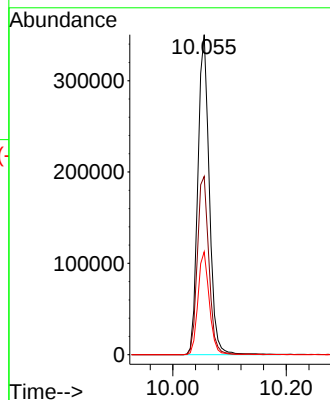

#68
m/p-Xylenes
Concen: 0.377 ug/l
RT: 10.305 min Scan# 1512
Delta R.T. 0.006 min
Lab File: VX046973.D
Acq: 14 Jul 2025 15:02

Tgt Ion:106 Resp: 2570
Ion Ratio Lower Upper
106 100
91 228.0 164.6 246.8


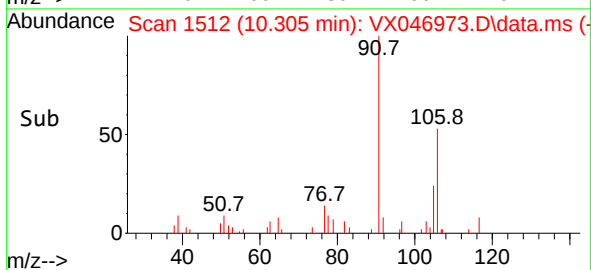
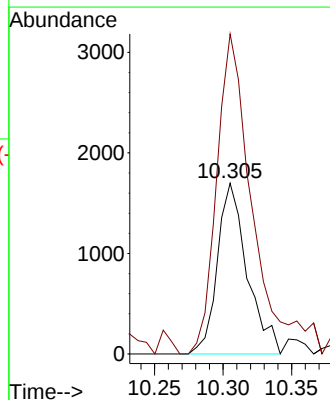





#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 12.018 min Scan# 1
 Delta R.T. -0.000 min
 Lab File: VX046973.D
 Acq: 14 Jul 2025 15:02




Instrument :
 MSVOA_X
 ClientSampleId :
 MOO-25-0196


Tgt Ion:152 Resp: 243403
 Ion Ratio Lower Upper
 152 100
 115 62.3 42.4 127.1
 150 157.9 0.0 349.2

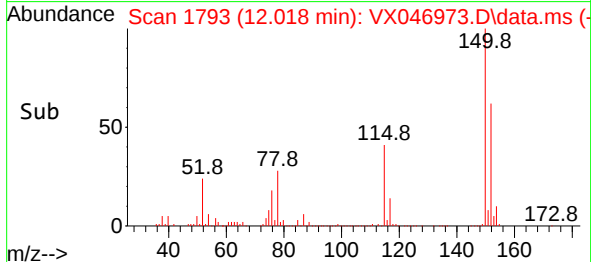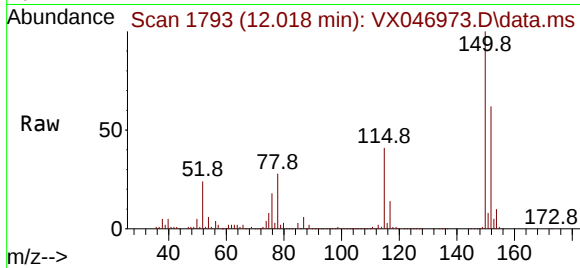

#76
 1,2,3-Trichloropropane
 Concen: 33.223 ug/l
 RT: 11.079 min Scan# 1639
 Delta R.T. -0.159 min
 Lab File: VX046973.D
 Acq: 14 Jul 2025 15:02

Tgt Ion: 75 Resp: 124948
 Ion Ratio Lower Upper
 75 100
 77 1.4 20.6 61.8#




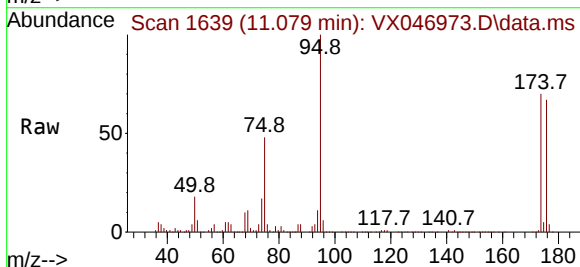




#78
n-propylbenzene
Concen: 0.291 ug/l
RT: 11.305 min Scan# 1676
Delta R.T. 0.006 min
Lab File: VX046973.D
Acq: 14 Jul 2025 15:02




Instrument :
MSVOA_X
ClientSampleId :
MOO-25-0196


Tgt Ion: 91 Resp: 6012
Ion Ratio Lower Upper
91 100
120 18.0 11.2 33.5

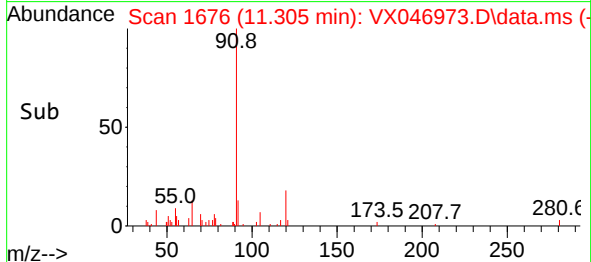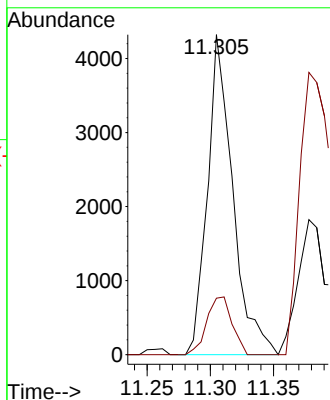

#79
2-Chlorotoluene
Concen: 0.320 ug/l
RT: 11.378 min Scan# 1688
Delta R.T. 0.018 min
Lab File: VX046973.D
Acq: 14 Jul 2025 15:02

Tgt Ion: 91 Resp: 3901
Ion Ratio Lower Upper
91 100
126 0.0 16.6 49.8#


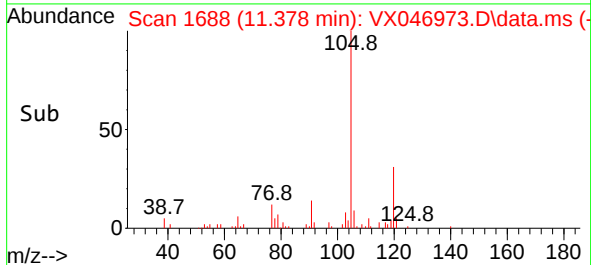
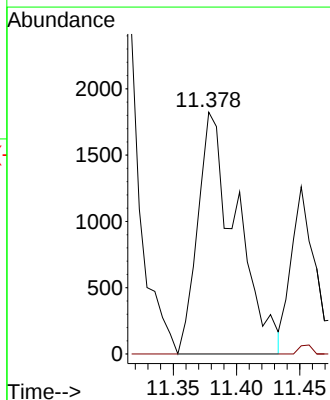





#80
1,3,5-Trimethylbenzene
Concen: 0.835 ug/l
RT: 11.451 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX046973.D
Acq: 14 Jul 2025 15:02




Instrument :
MSVOA_X
ClientSampleId :
MOO-25-0196


Tgt Ion:105 Resp: 11608
Ion Ratio Lower Upper
105 100
120 45.5 24.1 72.4

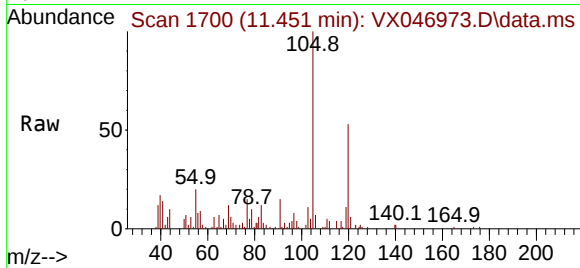

#81
trans-1,4-Dichloro-2-butene
Concen: 89.153 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.061 min
Lab File: VX046973.D
Acq: 14 Jul 2025 15:02

Tgt Ion: 75 Resp: 124948
Ion Ratio Lower Upper
75 100
53 0.3 83.7 125.5#
89 0.0 38.2 57.2#

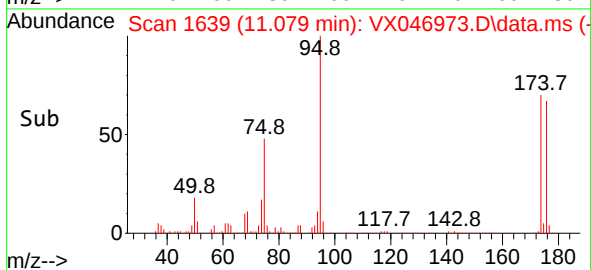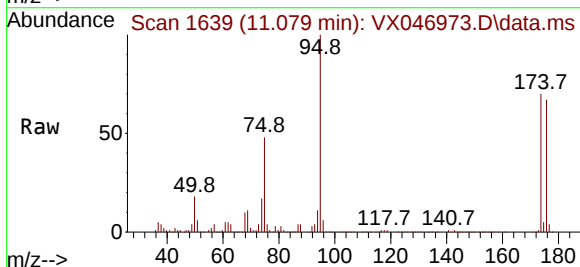



#83

tert-Butylbenzene

Concen: 0.657 ug/l

RT: 11.969 min Scan# 1785

Delta R.T. 0.256 min

Lab File: VX046973.D

Acq: 14 Jul 2025 15:02

Instrument :

MSVOA_X

ClientSampleId :

MOO-25-0196





Tgt Ion:119 Resp: 9436

Ion Ratio Lower Upper

119 100

91 32.1 28.7 86.3

134 29.3 11.4 34.2

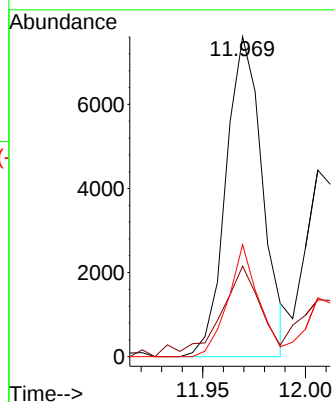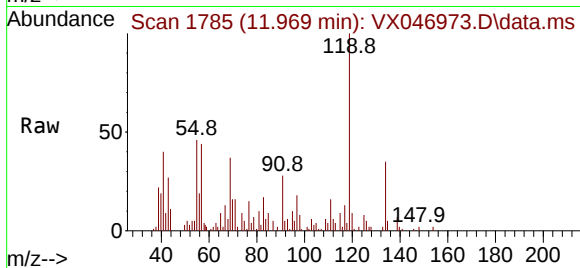

#84

1,2,4-Trimethylbenzene

Concen: 3.587 ug/l

RT: 11.750 min Scan# 1749

Delta R.T. -0.000 min

Lab File: VX046973.D




Acq: 14 Jul 2025 15:02


Tgt Ion:105 Resp: 50409

Ion Ratio Lower Upper

105 100

120 43.8 23.3 69.8



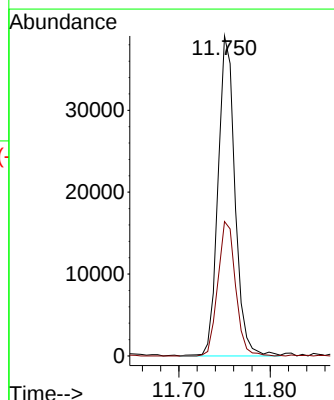
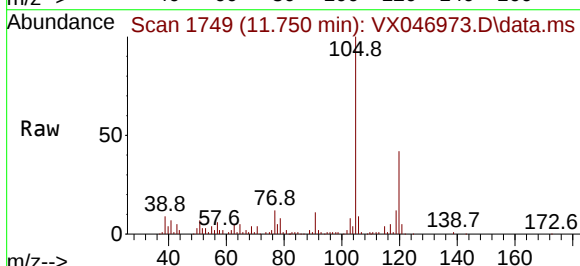




#85
 sec-Butylbenzene
 Concen: 0.390 ug/l
 RT: 11.890 min Scan# 1771
 Delta R.T. 0.006 min
 Lab File: VX046973.D
 Acq: 14 Jul 2025 15:02




Instrument :
 MSVOA_X
 ClientSampleId :
 MOO-25-0196


Tgt Ion:105 Resp: 7059
 Ion Ratio Lower Upper
 105 100
 134 25.7 9.9 29.7

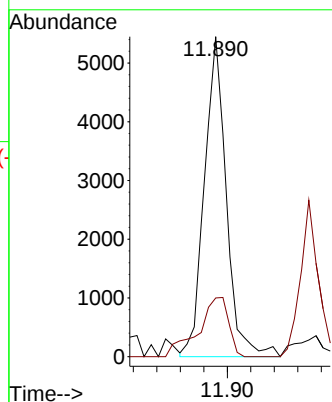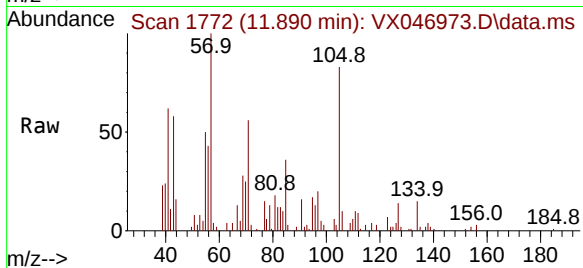

#86
 p-Isopropyltoluene
 Concen: 0.644 ug/l
 RT: 11.969 min Scan# 1785
 Delta R.T. -0.037 min
 Lab File: VX046973.D
 Acq: 14 Jul 2025 15:02

Tgt Ion:119 Resp: 9767
 Ion Ratio Lower Upper
 119 100
 134 28.3 13.0 39.0
 91 31.0 12.0 36.1



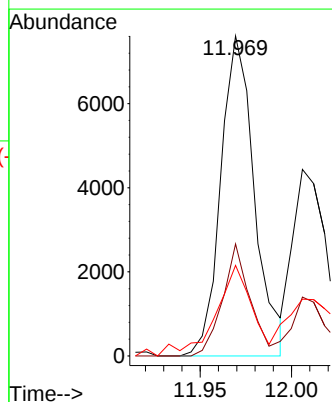
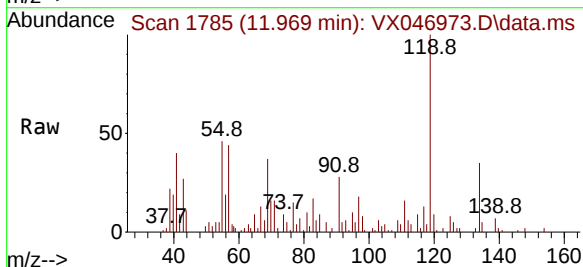




#89
n-Butylbenzene
Concen: 2.016 ug/l
RT: 12.329 min Scan# 1844
Delta R.T. -0.000 min
Lab File: VX046973.D
Acq: 14 Jul 2025 15:02




Instrument :
MSVOA_X
ClientSampleId :
MOO-25-0196


Tgt Ion: 91 Resp: 28725
Ion Ratio Lower Upper
91 100
92 36.5 27.0 81.0
134 79.2 12.8 38.4#

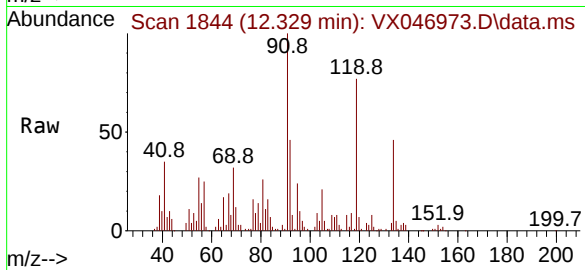

#90
Hexachloroethane
Concen: 1.386 ug/l
RT: 12.530 min Scan# 1877
Delta R.T. -0.006 min
Lab File: VX046973.D
Acq: 14 Jul 2025 15:02

Tgt Ion: 117 Resp: 3724
Ion Ratio Lower Upper
117 100
201 1.0 35.8 107.4#


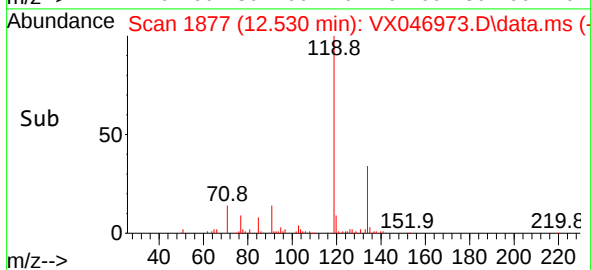

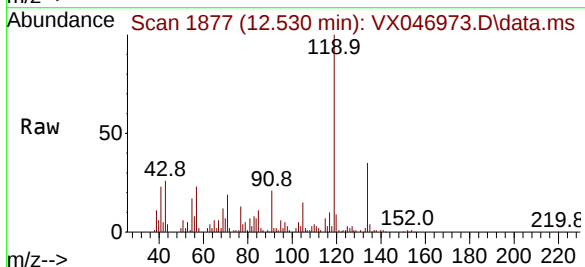




#92
1,2-Dibromo-3-Chloropropane
Concen: 0.640 ug/l
RT: 12.933 min Scan# 1944
Delta R.T. -0.006 min
Lab File: VX046973.D
Acq: 14 Jul 2025 15:02




Instrument :
MSVOA_X
ClientSampleId :
MOO-25-0196


Tgt Ion: 75 Resp: 527
Ion Ratio Lower Upper
75 100
155 0.0 43.1 129.4#
157 0.0 56.5 169.5#

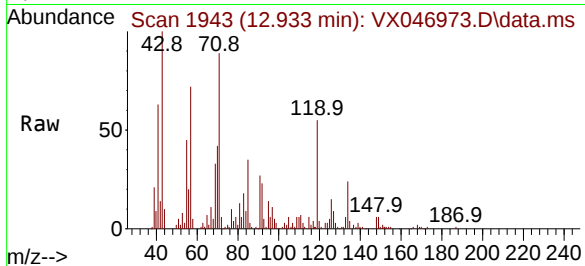

#95
Naphthalene
Concen: 1.601 ug/l
RT: 13.774 min Scan# 2081
Delta R.T. -0.000 min
Lab File: VX046973.D
Acq: 14 Jul 2025 15:02


Tgt Ion: 128 Resp: 22140
Ion Ratio Lower Upper
128 100
127 22.7 10.2 15.4#
129 17.2 8.6 13.0#

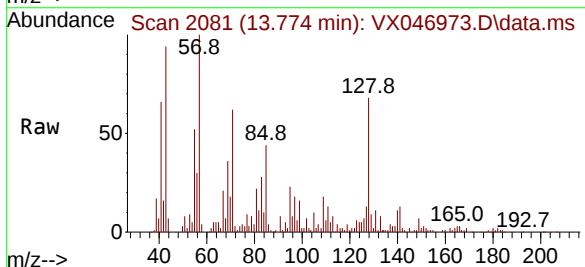



#96
 1,2,3-Trichlorobenzene
 Concen: 0.719 ug/l
 RT: 13.975 min Scan# 21
 Delta R.T. 0.018 min
 Lab File: VX046973.D
 Acq: 14 Jul 2025 15:02

Instrument :
 MSVOA_X
 ClientSampleId :
 MOO-25-0196



Tgt Ion:180 Resp: 3564
 Ion Ratio Lower Upper
 180 100
 182 7.2 46.7 140.1#
 145 387.2 16.8 50.3#

