

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX071519\
 Data File : VX010876.D
 Acq On : 15 Jul 2019 11:59
 Operator : JC/SP
 Sample : K3779-01
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 390711759.3-VOA

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X061919W.M

Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.209	6	9	15	rVB	22881	30960	2.69%	0.340%
2	1.294	19	23	27	rVB3	11226	14929	1.29%	0.164%
3	1.392	35	39	47	rVB	18269	21925	1.90%	0.241%
4	1.654	79	82	88	rBV	16550	29897	2.59%	0.328%
5	2.190	164	170	179	rBV2	29896	52167	4.52%	0.573%
6	2.452	206	213	218	rBV2	31003	58244	5.05%	0.639%
7	2.495	218	220	227	rBV	14525	29958	2.60%	0.329%
8	3.038	299	309	319	rBV	102694	234274	20.32%	2.571%
9	3.196	328	335	342	rVB	4311	11645	1.01%	0.128%
10	4.690	569	580	596	rBV	145105	475756	41.26%	5.221%
11	5.129	642	652	670	rBV2	166662	505535	43.84%	5.548%
12	5.501	699	713	727	rBV	134964	392969	34.08%	4.313%
13	5.659	727	739	756	rVB	227707	647024	56.12%	7.101%
14	6.061	796	805	815	rBV2	132890	345673	29.98%	3.794%
15	6.141	815	818	827	rVB3	9263	21509	1.87%	0.236%
16	6.342	840	851	861	rVB6	6177	20208	1.75%	0.222%
17	6.446	861	868	878	rBV10	5007	15067	1.31%	0.165%
18	6.860	924	936	950	rBV	339437	809777	70.23%	8.887%
19	7.738	1074	1080	1088	rBV	14806	30334	2.63%	0.333%
20	7.976	1112	1119	1125	rBV3	8498	16584	1.44%	0.182%
21	8.616	1220	1224	1227	rBV2	8299	13046	1.13%	0.143%
22	8.713	1233	1240	1247	rBV	726400	1117040	96.88%	12.259%
23	8.781	1247	1251	1260	rVB3	14424	27503	2.39%	0.302%
24	8.872	1260	1266	1271	rBV	10062	17165	1.49%	0.188%
25	9.439	1351	1359	1364	rBV	14497	25636	2.22%	0.281%
26	9.549	1373	1377	1382	rBV2	18946	28736	2.49%	0.315%
27	9.616	1382	1388	1395	rVB6	6191	13143	1.14%	0.144%
28	10.110	1459	1469	1482	rBV2	739934	1153031	100.00%	12.654%
29	10.360	1504	1510	1517	rVB	64960	96567	8.38%	1.060%
30	10.695	1561	1565	1573	rVB	64621	87677	7.60%	0.962%
31	11.012	1612	1617	1622	rVB	13456	19663	1.71%	0.216%
32	11.134	1632	1637	1643	rBV	631975	797010	69.12%	8.747%
33	11.231	1649	1653	1658	rVB5	9957	17064	1.48%	0.187%
34	11.426	1680	1685	1688	rBV3	11827	22747	1.97%	0.250%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX071519\
 Data File : VX010876.D
 Acq On : 15 Jul 2019 11:59
 Operator : JC/SP
 Sample : K3779-01
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 390711759.3-VOA

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X061919W.M
 Title : SW846 8260

35	11.512	1694	1699	1703	rVB2	8759	13575	1.18%	0.149%
36	11.664	1720	1724	1734	rVB	25395	36850	3.20%	0.404%
37	11.804	1738	1747	1752	rBV	31567	43441	3.77%	0.477%
38	11.938	1765	1769	1777	rVB4	18059	24696	2.14%	0.271%
39	12.018	1777	1782	1785	rBV7	7001	12172	1.06%	0.134%
40	12.079	1785	1792	1799	rVV2	750216	1114352	96.65%	12.230%
41	12.140	1799	1802	1807	rVB	20164	24973	2.17%	0.274%
42	12.298	1823	1828	1832	rBV	54822	73028	6.33%	0.801%
43	12.390	1837	1843	1851	rVB6	12448	28145	2.44%	0.309%
44	12.469	1851	1856	1861	rBV3	12094	23284	2.02%	0.256%
45	12.585	1870	1875	1885	rVB7	6236	17387	1.51%	0.191%
46	12.664	1885	1888	1892	rVB	13504	16417	1.42%	0.180%
47	12.725	1892	1898	1900	rBV6	7936	12965	1.12%	0.142%
48	12.963	1933	1937	1941	rVV2	24532	39812	3.45%	0.437%
49	13.018	1941	1946	1949	rVB6	13844	21930	1.90%	0.241%
50	13.341	1994	1999	2004	rBV3	19449	28566	2.48%	0.314%
51	13.481	2017	2022	2025	rBV2	16581	20750	1.80%	0.228%
52	13.530	2025	2030	2033	rVV	28410	42020	3.64%	0.461%
53	13.566	2033	2036	2044	rVB	37003	50376	4.37%	0.553%
54	13.646	2044	2049	2053	rBV7	8975	13375	1.16%	0.147%
55	13.828	2074	2079	2085	rVB	103391	135181	11.72%	1.484%
56	13.926	2088	2095	2100	rVB	9718	20196	1.75%	0.222%
57	13.987	2100	2105	2114	rBV	9930	26171	2.27%	0.287%
58	14.694	2218	2221	2223	rBV2	12636	16926	1.47%	0.186%
59	14.725	2223	2226	2233	rVB4	15126	21419	1.86%	0.235%
60	14.834	2240	2244	2249	rVB2	13691	20162	1.75%	0.221%
61	16.413	2495	2503	2511	rBV4	6196	13155	1.14%	0.144%


Sum of corrected areas: 9111787

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX071519\
Data File : VX010876.D
Acq On : 15 Jul 2019 11:59
Operator : JC/SP
Sample : K3779-01
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
390711759.3-VOA

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X061919W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

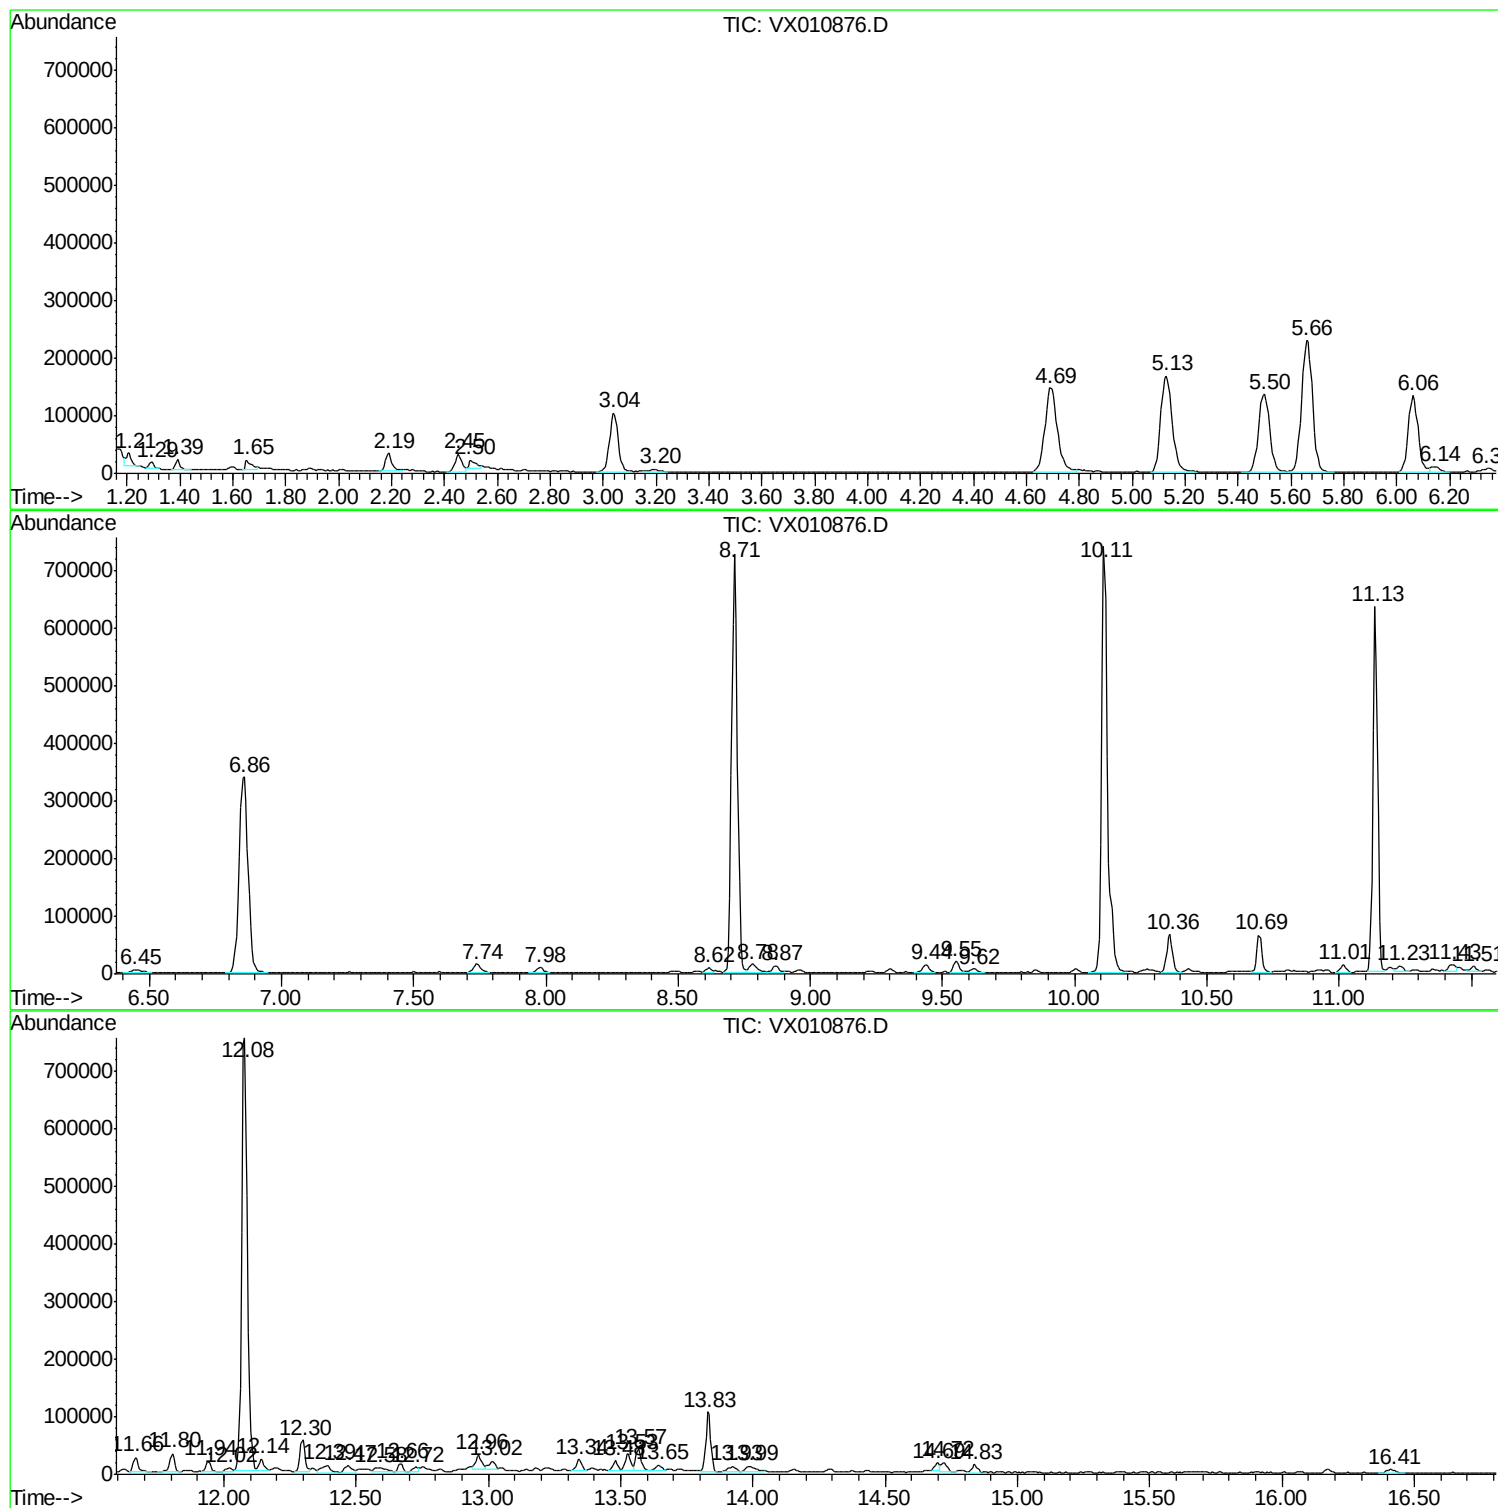

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX071519\
Data File : VX010876.D
Acq On : 15 Jul 2019 11:59
Operator : JC/SP
Sample : K3779-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
390711759.3-VOA

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X061919W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX071519\
Data File : VX010876.D
Acq On : 15 Jul 2019 11:59
Operator : JC/SP
Sample : K3779-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
390711759.3-VOA

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X061919W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc