

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071521\
 Data File : VX023311.D
 Acq On : 15 Jul 2021 19:57
 Operator : JC/MD
 Sample : M3061-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Jul 16 03:55:27 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X070221W.M
 Quant Title : SW846 8260
 QLast Update : Fri Jul 02 14:29:42 2021
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.562	168	238029	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.769	114	387310	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.061	117	360773	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	159739	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.964	65	160716	50.238	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	= 100.480%	
35) Dibromofluoromethane	5.397	113	125805	50.300	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 100.600%	
50) Toluene-d8	8.653	98	467812	50.143	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	= 100.280%	
62) 4-Bromofluorobenzene	11.085	95	179547	49.850	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	= 99.700%	
Target Compounds						
					Qvalue	
3) Chloromethane	1.294	50	458	0.215	ug/l #	73
5) Bromomethane	1.611	94	559	Below Cal	#	45
11) Tert butyl alcohol	2.983	59	2860	4.250	ug/l #	73
12) 1,1-Dichloroethene	2.318	96	657	0.310	ug/l #	87
13) Acrolein	2.239	56	256	0.571	ug/l #	14
14) Allyl chloride	2.648	41	780	0.212	ug/l #	49
15) Acrylonitrile	3.123	53	5272	4.029	ug/l #	34
16) Acetone	2.386	43	37810	29.874	ug/l	90
17) Carbon Disulfide	2.520	76	4612	1.031	ug/l #	90
18) Methyl Acetate	2.715	43	1120	0.365	ug/l	92
19) Methyl tert-butyl Ether	3.123	73	281988	35.534	ug/l #	82
20) Methylene Chloride	2.788	84	694	0.255	ug/l #	75
23) Vinyl Acetate	3.861	43	9861	1.499	ug/l #	68
25) 2-Butanone	4.580	43	19043	9.978	ug/l	95
27) cis-1,2-Dichloroethene	4.513	96	858	0.309	ug/l	90
29) Tetrahydrofuran	5.031	42	1065	0.868	ug/l #	37
31) Cyclohexane	5.483	56	4558	1.190	ug/l #	89
36) 1,1-Dichloropropene	5.556	75	17952	5.199	ug/l #	50
37) Ethyl Acetate	4.580	43	19043	5.056	ug/l #	64
38) Carbon Tetrachloride	5.562	117	25107	6.966	ug/l #	15
43) Isopropyl Acetate	6.360	43	1489	0.238	ug/l #	57
44) Trichloroethene	7.129	130	17664	6.211	ug/l	99
51) 4-Methyl-2-Pentanone	8.586	43	2539	0.654	ug/l	99
55) 1,1,2-Trichloroethane	9.281	97	14864	5.456	ug/l #	15
58) 2-Chloroethyl Vinyl ether	8.409	63	101	4.733	ug/l #	45
59) 2-Hexanone	9.433	43	2767	0.929	ug/l	83
60) Dibromochloromethane	9.281	129	1600116	496.371	ug/l #	11
64) Tetrachloroethene	9.281	164	1631859	567.110	ug/l	96
74) N-amyl acetate	10.860	43	1287	0.270	ug/l #	59
76) 1,2,3-Trichloropropane	11.085	75	92140	28.664	ug/l #	38
81) trans-1,4-Dichloro-2-b...	11.085	75	92140	77.176	ug/l #	12
84) 1,2,4-Trimethylbenzene	11.756	105	2213	0.231	ug/l #	54
90) Hexachloroethane	12.652	117	61	3.029	ug/l #	9
95) Naphthalene	13.780	128	1987	1.438	ug/l #	93

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071521\
Data File : VX023311.D
Acq On : 15 Jul 2021 19:57
Operator : JC/MD
Sample : M3061-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Jul 16 03:55:27 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X070221W.M
Quant Title : SW846 8260
QLast Update : Fri Jul 02 14:29:42 2021
Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


(#)=qualifier out of range (m)=manual integration (+)=signals summed						

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071521\
Data File : VX023311.D
Acq On : 15 Jul 2021 19:57
Operator : JC/MD
Sample : M3061-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Jul 16 03:55:27 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X070221W.M
Quant Title : SW846 8260
QLast Update : Fri Jul 02 14:29:42 2021
Response via : Initial Calibration




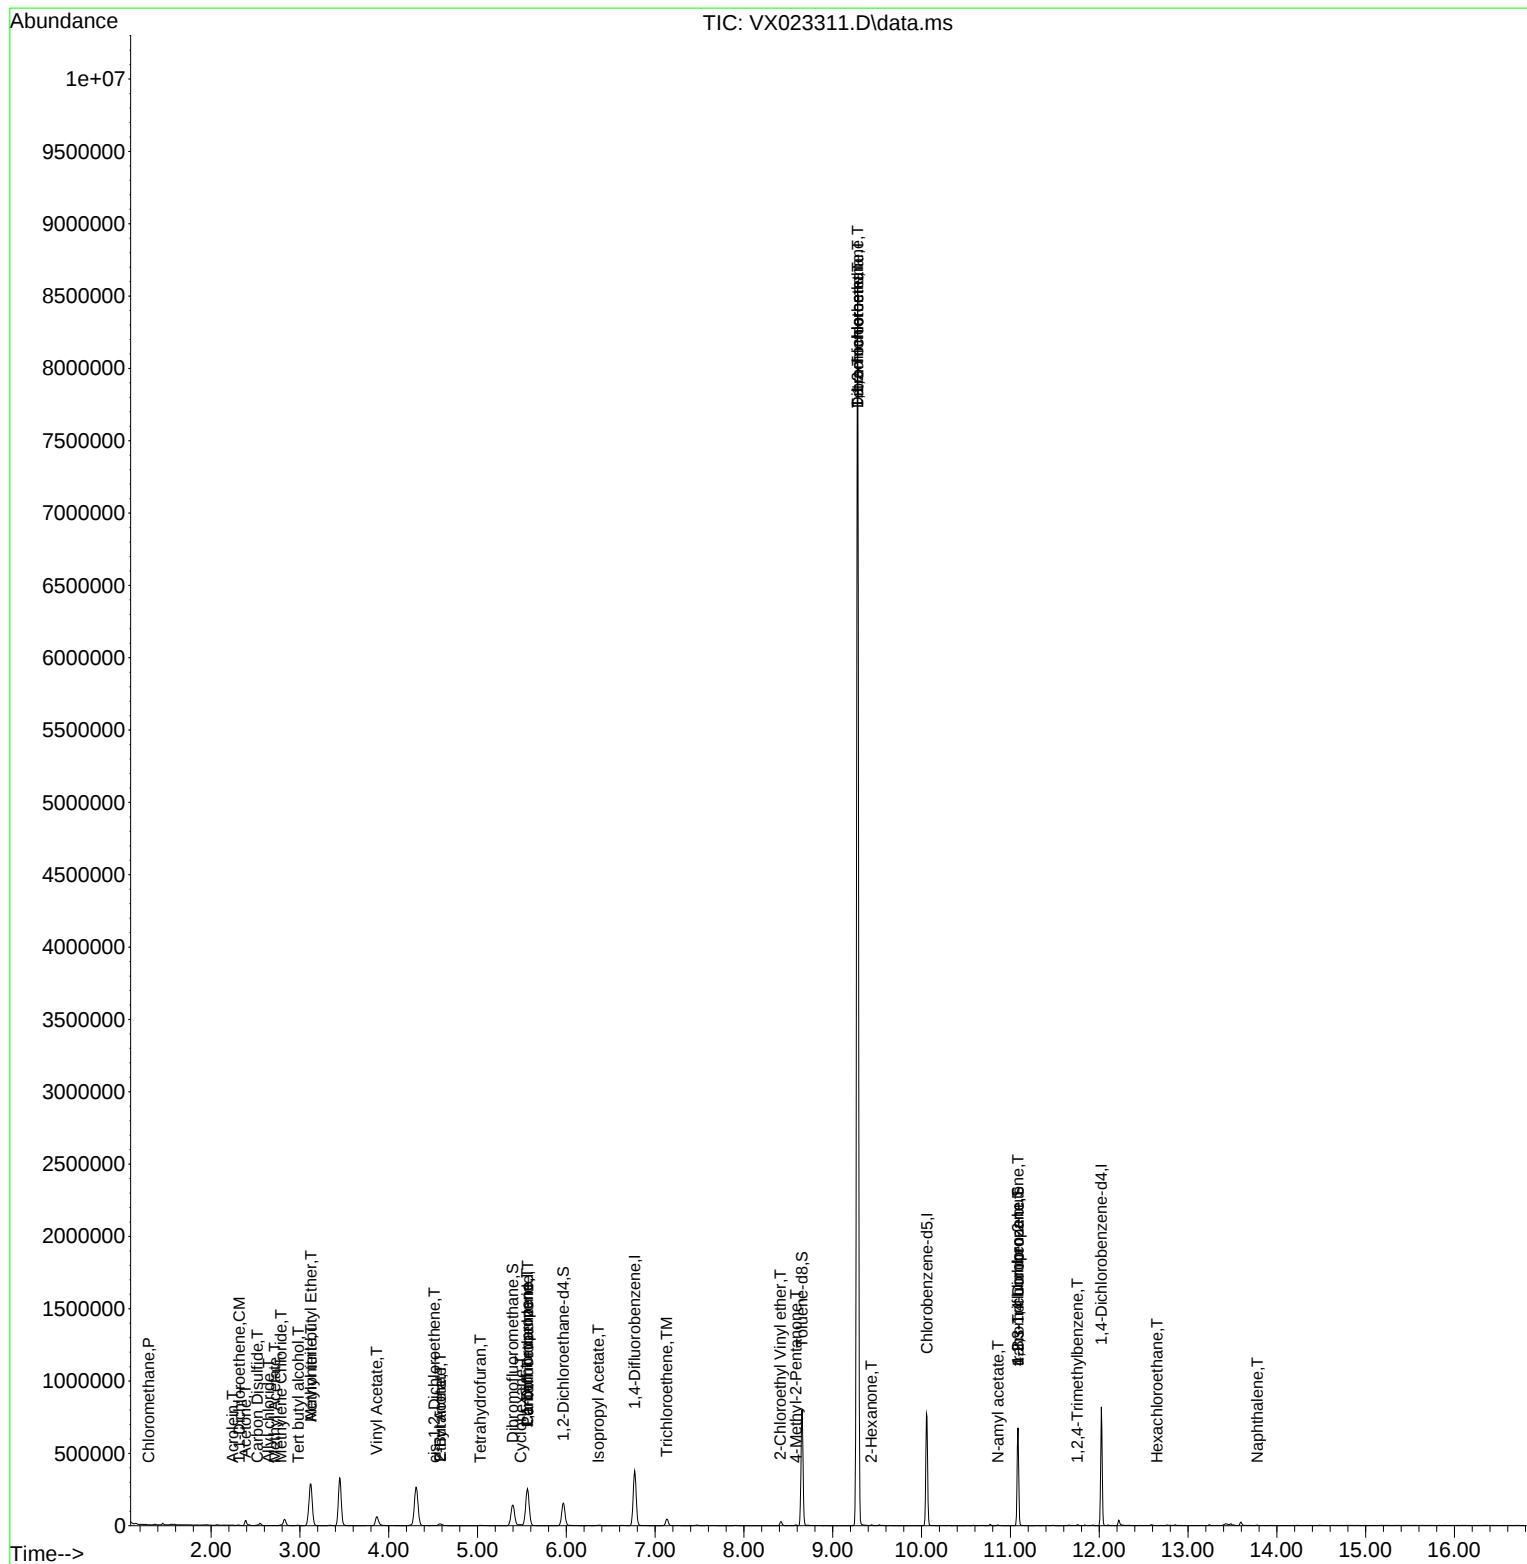




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.562 min Scan# 734
Delta R.T. -0.000 min
Lab File: VX023311.D
Acq: 15 Jul 2021 19:57




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:168 Resp: 238029
Ion Ratio Lower Upper
168 100
99 62.5 45.8 68.6

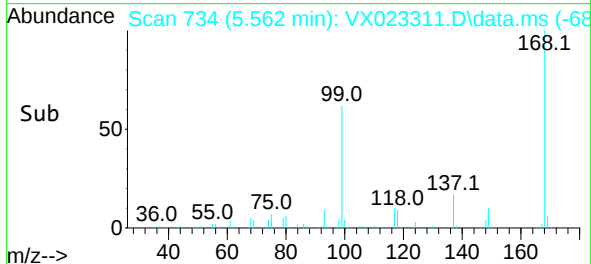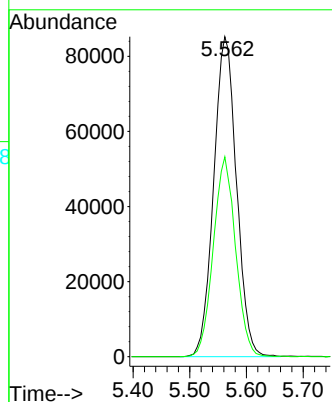

#3
Chloromethane
Concen: 0.215 ug/l
RT: 1.294 min Scan# 34
Delta R.T. 0.000 min
Lab File: VX023311.D
Acq: 15 Jul 2021 19:57

Tgt Ion: 50 Resp: 458
Ion Ratio Lower Upper
50 100
52 17.7 26.4 39.6#


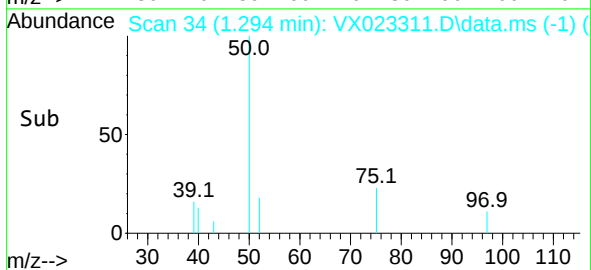
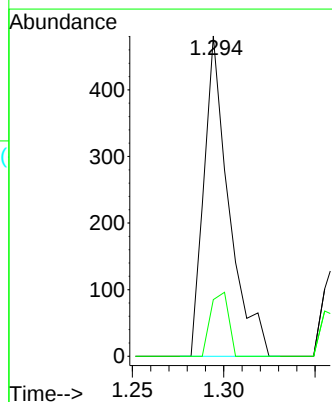
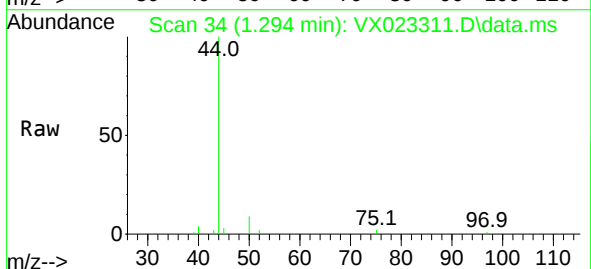


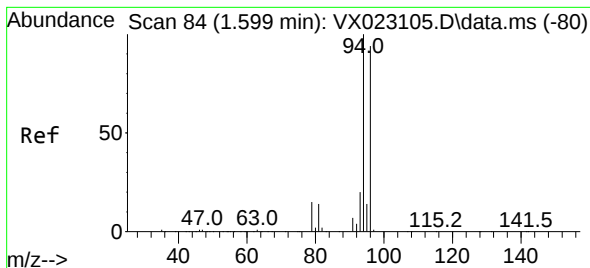

#5
Bromomethane
Concen: Below Cal
RT: 1.611 min Scan# 86
Delta R.T. 0.012 min
Lab File: VX023311.D
Acq: 15 Jul 2021 19:57




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 94 Resp: 559
Ion Ratio Lower Upper
94 100
96 41.6 76.4 114.6#

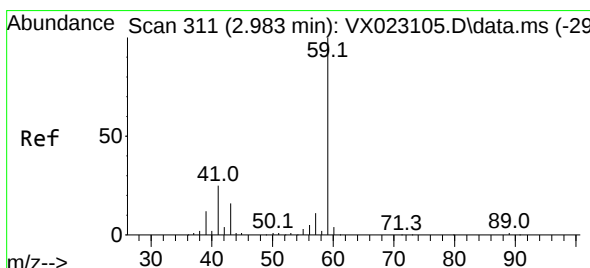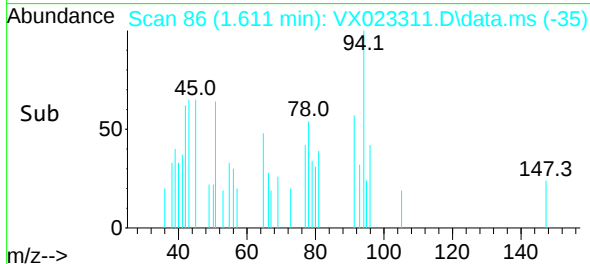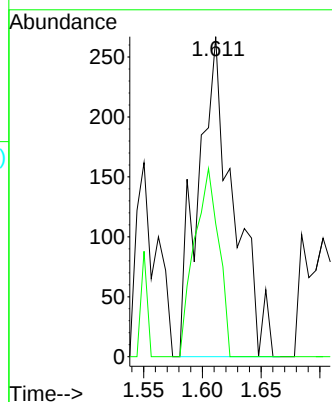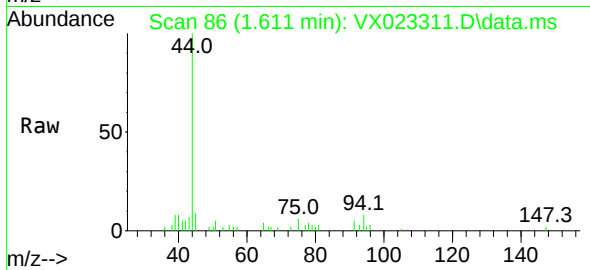

#11
Tert butyl alcohol
Concen: 4.250 ug/l
RT: 2.983 min Scan# 311
Delta R.T. 0.000 min
Lab File: VX023311.D
Acq: 15 Jul 2021 19:57

Tgt Ion: 59 Resp: 2860
Ion Ratio Lower Upper
59 100
57 0.0 7.8 11.8#

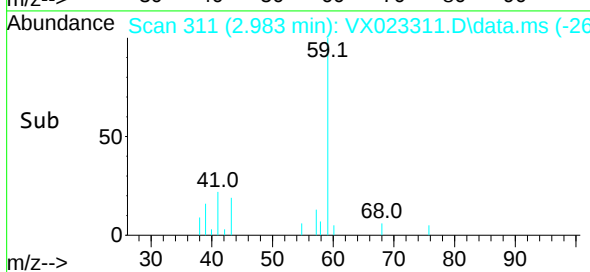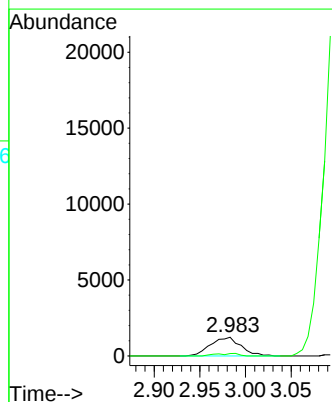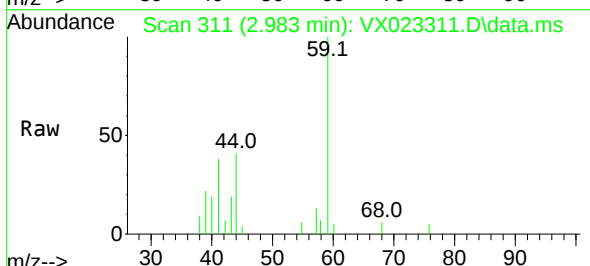



#12

1,1-Dichloroethene

Concen: 0.310 ug/l

RT: 2.318 min Scan# 202

Delta R.T. -0.001 min

Lab File: VX023311.D

Acq: 15 Jul 2021 19:57





Tgt Ion: 96 Resp: 657

Ion Ratio Lower Upper

96 100

61 164.7 124.6 187.0

98 85.1 50.6 76.0#

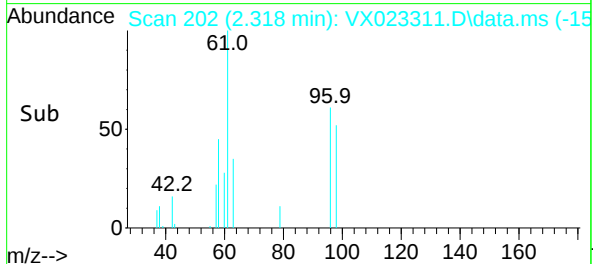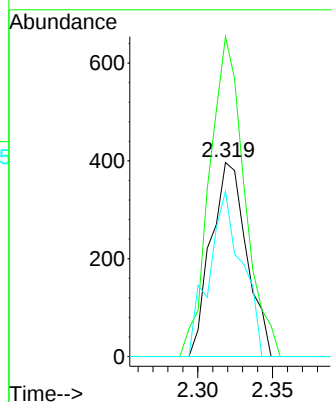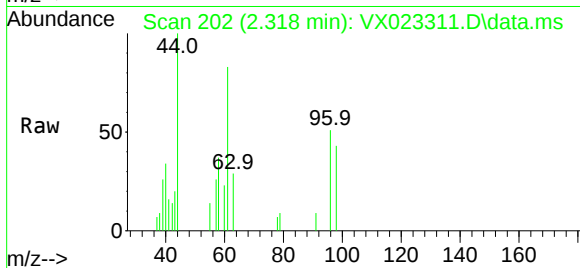

#13

Acrolein

Concen: 0.571 ug/l

RT: 2.239 min Scan# 189

Delta R.T. -0.006 min

Lab File: VX023311.D




Acq: 15 Jul 2021 19:57


Tgt Ion: 56 Resp: 256

Ion Ratio Lower Upper

56 100

55 0.0 56.4 84.6#

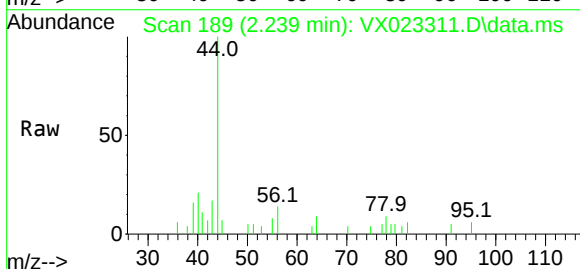



#14

Allyl chloride

Concen: 0.212 ug/l

RT: 2.648 min Scan# 256





Delta R.T. -0.018 min

Lab File: VX023311.D

Acq: 15 Jul 2021 19:57

Tgt Ion: 41	Resp: 780
Ion Ratio	Lower Upper
41 100	
39 30.1	51.6 77.4#
76 0.0	30.5 45.7#

Instrument :
MSVOA_X
ClientSampleId :



#15

Acrylonitrile

Concen: 4.029 ug/l




RT: 3.123 min Scan# 334


Delta R.T. 0.048 min

Lab File: VX023311.D

Acq: 15 Jul 2021 19:57

Tgt Ion: 53	Resp: 5272
Ion Ratio	Lower Upper
53 100	
52 21.6	65.3 97.9#
51 72.2	28.2 42.2#


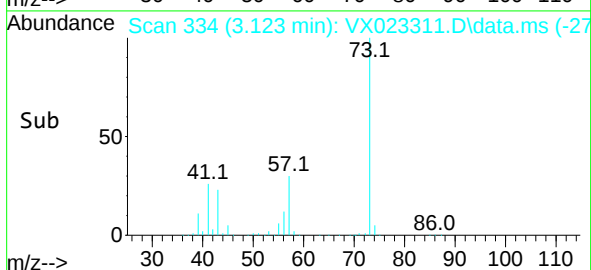






#16
Acetone
Concen: 29.874 ug/l
RT: 2.386 min Scan# 213
Delta R.T. -0.006 min
Lab File: VX023311.D
Acq: 15 Jul 2021 19:57




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 43 Resp: 37810
Ion Ratio Lower Upper
43 100
58 28.8 27.8 41.8

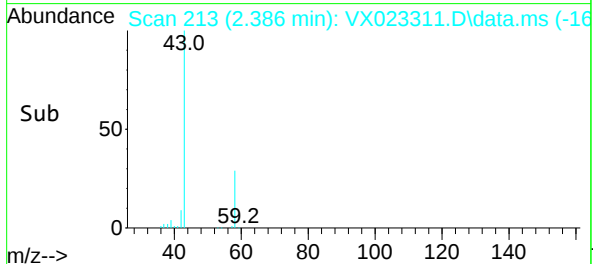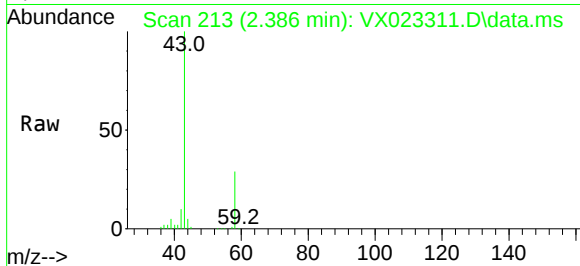

#17
Carbon Disulfide
Concen: 1.031 ug/l
RT: 2.520 min Scan# 235
Delta R.T. 0.006 min
Lab File: VX023311.D
Acq: 15 Jul 2021 19:57

Tgt Ion: 76 Resp: 4612
Ion Ratio Lower Upper
76 100
78 12.5 7.2 10.8#


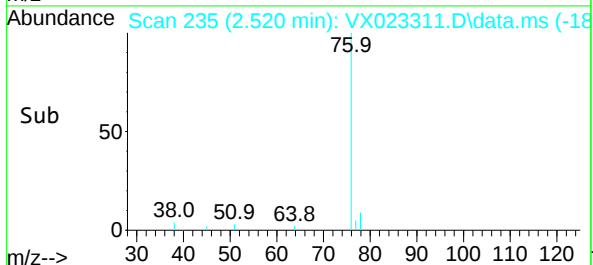

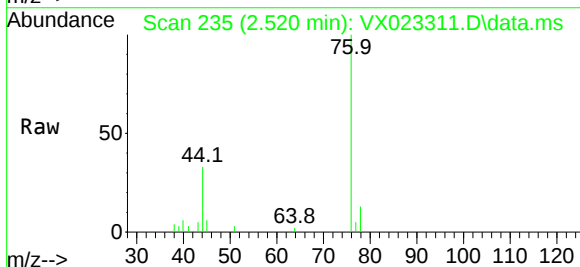




#18
Methyl Acetate
Concen: 0.365 ug/l
RT: 2.715 min Scan# 267
Delta R.T. -0.000 min
Lab File: VX023311.D
Acq: 15 Jul 2021 19:57




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion: 43 Resp: 1120
Ion Ratio Lower Upper
43 100
74 23.5 21.9 32.9

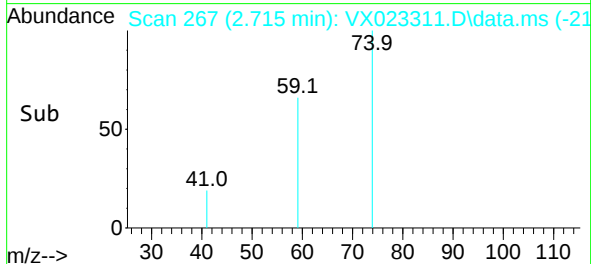

#19
Methyl tert-butyl Ether
Concen: 35.534 ug/l
RT: 3.123 min Scan# 334
Delta R.T. 0.000 min
Lab File: VX023311.D
Acq: 15 Jul 2021 19:57

Tgt Ion: 73 Resp: 281988
Ion Ratio Lower Upper
73 100
57 29.7 17.1 25.7#

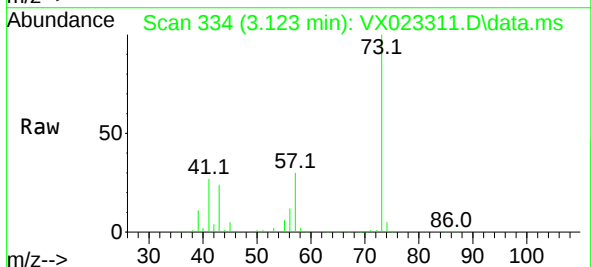



#20

Methylene Chloride

Concen: 0.255 ug/l

RT: 2.788 min Scan# 279

Delta R.T. -0.006 min

Lab File: VX023311.D

Acq: 15 Jul 2021 19:57

Tgt Ion: 84 Resp: 694





Ion Ratio Lower Upper

84 100

49 129.0 88.6 132.8

51 73.2 27.0 40.6#

86 75.7 50.3 75.5#

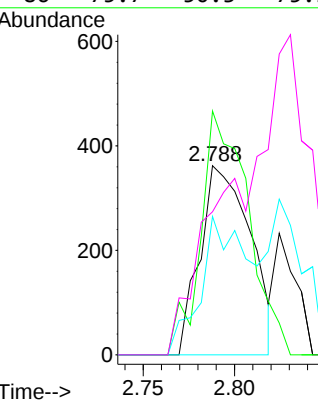

#23

Vinyl Acetate

Concen: 1.499 ug/l

RT: 3.861 min Scan# 455

Delta R.T. 0.128 min

Lab File: VX023311.D




Acq: 15 Jul 2021 19:57


Tgt Ion: 43 Resp: 9861

Ion Ratio Lower Upper

43 100

86 0.0 9.9 14.9#


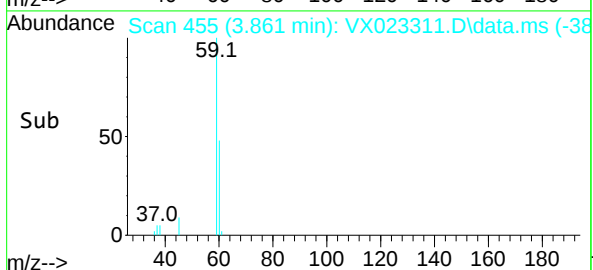
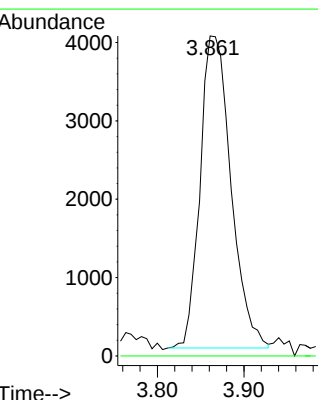





#25
2-Butanone
Concen: 9.978 ug/l
RT: 4.580 min Scan# 573
Delta R.T. 0.012 min
Lab File: VX023311.D
Acq: 15 Jul 2021 19:57




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 43 Resp: 19043
Ion Ratio Lower Upper
43 100
72 27.1 23.7 35.5

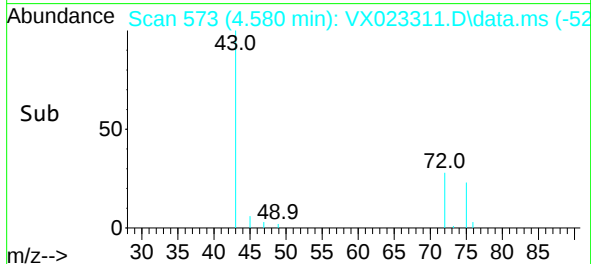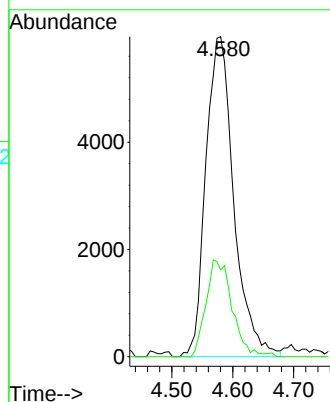

#27
cis-1,2-Dichloroethene
Concen: 0.309 ug/l
RT: 4.513 min Scan# 562
Delta R.T. 0.018 min
Lab File: VX023311.D
Acq: 15 Jul 2021 19:57

Tgt Ion: 96 Resp: 858
Ion Ratio Lower Upper
96 100
61 133.1 0.0 285.6
98 52.9 0.0 129.6

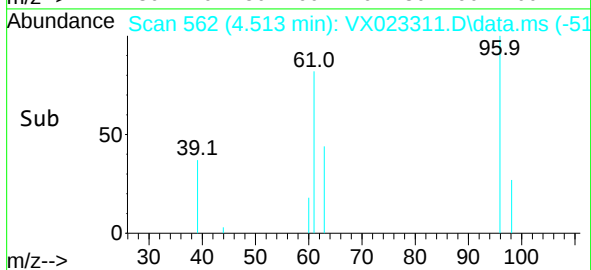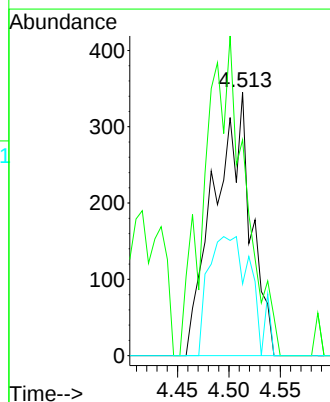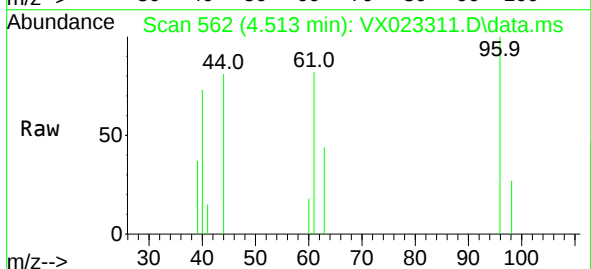



#29

Tetrahydrofuran

Concen: 0.868 ug/l

RT: 5.031 min Scan# 647





Delta R.T. 0.012 min

Lab File: VX023311.D

Acq: 15 Jul 2021 19:57

Tgt Ion:	42	Resp:	1065
Ion	Ratio	Lower	Upper
42	100		
72	0.0	41.7	62.5#
71	13.1	38.4	57.6#

Instrument :
MSVOA_X
ClientSampleId :

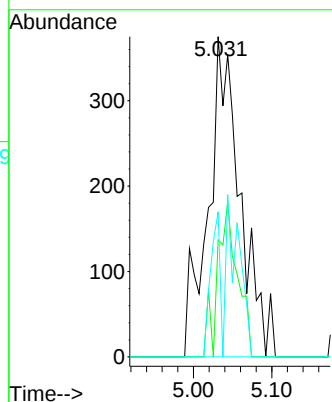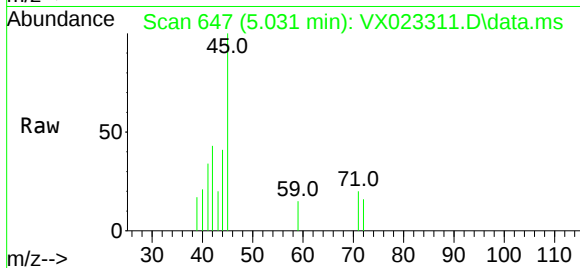

#31

Cyclohexane

Concen: 1.190 ug/l




RT: 5.483 min Scan# 721


Delta R.T. 0.006 min

Lab File: VX023311.D

Acq: 15 Jul 2021 19:57

Tgt Ion:	56	Resp:	4558
Ion	Ratio	Lower	Upper
56	100		
69	38.3	25.3	37.9#
84	79.8	71.4	107.0


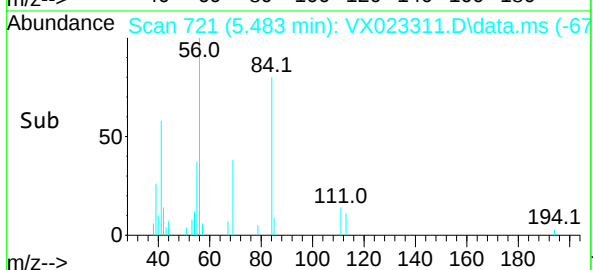

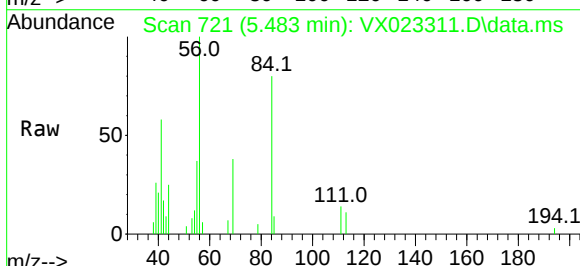




#33
1,2-Dichloroethane-d4
Concen: 50.238 ug/l
RT: 5.964 min Scan# 800
Delta R.T. 0.000 min
Lab File: VX023311.D
Acq: 15 Jul 2021 19:57




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 65 Resp: 160716
Ion Ratio Lower Upper
65 100
67 50.3 0.0 105.4

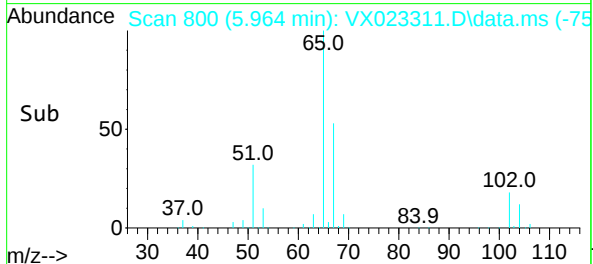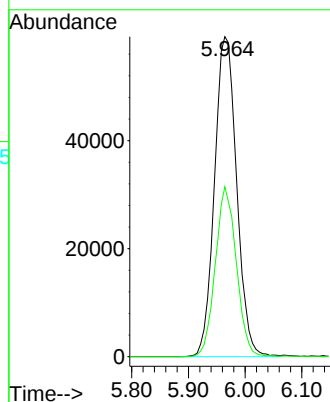

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.769 min Scan# 932
Delta R.T. -0.000 min
Lab File: VX023311.D
Acq: 15 Jul 2021 19:57

Tgt Ion: 114 Resp: 387310
Ion Ratio Lower Upper
114 100
63 20.5 0.0 40.8
88 16.6 0.0 32.8


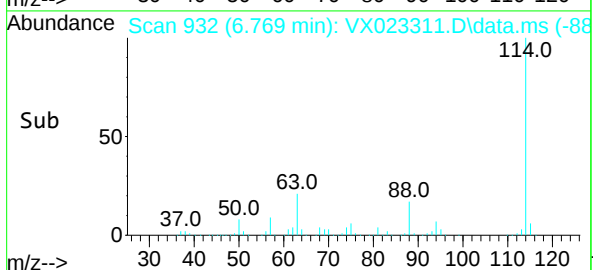
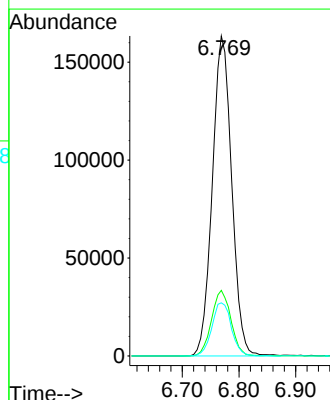





#35
Dibromofluoromethane
Concen: 50.300 ug/l
RT: 5.397 min Scan# 707
Delta R.T. 0.000 min
Lab File: VX023311.D
Acq: 15 Jul 2021 19:57




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:113 Resp: 125805
Ion Ratio Lower Upper
113 100
111 102.0 81.9 122.9
192 19.2 16.7 25.1

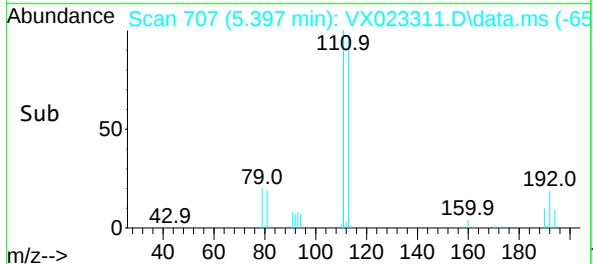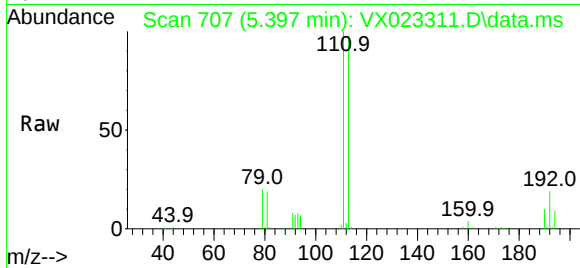

#36
1,1-Dichloropropene
Concen: 5.199 ug/l
RT: 5.556 min Scan# 733
Delta R.T. -0.146 min
Lab File: VX023311.D
Acq: 15 Jul 2021 19:57

Tgt Ion: 75 Resp: 17952
Ion Ratio Lower Upper
75 100
110 10.8 18.1 54.4#
77 0.0 25.3 37.9#

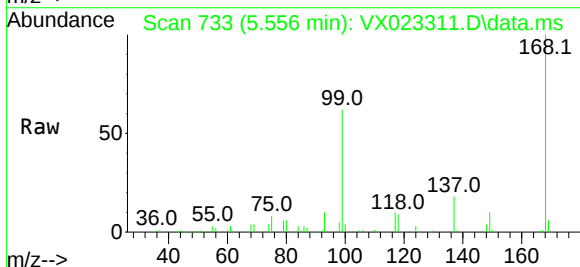



#37

Ethyl Acetate

Concen: 5.056 ug/l

RT: 4.580 min Scan# 573





Delta R.T. -0.147 min

Lab File: VX023311.D

Acq: 15 Jul 2021 19:57

Instrument :
MSVOA_X
ClientSampleId :

Tgt Ion: 43	Resp:	19043
Ion Ratio	Lower	Upper
43	100	
61	0.0	12.8
70	0.0	10.5

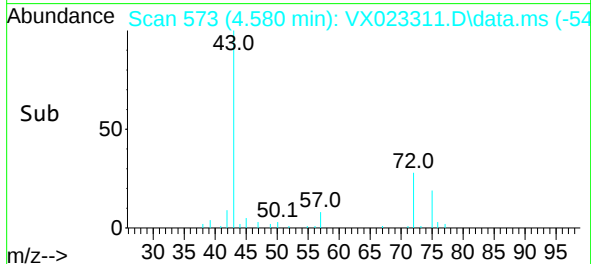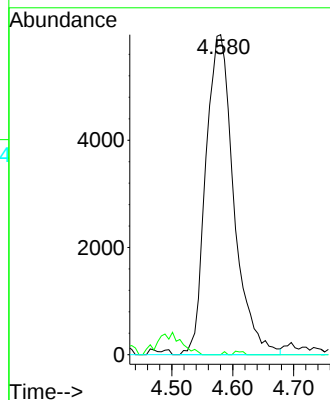

#38

Carbon Tetrachloride

Concen: 6.966 ug/l




RT: 5.562 min Scan# 734


Delta R.T. -0.122 min

Lab File: VX023311.D

Acq: 15 Jul 2021 19:57

Tgt Ion: 117	Resp:	25107
Ion Ratio	Lower	Upper
117	100	
119	3.8	76.2
121	0.0	24.8


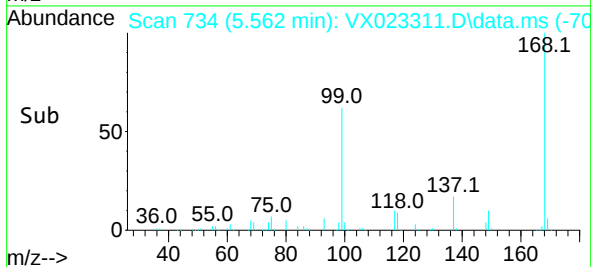
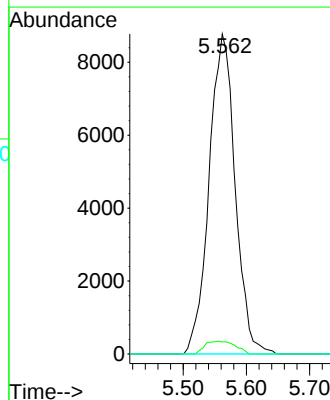
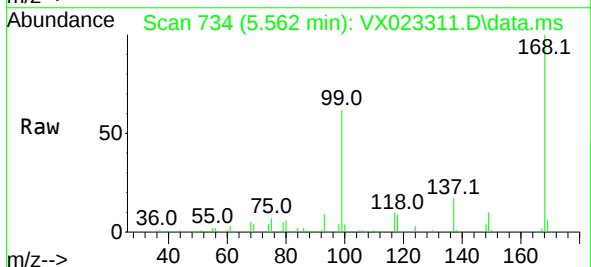




#43
Isopropyl Acetate
Concen: 0.238 ug/l
RT: 6.360 min Scan# 865
Delta R.T. 0.006 min
Lab File: VX023311.D
Acq: 15 Jul 2021 19:57




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion: 43 Resp: 1489
Ion Ratio Lower Upper
43 100
61 0.0 18.2 27.4#
87 0.0 12.5 18.7#

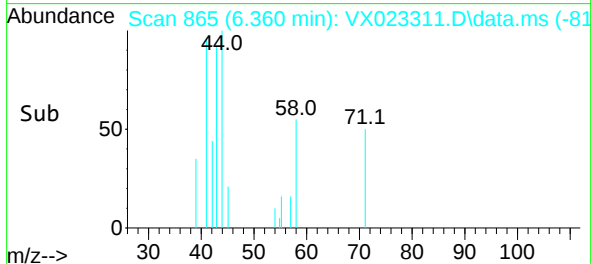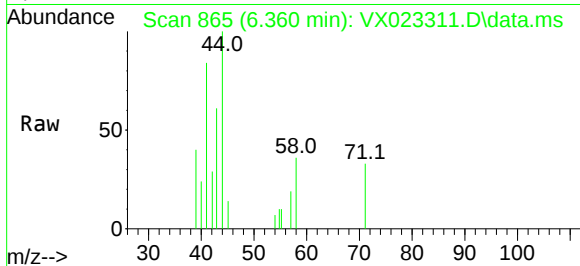

#44
Trichloroethene
Concen: 6.211 ug/l
RT: 7.129 min Scan# 991
Delta R.T. -0.006 min
Lab File: VX023311.D
Acq: 15 Jul 2021 19:57

Tgt Ion:130 Resp: 17664
Ion Ratio Lower Upper
130 100
95 100.4 0.0 198.0


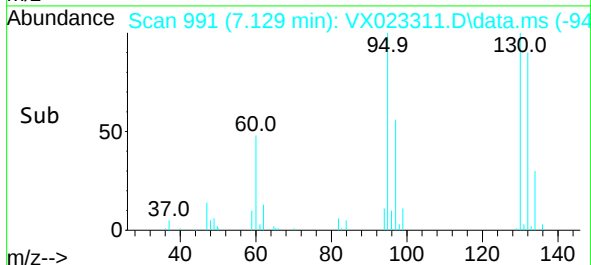

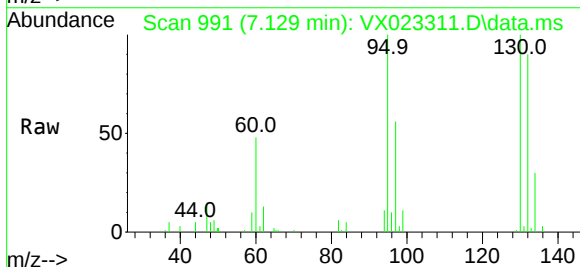




#50
Toluene-d8
Concen: 50.143 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. -0.000 min
Lab File: VX023311.D
Acq: 15 Jul 2021 19:57




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion: 98 Resp: 467812
Ion Ratio Lower Upper
98 100
100 63.5 51.9 77.9

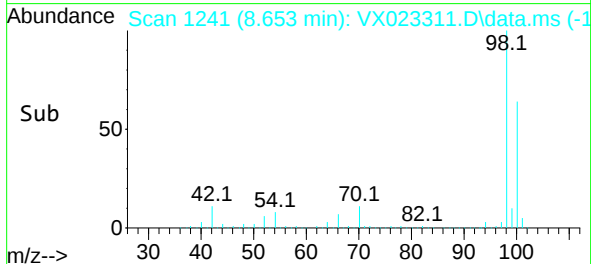

#51
4-Methyl-2-Pentanone
Concen: 0.654 ug/l
RT: 8.586 min Scan# 1230
Delta R.T. 0.006 min
Lab File: VX023311.D
Acq: 15 Jul 2021 19:57


Tgt Ion: 43 Resp: 2539
Ion Ratio Lower Upper
43 100
58 43.8 35.4 53.0

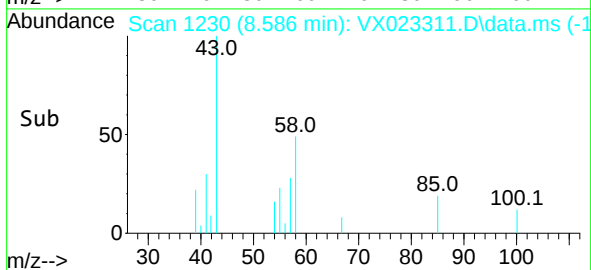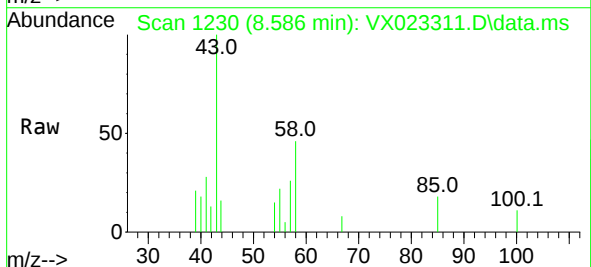






#55
1,1,2-Trichloroethane
Concen: 5.456 ug/l
RT: 9.281 min Scan# 1344
Delta R.T. 0.122 min
Lab File: VX023311.D
Acq: 15 Jul 2021 19:57

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion:	97	Resp:	14864
Ion	Ratio	Lower	Upper
97	100		
83	213.5	69.3	103.9#
85	33.7	44.3	66.5#
99	15.6	50.3	75.5#

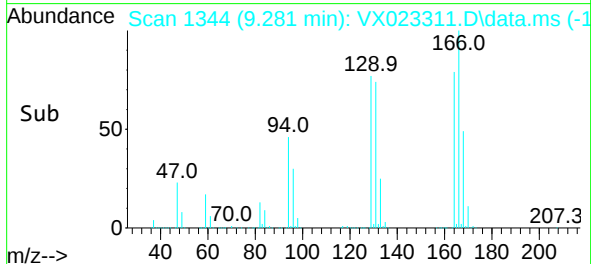

#58
2-Chloroethyl Vinyl ether
Concen: 4.733 ug/l
RT: 8.409 min Scan# 1201
Delta R.T. 0.159 min
Lab File: VX023311.D
Acq: 15 Jul 2021 19:57

Tgt Ion:	63	Resp:	101
Ion	Ratio	Lower	Upper
63	100		
106	0.0	23.5	35.3#


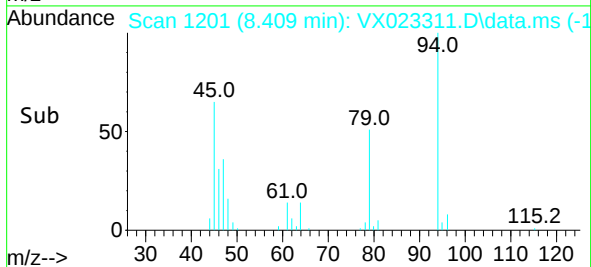

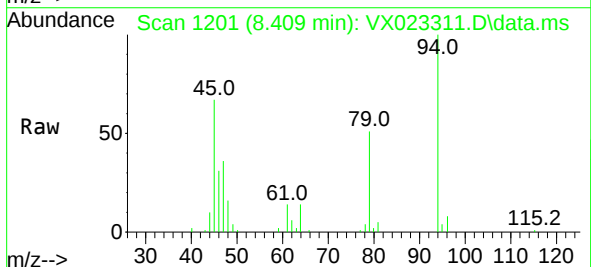




#59
2-Hexanone
Concen: 0.929 ug/l
RT: 9.433 min Scan# 1369
Delta R.T. 0.000 min
Lab File: VX023311.D
Acq: 15 Jul 2021 19:57




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 43 Resp: 2767
Ion Ratio Lower Upper
43 100
58 49.0 30.9 92.8

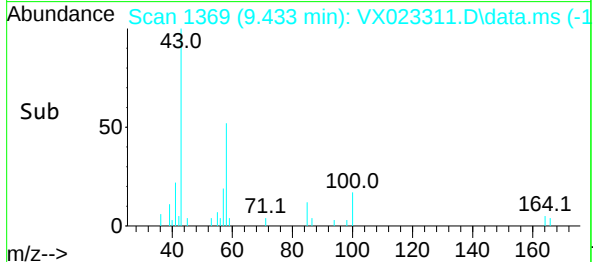

#60
Dibromochloromethane
Concen: 496.371 ug/l
RT: 9.281 min Scan# 1344
Delta R.T. -0.244 min
Lab File: VX023311.D
Acq: 15 Jul 2021 19:57

Tgt Ion: 129 Resp: 1600116
Ion Ratio Lower Upper
129 100
127 0.0 38.4 115.2#


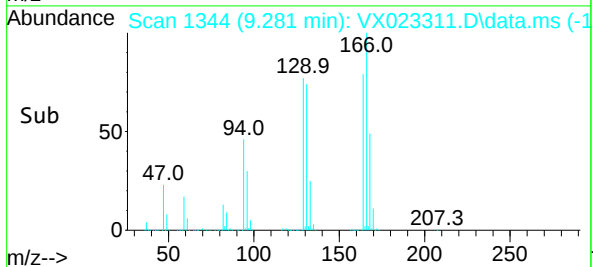

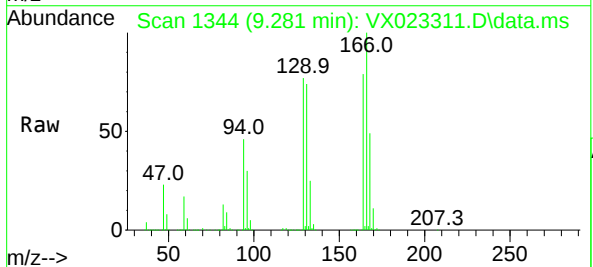




#62
4-Bromofluorobenzene
Concen: 49.850 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.000 min
Lab File: VX023311.D
Acq: 15 Jul 2021 19:57




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 95 Resp: 179547
Ion Ratio Lower Upper
95 100
174 77.4 0.0 154.6
176 73.3 0.0 155.8

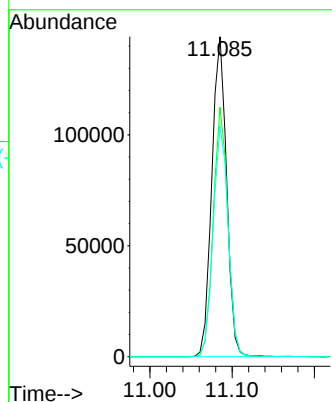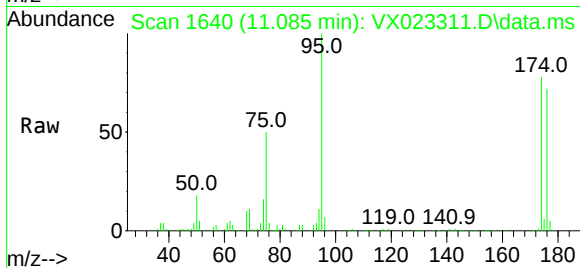

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.061 min Scan# 1472
Delta R.T. 0.000 min
Lab File: VX023311.D
Acq: 15 Jul 2021 19:57


Tgt Ion: 117 Resp: 360773
Ion Ratio Lower Upper
117 100
82 54.3 47.4 71.2
119 31.7 26.6 39.8

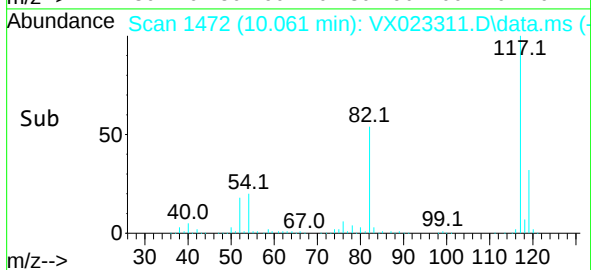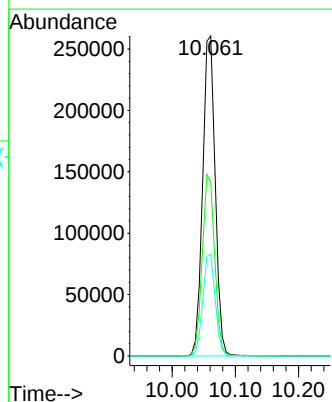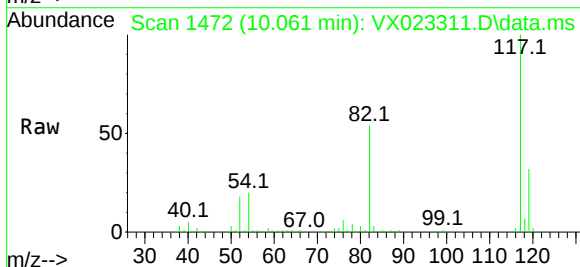






#64
Tetrachloroethene
Concen: 567.110 ug/l
RT: 9.281 min Scan# 1344
Delta R.T. -0.000 min
Lab File: VX023311.D
Acq: 15 Jul 2021 19:57

Instrument :
MSVOA_X
ClientSampled :




Tgt Ion:164 Resp: 1631859

Ion	Ratio	Lower	Upper
164	100		
166	126.8	103.4	155.2
129	97.1	70.8	106.2
131	93.5	72.5	108.7

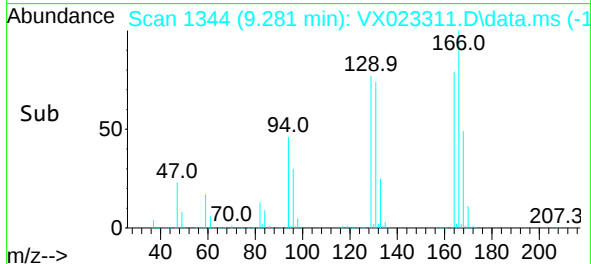




#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX023311.D
Acq: 15 Jul 2021 19:57

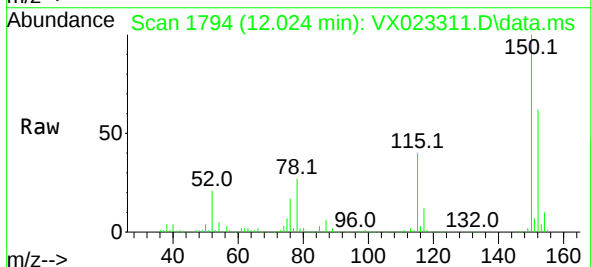

Tgt Ion:152 Resp: 159739


Ion	Ratio	Lower	Upper
152	100		
115	62.7	41.1	123.3
150	159.1	0.0	349.0

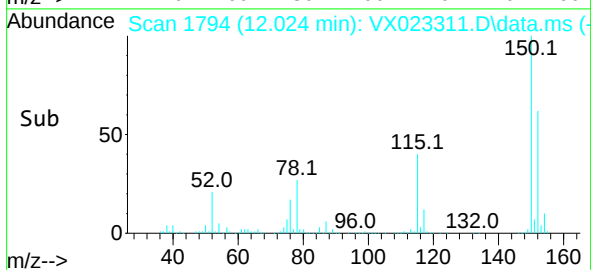



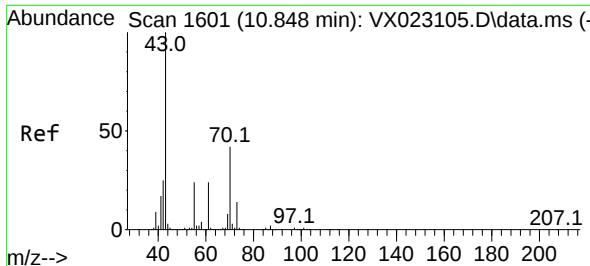


#74
N-amy1 acetate
Concen: 0.270 ug/l
RT: 10.860 min Scan# 1603
Delta R.T. 0.012 min
Lab File: VX023311.D
Acq: 15 Jul 2021 19:57

Instrument :
MSVOA_X
ClientSampled :



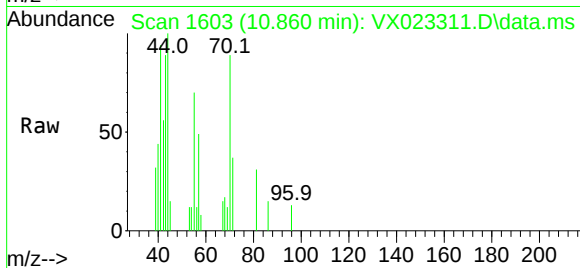



Tgt Ion:	43	Resp:	1287
Ion	Ratio	Lower	Upper
43	100		
70	64.3	39.0	58.6#
55	58.8	21.5	32.3#
61	0.0	22.1	33.1#

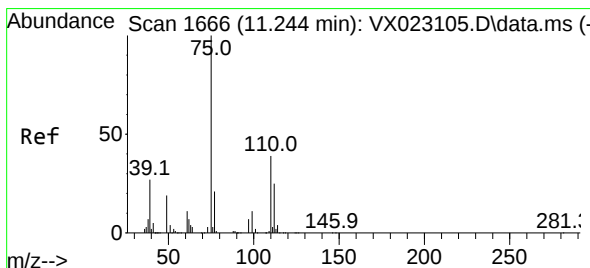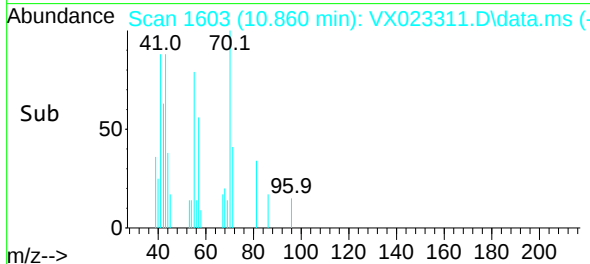

#76
1,2,3-Trichloropropane
Concen: 28.664 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. -0.159 min
Lab File: VX023311.D
Acq: 15 Jul 2021 19:57

Tgt Ion:	75	Resp:	92140
Ion	Ratio	Lower	Upper
75	100		
77	1.1	19.1	57.5#


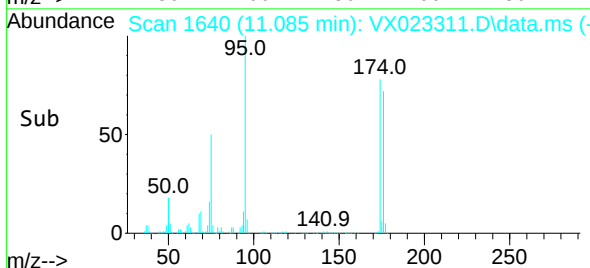

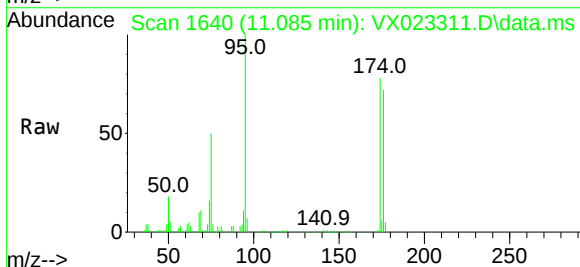




#81
trans-1,4-Dichloro-2-butene
Concen: 77.176 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.061 min
Lab File: VX023311.D
Acq: 15 Jul 2021 19:57




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 75 Resp: 92140
Ion Ratio Lower Upper
75 100
53 0.0 74.5 111.7#
89 0.0 37.9 56.9#

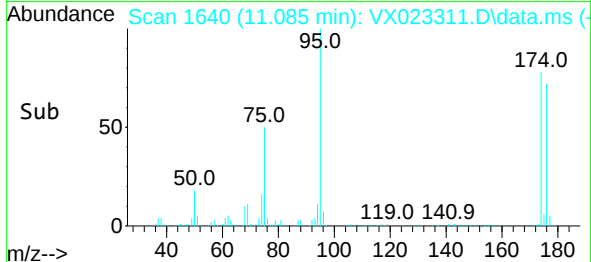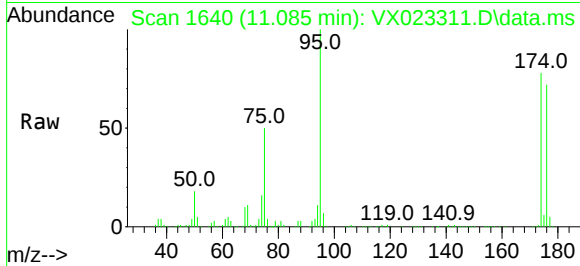

#84
1,2,4-Trimethylbenzene
Concen: 0.231 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. -0.000 min
Lab File: VX023311.D
Acq: 15 Jul 2021 19:57

Tgt Ion:105 Resp: 2213
Ion Ratio Lower Upper
105 100
120 14.7 22.4 67.3#


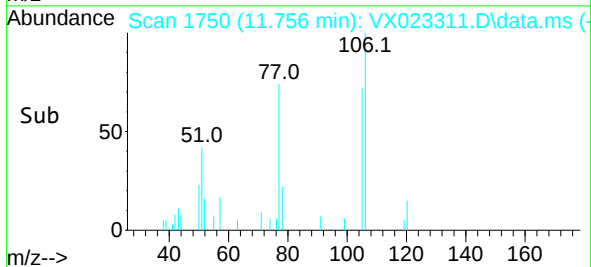

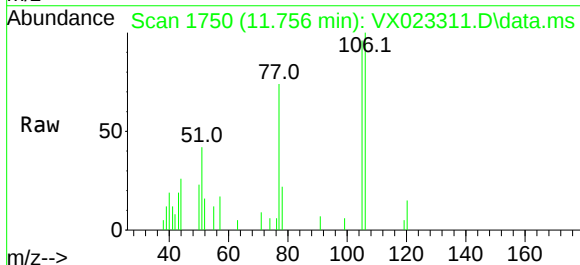




#90
Hexachloroethane
Concen: 3.029 ug/l
RT: 12.652 min Scan# 1897
Delta R.T. 0.110 min
Lab File: VX023311.D
Acq: 15 Jul 2021 19:57

Instrument :
MSVOA_X
ClientSampleId :

Tgt Ion:117 Resp: 61
Ion Ratio Lower Upper
117 100
201 0.0 40.4 121.2#

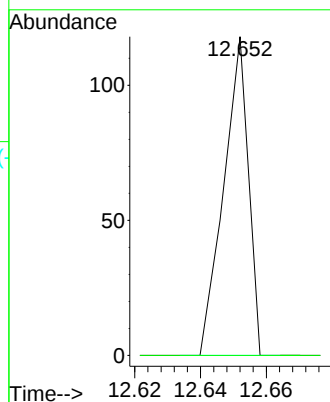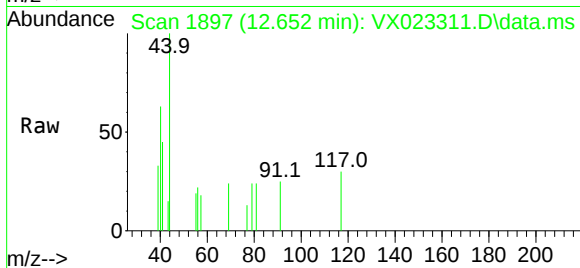

#95
Naphthalene
Concen: 1.438 ug/l
RT: 13.780 min Scan# 2082
Delta R.T. -0.000 min
Lab File: VX023311.D
Acq: 15 Jul 2021 19:57

Tgt Ion:128 Resp: 1987
Ion Ratio Lower Upper
128 100
127 17.6 10.3 15.5#
129 10.8 8.8 13.2

