

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071523\
 Data File : VX036551.D
 Acq On : 14 Jul 2023 10:10
 Operator : JC/MD
 Sample : VX0715WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0715WBL01

Quant Time: Jul 17 01:26:56 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X071423W.M
 Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 QLast Update : Fri Jul 14 04:32:22 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	4.903	128	34558	30.000	ug/l	0.00
28) 1,4-Difluorobenzene	6.763	114	186795	30.000	ug/l	0.00
57) Chlorobenzene-d5	10.055	117	166128	30.000	ug/l	0.00

System Monitoring Compounds						
27) 1,2-Dichloroethane-d4	5.958	65	83683	29.176	ug/l	0.00
Spiked Amount	30.000	Range	91 - 110	Recovery	=	97.267%
60) 4-Bromofluorobenzene	11.079	95	75164	27.893	ug/l	0.00
Spiked Amount	30.000	Range	63 - 112	Recovery	=	92.967%
63) Toluene-d8	8.647	98	230646	30.171	ug/l	0.00
Spiked Amount	30.000	Range	91 - 112	Recovery	=	100.567%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071523\
Data File : VX036551.D
Acq On : 14 Jul 2023 10:10
Operator : JC/MD
Sample : VX0715WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0715WBL01


Quant Time: Jul 17 01:26:56 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X071423W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
QLast Update : Fri Jul 14 04:32:22 2023
Response via : Initial Calibration

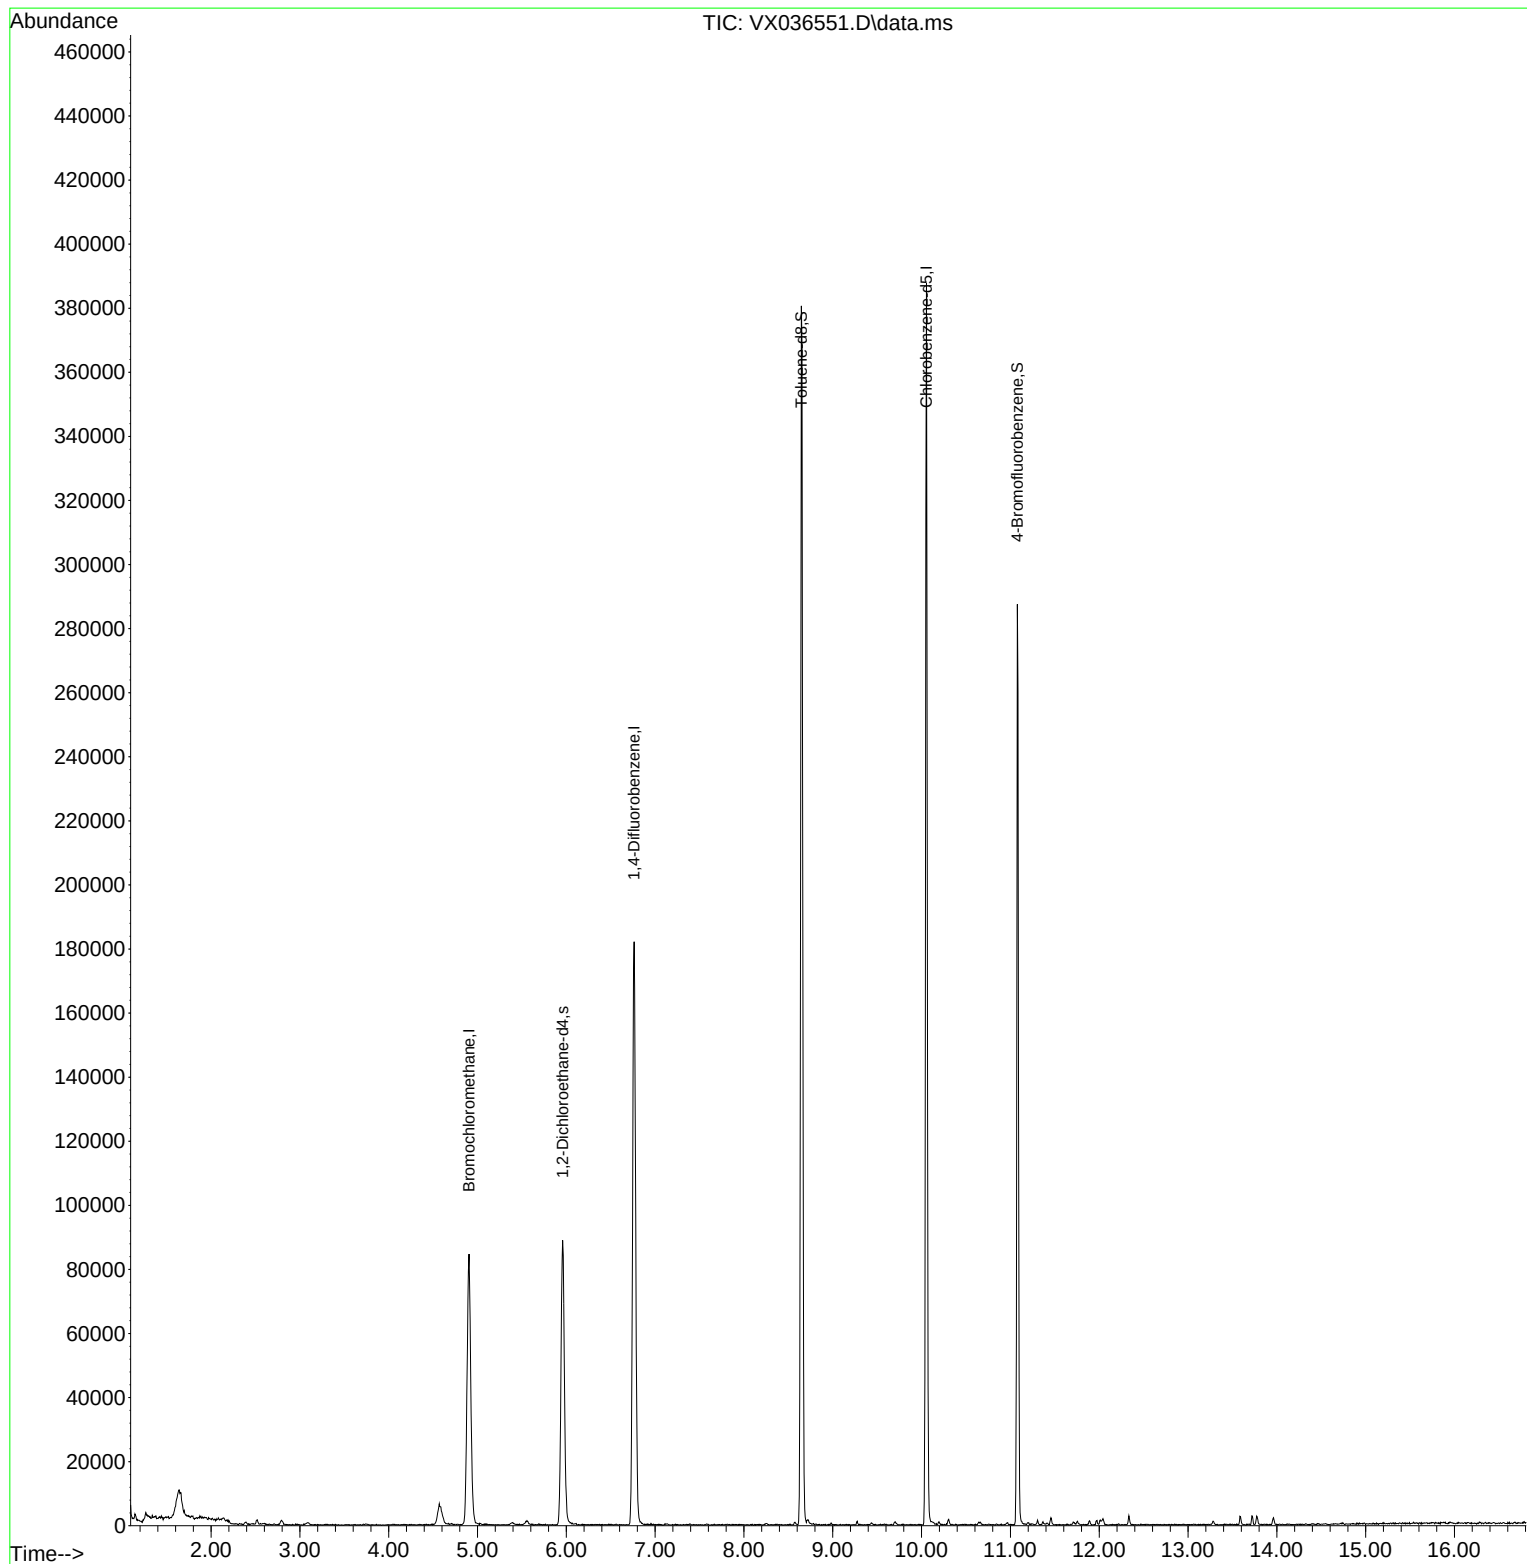



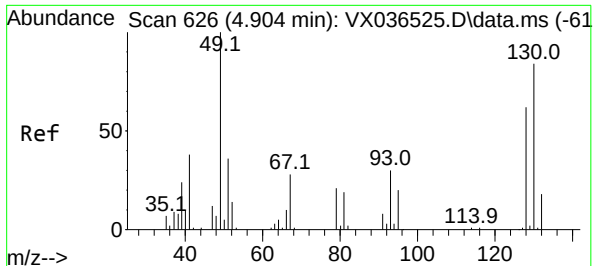


#1
Bromochloromethane
Concen: 30.000 ug/l
RT: 4.903 min Scan# 61
Delta R.T. -0.001 min
Lab File: VX036551.D
Acq: 14 Jul 2023 10:10

Instrument :
MSVOA_X
ClientSampleId :
VX0715WBL01



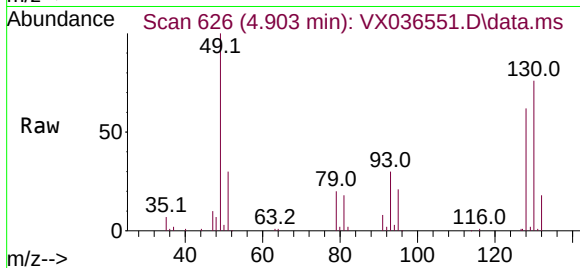



Tgt Ion:128 Resp: 34558
Ion Ratio Lower Upper
128 100
49 161.3 0.0 406.3
130 128.4 0.0 328.0

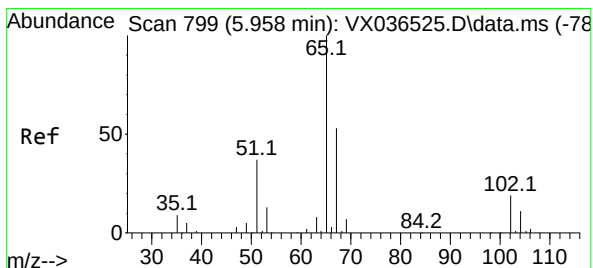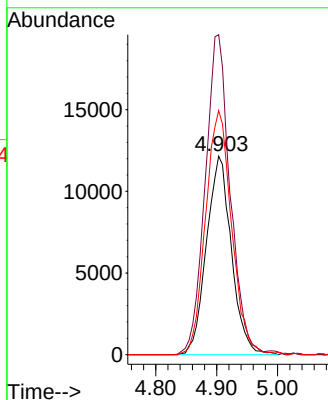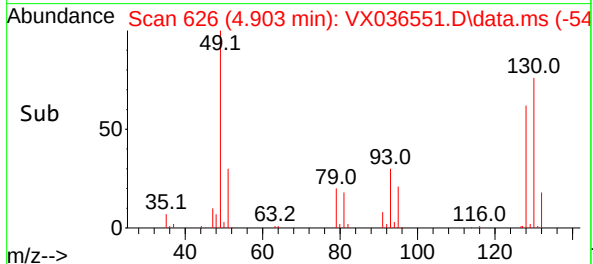

#27
1,2-Dichloroethane-d4
Concen: 29.176 ug/l
RT: 5.958 min Scan# 799
Delta R.T. -0.000 min
Lab File: VX036551.D
Acq: 14 Jul 2023 10:10

Tgt Ion: 65 Resp: 83683
Ion Ratio Lower Upper
65 100
67 53.0 42.1 63.1

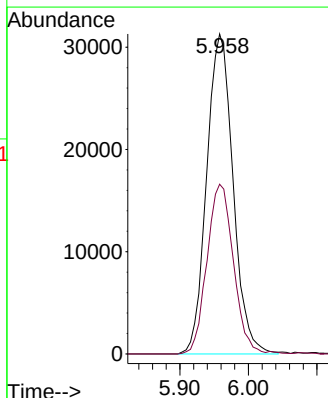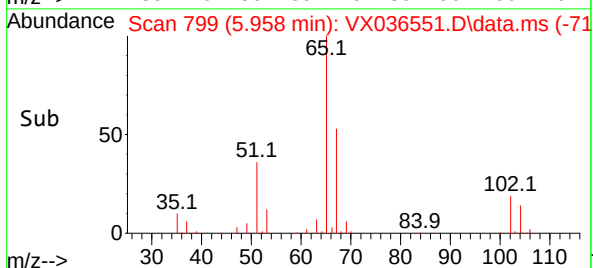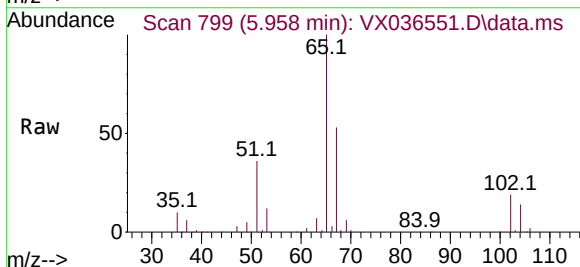

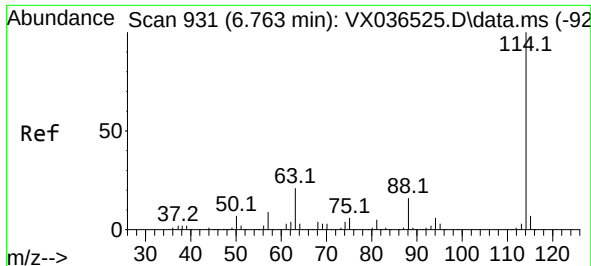

#28

1,4-Difluorobenzene

Concen: 30.000 ug/l

RT: 6.763 min Scan# 91

Delta R.T. -0.000 min

Lab File: VX036551.D

Acq: 14 Jul 2023 10:10

Instrument :

MSVOA_X

ClientSampleId :

VX0715WBL01





Tgt Ion:114 Resp: 186795

Ion Ratio Lower Upper

114 100

63 20.7 16.6 24.8

88 16.0 12.9 19.3

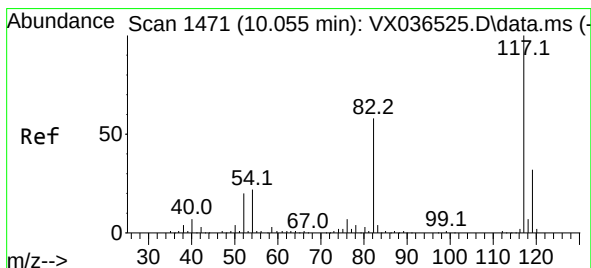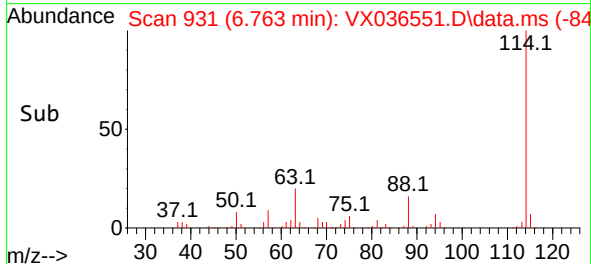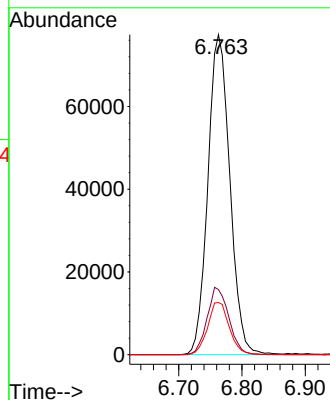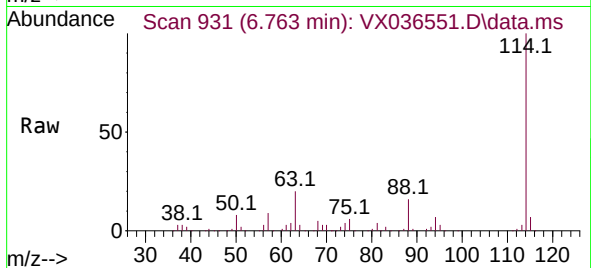

#57

Chlorobenzene-d5

Concen: 30.000 ug/l

RT: 10.055 min Scan# 1471

Delta R.T. -0.000 min

Lab File: VX036551.D

Acq: 14 Jul 2023 10:10




Tgt Ion:117 Resp: 166128


Ion Ratio Lower Upper

117 100

82 55.5 44.7 67.1

119 31.3 25.6 38.4


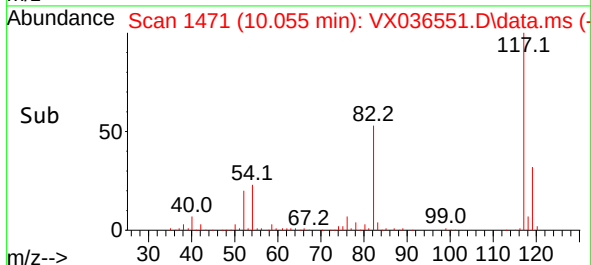
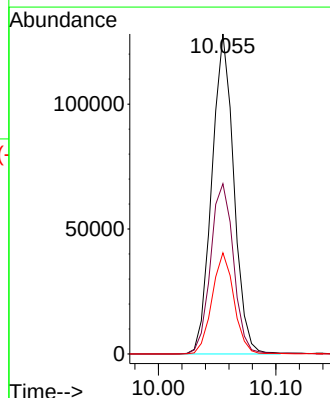
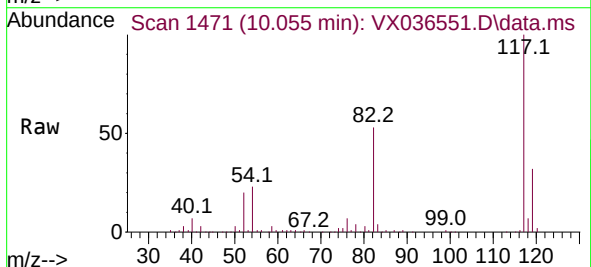


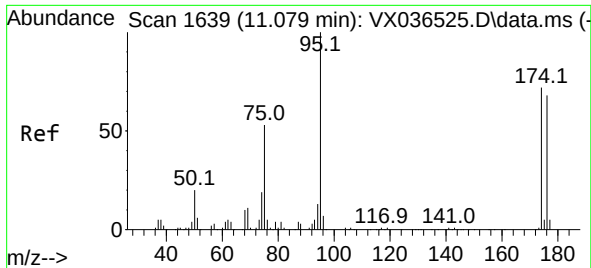

#60
4-Bromofluorobenzene
Concen: 27.893 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.000 min
Lab File: VX036551.D
Acq: 14 Jul 2023 10:10

Instrument :
MSVOA_X
ClientSampleId :
VX0715WBL01

Tgt Ion: 95 Resp: 75164
Ion Ratio Lower Upper
95 100
174 76.5 60.5 90.7
176 72.7 58.2 87.4

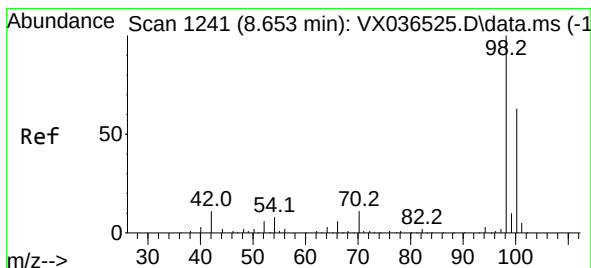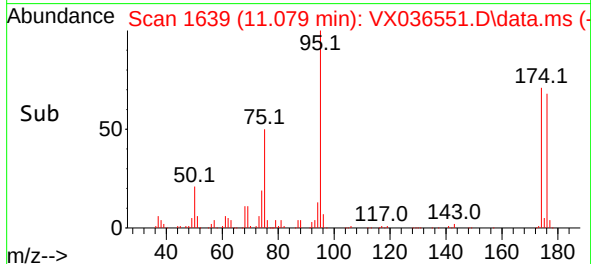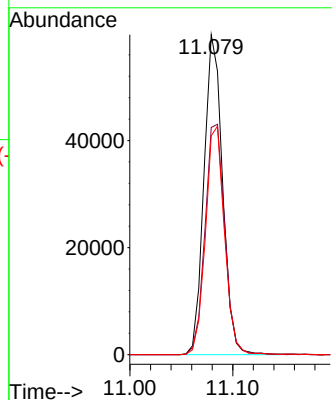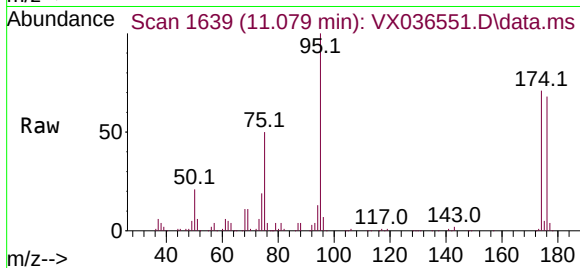

#63
Toluene-d8
Concen: 30.171 ug/l
RT: 8.647 min Scan# 1240
Delta R.T. -0.006 min
Lab File: VX036551.D
Acq: 14 Jul 2023 10:10

Tgt Ion: 98 Resp: 230646
Ion Ratio Lower Upper
98 100
100 63.7 51.6 77.4

