

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071523\
 Data File : VX036556.D
 Acq On : 14 Jul 2023 12:12
 Operator : JC/MD
 Sample : 03596-01DL 5X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 001-WILLETS-PT-BLVD(JULY)DL

Quant Time: Jul 17 01:29:00 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X071423W.M
 Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 QLast Update : Fri Jul 14 04:32:22 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Bromochloromethane	4.903	128	31575	30.000	ug/l	0.00
28) 1,4-Difluorobenzene	6.763	114	165105	30.000	ug/l	0.00
57) Chlorobenzene-d5	10.055	117	148886	30.000	ug/l	0.00
System Monitoring Compounds						
27) 1,2-Dichloroethane-d4	5.958	65	76455	29.174	ug/l	0.00
Spiked Amount 30.000	Range	91 - 110	Recovery	=	97.233%	
60) 4-Bromofluorobenzene	11.079	95	70688	29.269	ug/l	0.00
Spiked Amount 30.000	Range	63 - 112	Recovery	=	97.567%	
63) Toluene-d8	8.647	98	201298	29.382	ug/l	0.00
Spiked Amount 30.000	Range	91 - 112	Recovery	=	97.933%	
Target Compounds						
					Qvalue	
15) Acetone	2.392	58	43083	124.998	ug/l	97
16) Carbon Disulfide	2.508	76	1656	0.369	ug/l #	73
30) 2-Butanone	4.580	43	13504	8.614	ug/l #	80
58) 4-Methyl-2-Pentanone	8.580	43	2724	0.885	ug/l	94
62) Toluene	8.720	91	388344	46.488	ug/l	98
82) p-Isopropyltoluene	12.006	119	2012	0.269	ug/l	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071523\
Data File : VX036556.D
Acq On : 14 Jul 2023 12:12
Operator : JC/MD
Sample : 03596-01DL 5X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
001-WILLETS-PT-BLVD(JULY)DL

Quant Time: Jul 17 01:29:00 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X071423W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
QLast Update : Fri Jul 14 04:32:22 2023
Response via : Initial Calibration




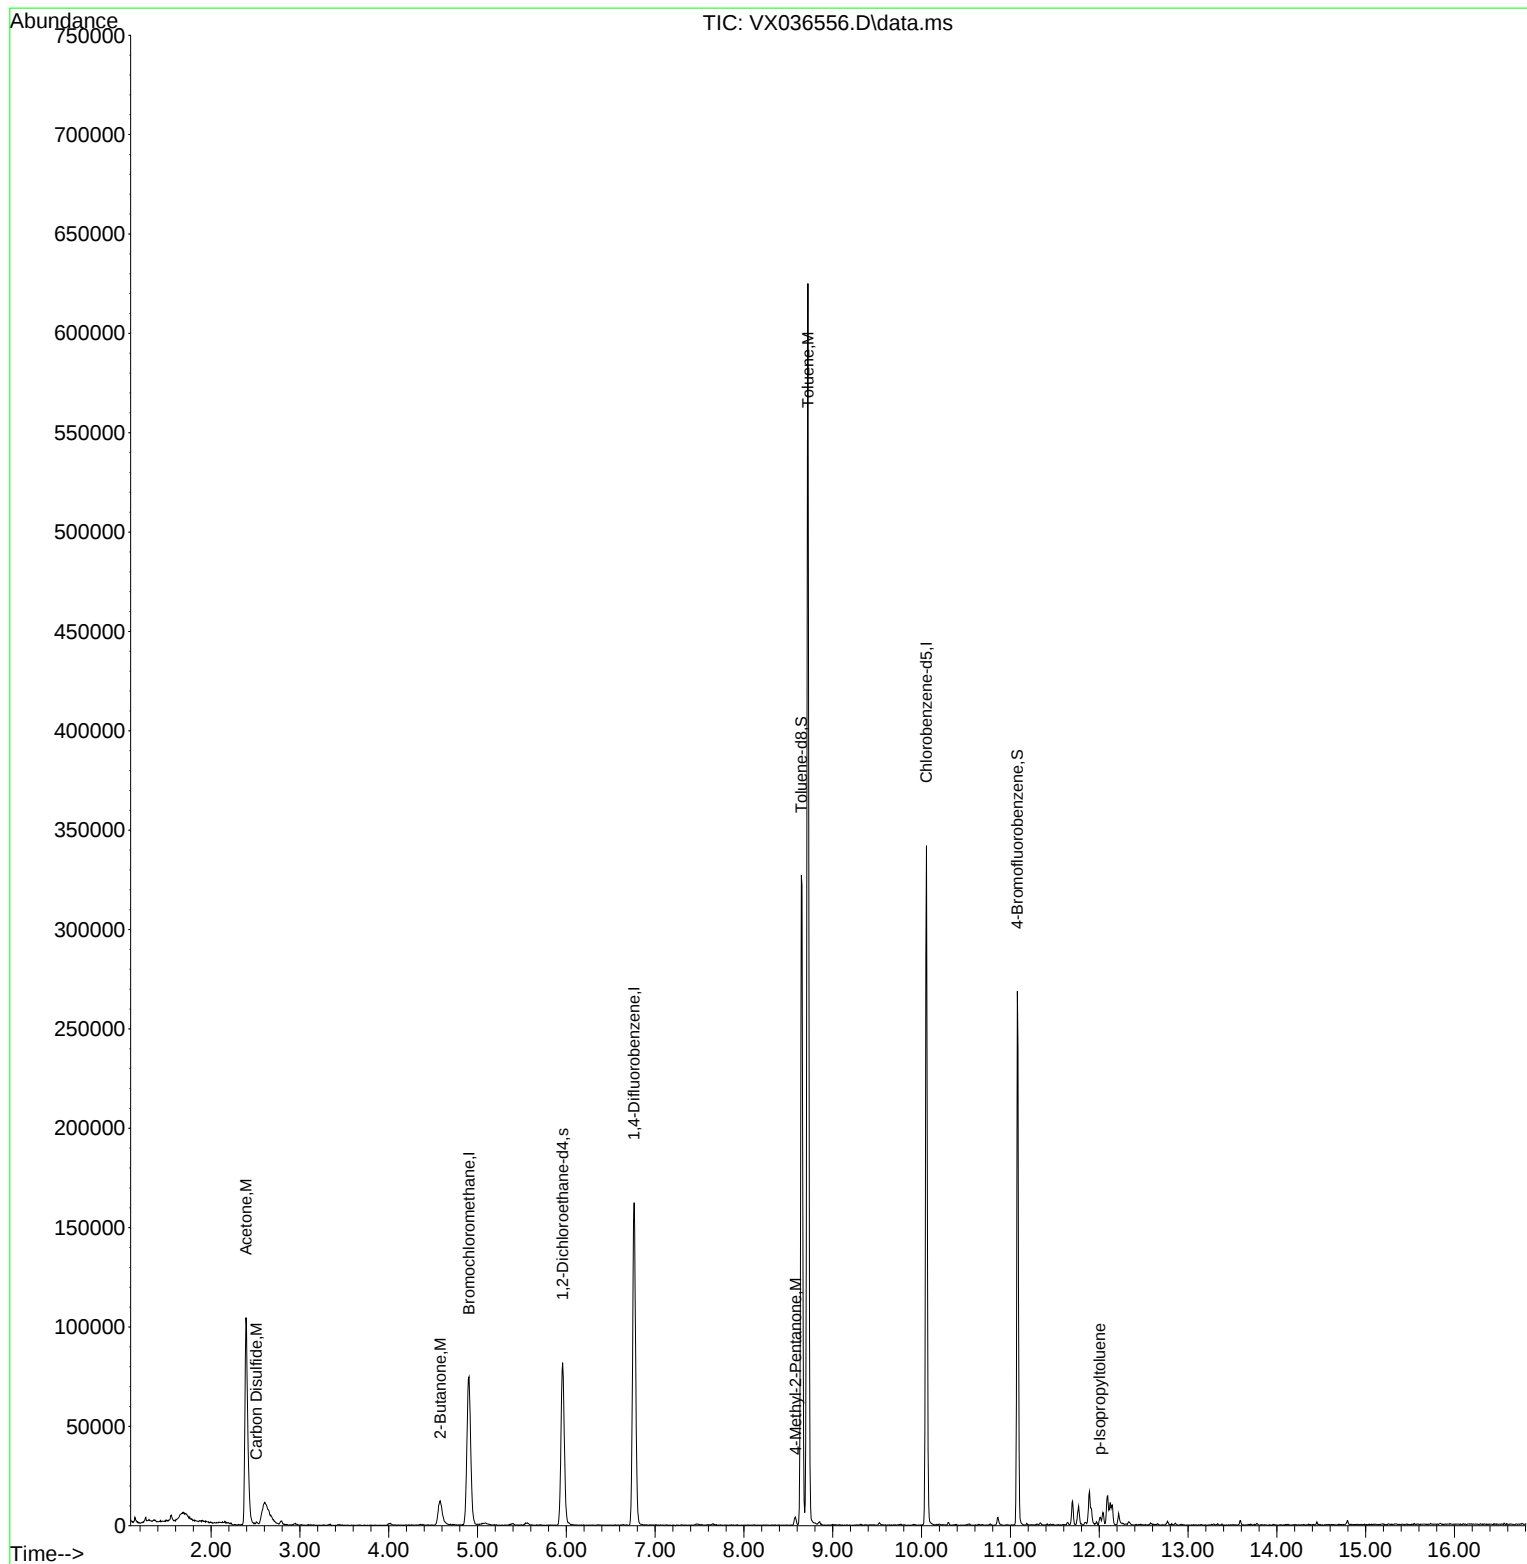


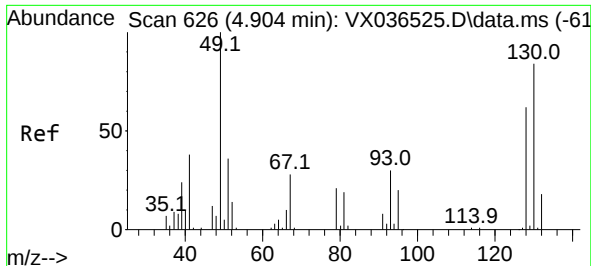

#1
Bromochloromethane
Concen: 30.000 ug/l
RT: 4.903 min Scan# 61
Delta R.T. -0.001 min
Lab File: VX036556.D
Acq: 14 Jul 2023 12:12




Instrument :
MSVOA_X
ClientSampleId :
001-WILLETS-PT-BLVD(JULY)DL


Tgt Ion:128 Resp: 31575
Ion Ratio Lower Upper
128 100
49 162.1 0.0 406.3
130 126.7 0.0 328.0

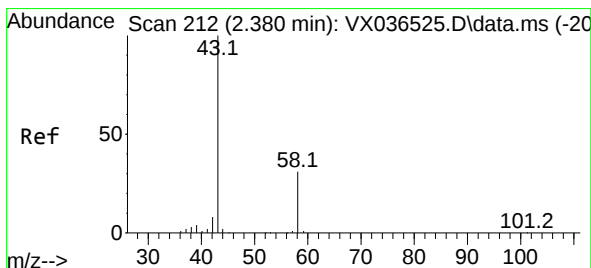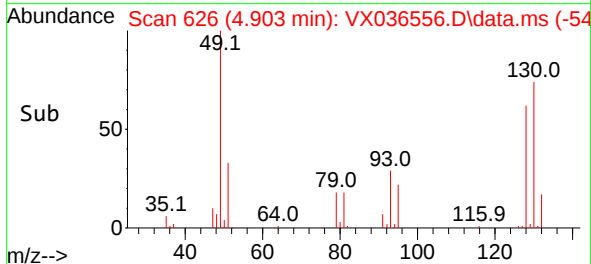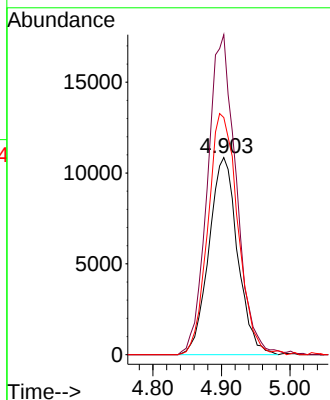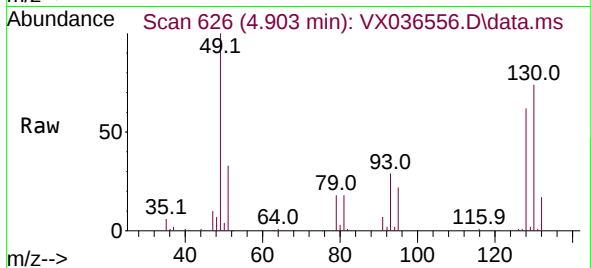

#15
Acetone
Concen: 124.998 ug/l
RT: 2.392 min Scan# 214
Delta R.T. 0.012 min
Lab File: VX036556.D
Acq: 14 Jul 2023 12:12

Tgt Ion: 58 Resp: 43083
Ion Ratio Lower Upper
58 100
43 332.2 261.0 391.4


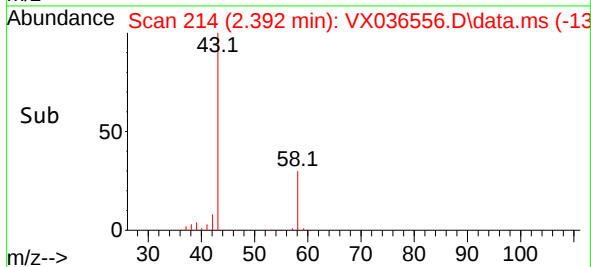
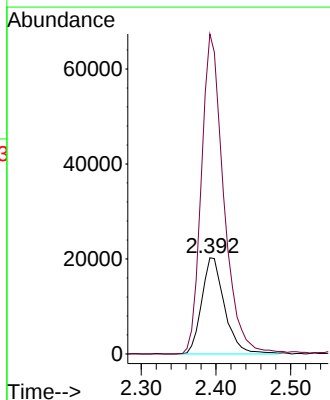
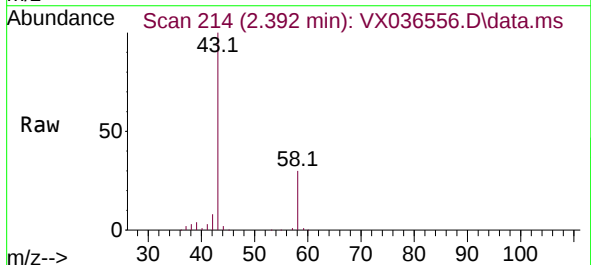


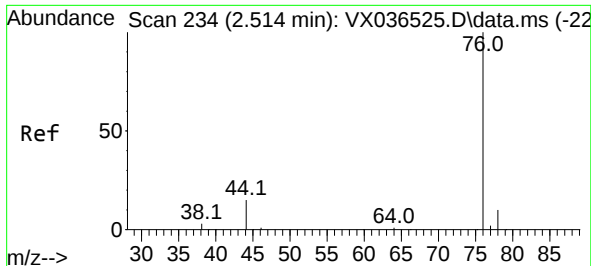

#16
Carbon Disulfide
Concen: 0.369 ug/l
RT: 2.508 min Scan# 21
Delta R.T. -0.006 min
Lab File: VX036556.D
Acq: 14 Jul 2023 12:12




Instrument :
MSVOA_X
ClientSampleId :
001-WILLETS-PT-BLVD(JULY)DL


Tgt Ion: 76 Resp: 1656
Ion Ratio Lower Upper
76 100
78 0.0 8.0 12.0#

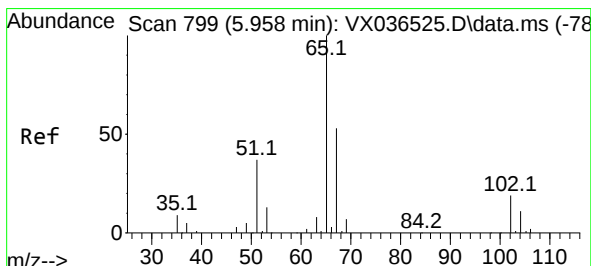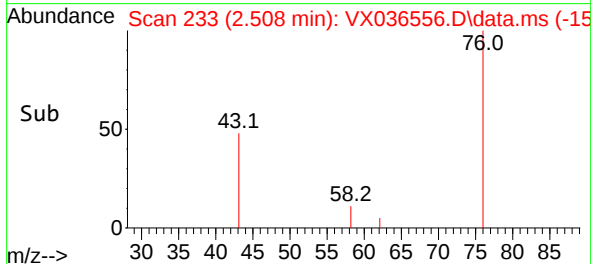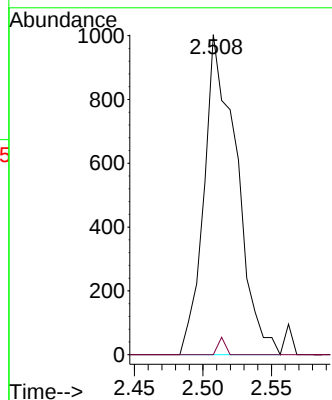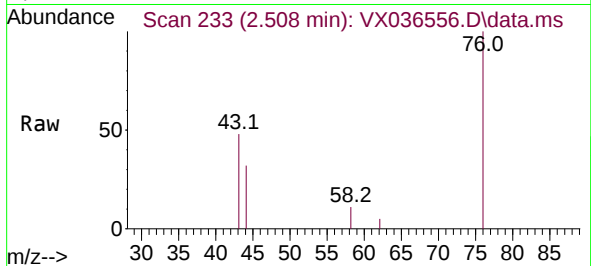

#27
1,2-Dichloroethane-d4
Concen: 29.174 ug/l
RT: 5.958 min Scan# 799
Delta R.T. -0.000 min
Lab File: VX036556.D
Acq: 14 Jul 2023 12:12

Tgt Ion: 65 Resp: 76455
Ion Ratio Lower Upper
65 100
67 52.2 42.1 63.1

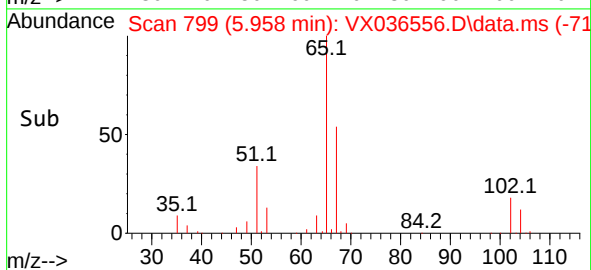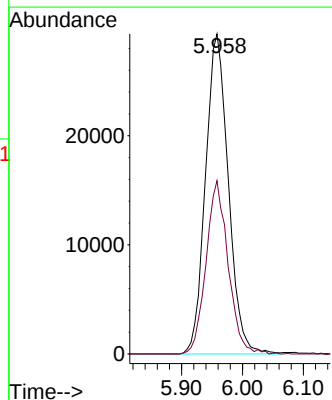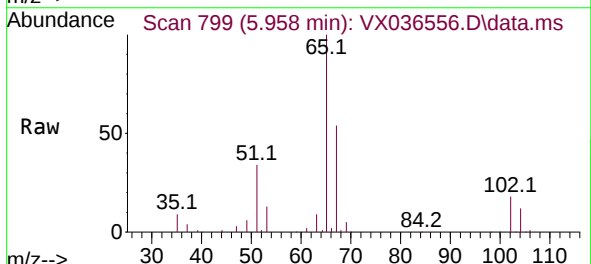

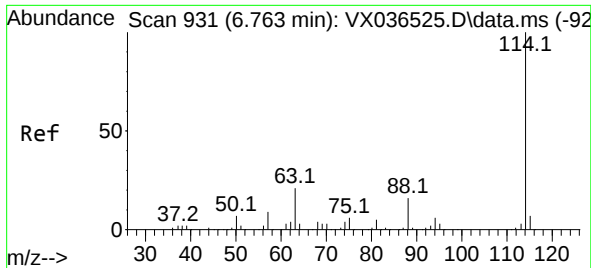

#28

1,4-Difluorobenzene

Concen: 30.000 ug/l

RT: 6.763 min Scan# 91

Delta R.T. -0.000 min

Lab File: VX036556.D

Acq: 14 Jul 2023 12:12

Instrument :

MSVOA_X

ClientSampleId :

001-WILLETS-PT-BLVD(JULY)DL





Tgt Ion:114 Resp: 165105

Ion Ratio Lower Upper

114 100

63 19.9 16.6 24.8

88 15.5 12.9 19.3

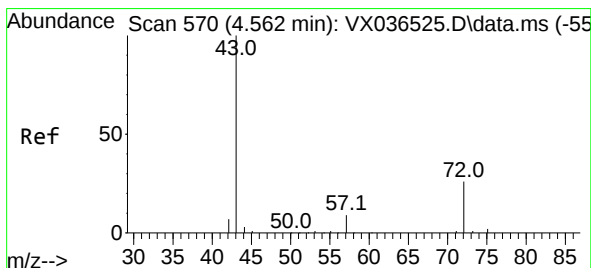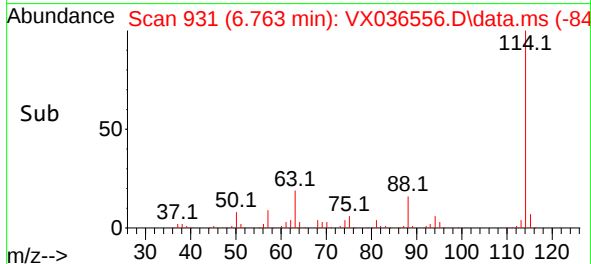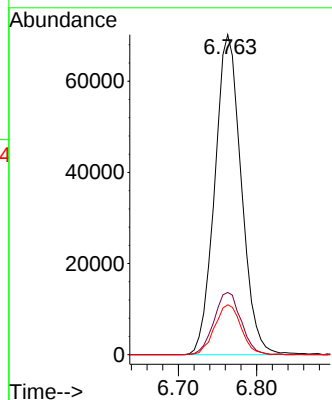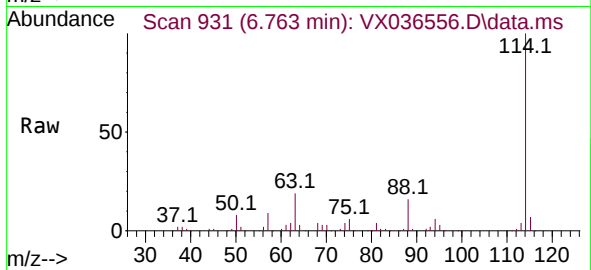

#30

2-Butanone

Concen: 8.614 ug/l

RT: 4.580 min Scan# 573

Delta R.T. 0.018 min

Lab File: VX036556.D

Acq: 14 Jul 2023 12:12




Tgt Ion: 43 Resp: 13504


Ion Ratio Lower Upper

43 100

57 4.9 6.4 9.6#

72 15.2 21.6 32.4#

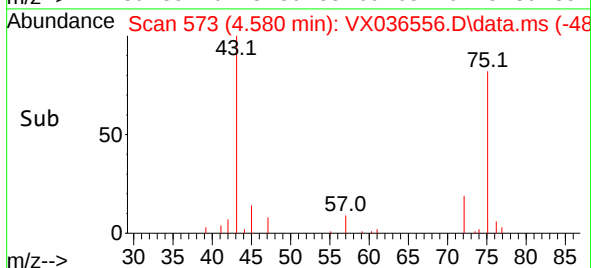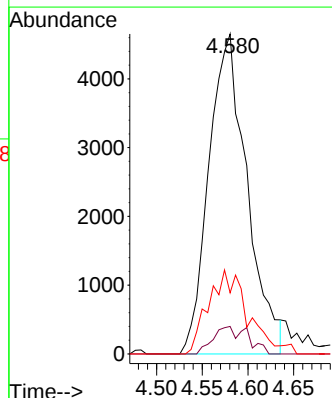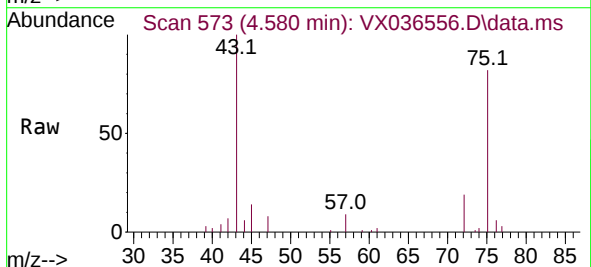

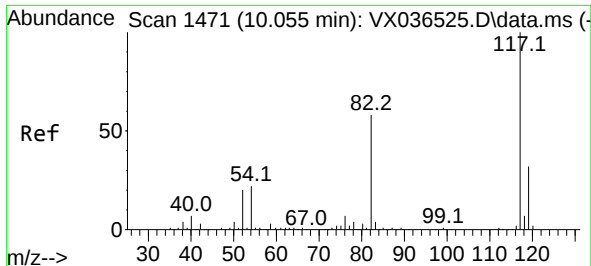

#57

Chlorobenzene-d5

Concen: 30.000 ug/l

RT: 10.055 min Scan# 1471

Delta R.T. -0.000 min

Lab File: VX036556.D

Acq: 14 Jul 2023 12:12

Instrument :

MSVOA_X

ClientSampleId :

001-WILLETS-PT-BLVD(JULY)DL





Tgt Ion:117 Resp: 148886

Ion Ratio Lower Upper

117 100

82 57.0 44.7 67.1

119 32.2 25.6 38.4

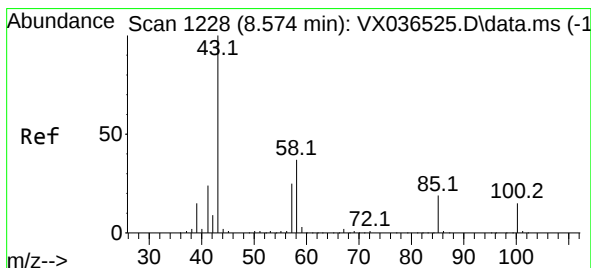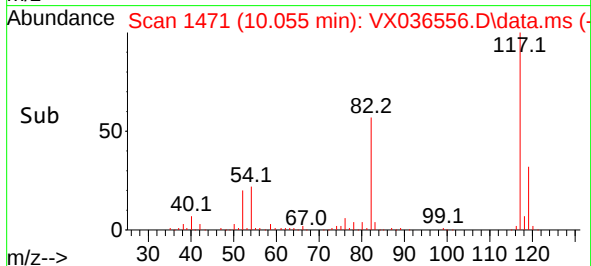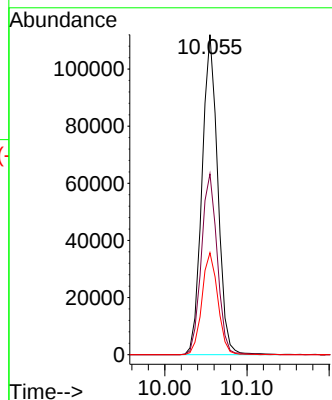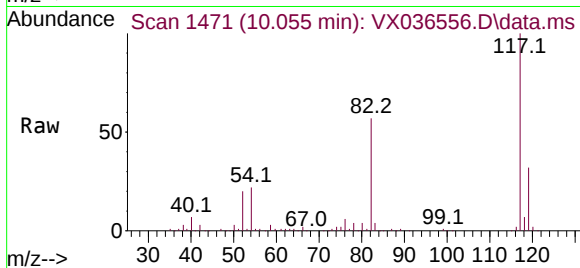

#58

4-Methyl-2-Pentanone

Concen: 0.885 ug/l

RT: 8.580 min Scan# 1229

Delta R.T. 0.006 min

Lab File: VX036556.D

Acq: 14 Jul 2023 12:12




Tgt Ion: 43 Resp: 2724


Ion Ratio Lower Upper

43 100

58 43.7 30.9 46.3

85 18.4 14.4 21.6


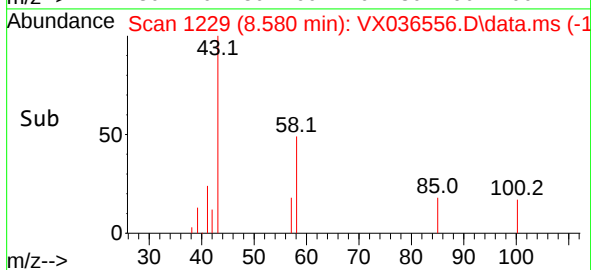
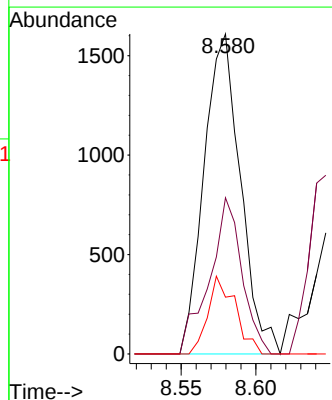
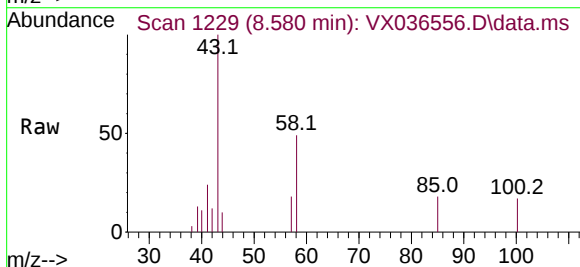


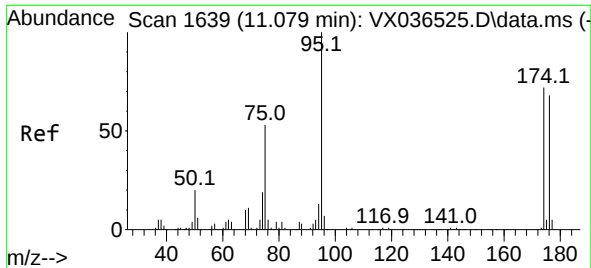

#60
4-Bromofluorobenzene
Concen: 29.269 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.000 min
Lab File: VX036556.D
Acq: 14 Jul 2023 12:12




Instrument :
MSVOA_X
ClientSampleId :
001-WILLETS-PT-BLVD(JULY)DL


Tgt Ion: 95 Resp: 70688
Ion Ratio Lower Upper
95 100
174 75.2 60.5 90.7
176 70.2 58.2 87.4

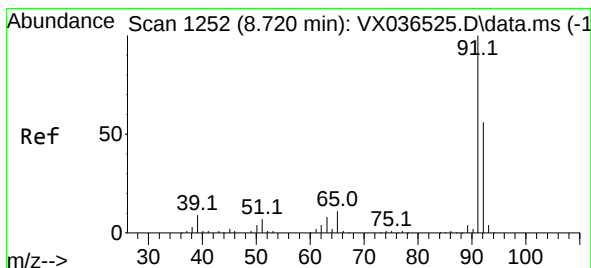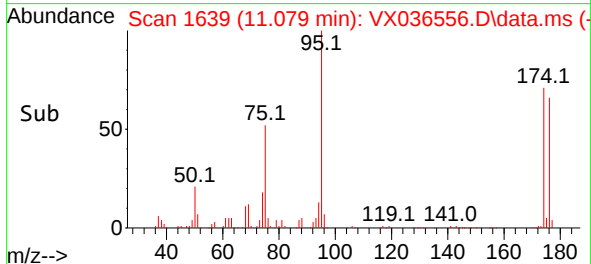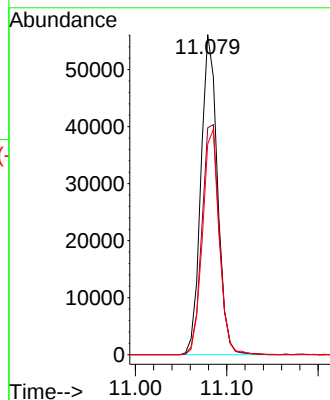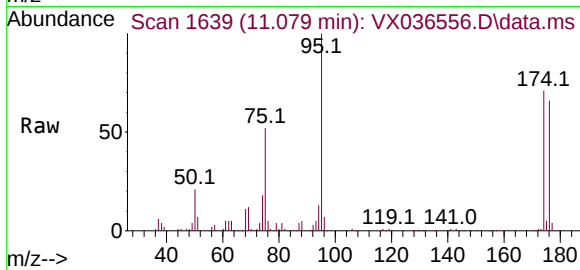

#62
Toluene
Concen: 46.488 ug/l
RT: 8.720 min Scan# 1252
Delta R.T. -0.000 min
Lab File: VX036556.D
Acq: 14 Jul 2023 12:12

Tgt Ion: 91 Resp: 388344
Ion Ratio Lower Upper
91 100
92 57.8 44.9 67.3

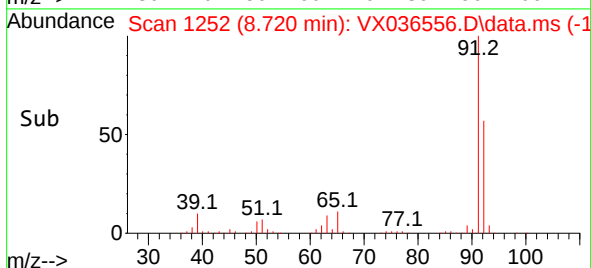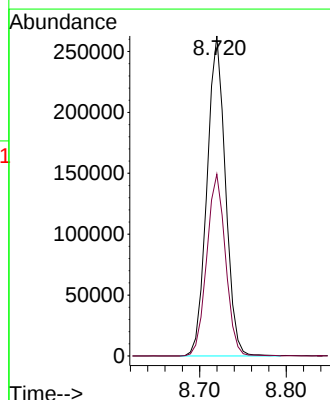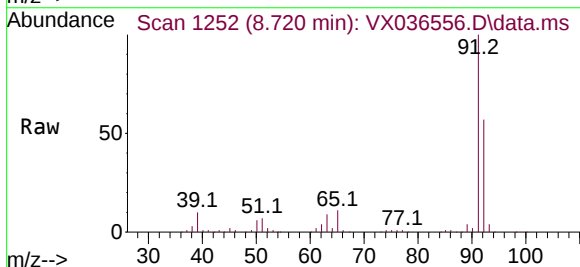

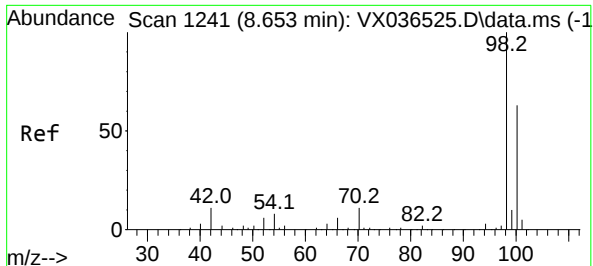

#63

Toluene-d8

Concen: 29.382 ug/l

RT: 8.647 min Scan# 11

Delta R.T. -0.006 min

Lab File: VX036556.D

Acq: 14 Jul 2023 12:12

Instrument :

MSVOA_X

ClientSampleId :





001-WILLETS-PT-BLVD(JULY)DL

Tgt Ion: 98 Resp: 201298

Ion Ratio Lower Upper

98 100

100 63.3 51.6 77.4

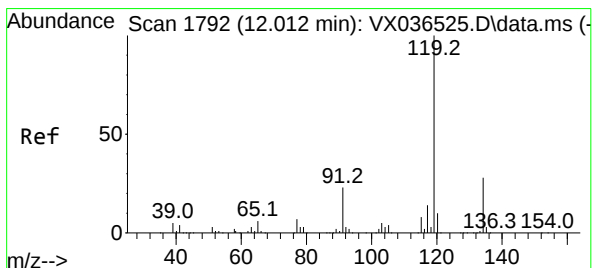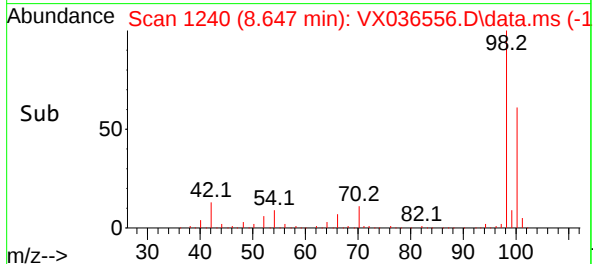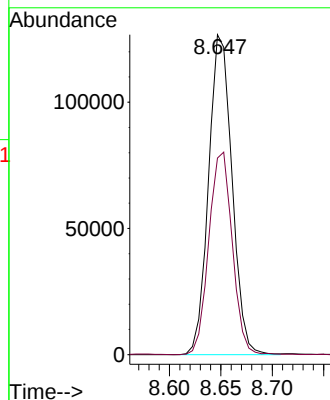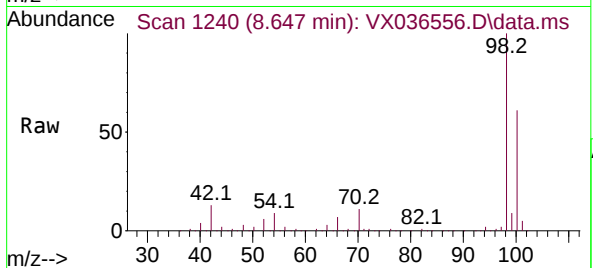

#82

p-Isopropyltoluene

Concen: 0.269 ug/l

RT: 12.006 min Scan# 1791

Delta R.T. -0.006 min

Lab File: VX036556.D

Acq: 14 Jul 2023 12:12

Tgt Ion: 119 Resp: 2012

Ion Ratio Lower Upper

119 100

134 22.3 0.0 53.2

91 20.8 0.0 49.4

