
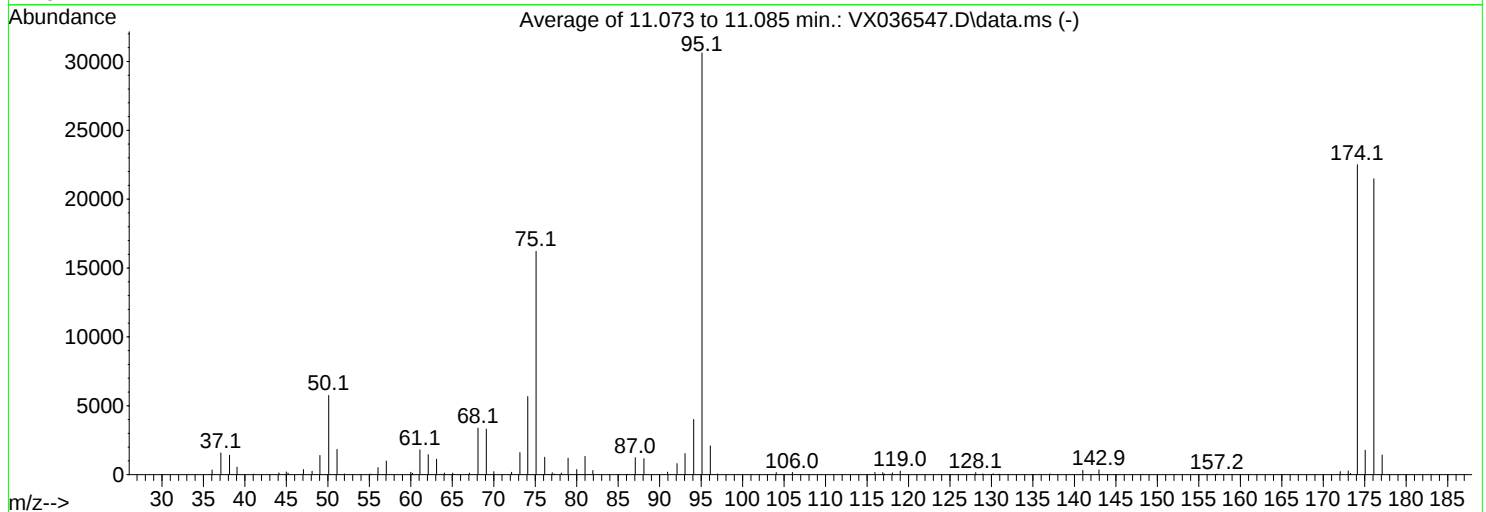


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071523\
 Data File : VX036547.D
 Acq On : 14 Jul 2023 08:21
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X071423W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Fri Jul 14 04:32:22 2023

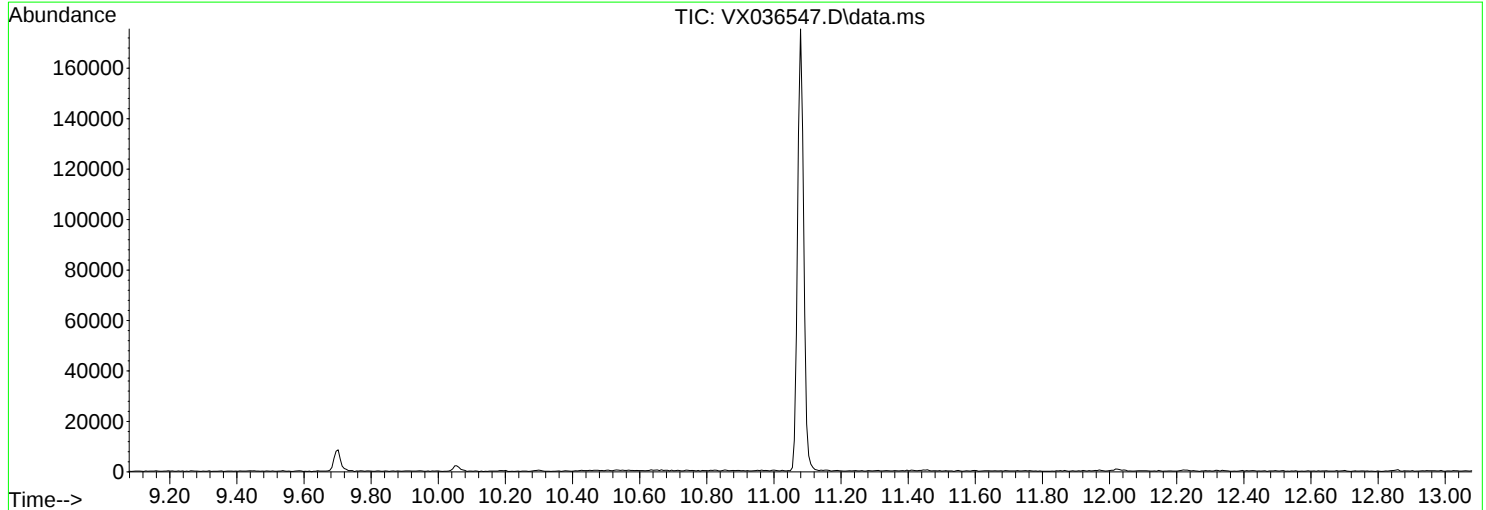

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.8	5755	PASS
75	95	30	60	52.9	16215	PASS
95	95	100	100	100.0	30624	PASS
96	95	5	9	6.8	2094	PASS
173	174	0.00	2	1.2	263	PASS
174	95	50	100	73.5	22504	PASS
175	174	5	9	7.9	1780	PASS
176	174	95	101	95.4	21480	PASS
177	176	5	9	6.6	1428	PASS