
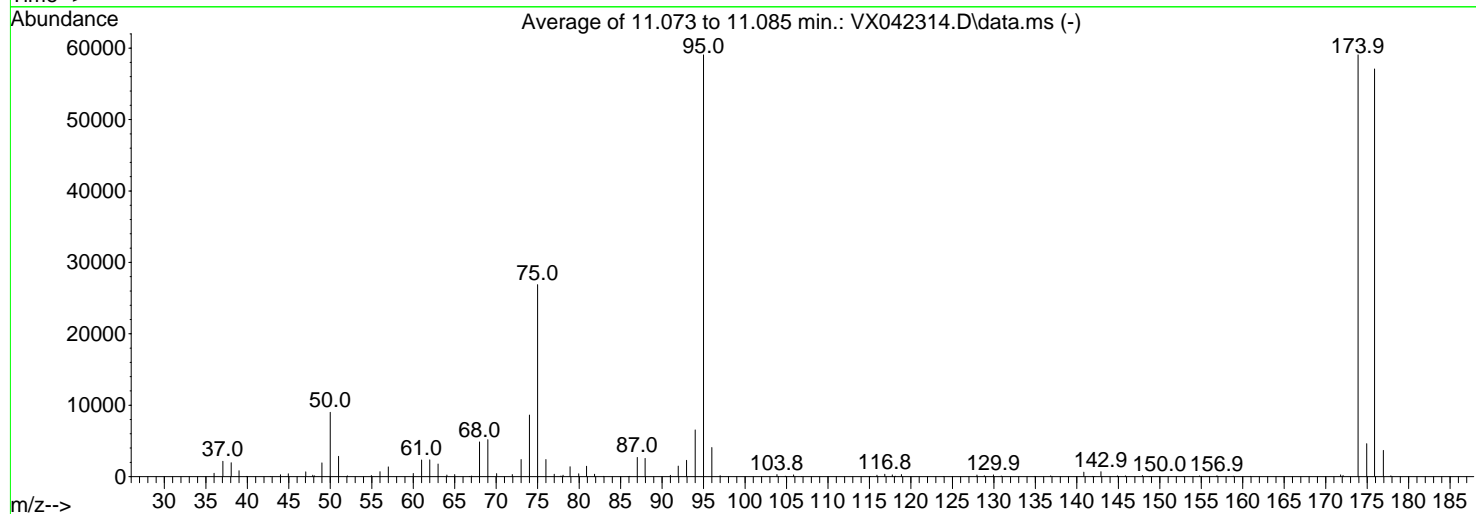


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071524\
 Data File : VX042314.D
 Acq On : 15 Jul 2024 08:35
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X061824W.M
 Title : SW846 8260
 Last Update : Fri Jun 21 23:51:58 2024

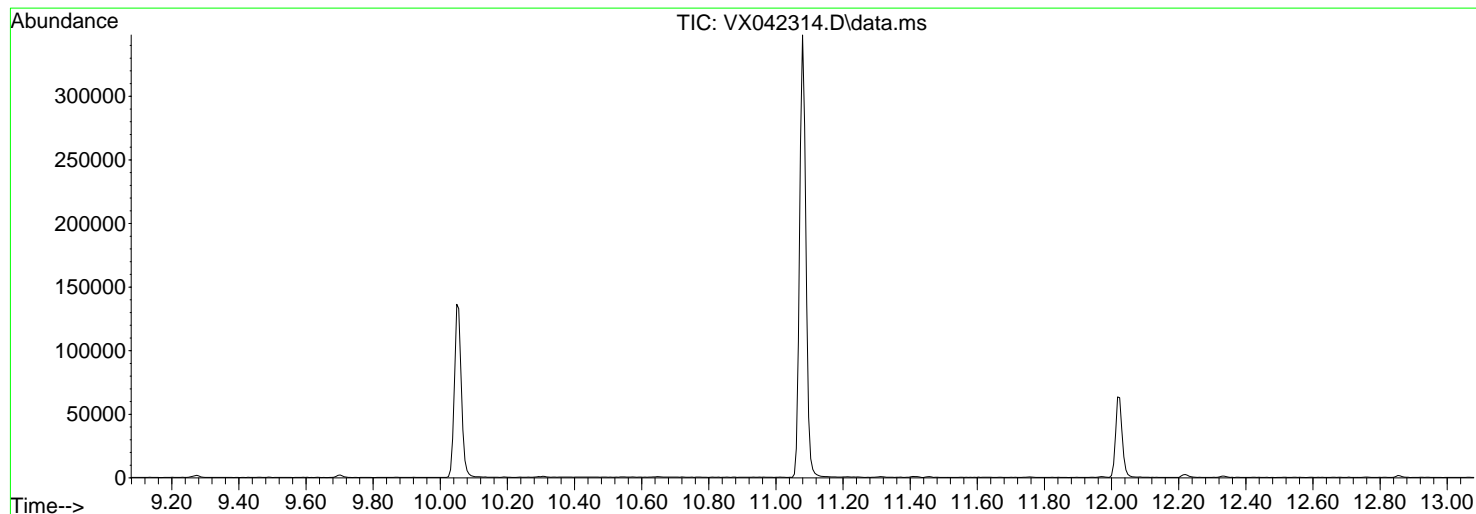

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.3	9010	PASS
75	95	30	60	45.5	26877	PASS
95	95	100	100	100.0	59061	PASS
96	95	5	9	6.9	4077	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	100.0	59059	PASS
175	174	5	9	7.8	4614	PASS
176	174	95	101	96.6	57077	PASS
177	176	5	9	6.4	3667	PASS