


Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX071618\
Data File : VX003388.D
Acq On : 16 Jul 2018 09:38
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X071618W.M
Title : SW846 8260
Last Update : Mon Jul 16 13:15:28 2018

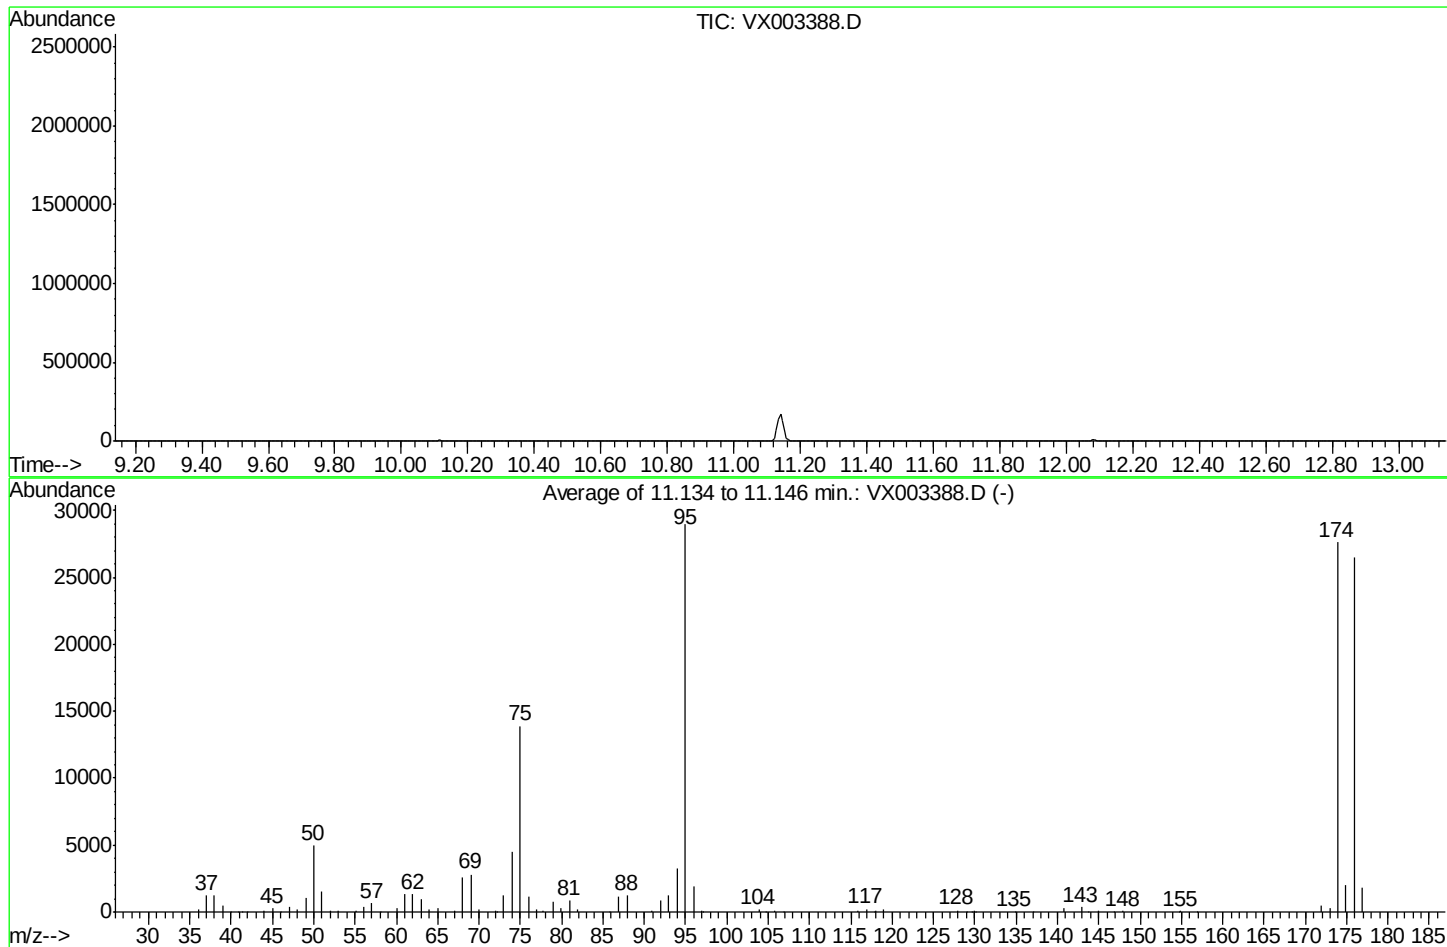

AutoFind: Scans 1730, 1731, 1732; Background Corrected with Scan 1723

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.1	4943	PASS
75	95	30	60	48.0	13897	PASS
95	95	100	100	100.0	28957	PASS
96	95	5	9	6.6	1898	PASS
173	174	0.00	2	1.0	268	PASS
174	95	50	100	95.4	27626	PASS
175	174	5	9	7.4	2038	PASS
176	174	95	101	95.7	26448	PASS
177	176	5	9	6.7	1772	PASS