


trans-1,4-Dichloro-2-butene

Response Ratio

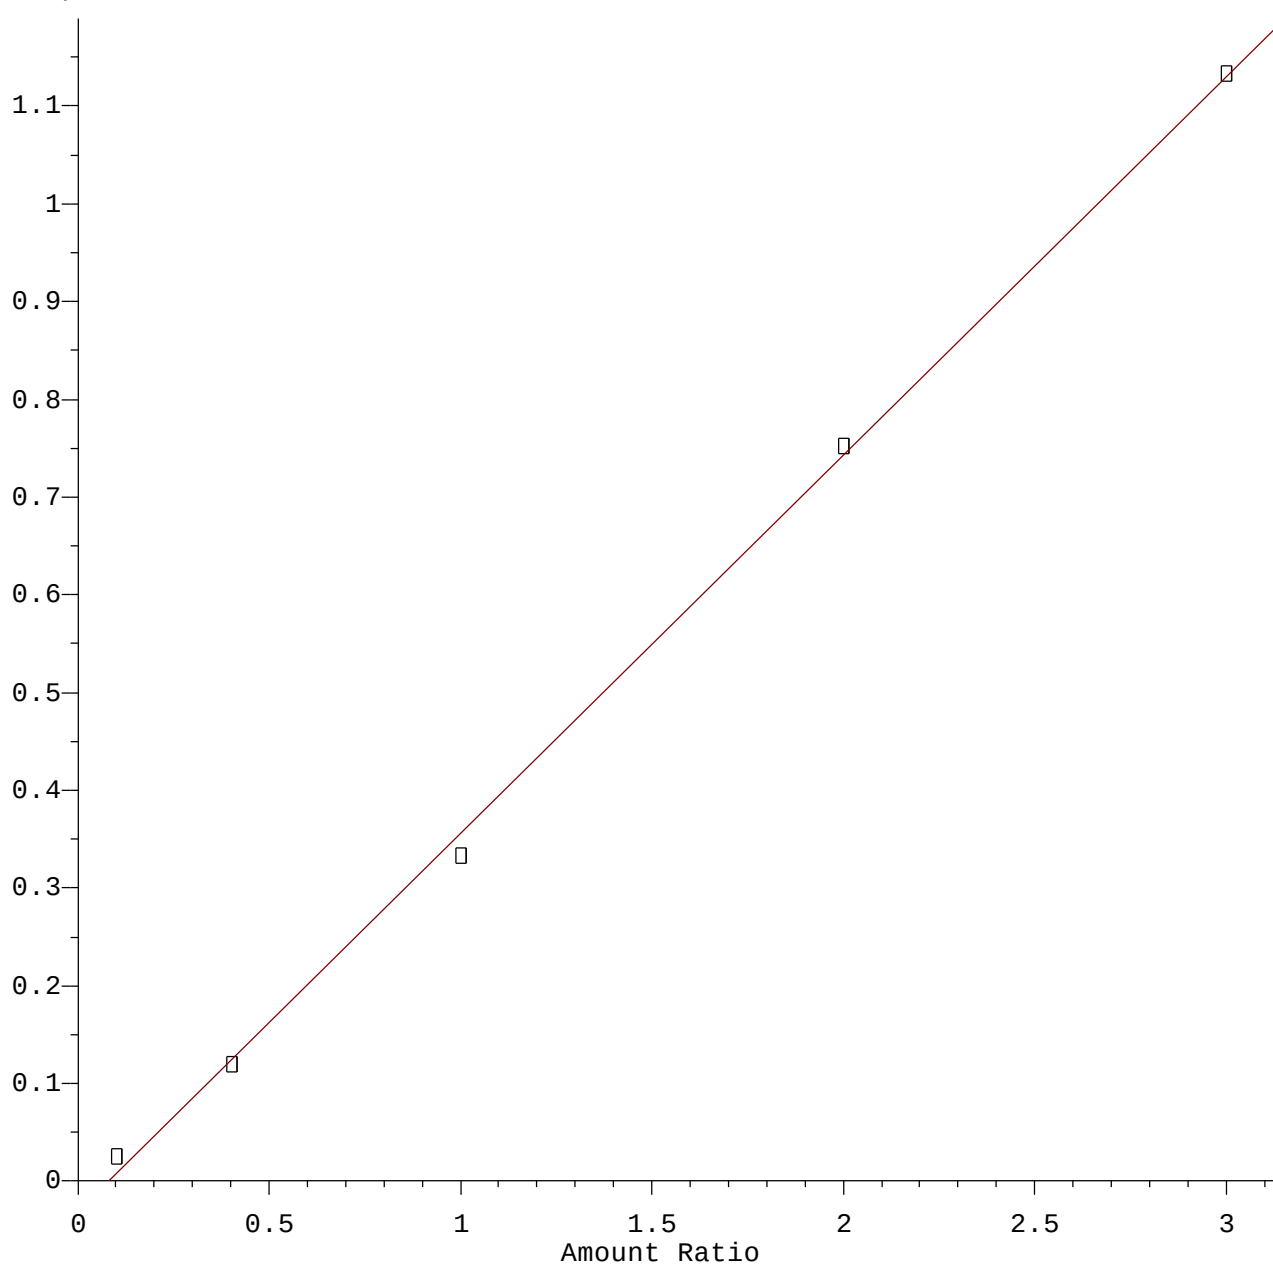


Resp Ratio = $3.87 \times 10^{-1} \times \text{Amt} - 3.08 \times 10^{-2}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X071619W.M
Calibration Table Last Updated: Wed Jul 24 05:39:23 2019


Dichlorodifluoromethane

Response Ratio

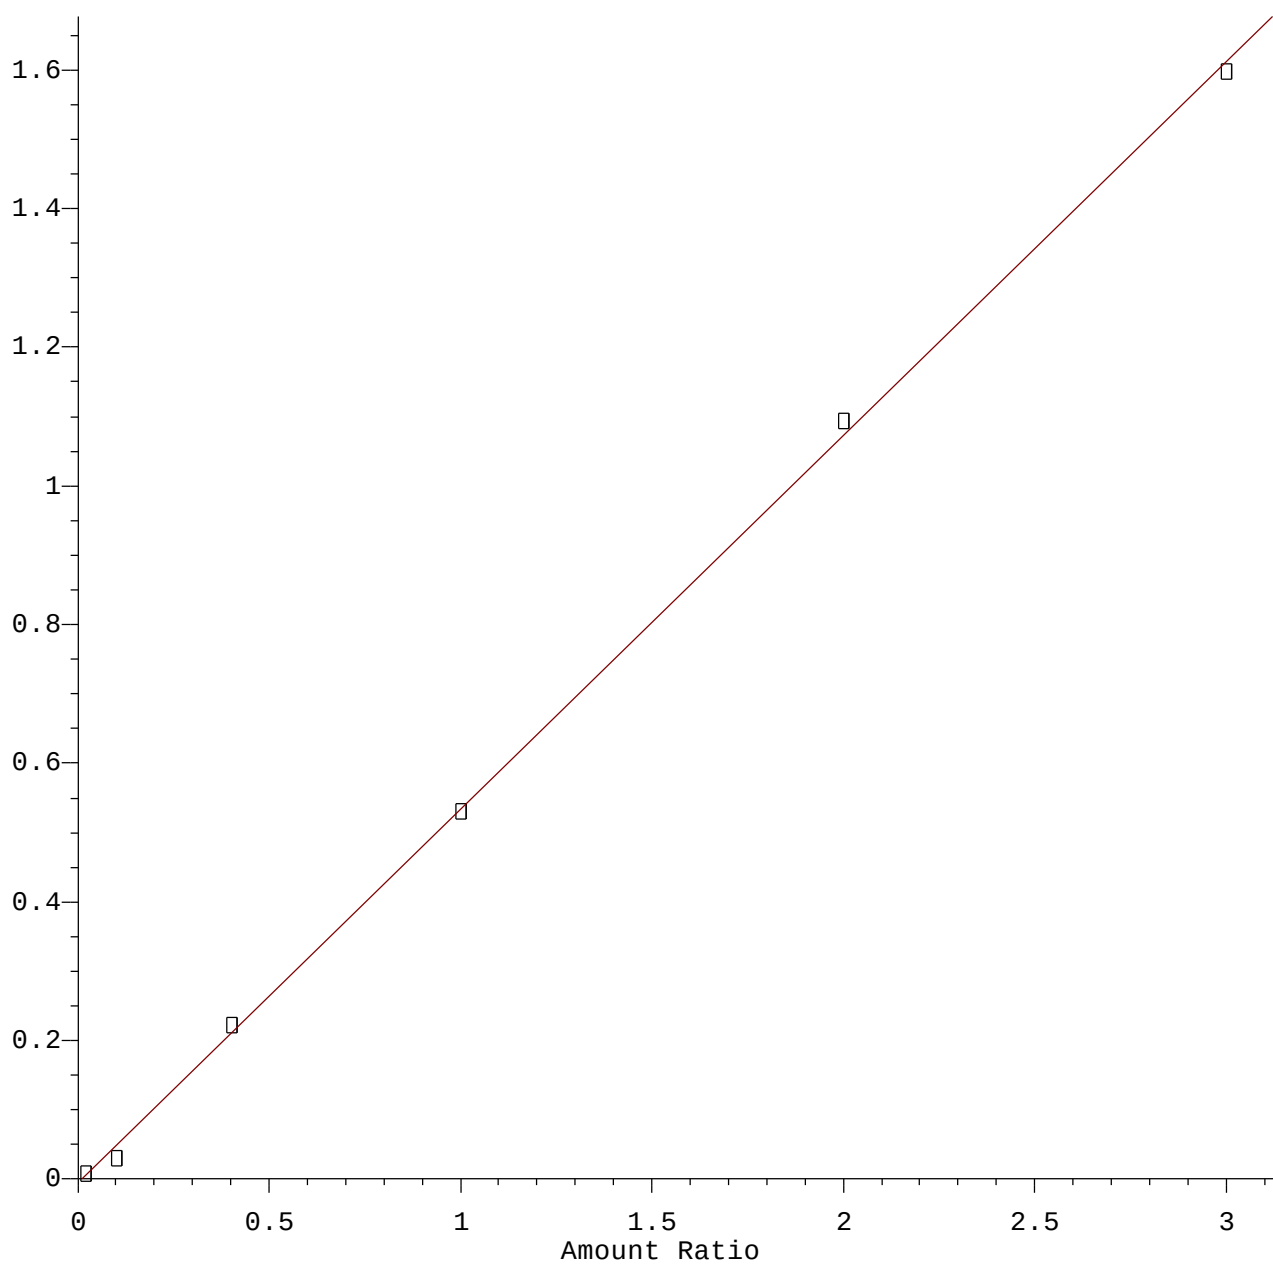


Resp Ratio = $5.39 \times 10^{-1} \times \text{Amt} - 5.89 \times 10^{-3}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X071619W.M
Calibration Table Last Updated: Wed Jul 24 05:39:23 2019

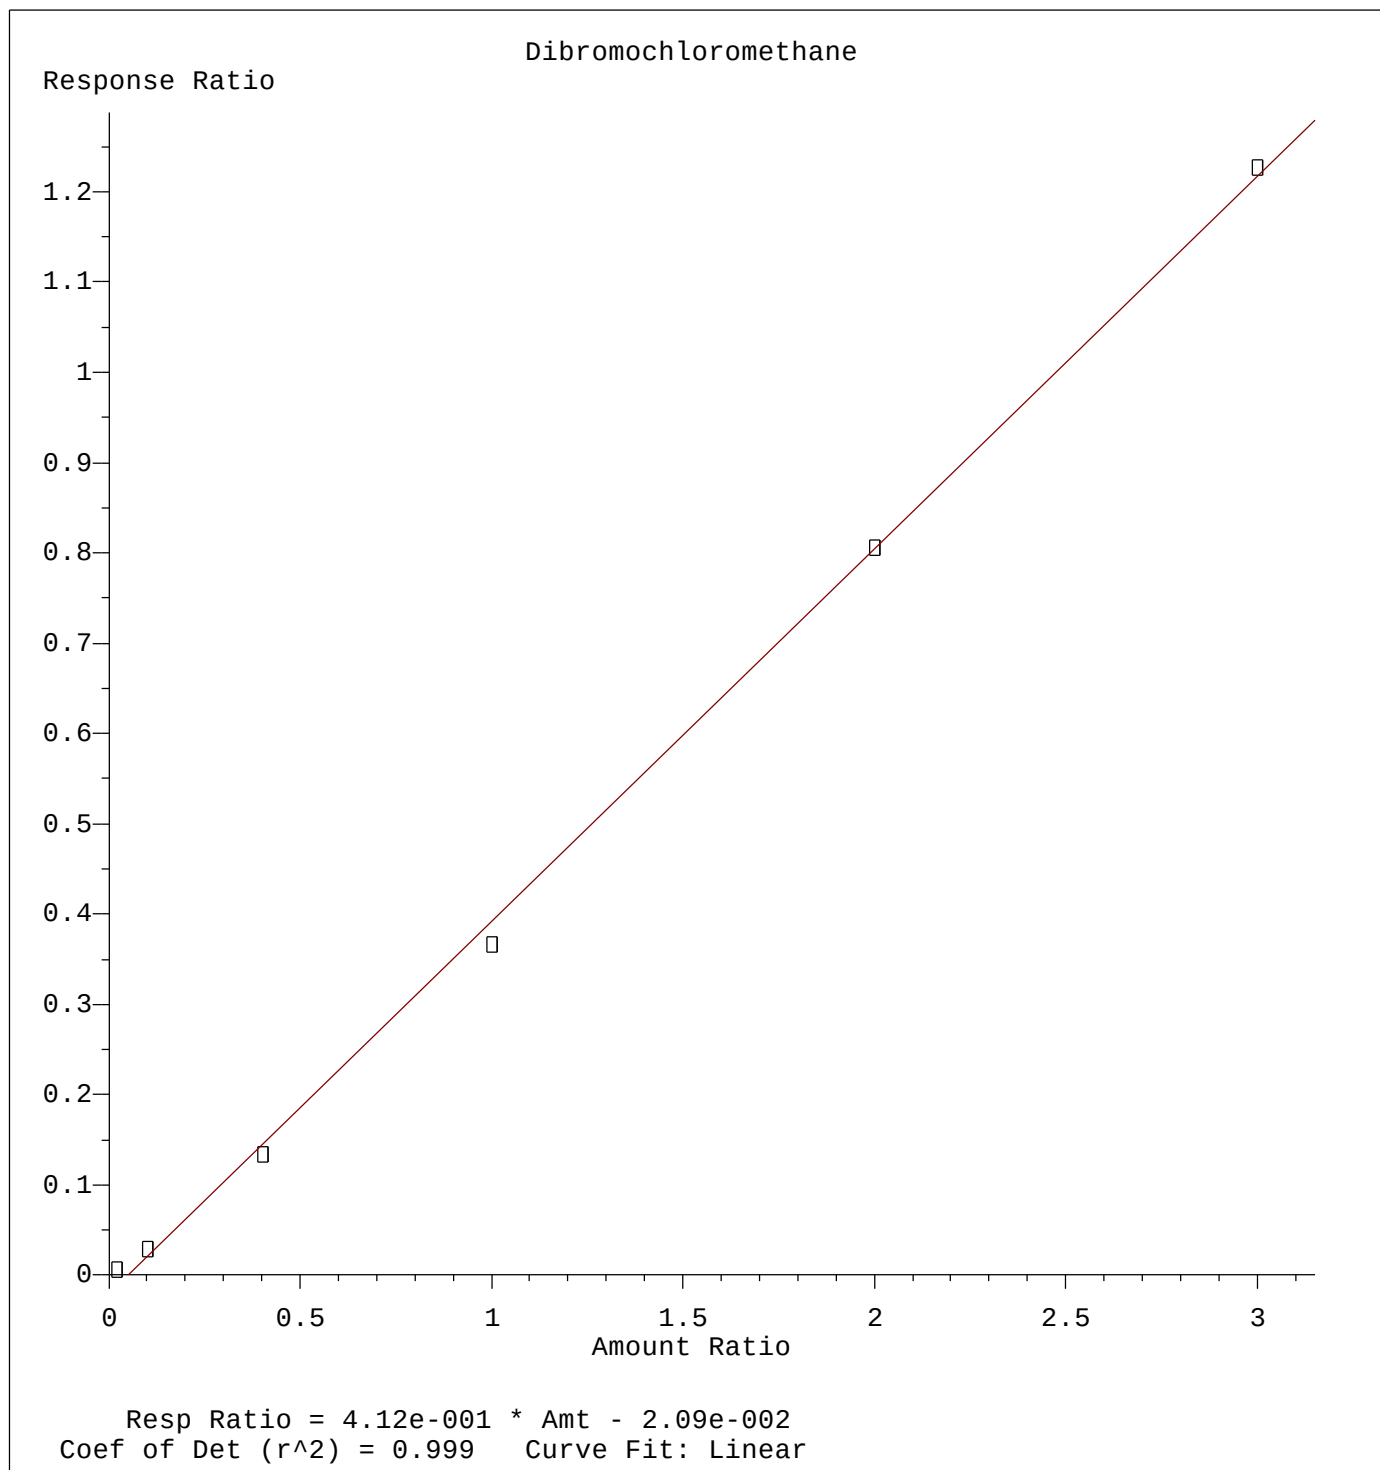

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X071619W.M
Calibration Table Last Updated: Wed Jul 24 05:39:23 2019

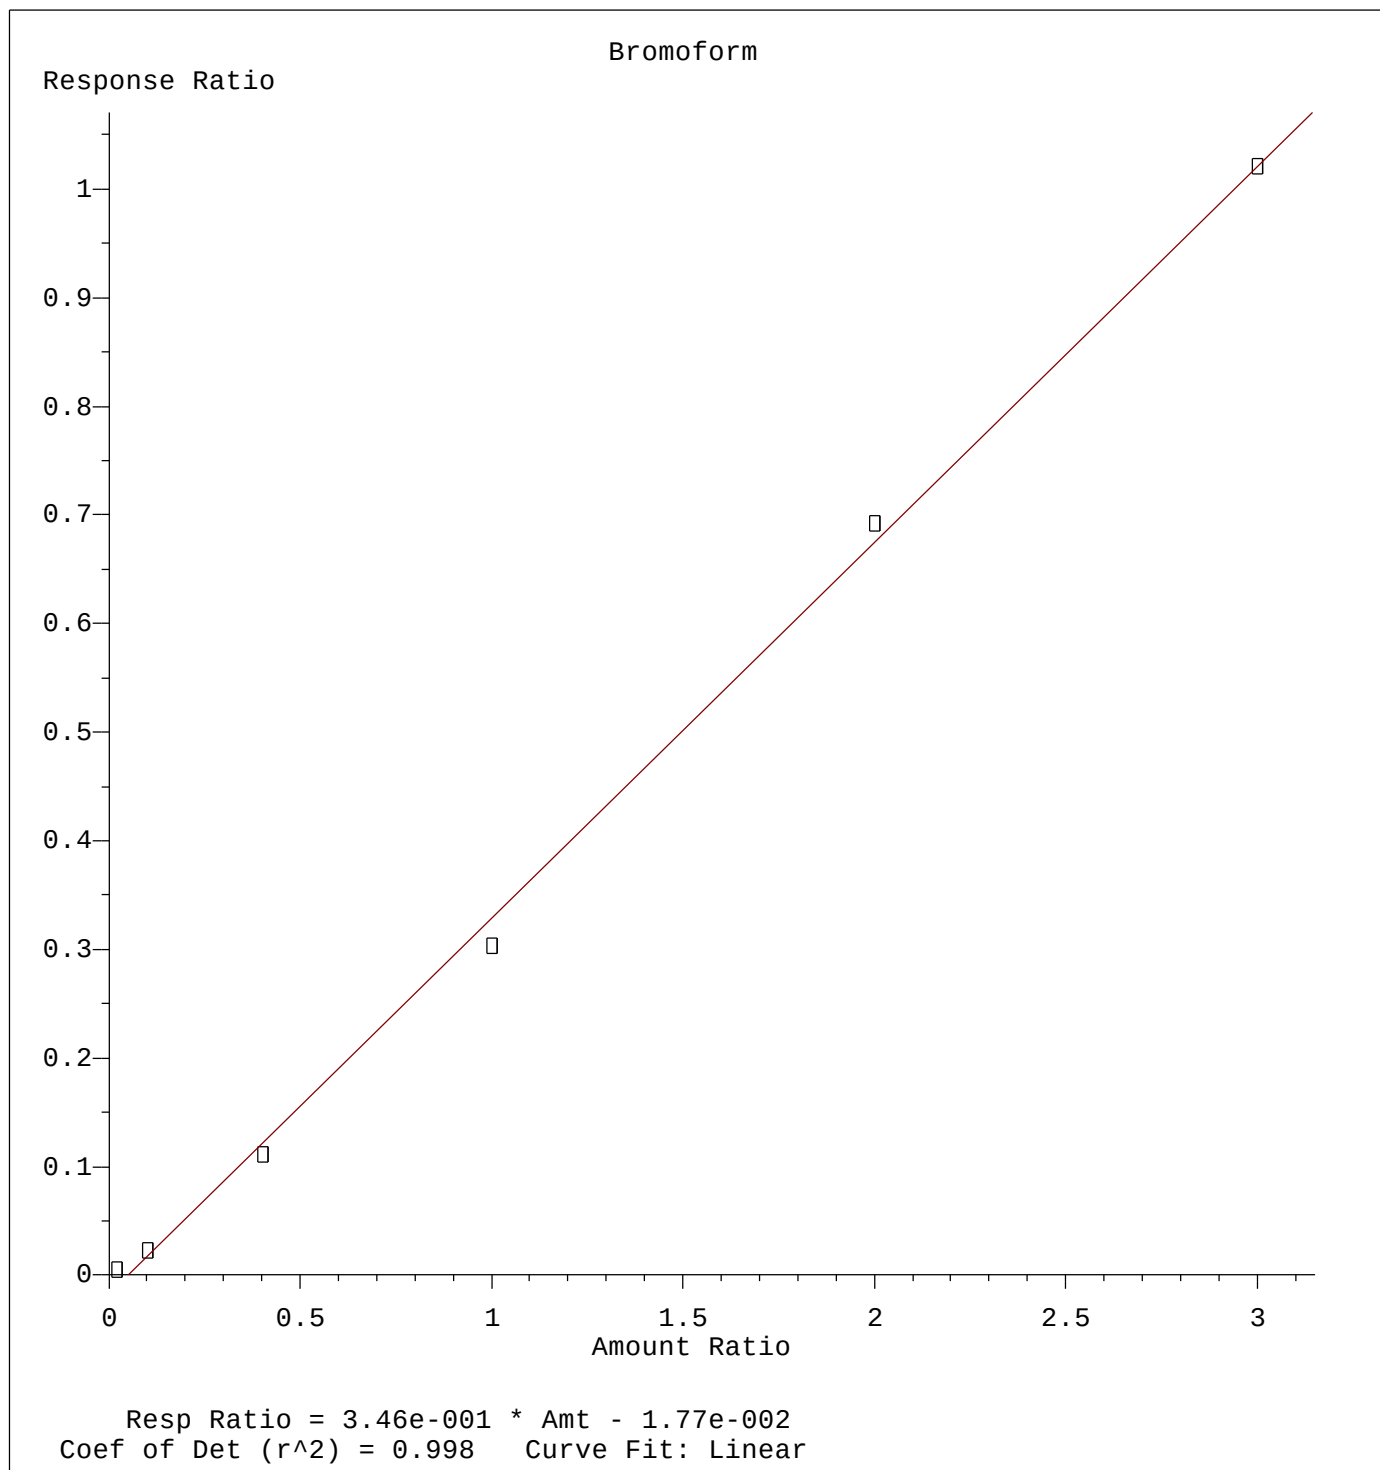

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X071619W.M
Calibration Table Last Updated: Wed Jul 24 05:39:23 2019