

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX071619\
 Data File : VX010906.D
 Acq On : 16 Jul 2019 14:08
 Operator : JC/SP
 Sample : VX0716WBL01
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0716WBL01

Quant Time: Jul 17 05:12:13 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X071619W.M
 Quant Title : SW846 8260
 QLast Update : Wed Jul 17 04:37:55 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.66	168	240442	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.85	114	372718	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.11	117	337827	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.08	152	152618	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	6.06	65	125448	49.04	ug/l	0.00
Spiked Amount						
			Recovery	=	98.08%	
35) Dibromofluoromethane	5.49	113	117737	49.77	ug/l	0.00
Spiked Amount						
			Recovery	=	99.54%	
50) Toluene-d8	8.71	98	445814	50.24	ug/l	0.00
Spiked Amount						
			Recovery	=	100.48%	
62) 4-Bromofluorobenzene	11.13	95	152771	46.84	ug/l	0.00
Spiked Amount						
			Recovery	=	93.68%	


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX071619\
Data File : VX010906.D
Acq On : 16 Jul 2019 14:08
Operator : JC/SP
Sample : VX0716WBL01
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0716WBL01

Quant Time: Jul 17 05:12:13 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X071619W.M
Quant Title : SW846 8260
QLast Update : Wed Jul 17 04:37:55 2019
Response via : Initial Calibration

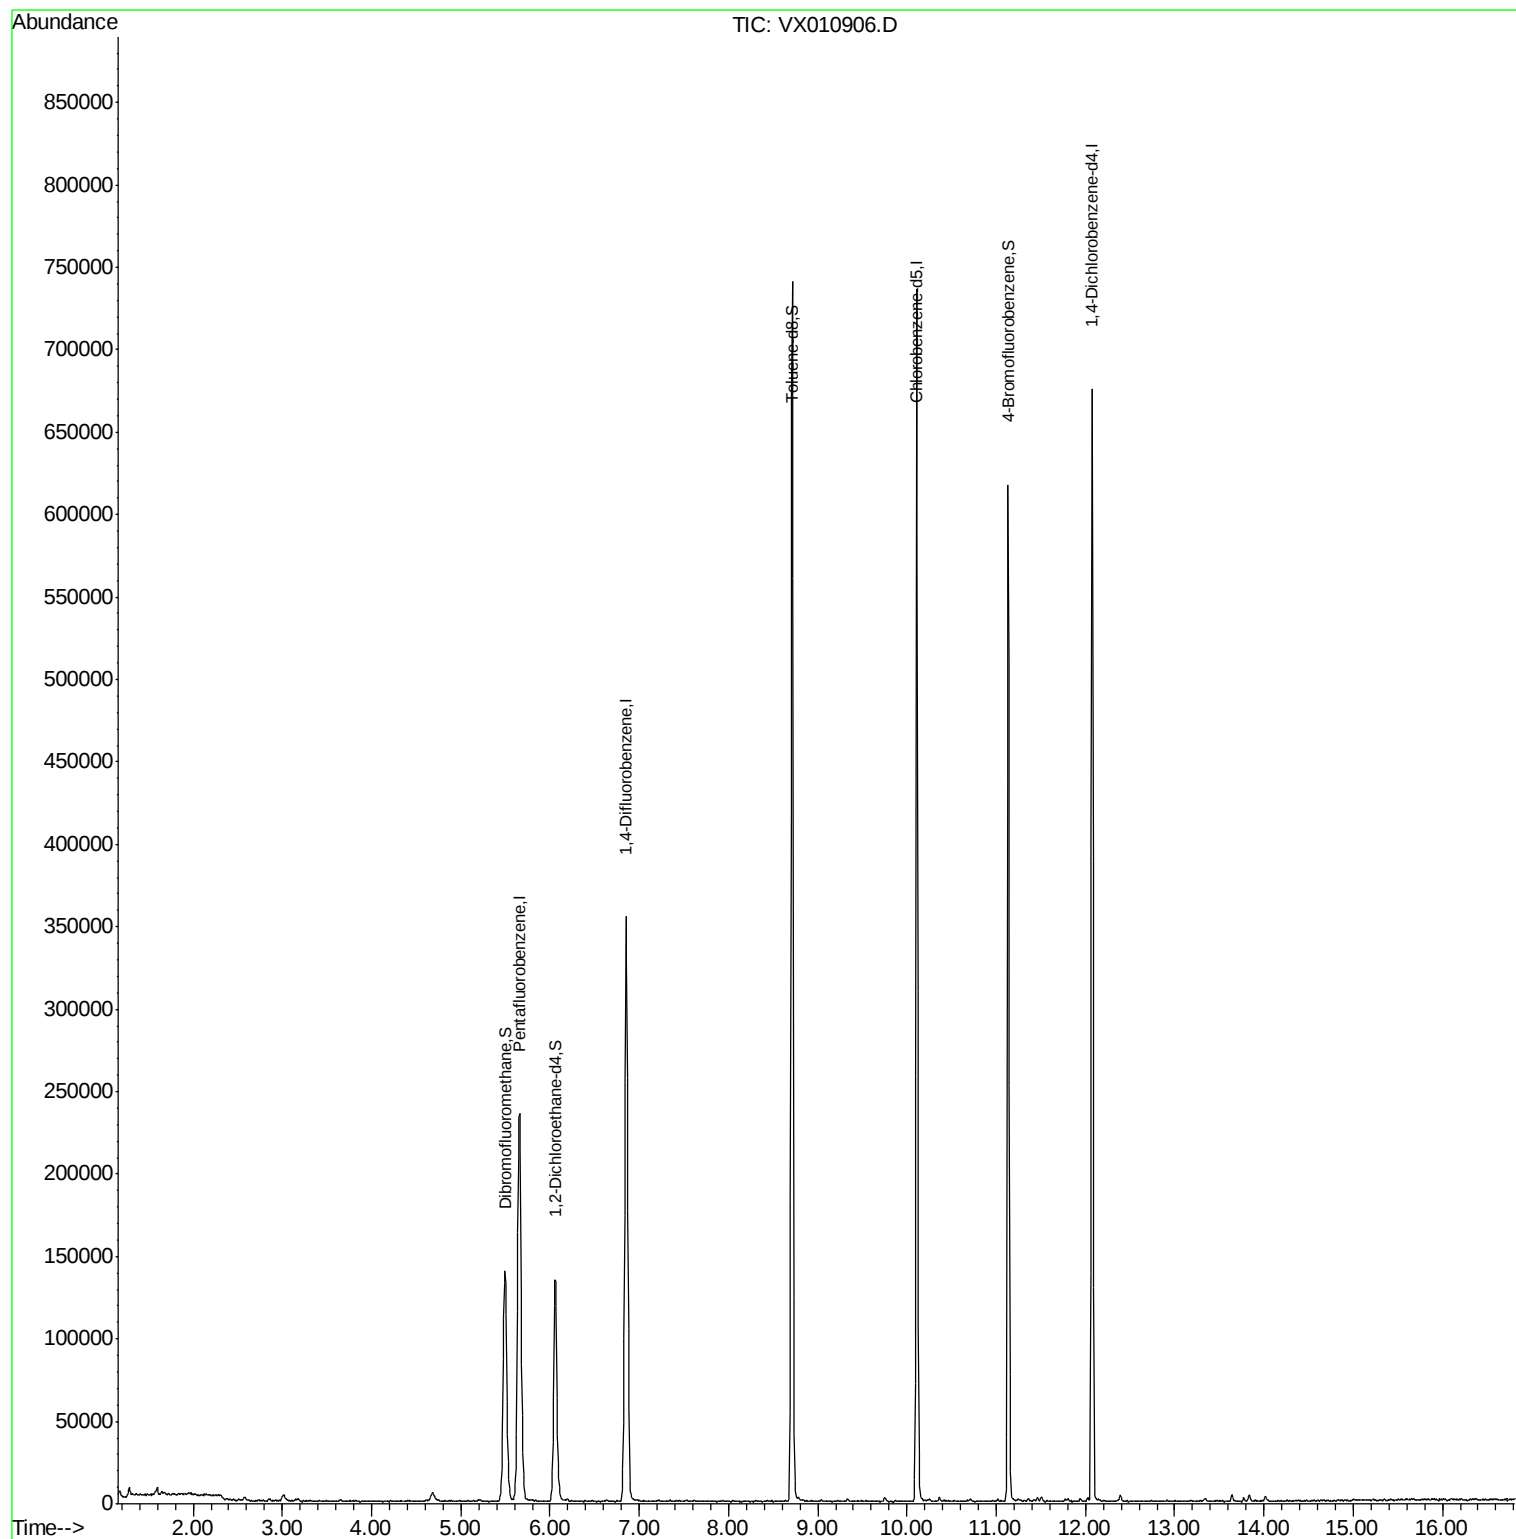

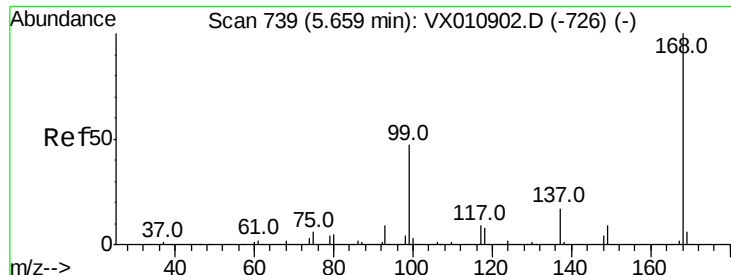

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.66 min Scan# 739

Delta R.T. -0.00 min

Lab File: VX010906.D

Acq: 16 Jul 2019 14:08

Instrument :

MSVOA_X

ClientSampleId :


VX0716WBL01

Tot Ion:168 Resp: 240442

Ion Ratio Lower Upper




168 100

99 48.0 37.6 56.4

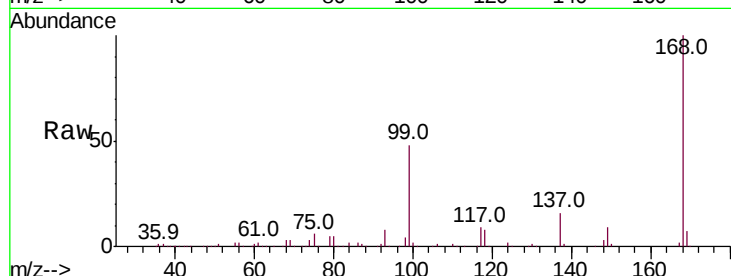

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

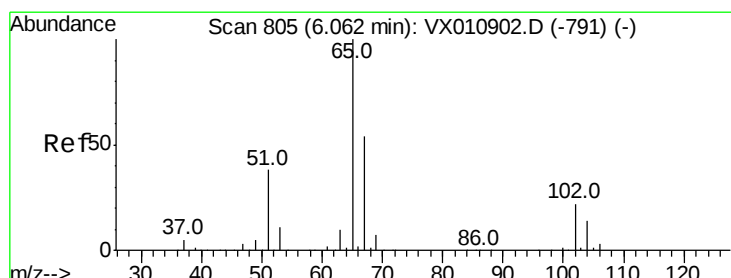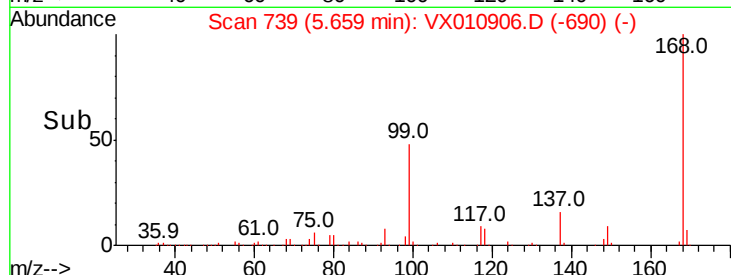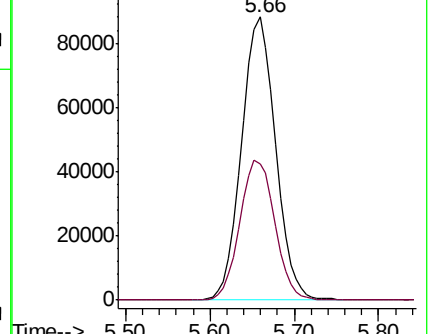

#33

1,2-Dichloroethane-d4

Concen: 49.043 ug/l

RT: 6.06 min Scan# 805

Delta R.T. -0.00 min

Lab File: VX010906.D


Acq: 16 Jul 2019 14:08

Tgt Ion: 65 Resp: 125448

Ion Ratio Lower Upper



65 100


67 53.7 0.0 107.8

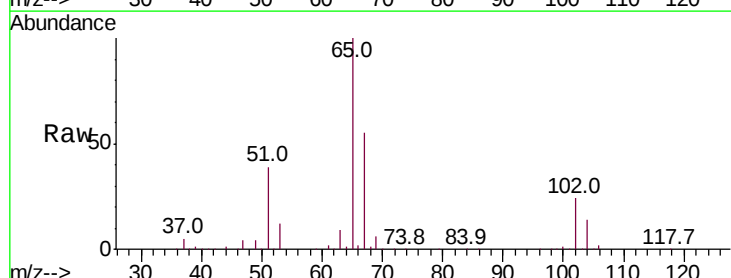

Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

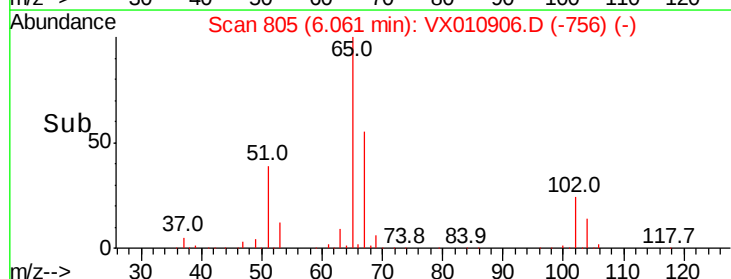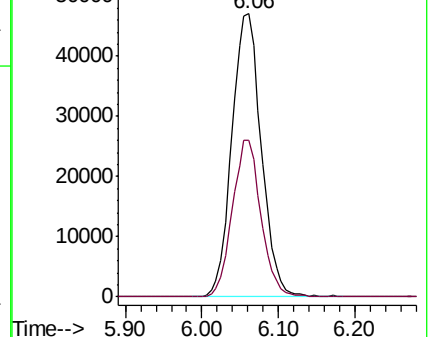

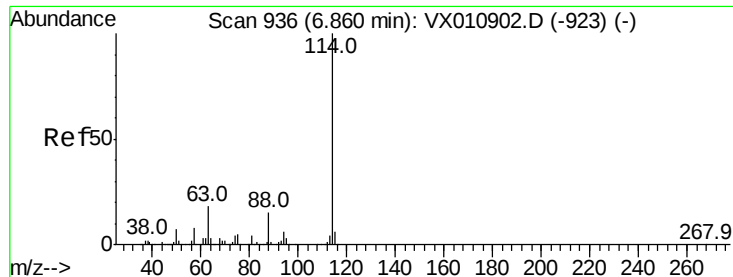

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.85 min Scan# 935

Delta R.T. -0.01 min

Lab File: VX010906.D

Acq: 16 Jul 2019 14:08

Instrument :

MSVOA_X

ClientSampleId :

VX0716WBL01


Tot Ion:114 Resp: 372718

Ion Ratio Lower Upper

114 100

63 19.1 0.0 35.6




88 15.5 0.0 29.8

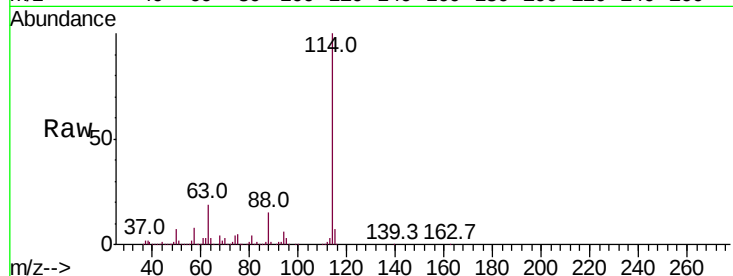

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

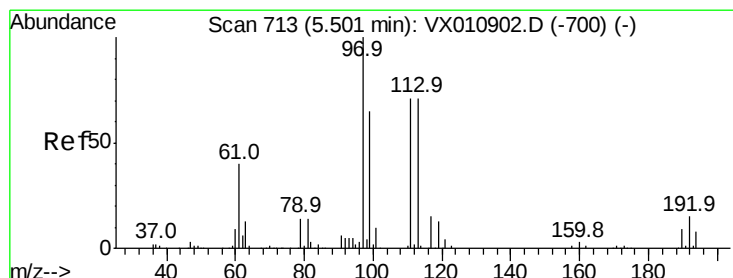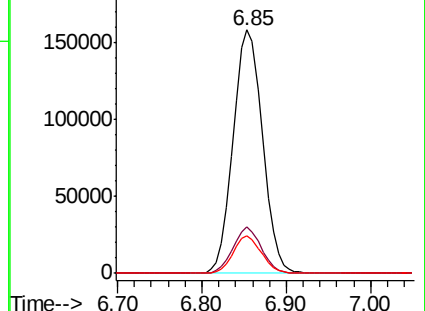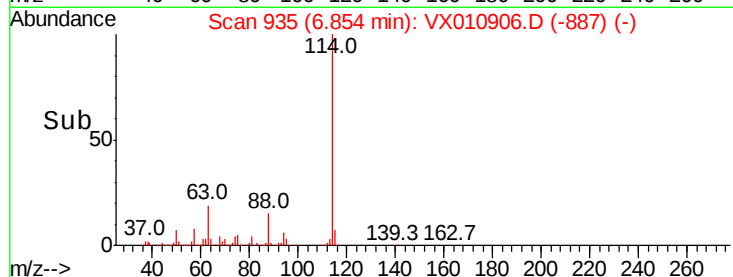

#35

Dibromofluoromethane

Concen: 49.768 ug/l

RT: 5.49 min Scan# 712

Delta R.T. -0.01 min

Lab File: VX010906.D

Acq: 16 Jul 2019 14:08


Tgt Ion:113 Resp: 117737

Ion Ratio Lower Upper

113 100

111 101.8 82.3 123.5



192 22.2 17.4 26.2

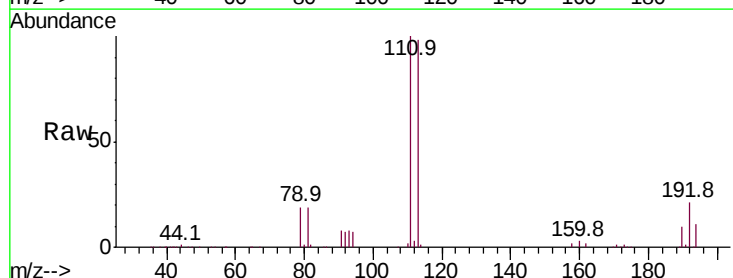


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V



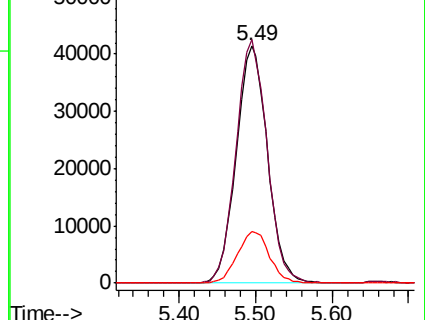
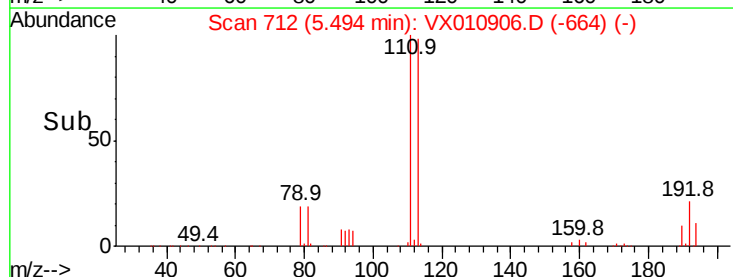


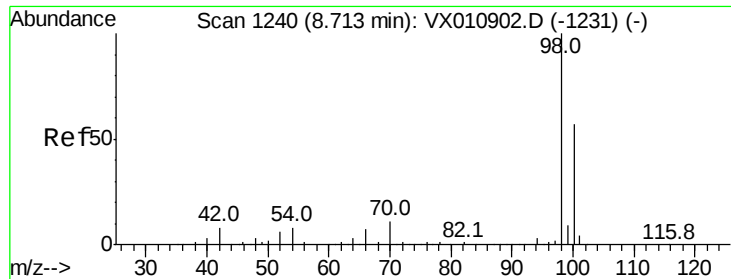

#50
Toluene-d8
Concen: 50.244 ug/l
RT: 8.71 min Scan# 1240
Delta R.T. -0.00 min
Lab File: VX010906.D
Acq: 16 Jul 2019 14:08




Instrument :
MSVOA_X
ClientSampleId :
VX0716WBL01


Tot Ion: 98 Resp: 445814
Ion Ratio Lower Upper
98 100
100 63.9 50.6 75.8

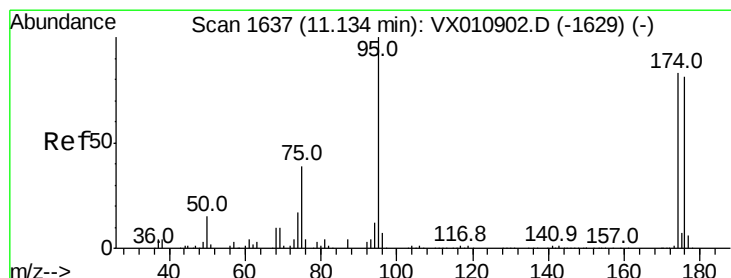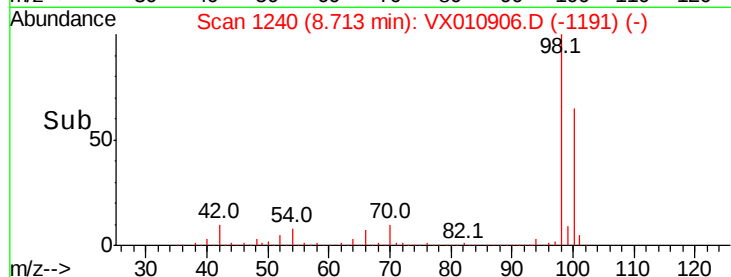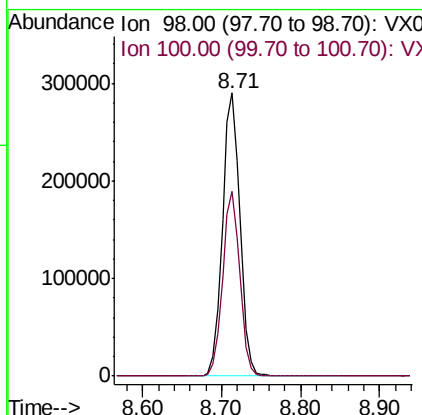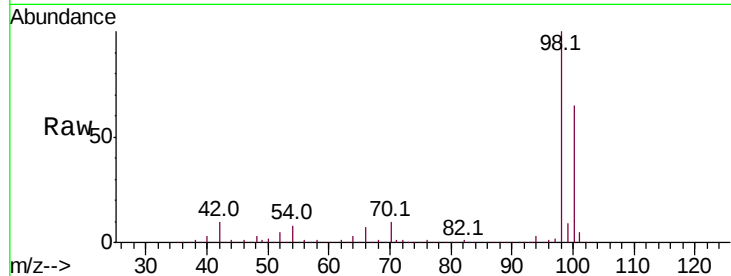

#62
4-Bromofluorobenzene
Concen: 46.842 ug/l
RT: 11.13 min Scan# 1637
Delta R.T. -0.00 min
Lab File: VX010906.D
Acq: 16 Jul 2019 14:08

Tgt Ion: 95 Resp: 152771
Ion Ratio Lower Upper
95 100
174 90.6 0.0 180.6
176 89.1 0.0 173.8


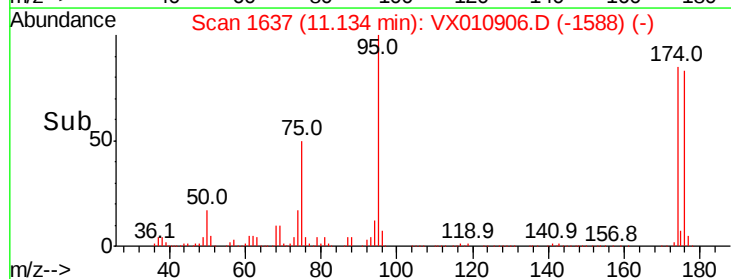
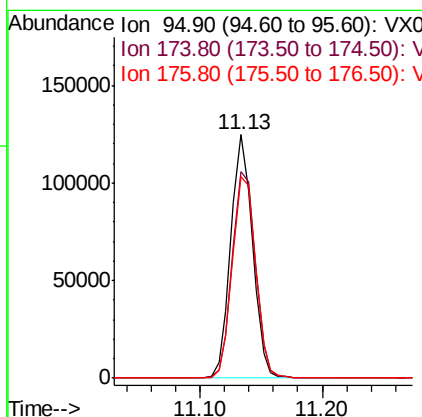
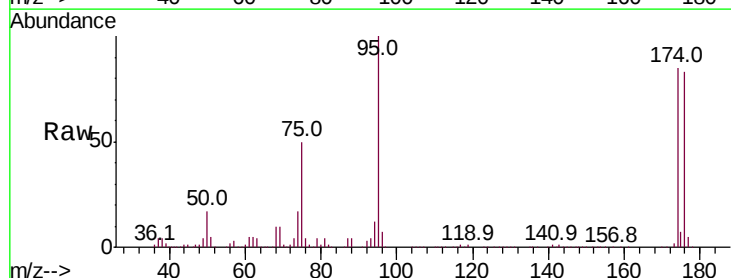


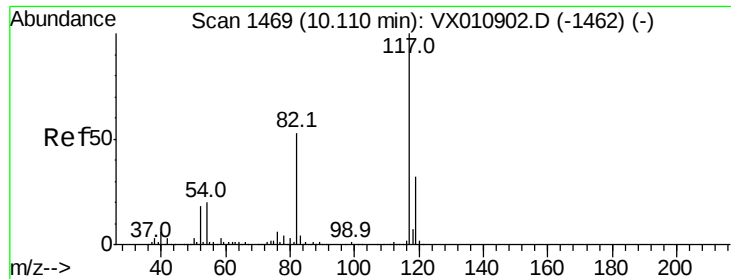

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.11 min Scan# 1469
Delta R.T. -0.00 min
Lab File: VX010906.D
Acq: 16 Jul 2019 14:08

Instrument :
MSVOA_X
ClientSampleId :
VX0716WBL01

Tot Ion	Ratio	Lower	Upper
117	100		
82	51.9	42.6	63.8
119	31.9	25.9	38.9

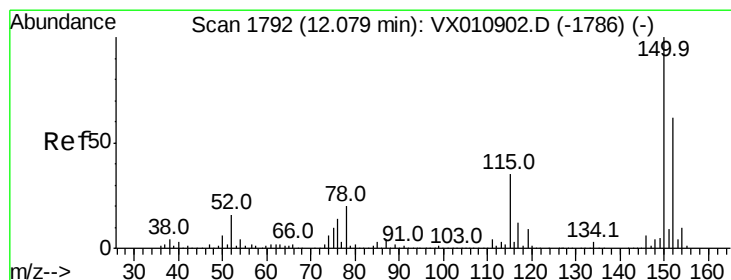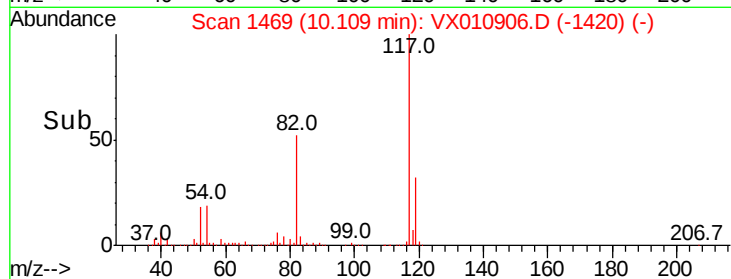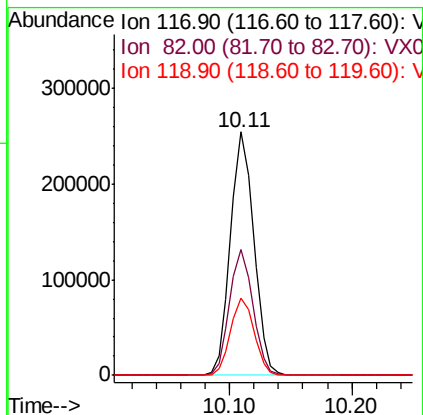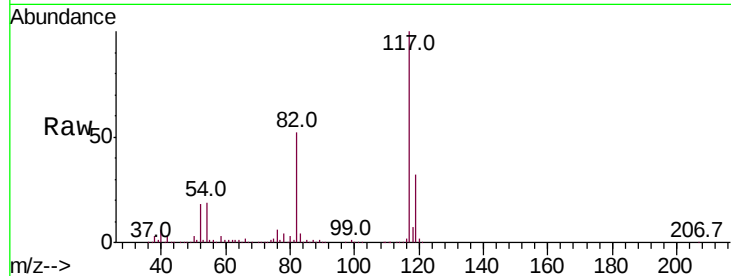

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.08 min Scan# 1792
Delta R.T. -0.00 min
Lab File: VX010906.D
Acq: 16 Jul 2019 14:08

Tgt Ion	Ratio	Lower	Upper
152	100		
115	55.8	39.7	119.1
150	157.8	0.0	345.6

