

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX071619\
 Data File : VX010918.D
 Acq On : 16 Jul 2019 19:48
 Operator : JC/SP
 Sample : K3791-18
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 FL-0628

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X071619W.M
 Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.276	16	20	28	rBV	22204	33962	3.02%	0.454%
2	2.605	227	238	245	rBV	11794	24169	2.15%	0.323%
3	5.501	701	713	723	rBV	133331	383152	34.04%	5.117%
4	5.659	729	739	759	rVB	230058	658549	58.51%	8.795%
5	6.061	794	805	818	rBV	133867	352085	31.28%	4.702%
6	6.860	926	936	947	rBV	346640	815847	72.48%	10.895%
7	7.464	1026	1035	1042	rVB4	7559	18344	1.63%	0.245%
8	8.713	1233	1240	1249	rBV	735520	1125540	100.00%	15.031%
9	9.677	1392	1398	1403	rBV2	7933	13221	1.17%	0.177%
10	10.110	1463	1469	1478	rBV	733405	985877	87.59%	13.166%
11	10.250	1485	1492	1501	rVB	30499	43853	3.90%	0.586%
12	10.353	1501	1509	1515	rBV	84338	129671	11.52%	1.732%
13	10.701	1562	1566	1575	rVB	9081	15958	1.42%	0.213%
14	10.835	1577	1588	1591	rBV6	6062	11566	1.03%	0.154%
15	11.018	1611	1618	1621	rBV	11179	14501	1.29%	0.194%
16	11.134	1632	1637	1643	rBV	636789	798060	70.90%	10.658%
17	11.359	1669	1674	1681	rBV	15843	24021	2.13%	0.321%
18	11.432	1681	1686	1688	rBV	25580	36165	3.21%	0.483%
19	11.506	1694	1698	1707	rVB	14172	22090	1.96%	0.295%
20	11.664	1717	1724	1733	rBV	72341	95929	8.52%	1.281%
21	11.804	1743	1747	1754	rVB	107624	133307	11.84%	1.780%
22	11.945	1767	1770	1774	rVB	8994	11321	1.01%	0.151%
23	12.024	1774	1783	1786	rBV	19267	24596	2.19%	0.328%
24	12.079	1786	1792	1798	rVV	750972	969824	86.17%	12.952%
25	12.140	1798	1802	1807	rVV	47539	60127	5.34%	0.803%
26	12.298	1820	1828	1830	rBV	20966	29705	2.64%	0.397%
27	12.323	1830	1832	1835	rVV	19433	20176	1.79%	0.269%
28	12.365	1835	1839	1847	rVB2	18083	29364	2.61%	0.392%
29	12.457	1847	1854	1859	rBV	14854	21077	1.87%	0.281%
30	12.518	1859	1864	1870	rBV	36588	46218	4.11%	0.617%
31	12.585	1870	1875	1877	rBV	24380	32863	2.92%	0.439%
32	12.609	1877	1879	1884	rVB	24902	25258	2.24%	0.337%
33	12.664	1884	1888	1892	rBV	22070	26687	2.37%	0.356%
34	12.755	1899	1903	1911	rVB4	18949	42608	3.79%	0.569%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX071619\
Data File : VX010918.D
Acq On : 16 Jul 2019 19:48
Operator : JC/SP
Sample : K3791-18
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FL-0628

Integration Parameters: RTEINT.P

Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X071619W.M
Title : SW846 8260

35	12.902	1922	1927	1931	rVB2	22059	31042	2.76%	0.415%
36	12.975	1931	1939	1942	rBV3	17354	28669	2.55%	0.383%
37	13.018	1942	1946	1953	rVV	31228	39498	3.51%	0.527%
38	13.079	1953	1956	1964	rVB4	8785	13913	1.24%	0.186%
39	13.194	1971	1975	1978	rBV2	11719	16379	1.46%	0.219%
40	13.304	1990	1993	1996	rBV4	8178	11958	1.06%	0.160%
41	13.341	1996	1999	2004	rVB2	49405	67253	5.98%	0.898%
42	13.475	2018	2021	2029	rVB	19581	28439	2.53%	0.380%
43	13.633	2043	2047	2053	rVV4	10472	21490	1.91%	0.287%
44	13.719	2059	2061	2068	rVB2	10066	13917	1.24%	0.186%
45	13.834	2072	2080	2087	rVB2	19404	40431	3.59%	0.540%
46	13.987	2098	2105	2108	rBV3	9164	14286	1.27%	0.191%
47	14.286	2147	2154	2159	rVB5	9506	19944	1.77%	0.266%
48	14.536	2191	2195	2201	rBV4	10694	15392	1.37%	0.206%
49	14.694	2213	2221	2225	rBV	19407	29057	2.58%	0.388%
50	14.840	2240	2245	2249	rBV2	13298	20749	1.84%	0.277%


Sum of corrected areas: 7488108

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX071619\
Data File : VX010918.D
Acq On : 16 Jul 2019 19:48
Operator : JC/SP
Sample : K3791-18
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FL-0628

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X071619W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

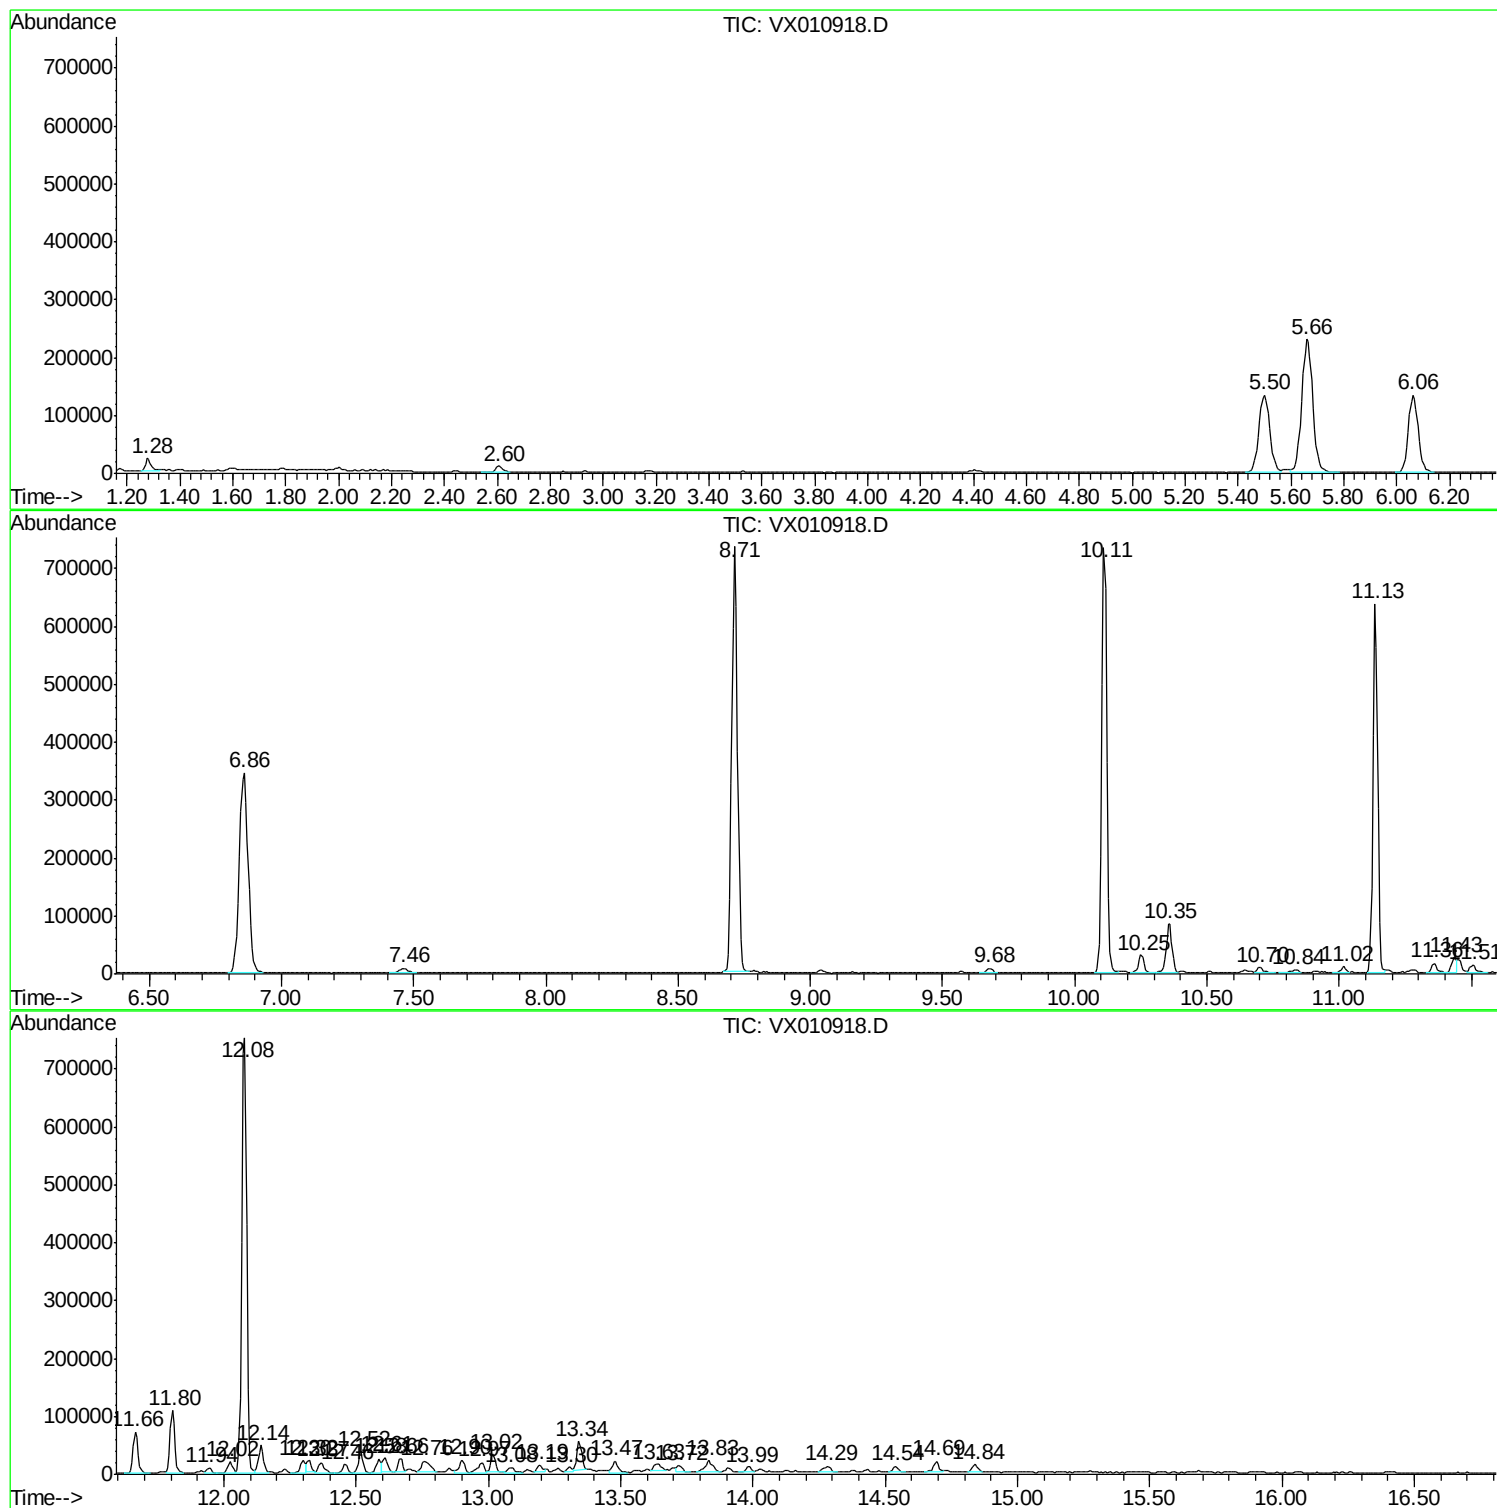

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX071619\
Data File : VX010918.D
Acq On : 16 Jul 2019 19:48
Operator : JC/SP
Sample : K3791-18
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FL-0628

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X071619W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX071619\
Data File : VX010918.D
Acq On : 16 Jul 2019 19:48
Operator : JC/SP
Sample : K3791-18
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FL-0628

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X071619W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc