


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX071619\
 Data File : VX010898.D
 Acq On : 16 Jul 2019 09:10
 Operator : JC/SP
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X071619W.M
 Title : SW846 8260
 Last Update : Wed Jul 17 06:57:45 2019

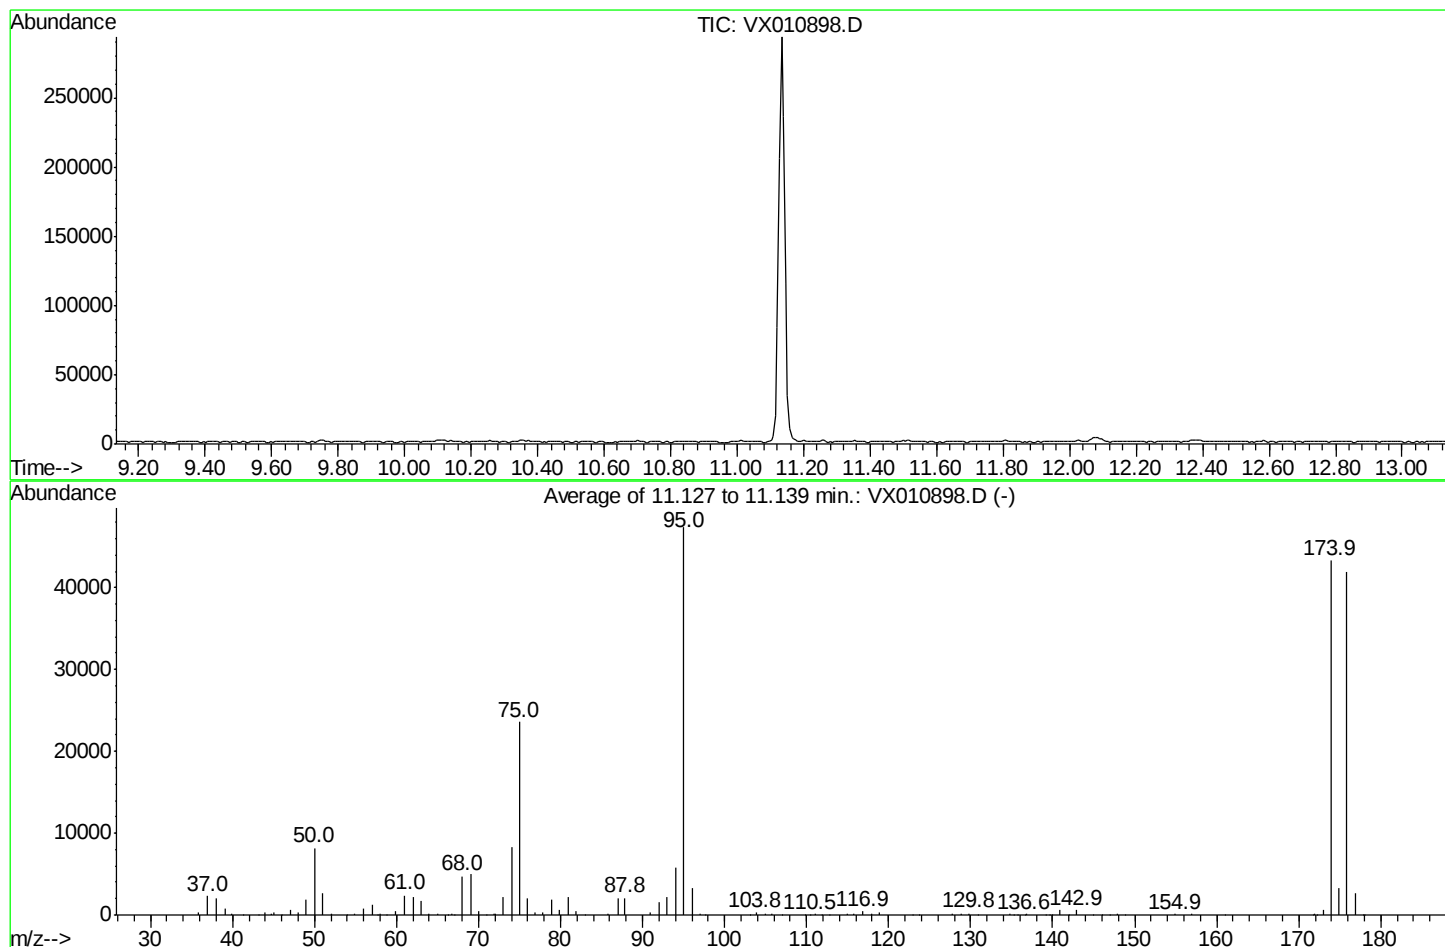

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1629

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.3	8212	PASS
75	95	30	60	49.8	23594	PASS
95	95	100	100	100.0	47384	PASS
96	95	5	9	7.1	3368	PASS
173	174	0.00	2	1.4	608	PASS
174	95	50	100	91.4	43288	PASS
175	174	5	9	7.7	3341	PASS
176	174	95	101	96.8	41896	PASS
177	176	5	9	6.3	2623	PASS