

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\WX071620\
 Data File : VX017408.D
 Acq On : 16 Jul 2020 21:47
 Operator : JC/SP
 Sample : L3328-07
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 DAY-5


Quant Time: Jul 17 01:04:20 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X071320W.M
 Quant Title : SW846 8260
 QLast Update : Tue Jul 14 02:59:51 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.63	168	248779	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.83	114	442892	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.10	117	459943	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.06	152	251292	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	6.03	65	176519	56.53	ug/l	0.00
Spiked Amount			Recovery	=	113.06%	
35) Dibromofluoromethane	5.47	113	149903	50.25	ug/l	0.00
Spiked Amount			Recovery	=	100.50%	
50) Toluene-d8	8.70	98	548314	50.95	ug/l	0.00
Spiked Amount			Recovery	=	101.90%	
62) 4-Bromofluorobenzene	11.12	95	226682	53.03	ug/l	0.00
Spiked Amount			Recovery	=	106.06%	

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
3) Chloromethane	1.32	50	632	0.267	ug/l #	55
5) Bromomethane	1.64	94	362	0.237	ug/l #	4
8) Diethyl Ether	2.17	74	424	0.303	ug/l	68
10) Methyl Iodide	2.50	142	41	2.387	ug/l #	39
11) Tert butyl alcohol	3.03	59	725	1.378	ug/l #	87
13) Acrolein	2.27	56	258	0.895	ug/l #	64
15) Acrylonitrile	3.10	53	300	0.235	ug/l #	74
16) Acetone	2.42	43	6600	5.925	ug/l	99
17) Carbon Disulfide	2.55	76	7050	1.067	ug/l #	94
18) Methyl Acetate	2.75	43	921	0.335	ug/l	100
20) Methylene Chloride	2.84	84	2973	1.094	ug/l #	95
31) Cyclohexane	5.54	56	1781	0.495	ug/l #	76
36) 1,1-Dichloropropene	5.62	75	19404	4.763	ug/l #	50
38) Carbon Tetrachloride	5.63	117	24775	5.194	ug/l #	19
39) Methylcyclohexane	7.45	83	4186	0.946	ug/l #	86
49) 1,4-Dioxane	7.73	88	28	0.424	ug/l #	1
55) 1,1,2-Trichloroethane	9.14	97	876	0.280	ug/l #	23
76) 1,2,3-Trichloropropane	11.12	75	114592	24.678	ug/l #	38
81) trans-1,4-Dichloro-2-buten	11.12	75	114592	62.603	ug/l #	11
85) sec-Butylbenzene	11.93	105	5709	0.377	ug/l	99
86) p-Isopropyltoluene	12.22	119	4455	0.311	ug/l	92
89) n-Butylbenzene	12.37	91	3731	0.306	ug/l	100
90) Hexachloroethane	12.65	117	4864	1.789	ug/l #	8
92) 1,2-Dibromo-3-Chloropropan	12.96	75	704	0.558	ug/l #	1
95) Naphthalene	13.82	128	3527	0.229	ug/l #	44

(#) = qualifier out of range (m) = manual integration (+) = signals summed

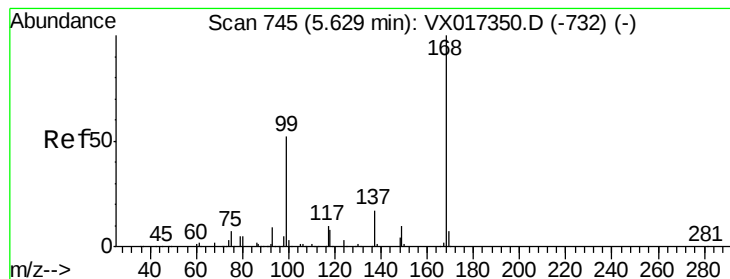

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.63 min Scan# 746

Delta R.T. 0.01 min

Lab File: VX017408.D

Acq: 16 Jul 2020 21:47

Instrument :

MSVOA_X

ClientSampled :


DAY-5

Tot Ion:168 Resp: 248779

Ion Ratio Lower Upper

168 100

99 54.0 41.6 62.4



Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.63

100000

80000



60000

40000

20000

0

Time-->



#3

Chloromethane

Concen: 0.267 ug/l

RT: 1.32 min Scan# 38

Delta R.T. 0.01 min

Lab File: VX017408.D


Acq: 16 Jul 2020 21:47

Tgt Ion: 50 Resp: 632

Ion Ratio Lower Upper

50 100

52 59.1 26.7 40.1#



Abundance Ion 49.90 (49.60 to 50.60): VX0

Ion 51.90 (51.60 to 52.60): VX0

1.32

600

500

400


300


200

100

0

Time-->



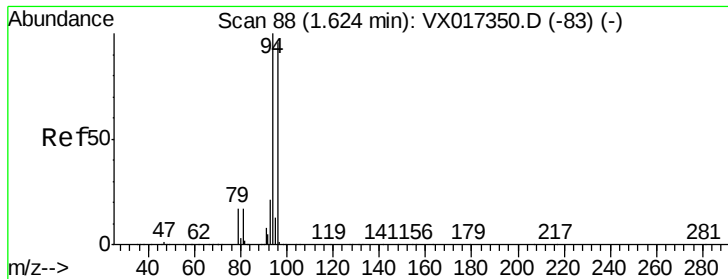

#5

Bromomethane

Concen: 0.237 ug/l

RT: 1.64 min Scan# 91

Delta R.T. 0.02 min

Lab File: VX017408.D

Acq: 16 Jul 2020 21:47

Instrument :

MSVOA_X

ClientSampled :


DAY-5

Tot Ion: 94 Resp: 362

Ion Ratio Lower Upper




94 100

96 1.7 76.6 115.0#

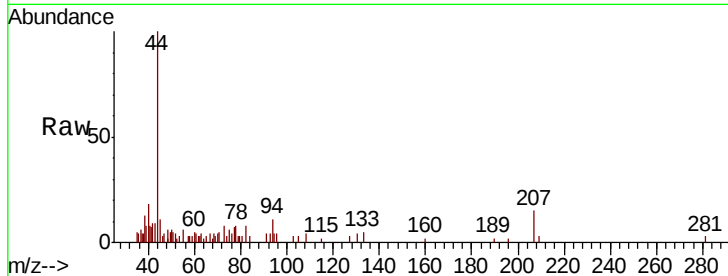

Abundance Ion 93.90 (93.60 to 94.60): VX0

Ion 95.90 (95.60 to 96.60): VX0

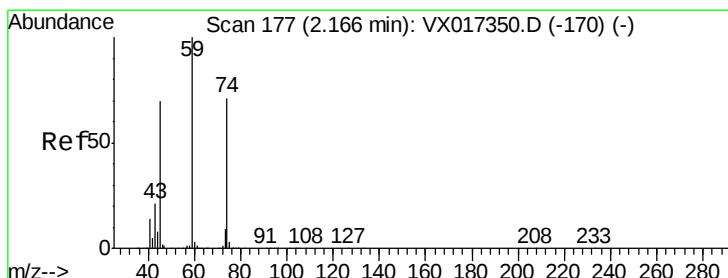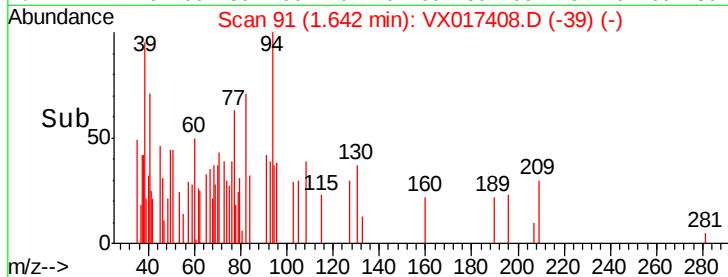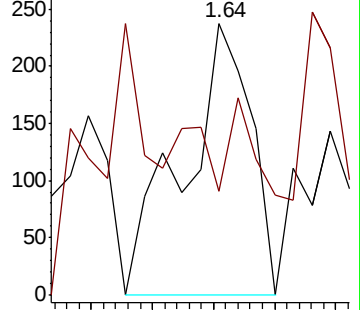

#8

Diethyl Ether

Concen: 0.303 ug/l

RT: 2.17 min Scan# 177

Delta R.T. -0.00 min

Lab File: VX017408.D


Acq: 16 Jul 2020 21:47

Tgt Ion: 74 Resp: 424

Ion Ratio Lower Upper



74 100


45 63.0 47.2 141.6

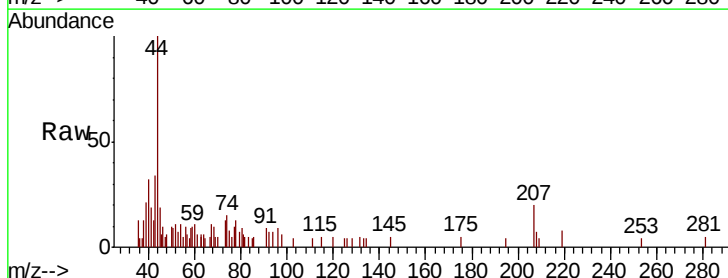

Abundance Ion 74.00 (73.70 to 74.70): VX0

Ion 45.00 (44.70 to 45.70): VX0

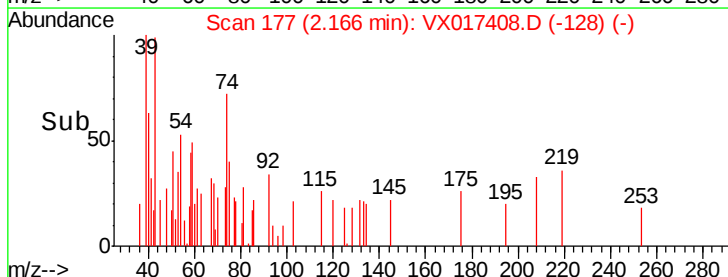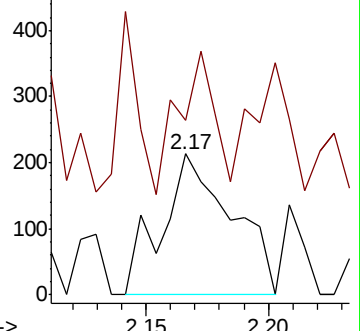







#10
Methyl Iodide
Concen: 2.387 ug/l
RT: 2.50 min Scan# 232
Delta R.T. 0.01 min
Lab File: VX017408.D
Acq: 16 Jul 2020 21:47

Instrument :
MSVOA_X
ClientSampled :
DAY-5

Tot Ion:142 Resp: 41
Ion Ratio Lower Upper
142 100
127 0.0 36.8 55.2#
141 0.0 11.4 17.0#




Abundance Ion 141.80 (141.50 to 142.50): V
Ion 126.80 (126.50 to 127.50): V
Ion 140.80 (140.50 to 141.50): V


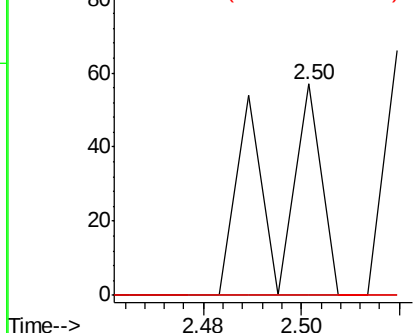



#11
Tert butyl alcohol
Concen: 1.378 ug/l
RT: 3.03 min Scan# 318
Delta R.T. 0.01 min
Lab File: VX017408.D
Acq: 16 Jul 2020 21:47

Tgt Ion: 59 Resp: 725
Ion Ratio Lower Upper
59 100
57 15.2 8.3 12.5#



Abundance Ion 59.00 (58.70 to 59.70): VX0
Ion 57.00 (56.70 to 57.70): VX0

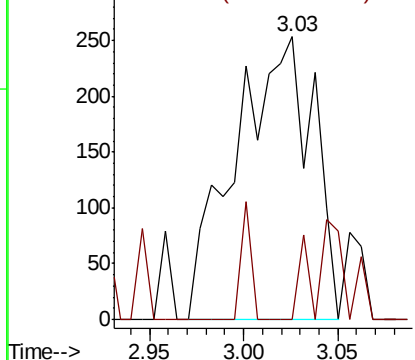



#13

Acrolein

Concen: 0.895 ug/l

RT: 2.27 min Scan# 194

Delta R.T. -0.01 min

Lab File: VX017408.D

Acq: 16 Jul 2020 21:47

Instrument :

MSVOA_X

ClientSampled :


DAY-5

Tot Ion: 56 Resp: 258

Ion Ratio Lower Upper




56 100

55 101.2 57.1 85.7#



Abundance Ion 56.00 (55.70 to 56.70): VX0

Ion 55.00 (54.70 to 55.70): VX0

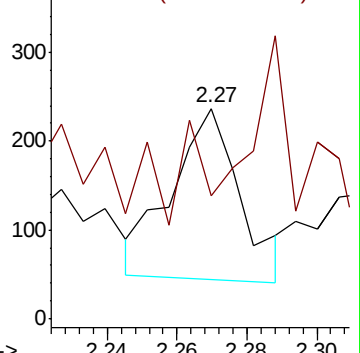

#15

Acrylonitrile

Concen: 0.235 ug/l

RT: 3.10 min Scan# 331

Delta R.T. -0.01 min

Lab File: VX017408.D

Acq: 16 Jul 2020 21:47


Tgt Ion: 53 Resp: 300

Ion Ratio Lower Upper

53 100

52 55.3 65.8 98.6#



51 26.0 29.2 43.8#




Abundance Ion 53.00 (52.70 to 53.70): VX0

Ion 52.00 (51.70 to 52.70): VX0

Ion 51.00 (50.70 to 51.70): VX0

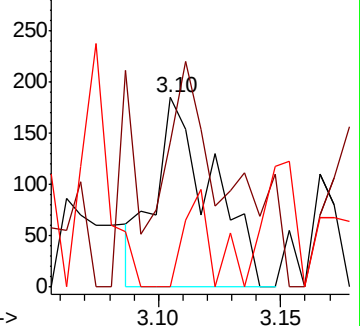



#16

Acetone

Concen: 5.925 ug/l

RT: 2.42 min Scan# 219

Delta R.T. -0.00 min

Lab File: VX017408.D

Acq: 16 Jul 2020 21:47

Instrument :

MSVOA_X

ClientSampleId :





DAY-5

Tot Ion: 43 Resp: 6600

Ion Ratio Lower Upper

43 100

58 30.6 24.2 36.2

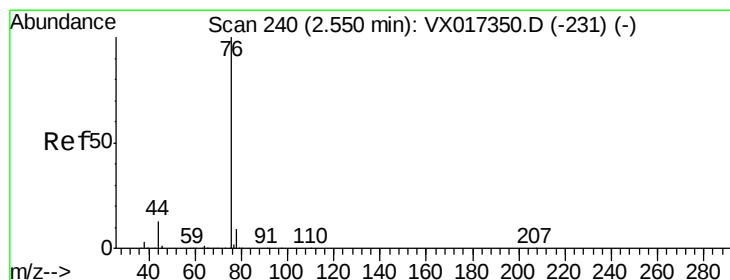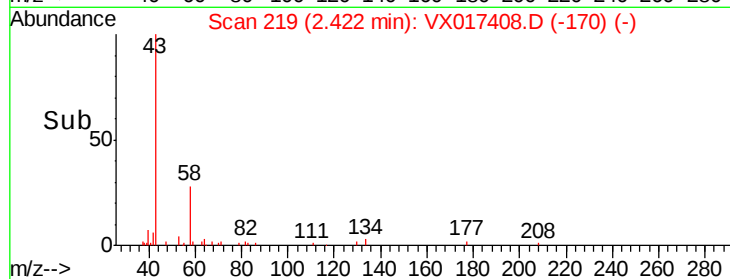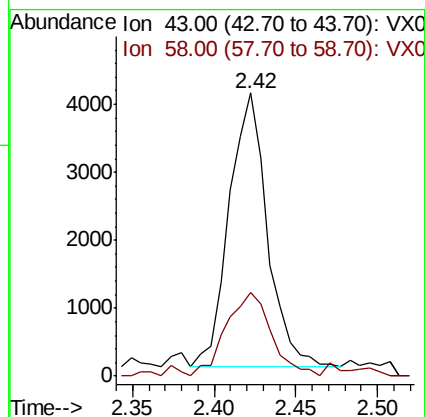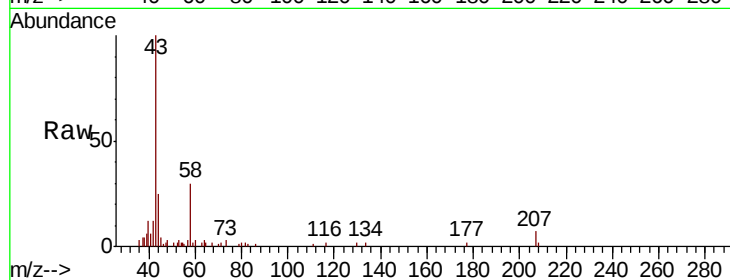

#17

Carbon Disulfide

Concen: 1.067 ug/l

RT: 2.55 min Scan# 240

Delta R.T. -0.00 min

Lab File: VX017408.D




Acq: 16 Jul 2020 21:47


Tgt Ion: 76 Resp: 7050

Ion Ratio Lower Upper

76 100

78 11.2 7.3 10.9#


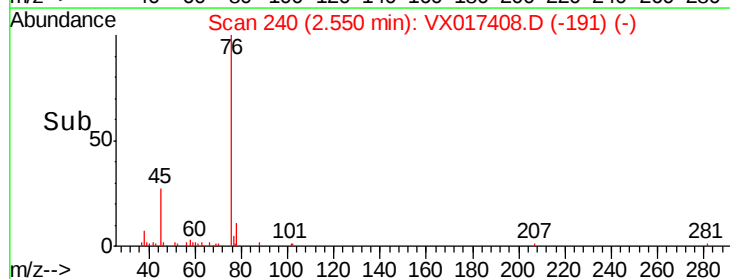
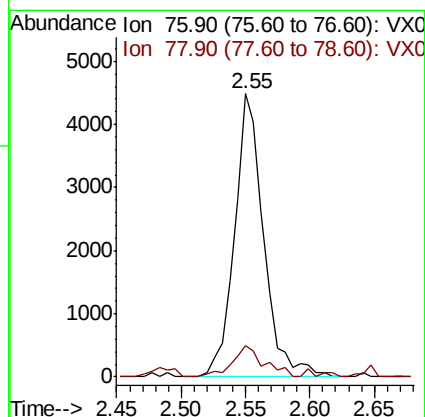
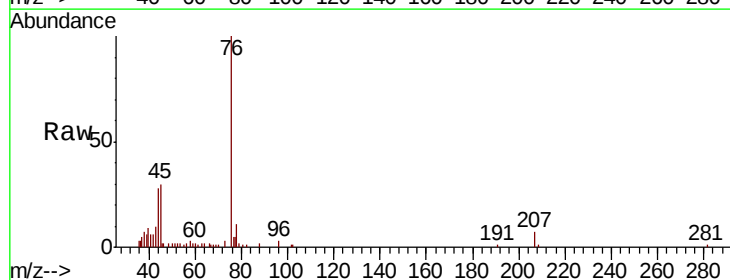


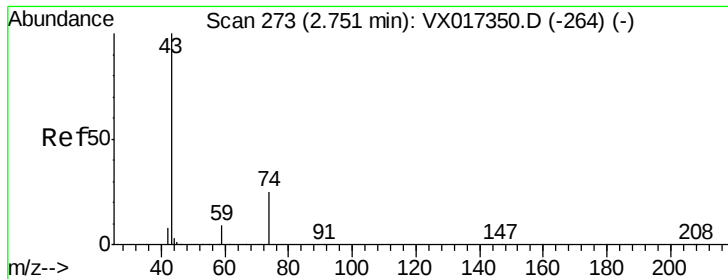

#18
Methyl Acetate
Concen: 0.335 ug/l
RT: 2.75 min Scan# 273
Delta R.T. -0.00 min
Lab File: VX017408.D
Acq: 16 Jul 2020 21:47




Instrument :
MSVOA_X
ClientSampled :
DAY-5


Tot Ion: 43 Resp: 921
Ion Ratio Lower Upper
43 100
74 24.1 19.4 29.2

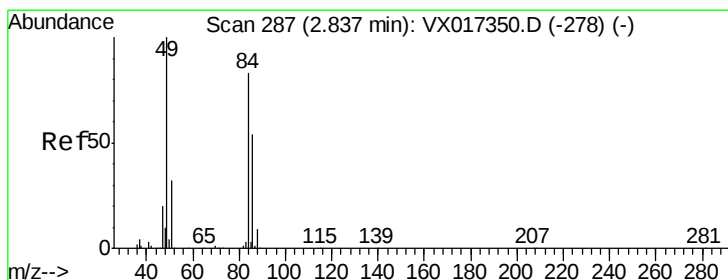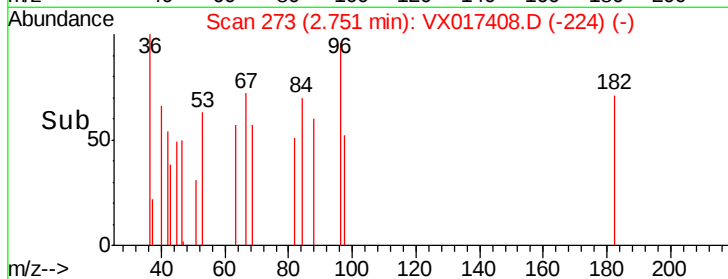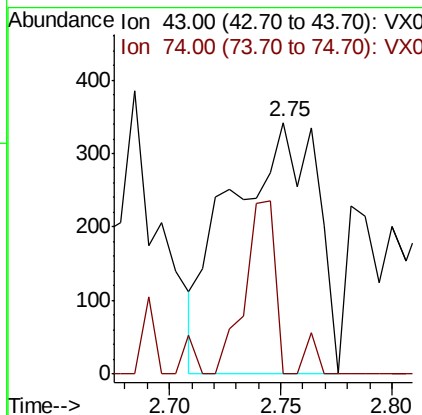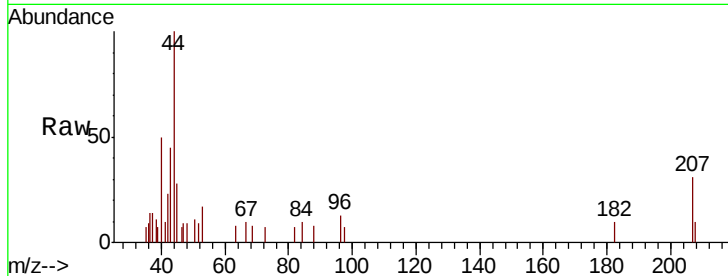

#20
Methylene Chloride
Concen: 1.094 ug/l
RT: 2.84 min Scan# 287
Delta R.T. -0.00 min
Lab File: VX017408.D
Acq: 16 Jul 2020 21:47

Tgt Ion: 84 Resp: 2973
Ion Ratio Lower Upper
84 100
49 119.4 95.8 143.8
51 28.3 31.0 46.4#
86 59.6 51.8 77.8


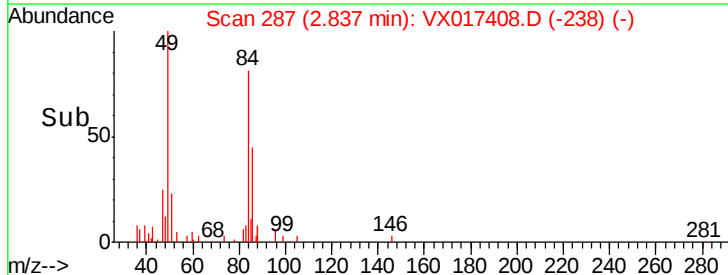
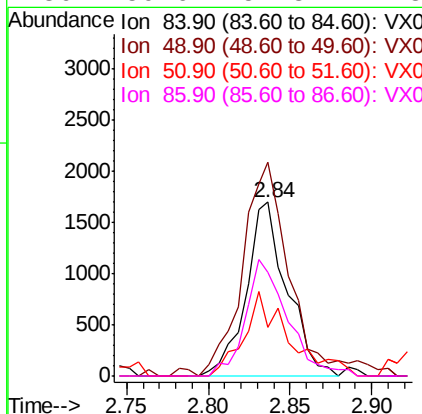
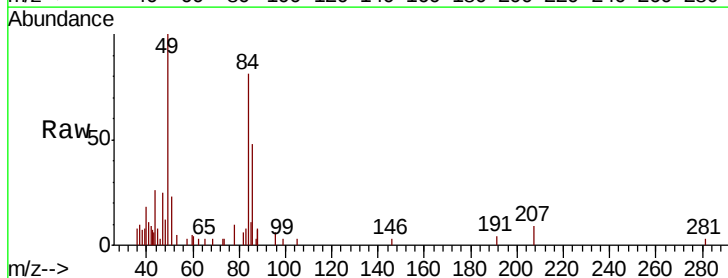


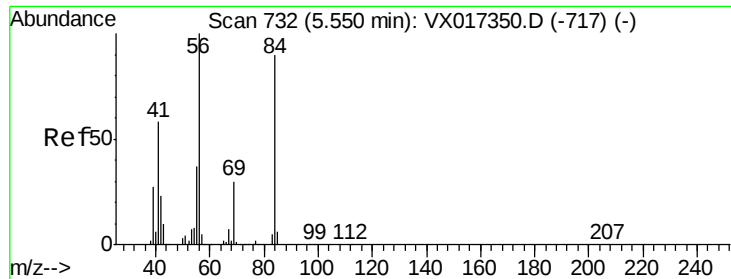

#31
Cyclohexane
Concen: 0.495 ug/l
RT: 5.54 min Scan# 730
Delta R.T. -0.01 min
Lab File: VX017408.D
Acq: 16 Jul 2020 21:47




Instrument :
MSVOA_X
ClientSampled :
DAY-5


Tot Ion: 56 Resp: 1781
Ion Ratio Lower Upper
56 100
69 44.7 23.7 35.5#
84 69.0 71.8 107.6#

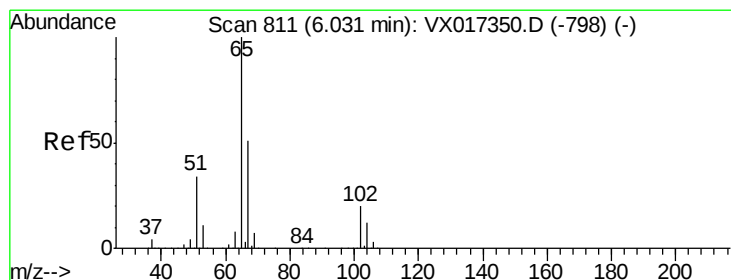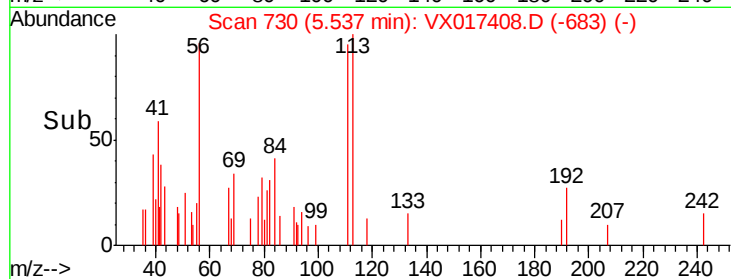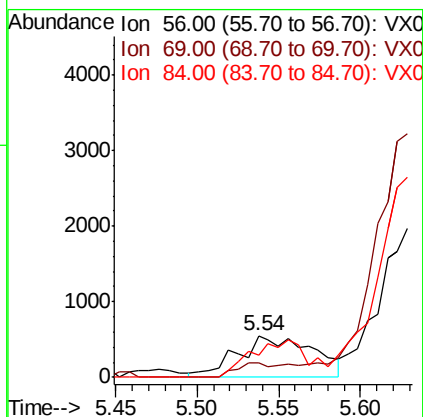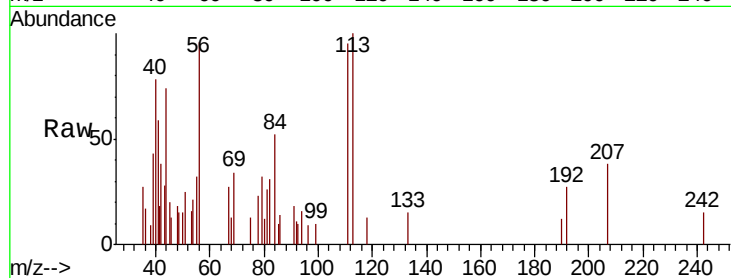

#33
1,2-Dichloroethane-d4
Concen: 56.533 ug/l
RT: 6.03 min Scan# 811
Delta R.T. -0.00 min
Lab File: VX017408.D
Acq: 16 Jul 2020 21:47

Tgt Ion: 65 Resp: 176519
Ion Ratio Lower Upper
65 100
67 51.8 0.0 101.6

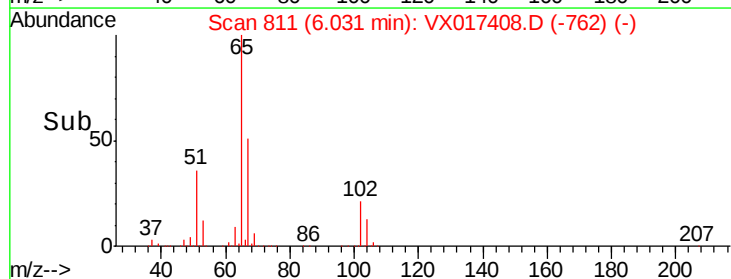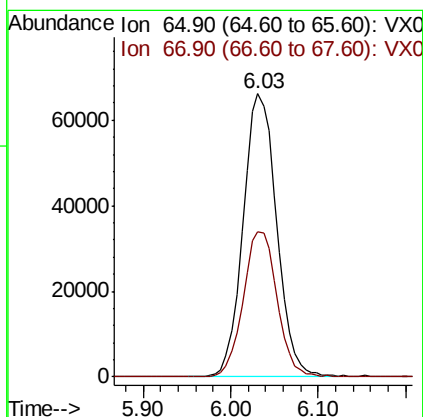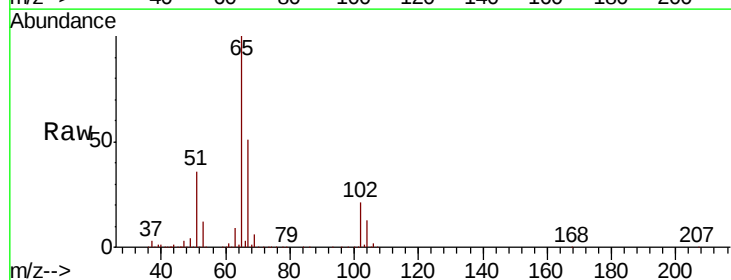



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.83 min Scan# 942

Delta R.T. -0.00 min

Lab File: VX017408.D

Acq: 16 Jul 2020 21:47

Instrument :

MSVOA_X

ClientSampleId :

DAY-5


Tot Ion:114 Resp: 442892

Ion Ratio Lower Upper

114 100

63 20.6 0.0 40.0




88 15.6 0.0 32.8

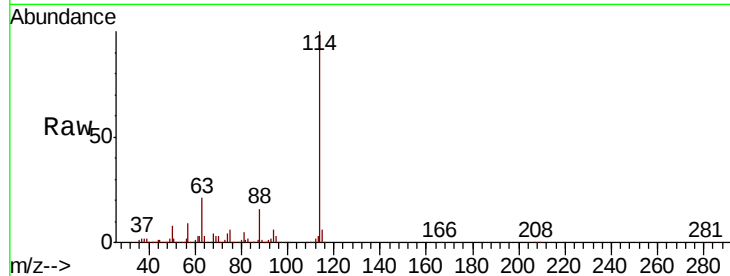

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

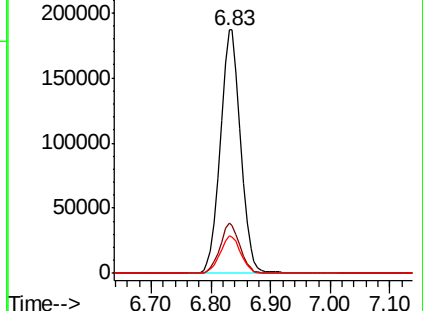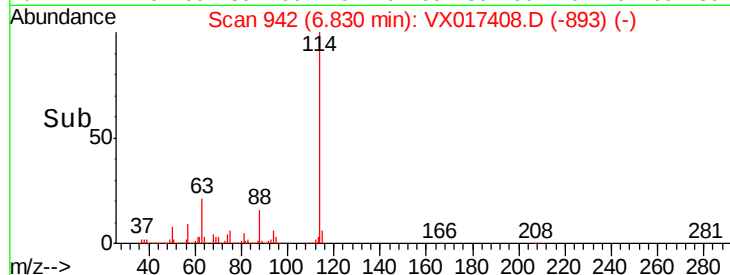

#35

Dibromofluoromethane

Concen: 50.246 ug/l

RT: 5.47 min Scan# 719

Delta R.T. -0.00 min

Lab File: VX017408.D

Acq: 16 Jul 2020 21:47


Tgt Ion:113 Resp: 149903

Ion Ratio Lower Upper

113 100

111 103.7 82.4 123.6



192 21.4 17.2 25.8




Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V



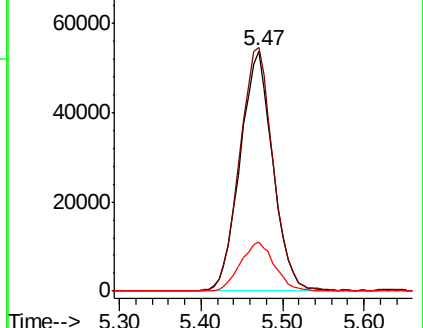



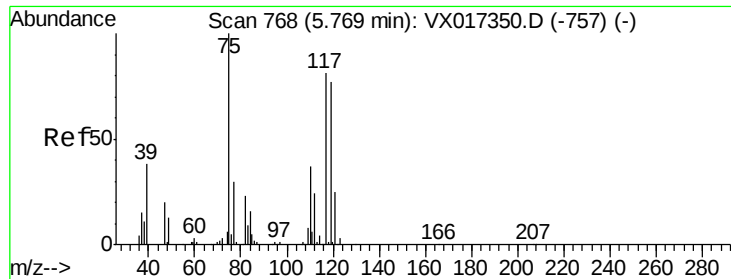

#36
 1,1-Dichloropropene
 Concen: 4.763 ug/l
 RT: 5.62 min Scan# 744
 Delta R.T. -0.15 min
 Lab File: VX017408.D
 Acq: 16 Jul 2020 21:47




Instrument :
 MSVOA_X
 ClientSampleId :
 DAY-5


Tot Ion	75	110	77	Resp	Lower	Upper
19404	100	10.9	0.2		18.6	55.8#
					24.9	37.3#

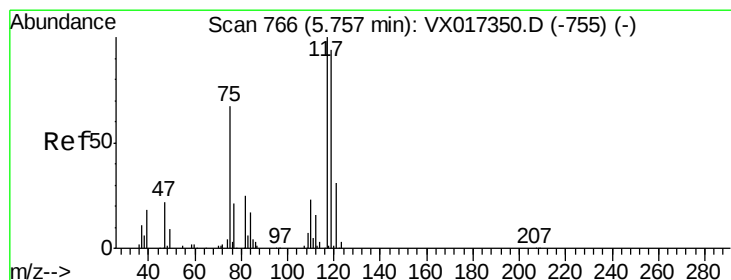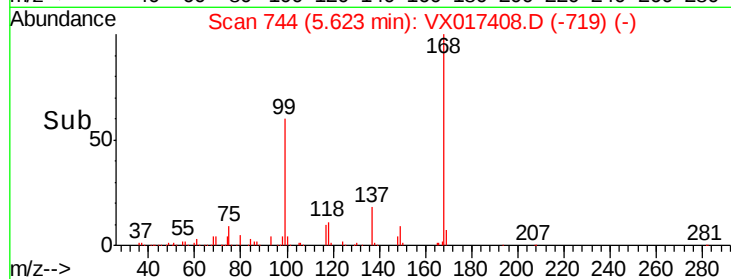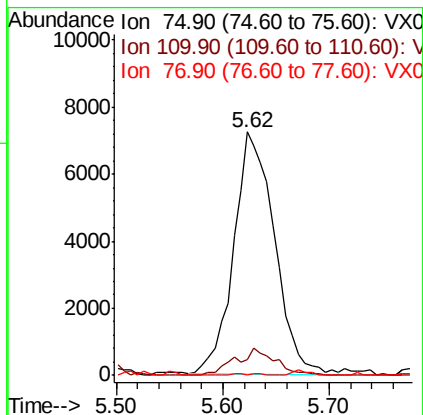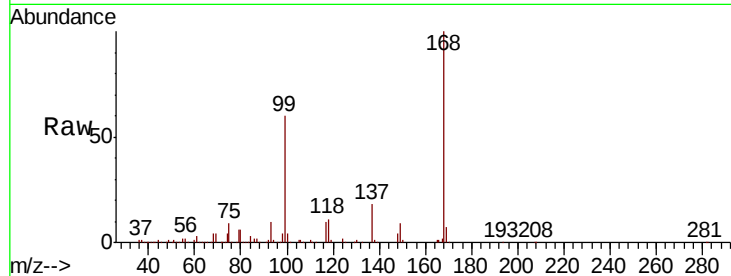

#38
 Carbon Tetrachloride
 Concen: 5.194 ug/l
 RT: 5.63 min Scan# 745
 Delta R.T. -0.13 min
 Lab File: VX017408.D
 Acq: 16 Jul 2020 21:47

Tgt Ion	117	119	121	Resp	Lower	Upper
24775	100	7.5	0.0		74.7	112.1#
					24.5	36.7#

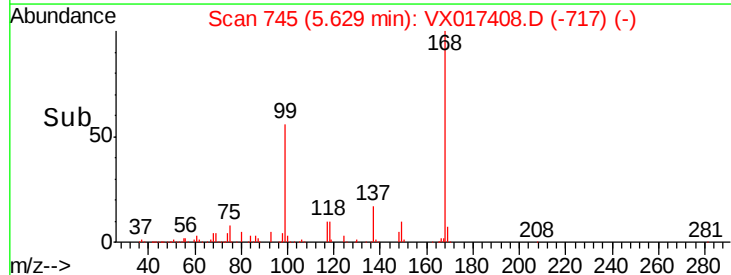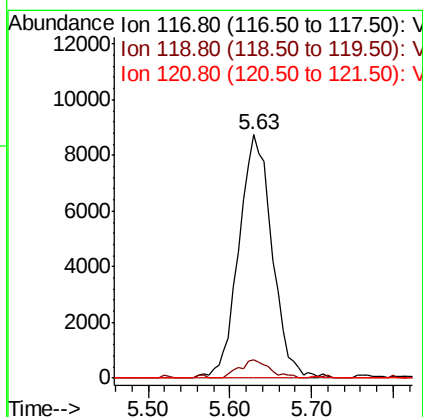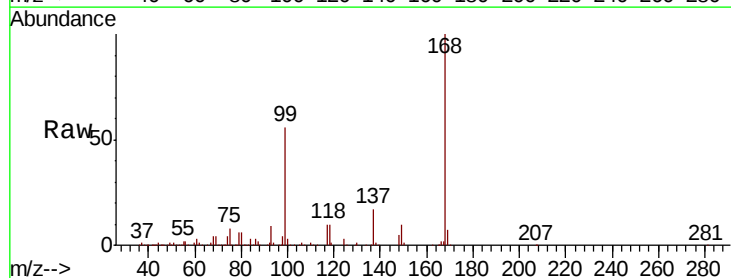


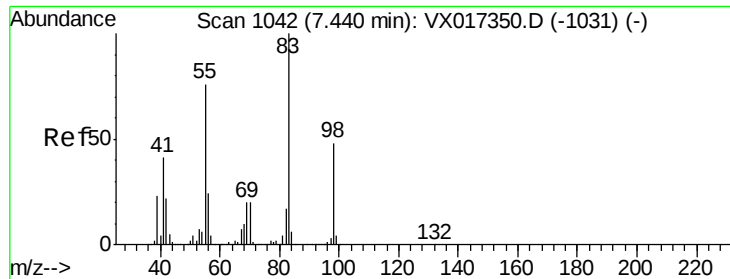




#39
Methvlcvclohexane
Concen: 0.946 ug/l
RT: 7.45 min Scan# 1043
Delta R.T. 0.01 min
Lab File: VX017408.D
Acq: 16 Jul 2020 21:47

Instrument :
MSVOA_X
ClientSampleId :
DAY-5

Tot Ion: 83 Resp: 4186
Ion Ratio Lower Upper
83 100
55 82.9 61.2 91.8
98 63.5 38.1 57.1#

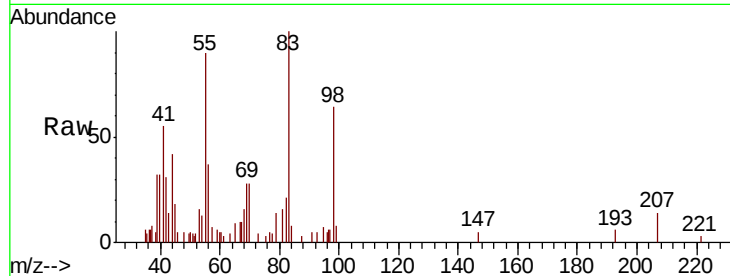


Abundance Ion 83.00 (82.70 to 83.70): VX0
Ion 55.00 (54.70 to 55.70): VX0
Ion 98.00 (97.70 to 98.70): VX0

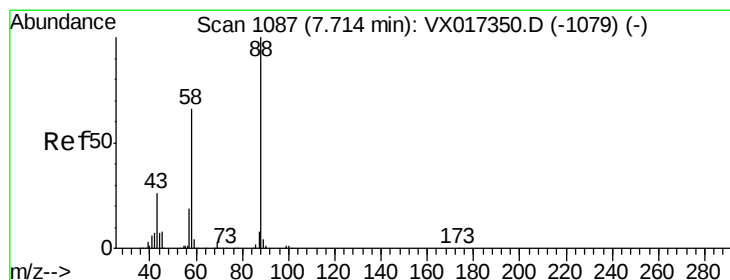
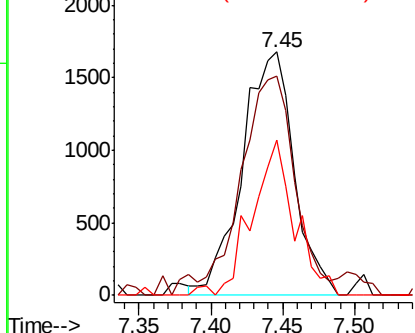



#49
1,4-Dioxane
Concen: 0.424 ug/l
RT: 7.73 min Scan# 1090
Delta R.T. 0.02 min
Lab File: VX017408.D
Acq: 16 Jul 2020 21:47

Tgt Ion: 88 Resp: 28
Ion Ratio Lower Upper
88 100
43 0.0 25.6 38.4#
58 582.1 53.9 80.9#



Abundance Ion 88.00 (87.70 to 88.70): VX0
Ion 43.00 (42.70 to 43.70): VX0
Ion 58.00 (57.70 to 58.70): VX0

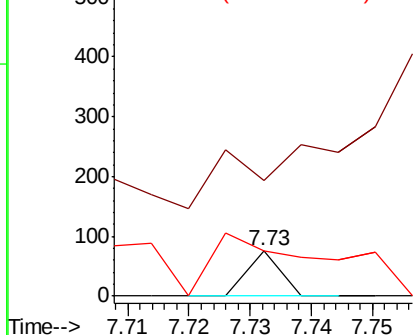



#50

Toluene-d8

Concen: 50.951 ug/l

RT: 8.70 min Scan# 1248

Delta R.T. -0.00 min

Lab File: VX017408.D

Acq: 16 Jul 2020 21:47

Instrument :

MSVOA_X

ClientSampleId :


DAY-5

Tot Ion: 98 Resp: 548314

Ion Ratio Lower Upper

98 100

100 65.8 53.4 80.2

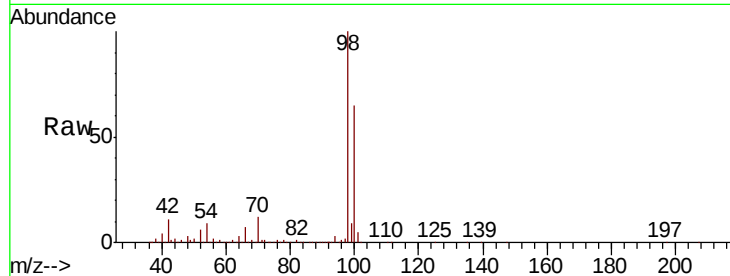

Abundance Ion 98.00 (97.70 to 98.70): VX0

Ion 100.00 (99.70 to 100.70): VX

8.70

400000

300000



200000

100000

0

8.60 8.70 8.80 8.90

Time-->

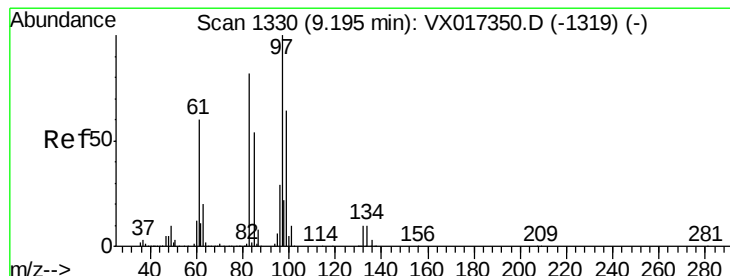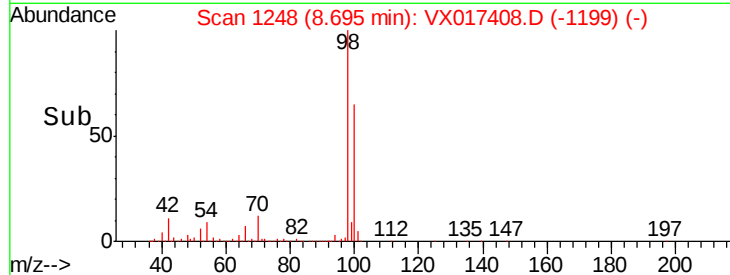

#55

1,1,2-Trichloroethane

Concen: 0.280 ug/l

RT: 9.14 min Scan# 1321

Delta R.T. -0.05 min

Lab File: VX017408.D

Acq: 16 Jul 2020 21:47

Tgt Ion: 97 Resp: 876


Ion Ratio Lower Upper

97 100

83 16.1 65.8 98.6#

85 0.0 42.8 64.2#

99 0.0 51.2 76.8#

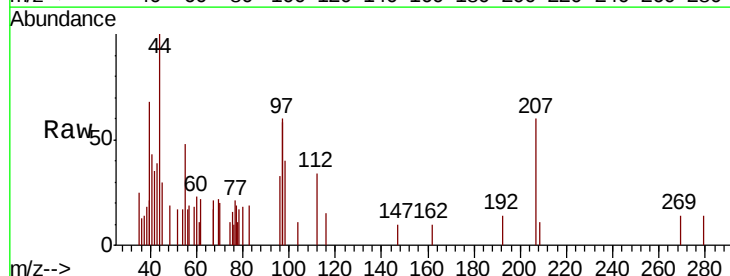

Abundance Ion 96.90 (96.60 to 97.60): VX0

Ion 82.90 (82.60 to 83.60): VX0

Ion 84.90 (84.60 to 85.60): VX0

Ion 98.90 (98.60 to 99.60): VX0

800

600


400


200

0

9.10 9.15 9.20

Time-->

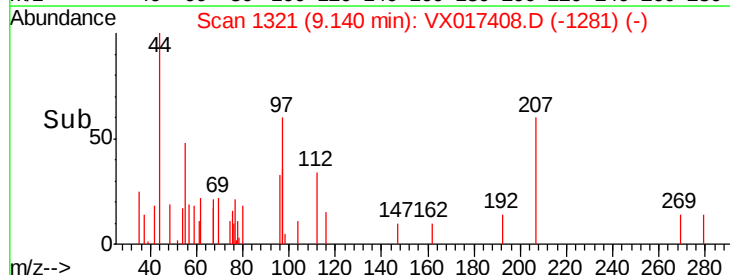



#62

4-Bromofluorobenzene

Concen: 53.029 ug/l

RT: 11.12 min Scan# 1646

Delta R.T. -0.00 min

Lab File: VX017408.D

Acq: 16 Jul 2020 21:47

Instrument :

MSVOA_X

ClientSampleId :

DAY-5


Tot Ion: 95 Resp: 226682

Ion Ratio Lower Upper

95 100

174 80.9 0.0 175.8




176 78.4 0.0 164.6



Abundance Ion 94.90 (94.60 to 95.60): VX017350.D (-1639) (-)

Ion 173.80 (173.50 to 174.50): VX017350.D (-1639) (-)

Ion 175.80 (175.50 to 176.50): VX017350.D (-1639) (-)

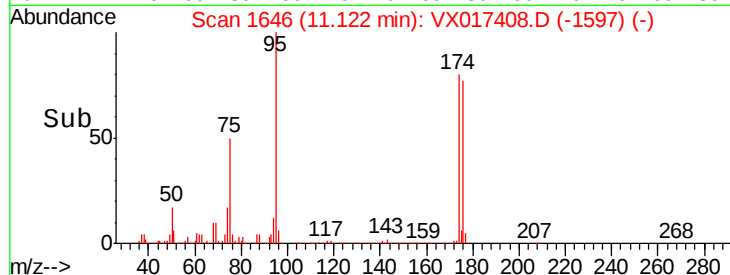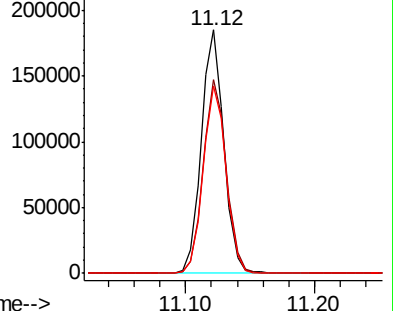

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.10 min Scan# 1478

Delta R.T. -0.00 min

Lab File: VX017408.D

Acq: 16 Jul 2020 21:47


Tgt Ion: 117 Resp: 459943

Ion Ratio Lower Upper

117 100

82 54.0 42.0 63.0



119 33.0 26.3 39.5




Abundance Ion 116.90 (116.60 to 117.60): VX017350.D (-1468) (-)

Ion 82.00 (81.70 to 82.70): VX017350.D (-1468) (-)

Ion 118.90 (118.60 to 119.60): VX017350.D (-1468) (-)

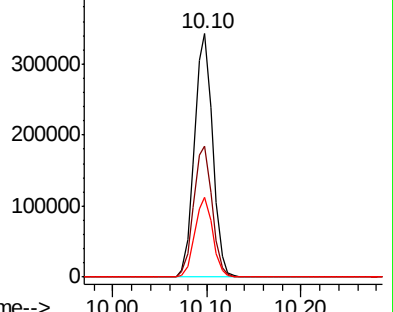

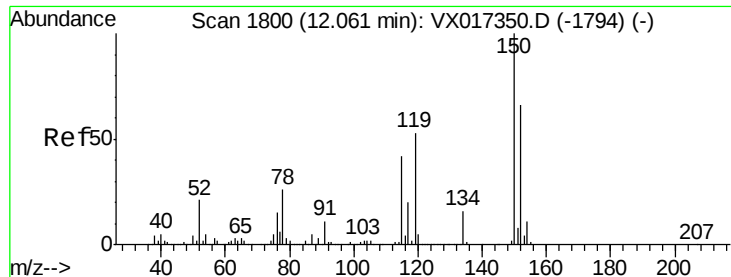

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.06 min Scan# 1800

Delta R.T. -0.00 min

Lab File: VX017408.D

Acq: 16 Jul 2020 21:47

Instrument :

MSVOA_X

ClientSampleId :

DAY-5


Tot Ion:152 Resp: 251292

Ion Ratio Lower Upper

152 100

115 57.3 39.9 119.7




150 158.3 0.0 343.4

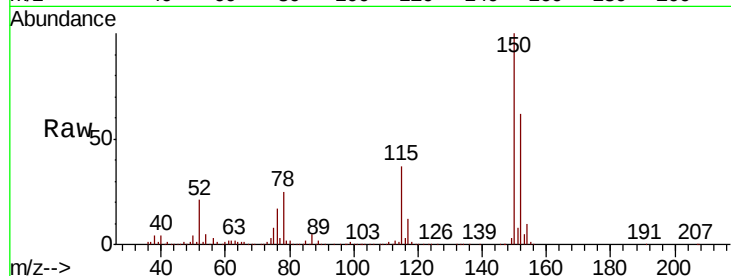

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

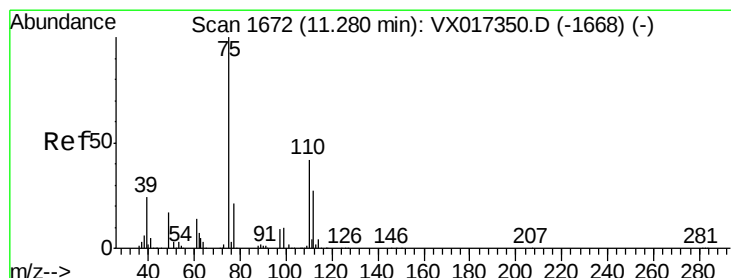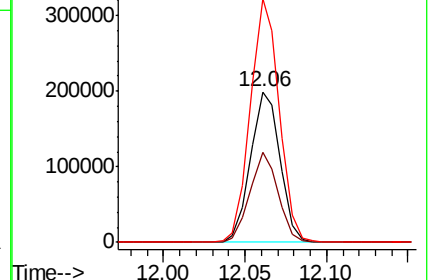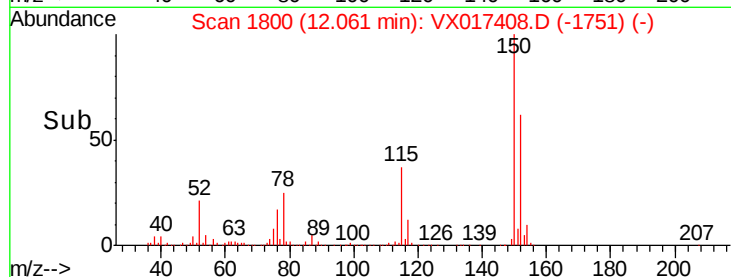

#76

1,2,3-Trichloropropane

Concen: 24.678 ug/l

RT: 11.12 min Scan# 1646

Delta R.T. -0.16 min

Lab File: VX017408.D


Acq: 16 Jul 2020 21:47

Tgt Ion: 75 Resp: 114592

Ion Ratio Lower Upper



75 100


77 1.7 20.3 60.9#

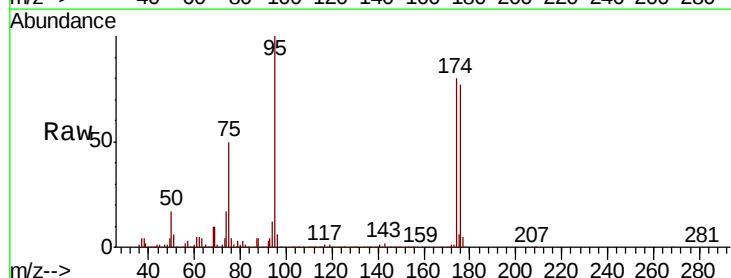

Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 77.00 (76.70 to 77.70): VX0

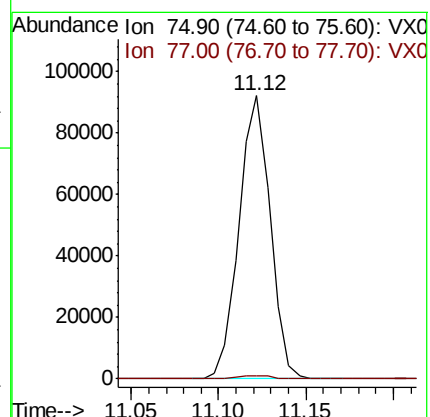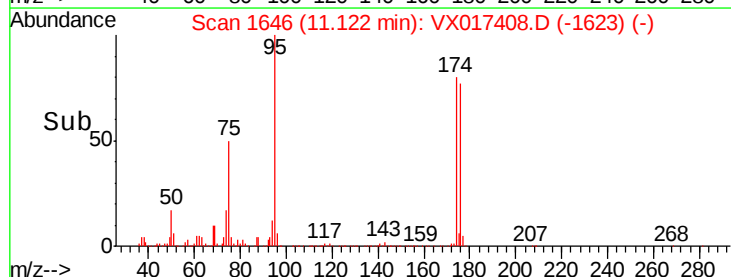

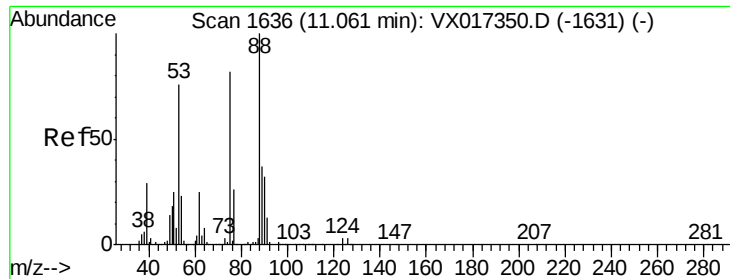

#81

trans-1,4-Dichloro-2-butene

Concen: 62.603 ug/l

RT: 11.12 min Scan# 1646

Delta R.T. 0.06 min

Lab File: VX017408.D

Acq: 16 Jul 2020 21:47

Instrument :

MSVOA_X

ClientSampleId :

DAY-5


Tot Ion: 75 Resp: 114592

Ion Ratio Lower Upper




75 100

53 0.5 76.5 114.7#

89 0.0 38.1 57.1#

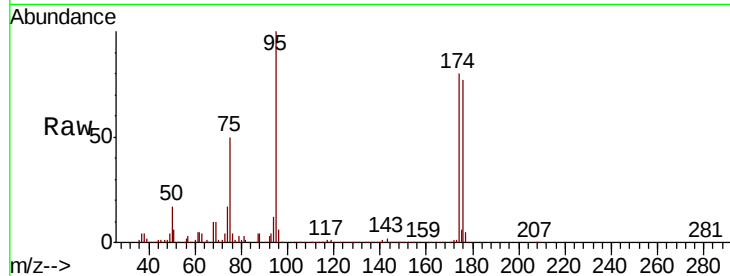

Abundance Ion 74.90 (74.60 to 75.60): VX0
Ion 53.00 (52.70 to 53.70): VX0
Ion 88.90 (88.60 to 89.60): VX0

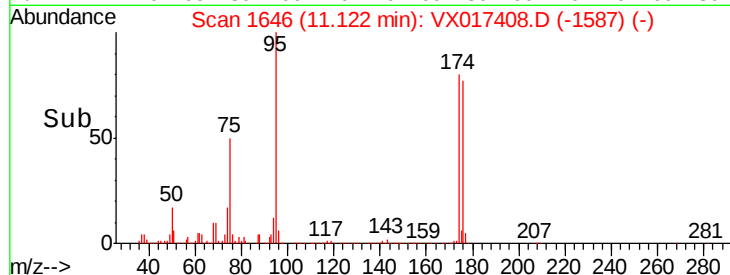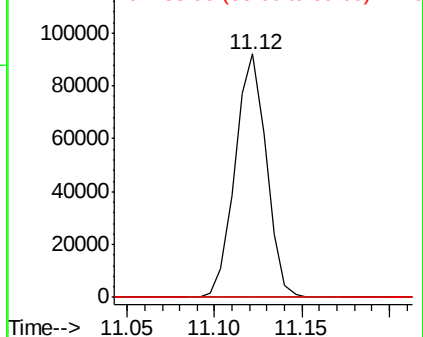

#85

sec-Butylbenzene

Concen: 0.377 ug/l

RT: 11.93 min Scan# 1778

Delta R.T. -0.01 min

Lab File: VX017408.D


Acq: 16 Jul 2020 21:47

Tgt Ion: 105 Resp: 5709



Ion Ratio Lower Upper


105 100

134 20.5 10.5 31.5



Abundance Ion 105.00 (104.70 to 105.70): V
Ion 134.00 (133.70 to 134.70): V




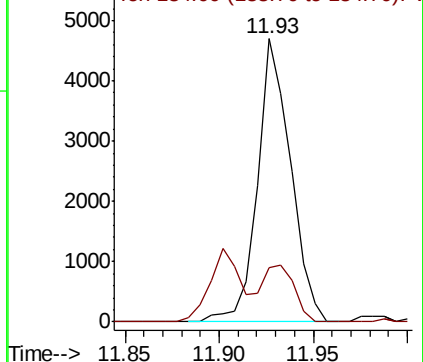




#86
p-Isopropyltoluene
Concen: 0.311 ug/l
RT: 12.22 min Scan# 1826
Delta R.T. 0.17 min
Lab File: VX017408.D
Acq: 16 Jul 2020 21:47




Instrument :
MSVOA_X
ClientSampled :
DAY-5


Tot Ion: 119 Resp: 4455
Ion Ratio Lower Upper
119 100
134 28.3 13.5 40.5
91 30.2 11.8 35.3

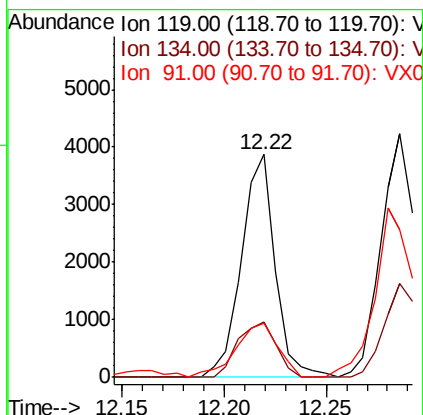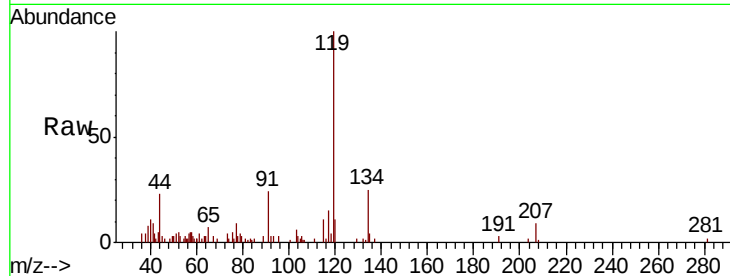

#89
n-Butylbenzene
Concen: 0.306 ug/l
RT: 12.37 min Scan# 1851
Delta R.T. -0.00 min
Lab File: VX017408.D
Acq: 16 Jul 2020 21:47

Tgt Ion: 91 Resp: 3731
Ion Ratio Lower Upper
91 100
92 53.7 27.0 81.0
134 28.1 14.1 42.2

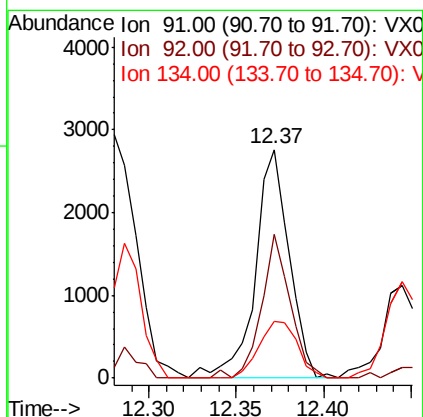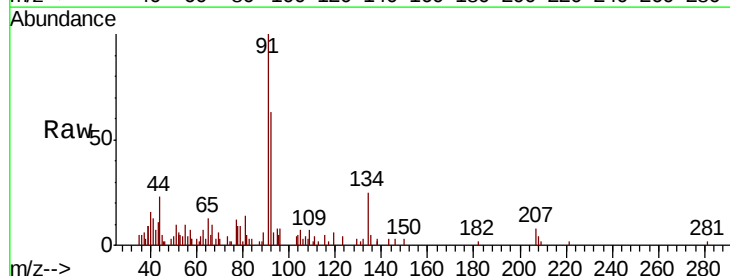



#90

Hexachloroethane

Concen: 1.789 ug/l

RT: 12.65 min Scan# 1897

Delta R.T. 0.07 min

Lab File: VX017408.D

Acq: 16 Jul 2020 21:47

Instrument :

MSVOA_X

ClientSampled :


DAY-5

Tot Ion:117 Resp: 4864

Ion Ratio Lower Upper




117 100

201 0.0 41.0 123.0#

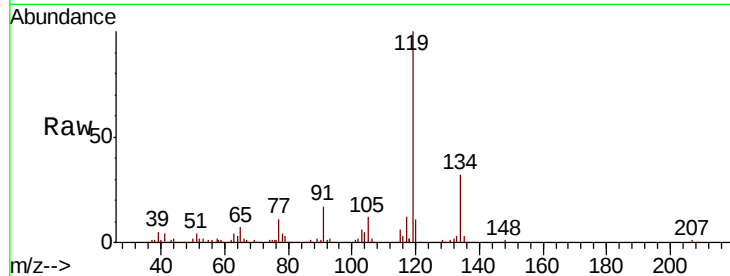

Abundance Ion 116.80 (116.50 to 117.50): V

Ion 200.70 (200.40 to 201.40): V

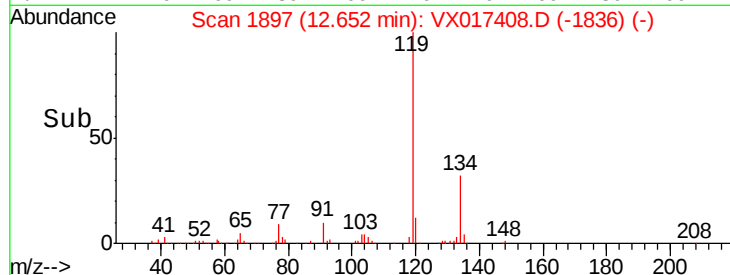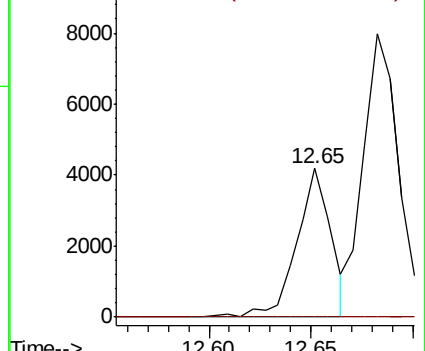

#92

1,2-Dibromo-3-Chloropropane

Concen: 0.558 ug/l

RT: 12.96 min Scan# 1948

Delta R.T. -0.02 min

Lab File: VX017408.D

Acq: 16 Jul 2020 21:47


Tgt Ion: 75 Resp: 704

Ion Ratio Lower Upper

75 100

155 0.0 46.5 139.3#



157 0.0 58.0 173.9#




Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 154.80 (154.50 to 155.50): V

Ion 156.80 (156.50 to 157.50): V

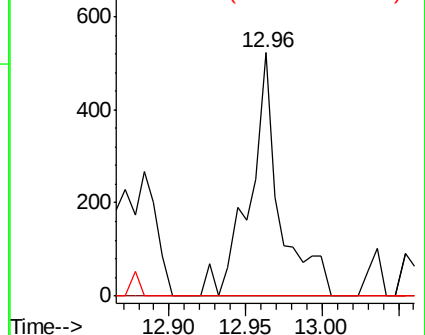


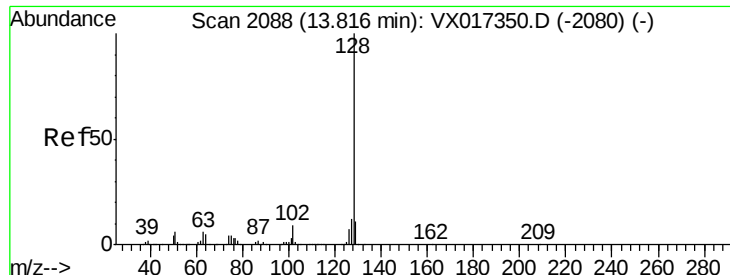

#95
Naphthalene
Concen: 0.229 ug/l
RT: 13.82 min Scan# 2088
Delta R.T. -0.00 min
Lab File: VX017408.D
Acq: 16 Jul 2020 21:47

Instrument :
MSVOA_X
ClientSampleId :
DAY-5

Tot Ion:128 Resp: 3527
Ion Ratio Lower Upper
128 100
127 21.4 10.2 15.4#
129 47.1 8.9 13.3#



Abundance Ion 128.00 (127.70 to 128.70): V
Ion 127.00 (126.70 to 127.70): V
Ion 129.00 (128.70 to 129.70): V

