

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX071620\
 Data File : VX017405.D
 Acq On : 16 Jul 2020 20:38
 Operator : JC/SP
 Sample : L3334-01 20X
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 I-OC-4

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X071320W.M
 Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.648	74	92	93	rBV	24281	100662	6.81%	1.046%
2	2.428	214	220	227	rVB	16591	29422	1.99%	0.306%
3	2.544	232	239	249	rBV	346050	565156	38.21%	5.874%
4	2.831	280	286	296	rVB	14609	28269	1.91%	0.294%
5	4.678	578	589	603	rVB5	6208	27480	1.86%	0.286%
6	5.172	662	670	679	rBV3	8935	26364	1.78%	0.274%
7	5.464	704	718	733	rBV	164000	473436	32.01%	4.921%
8	5.629	733	745	757	rVV	250027	698773	47.24%	7.263%
9	6.031	799	811	820	rBV	166940	445910	30.14%	4.635%
10	6.111	820	824	837	rVB2	11426	30955	2.09%	0.322%
11	6.830	932	942	959	rBV	408189	959348	64.85%	9.971%
12	8.458	1204	1209	1214	rBV	24432	43232	2.92%	0.449%
13	8.695	1240	1248	1256	rBV	892254	1358161	91.82%	14.117%
14	8.891	1275	1280	1288	rVB	15244	25509	1.72%	0.265%
15	10.098	1471	1478	1487	rBV	978162	1330498	89.95%	13.829%
16	10.348	1514	1519	1525	rVB3	12382	24011	1.62%	0.250%
17	11.122	1638	1646	1654	rBV	895154	1119259	75.67%	11.634%
18	12.061	1794	1800	1808	rBV	1215057	1479224	100.00%	15.375%
19	13.816	2081	2088	2099	rBV	664393	797146	53.89%	8.285%
20	13.908	2099	2103	2109	rVB	25571	36747	2.48%	0.382%
21	14.676	2222	2229	2236	rBV	13539	21420	1.45%	0.223%


Sum of corrected areas: 9620982

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX071620\
Data File : VX017405.D
Acq On : 16 Jul 2020 20:38
Operator : JC/SP
Sample : L3334-01 20X
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
I-OC-4

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X071320W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

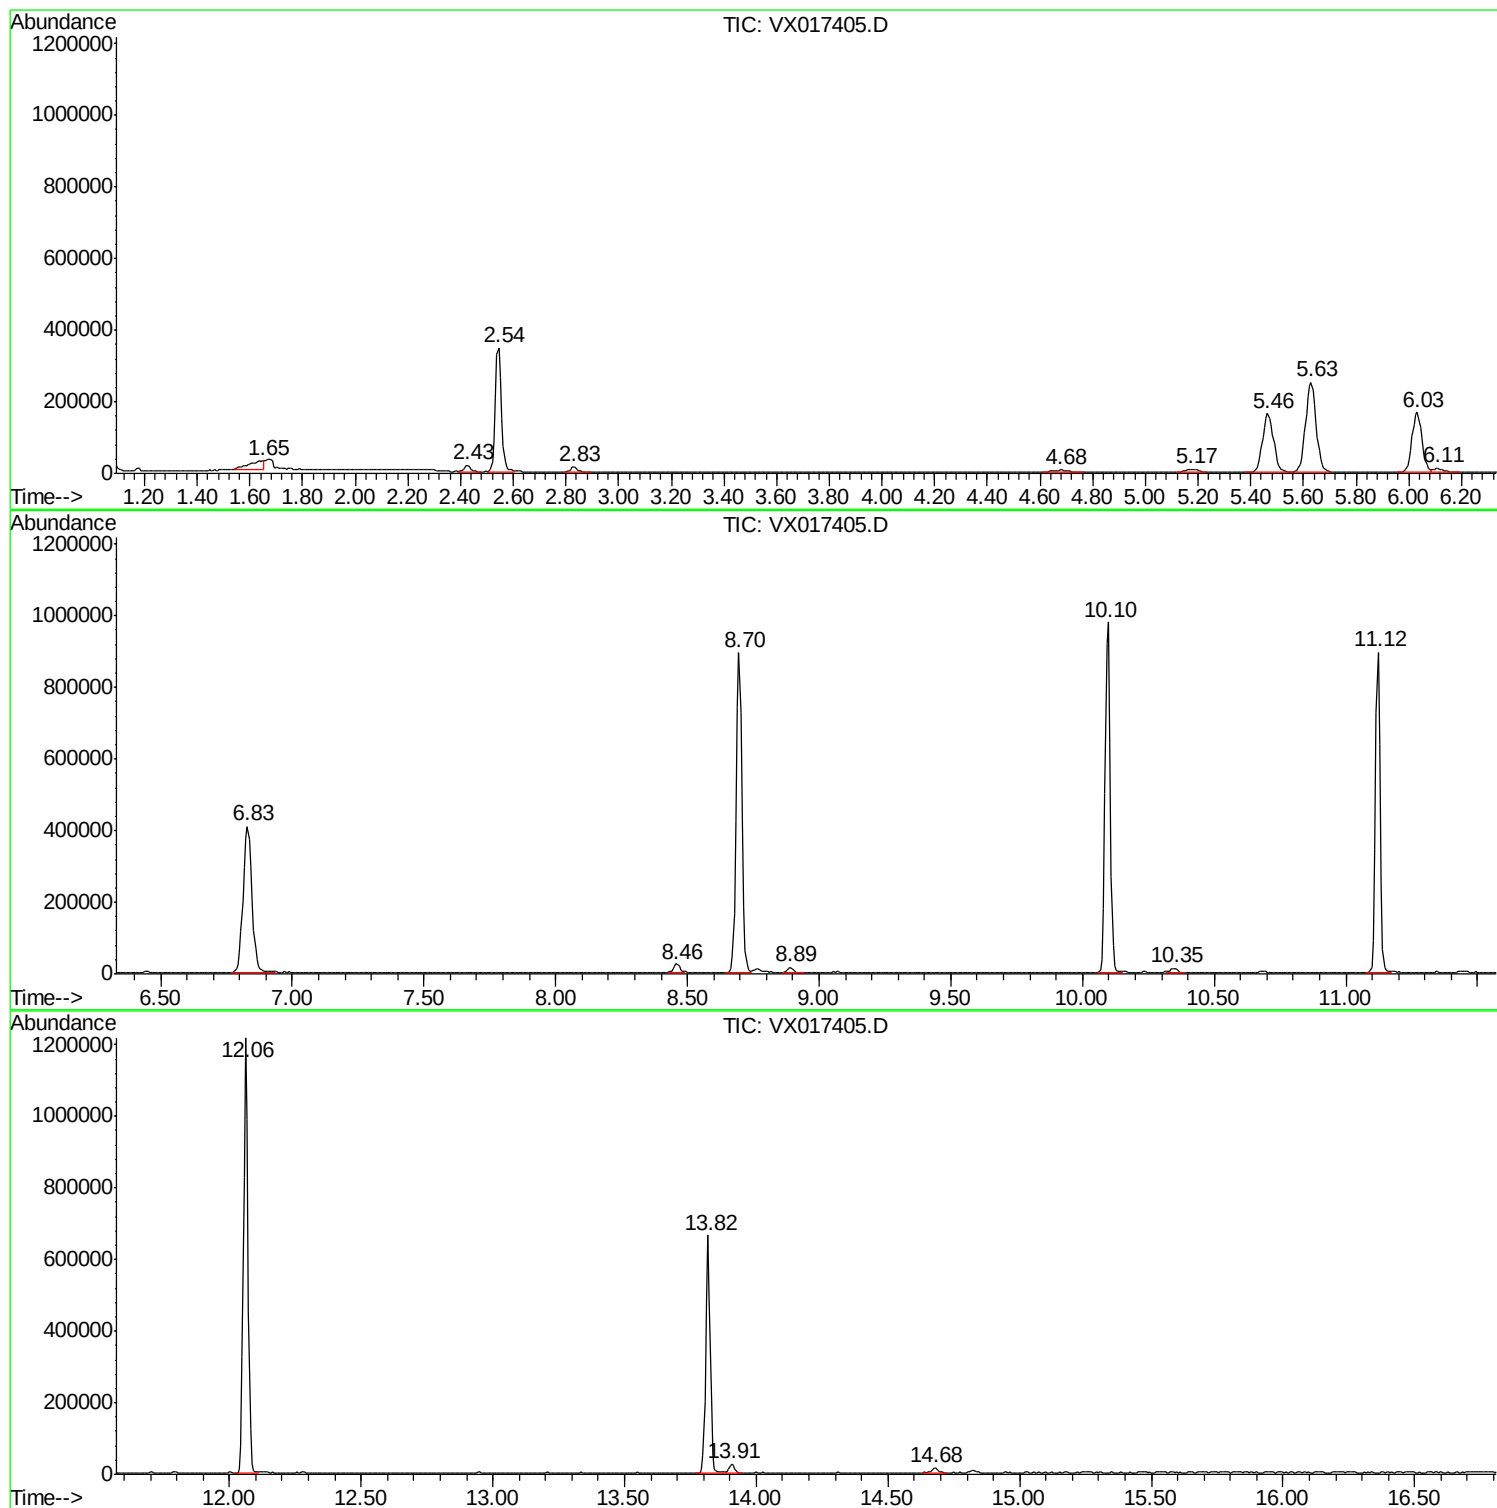

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX071620\
Data File : VX017405.D
Acq On : 16 Jul 2020 20:38
Operator : JC/SP
Sample : L3334-01 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
I-OC-4

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X071320W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown1.65 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.65	7.20 ug/l	100662	Pentafluorobenzene	5.63

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Propanoic acid, 2-chloro-, ethyl...	136	C5H9ClO2	000535-13-7	22
2			1,4-Bis[2-[2-(2-chloroethoxy)eth...	410	C18H28Cl2O6	199984-37-7	17
3			Ethanol, 2-chloro-, phosphite (3:1)	268	C6H12Cl3O3P	000140-08-9	12
4			1,3-Dioxonane, 5,5,6,6,7,7,8,8-o...	274	C7H6F8O2	036301-47-0	12
5			Phosgene	98	CCl2O	000075-44-5	12

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX071620\
Data File : VX017405.D
Acq On : 16 Jul 2020 20:38
Operator : JC/SP
Sample : L3334-01 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
I-OC-4

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X071320W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown1.65	1.65	7.2	ug/l	100662	1	5.63	698773	50.0