

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071621\
 Data File : VX023316.D
 Acq On : 16 Jul 2021 10:20
 Operator : JC/MD
 Sample : VX0716WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0716WBL01

Quant Time: Jul 17 02:06:51 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X070221W.M
 Quant Title : SW846 8260
 QLast Update : Fri Jul 02 14:29:42 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.562	168	229369	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.769	114	372181	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	330215	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	140673	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.964	65	157588	51.120	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	102.240%
35) Dibromofluoromethane	5.391	113	122246	50.864	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	101.720%
50) Toluene-d8	8.653	98	438754	48.940	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	97.880%
62) 4-Bromofluorobenzene	11.085	95	158426	45.774	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	91.540%
Target Compounds						
16) Acetone	2.386	43	5669	4.648	ug/l	Qvalue 90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071621\
Data File : VX023316.D
Acq On : 16 Jul 2021 10:20
Operator : JC/MD
Sample : VX0716WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0716WBL01

Quant Time: Jul 17 02:06:51 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X070221W.M
Quant Title : SW846 8260
QLast Update : Fri Jul 02 14:29:42 2021
Response via : Initial Calibration




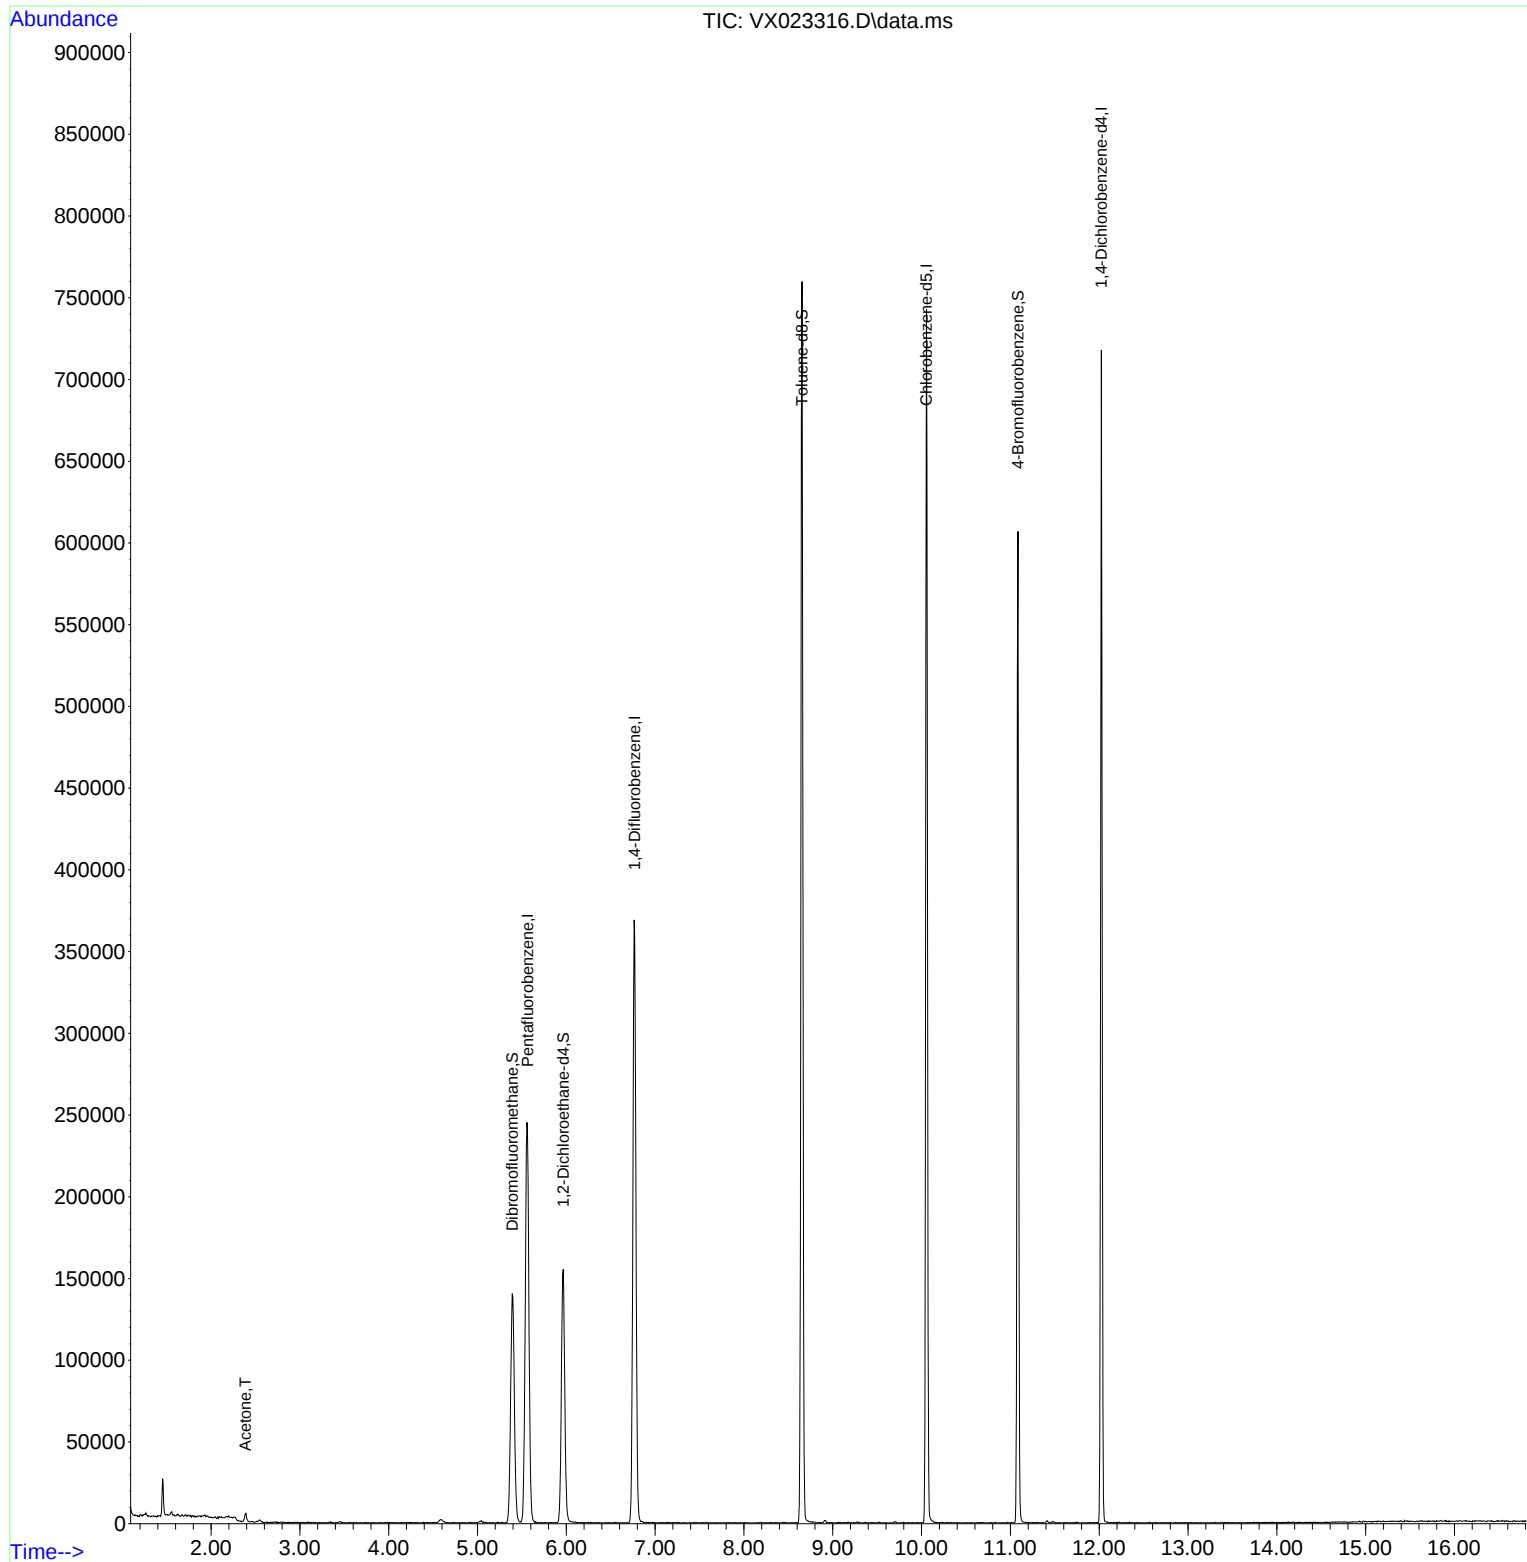


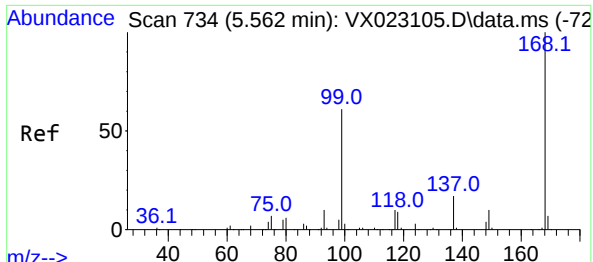

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.562 min Scan# 734
Delta R.T. -0.000 min
Lab File: VX023316.D
Acq: 16 Jul 2021 10:20




Instrument :
MSVOA_X
ClientSampleId :
VX0716WBL01


Tgt Ion:168 Resp: 229369
Ion Ratio Lower Upper
168 100
99 58.2 45.8 68.6

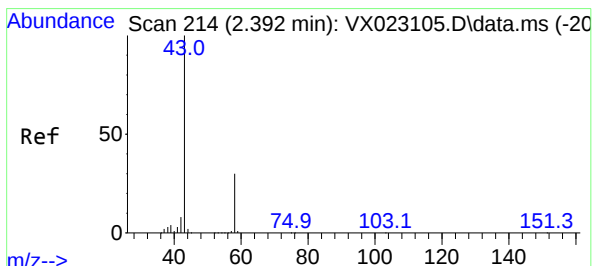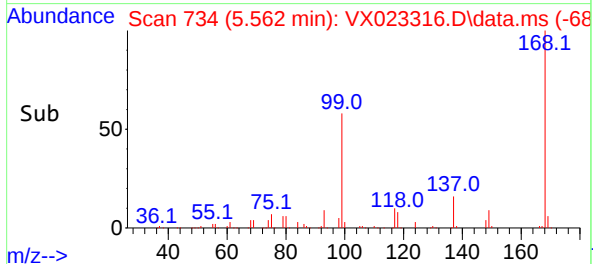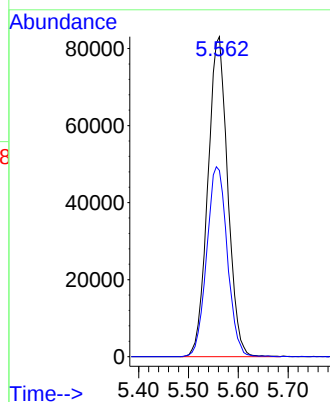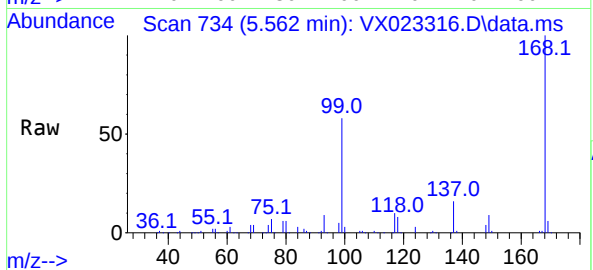

#16
Acetone
Concen: 4.648 ug/l
RT: 2.386 min Scan# 213
Delta R.T. -0.006 min
Lab File: VX023316.D
Acq: 16 Jul 2021 10:20

Tgt Ion: 43 Resp: 5669
Ion Ratio Lower Upper
43 100
58 29.0 27.8 41.8

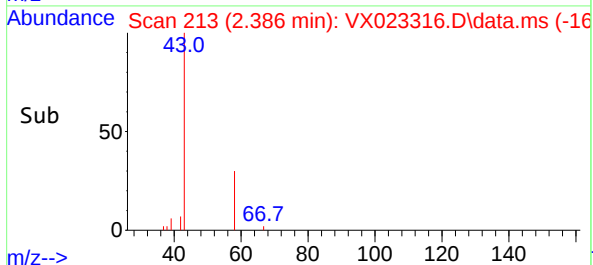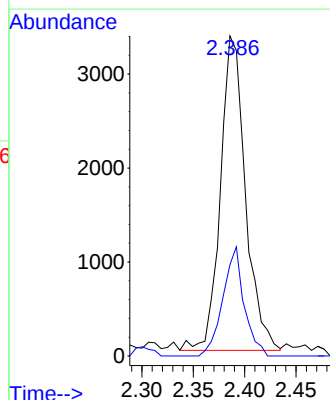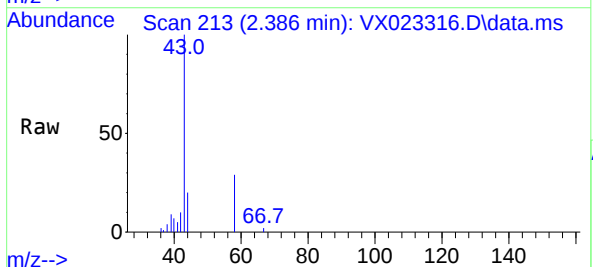




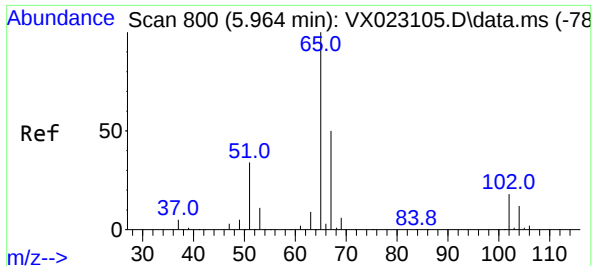


#33

1,2-Dichloroethane-d4
Concen: 51.120 ug/l
RT: 5.964 min Scan# 800
Delta R.T. 0.000 min
Lab File: VX023316.D
Acq: 16 Jul 2021 10:20

Instrument :
MSVOA_X
ClientSampleId :
VX0716WBL01




Tgt Ion: 65 Resp: 157588
Ion Ratio Lower Upper
65 100
67 50.8 0.0 105.4

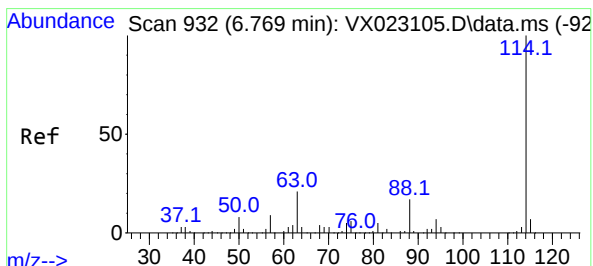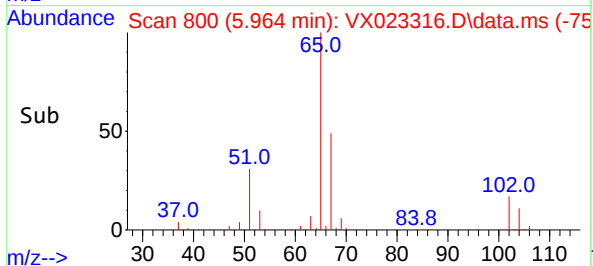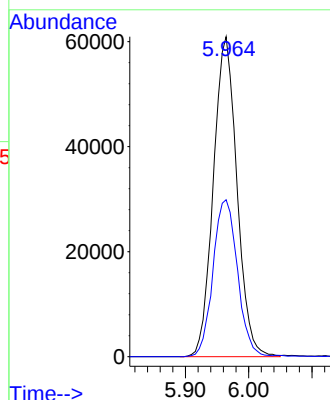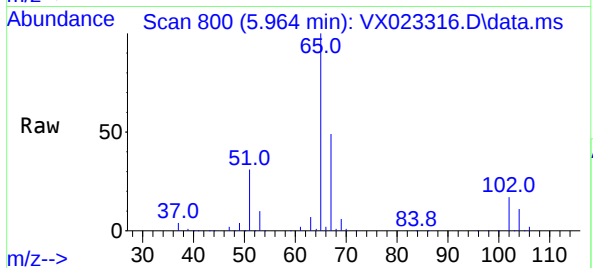


#34

1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.769 min Scan# 932
Delta R.T. 0.000 min
Lab File: VX023316.D
Acq: 16 Jul 2021 10:20

Tgt Ion: 114 Resp: 372181
Ion Ratio Lower Upper
114 100
63 20.4 0.0 40.8
88 16.1 0.0 32.8


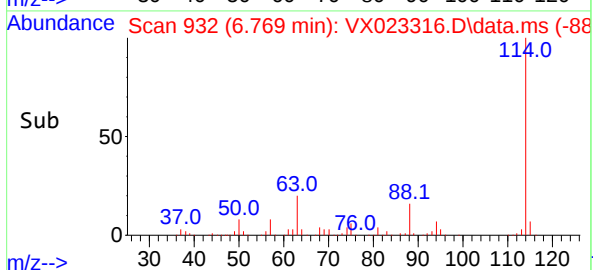
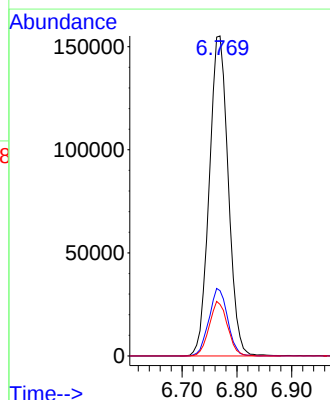
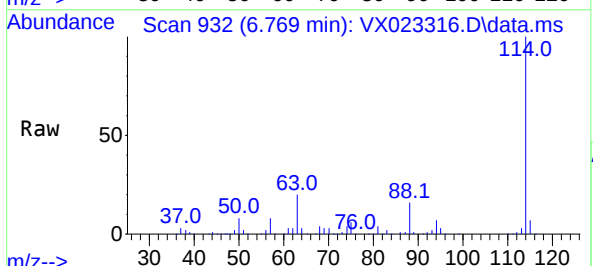


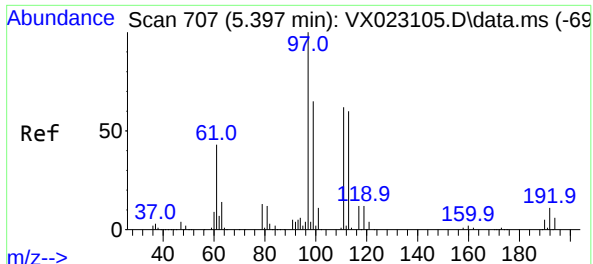

#35
Dibromofluoromethane
Concen: 50.864 ug/l
RT: 5.391 min Scan# 706
Delta R.T. -0.006 min
Lab File: VX023316.D
Acq: 16 Jul 2021 10:20




Instrument :
MSVOA_X
ClientSampleId :
VX0716WBL01


Tgt Ion:113 Resp: 122246
Ion Ratio Lower Upper
113 100
111 101.8 81.9 122.9
192 19.2 16.7 25.1

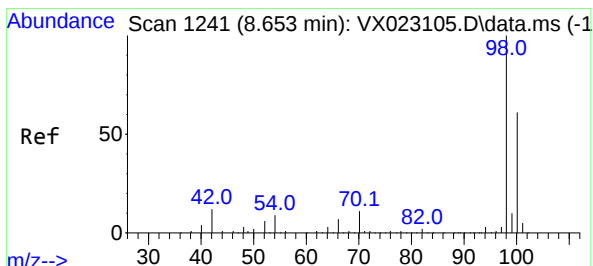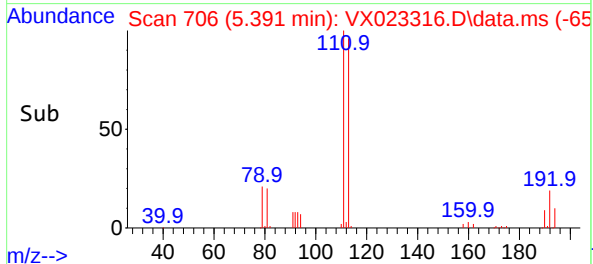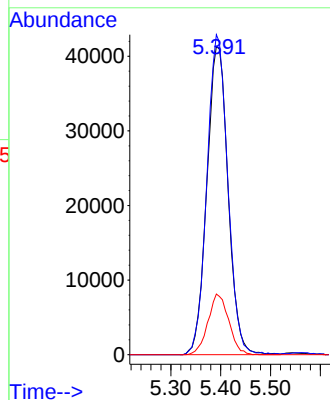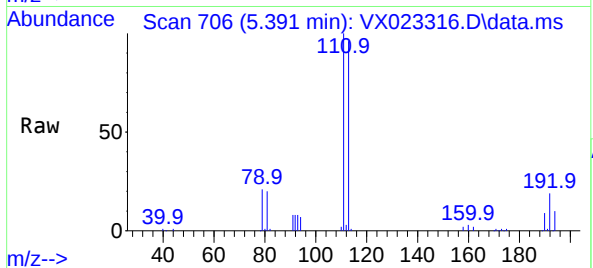

#50
Toluene-d8
Concen: 48.940 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. -0.000 min
Lab File: VX023316.D
Acq: 16 Jul 2021 10:20

Tgt Ion: 98 Resp: 438754
Ion Ratio Lower Upper
98 100
100 65.0 51.9 77.9


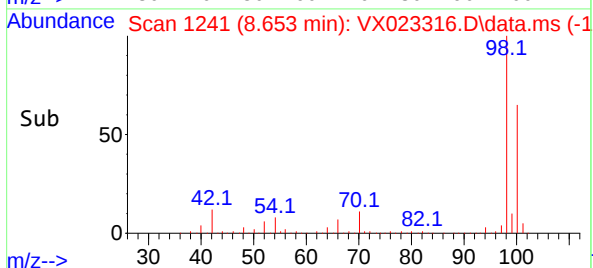
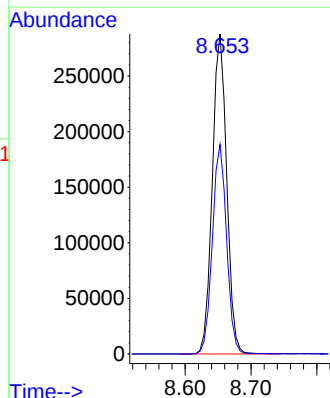
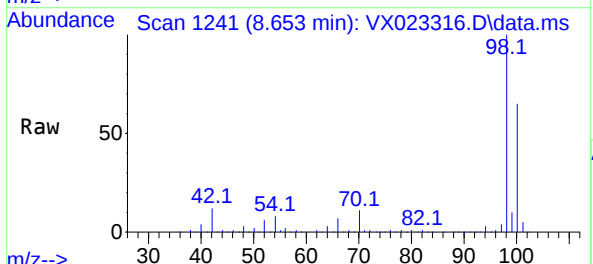


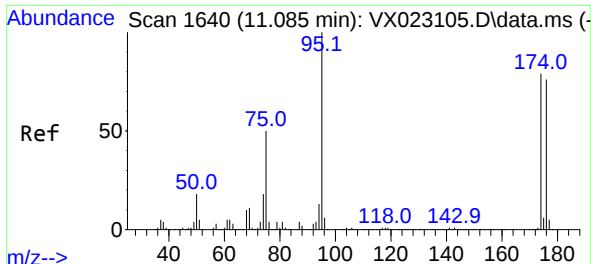

#62
4-Bromofluorobenzene
Concen: 45.774 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.000 min
Lab File: VX023316.D
Acq: 16 Jul 2021 10:20




Instrument :
MSVOA_X
ClientSampleId :
VX0716WBL01


Tgt Ion: 95 Resp: 158426
Ion Ratio Lower Upper
95 100
174 77.3 0.0 154.6
176 74.5 0.0 155.8

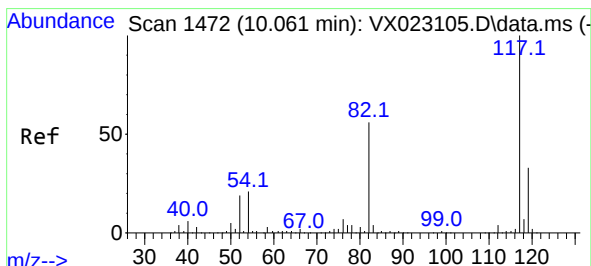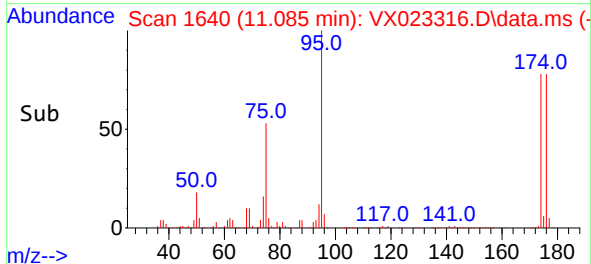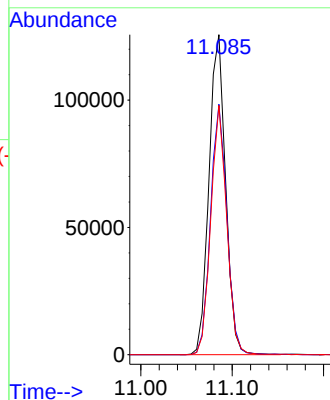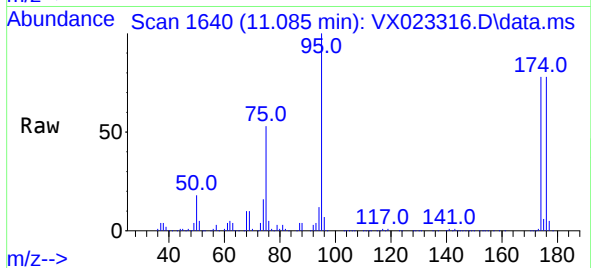

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.006 min
Lab File: VX023316.D
Acq: 16 Jul 2021 10:20

Tgt Ion: 117 Resp: 330215
Ion Ratio Lower Upper
117 100
82 58.1 47.4 71.2
119 31.1 26.6 39.8

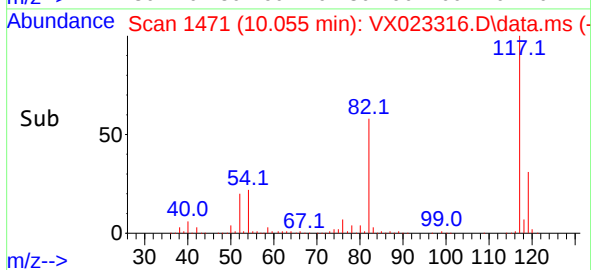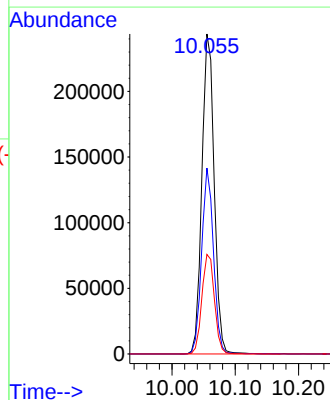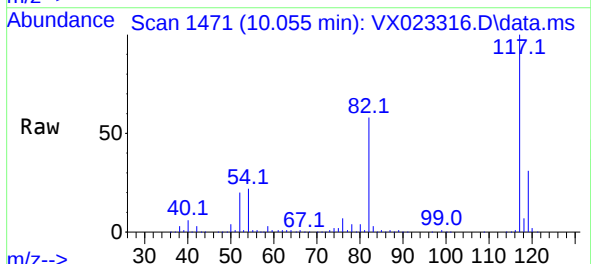

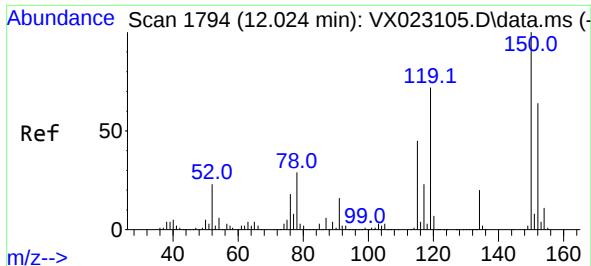

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 12.024 min Scan# 1794
 Delta R.T. 0.000 min
 Lab File: VX023316.D
 Acq: 16 Jul 2021 10:20

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0716WBL01

Tgt Ion:152 Resp: 140673
 Ion Ratio Lower Upper
 152 100
 115 61.9 41.1 123.3
 150 155.7 0.0 349.0

