

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071621\
 Data File : VX023328.D
 Acq On : 16 Jul 2021 15:32
 Operator : JC/MD
 Sample : M3087-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 STORAGE-BLANK-SAMPLE-MANA

Integration Parameters: RTEINT.P
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X070221W.M
 Title : SW846 8260

Signal : TIC: VX023328.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.252	24	27	33	rBV	187797	172846	15.79%	2.921%
2	2.550	231	240	247	rBV	16002	28690	2.62%	0.485%
3	4.593	561	575	587	rBV	7536	24670	2.25%	0.417%
4	5.397	695	707	720	rBV2	131920	379145	34.64%	6.408%
5	5.562	723	734	749	rVB2	229344	649640	59.35%	10.980%
6	5.964	789	800	815	rBV	144598	385560	35.22%	6.517%
7	6.769	921	932	945	rBV	348367	816281	74.57%	13.796%
8	8.653	1234	1241	1252	rBV	707685	1094670	100.00%	18.502%
9	10.055	1466	1471	1490	rVB	645485	926546	84.64%	15.660%
10	11.085	1634	1640	1655	rBV	539822	693277	63.33%	11.717%
11	12.024	1789	1794	1802	rBV	602338	745276	68.08%	12.596%




Sum of corrected areas: 5916601

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071621\
Data File : VX023328.D
Acq On : 16 Jul 2021 15:32
Operator : JC/MD
Sample : M3087-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SAMPLE-MANA

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X070221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

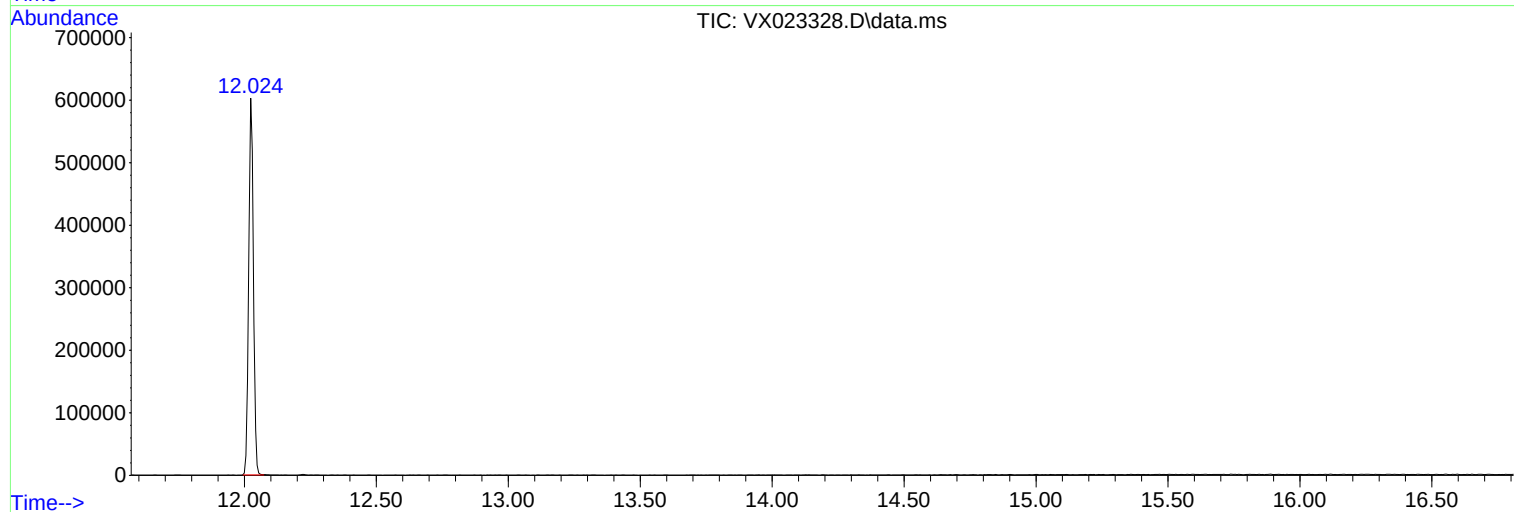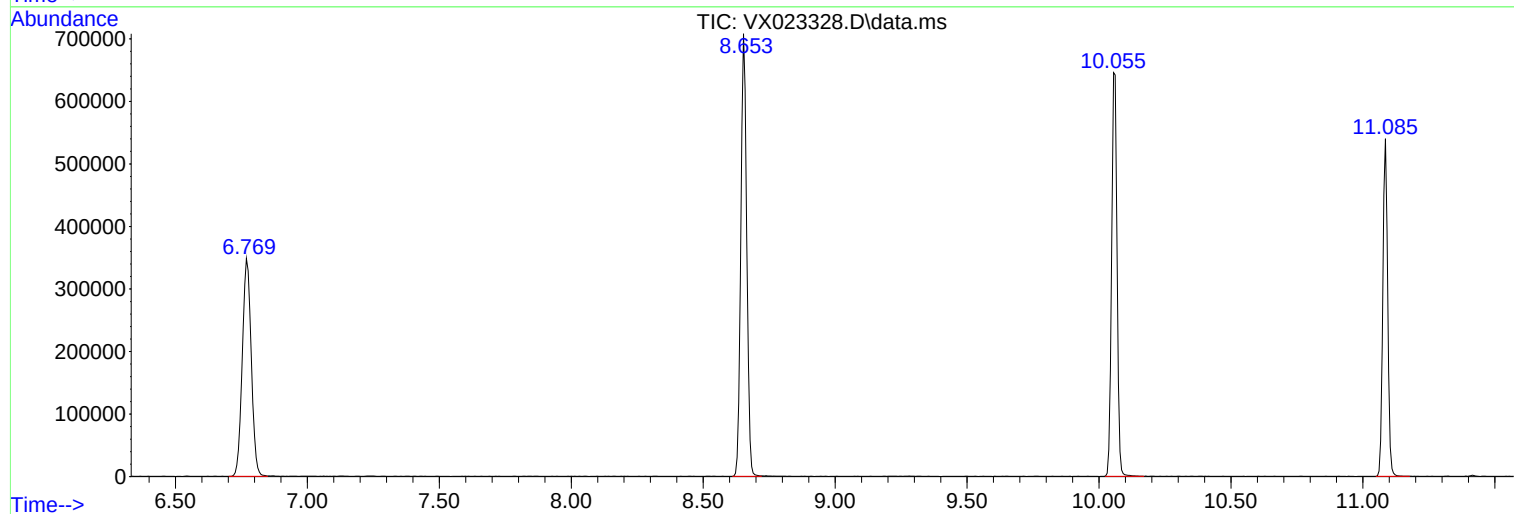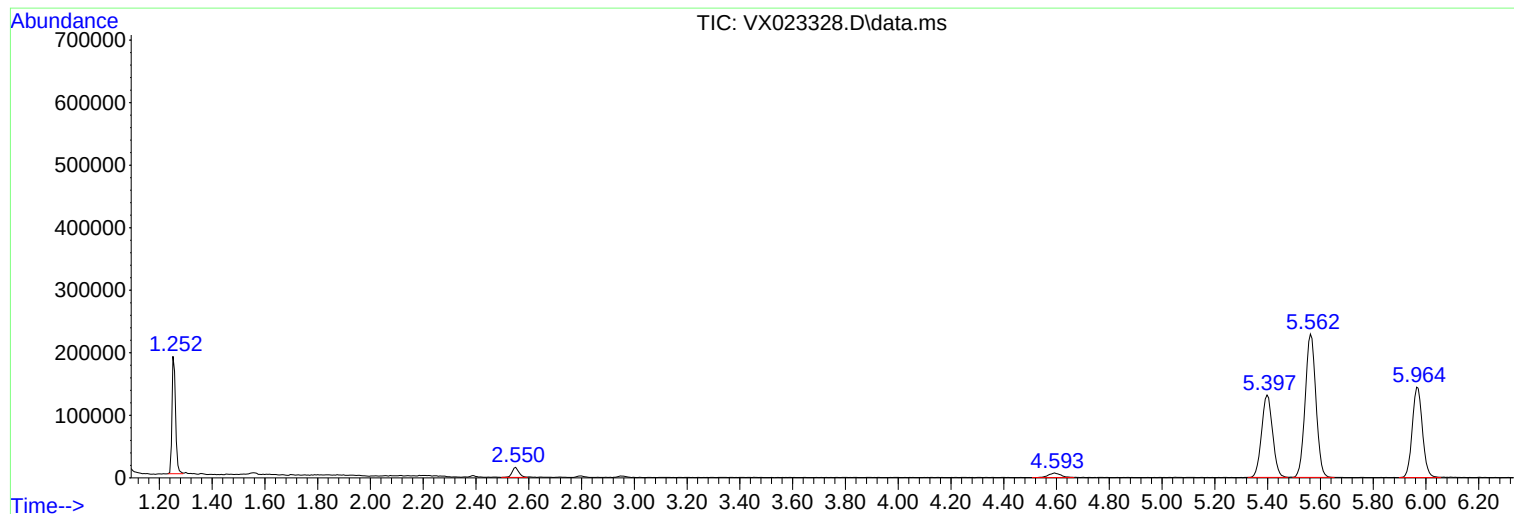

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071621\
Data File : VX023328.D
Acq On : 16 Jul 2021 15:32
Operator : JC/MD
Sample : M3087-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SAMPLE-MANA

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X070221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071621\
Data File : VX023328.D
Acq On : 16 Jul 2021 15:32
Operator : JC/MD
Sample : M3087-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SAMPLE-MANA

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X070221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------