
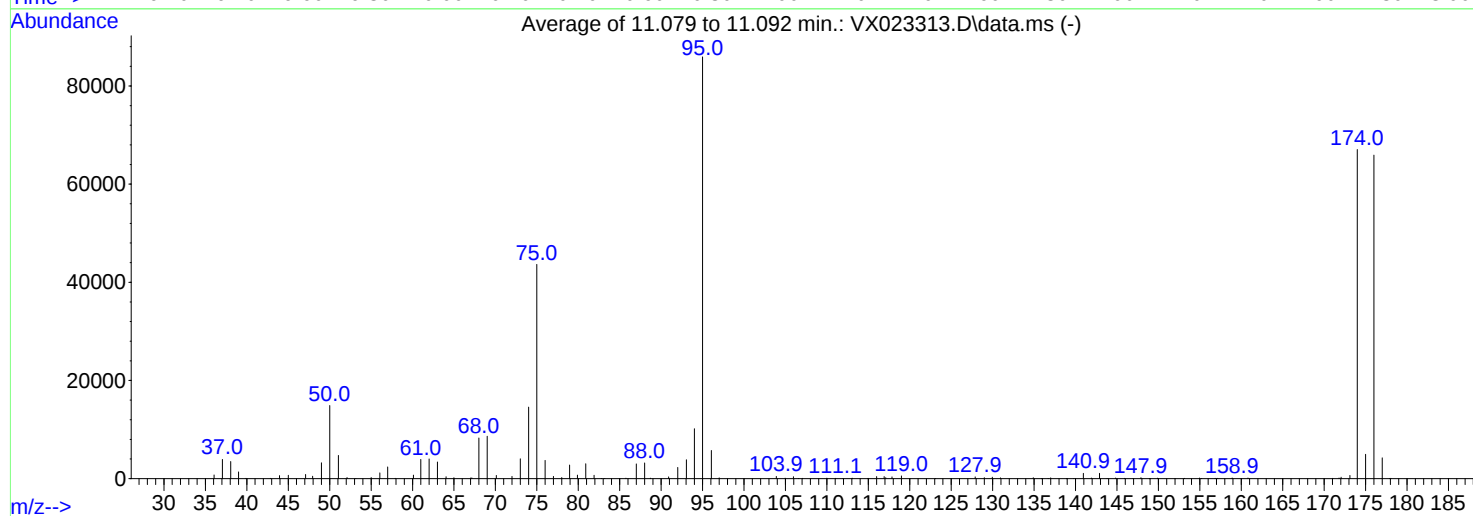


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX071621\
 Data File : VX023313.D
 Acq On : 16 Jul 2021 08:40
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X070221W.M
 Title : SW846 8260
 Last Update : Fri Jul 02 14:29:42 2021

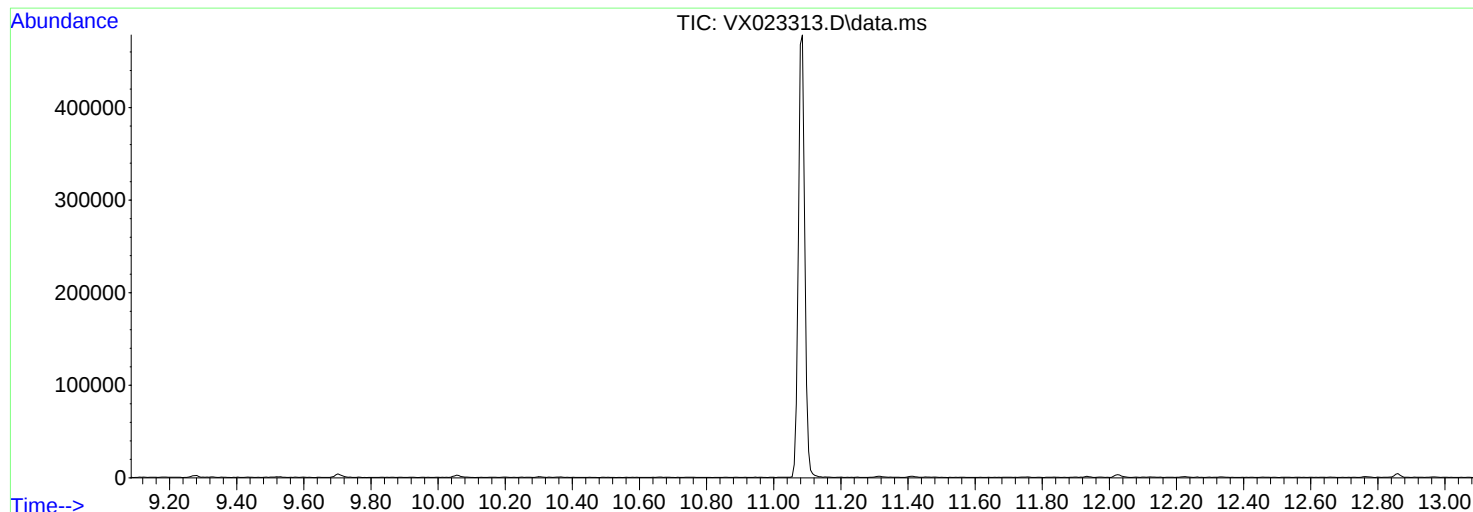

AutoFind: Scans 1639, 1640, 1641; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.3	14896	PASS
75	95	30	60	50.8	43640	PASS
95	95	100	100	100.0	85931	PASS
96	95	5	9	6.7	5725	PASS
173	174	0.00	2	1.0	649	PASS
174	95	50	100	78.0	67043	PASS
175	174	5	9	7.4	4972	PASS
176	174	95	101	98.3	65920	PASS
177	176	5	9	6.5	4255	PASS