


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX071718\
 Data File : VX003413.D
 Acq On : 17 Jul 2018 07:34
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X071618W.M
 Title : SW846 8260
 Last Update : Mon Jul 16 13:15:28 2018

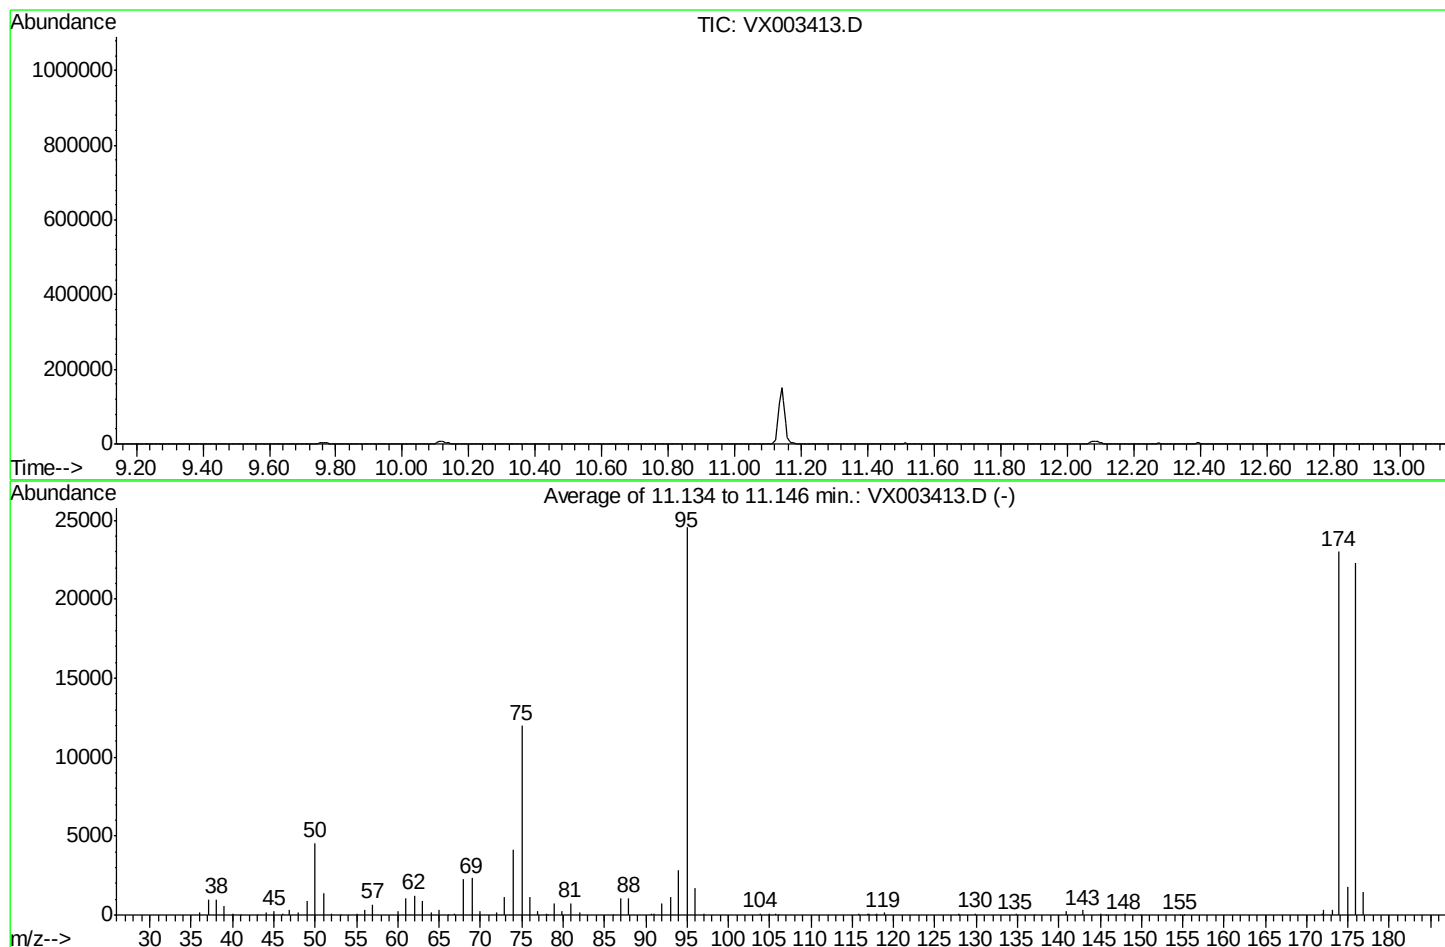

AutoFind: Scans 1730, 1731, 1732; Background Corrected with Scan 1724

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.5	4549	PASS
75	95	30	60	48.8	11984	PASS
95	95	100	100	100.0	24544	PASS
96	95	5	9	7.1	1742	PASS
173	174	0.00	2	1.3	308	PASS
174	95	50	100	93.7	23000	PASS
175	174	5	9	7.6	1754	PASS
176	174	95	101	96.7	22251	PASS
177	176	5	9	6.6	1475	PASS